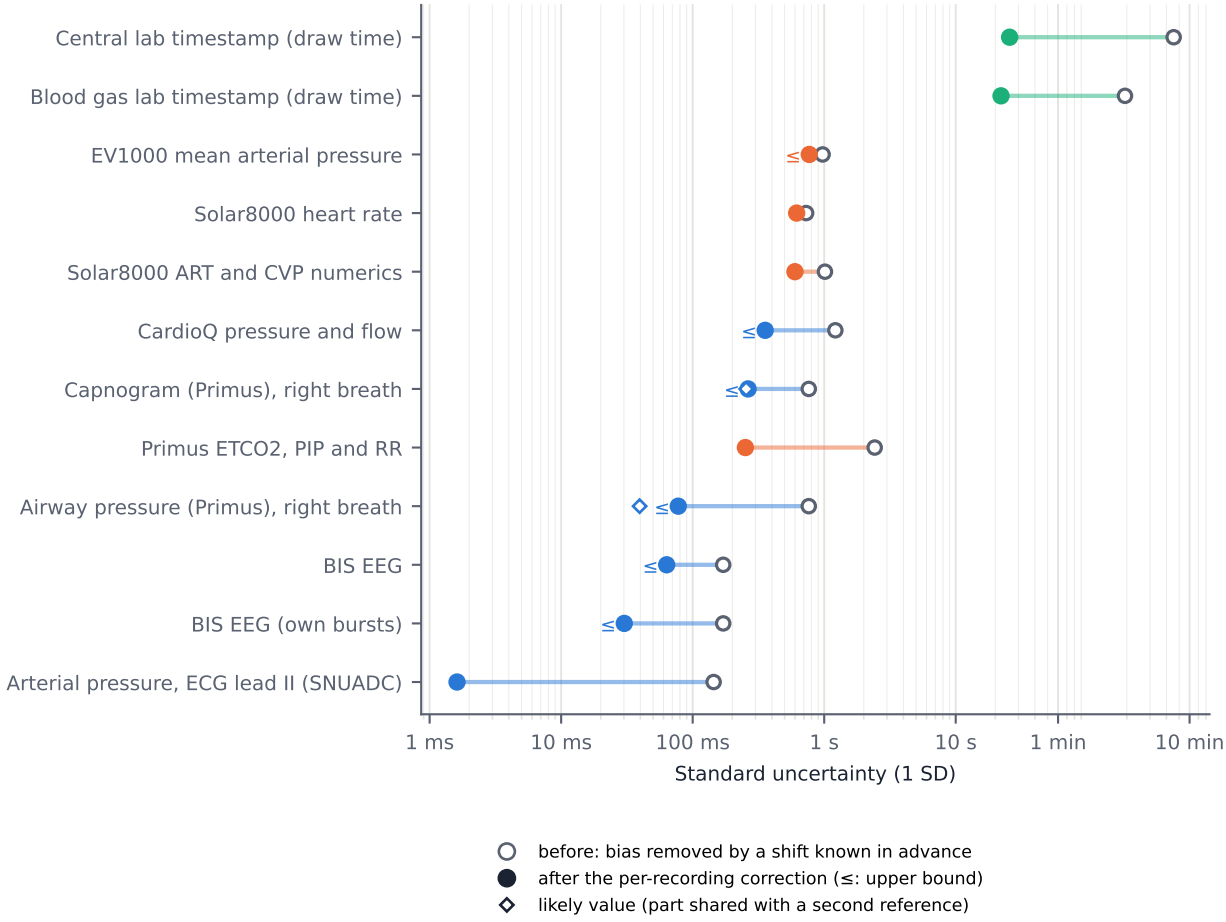
Central lab timestamp (draw time)
Blood gas lab timestamp (draw time)
EV1000 mean arterial pressure
Solar8000 heart rate
Solar8000 ART and CVP numerics
CardioQ pressure and flow
Capnogram (Primus), right breath
Primus ETCO2, PIP and RR
Airway pressure (Primus), right breath
BIS EEG
BIS EEG (own bursts)
Arterial pressure, ECG lead II (SNUADC)
1 ms
10 ms
100 ms
1 s
10 s
1 min
10 min
Standard uncertainty (1 SD)
before: bias removed by a shift known in advance
after the per-recording correction (≤: upper bound)
likely value (part shared with a second reference)