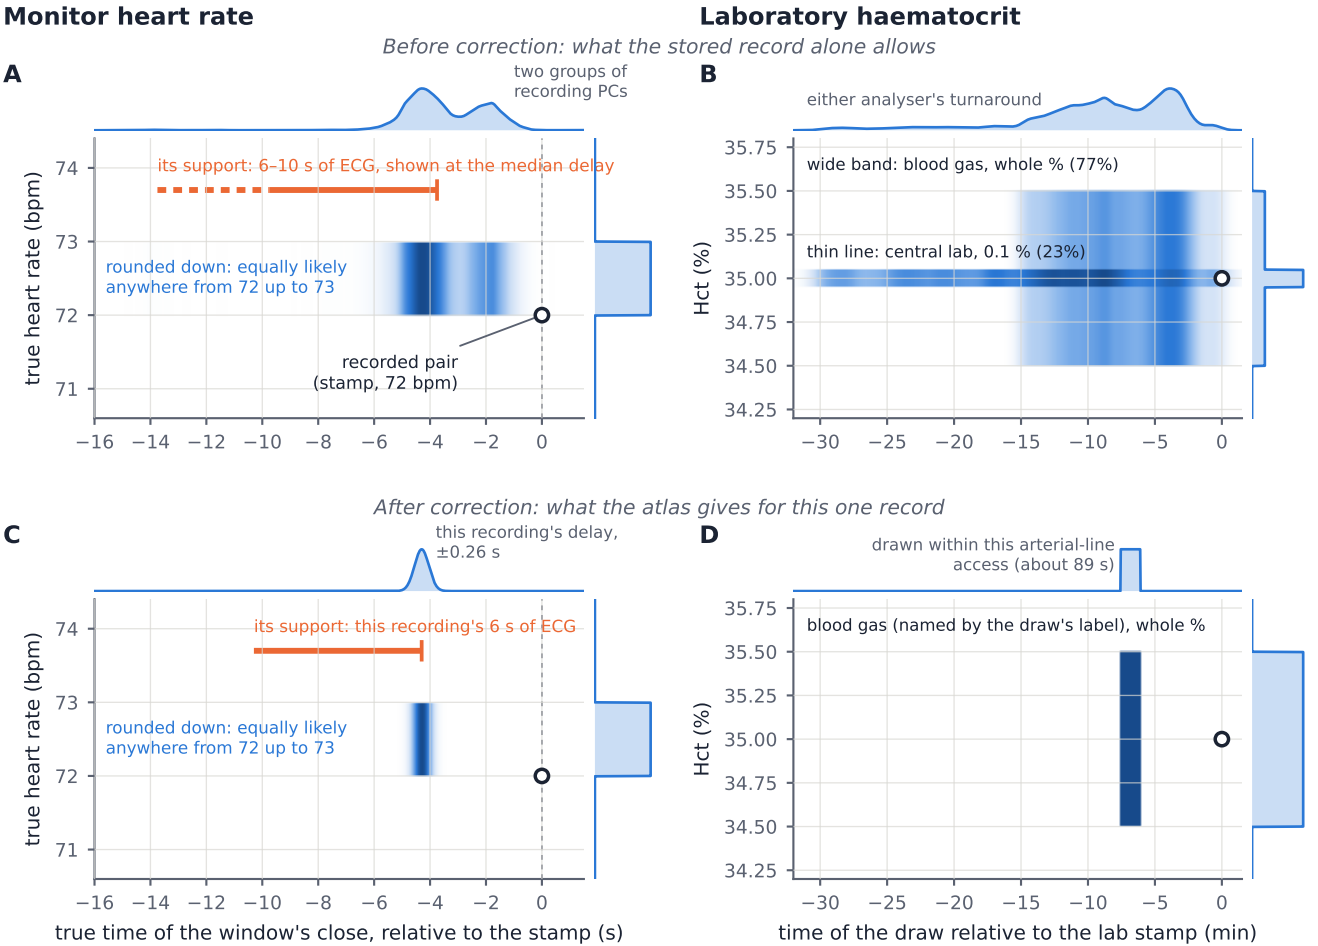

Monitor heart rate
Laboratory haematocrit
Before correction: what the stored record alone allows
A
two groups of recording PCs
its support: 6–10 s of ECG, shown at the median delay
rounded down: equally likely anywhere from 72 up to 73
recorded pair (stamp, 72 bpm)
true heart rate (bpm)
74
73
72
71
−16 −14 −12 −10 −8 −6 −4 −2 0
B
either analyser's turnaround
wide band: blood gas, whole % (77%)
thin line: central lab, 0.1 % (23%)
Hct (%)
35.75
35.50
35.25
35.00
34.75
34.50
34.25
−30 −25 −20 −15 −10 −5 0
After correction: what the atlas gives for this one record
C
this recording's delay, ±0.26 s
its support: this recording's 6 s of ECG
rounded down: equally likely anywhere from 72 up to 73
true heart rate (bpm)
74
73
72
71
−16 −14 −12 −10 −8 −6 −4 −2 0
true time of the window's close, relative to the stamp (s)
D
drawn within this arterial-line access (about 89 s)
blood gas (named by the draw's label), whole %
Hct (%)
35.75
35.50
35.25
35.00
34.75
34.50
34.25
−30 −25 −20 −15 −10 −5 0
time of the draw relative to the lab stamp (min)