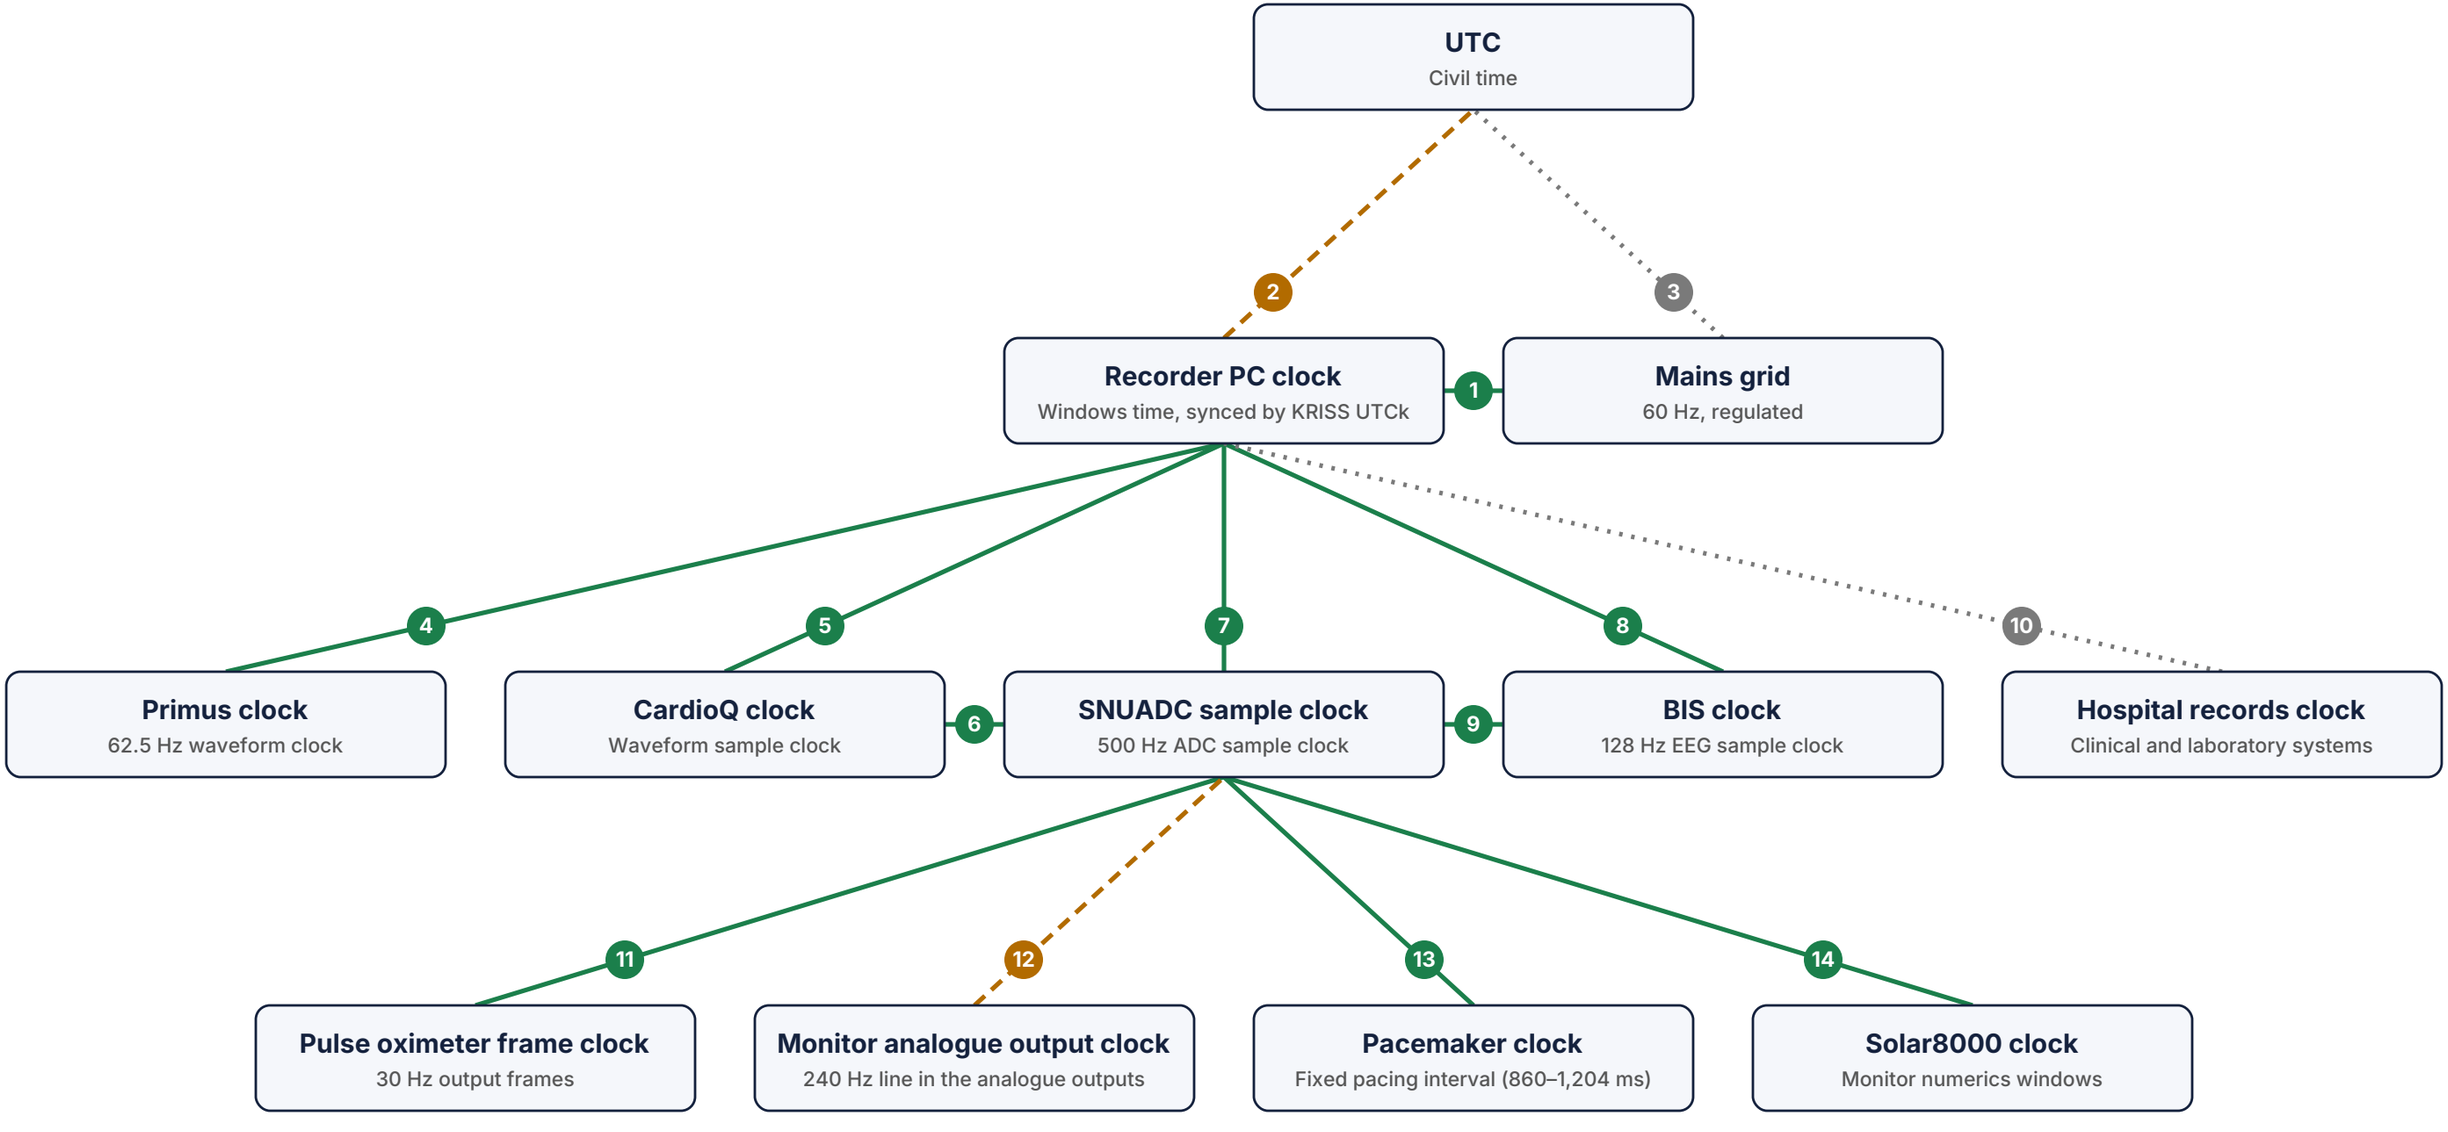
UTC
Civil time
2
3
Recorder PC clock
Windows time, synced by KRISS UTCk
1
Mains grid
60 Hz, regulated
4
5
7
8
10
Primus clock
62.5 Hz waveform clock
CardioQ clock
Waveform sample clock
6
SNUADC sample clock
500 Hz ADC sample clock
9
BIS clock
128 Hz EEG sample clock
Hospital records clock
Clinical and laboratory systems
11
12
13
14
Pulse oximeter frame clock
30 Hz output frames
Monitor analogue output clock
240 Hz line in the analogue outputs
Pacemaker clock
Fixed pacing interval (860–1,204 ms)
Solar8000 clock
Monitor numerics windows
measured
estimated
assumed