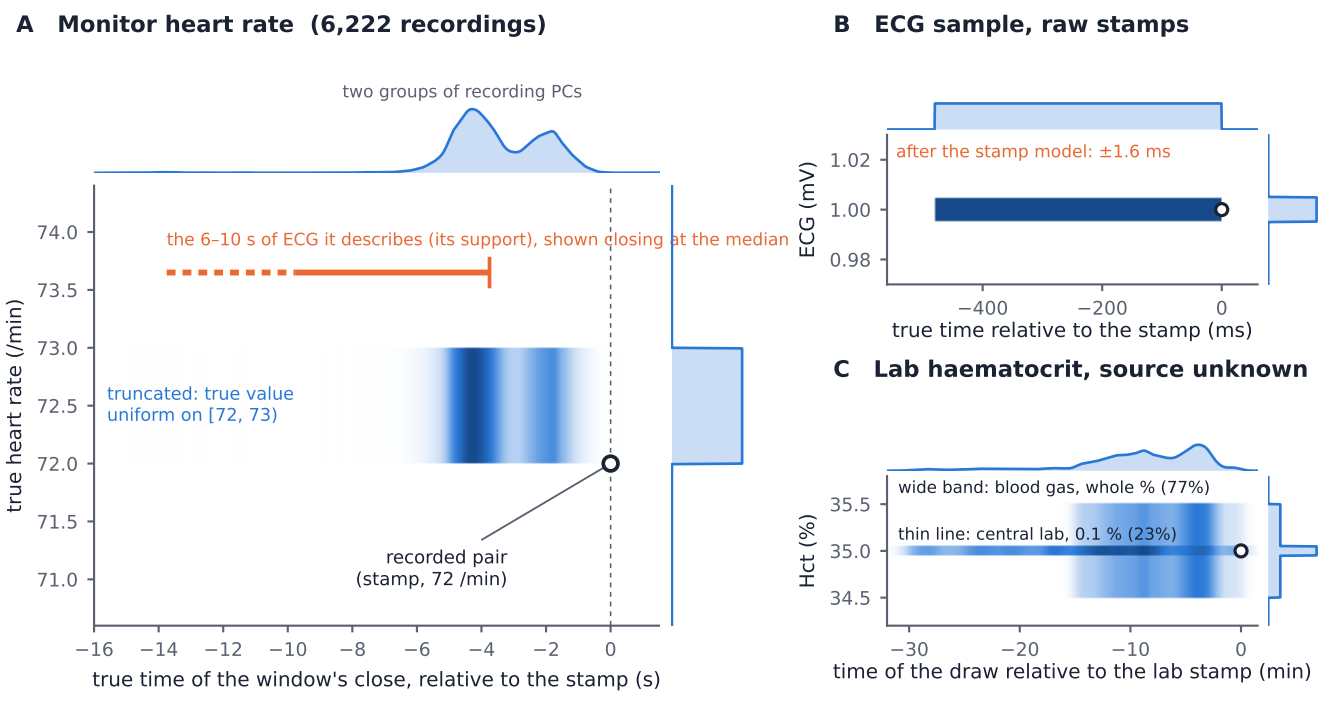

A Monitor heart rate (6,222 recordings)
two groups of recording PCs
the 6–10 s of ECG it describes (its support), shown closing at the median
truncated: true value
uniform on [72, 73)
recorded pair
(stamp, 72 /min)
true heart rate (/min)
74.0
73.5
73.0
72.5
72.0
71.5
71.0
−16
−14
−12
−10
−8
−6
−4
−2
0
true time of the window's close, relative to the stamp (s)
B ECG sample, raw stamps
after the stamp model: ±1.6 ms
ECG (mV)
1.02
1.00
0.98
−400
−200
0
true time relative to the stamp (ms)
C Lab haematocrit, source unknown
wide band: blood gas, whole % (77%)
thin line: central lab, 0.1 % (23%)
Hct (%)
35.5
35.0
34.5
−30
−20
−10
0
time of the draw relative to the lab stamp (min)