




ANSI/HL7 V2.4-2000

October 6, 2000

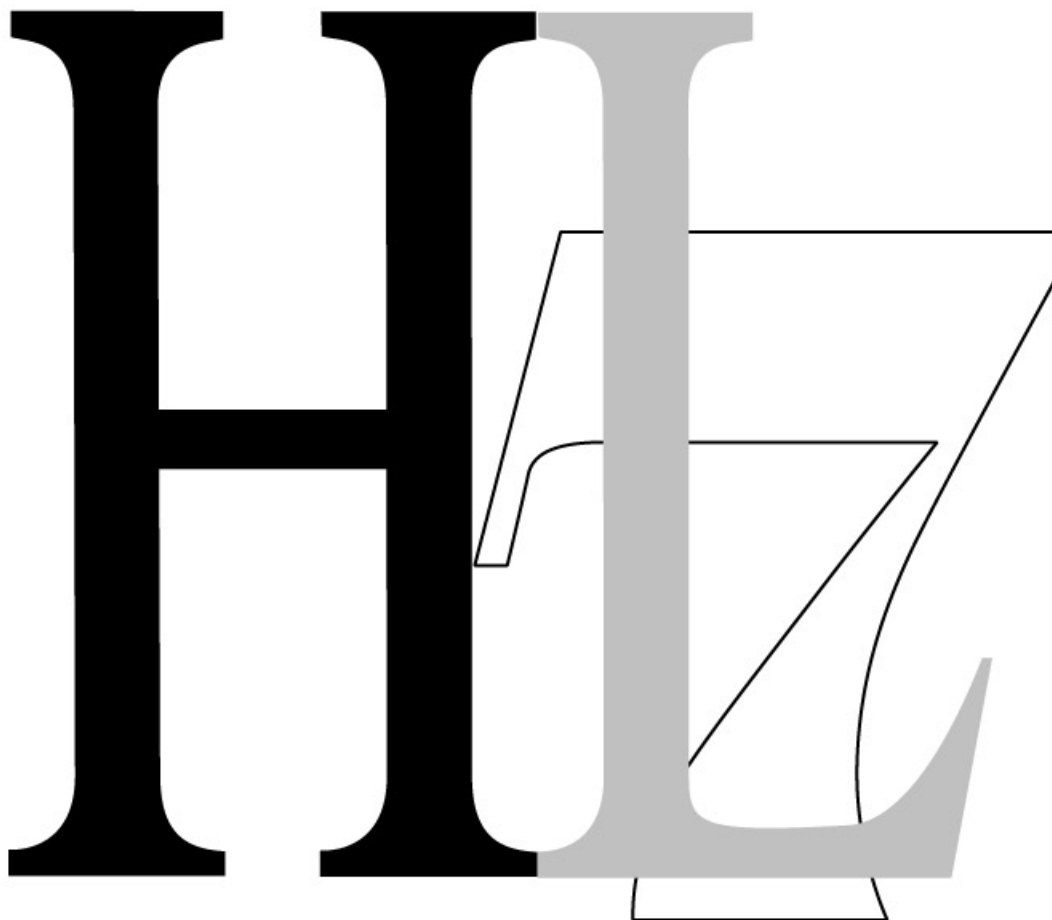

HL7 STANDARD VERSION 2.4

An Application Protocol for Electronic Data Exchange in Healthcare Environments

The Global Healthcare Messaging Standard

Health Level Seven 3300 Washtenaw, Suite 227 Ann Arbor, MI 48104-4261

Phone: 734-677-7777 Fax: 734-677-6622 Email: hq@HL7.org Internet: <http://www.HL7.org>

Printed in Ann Arbor, MI USA. Copyright ©2000 by Health Level Seven, Inc. ALL RIGHTS RESERVED

Reproduction of this material in any form is strictly forbidden without the written permission of the publisher

Chapter 13 of the HL7 V2.4 Standard is identical to the information in Section 6 of NCCLS Laboratory Automation: Communications With Automated Clinical Laboratory Systems, Instruments, Devices, and Information Systems; Approved Standard - NCCLS Document AUTO3-A [ISBN 1-56238-361-2]. NCCLS, 940 West Valley Road, Suite 1400, Wayne PA 19087-1898 USA, 2000. www.nccls.org