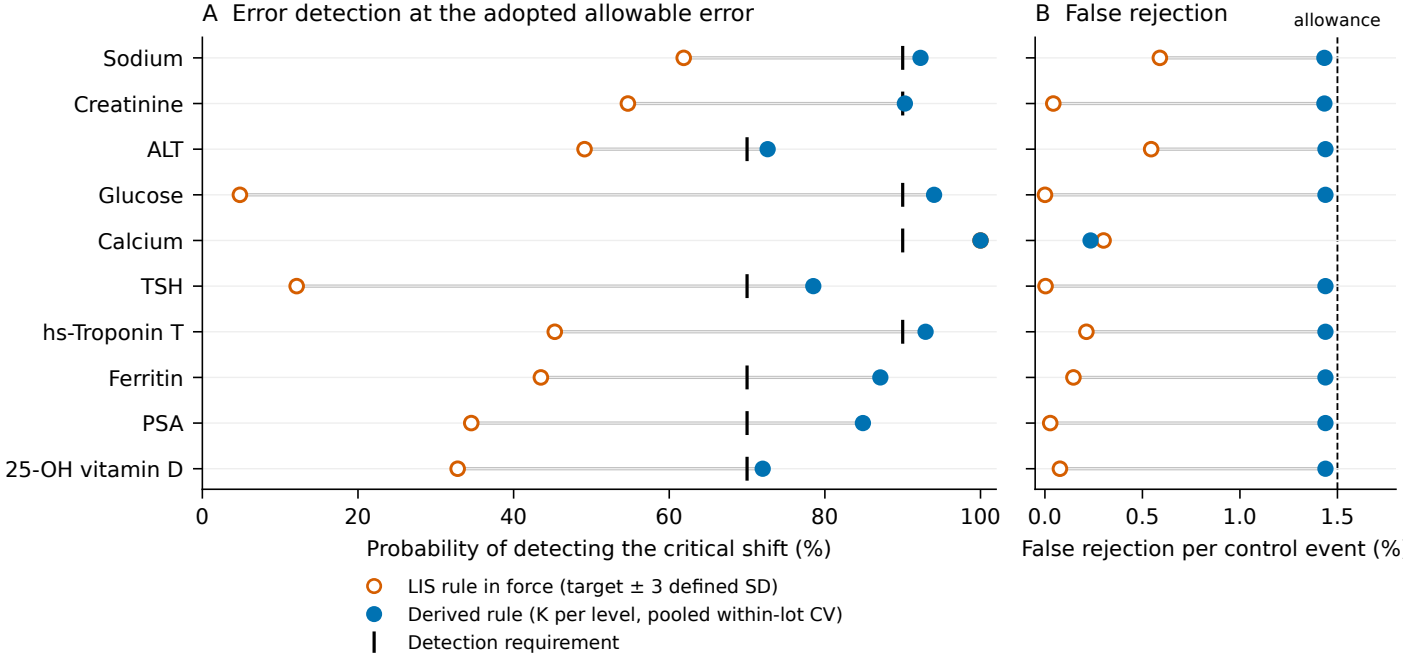
A Error detection at the adopted allowable error
B False rejection
allowance
Sodium
Creatinine
ALT
Glucose
Calcium
TSH
hs-Troponin T
Ferritin
PSA
25-OH vitamin D
0
20
40
60
80
100
0.0
0.5
1.0
1.5
Probability of detecting the critical shift (%)
False rejection per control event (%)
LIS rule in force (target ± 3 defined SD)
Derived rule (K per level, pooled within-lot CV)
Detection requirement