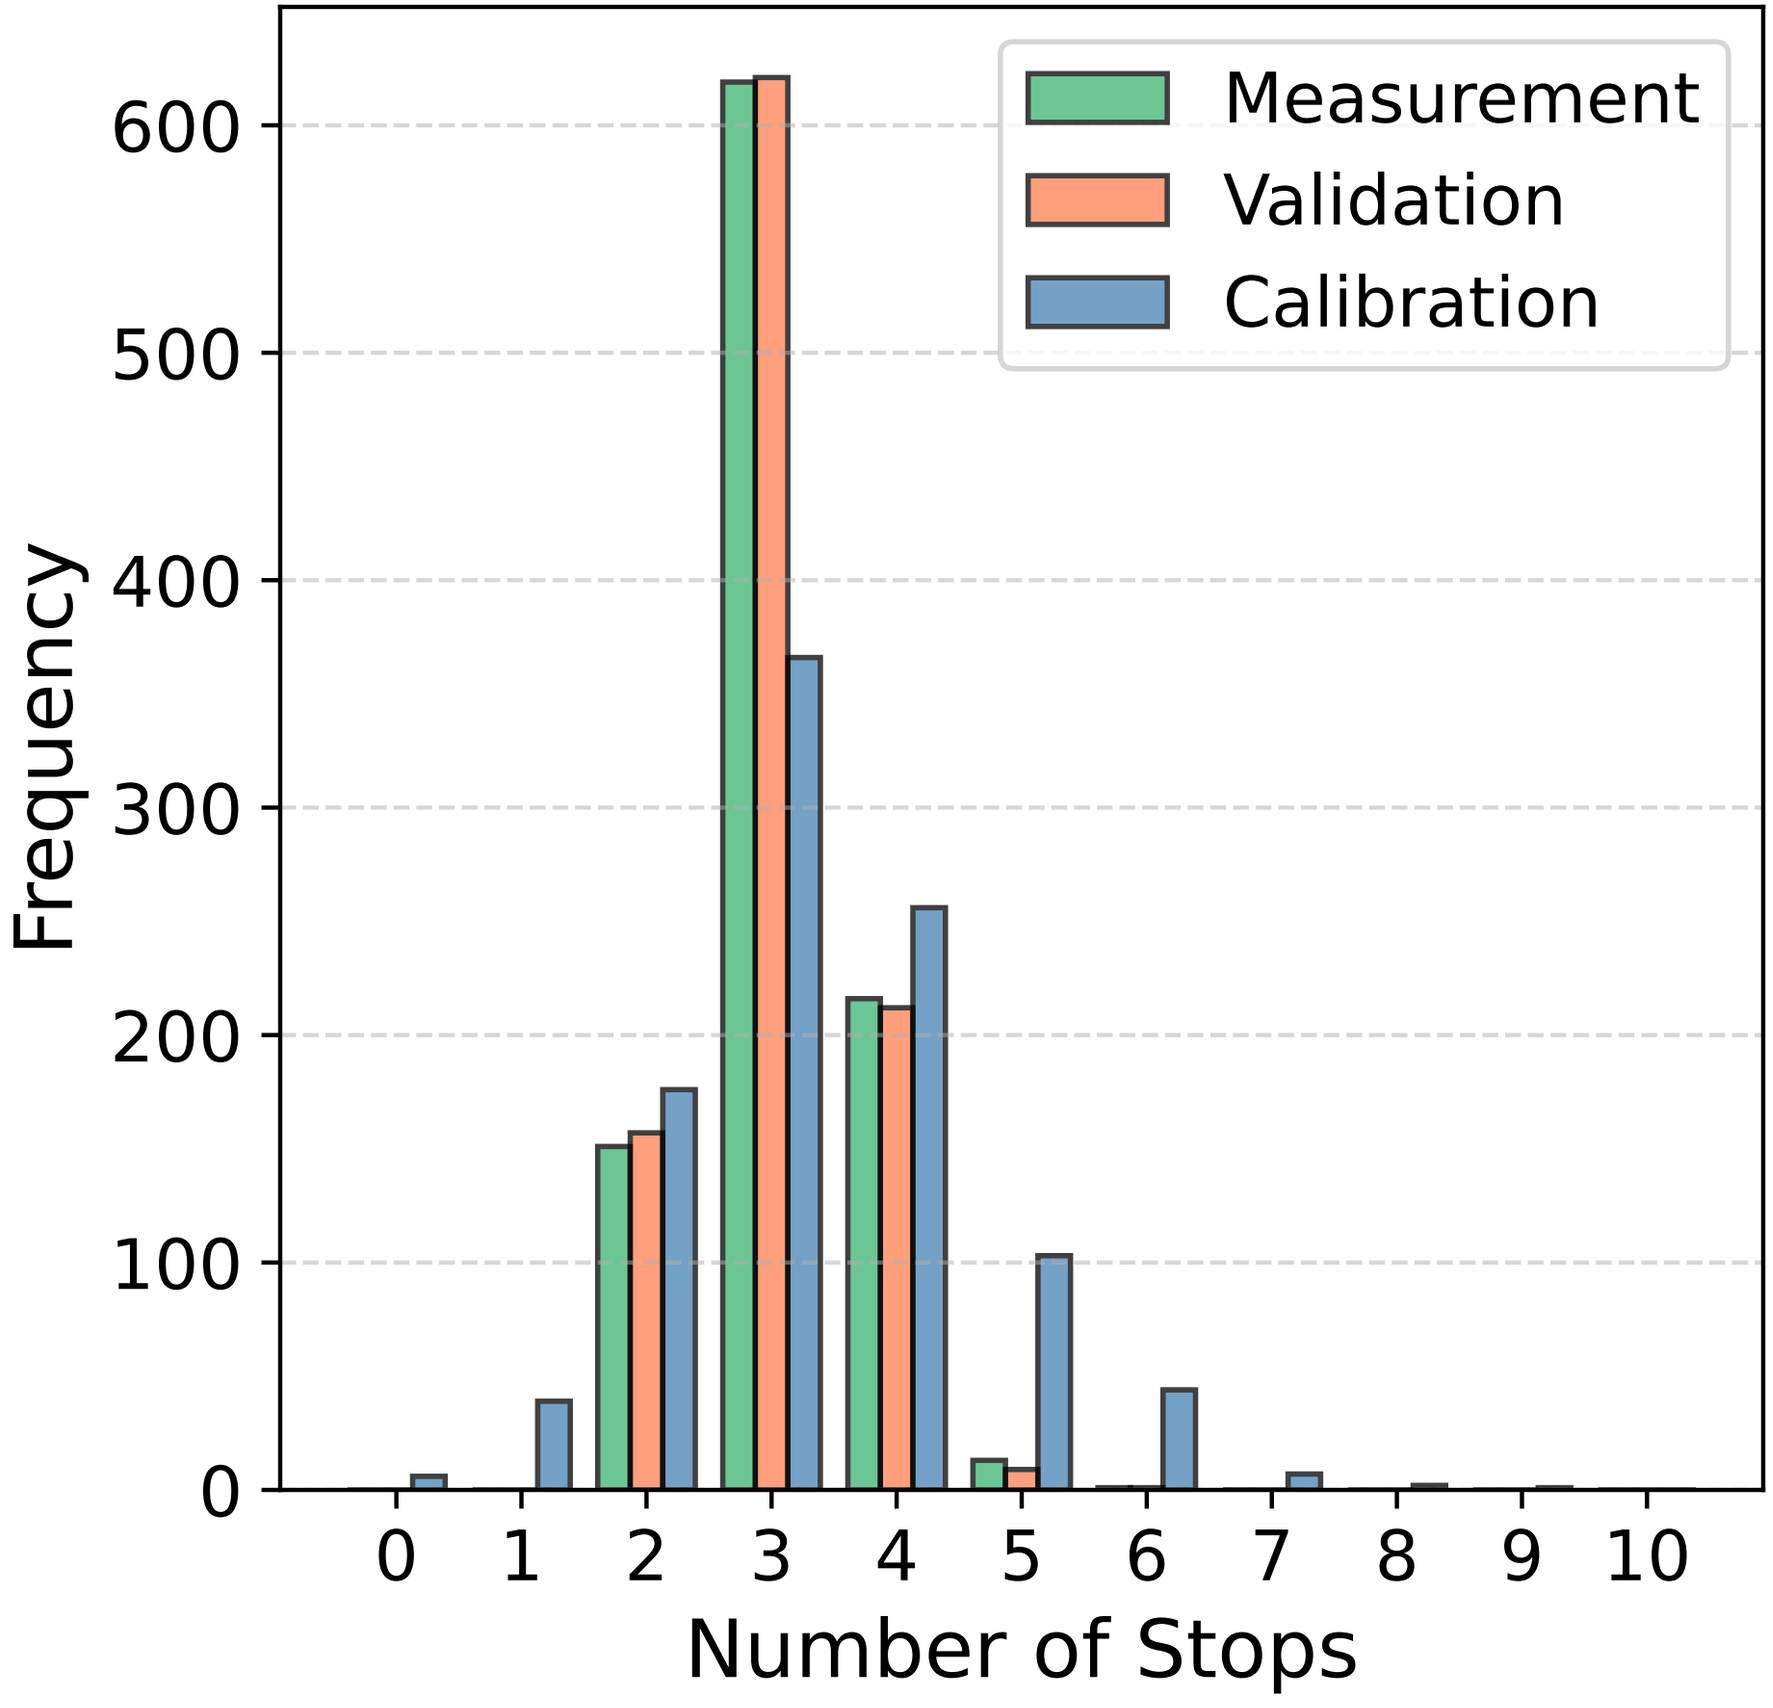
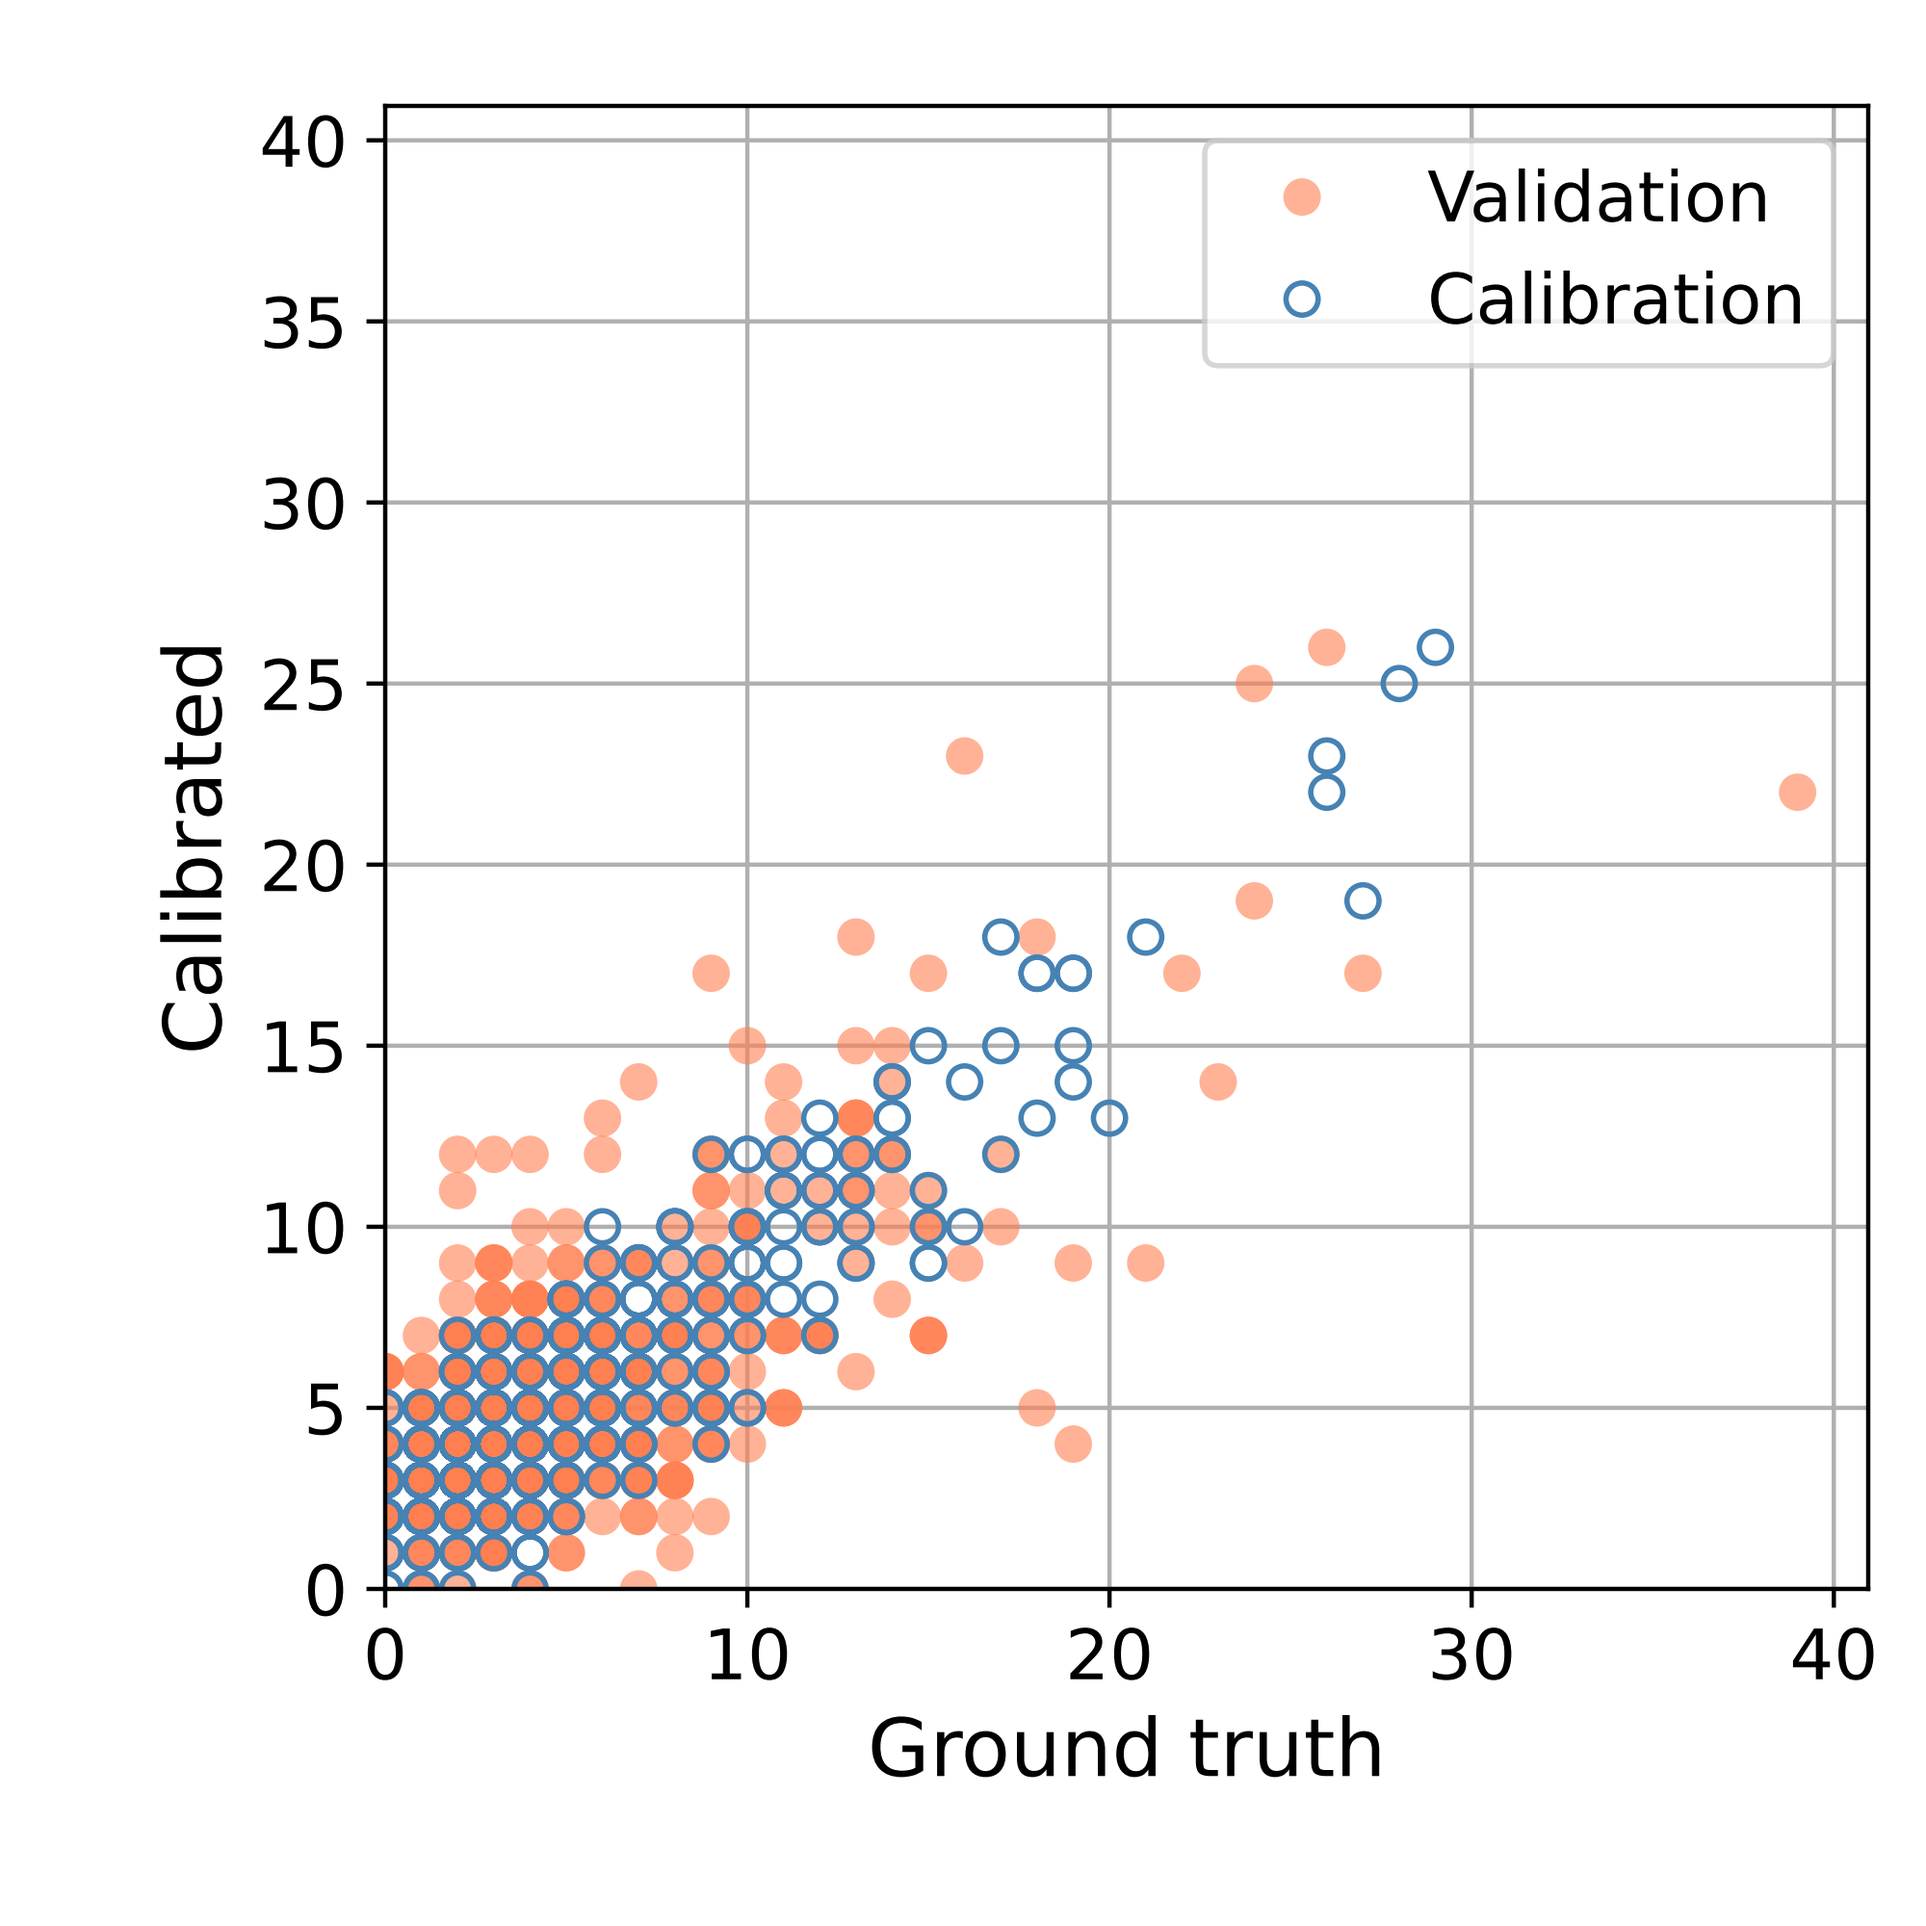
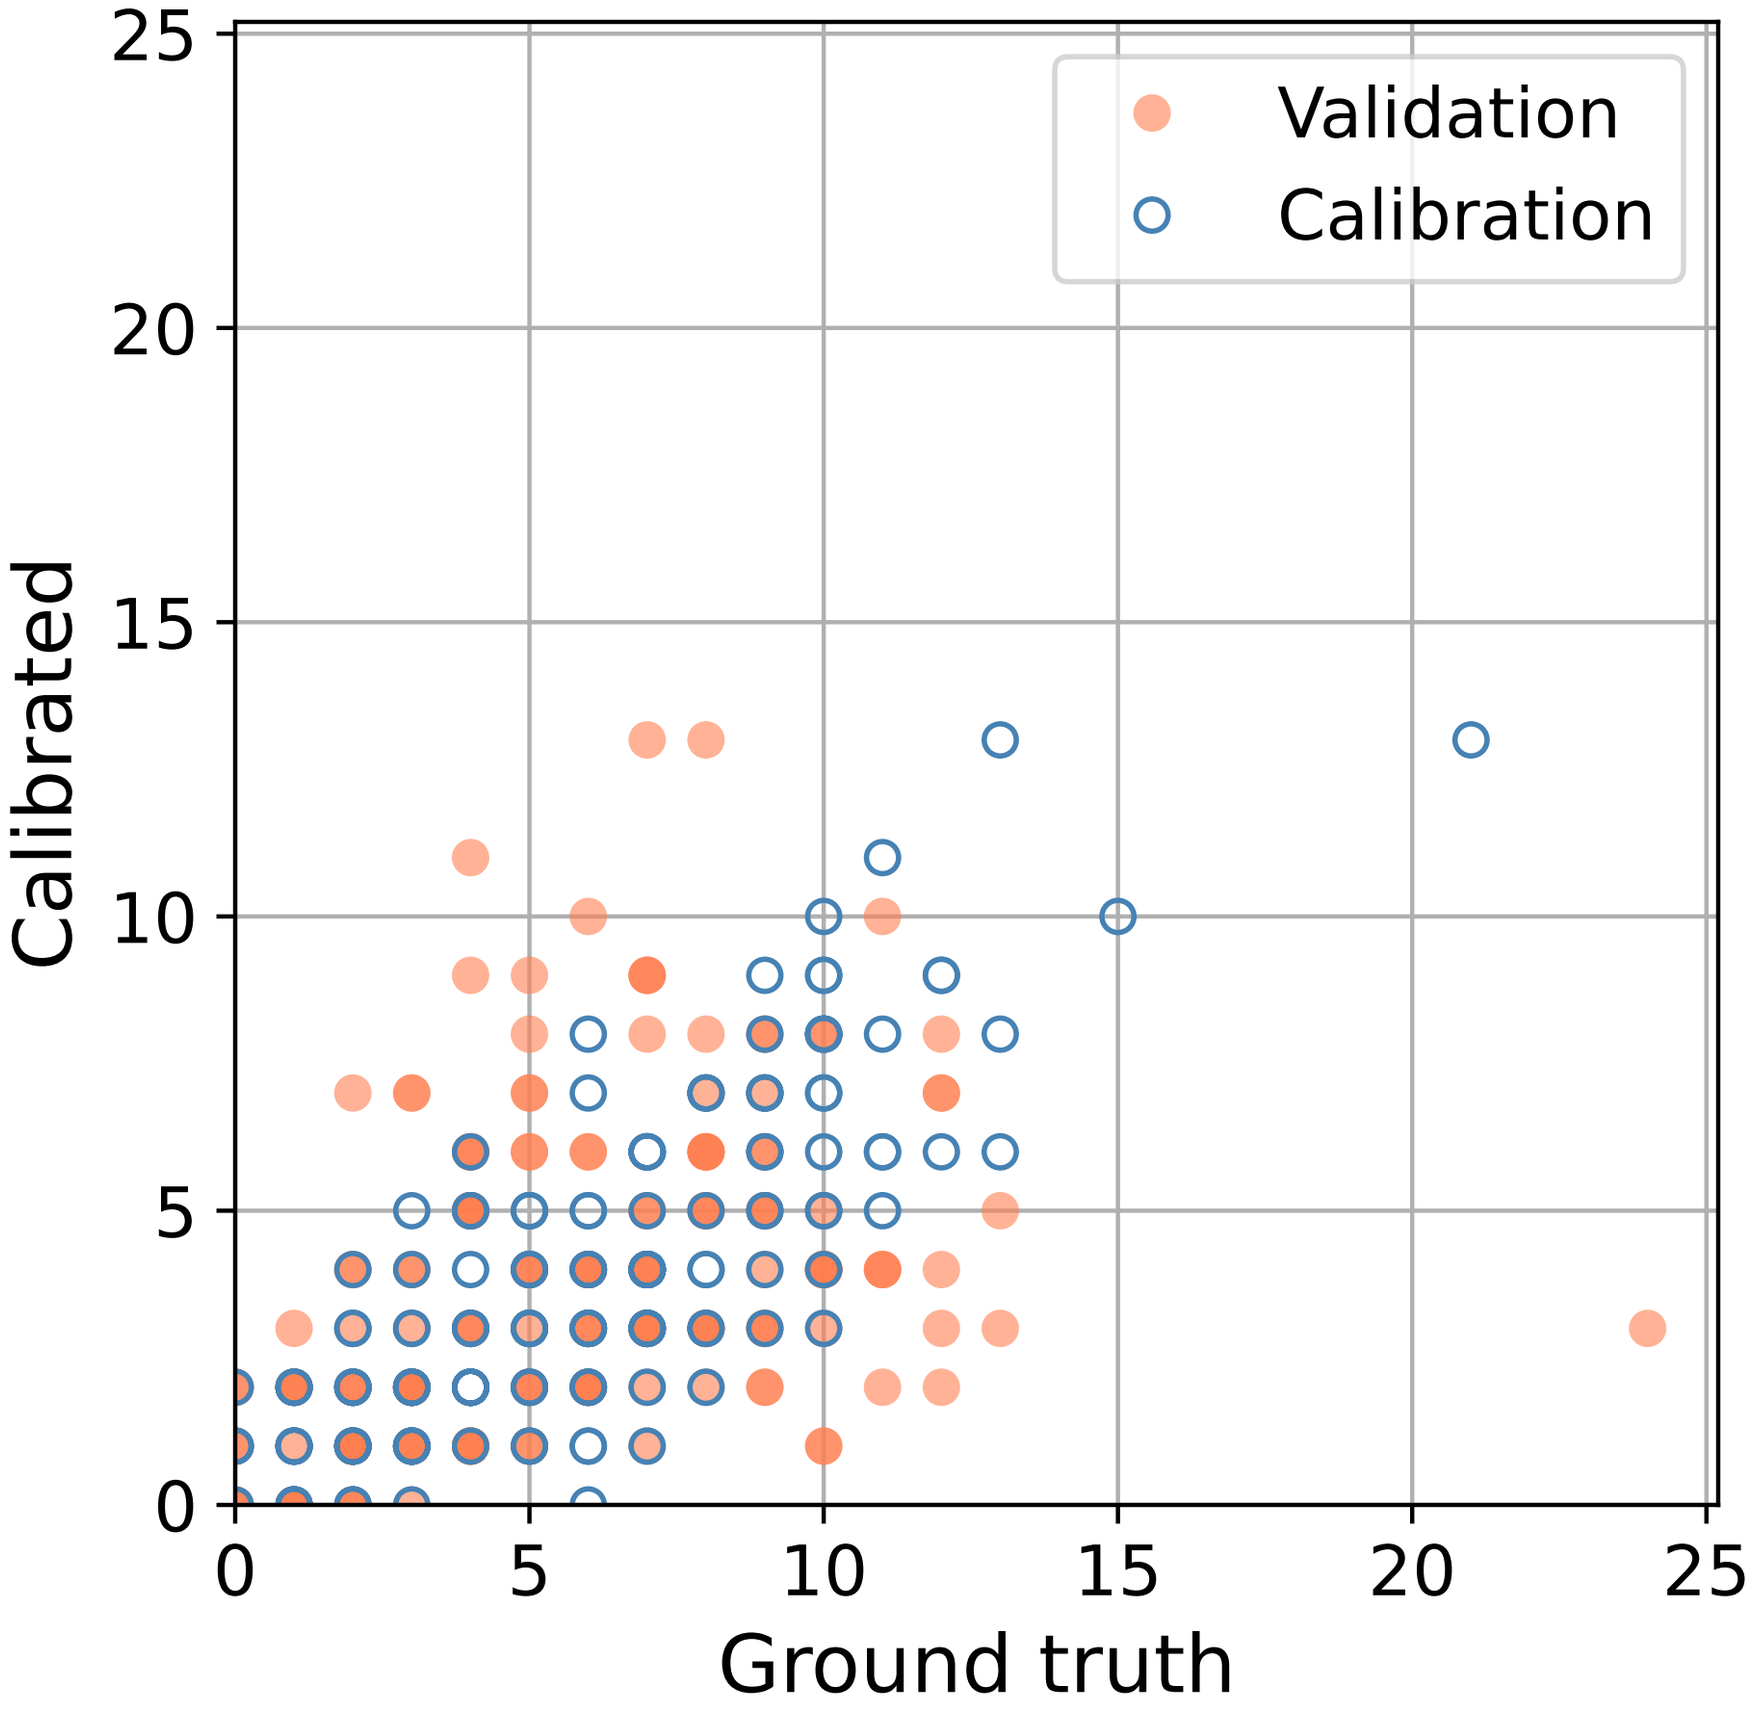
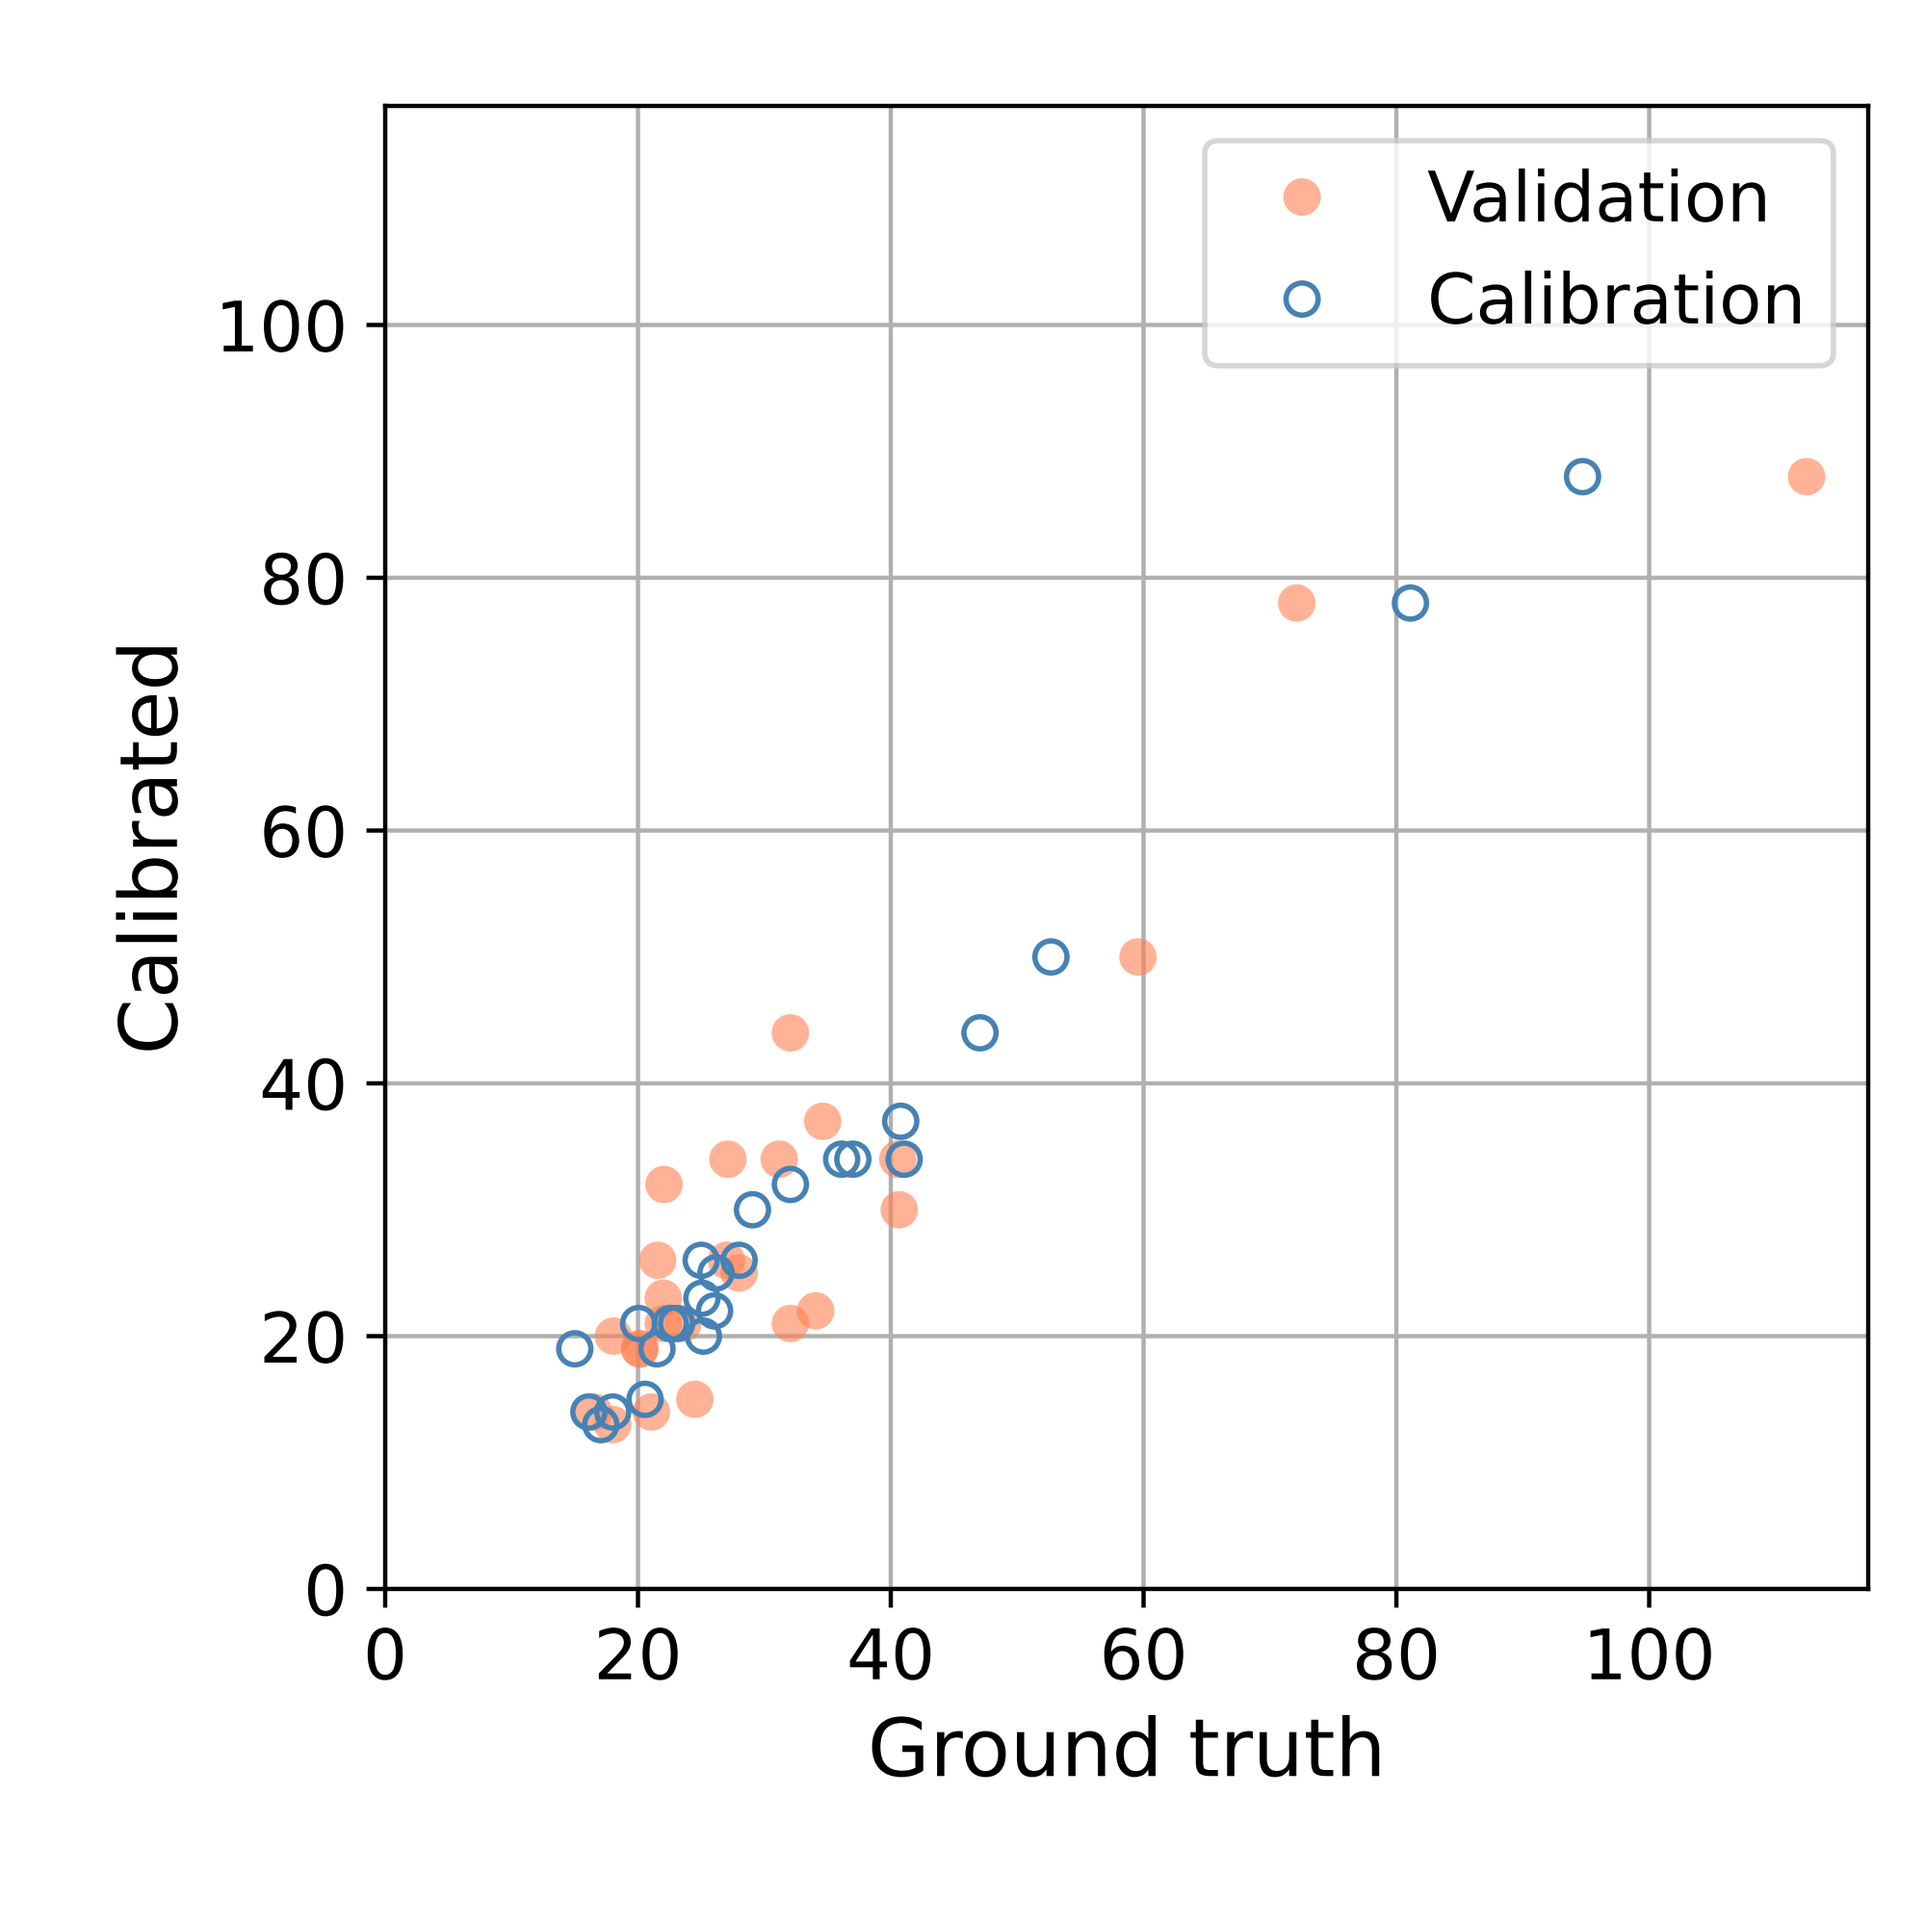
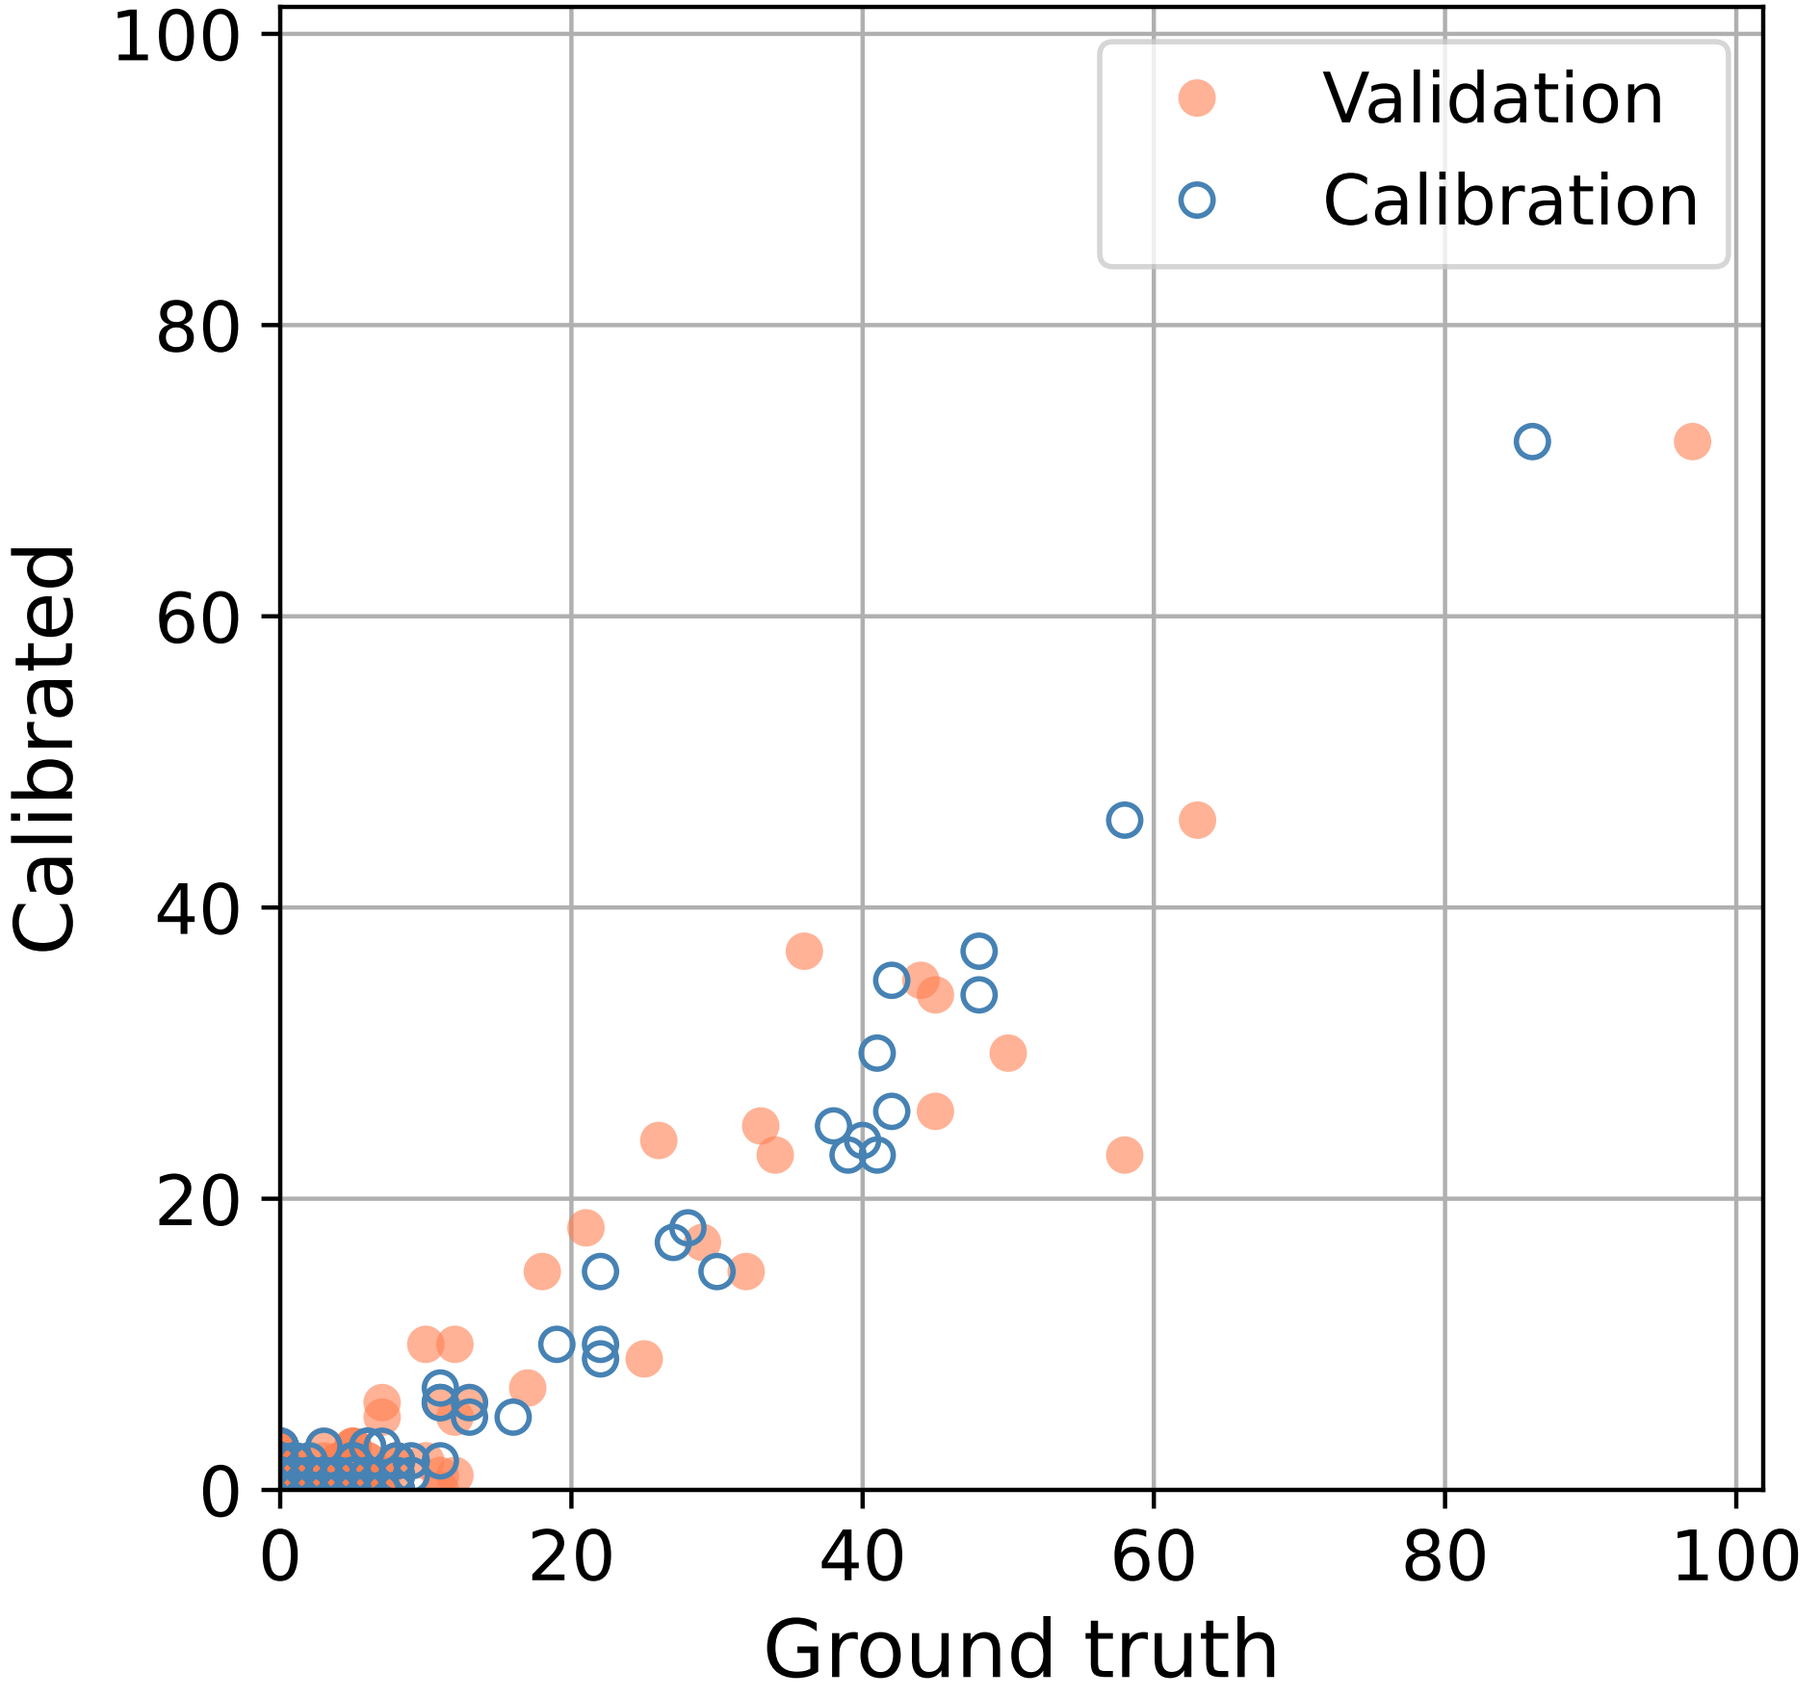
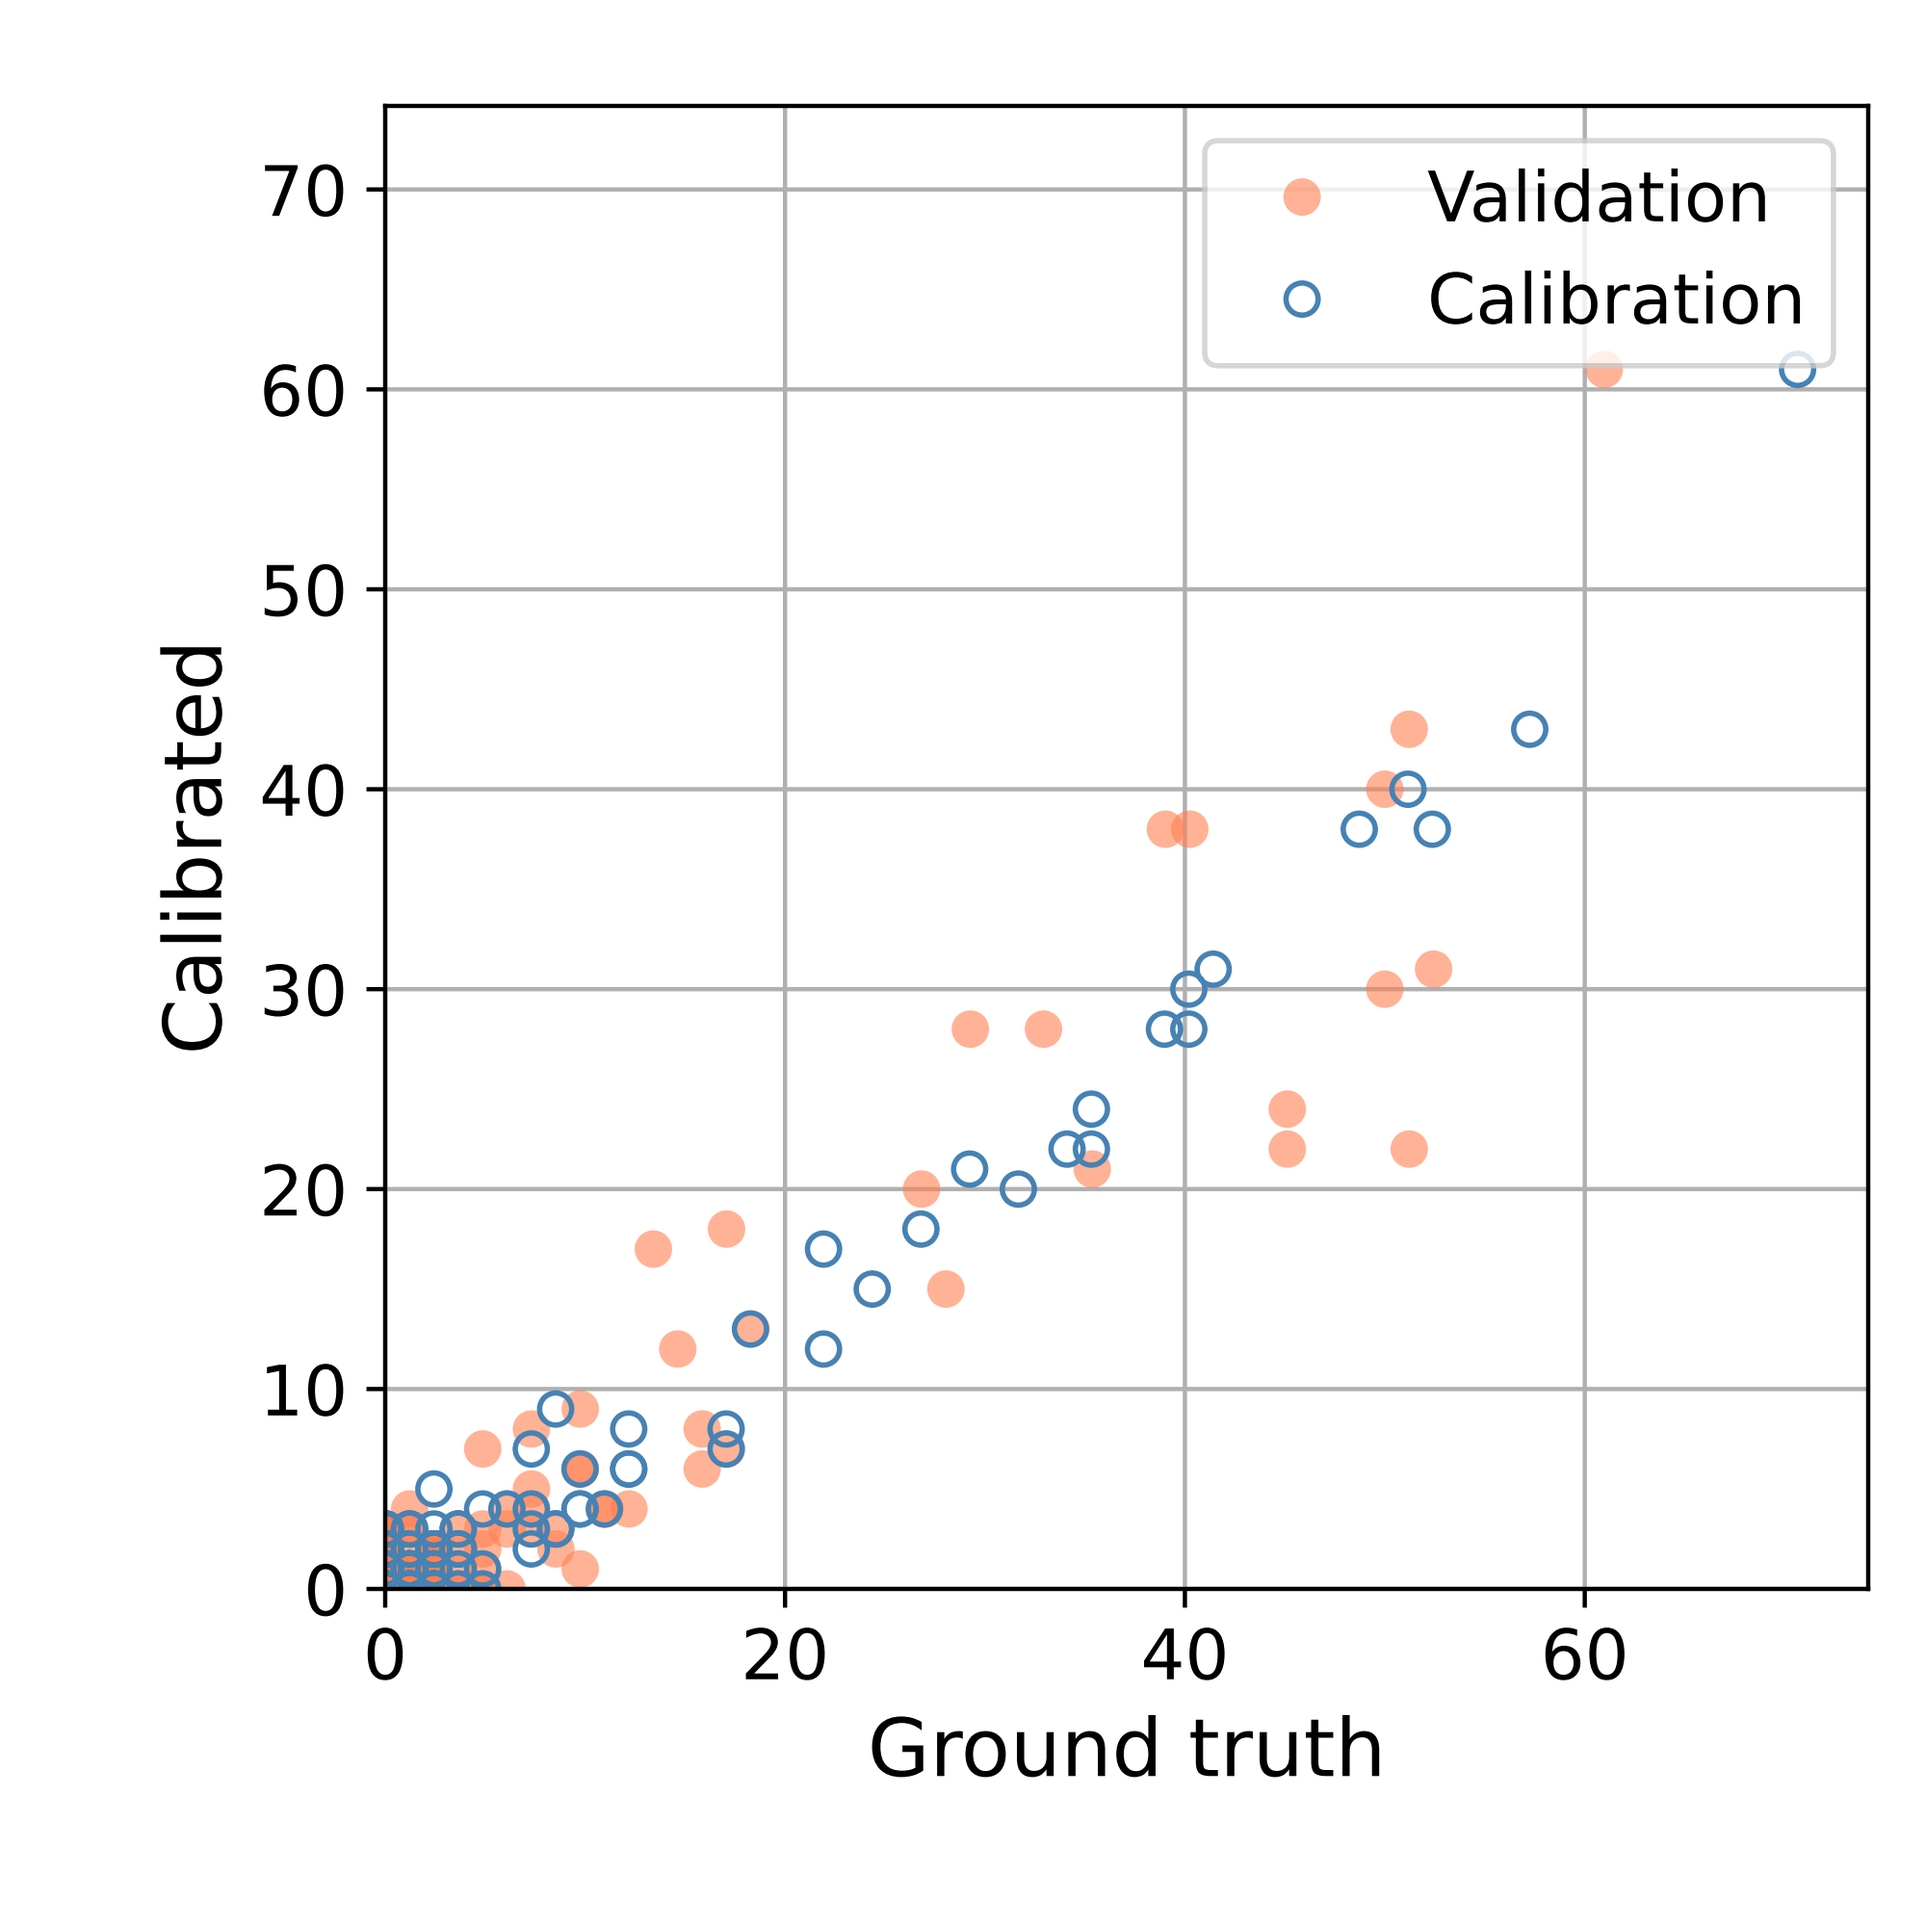

Measurement
Validation
Calibration
Frequency
600
500
400
300
200
100
0
0
1
2
3
4
5
6
7
8
9
10
Number of Stops

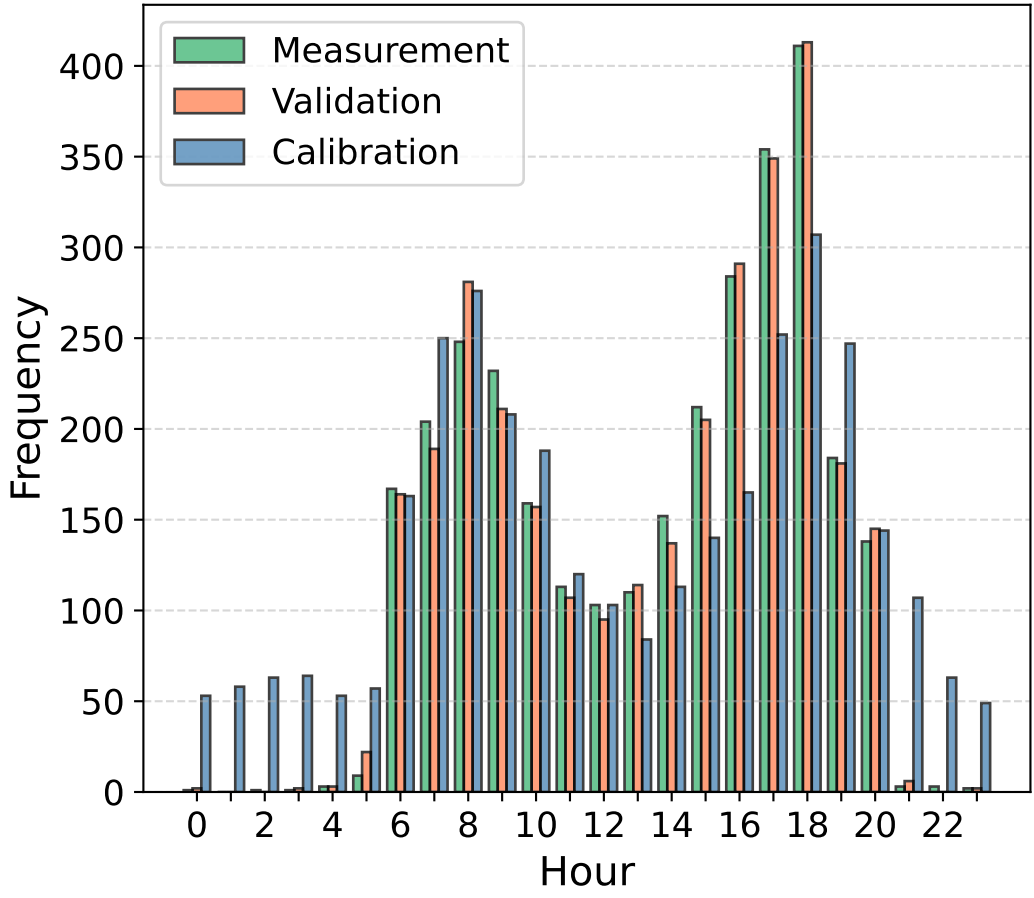

Validation
Calibration
Calibrated
Ground truth
0
5
10
15
20
25
30
35
40
0
10
20
30
40


Validation
Calibration
Calibrated
Ground truth
0
5
10
15
20
25


Validation
Calibration
Calibrated
Ground truth
0
20
40
60
80
100


Validation
Calibration
Calibrated
Ground truth
0
20
40
60
80
100


Validation
Calibration
Calibrated
Ground truth
0
10
20
30
40
50
60
70
0
20
40
60


Measurement
Validation
Calibration
Frequency
0
50
100
150
200
250
300
350
400
0
2
4
6
8
10
12
14
16
18
20
22
Hour