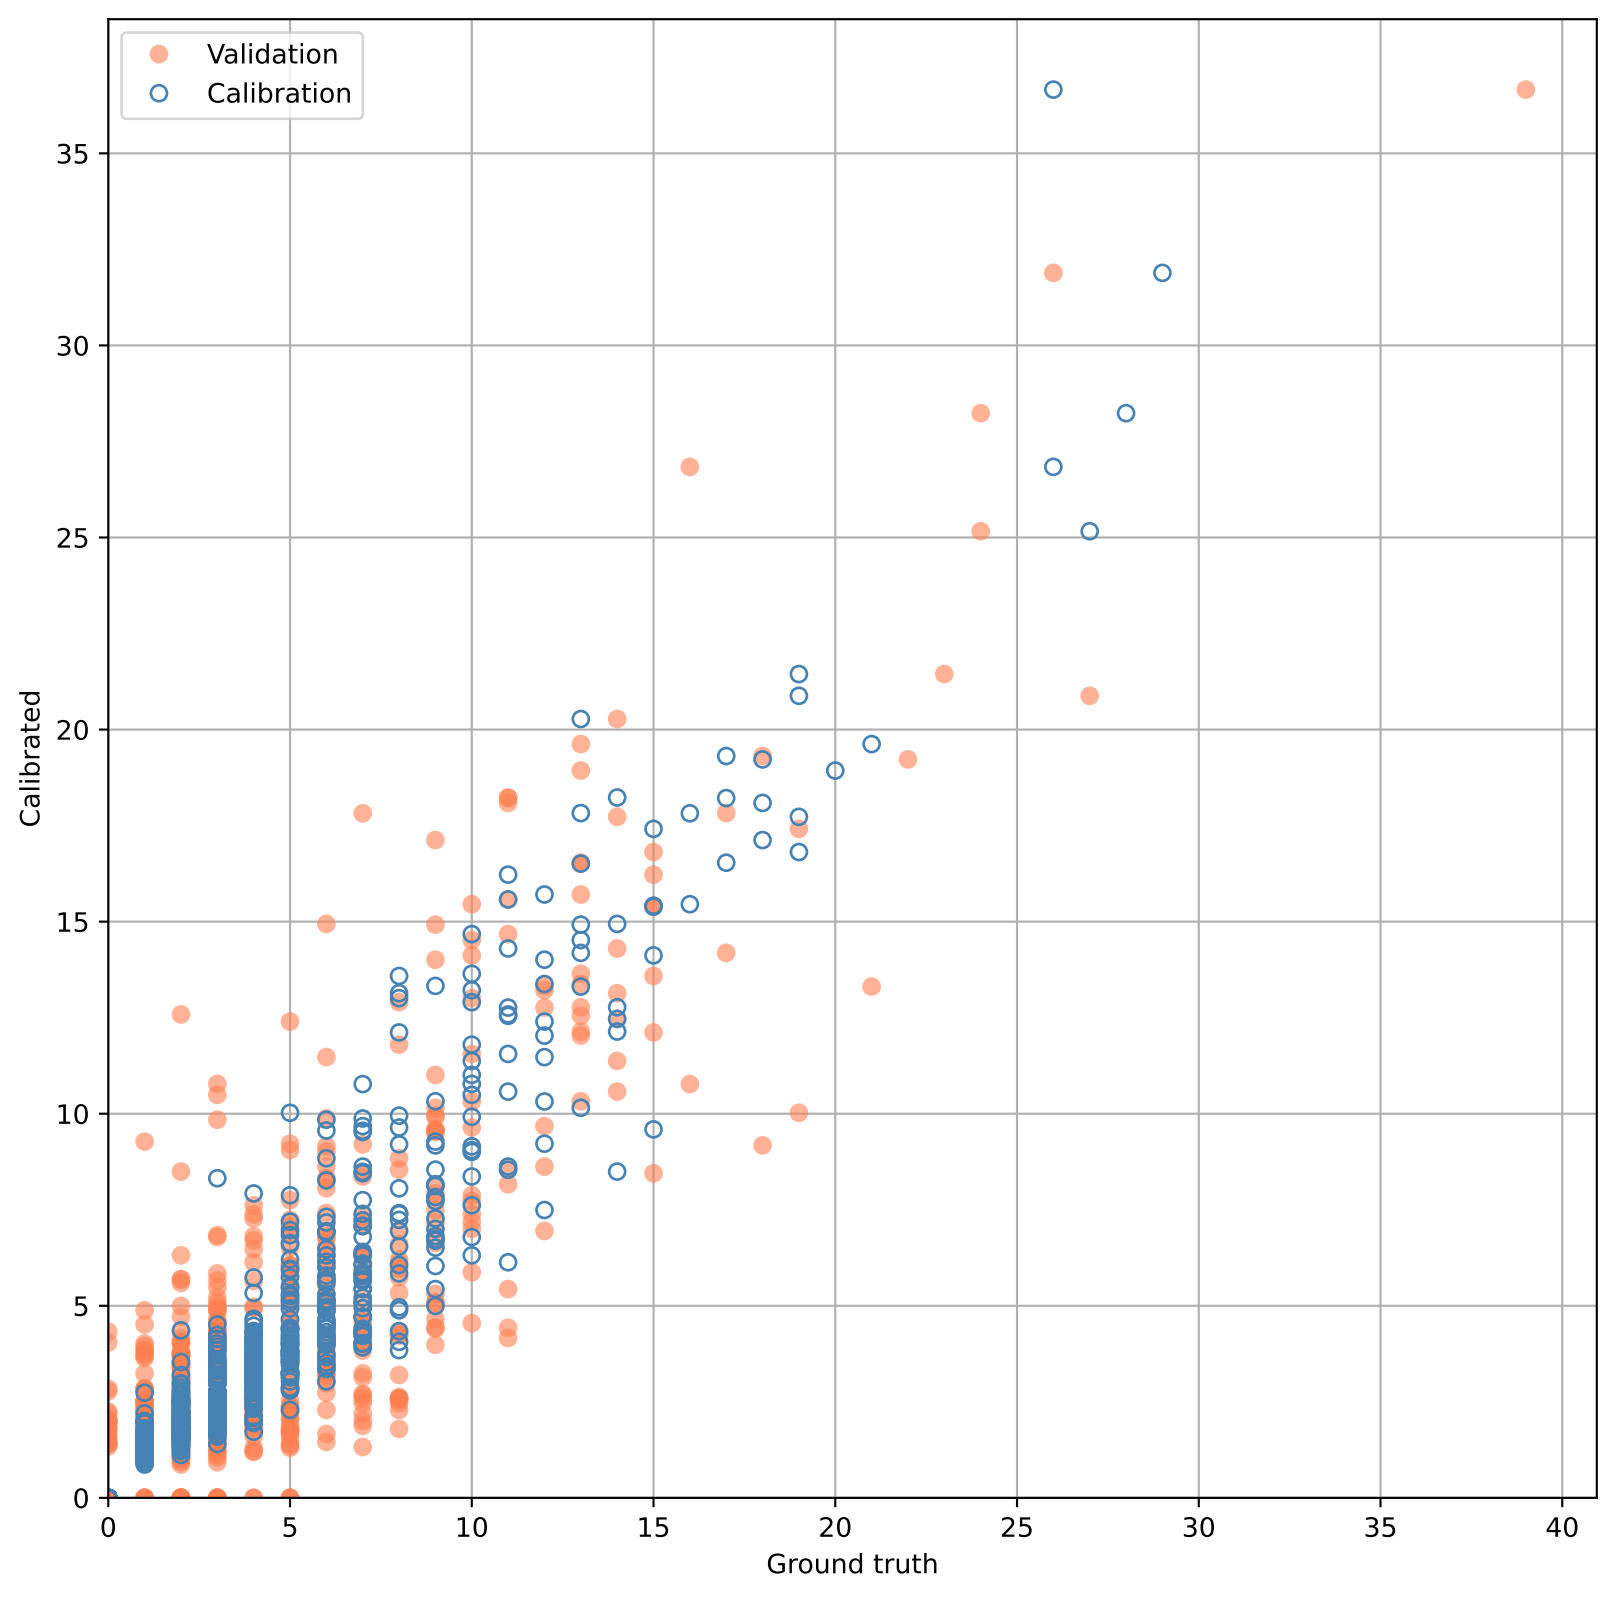
Validation
Calibration
Calibrated
Ground truth
0
5
10
15
20
25
30
35
40