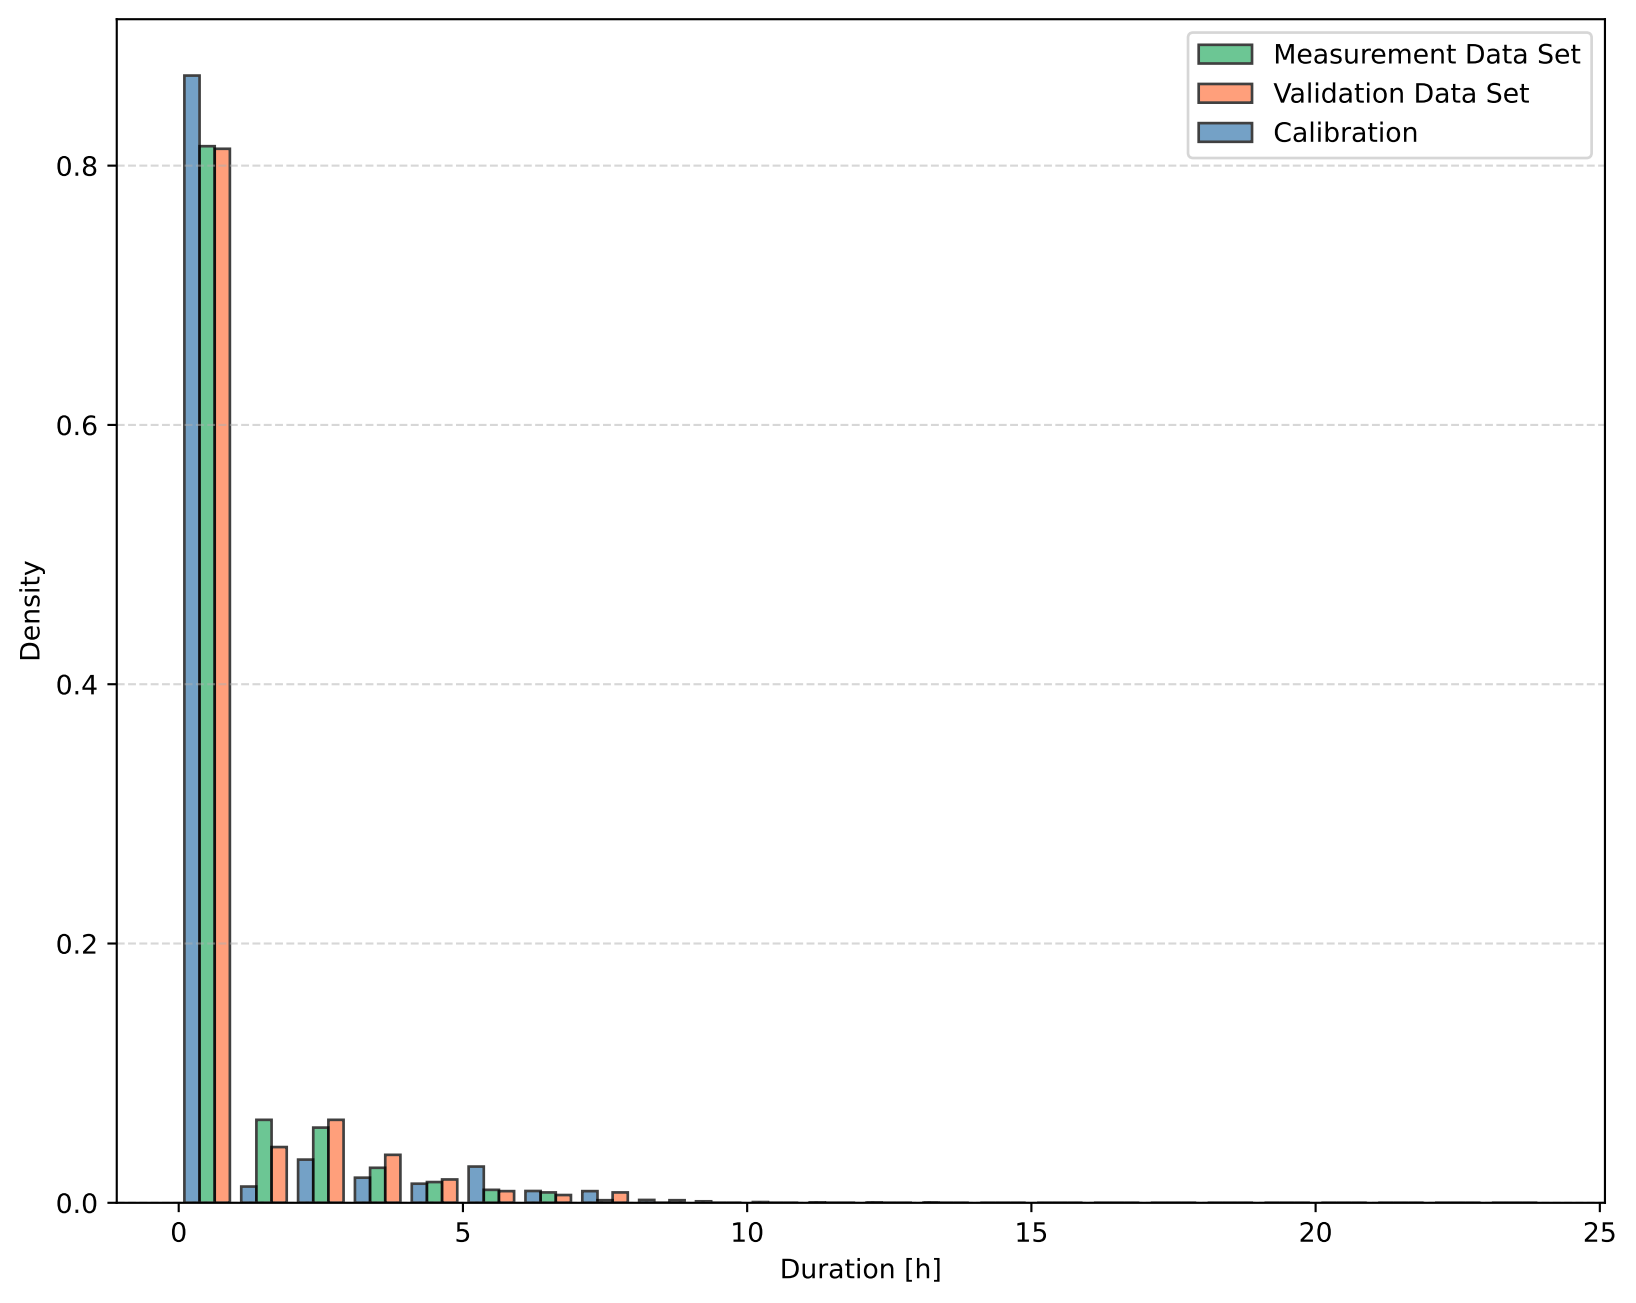
Measurement Data Set
Validation Data Set
Calibration
Density
0.0
0.2
0.4
0.6
0.8
0
5
10
15
20
25
Duration [h]