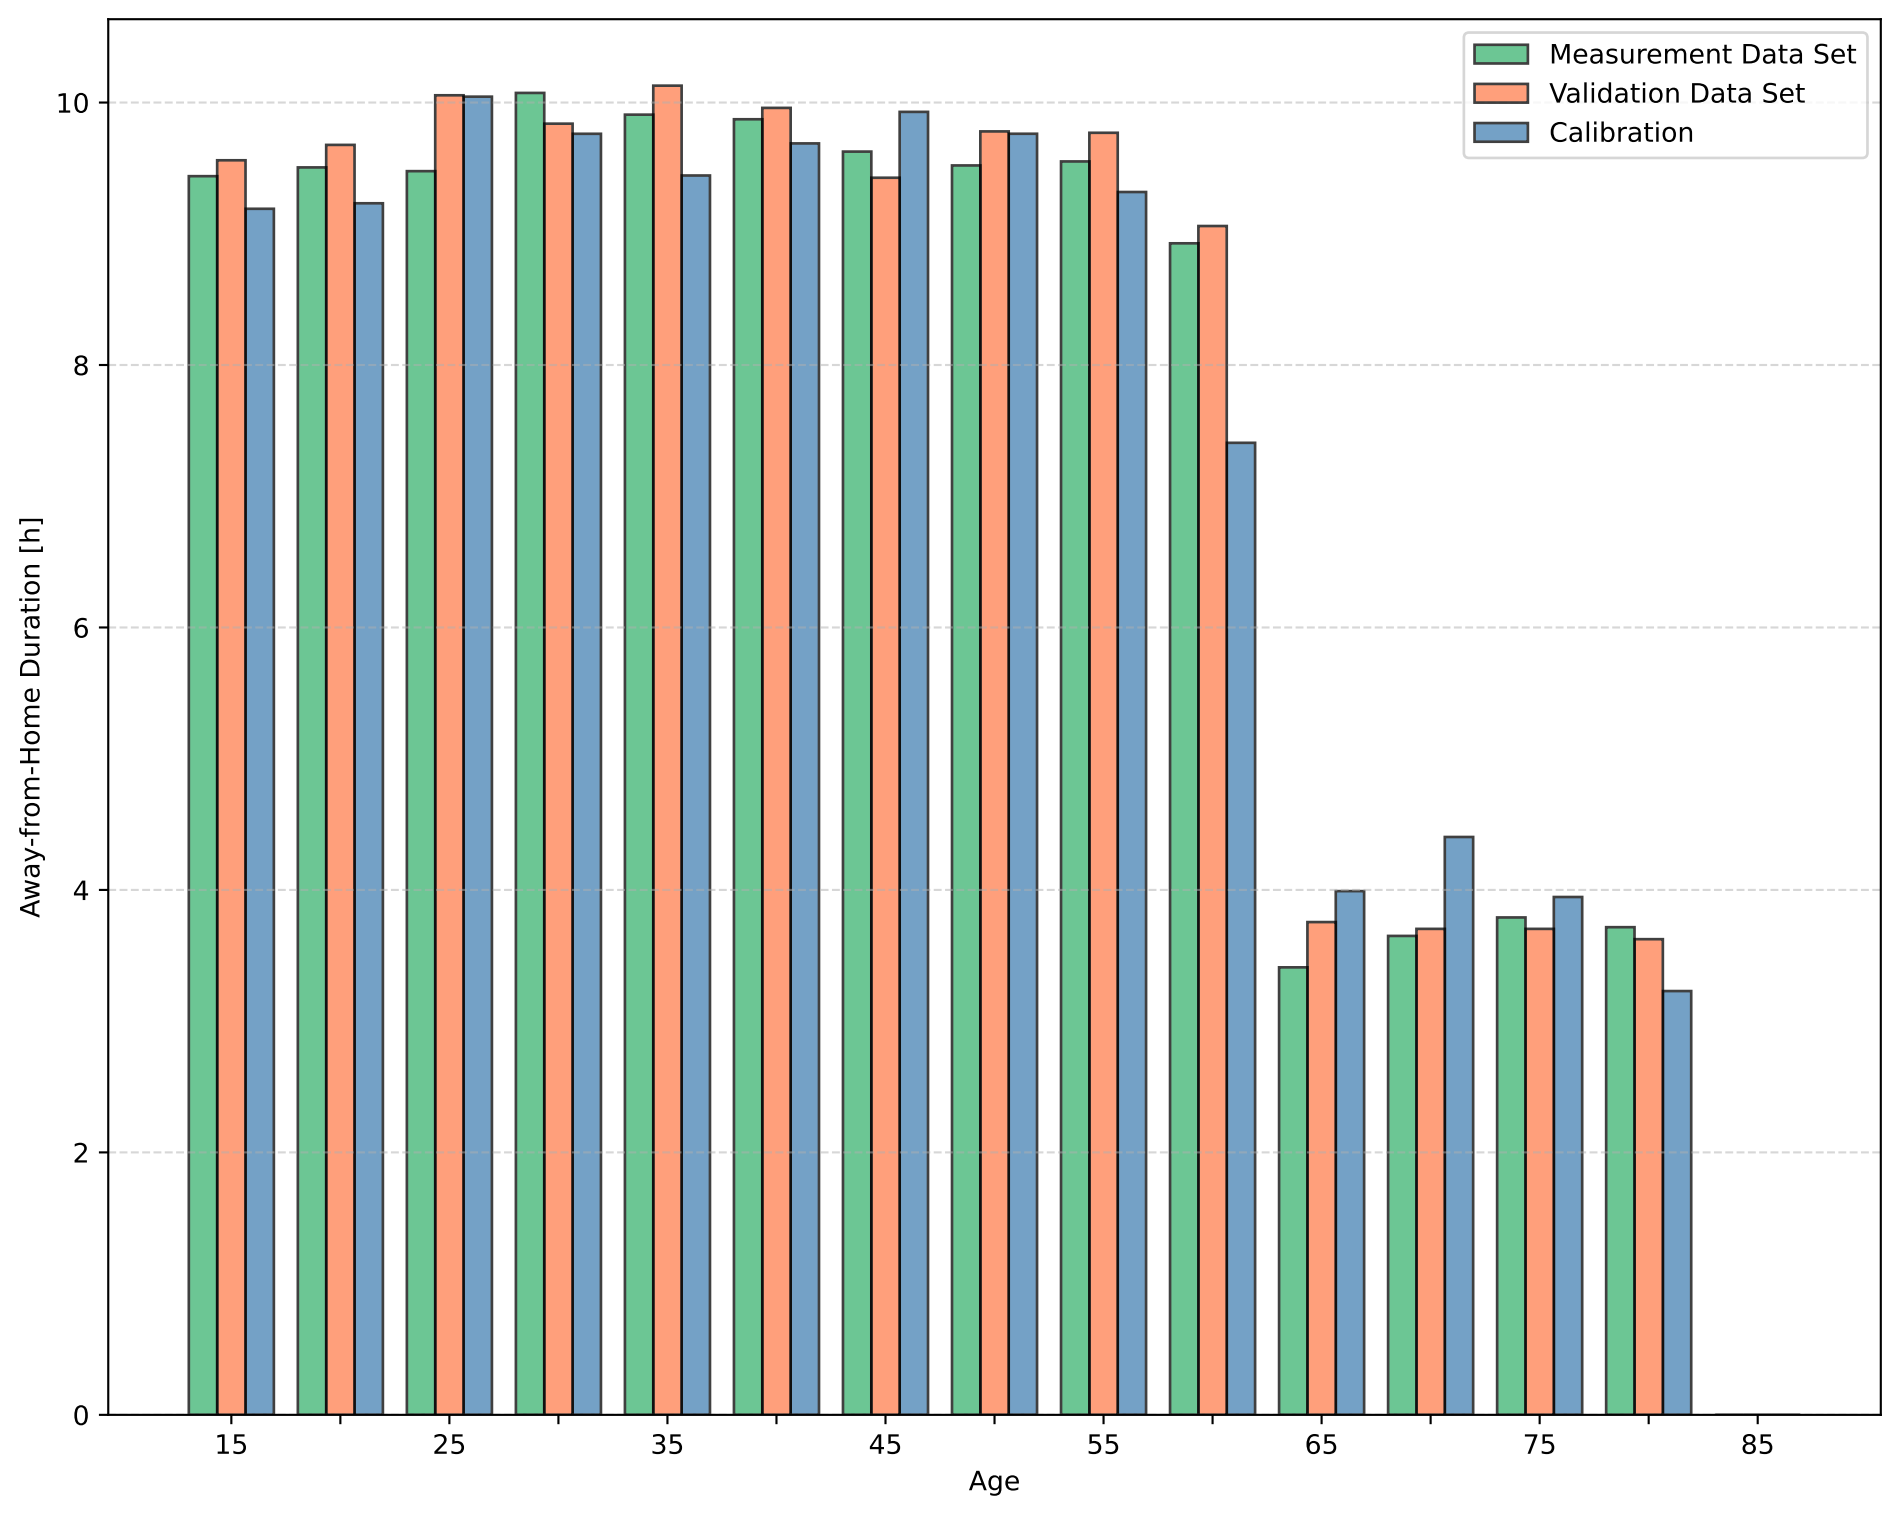
Measurement Data Set
Validation Data Set
Calibration
Away-from-Home Duration [h]
0
2
4
6
8
10
15
25
35
45
55
65
75
85
Age