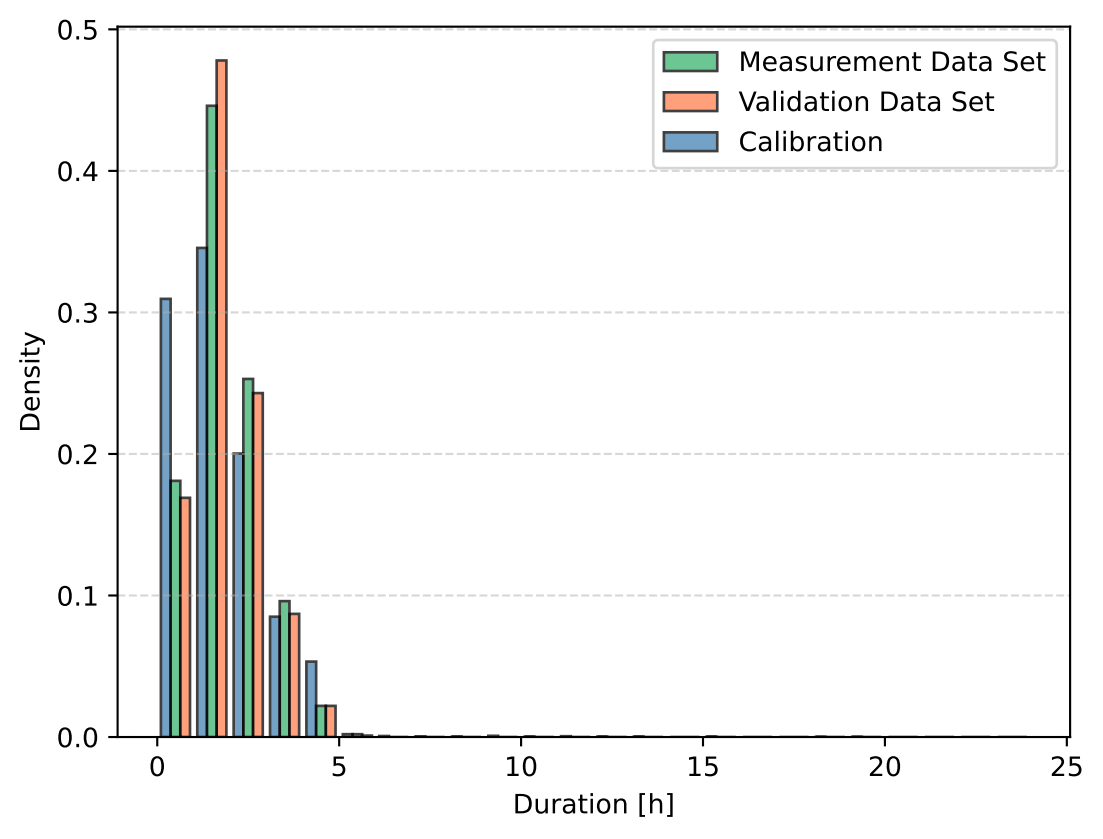
Measurement Data Set
Validation Data Set
Calibration
Density
Duration [h]
0.0
0.1
0.2
0.3
0.4
0.5
0
5
10
15
20
25