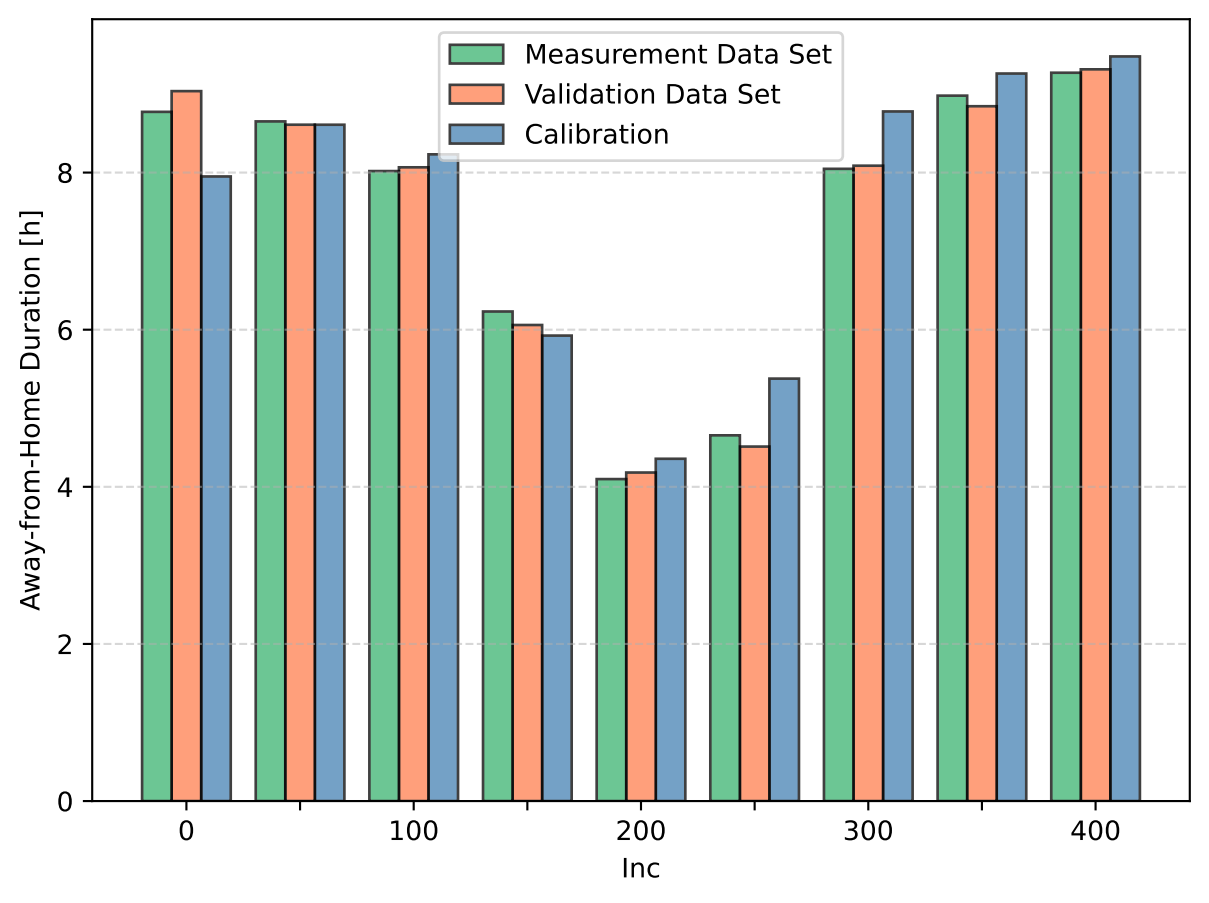
Measurement Data Set
Validation Data Set
Calibration
Away-from-Home Duration [h]
0
2
4
6
8
0
100
200
300
400
Inc