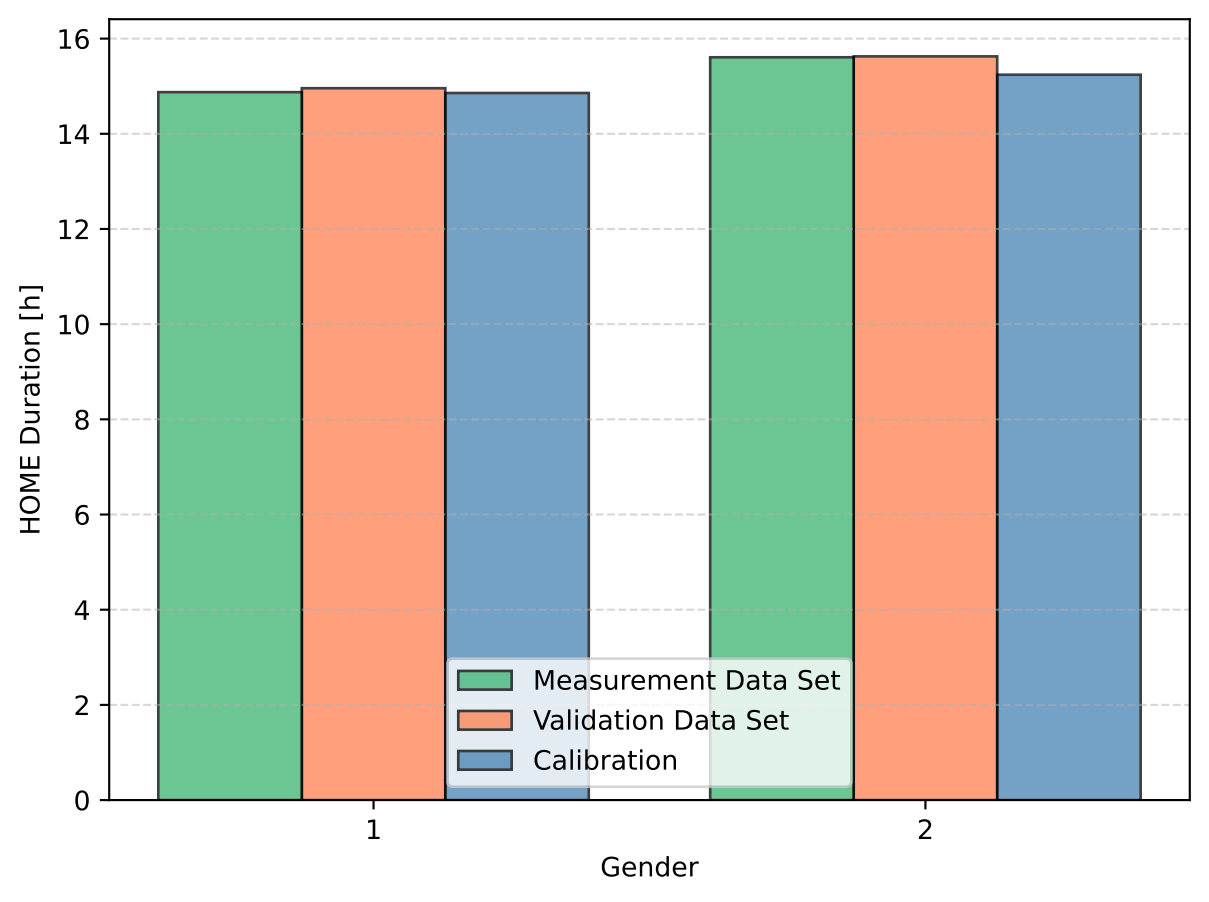
16
14
12
10
8
6
4
2
0
HOME Duration [h]
Measurement Data Set
Validation Data Set
Calibration
1
2
Gender