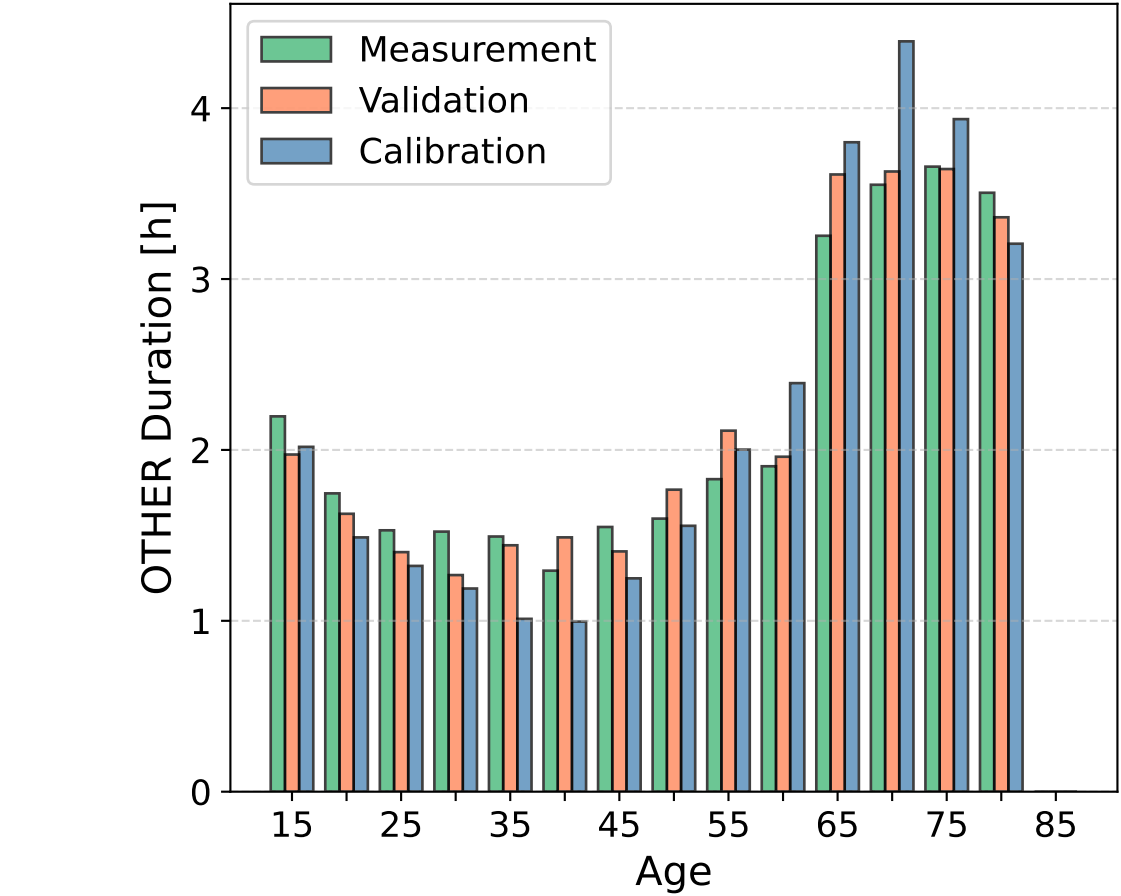
Measurement
Validation
Calibration
OTHER Duration [h]
0
1
2
3
4
15
25
35
45
55
65
75
85
Age