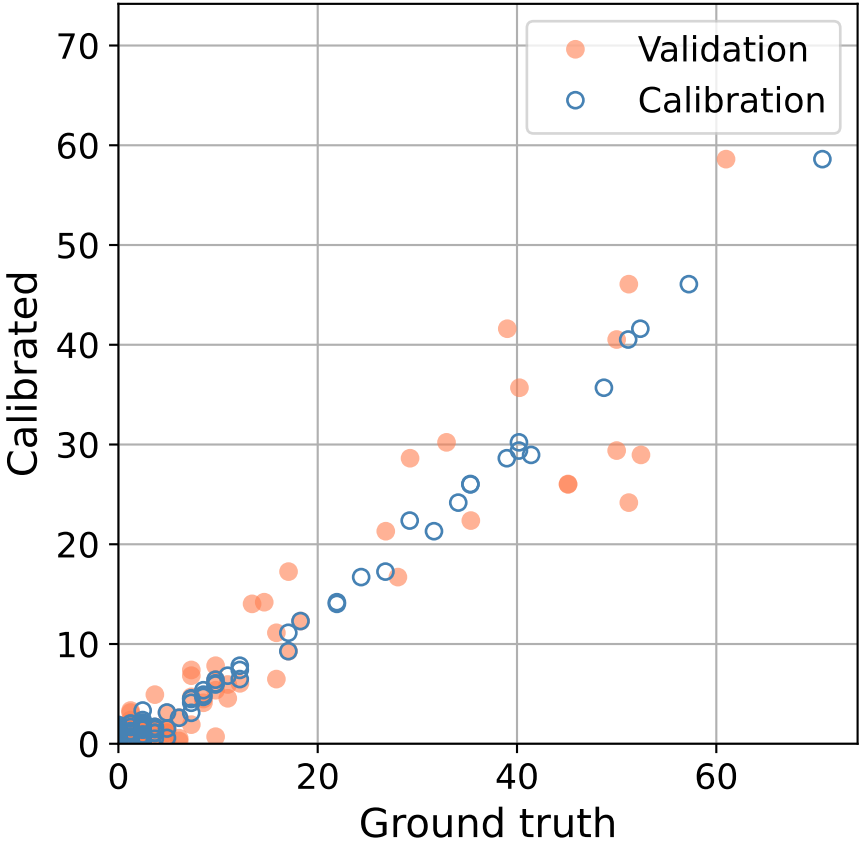
Validation
Calibration
Calibrated
Ground truth
0
10
20
30
40
50
60
70
0
20
40
60