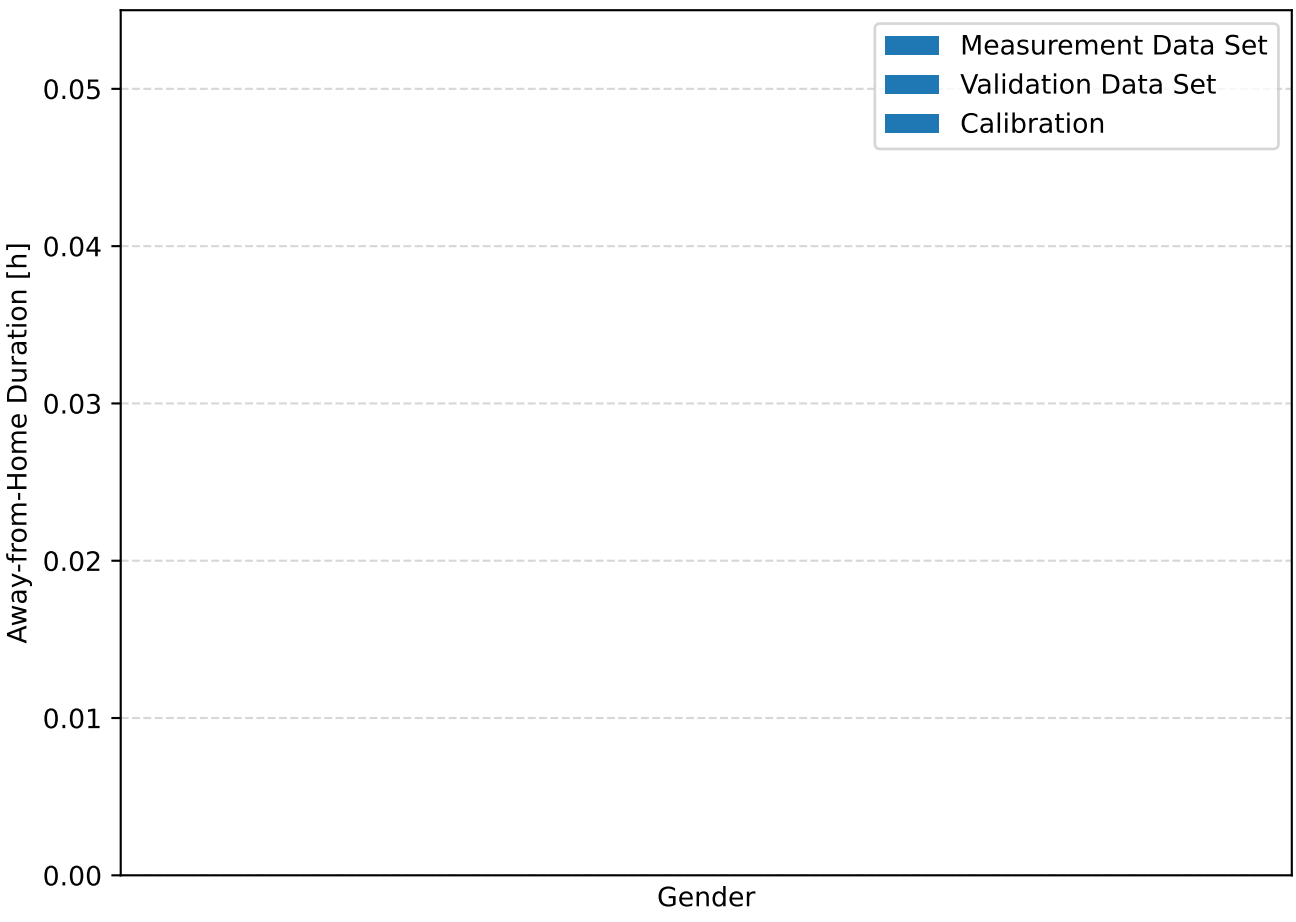
Measurement Data Set
Validation Data Set
Calibration
0.05
0.04
0.03
0.02
0.01
0.00
Away-from-Home Duration [h]
Gender