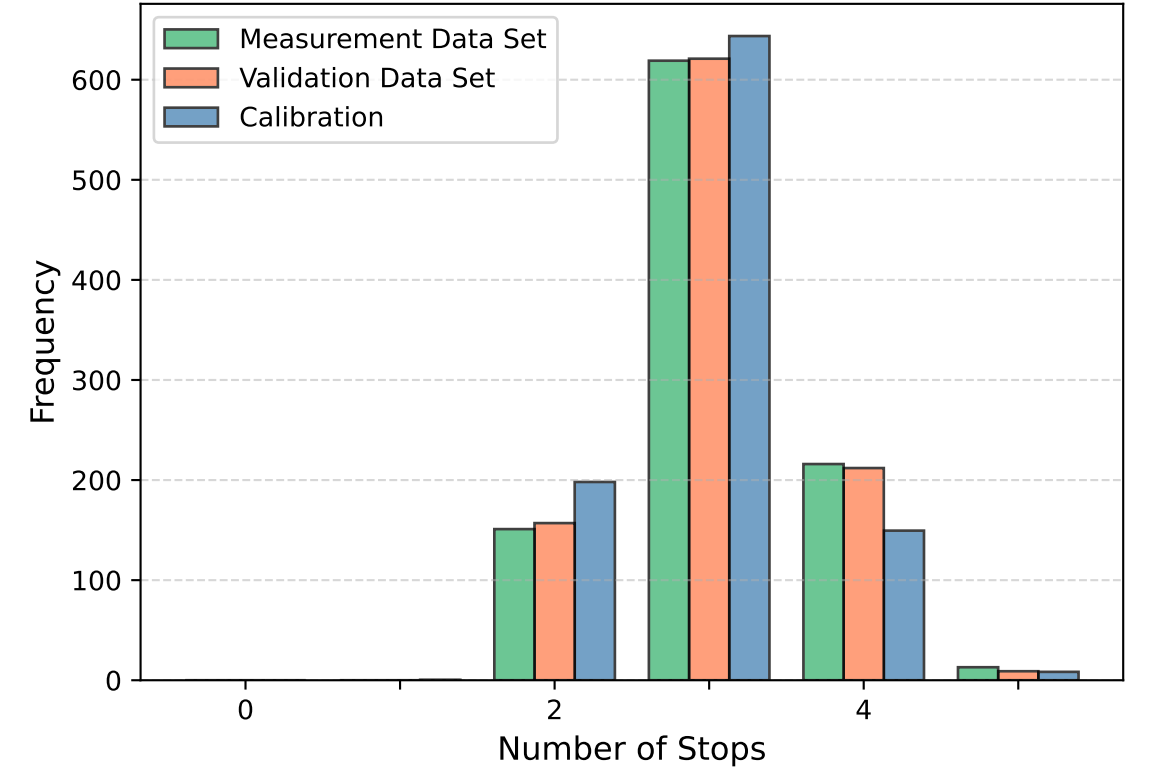
Measurement Data Set
Validation Data Set
Calibration
Frequency
600
500
400
300
200
100
0
0
2
4
Number of Stops