

## INTRODUCTION

Artificial Intelligence has the potential to alter many application domains fundamentally. One prominent example is clinical radiology. The literature hypothesizes that Deep Learning algorithms will profoundly affect the clinical workflow. In this work, we utilized the unprecedented opportunity presented by developing Radiomics to investigate how a *Multi-Modality* Framework and AI could add value in the Medical Imaging (MI) chain, including improvements of workflow efficiency and quality, as well as reducing and preventing errors, or even variability.

## BACKGROUND

A vital component of this research will be the access to a significant number of clinical settings and radiologists (FRANCISCO, 2017; CALISTO, F. M., 2019). Our work, proposes a protocol and guidelines to validate and test the introduction of an *AI-Assisted* Framework with several clinical users. The goal of the test is to compare both current and novel AI approach, measuring the user performance, efficiency and efficacy. Also, we will use an eye-tracking device to track the participant's eye movements during patient diagnosis. The purpose of this framework is to involve an *AI-Assisted* tool (*Assistant*) into several MI technologies at an autonomous patient diagnosis level. For the Machine Learning (ML) and Deep Learning (DL) component we will use several technologies, promoting and feeding our Convolutional Neural Networks (CNN) and Deep Reinforcement Learning (DRL) techniques (MAICAS et al., 2017). Other central component of our framework is a distributed-based PACS pairwise with ubiquitous web technologies and based on *Open Source* (OS) libraries.

List of used technologies that support our work:

- 1 NodeJS;
- 2 CornerstoneJS (HOSTETTER; KHANNA; MANDELL, 2018);
- 3 Orthanc (JODOGNE et al., 2013);

## FRAMEWORK

The next Figures 2, 3 e 4 are samples of our working framework:

Figure 2 – Full UI of the Framework showing a patient's MI.

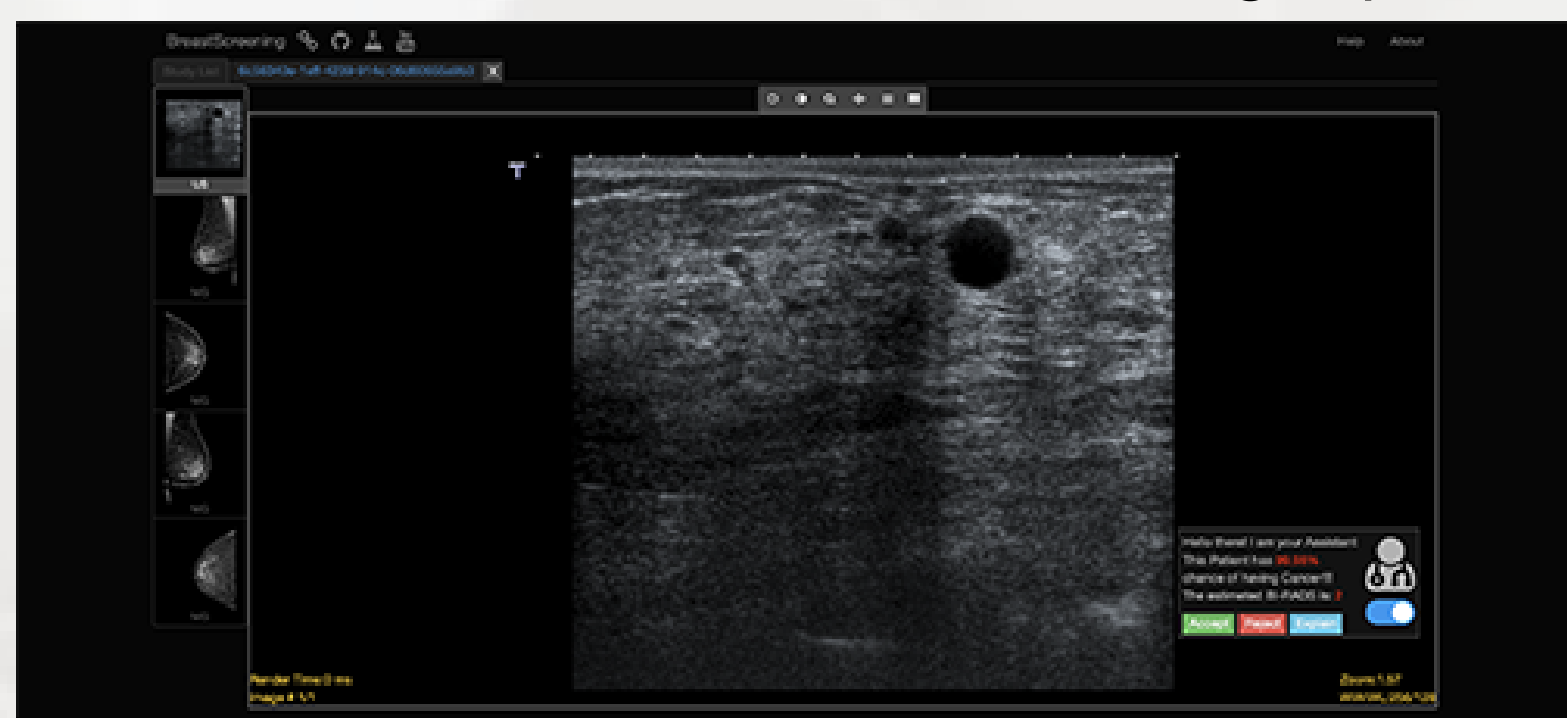


Figure 3 – The Assistant options and buttons.


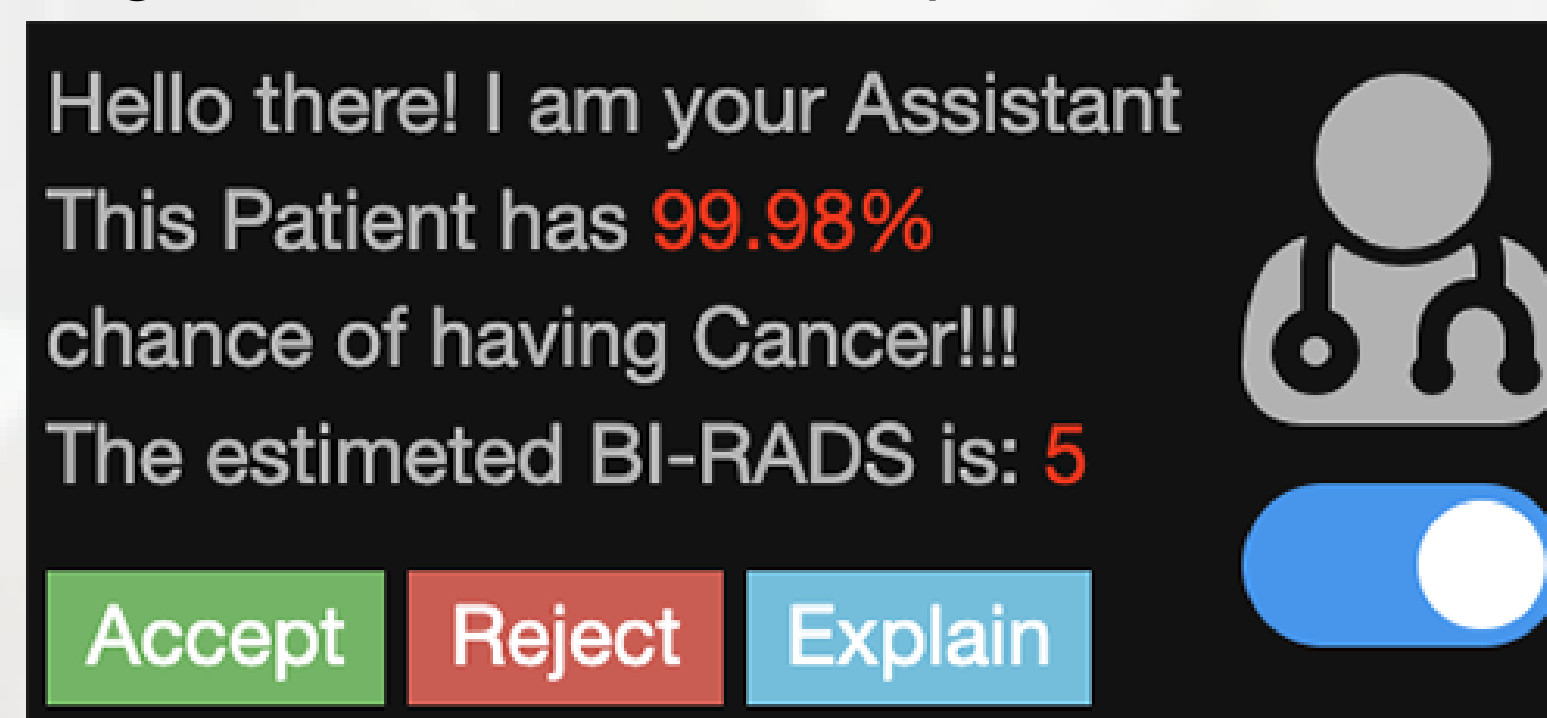


Figure 4 – Result of the "Explain" button.

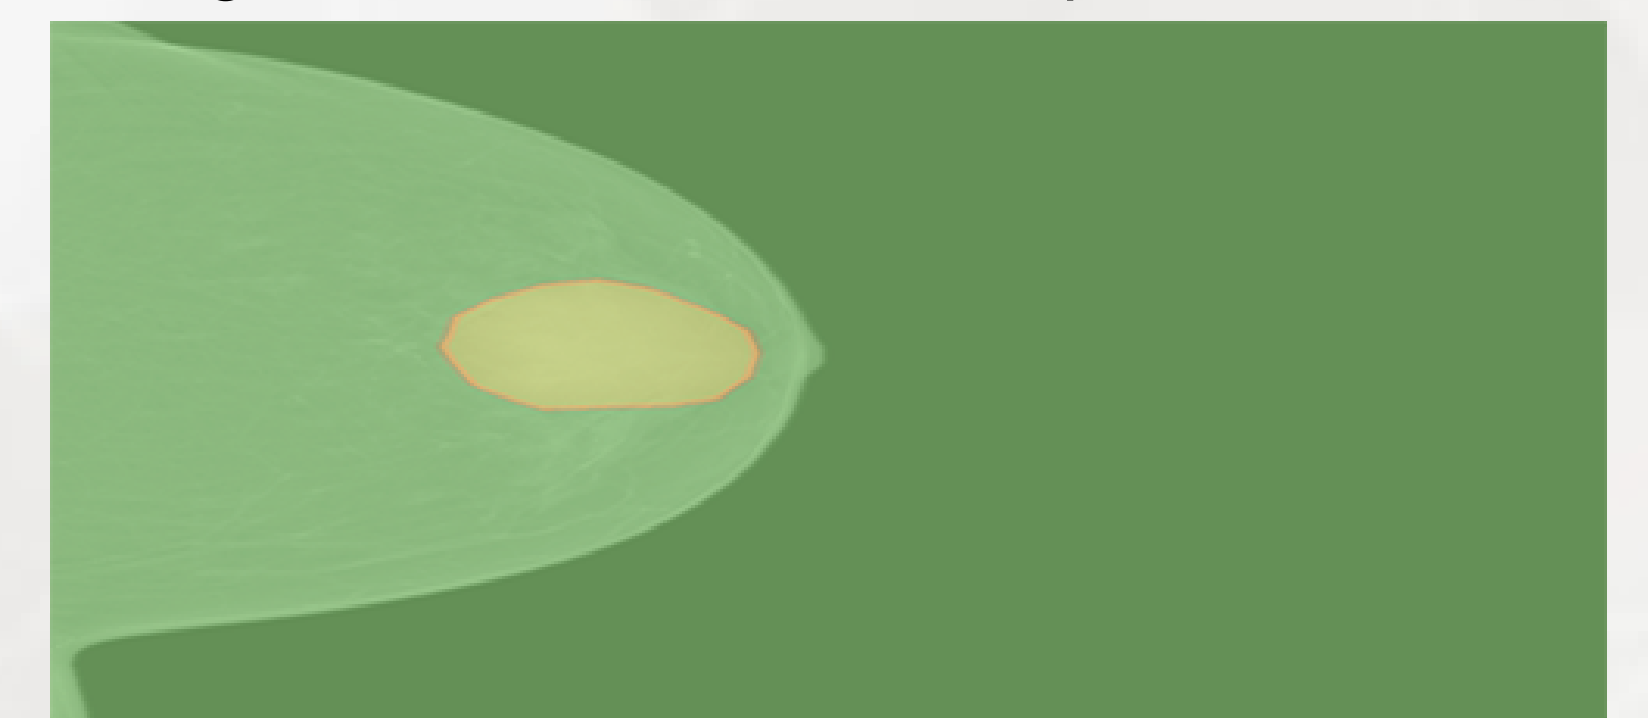

## FUTURE WORK AND CONCLUSIONS

Our work is a first attempt to test the potential of Radiomics in a real-world clinical scenario. More than answering our research questions it opens a number of new avenues for further investigation. This research leverages on previous work implementing DL for active breast lesion detection. However, integrating the Framework on a pipeline requires a lot of engineering work. For effective clinical application, our work requires a proper clinical trial procedure which is out of the scope of this poster. Ultimately, we believe there is significant room for future investigations - to which this work is an important but only initial step - and we hope to see further exploration on the topic.

## ACKNOWLEDGEMENTS


Support received for the development of this work and participation in this event:



## METHODOLOGY

Participants will take part in the tests at our formed institution protocols (e.g., Hospital Fernando Fonseca - HFF). The validation of the framework will take place in a typical *Radiology Room* (RR) environment and workflow (Figure 1). Note takers and data logger(s) will monitor the sessions for observation in the RR, connected by screen recording feed. The test sessions will be recorded and further analyzed.

Figure 1 – Artificial Intelligence (AI) supporting the Medical Imaging (MI) current situation with decision making as a second opinion to Radiologists. Starting at the image acquisition from each patient, to the phase of putting those images on a patient database. From there, Radiologists can examine each image and writing a final report. At this point, researchers can add a second opinion to support the medical decision with trained models of AI and autonomous reporting of the results.

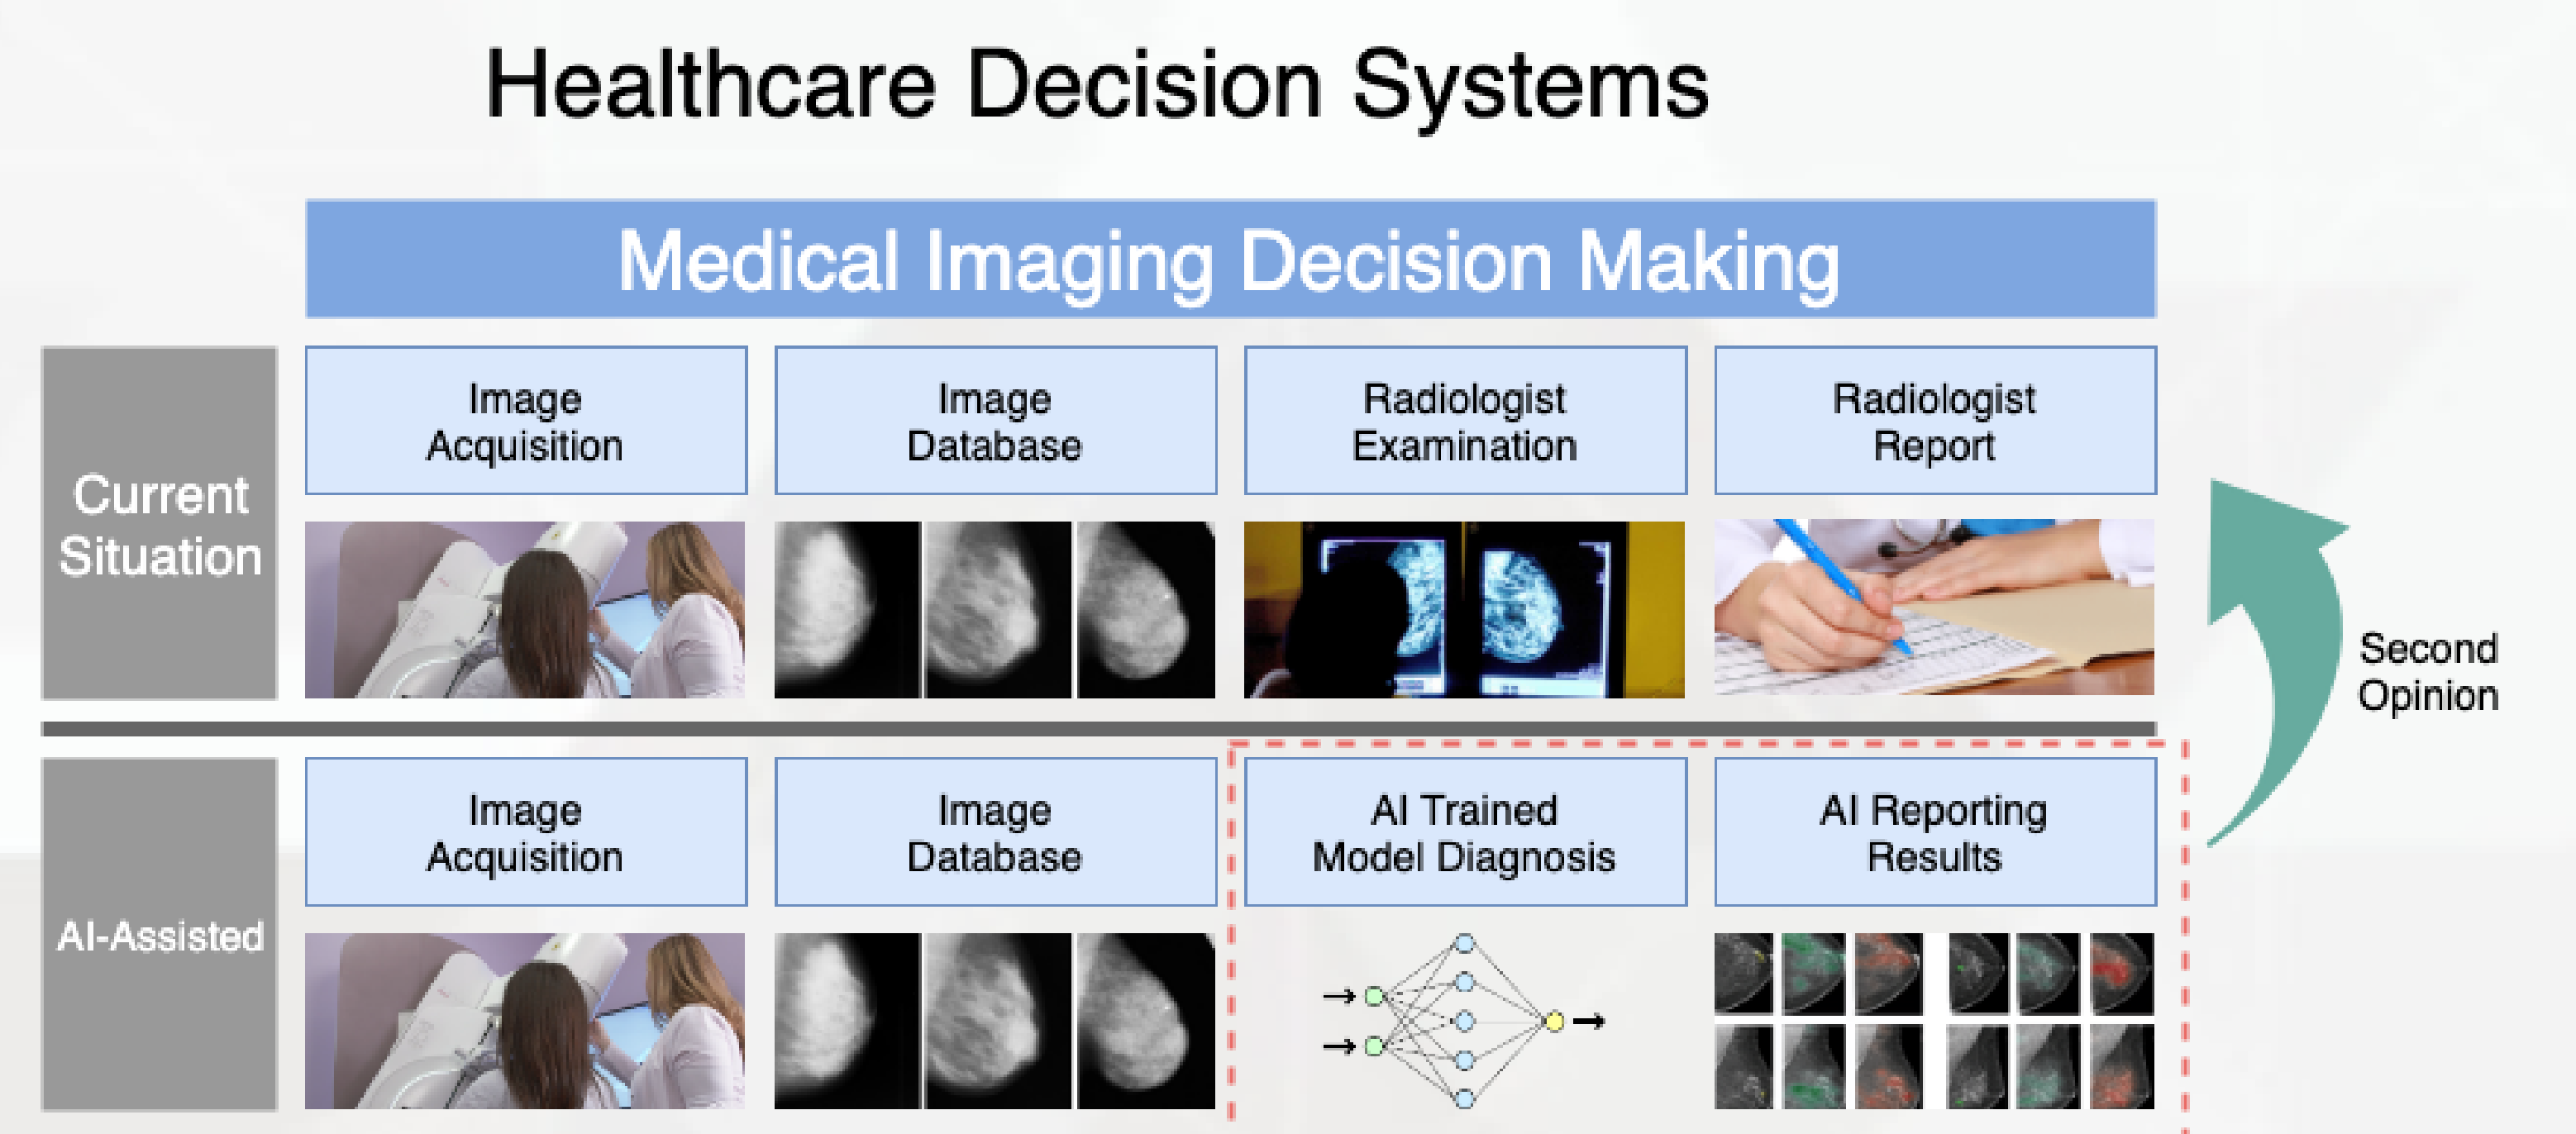

Source: Francisco Calisto (2019).

We propose and measure a second opinion in regard to the current RR situation (see our User Testing Guide (CALISTO, F. M., 2019) for more details). The second opinion will take advantage of our AI trained models (*Assistant*), as well as it reporting results. To measure efficiency and efficacy of our *Assistant* we will use a set of scales. The scales are: (1) NASA-TLX; (2) SUS; and (3) DOTS.

## REFERENCES

- 1 CALISTO, F. **Medical Imaging Potential Decision Making Support Of Artificial Intelligence**. en. [S.l.]: ResearchGate, 2019. DOI: 10.13140/rg.2.2.28001.76642. Available from: <<http://rgdoi.net/10.13140/rg.2.2.28001.76642>>.
- 2 CALISTO, F. M. **Assistant Introduction: User Testing Guide For A Comparison Between Multi-Modality and AI-Assisted Systems**. en. Madeira Interactive Technologies Institute, 2019. DOI: 10.13140/rg.2.2.16566.14403/1. Available from: <<http://rgdoi.net/10.13140/rg.2.2.16566.14403/1>>.
- 3 FRANCISCO, C. **Medical Imaging Multimodality Breast Cancer Diagnosis User Interface**. Oct. 2017. MSc Thesis – Instituto Superior Técnico, Avenida Rovisco Pais 1, 1049-001 Lisboa - Portugal (EU). A Medical Imaging for Multimodality of Breast Cancer Diagnosis by an User Interface.
- 4 HOSTETTER, J.; KHANNA, N.; MANDELL, J. C. Integration of a zero-footprint cloud-based picture archiving and communication system with customizable forms for radiology research and education. **Academic radiology**, Elsevier, 2018.
- 5 JODOGNE, S. et al. Orthanc – A Lightweight, RESTful DICOM Server for Healthcare and Medical Research. In: **BIOMEDICAL Imaging (ISBI), IEEE 10th International Symposium on**. San Francisco, CA, USA: [s.n.], Apr. 2013. p. 190–193. Available from: <<http://orbi.ulg.ac.be/handle/2268/163949>>.
- 6 MAICAS, G. et al. Deep reinforcement learning for active breast lesion detection from dce-mri. In: **SPRINGER. INTERNATIONAL Conference on Medical Image Computing and Computer-Assisted Intervention**. [S.l.: s.n.], 2017. p. 665–673.