

TABLE OF CONTENTS

TABLE OF CONTENTS	1
1- OVERVIEW	2
2- TOOLS AND INSTRUMENTS REQUIRED	2
3 - PREREQUISITES	2
4- TEST SWITCH AND TEST LED DEFINITIONS	3
5- SSM CAL SWITCH	6
6- TR VOLTAGE ADJUSTMENT WITH PULSE TRAIN.....	8
6-1 Hardware Preparation	8
6-2 TR Voltage (Positive) Adjustments	9
6-3 Cable and Test Switch Restoration.....	11
7- MULTI-COIL OPTION.....	12
7-1 Multi-Coil Driver Enable/Disable	12
7-1-1 Via the Software (Alternate Proprietary GE Procedure).....	12
7-2 Multi-Coil –5 VDC Power Supply Adjustments.....	16
8- PAC VOLTAGE CONFIGURATION	17
8-1 Via the Software (Alternate Proprietary GE Procedure).....	17
8-2 Via the Front Panel Switches	20
9- POWER MONITOR TYPE CONFIGURATION	21
9-1 Via the Software (Alternate Proprietary GE Procedure).....	21
9-2 Via the Front Panel Switches	24
10 - SYSTEM RESTORATION.....	25
REVISION HISTORY.....	26

1- OVERVIEW

This procedure describes the setup and calibration of the Communications Pin Driver (CPD) Board in the System Support Module (SSM) for the following:

- 1.0T and 1.5T RF/PEN II cabinet
- 1.0T & 1.5T RF/PDU cabinet
- 1.5T SRF cabinet

Note

See *Dynamic Disable / TR Driver board adjustments* procedure for systems with both RF and Penetration cabinets (4X to 5.4 Hardware). See *Pin Switch Driver Board Set Up And Calibration* procedure for RF/PEN cabinets (5.5 Hardware).

2- TOOLS AND INSTRUMENTS REQUIRED

No special test equipment is required to perform the calibration in **Section 4 - SSM CAL SWITCH** or **Section 8 - POWER MONITOR TYPE CONFIGURATION**. Special equipment may be required for completing the checks or adjustments in the other sections. Refer to Table 2-1 for the equipment required *if it is necessary* to complete the adjustments or checks in these sections. The field laptop and null-modem cable listed in Table 2-1 are required if one is going to use the proprietary software to configure the SSM.

TABLE 2-1
EQUIPMENT REQUIRED

Item	Description	Part Number
1.	100 MHz Scope	46-183029P61
2.	Digital Multimeter (DMM)	46-194427P49
3.	Pot Tweaker	46-194427P361
4.	Null-modem serial cable (provided in every GRFD cabinet)	2124497-46
5.	Field laptop	N/A

3 - PREREQUISITES

WARNING!

FAILURE TO PROPERLY CONFIGURE JUMPER JP1 ON THE HIGH VOLTAGE BOARD COULD POSSIBLY RESULT IN SNR DEGRADATION AND DYNAMIC DISABLE OR DIRECT DRIVE FAILURES.

The SSM High Voltage (HV) Board jumper, JP1, must be set to either the 1000V position for 1.5T or 500V position for 1.0T systems. This high voltage bias is for the Body 1 and Body 2 Dynamic Disable Circuits in the RF body coil and the Direct Drive Circuitry (DD) in the body hybrid splitter. Jumper JP1 should come preset for all new installations and should not require changing. If the HV board ever fails, however, and is replaced, the position of this jumper on the new board should be checked before it is installed.

4- TEST SWITCH AND TEST LED DEFINITIONS

The following Table lists the SSM Test Switch positions and Test LED Definitions. This table is referenced when using the Front Panel Switches sections.

TABLE 4-1
TEST SWITCH AND TEST LED DEFINITIONS

Task	Switch Number	Position	Item Controlled	LED Bank 1	LED Bank 2
Normal Operation:	1	Down		MDS comm status	Head T/R fault
	2	-----	(When one	NB comm status	Body T/R fault
	3	-----	of these 10 is in	Monitor A comm	Spectro T/R fault
	4	-----	use, the others	status	
			are inactive)	Monitor B comm	Body Coil 1 fault
	5	-----		status	
	6	-----		PS fault	Dyn Disable fault
	7	-----		top cover open	Body Coil 2 fault
	8	-----		MC faults disabled	Multi-coil 1 fault
	9	-----		T/R faults disabled	Multi-coil 2 fault
	10	-----		DD faults disabled	Multi-coil 3 fault
Static Control of Drivers:				DD open ckt adj failure	Multi-coil 4 fault
	1	UP		Head T/R open	Dyn Disable open
	2	DOWN		Head T/R short	Dyn Disable short
	3	DOWN		Body T/R open	Multi-coil 1 short
	4	DOWN		Body T/R short	Multi-coil 1 open
	5	UP	MC1 drv enable	Spectro T/R open	Multi-coil 2 short
	5	DOWN	MC1 drv disable		
	6	UP	MC2 drv enable	Spectro T/R short	Multi-coil 2 open
	6	DOWN	MC2 drv disable		
	7	UP	MC3 drv enable	Body Coil 1 open	Multi-coil 3 short
T/Rs Disabled:	7	DOWN	MC3 drv disable		
	8	UP	MC4 drv enable	Body Coil 1 short	Multi-coil 3 open
	8	DOWN	MC4 drv disable		
	9	UP	Source Mode	Body Coil 2 open	Multi-coil 4 short
	10	UP			
	9	DOWN	Sink Mode	Body Coil 2 short	Multi-coil 4 open
	10	DOWN			

4- TEST SWITCH AND TEST LED DEFINITIONS (continued)

TABLE 4-1 (CONTINUED)
TEST SWITCH AND TEST LED DEFINITIONS

Task	Switch Number	Position	Item Controlled	LED Bank 1	LED Bank 2
Pulse Control of Drivers:	1	UP		Head T/R open	Dyn Disable open
	2	DOWN		Head T/R short	Dyn Disable short
	3	UP		Body T/R open	Multi-coil 1 short
	4	DOWN		Body T/R short	Multi-coil 1 open
	5	UP	MC1 drv enable	Spectro T/R open	Multi-coil 2 short
	5	DOWN	MC1 drv disable		
	6	UP	MC2 drv enable	Spectro T/R short	Multi-coil 2 open
	6	DOWN	MC2 drv disable		
	7	UP	MC3 drv enable	Body Coil 1 open	Multi-coil 3 short
	7	DOWN	MC3 drv disable		
	8	UP	MC4 drv enable	Body Coil 1 short	Multi-coil 3 open
	8	DOWN	MC4 drv disable		
	9	UP	Source Mode	Body Coil 2 open	Multi-coil 4 short
	10	UP			
	9	DOWN	Sink Mode	Body Coil 2 short	Multi-coil 4 open
	10	DOWN			
PS Override Tests	1	UP		Dock enable	-----
	2	DOWN		PAC 8V	-----
	3	DOWN		PAC 9V	-5V Supply too high
	4	UP			-15V Supply too high
	5	UP	Dock disable	Bore vent	+15V Supply too high
	5	DOWN	Dock enable		
	6	UP	PAC 9V	Patient Alignment Light	HV Sense too high
	6	DOWN	PAC 8V		
	7	UP	Bore light enable	Bore light	-5V Supply too low
	7	DOWN	Bore light disable		
	8	UP	PAL enable	-----	-15V Supply too low
	8	DOWN	PAL disable		
	9	UP	Bore vent enable	MCD enable	+15V Supply too low
	9	DOWN	Bore vent disable		
	10	-----		-----	HV sense too low

4- TEST SWITCH AND TEST LED DEFINITIONS (continued)

TABLE 4-1 (CONTINUED)
TEST SWITCH AND TEST LED DEFINITIONS


Task	Switch Number	Position	Item Controlled	LED Bank 1	LED Bank 2
				<u>Monitor A</u>	<u>Monitor B</u>
Monitor Fault Summary	1	UP		RF without unblank	RF without unblank
	2	UP		-15V Supply fault	-15V supply fault
	3	DOWN		Body Pwr limit fault	Body pwr limit fault
	4	UP		Head Pwr limit fault	Head pwr limit fault
	5	-----		Spectro Pwr limit fault	Spectro pwr limit fault
	6	-----		Duty Cycle fault	Duty cycle fault
	7	-----		RF Pulse Width fault	RF pulse width fault
	8	-----		+15V Supply fault	+15V supply fault
	9	-----		Body Cable fault	Body cable fault
	10	-----		Head/Spectro Cable fault	Head/spectro cable fault
Multi-coil Configuration	1	UP		Multi-coil 1 enable	-----
	2	DOWN		Multi-coil 2 enable	-----
	3	UP		Multi-coil 3 enable	-----
	4	UP		Multi-coil 4 enable	-----
	5	UP	MC1 enable	-----	-----
	5	DOWN	MC1 disable		
	6	UP	MC2 enable	-----	-----
	6	DOWN	MC2 disable		
	7	UP	MC3 enable	-----	-----
	7	DOWN	MC3 disable		
	8	UP	MC4 enable	-----	-----
	8	DOWN	MC4 disable		
	9	-----		-----	-----
	10	UP, then DOWN	Program	-----	-----
Monitor Type Configuration	1	UP		-----	-----
	2	UP		Monitor A 1.0T	Monitor B 1.0T
	3	UP		-----	-----
	4	UP		Monitor A 1.5T w/EFB	Monitor A 1.5T w/EFB
	5	UP, 6 DOWN=1.0T		-----	-----
	5	UP AND 6 UP=1.5T		-----	-----
	7	-----		-----	-----
	8	-----		-----	-----
	9	-----		-----	-----
	10	UP, then DOWN	Program	-----	-----

5- SSM CAL SWITCH

WARNING!

THE SSM WILL NOT FAULT IF IT IS CALIBRATED WITH A DISCONNECTION OR POOR CONNECTION TO ONE OF THE 4 MAGNET ROOM DYNAMIC DISABLE BIAS LINES (J72, J73, J75, AND J76 ON THE MAGNET ROOM SIDE OF THE PENETRATION PANEL). IMAGE SNR DEGRADATION WILL BE NOTICED BUT THE SSM MAY NOT FAULT. INSPECT THE FOUR BIAS LINE CONNECTIONS FROM THE PEN PANEL TO THE RF COIL BEFORE PERFORMING THIS CALIBRATION.


1. Press and release the CAL switch on the front of the SSM (see Illustration 5-1). This samples the open circuit fault detect signals and adjusts the threshold accordingly for the Dynamic Disable Circuits: J42 (Body 1), J43 (Body 2), and J44 (Direct Drive). When the CAL switch is pressed the LEDs labeled TEST, DRV FLT, and PS FLT will illuminate (this does not indicate a fault).

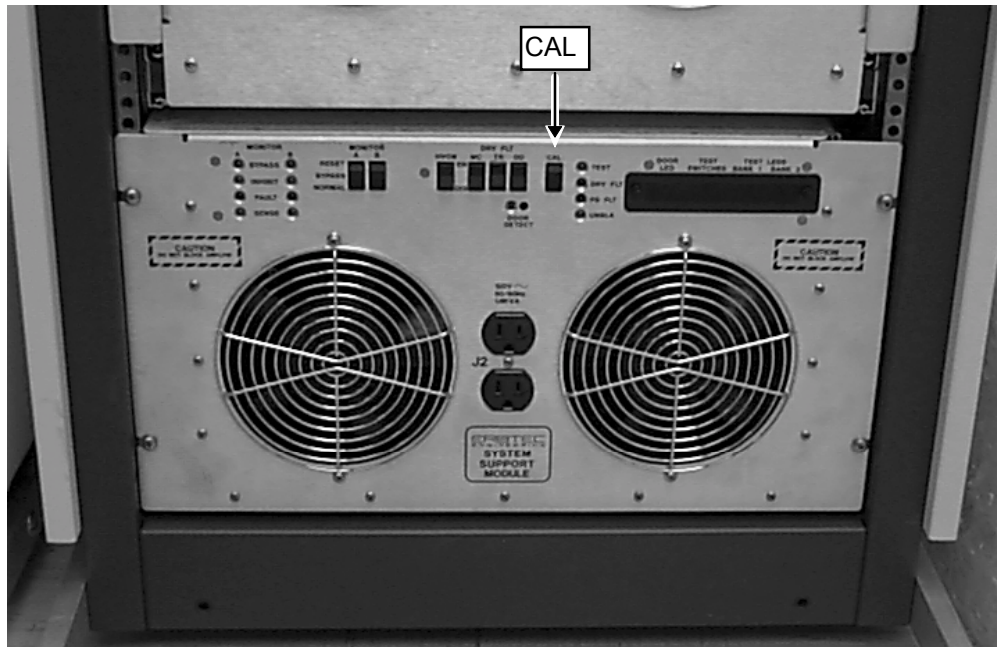

SSM CAL SWITCH LOCATION
ILLUSTRATION 5-1

5- SSM CAL SWITCH (CONTINUED)

2. View the front panel LEDs. Ensure the Bank 1, LED #10 is OFF (see Illustration 5-2). This LED indicates the adjustment process was successful.

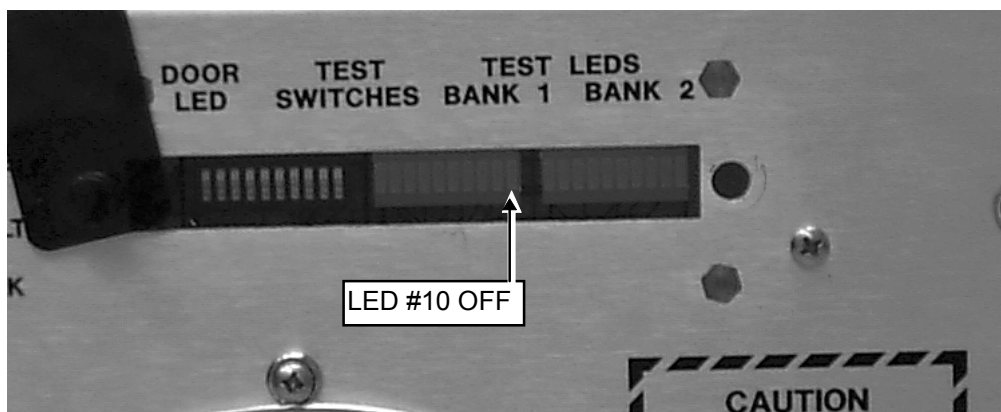

SSM FRONT PANEL LEDs
ILLUSTRATION 5-2


6- TR VOLTAGE ADJUSTMENT WITH PULSE TRAIN

Note

The TR Voltages are factory set and should not require adjustment. This section was included for troubleshooting purposes and is not intended to be performed as a normal part of the calibration process.

6-1 Hardware Preparation

1. Extend the SSM chassis. Allow sufficient cable slack to avoid pinching or straining. Open the lids.
2. Verify cables (and their respective loads) are properly connected to J409 (Head TR) and J408 (Body TR); see Illustration 6-1.

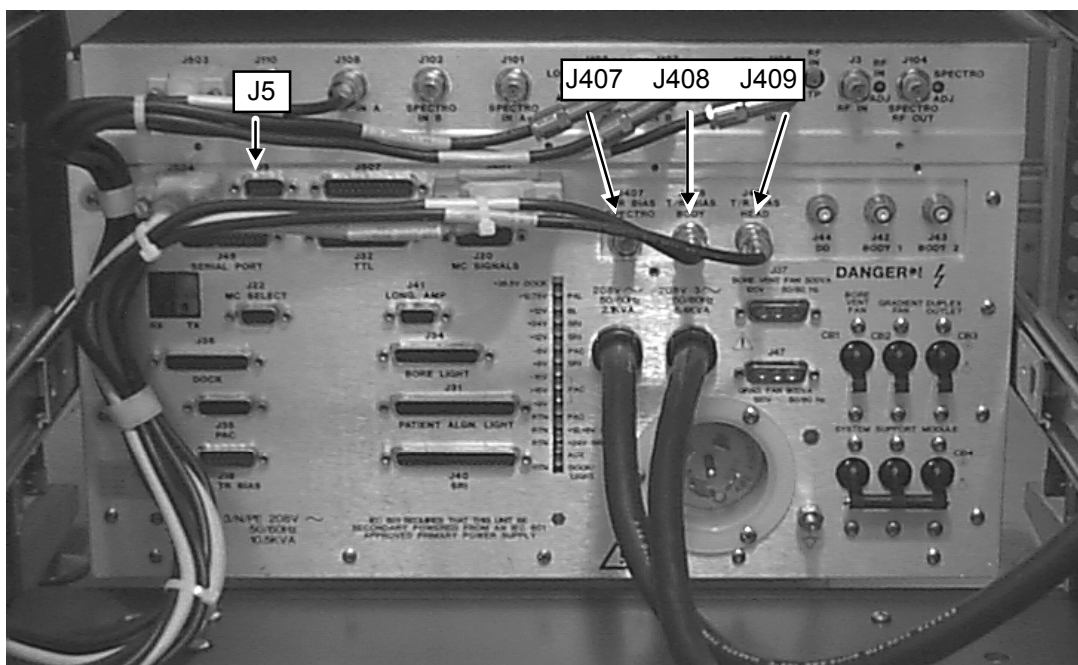


CABLES LOCATIONS ON SSM
ILLUSTRATION 6-1

3. At the SSM disconnect J5 (UNBLK EN); see Illustration 6-1.
4. Configure the front panel DIP switches as shown in Illustration 6-2. This should generate a periodic unblank pulse train. Refer to Table 3-1 for the test switch and test LED definitions.

Note

Order of DIP switch placement is important, otherwise, system will not recognize changes. Place DIP Switch #3 in the UP position first and **then Switch #1** in the UP position. Entering test mode may cause RF Amp fault; this is normal and may be disregarded.


6-1 Hardware Preparation (continued)

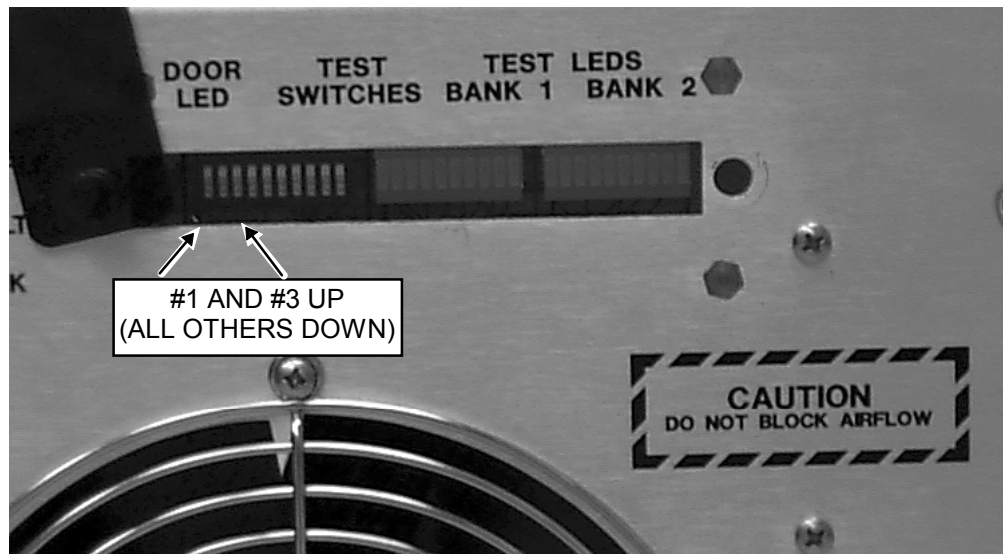

DIP SWITCH CONFIGURATION
ILLUSTRATION 6-2


6-2 TR Voltage (Positive) Adjustments

1. Connect an oscilloscope to monitor the Body TR at TP18 (BTR-OUT); see Illustration 6-3. Adjust R99 until the positive going portion of the Body TR pulse is 4.00 VDC as referenced to ground level. See Illustration 6-4. The negative portion (not adjustable) will measure approximately -12.25 VDC as referenced to ground.

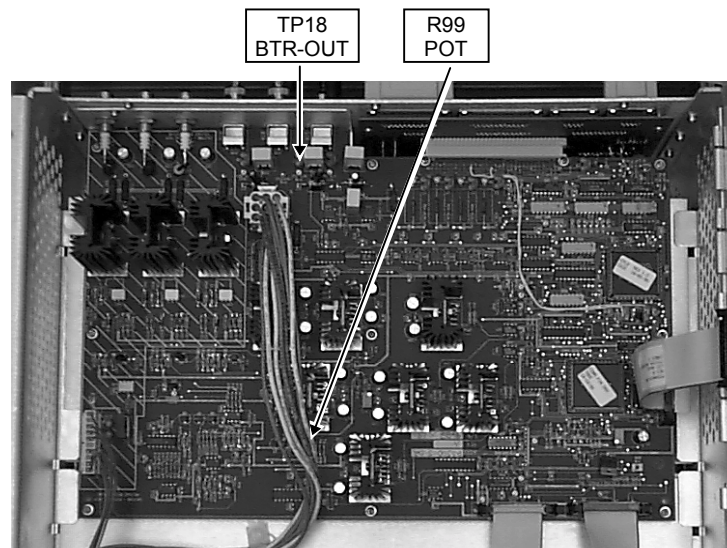


TR VOLTAGE ADJUSTMENT/BODY TR TEST POINT
ILLUSTRATION 6-3

6-2 TR Voltage (Positive) Adjustments (continued)

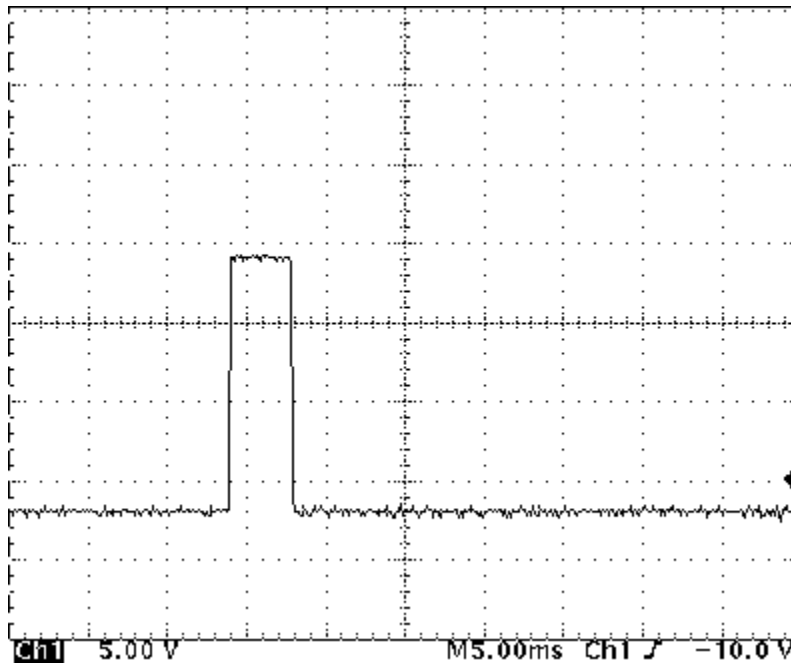


BODY TR SCOPE WAVEFORM SEEN AT TP18 (BTR-OUT)
ILLUSTRATION 6-4

2. Connect an oscilloscope to monitor the Head TR at TP22 (HTR-OUT); see Illustration 6-5. Adjust R104 until the positive going portion of the Head TR pulse is 8.00 VDC as referenced to ground level. See Illustration 6-6. The negative portion (not adjustable) will measure approximately -12.25 VDC as referenced to ground.

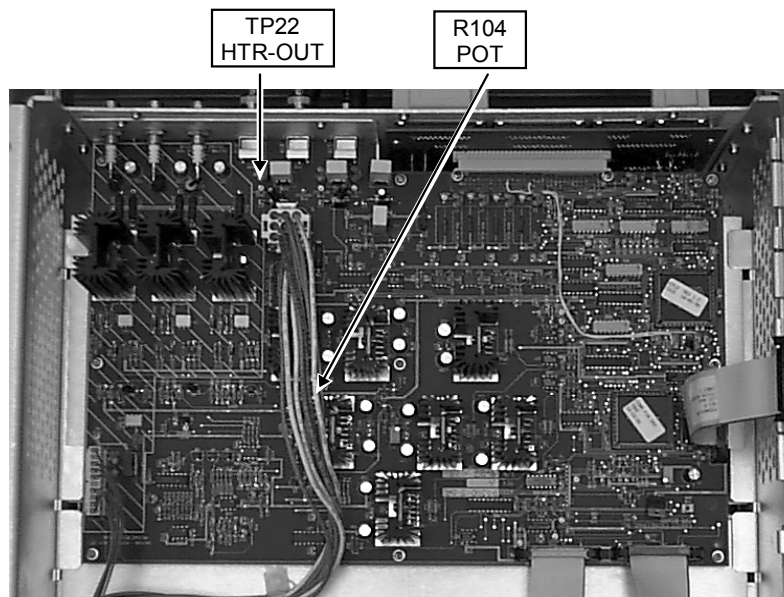

TR VOLTAGE ADJUSTMENT/HEAD TR TEST POINT
ILLUSTRATION 6-5

6-2 TR Voltage (Positive) Adjustments (continued)

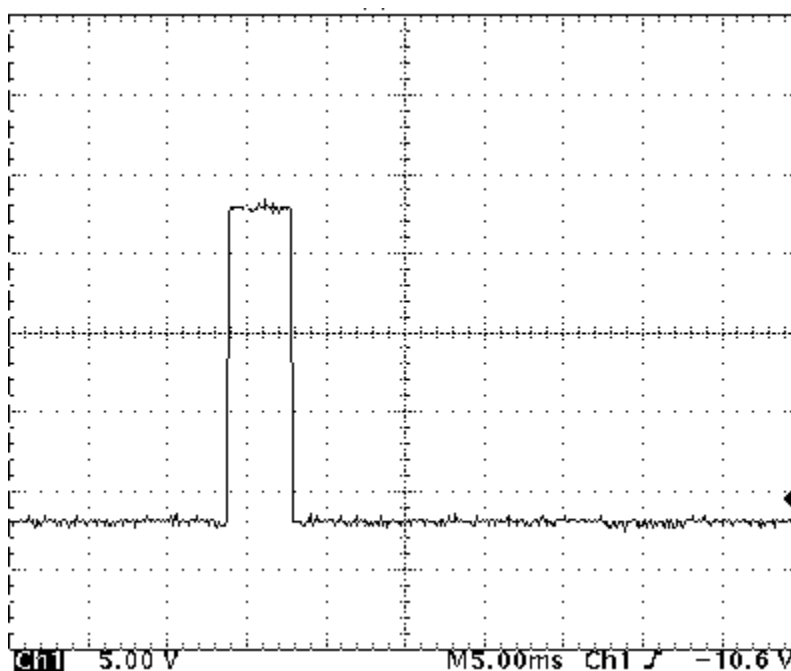

HEAD TR SCOPE WAVEFORM SEEN AT TP22 (HTR-OUT)
ILLUSTRATION 6-6

Note

For Spectro TR adjustments please refer to the appropriate Spectroscopy (MNS) Subsystem Setup and Calibration Tab.

6-3 Cable and Test Switch Restoration

1. Place DIP switch #3 and #1 (respectively) in the Down position. Place all other switches in the Down position.
2. Reconnect J5 (UNBLK EN) at the rear of the SSM.
3. If not proceeding to next section, refer to **Section 10 - System Restoration**.

7- MULTI-COIL OPTION

Note

Disabling is not normally required (even on systems without the Multi-Coil Option). Each SSM (CPD Board) is shipped from the factory with all four Multi-Coil Drivers enabled. This section was included mainly for troubleshooting purposes and should not need to be performed as a part of the normal calibration process.


7-1 Multi-Coil Driver Enable/Disable

The Multi-Coil Drivers can be enabled and disabled in one of two ways: an alternate proprietary GE procedure via the laptop diagnostic software (Section 7-1-1) or via the front panel switches (Section 7-1-2).

The setting should be verified if the spare board seal is broken.

7-1-1 Via the Software (Alternate Proprietary GE Procedure)

1. Connect the laptop to J46 Serial Port of the SSM via the null-modem serial cable. If the null-modem cable normally shipped with the RF/PDU or SRF cabinet is not available, a standard 9-pin to 25-pin serial cable with a null-modem adapter can be used instead. See Illustration 7-1.

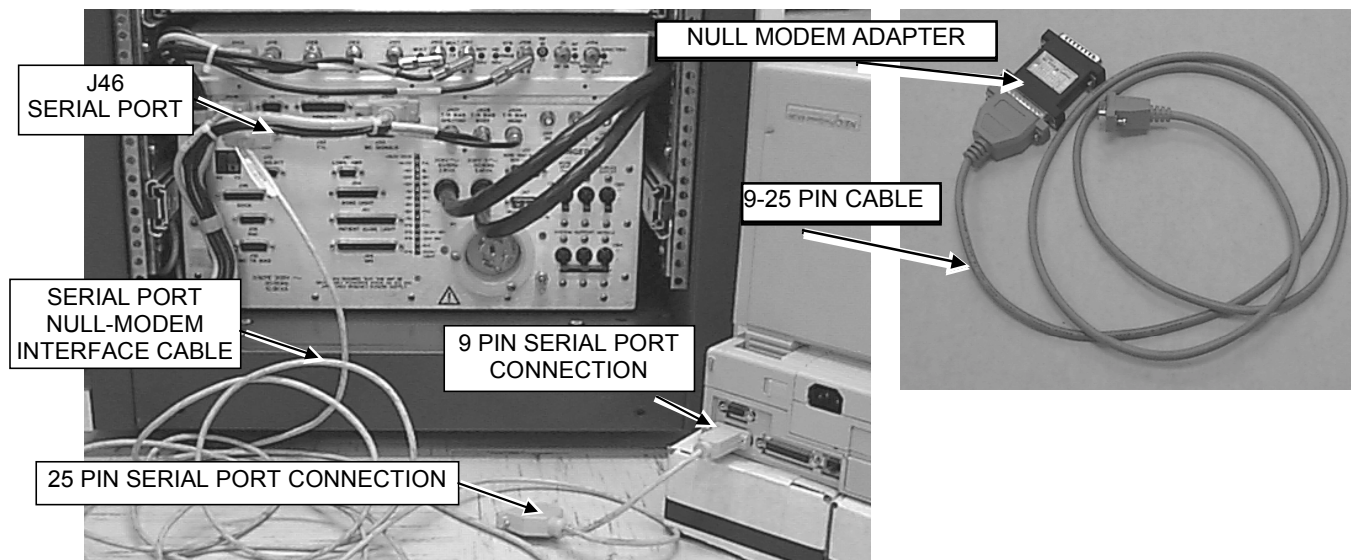

LAPTOP CONNECTED TO SSM
ILLUSTRATION 7-1

7-1-1 Via the Software (Alternate Proprietary GE Procedure) (continued)

2. Run the program CPD.EXE. See Table 7-1.

Note

Only version 2.0 of CPD.EXE is compatible with all MR system types. This is the version available from the 8.X Service Methods CDROM, revision 12 and later.

TABLE 7-1
ALTERNATE PROPRIETARY PROCEDURE — LAPTOP SOFTWARE

Start the software diagnostic program CPD.EXE on the laptop.

Note

The CPD.EXE program, if not loaded on the service laptop, can be loaded from the Signa LX MR Service Methods CD-ROM 2160623-1. Insert the CD-ROM into the drive. Under Windows 95/98 use the cursor to select "**Start**" and then "**Run**" and then "**Browse**". Select the CDROM drive from the down arrow to the right of the "**Look in:**" entry box in the "**Browse**" menu. In the edit box type the following (include the quotes): "**d:\mrtools\Setup.exe**"

Follow the setup program instructions to install the tool onto the laptop. The CPD.EXE must be run in MS-DOS mode and not from a Windows shell to DOS. In Windows95/98 perform the following steps:

- 1) **[Start], [Shut Down...], Restart the computer in MS-DOS mode?, [Yes]**

Note

It may take up to 1.5 minutes for some Dell laptops to restart in MS-DOS mode.

- 2) At the C:\Windows> prompt, type **cd \cclass\rfertools<ENTER>**
- 3) At the C:\CCLASS\ERBTEC> prompt type **cpd.exe<ENTER>**

3. A message that reads, "*OOPS no CRC value today XXXX. Press a key.*" may be displayed if using the version 2.0 software. This is normal. Press any key to continue.
 - a. The main selection screen will be displayed. Note the headline at the top of the screen that reads, "*CPD.EXE Rev 2.0 CRC XXXX*" where *XXXX* is some hexadecimal value.
 - b. If the hexadecimal value is all zeros then select "**E**" to exit from the CPD.EXE program and then restart it again.
 - c. Verify that status of the hexadecimal value as in the previous step. Failure to verify that the hexadecimal value is not all zeros may result in the program reporting erroneous values.
 - d. If the hexadecimal value is not all zeros then continue with the next step.
4. Select the *C) Perform Special Operations* menu.
5. Select *F) Change Multi-coil Configuration*.

7-1-1 Via the Software (Alternate Proprietary GE Procedure) (continued)

6. Answer the questions. See Illustration 7-2.

Current Multi-coil configuration is : 0F

Multi-coil 1 ENABLED

Multi-coil 2 ENABLED

Multi-coil 3 ENABLED

Multi-coil 4 ENABLED

Do you wish to change any of them? y or n

Enter the numbers of the Multi-coils you wish to change state separated by spaces

(i.e. 1 3 will change Multi-coils 1 and 3)

Enter 0 to leave the Multi-coils as they are


SELECTION: F) CHANGE MULTI-COIL CONFIGURATION

ILLUSTRATION 7-2

7. Press **<Esc>** twice to exit to DOS. To return to Windows, type **exit<ENTER>**.
8. Cycle the main breaker power at the SSM by turning CB4 to the OFF position, waiting 15 seconds, then setting CB4 to the ON position. This step saves the changes to the SSM.

7-1-2 Via the Front Panel Switches

1. Remove the plastic cover from the Test Switch and Test LEDs window on the front of the SSM. See Illustration 7-3.

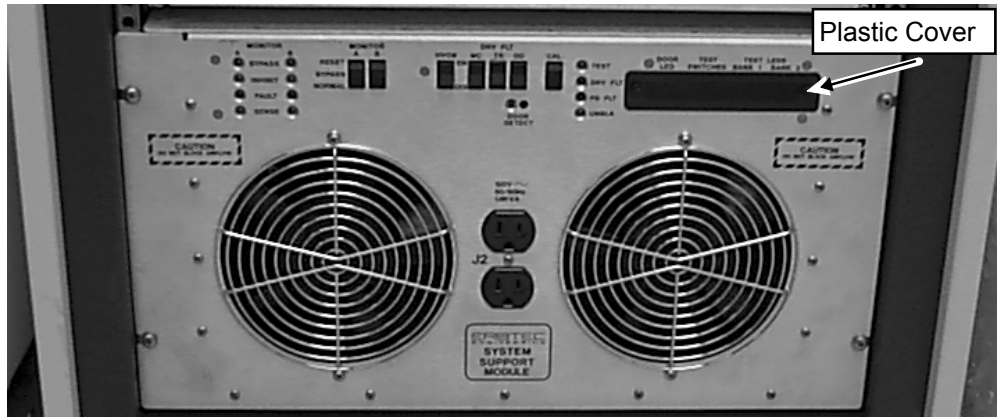

TEST SWITCH AND TEST LEDs WINDOW
ILLUSTRATION 7-3

Note


Place DIP Switch #1 in the UP position last. Order of DIP switch placement is important otherwise system will not recognize changes.

2. Place switches 3, 4, and 1 in the Up position. Ensure that all other switches are in the Down position.
3. To program the correct Multi-Coil Driver configuration to the CPD Board, perform one of the following steps. This procedure references Table 4-1, Multi-Coil Driver Configuration.
 - a. To disable all Multi-Coil Drivers, place switches 5, 6, 7, & 8 in the Down position and proceed to step 4.
 - b. To disable Multi-Coil Drivers 3 & 4, place switches 5 & 6 in the Up position and proceed to step 4.
 - c. To enable all Multi-Coil Drivers, place switches 5, 6, 7, & 8 in the Up position and proceed to step 4.
4. Place switch #10 in the Up position.
5. Place switch # 10 in the Down position. Bank 1 LEDs 1, 2, 3, & 4 are illuminated and remain illuminated once switch #10 is in Down position.
6. Place switch #1 in the Down position. Bank 1 LED 1 will illuminate for approximately one minute, then extinguish.
7. Place all switches in the Down position.
8. Cycle the main circuit breaker power at the SSM by turning CB4 to the OFF position, waiting 15 seconds, then setting CB4 to the ON position. This step saves the changes to the SSM.
9. Replace the plastic cover on the front of the SSM.

7-2 Multi-Coil –5 VDC Power Supply Adjustments


Note

Verify that the cables are properly connected (not swapped) at J20 (Multi-Coil Signals, labeled MR1-A7-J20) and J18 (Multi-coil TR Bias, labeled MR1-A7-J18); see Illustration 7-4.

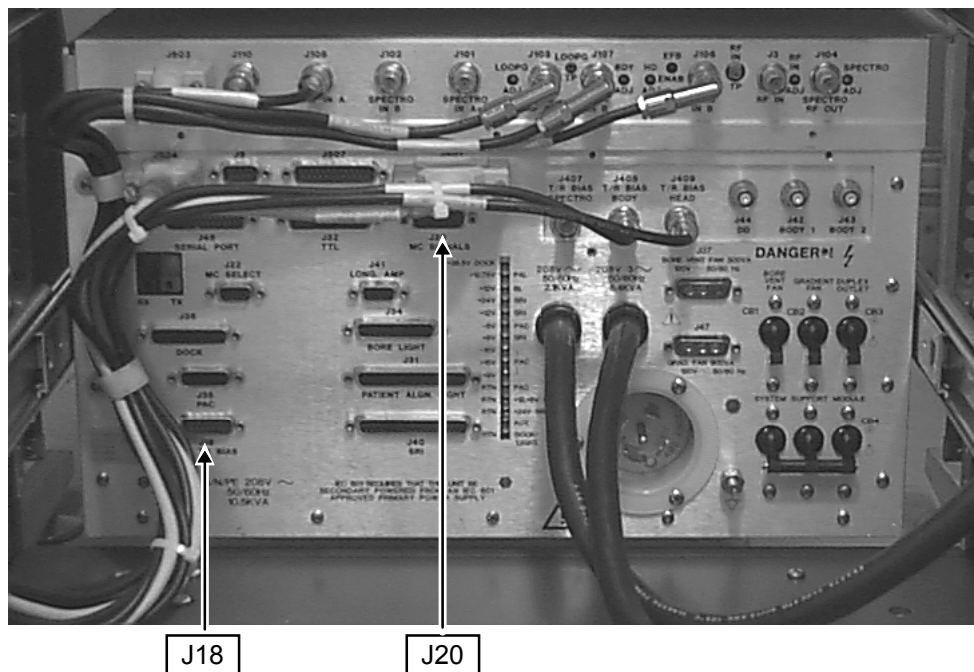

**CABLES CONNECTED TO CORRECT LOCATIONS — MULTI-COIL
ILLUSTRATION 7-4**

1. Connect an oscilloscope or a Digital Volt-Meter to the CPD Board test point TP1 (–5VDC) with reference to ground; see Illustration 7-5. Adjust R11 until the voltage measured is –5.00 VDC (± 0.05 VDC).

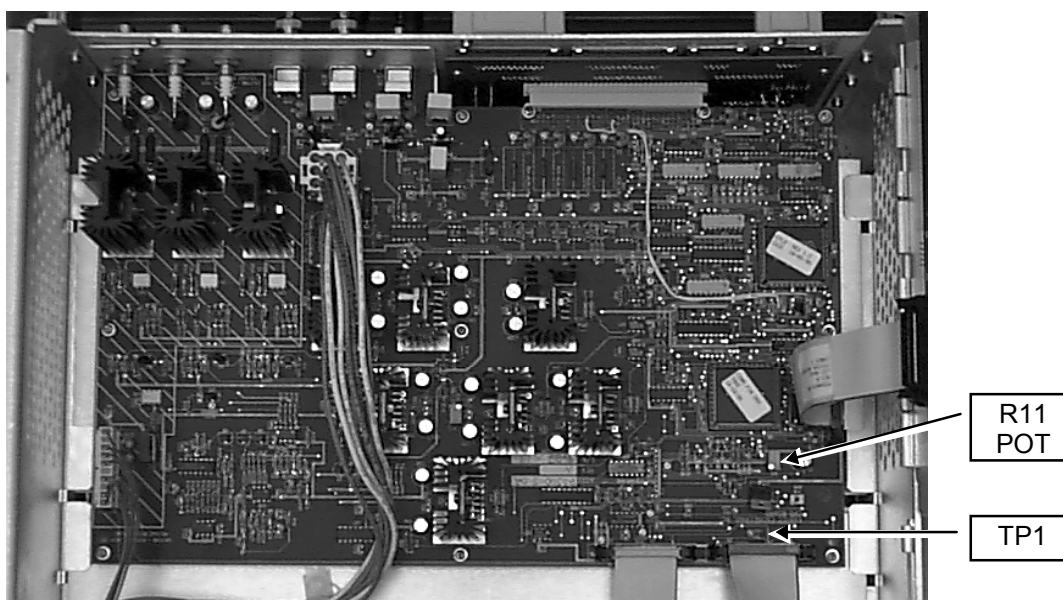

**MULTI-COIL ADJUSTMENT/ –5VDC AT TP1
ILLUSTRATION 7-5**

8- PAC VOLTAGE CONFIGURATION

The PAC is preset to 9 VDC at the factory (setting should be verified if the spare board seal is broken).

The PAC Voltage can be verified via an alternate proprietary GE procedure using the laptop diagnostic software (Section 8-1). To change the PAC voltage setting use, Section 8-2, Via the Front Panel Switches.

Note

Systems without a fiber optic repeater at the Pen wall need to set the PAC voltage to 8 Volts DC.

CAUTION


Possible equipment damage. To prevent possible damage to equipment due to incorrect voltage settings, systems without fiber optic repeater at the Pen wall need to set the PAC voltage to 8 Volts DC.

8-1 Via the Software (Alternate Proprietary GE Procedure)

Note

The alternate proprietary GE procedure via the laptop software does not work properly for setting the PAC voltage, but can be used to verify the current PAC voltage setting. The following steps describe the PAC voltage setting verification procedure. To change settings use section 8-2 via the Front Panel Switches.

1. Connect the laptop to J46 Serial Port of the SSM via the null-modem serial cable. If the null-modem cable normally shipped with the RF/PDU or SRF cabinet is not available, a standard 9-pin to 25-pin serial cable with a null-modem adapter can be used instead. See Illustration 8-1.

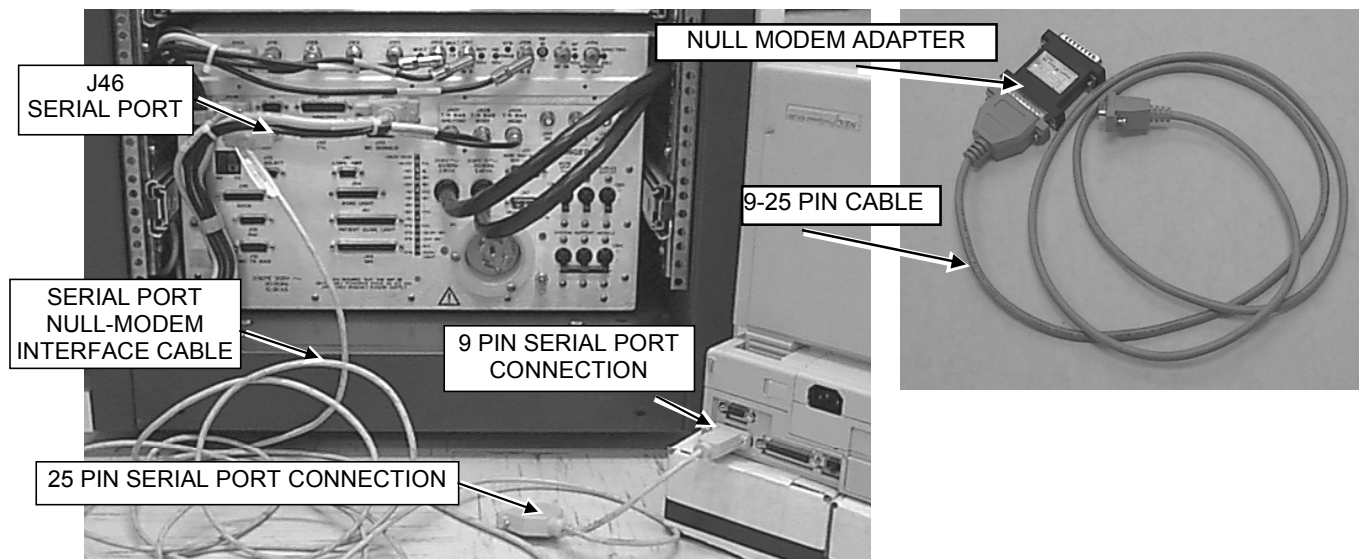

LAPTOP CONNECTED TO SSM
ILLUSTRATION 8-1

8-1 Via the Software (Alternate Proprietary GE Procedure) (continued)

2. Run the program CPD.EXE. See Table 8-1.

Note

Only version 2.0 of CPD.EXE is compatible with all MR system types. This is the version available from the 8.X Service Methods CDROM, revision 12 and later.

TABLE 8-1

ALTERNATE PROPRIETARY PROCEDURE — LAPTOP SOFTWARE

Start the software diagnostic program CPD.EXE on the laptop.

Note

The CPD.EXE program, if not loaded on the service laptop, can be loaded from the Signa LX MR Service Methods CD-ROM 2160623-1. Insert the CD-ROM into the drive. Under Windows 95/98 use the cursor to select "**Start**" and then "**Run**" and then "**Browse**". Select the CDROM drive from the down arrow to the right of the "**Look in:**" entry box in the "**Browse**" menu. In the edit box type the following (include the quotes): "**d:\mrtools\Setup.exe**"

Follow the setup program instructions to install the tool onto the laptop. The CPD.EXE must be run in MS-DOS mode and not from a Windows shell to DOS. In Windows95/98 perform the following steps:

- 2) [**Start**], [**Shut Down...**], **Restart the computer in MS-DOS mode?**, [**Yes**]

Note

It may take up to 1.5 minutes for some Dell laptops to restart in MS-DOS mode.

- 2) At the C:\Windows> prompt, type **cd \cclass\rfertools<ENTER>**
- 3) At the C:\CCLASS\ERBTEC> prompt type **cpd.exe<ENTER>**

3. A message that reads, "*OOPS no CRC value today XXXX. Press a key.*" may be displayed if using the version 2.0 software. This is normal. Press any key to continue.
 - a. The main selection screen will be displayed. Note the headline at the top of the screen that reads, "*CPD.EXE Rev 2.0 CRC XXXX*" where *XXXX* is some hexadecimal value.
 - b. If the hexadecimal value is all zeros then select "**E**" to exit from the CPD.EXE program and then restart it again.
 - c. Verify that status of the hexadecimal value as in the previous step. Failure to verify that the hexadecimal value is not all zeros may result in the program reporting erroneous values.
 - d. If the hexadecimal value is not all zeros then continue with the next step.
4. Select the *C) Perform Special Operations* menu.
5. Select *H) Change PAC Power Supply Voltage (8V, 9V)*.

8-1 Via the Software (Alternate Proprietary GE Procedure) (continued)

6. The current PAC configuration is shown (see Illustration 8-2).

Current PAC 8/9 V configuration is : 9V

Do you wish to change it? <Y> or <N>

SELECTION: H) CHANGE PAC POWER SUPPLY VOLTAGE (8V, 9V)

ILLUSTRATION 8-2

7. Type **N<ENTER>**.
8. Press **<Esc>** twice to exit to DOS. To return to Windows, type **exit<ENTER>**.
9. Cycle the main breaker power at the SSM by turning CB4 to the OFF position, waiting 15 seconds, then setting CB4 to the ON position. This step saves the changes to the SSM.

8-2 Via the Front Panel Switches (continued)


5. Place all other switches in the Down position.
6. Cycle the main breaker power at the SSM by turning CB4 to the OFF position, waiting 15 seconds, then setting CB4 to the ON position. This step saves the changes to the SSM.
7. Replace the plastic cover on the front of the SSM.
8. Connect the Fiber Optic cables to RX & TX on rear of SSM.
9. Perform TPS Reset by clicking the **[Service Desktop]** icon and clicking the **[TPS Reset]** button on the Service Rx.

9- POWER MONITOR TYPE CONFIGURATION

The power monitor should be checked to verify that it is set to either 1.5T or 1.0T, depending on the field strength of the system. The default setting for replacement boards is 1.5T. The power monitor type can be changed one of two ways: an alternate proprietary GE procedure via the laptop diagnostic software (Section 9-1) or via the front panel switches (Section 9-2).

9-1 Via the Software (Alternate Proprietary GE Procedure)

1. Connect the laptop to J46 Serial Port of the SSM via the null-modem serial cable. If the null-modem cable normally shipped with the RF/PDU or SRF cabinet is not available, a standard 9-pin to 25-pin serial cable with a null-modem adapter can be used instead. See Illustration 9-1.

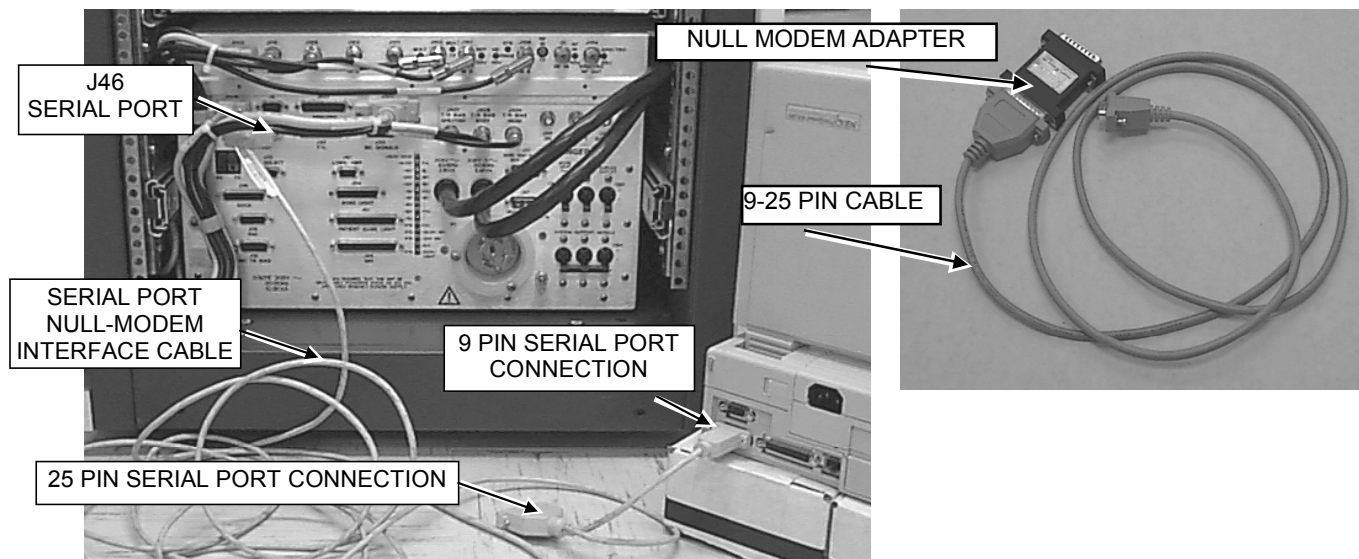

LAPTOP CONNECTED TO SSM
ILLUSTRATION 9-1

9-1 Via the Software (Alternate Proprietary GE Procedure) (continued)

2. Run the program CPD.EXE. See Table 9-1.

Note

Only version 2.0 of CPD.EXE is compatible with all MR system types. This is the version available from the 8.X Service Methods CDROM, revision 12 and later.

TABLE 9-1

ALTERNATE PROPRIETARY PROCEDURE — LAPTOP SOFTWARE

Start the software diagnostic program CPD.EXE on the laptop.

Note

The CPD.EXE program, if not loaded on the service laptop, can be loaded from the Signa LX MR Service Methods CD-ROM 2160623-1. Insert the CD-ROM into the drive. Under Windows 95/98 use the cursor to select "**Start**" and then "**Run**" and then "**Browse**". Select the CDROM drive from the down arrow to the right of the "**Look in:**" entry box in the "**Browse**" menu. In the edit box type the following (include the quotes): "**d:\mrtools\Setup.exe**"

Follow the setup program instructions to install the tool onto the laptop. The CPD.EXE must be run in MS-DOS mode and not from a Windows shell to DOS. In Windows95/98 perform the following steps:

- 3) **[Start], [Shut Down...], Restart the computer in MS-DOS mode?, [Yes]**

Note

It may take up to 1.5 minutes for some Dell laptops to restart in MS-DOS mode.

- 2) At the C:\Windows> prompt, type **cd \cclass\rfertools<ENTER>**
- 3) At the C:\CCLASS\ERBTEC> prompt type **cpd.exe<ENTER>**

3. A message that reads, "*OOPS no CRC value today XXXX. Press a key.*" may be displayed if using the version 2.0 software. This is normal. Press any key to continue.
 - a. The main selection screen will be displayed. Note the headline at the top of the screen that reads, "*CPD.EXE Rev 2.0 CRC XXXX*" where *XXXX* is some hexadecimal value.
 - b. If the hexadecimal value is all zeros then select "**E**" to exit from the CPD.EXE program and then restart it again.
 - c. Verify that status of the hexadecimal value as in the previous step. Failure to verify that the hexadecimal value is not all zeros may result in the program reporting erroneous values.
 - d. If the hexadecimal value is not all zeros then continue with the next step.
4. Select the C) *Perform Special Operations* menu.
5. Select G) *Change Power Monitor Type*.

9-1 Via the Software (Alternate Proprietary GE Procedure) (continued)

6. Type y<ENTER> and type letter of one of the following power monitor types. See Illustration 9-2.
 - a. **For the RF/PEN II Cabinet:**
1.0T Systems, choose **C**.
1.5T Systems, choose **D**.
 - b. **For the RF/PDU Cabinet:**
Cabinet with the Solid State TELI RF Amplifiers choose **C**.
Cabinet with the Solid State ANALOGIC RF Amplifiers choose **D**.

Current Power Monitor Configuration is : 1.5T

Do you wish to change it? <Y> or <N> y

Choose one of the following configurations:

- A) 0.5T
- B) 0.7T
- C) 1.0T
- D) 1.5T

SELECTION: G) CHANGE POWER MONITOR TYPE (1.0T, 1.5T)

ILLUSTRATION 9-2

7. Press <Esc> twice to exit to DOS. To return to Windows, type **exit<ENTER>**.
8. Cycle the main breaker power at the SSM by turning CB4 to the OFF position, waiting 15 seconds, then setting CB4 to the ON position. This step saves the changes to the SSM.

9-2 Via the Front Panel Switches

1. Remove the plastic cover on the front of the SSM.

Note

Place DIP Switch #1 in the UP position last. Order of DIP switch placement is important otherwise system will not recognize changes.

2. Place switches 3, 2, 4, and 1 in the Up position. Ensure that all other switches are in the Down position (See Illustration 9-1). Depending on the current configuration of the Power Monitor LED BANK 1 and LED BANK 2 will each show either LED # 2, LED # 3, or LED # 4 illuminated. LED # 2 illuminated signifies a 1.0T, LED # 3 illuminated signifies a 0.7T, and LED # 4 illuminated signifies a 1.5T Power Monitor. It is not necessary to continue this procedure if the Power Monitor is already correctly configured.



DIP SWITCH CONFIGURATION FOR SETTING POWER MONITOR TYPE
ILLUSTRATION 9-1

- a. **To set the type to a 1.0T**, place switch 5 in the Up position and switch 6 in the Down position.
 - b. **To set the type to a 1.5T**, place switch 5 in the Up position and switch 6 in the Up position.
3. Place switch #10 in the Up position followed by the Down position. LED BANK 1 and LED BANK 2 will now change to show either LED # 2 (1.0T) or LED # 4 (1.5T) illuminated depending on the new setting of the Power Monitor.
 4. Place switch #1 in the Down position. None of the LEDs in LED BANK 1 and LED BANK 2 should now be illuminated.
 5. Place all other switches in the Down position.
 6. Cycle the main breaker power at the SSM by turning CB4 to the OFF position, waiting 15 seconds, then setting CB4 to the ON position. This step saves the changes to the SSM.
 7. Replace the plastic cover on the front of the SSM.

10 - SYSTEM RESTORATION

1. Close the SSM lids, replace all the lid screws, slide the SSM chassis back into the rack, and replace the four front screws.
2. Remove Laptop computer connection to SSM (J46), if applicable.
3. Replace cabinet covers.
4. Verify J5 is connected.
5. Perform a TPS reset.
6. Perform a Head Scan, Body Scan, and Multi-coil scan to verify the system is scanning normally.

REVISION HISTORY

REV	DATE	AUTHOR	PRIMARY REASONS FOR CHANGE
0	July 25, 1997	Karyl Verdon (Erbtec)	Initial Release - checked consistency w/existing files.
1	June 29, 1998	K. Keshena	Updated file to RF/PDU cabinet
2	December 28, 1998	K. Keshena	Added alternate proprietary procedure information, updated laptop portion to Windows95, and corrected switch orders for the front panel switch procedures.
3	January 25, 1999	R. Lambert & K. Keshena	Combined procedures, this procedure is for RF/PEN II and 1.0T & 1.5T RF/PDU systems. Clarified all sections.
4	November 16, 1999	R. Schmidt	Updated page 17 with correct path for loading CPD.exe program as well as latest CD-ROM part #'s for 5x & 8.x. Page 18 steps 7-2-2, 7-2-2-b, & 7-2-4 were validated and corrected per SPR's MRIge56704 & MRIge56649 in which LED 4 is illuminated, not LED 2.
5	October 6, 2000	D. Thome'	Added new Warning message about disconnected bias lines. Added reference to SRF cabinet. Added latest correct path for loading CPD.exe. Corrected section 7-2 concerning LEDs. Corrected section 6-1-2 concerning LED display for multi-coil configuration. Re-wrote document for class C.
6	March 12, 2001	D Thome'	Added reference to 0.7T Power Monitor configuration information. Added notes and comments to clarify calibration procedure.
7	April 20, 2001	D. Thome'	Added Section 3 to check JP1 on HV Board. Added new path for loading cpd.exe.