

**MI&CT ESERVICE NOTE
SN07011917a**

Class C information is Property of GE.

This short-term informational note is invalid 6 months after the issue date.

Date: February 7, 2007

Subject: Performix Ultra, ADV, NP++ X-ray Tube - New Pump

Effectivity: All Performix Ultra, ADV, and NP++ X-ray Tubes

Details: All Performix Ultra, ADV, and NP++ X-ray Tubes have begun shipping with new dual impeller pumps and filters. The new pump design is a reliability improvement. The 2 impellers reduce load on bearings and thus increase reliability. The filter is internal to the tube and will help maintain dielectric oil strength over life by removing particulate from the oil.

No tube form, fit, or function has been changed. This will **not** affect field service replacement procedures. The new filter is **not** field-replaceable.

No additional actions required by the Field Engineer.

No changes to tube part numbers. This is an update to the existing part number.


All electrical and mechanical connections are the same.

Affected Assemblies:


D3131T
D3132T
D3151T
D3152T
D3171T
D3172T
D3175T
D3176T
D3185T
D3186T

GE Healthcare MI&CT Class C eService Notes are copyright (c) protected to General Electric Company Inc with all rights reserved. Class C eService Notes issued by GE Healthcare are proprietary to GE Healthcare Systems. Disclosure to persons not employed by GE Healthcare or not in possession of a Advanced Service Agreement with GE Healthcare is prohibited.
Duplication and distribution of any class of eService Notes, in any form by entities other than GE Healthcare is strictly prohibited.

See picture below for example of previous and current oil pumps:

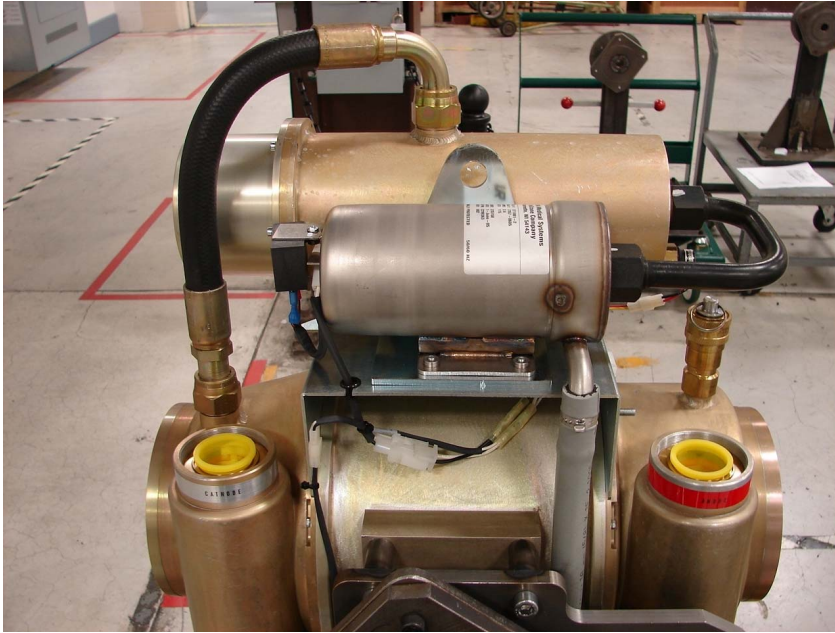

Picture 1: Previous Oil Pump

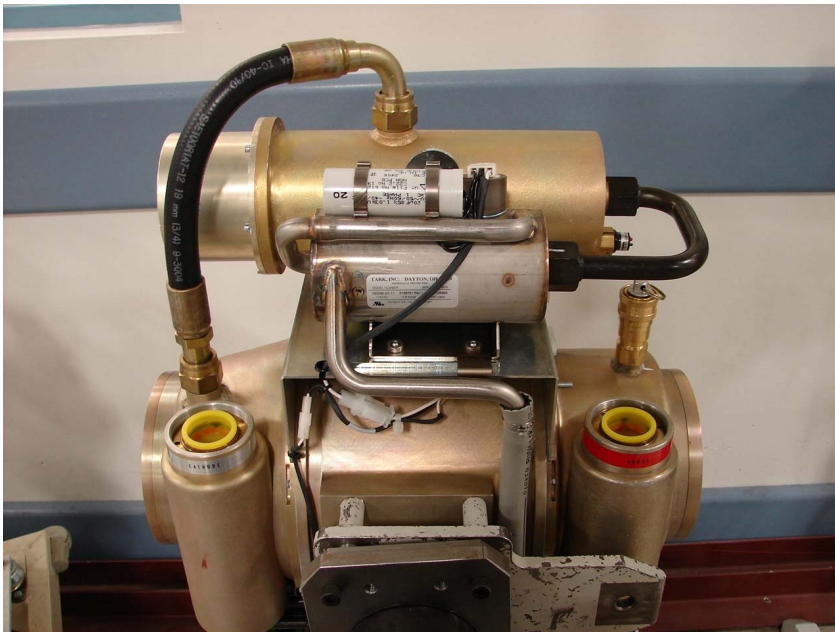

Picture 2: Current Oil Pump

**GE Healthcare MI&CT Class C eService Notes are copyright (c) protected to General Electric Company Inc with all rights reserved. Class C eService Notes issued by GE Healthcare are proprietary to GE Healthcare Systems. Disclosure to persons not employed by GE Healthcare or not in possession of a Advanced Service Agreement with GE Healthcare is prohibited.
Duplication and distribution of any class of eService Notes, in any form by entities other than GE Healthcare is strictly prohibited.**

Donna M. Murray
Installed Base Development Engineer
MI&CT Engineering Manager Signature_____