

GE Healthcare MI&CT Class C eService Notes are copyright (c) protected to General Electric Company Inc with all rights reserved. Class C eService Notes issued by GE Healthcare are proprietary to GE Healthcare. Disclosure to persons not employed by GE Healthcare or not in possession of an Advanced Service Agreement with GE Healthcare is prohibited. Duplication and distribution of any class of eService Notes, in any form by entities other than GE Healthcare is strictly prohibited.

MI&CT eSERVICE NOTE
SN08050216a

Class C information. Property of GE Healthcare

This short-term informational note is invalid 6 months after the issue date.


Date: October 6, 2008

Subject: Plenum cable cover FRU

Effectivity: VCT systems

Details:

Some Plenum upgrade kits were missing the plenum cable covers. See Illustration below. These covers are for secondary cable containment, in case a cable is not properly secured before putting covers back on.

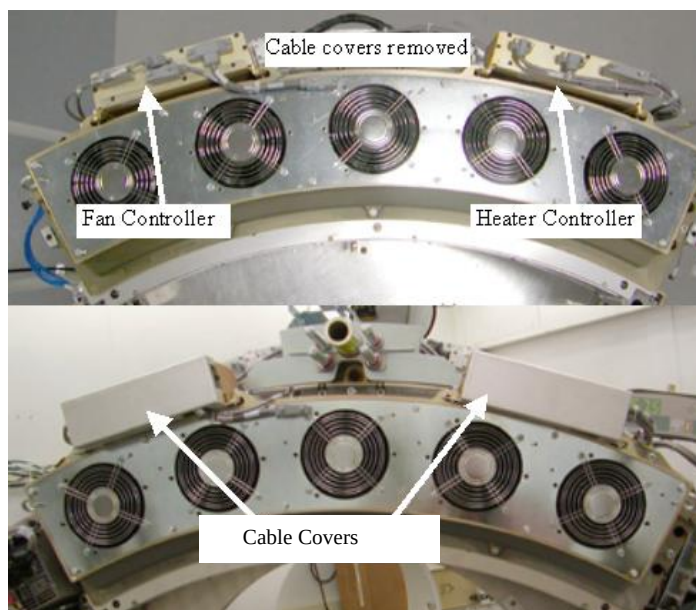

Resolution:

If you performed the upgrade and did not receive the covers with the upgrade kit, order 2 covers (part# 5170168) and install at your next site visit.

Affected Service Publication:

7.x VCT Service documentation 5193575

Tracking Number (PQR/SPR/ECR):

PQR 13165539 & 13155079

Steve Merritt
MICT Service Engineering