

Table of Contents

Chapter 1	
System Communications.....	3
Section 1.0 — Slip Ring Communications Interface - 2399621.....	4
Section 2.0 — Final Scan Control, Console Ethernet	5
Section 3.0 — Rotating Controller Interface Bus (RCIB) - 2399623.....	6
 Chapter 2	
X-Ray Generation	7
Section 1.0 — Tube Fans / Pump / SmartID Interface	8
Section 2.0 — JEDI Interface - kV Loop	9
Section 3.0 — JEDI Interface - mA Loop - 5141527	10
Section 4.0 — X-Ray Collimation & Filtration - 2399626.....	11
Section 5.0 — Exposure Enable and Final Command - 2399629	12
Section 6.0 — Tube Rotor Control.....	13
 Chapter 3	
Data Acquisition	15
Section 1.0 — Trigger Generation - 2399724	16
Section 2.0 — Detector Heater (DAS Item) - 2399725	17
 Chapter 4	
Patient Positioning	19
Section 1.0 — Alignment Lights - 2399726	20
Section 2.0 — Gantry Tilt, from Gantry, Console - 2399727	21
 Chapter 5	
Axial Control	23
Section 1.0 — Axial Servo Control / Dynamic Brake - 2399731	24
Section 2.0 — Axial Power Distribution - 2399732	25
 Chapter 6	
Operator I/O.....	27
Section 1.0 — Gantry Operator Interface and Displays - 2399733.....	28
Section 2.0 — Gantry Reset from Console	29


Section 3.0 — Gantry Reset from Console (All-In-One).....	30
Section 4.0 — Cardiac Options - 2399735	31
Section 5.0 — Pulmonary Options - 2399736.....	32
Section 6.0 — Site X-Ray Light, System Light - 2399738.....	33
Section 7.0 — Autovoice / Intercom - 2399739	34
 Chapter 7	
System Monitoring	35
Section 1.0 — Gantry Temperature and Balance Sensors - 2399740	36
Section 2.0 — Gantry Cover Fans - 2399741.....	37
 Chapter 8	
System Power Control	39
Section 1.0 — System E-Stop and Power Interlocks - 2399742	40
Section 2.0 — PDU - Gantry 120 VAC Control - 2399743	41
Section 3.0 — HV_DC_Control - 2399744.....	42
Section 4.0 — HP MDAS/GDAS Gantry Power Distribution - 2399627	43

THIS PAGE INTENTIONALLY BLANK.

Chapter 1

System Communications

Section 1.0 — Slip Ring Communications Interface - 2399621

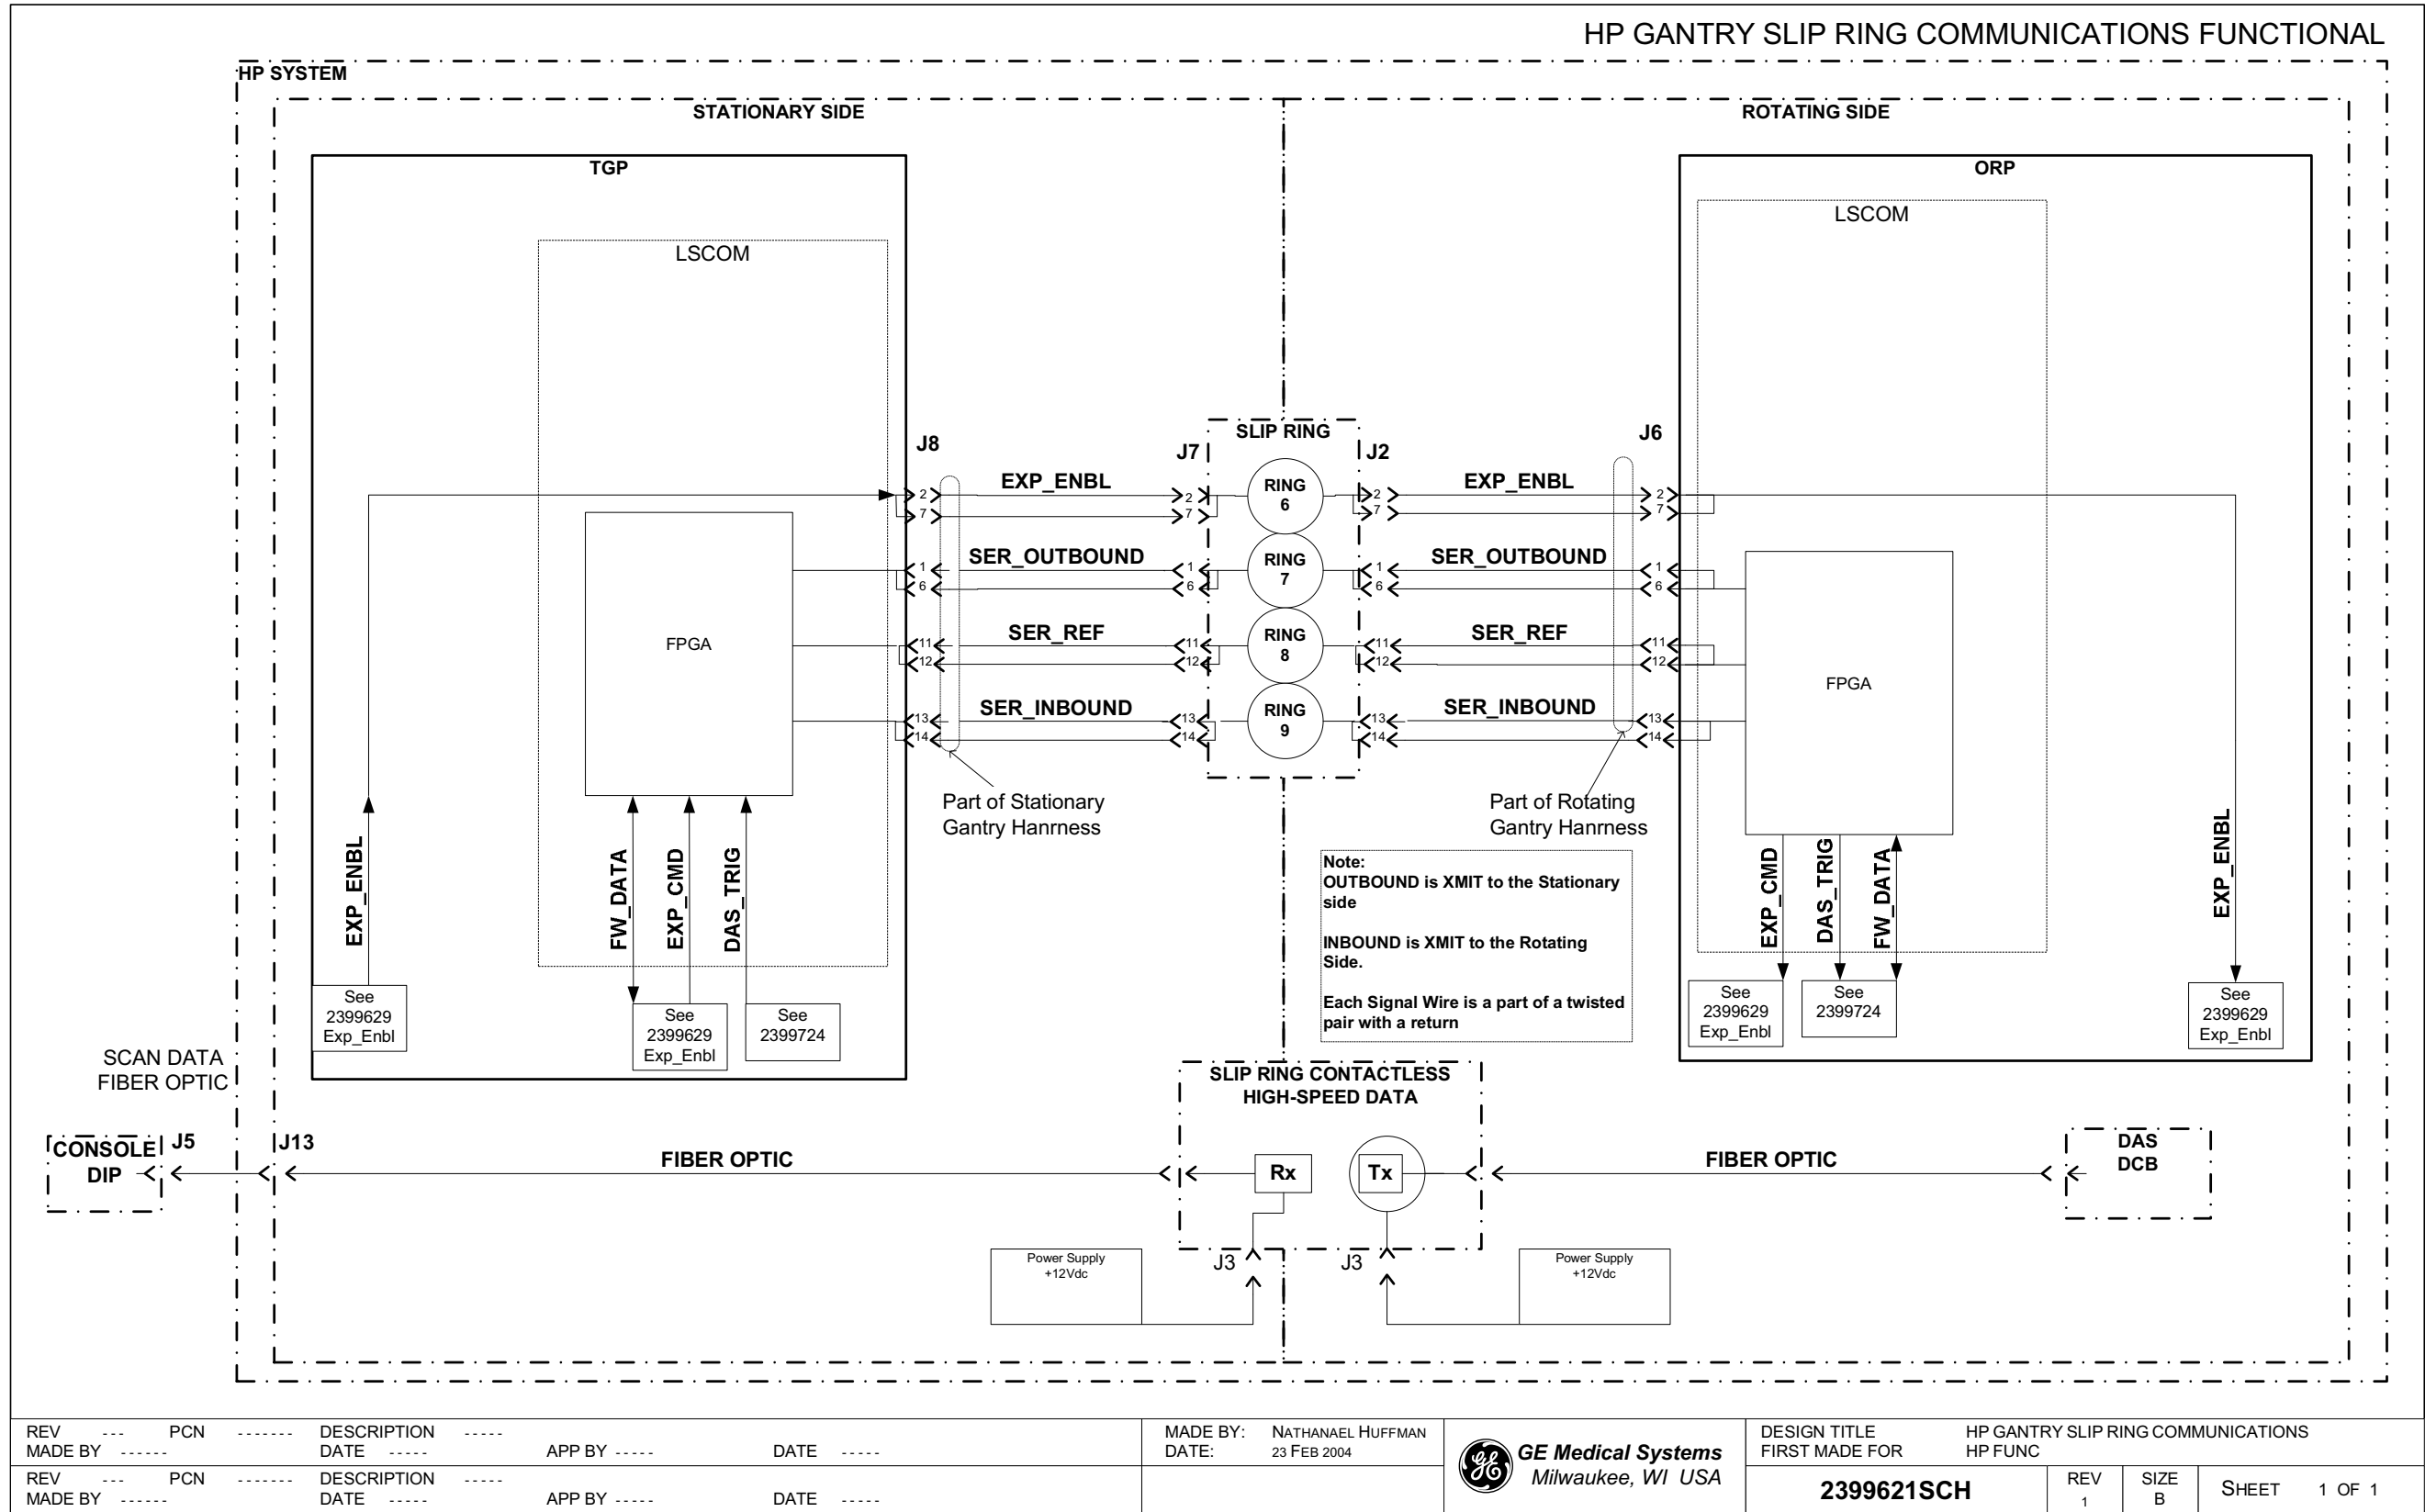

REV	---	PCN	-----	DESCRIPTION	-----	APP BY	-----	DATE	-----	MADE BY:	NATHANAEL HUFFMAN	 GE Medical Systems Milwaukee, WI USA	DESIGN TITLE FIRST MADE FOR				HP GANTRY SLIP RING COMMUNICATIONS HP FUNC			
REV	---	PCN	-----	DESCRIPTION	-----	APP BY	-----	DATE	-----	DATE:	23 FEB 2004		2399621SCH	REV	1	SIZE	B	SHEET	1 OF 1	

Figure 1-1 2399621 Sheet 1, Rev. 1

Section 2.0 — Final Scan Control, Console Ethernet

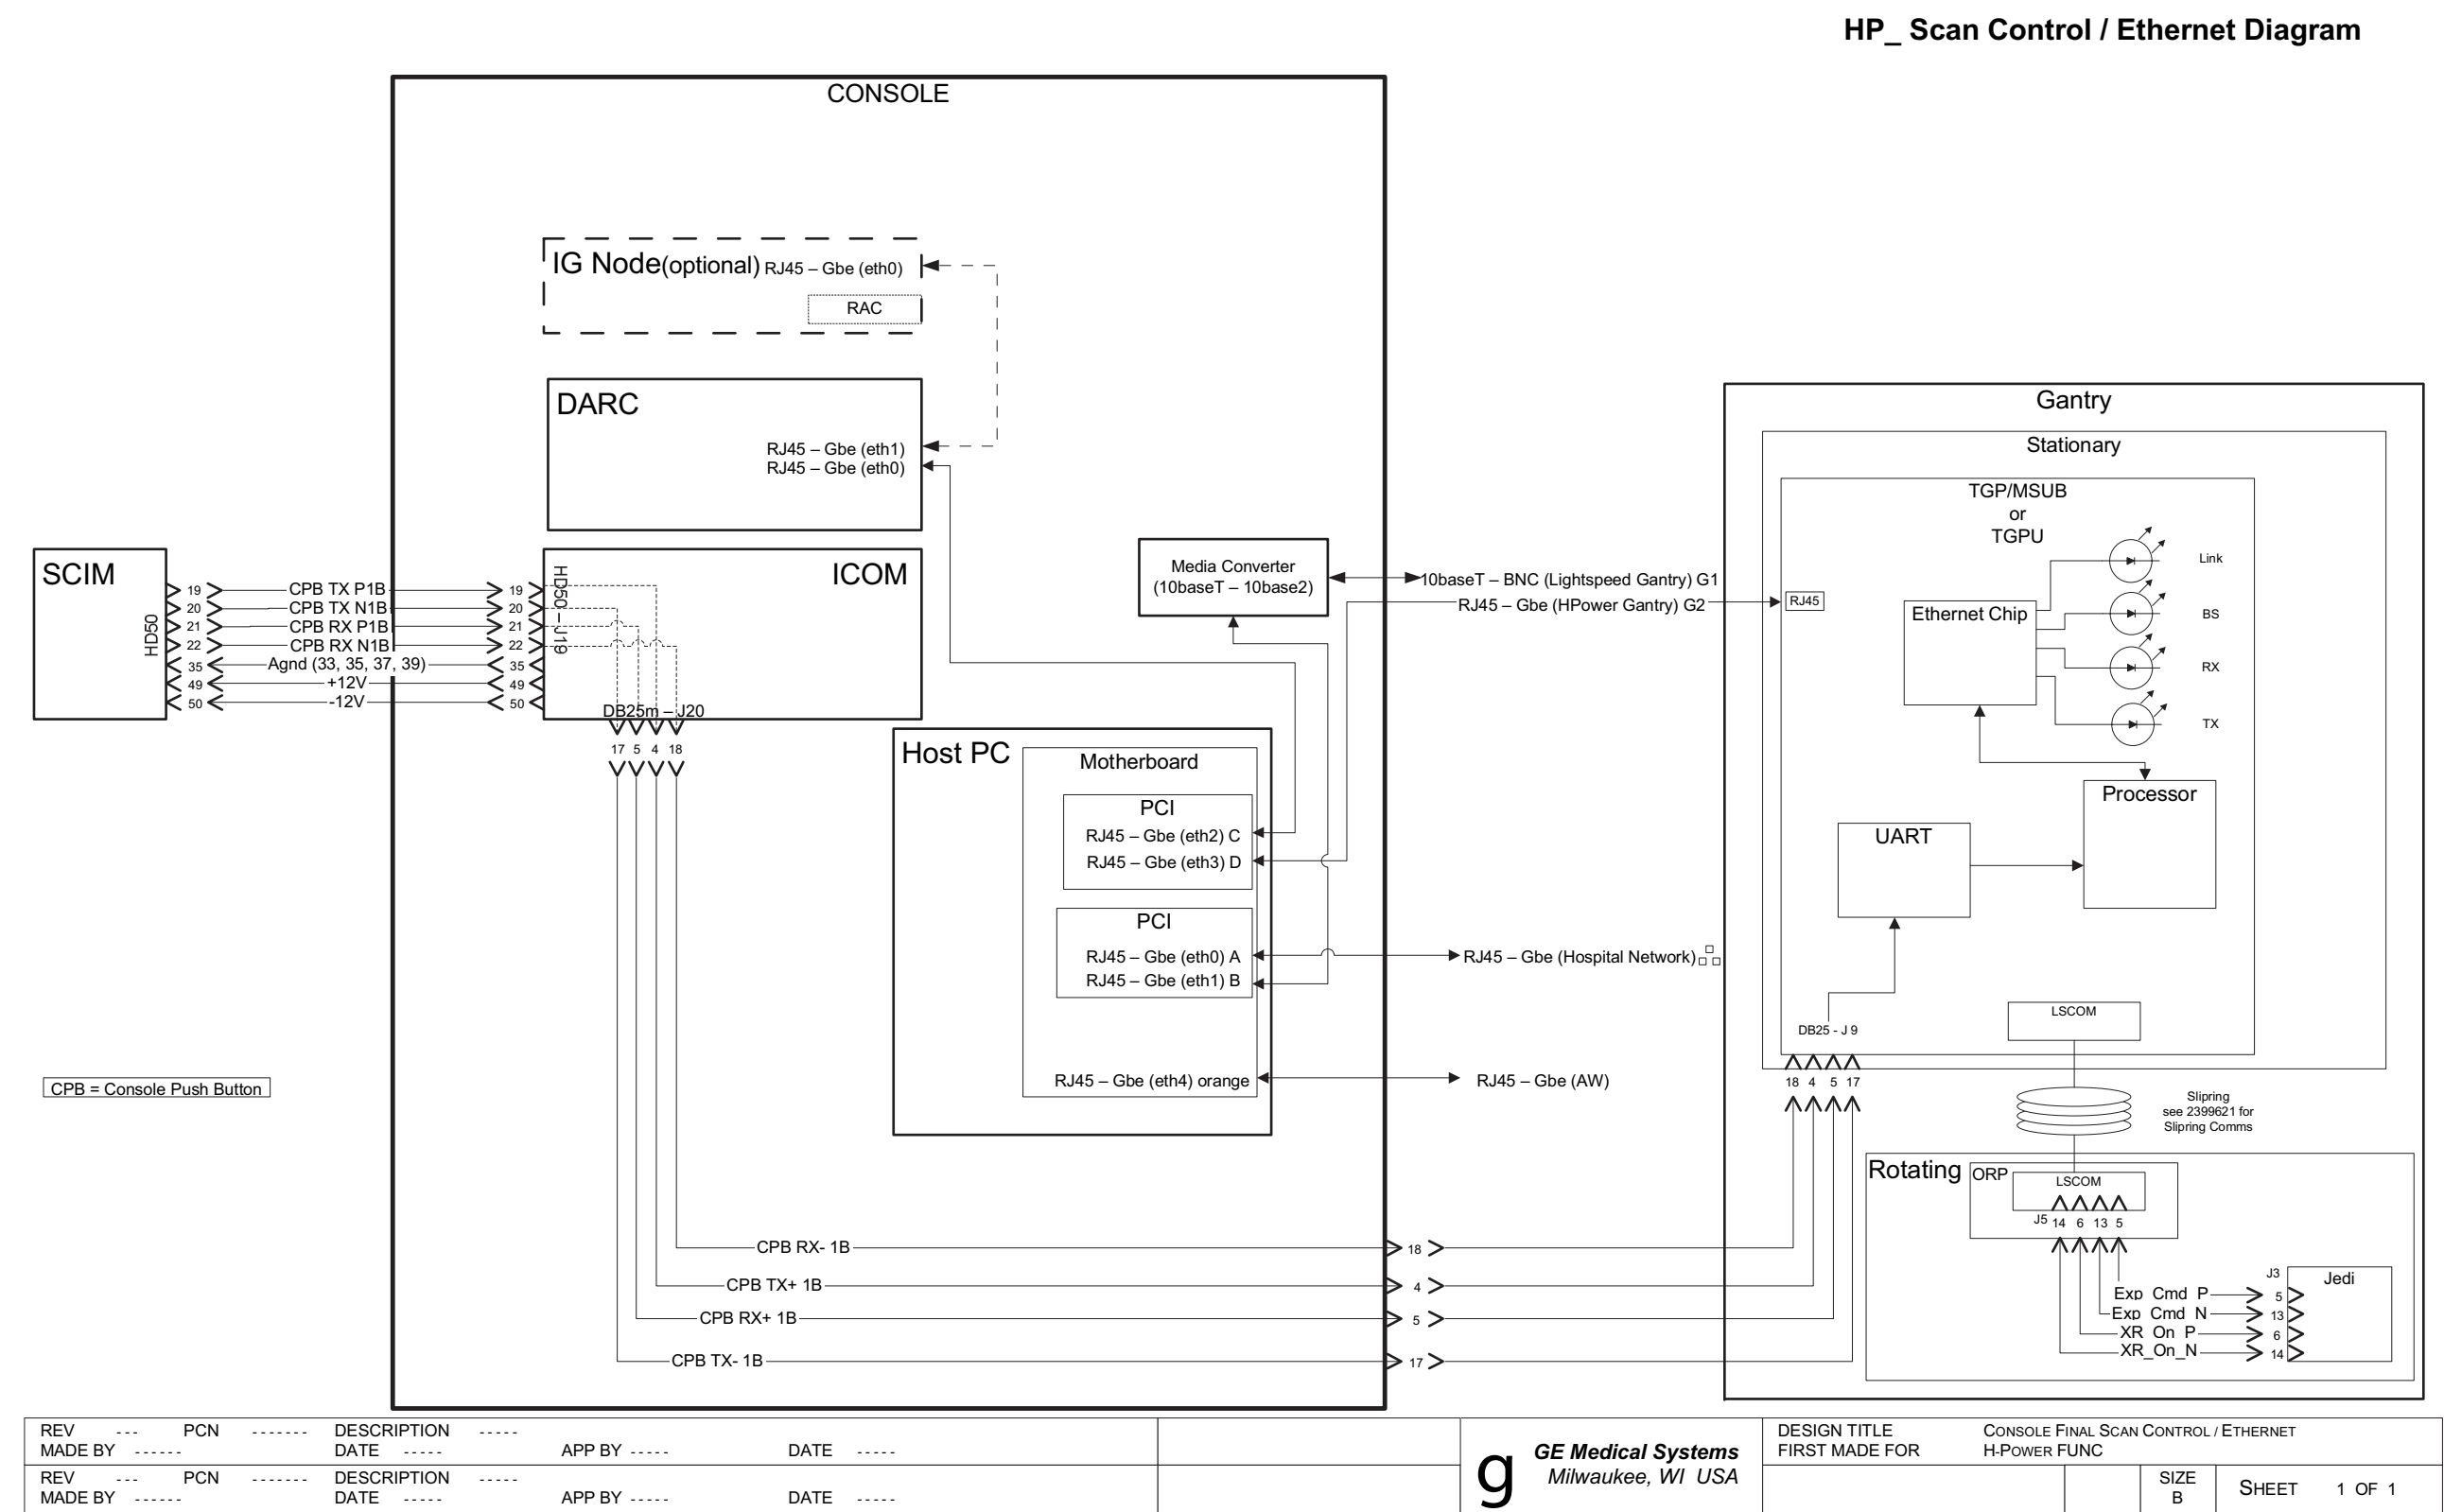


Figure 1-2 2399622 Sheet 1, Rev 1

Section 3.0 — Rotating Controller Interface Bus (RCIB) - 2399623

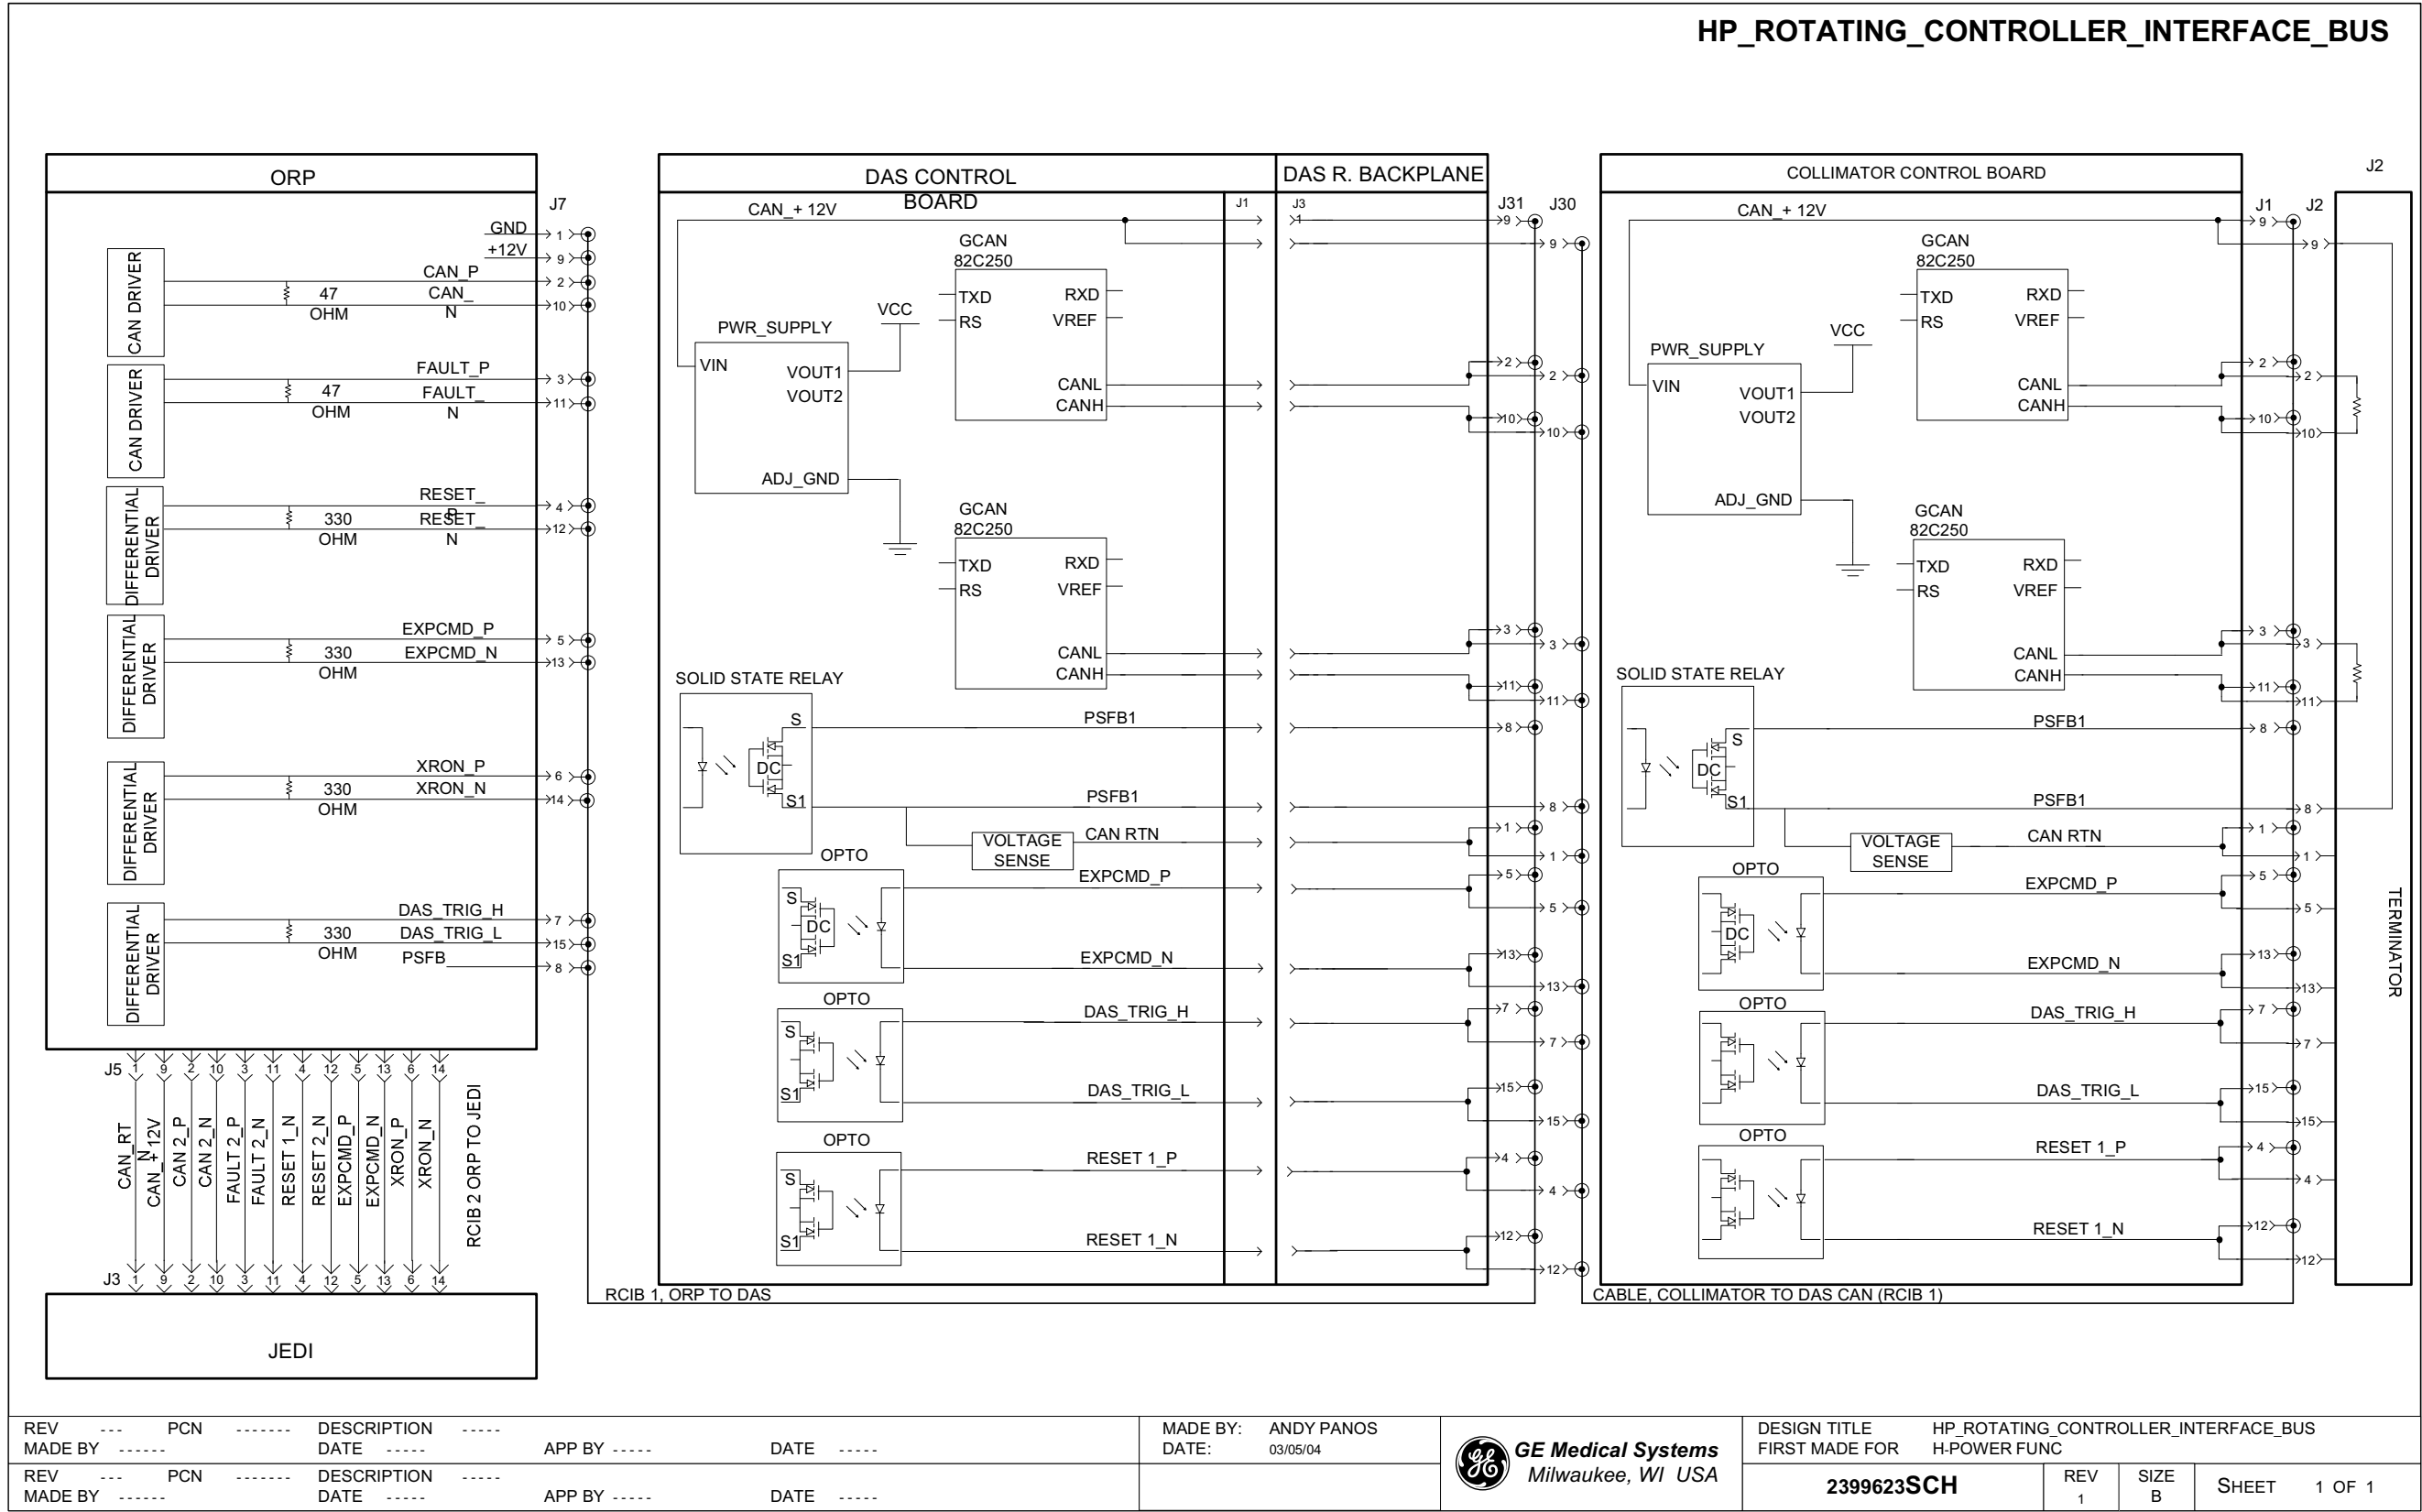


Figure 1-3 2399623 Sheet 1, Rev. 1

Chapter 2

X-Ray Generation

Section 1.0 — Tube Fans / Pump / SmartID Interface

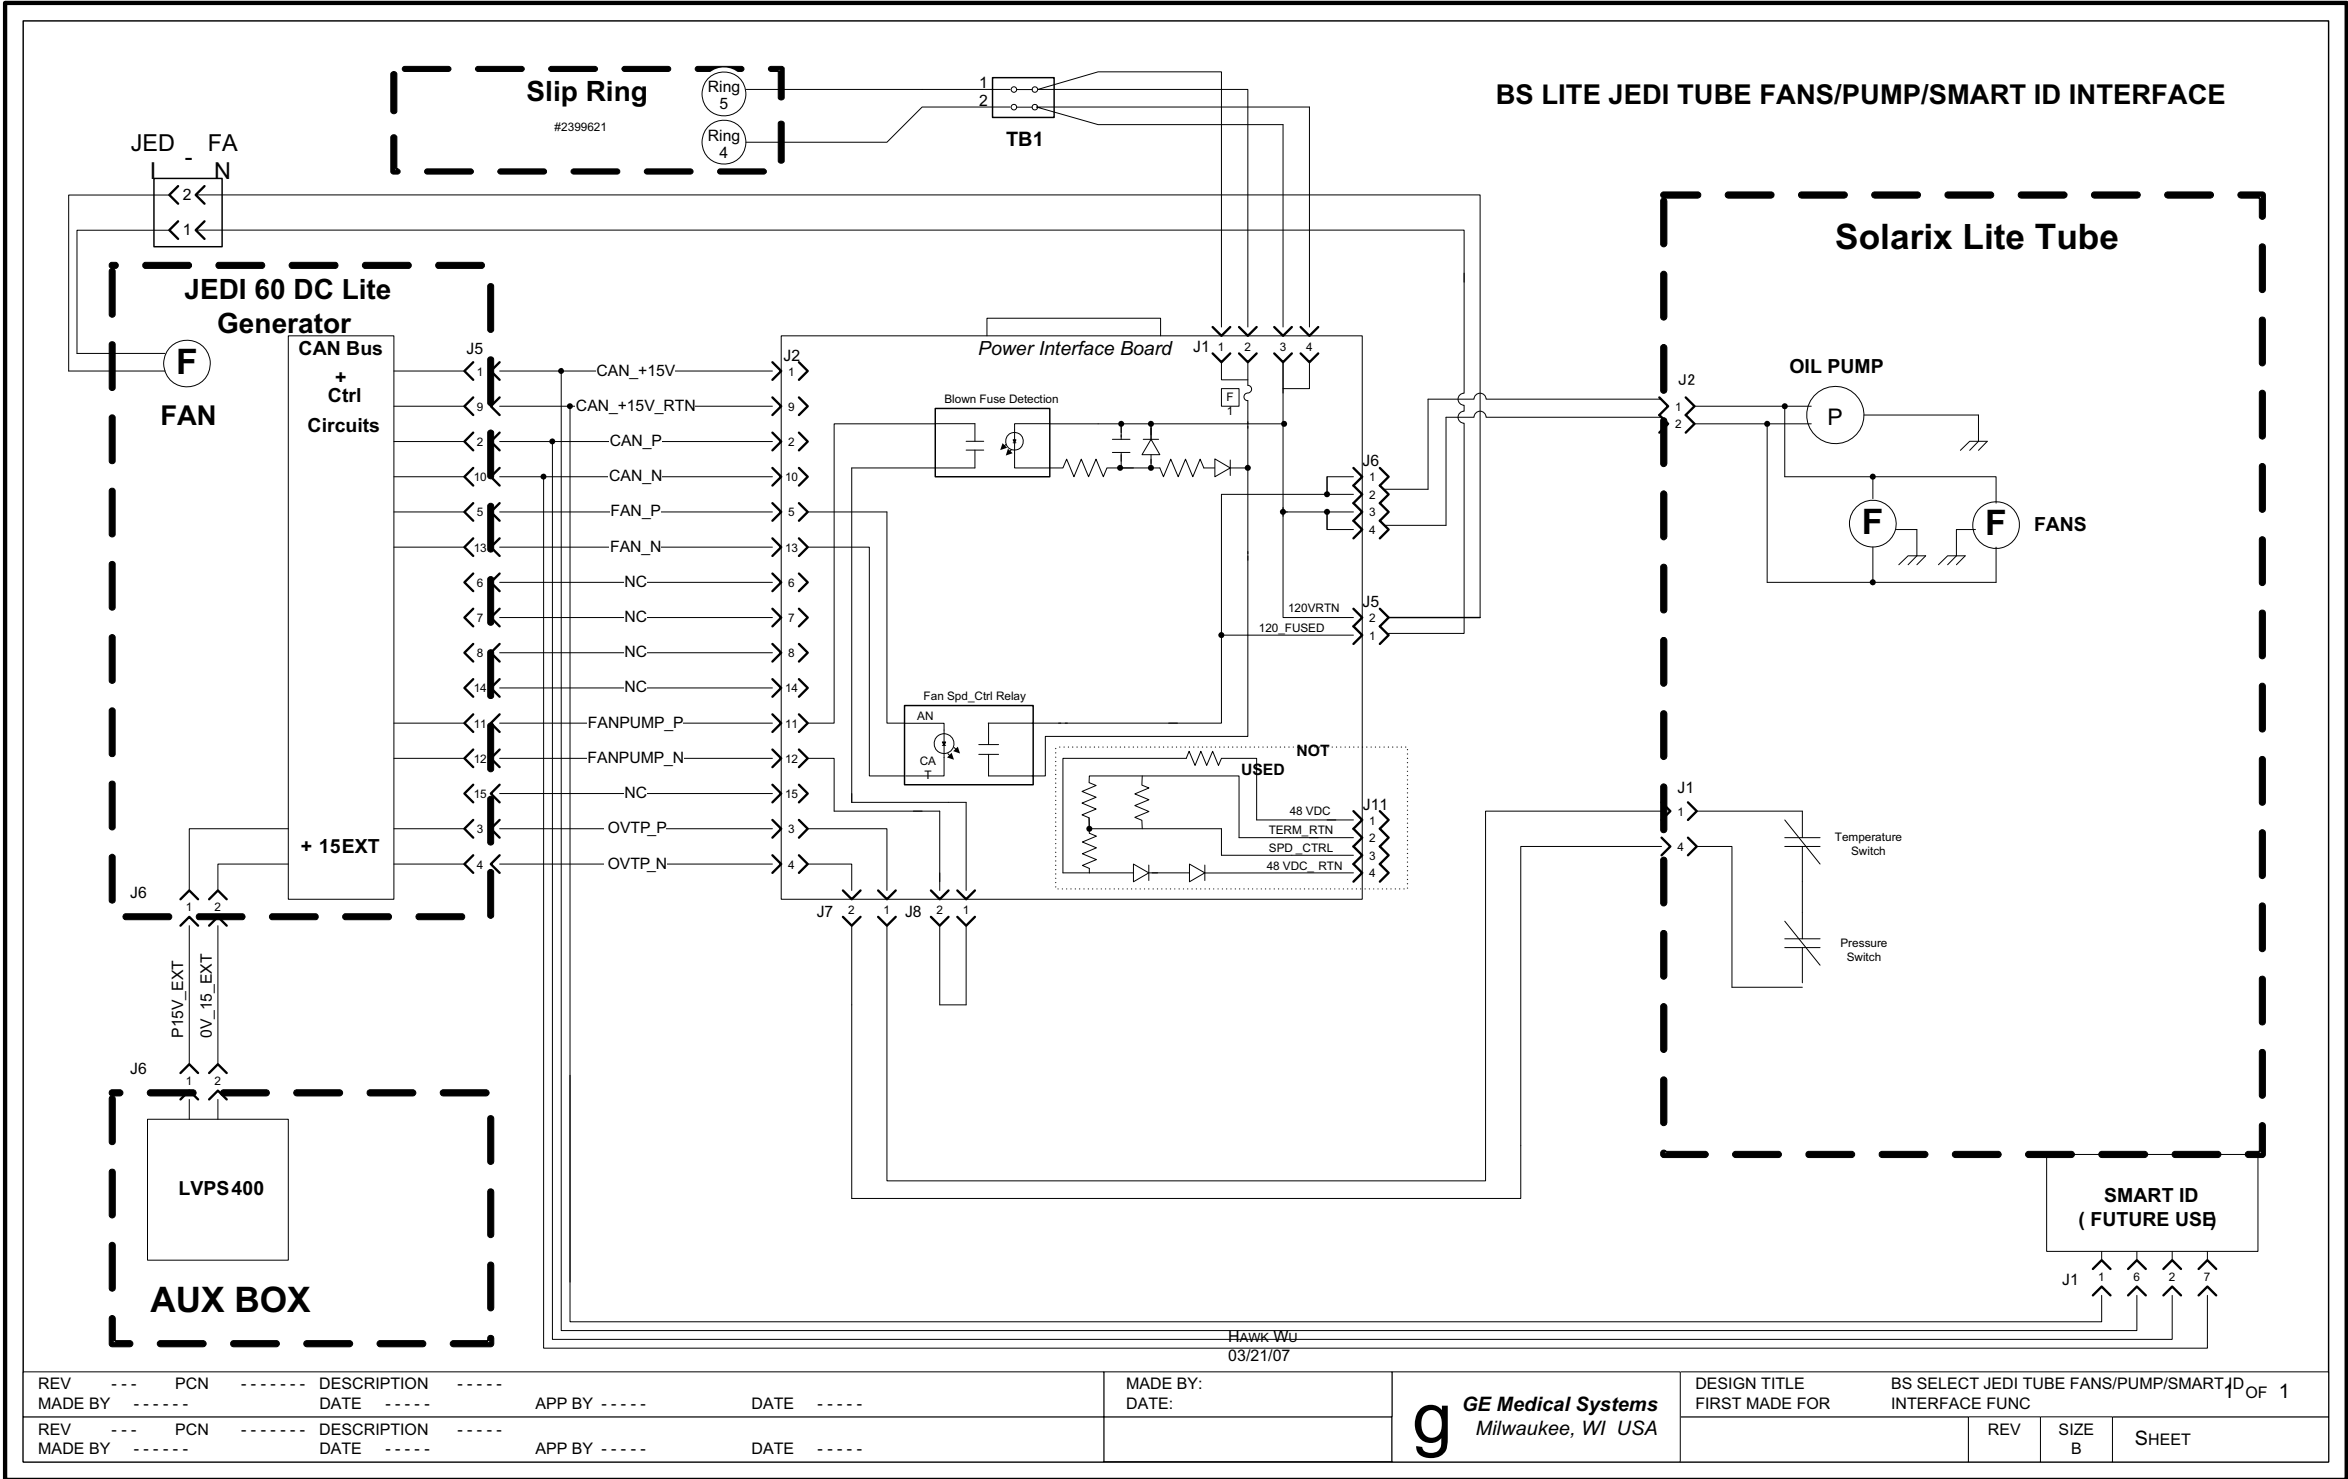


Figure 2-1 2399624 Sheet 1, Rev. 1

Section 2.0 — JEDI Interface - kV Loop

BS Lite JEDI kV Loop



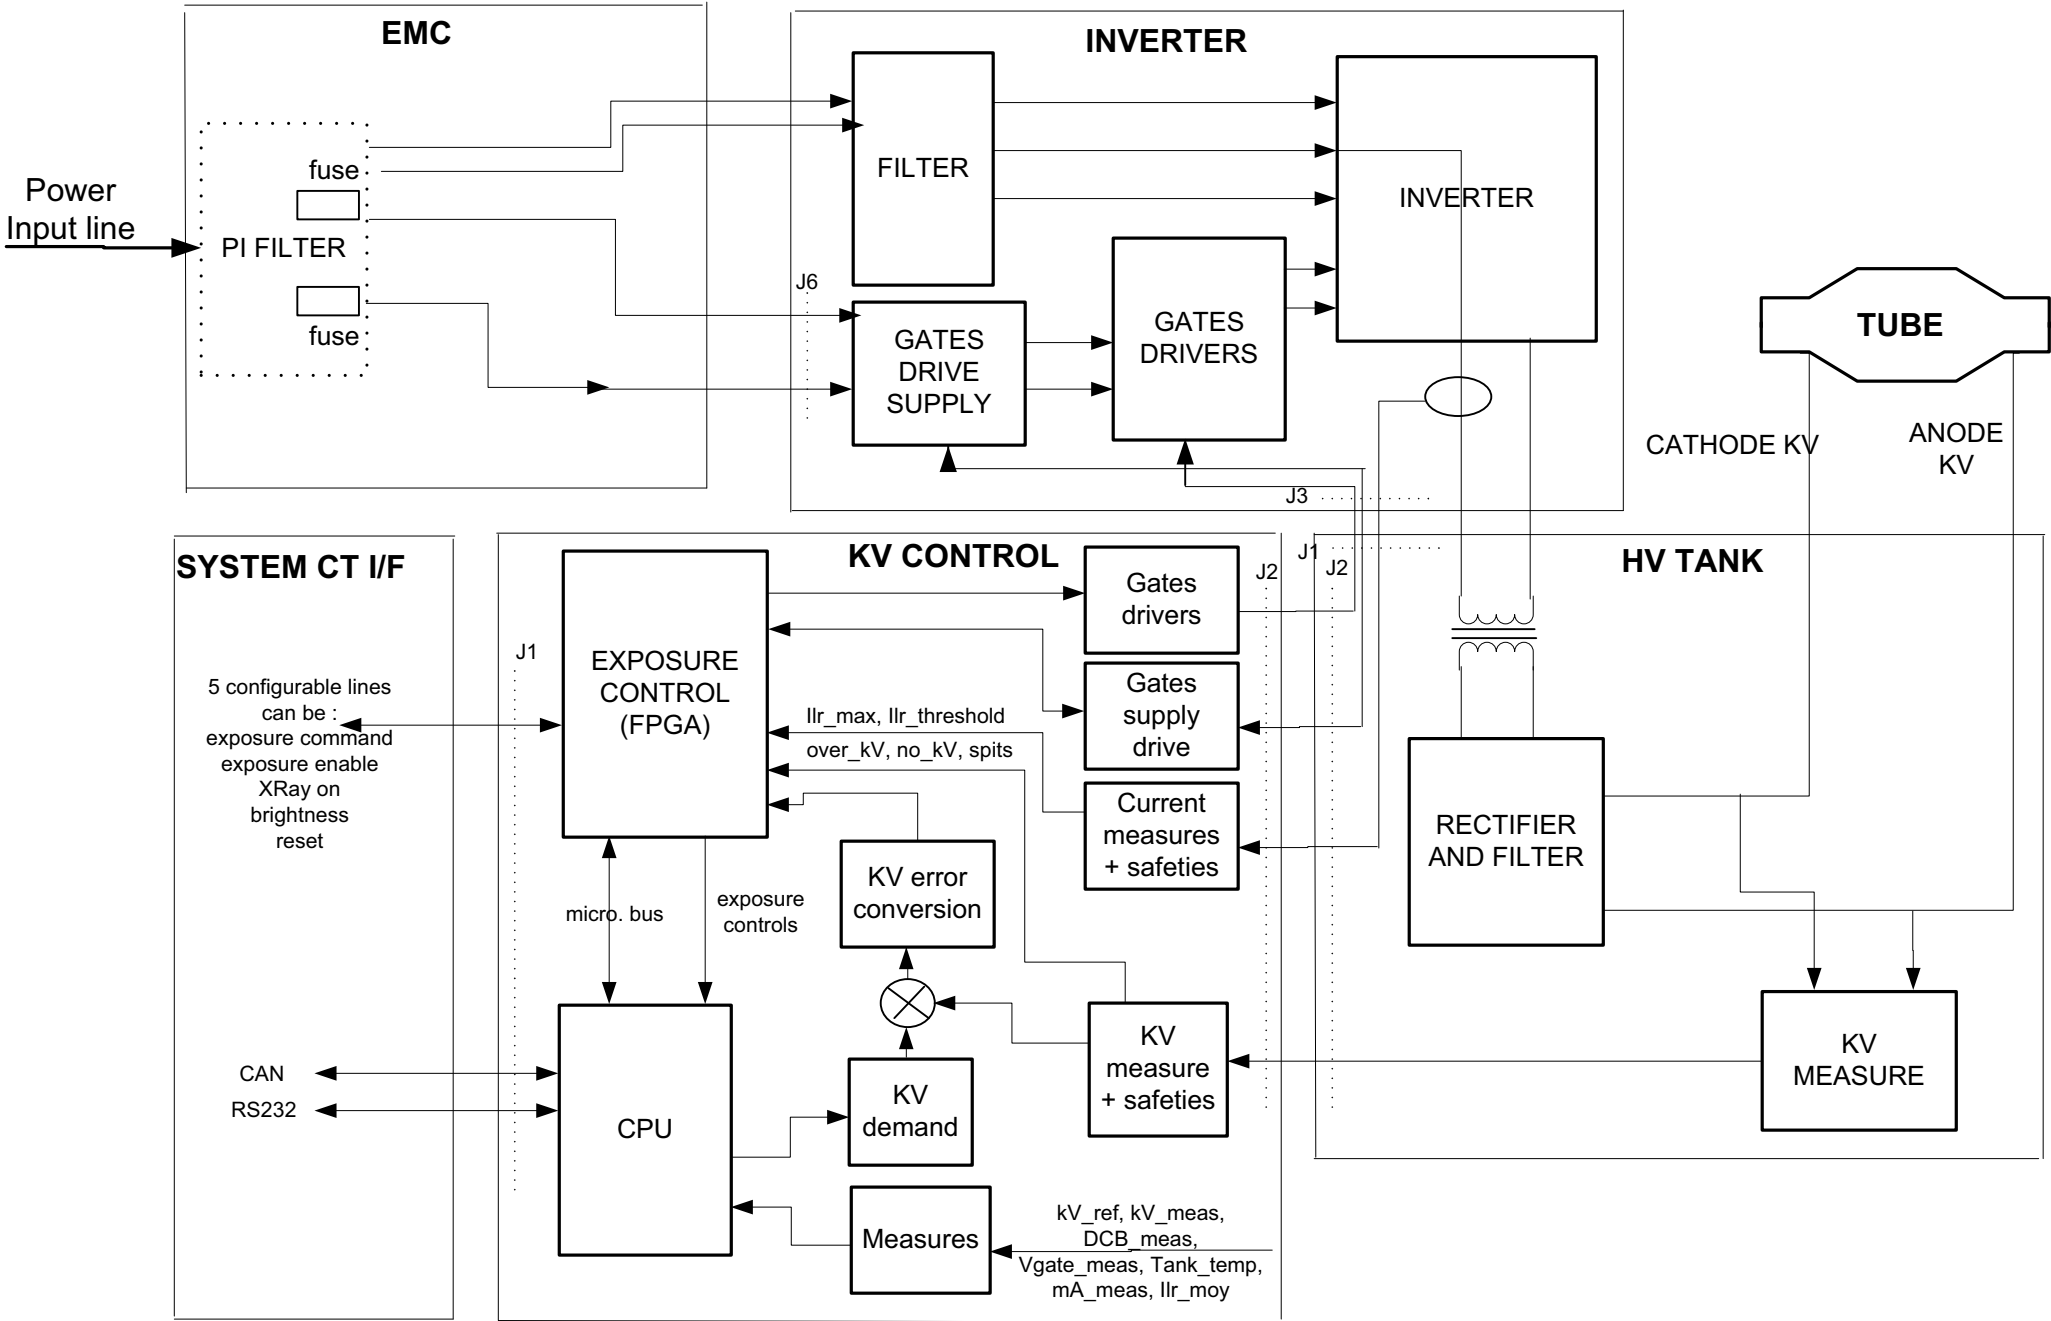


Figure 2-2 2399625 Sheet 1, Rev. 1

Figure 2-3 2399628 Sheet 1, Rev. 1



HP_X-Ray Collimation and Filtration



Section 5.0 — Exposure Enable and Final Command - 2399629

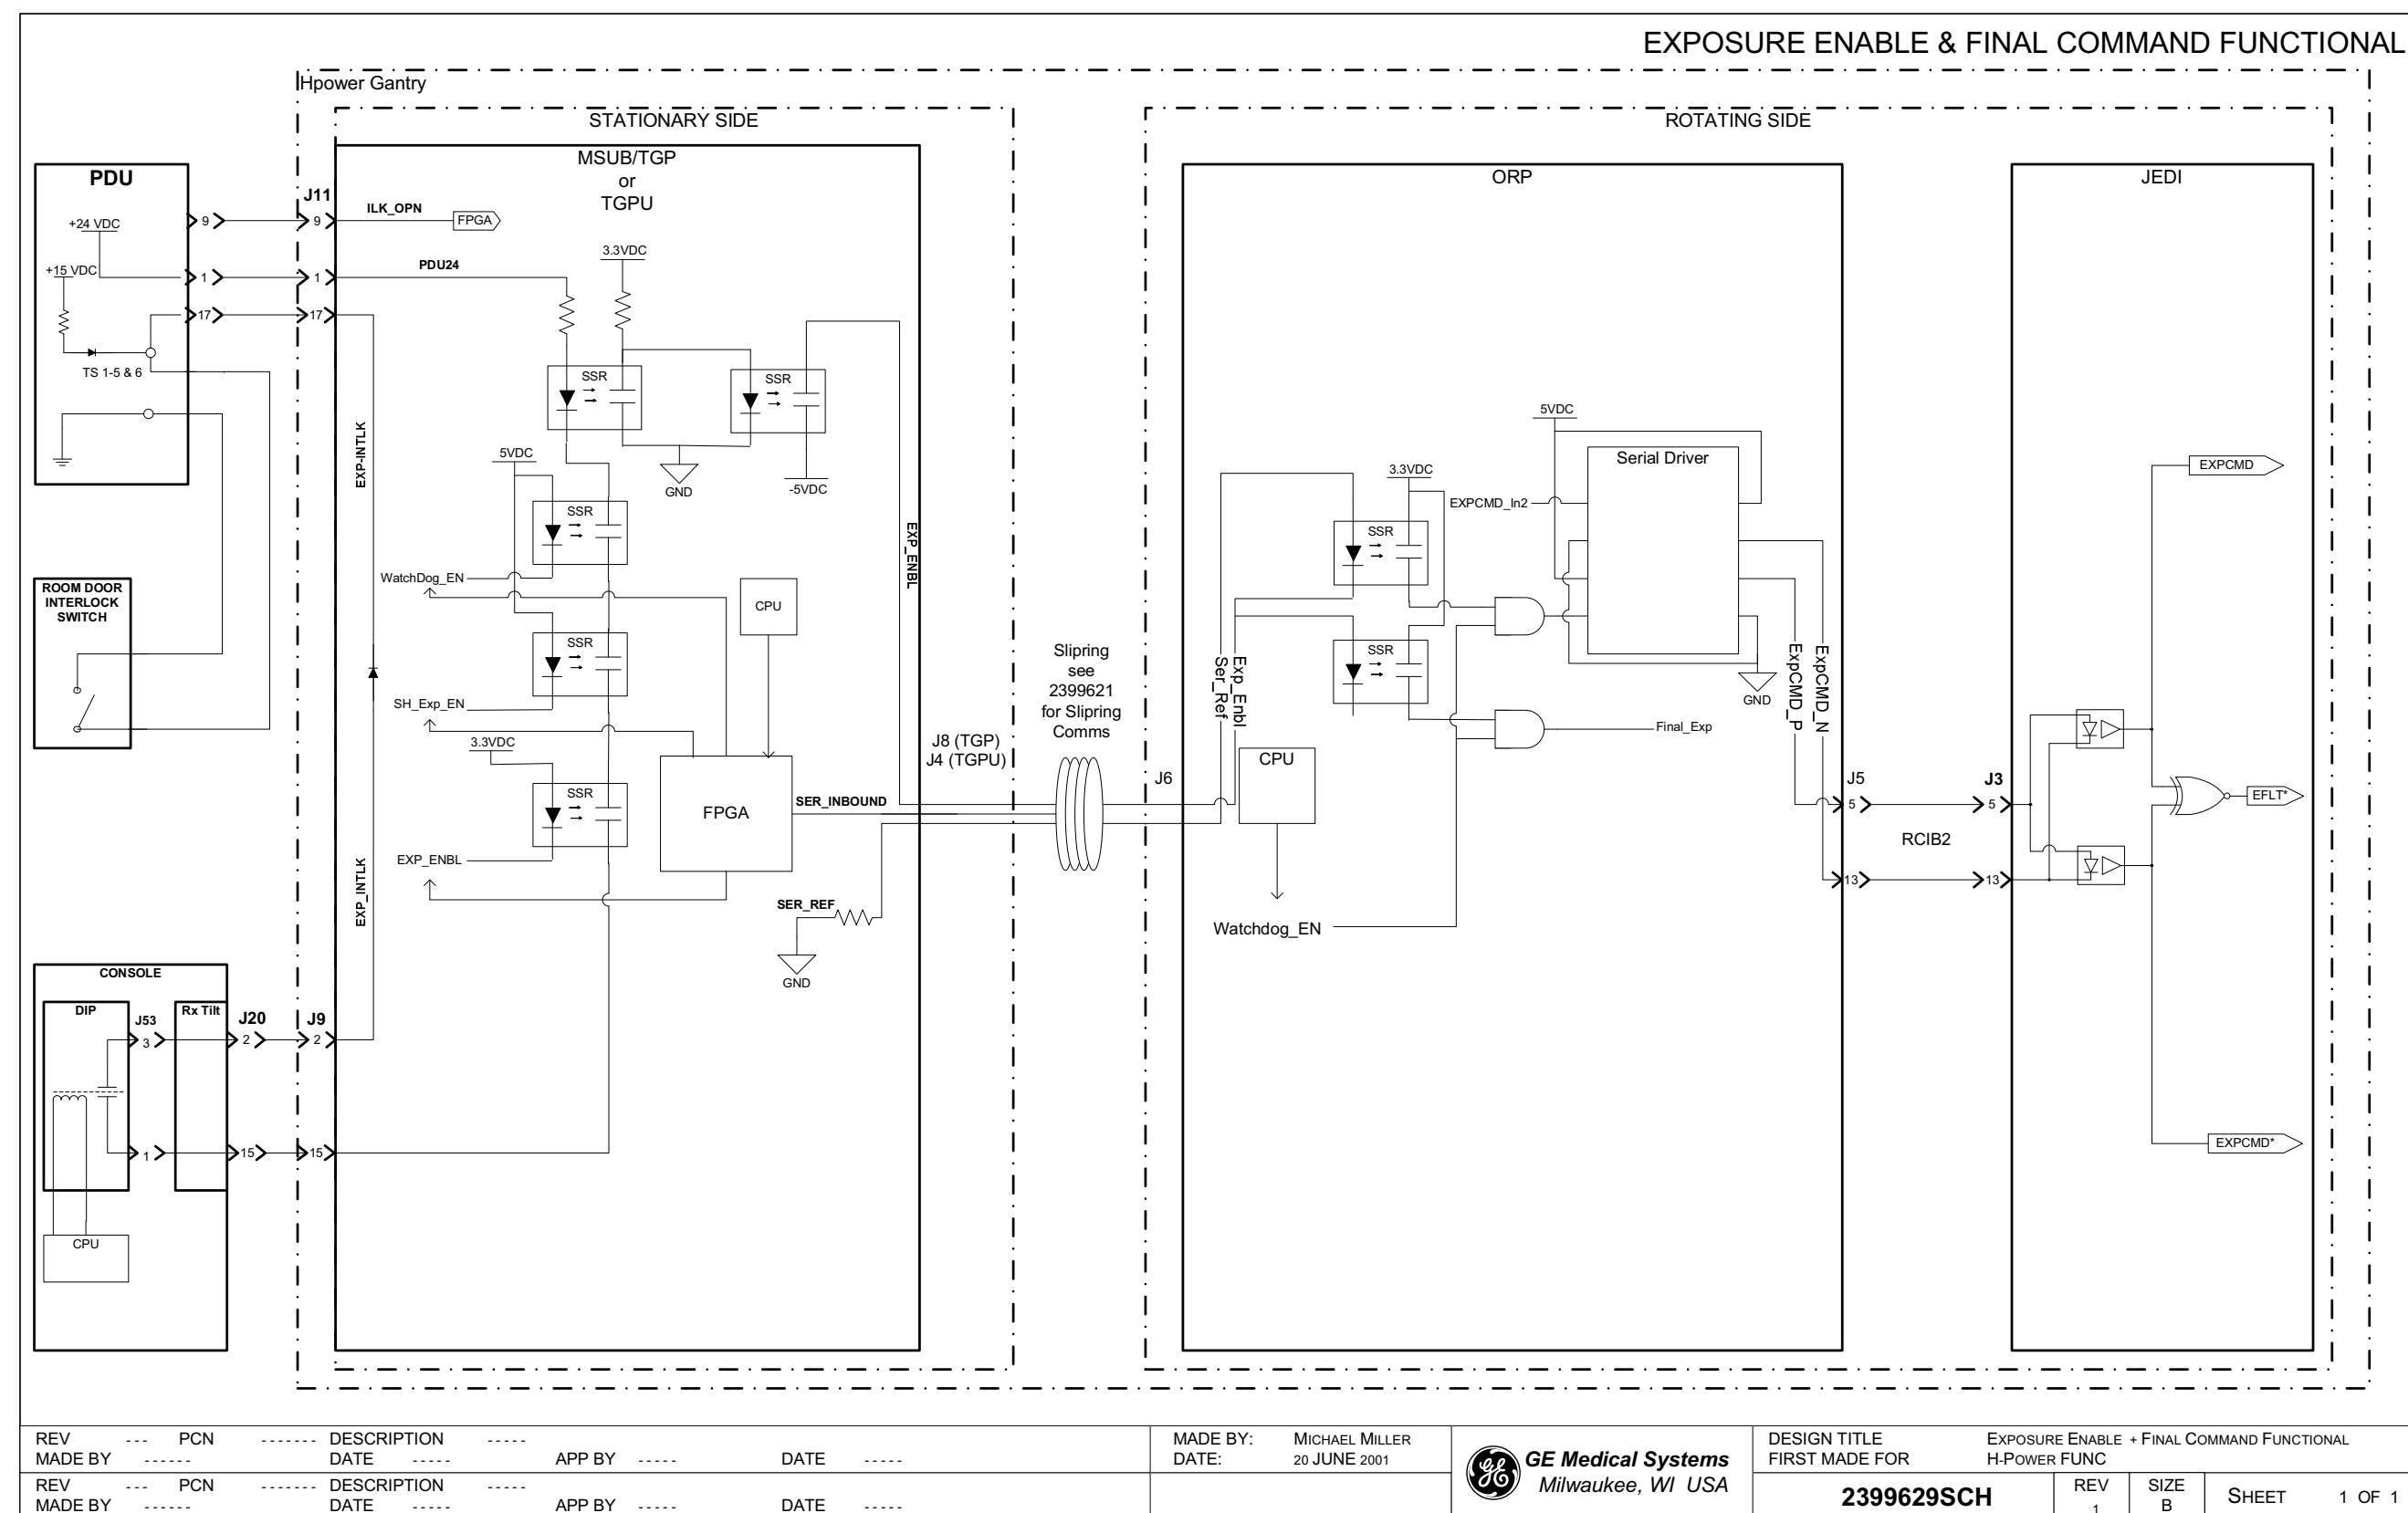


Figure 2-5 2399629 Sheet 1, Rev. 1

Section 6.0 — Tube Rotor Control


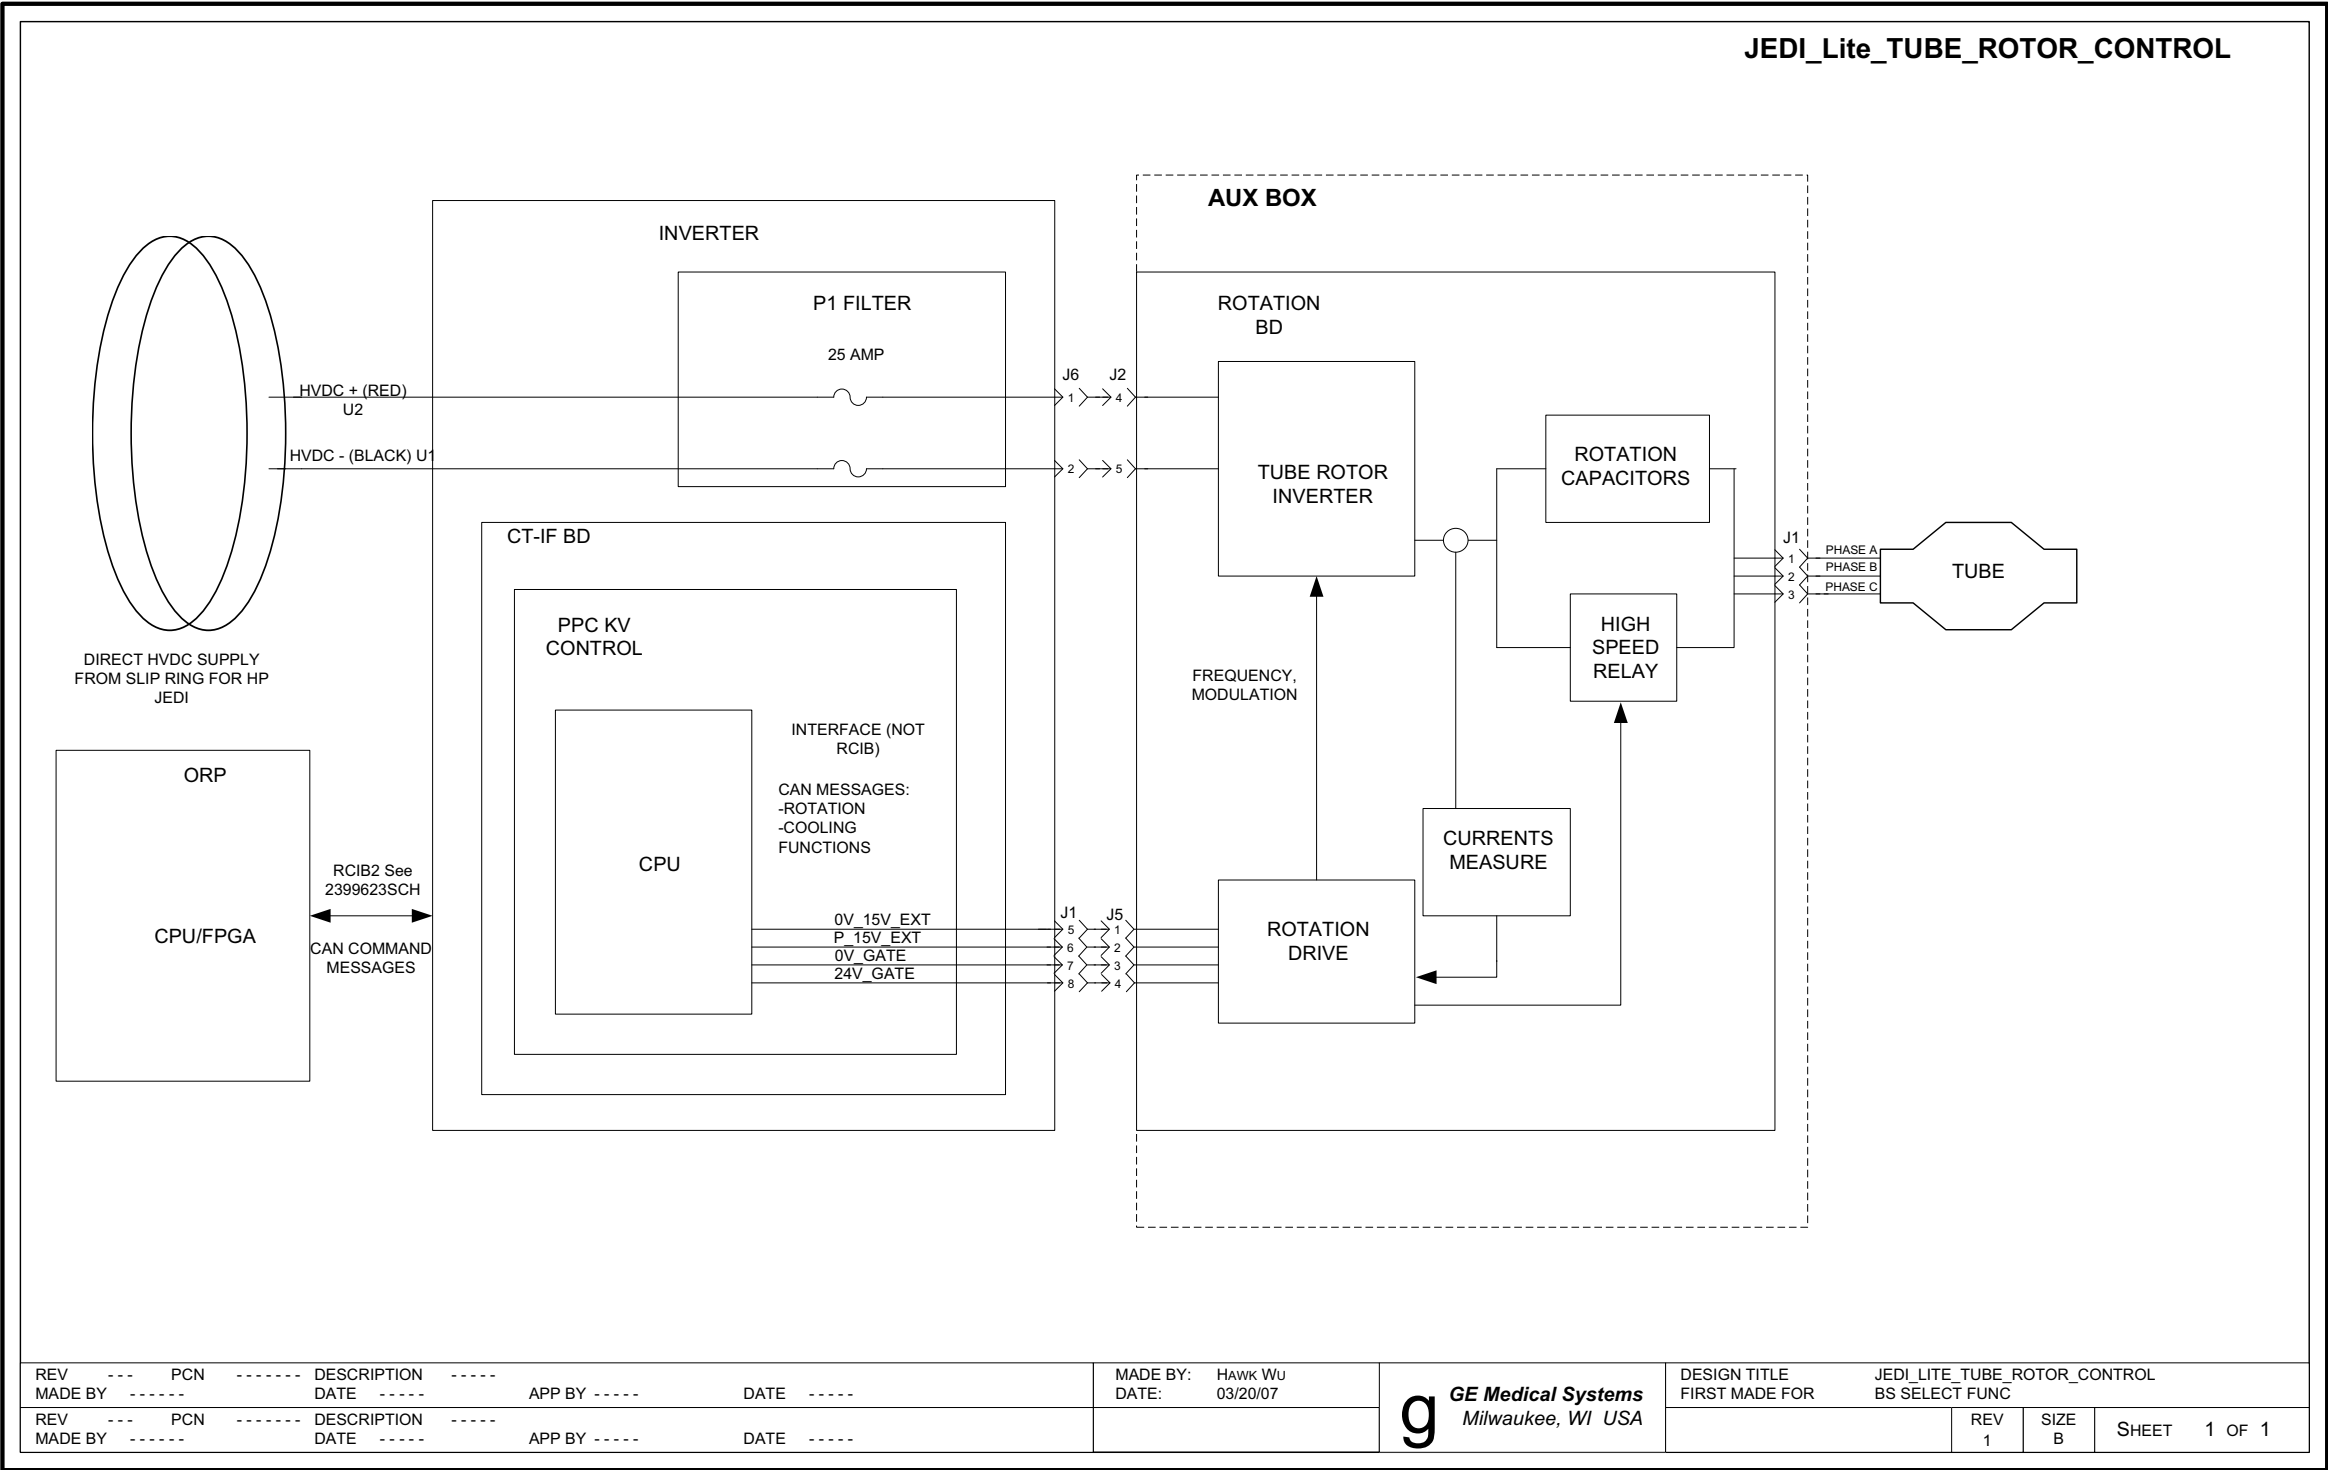


Figure 2-6 2399630 Sheet 1, Rev. 1

Chapter 3

Data Acquisition

Section 1.0 — Trigger Generation - 2399724

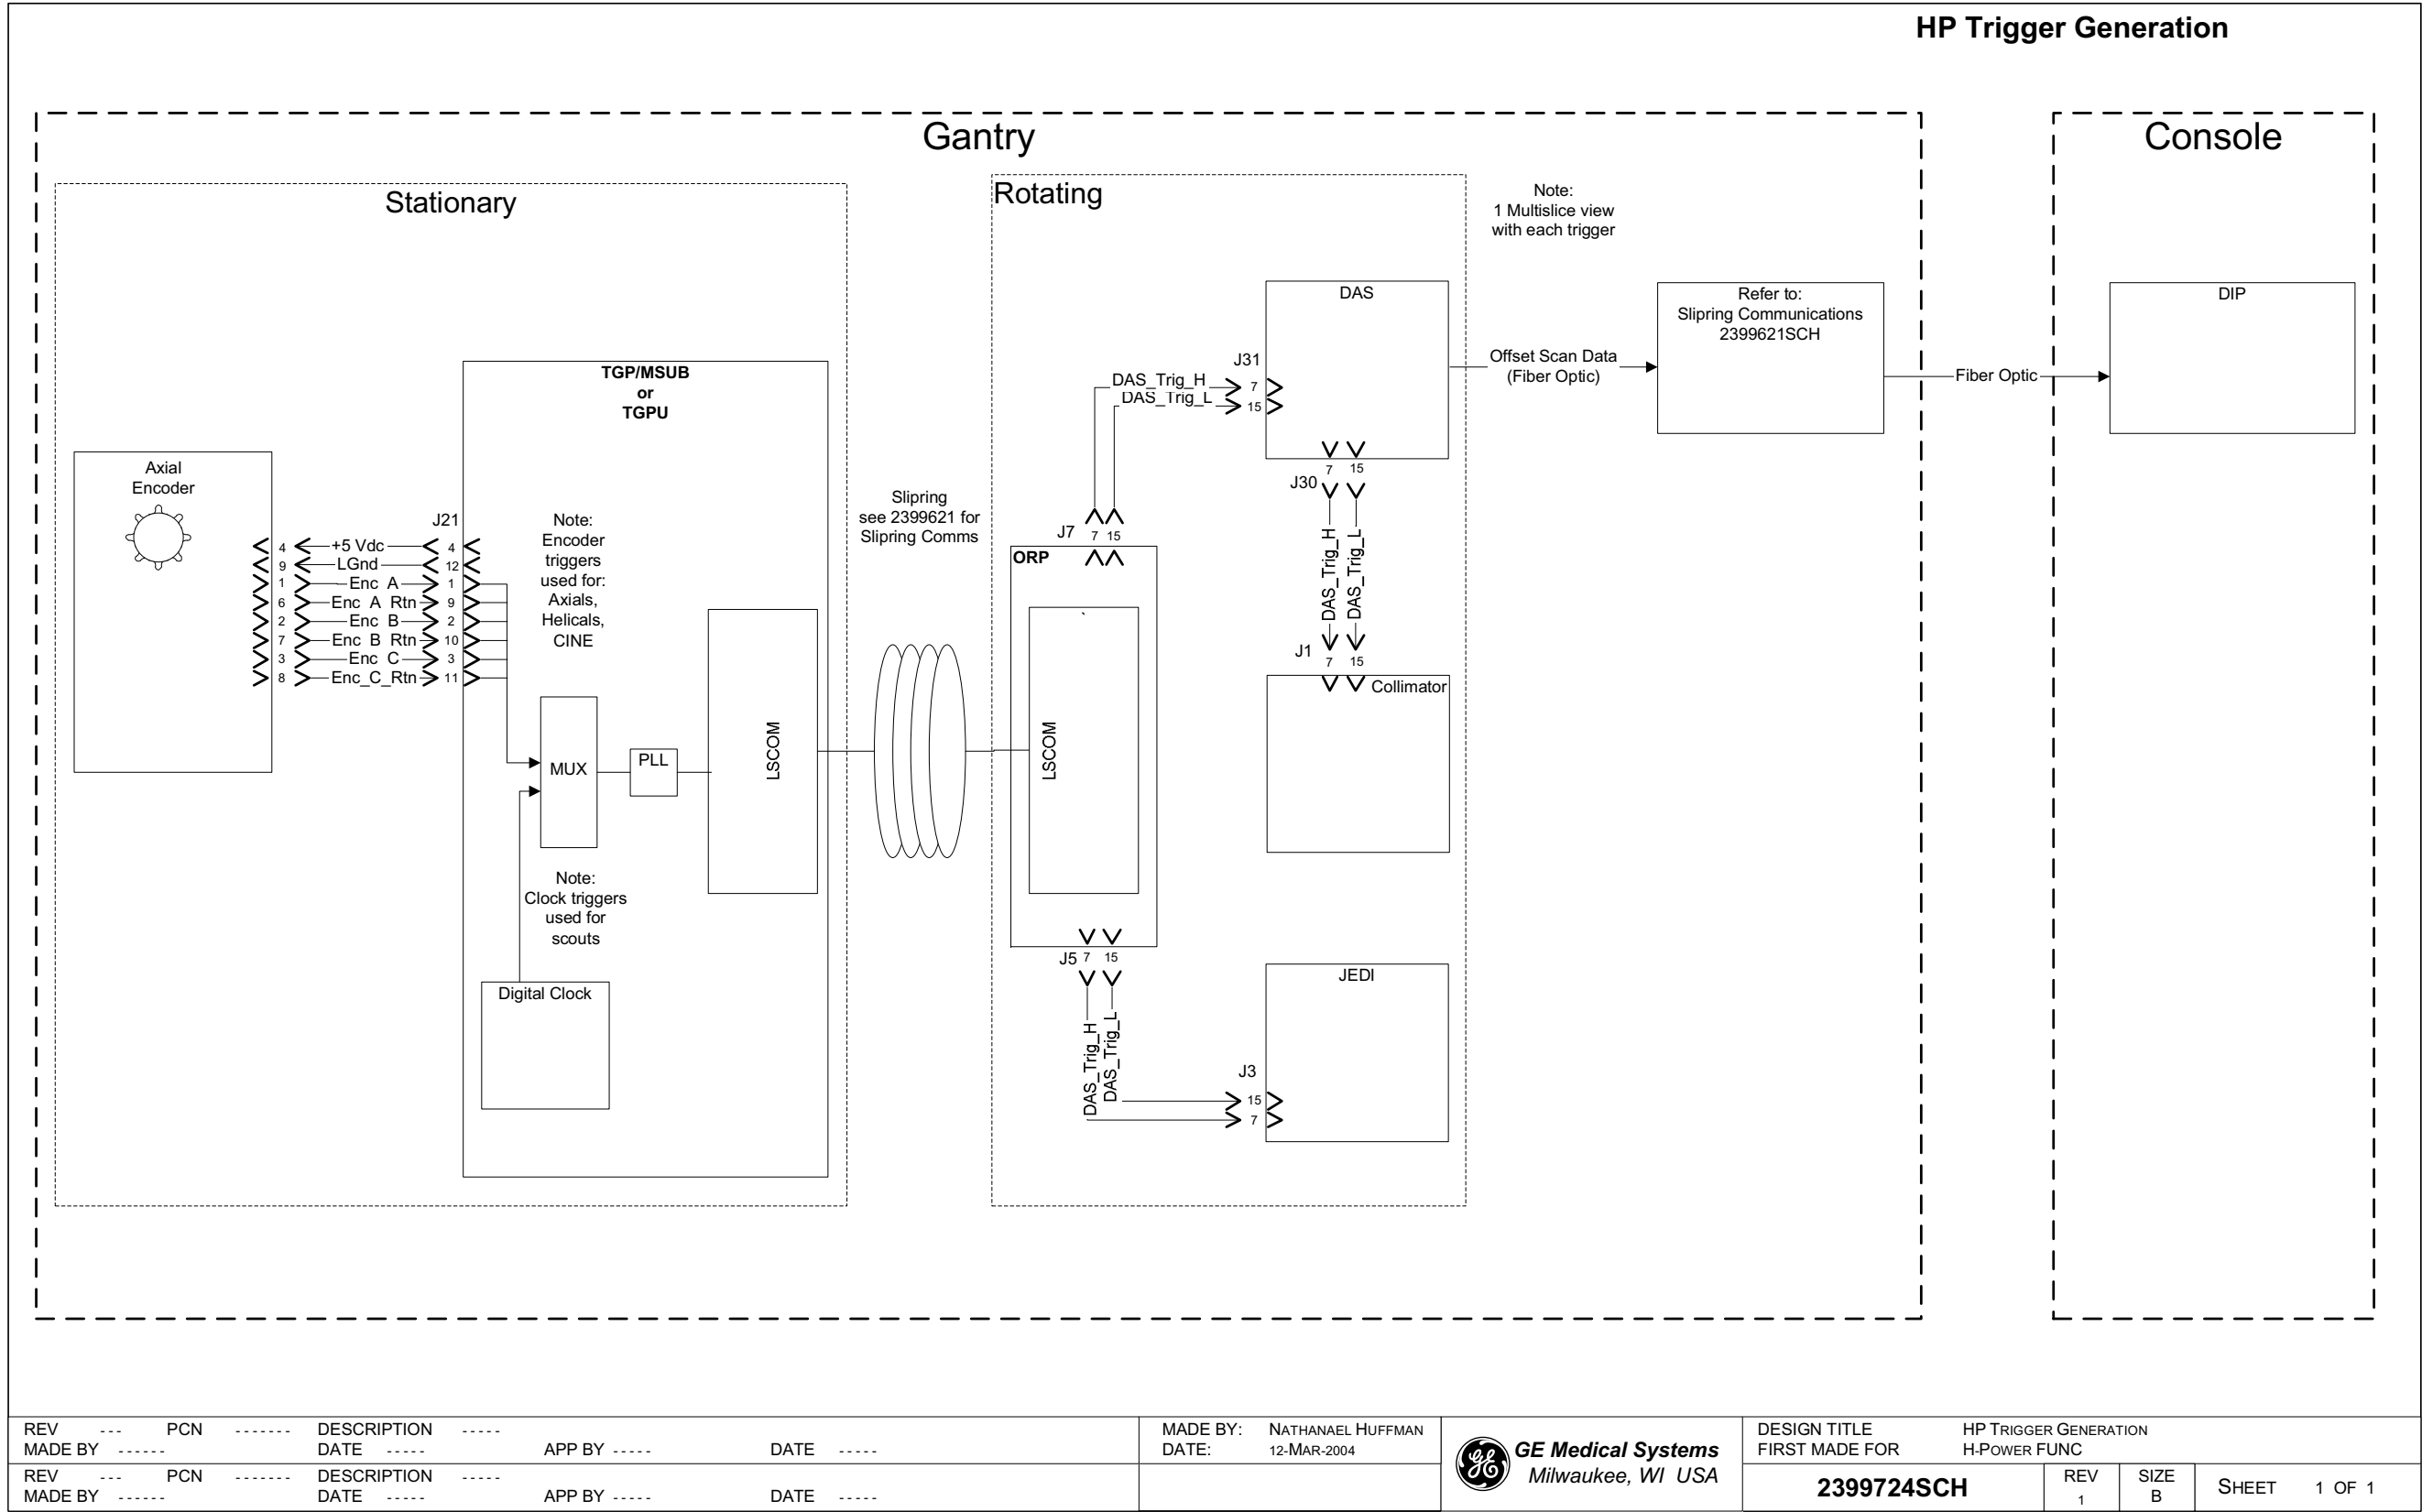

REV --- PCN ----- DESCRIPTION -----	MADE BY: NATHANAEL HUFFMAN	DESIGN TITLE HP TRIGGER GENERATION
MADE BY ----- DATE ----- APP BY ----- DATE -----	DATE: 12-MAR-2004	FIRST MADE FOR H-POWER FUNC
REV --- PCN ----- DESCRIPTION -----	GE Medical Systems Milwaukee, WI USA	2399724SCH
MADE BY ----- DATE ----- APP BY ----- DATE -----		REV 1 SIZE B SHEET 1 OF 1

Figure 3-1 2399724 Sheet 1, Rev. 1

Section 2.0 — Detector Heater (DAS Item) - 2399725

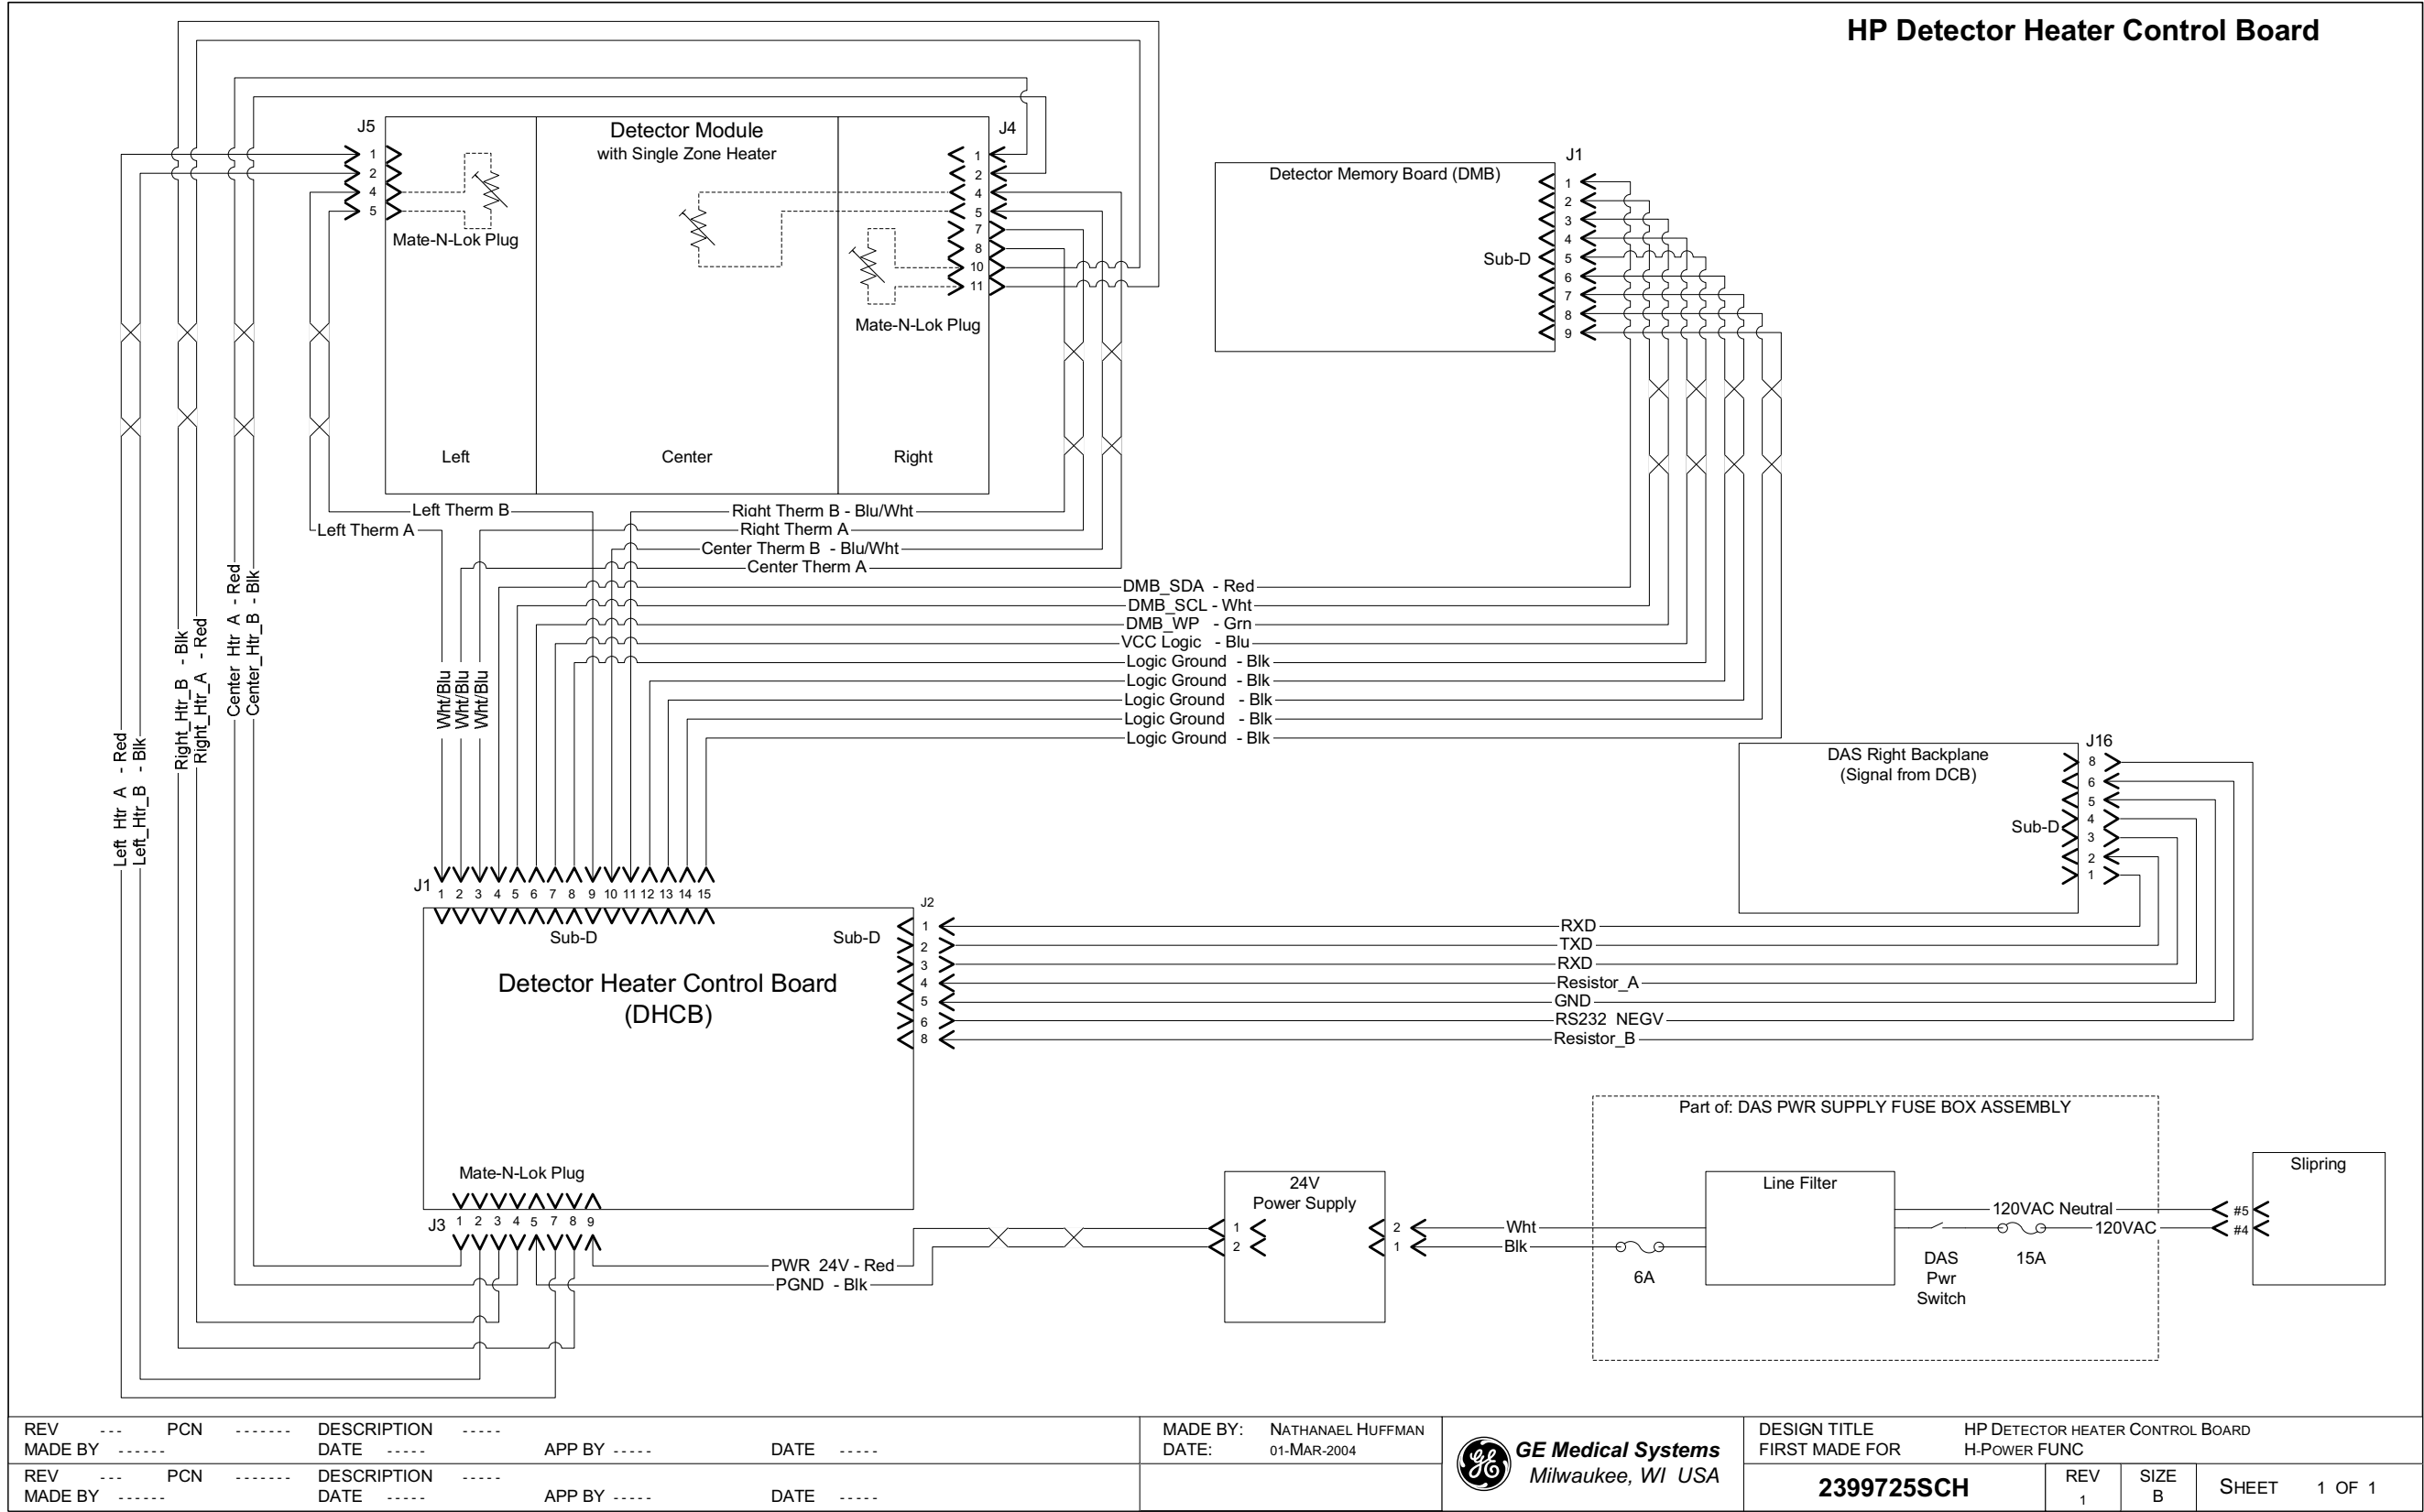


Figure 3-2 2399725 Sheet 1, Rev. 1

THIS PAGE INTENTIONALLY BLANK.

Chapter 4

Patient Positioning

HP_Alignment_Lights
RT_Alignment_Lights

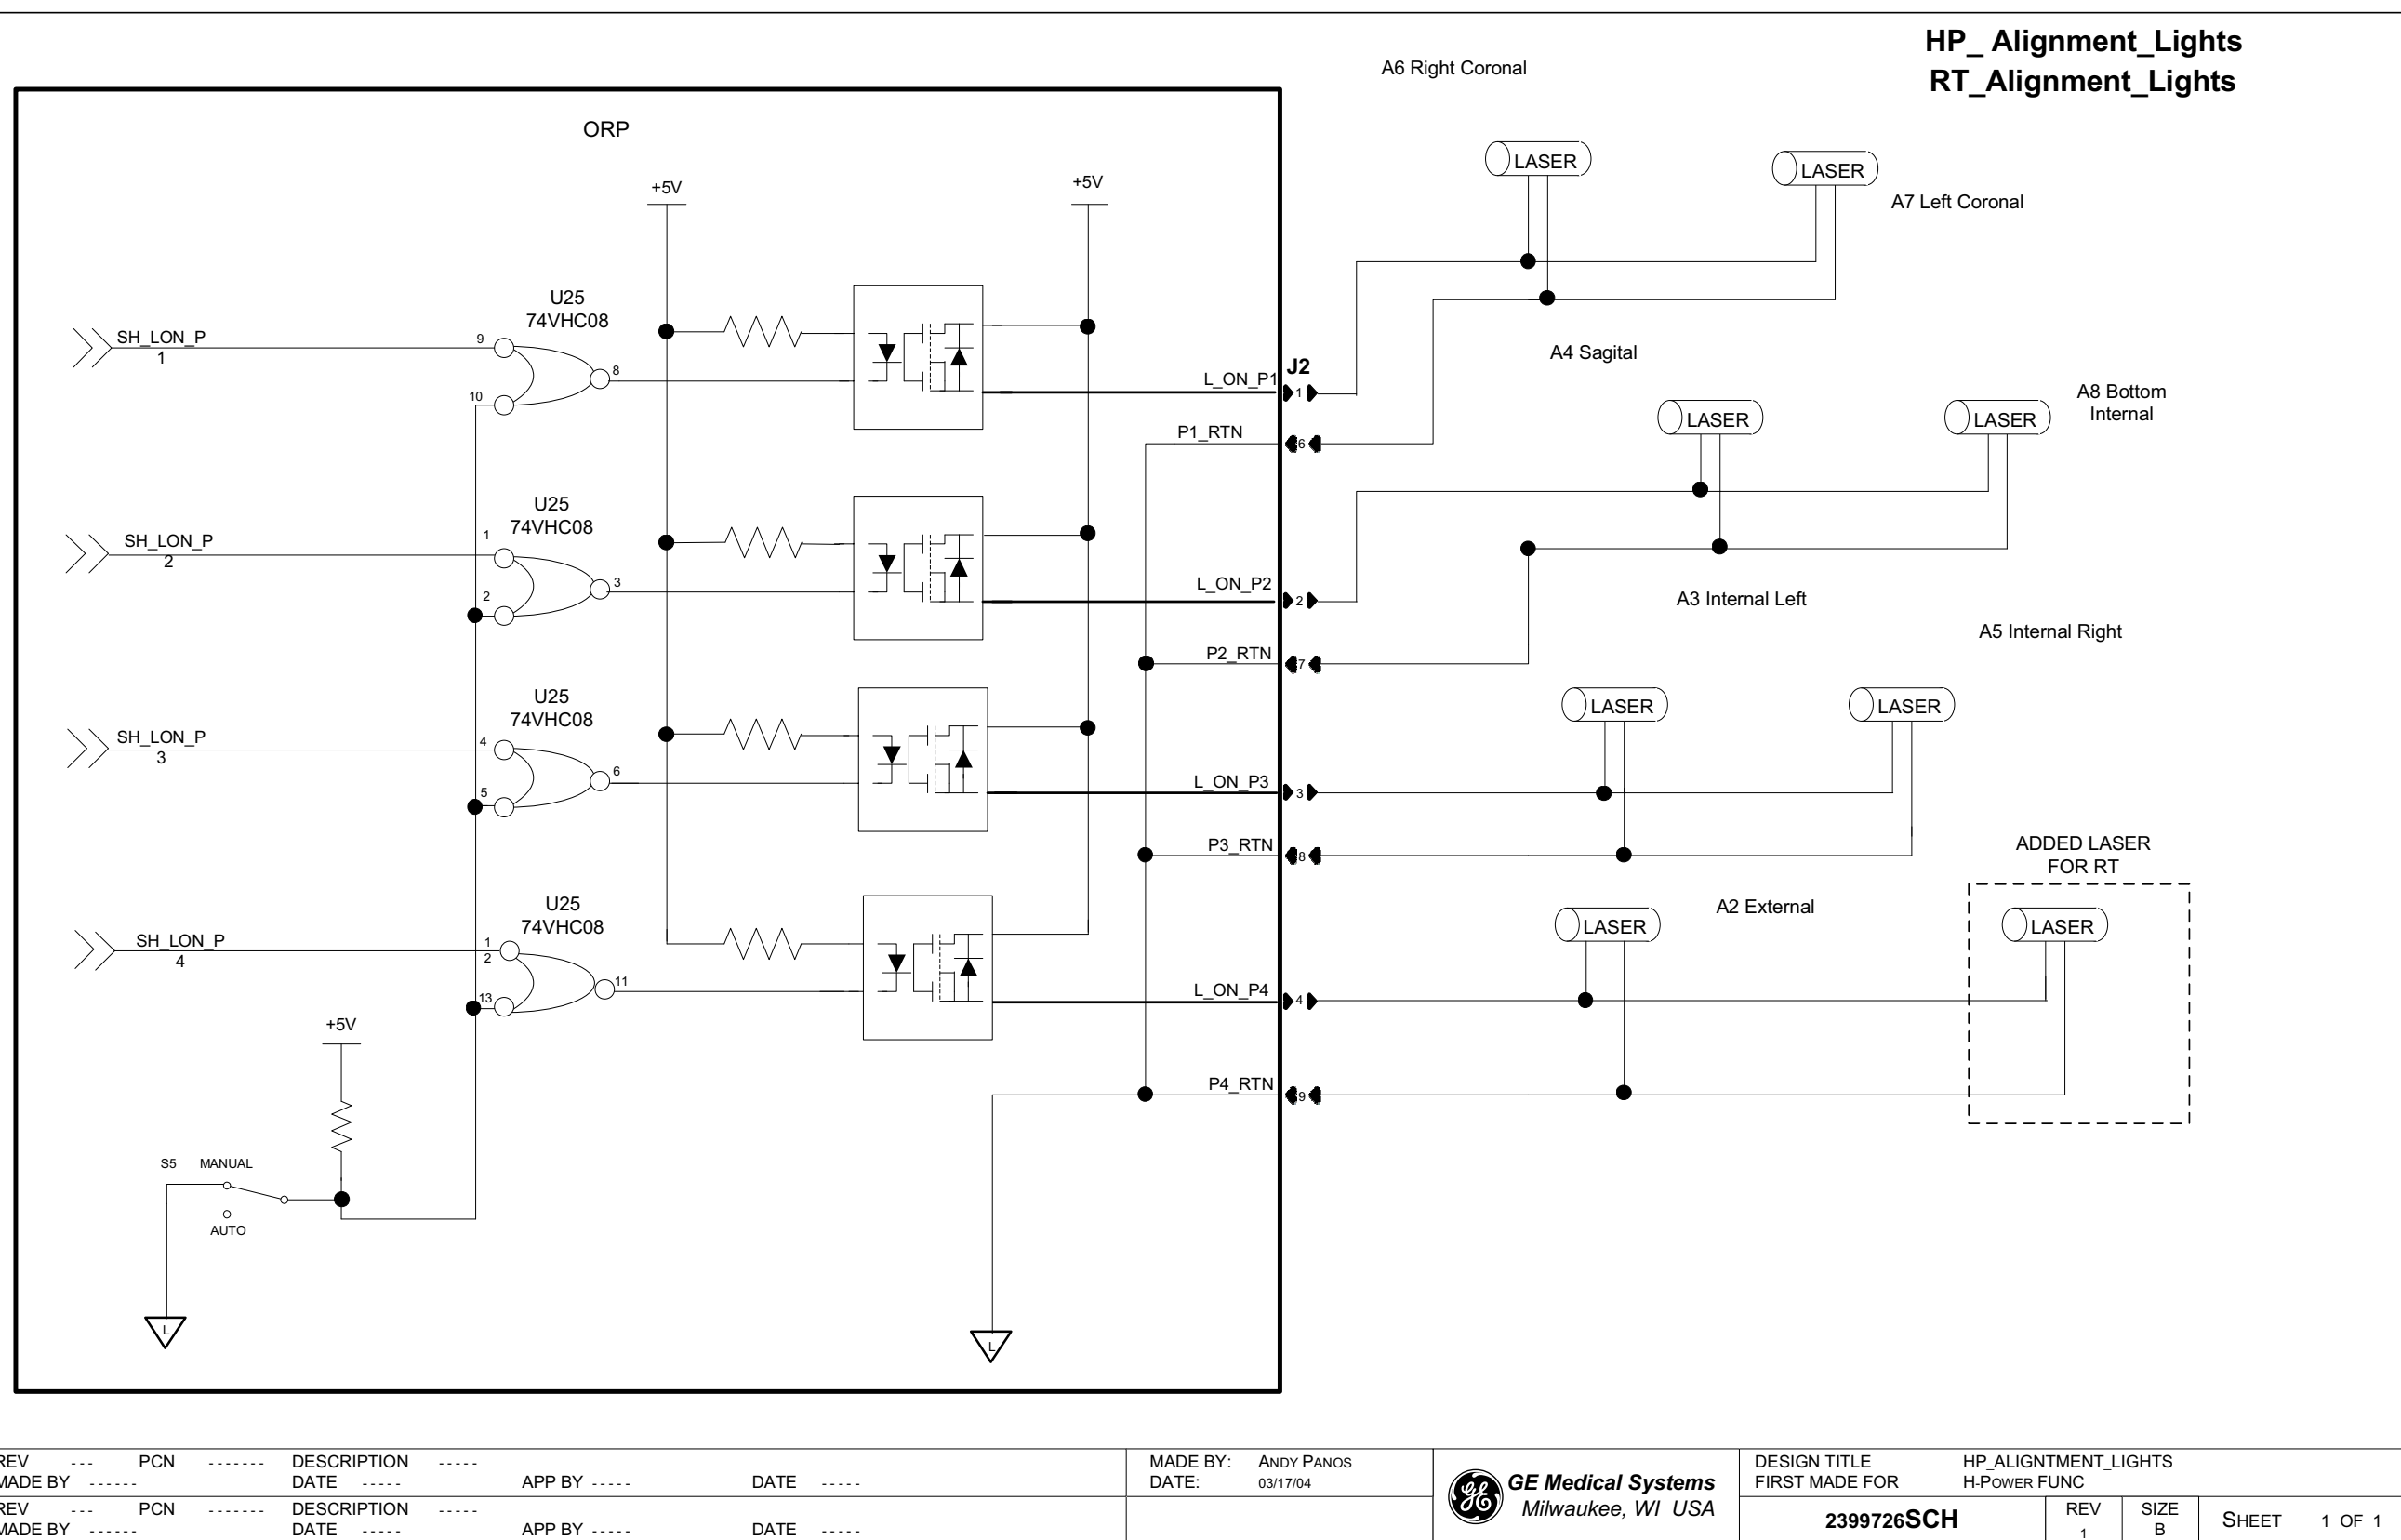


Figure 4-1 2399726 Sheet 1, Rev 1

Section 2.0 — Gantry Tilt, from Gantry, Console - 2399727

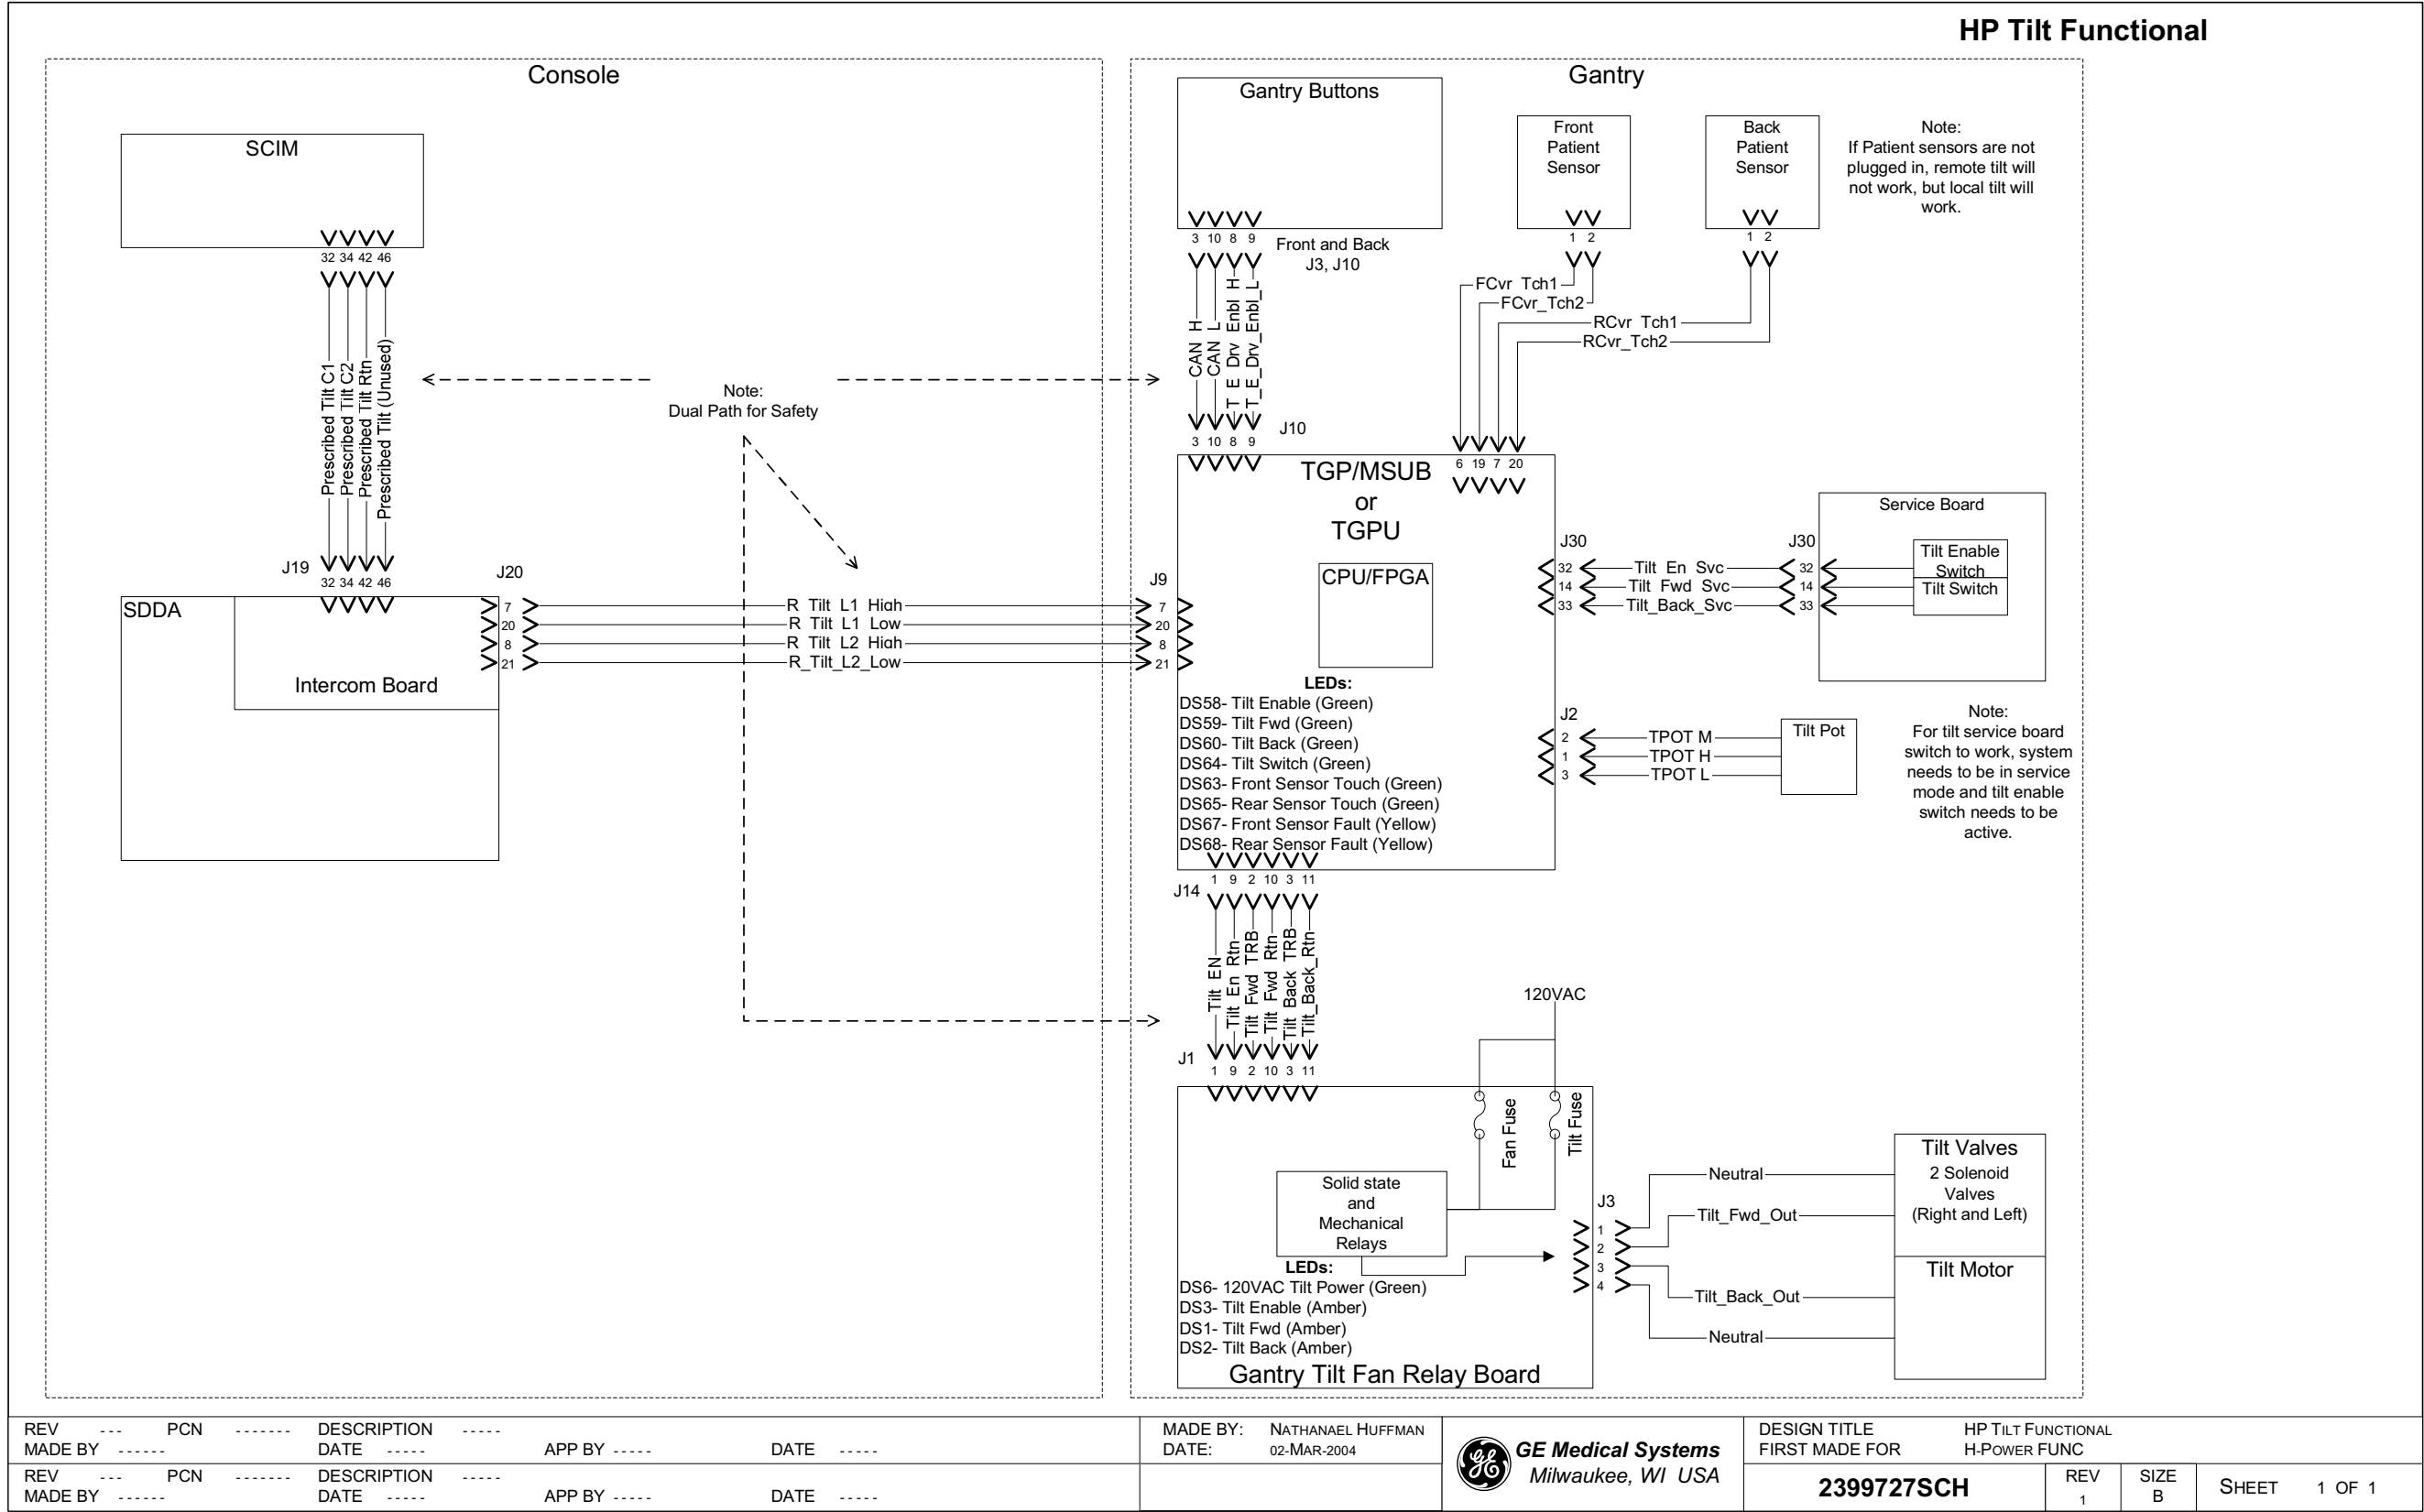


Figure 4-2 2399727 Sheet 1, Rev. 1

Chapter 5

Axial Control

HP AXIAL SERVO CONTROL + DYNAMIC BRAKE

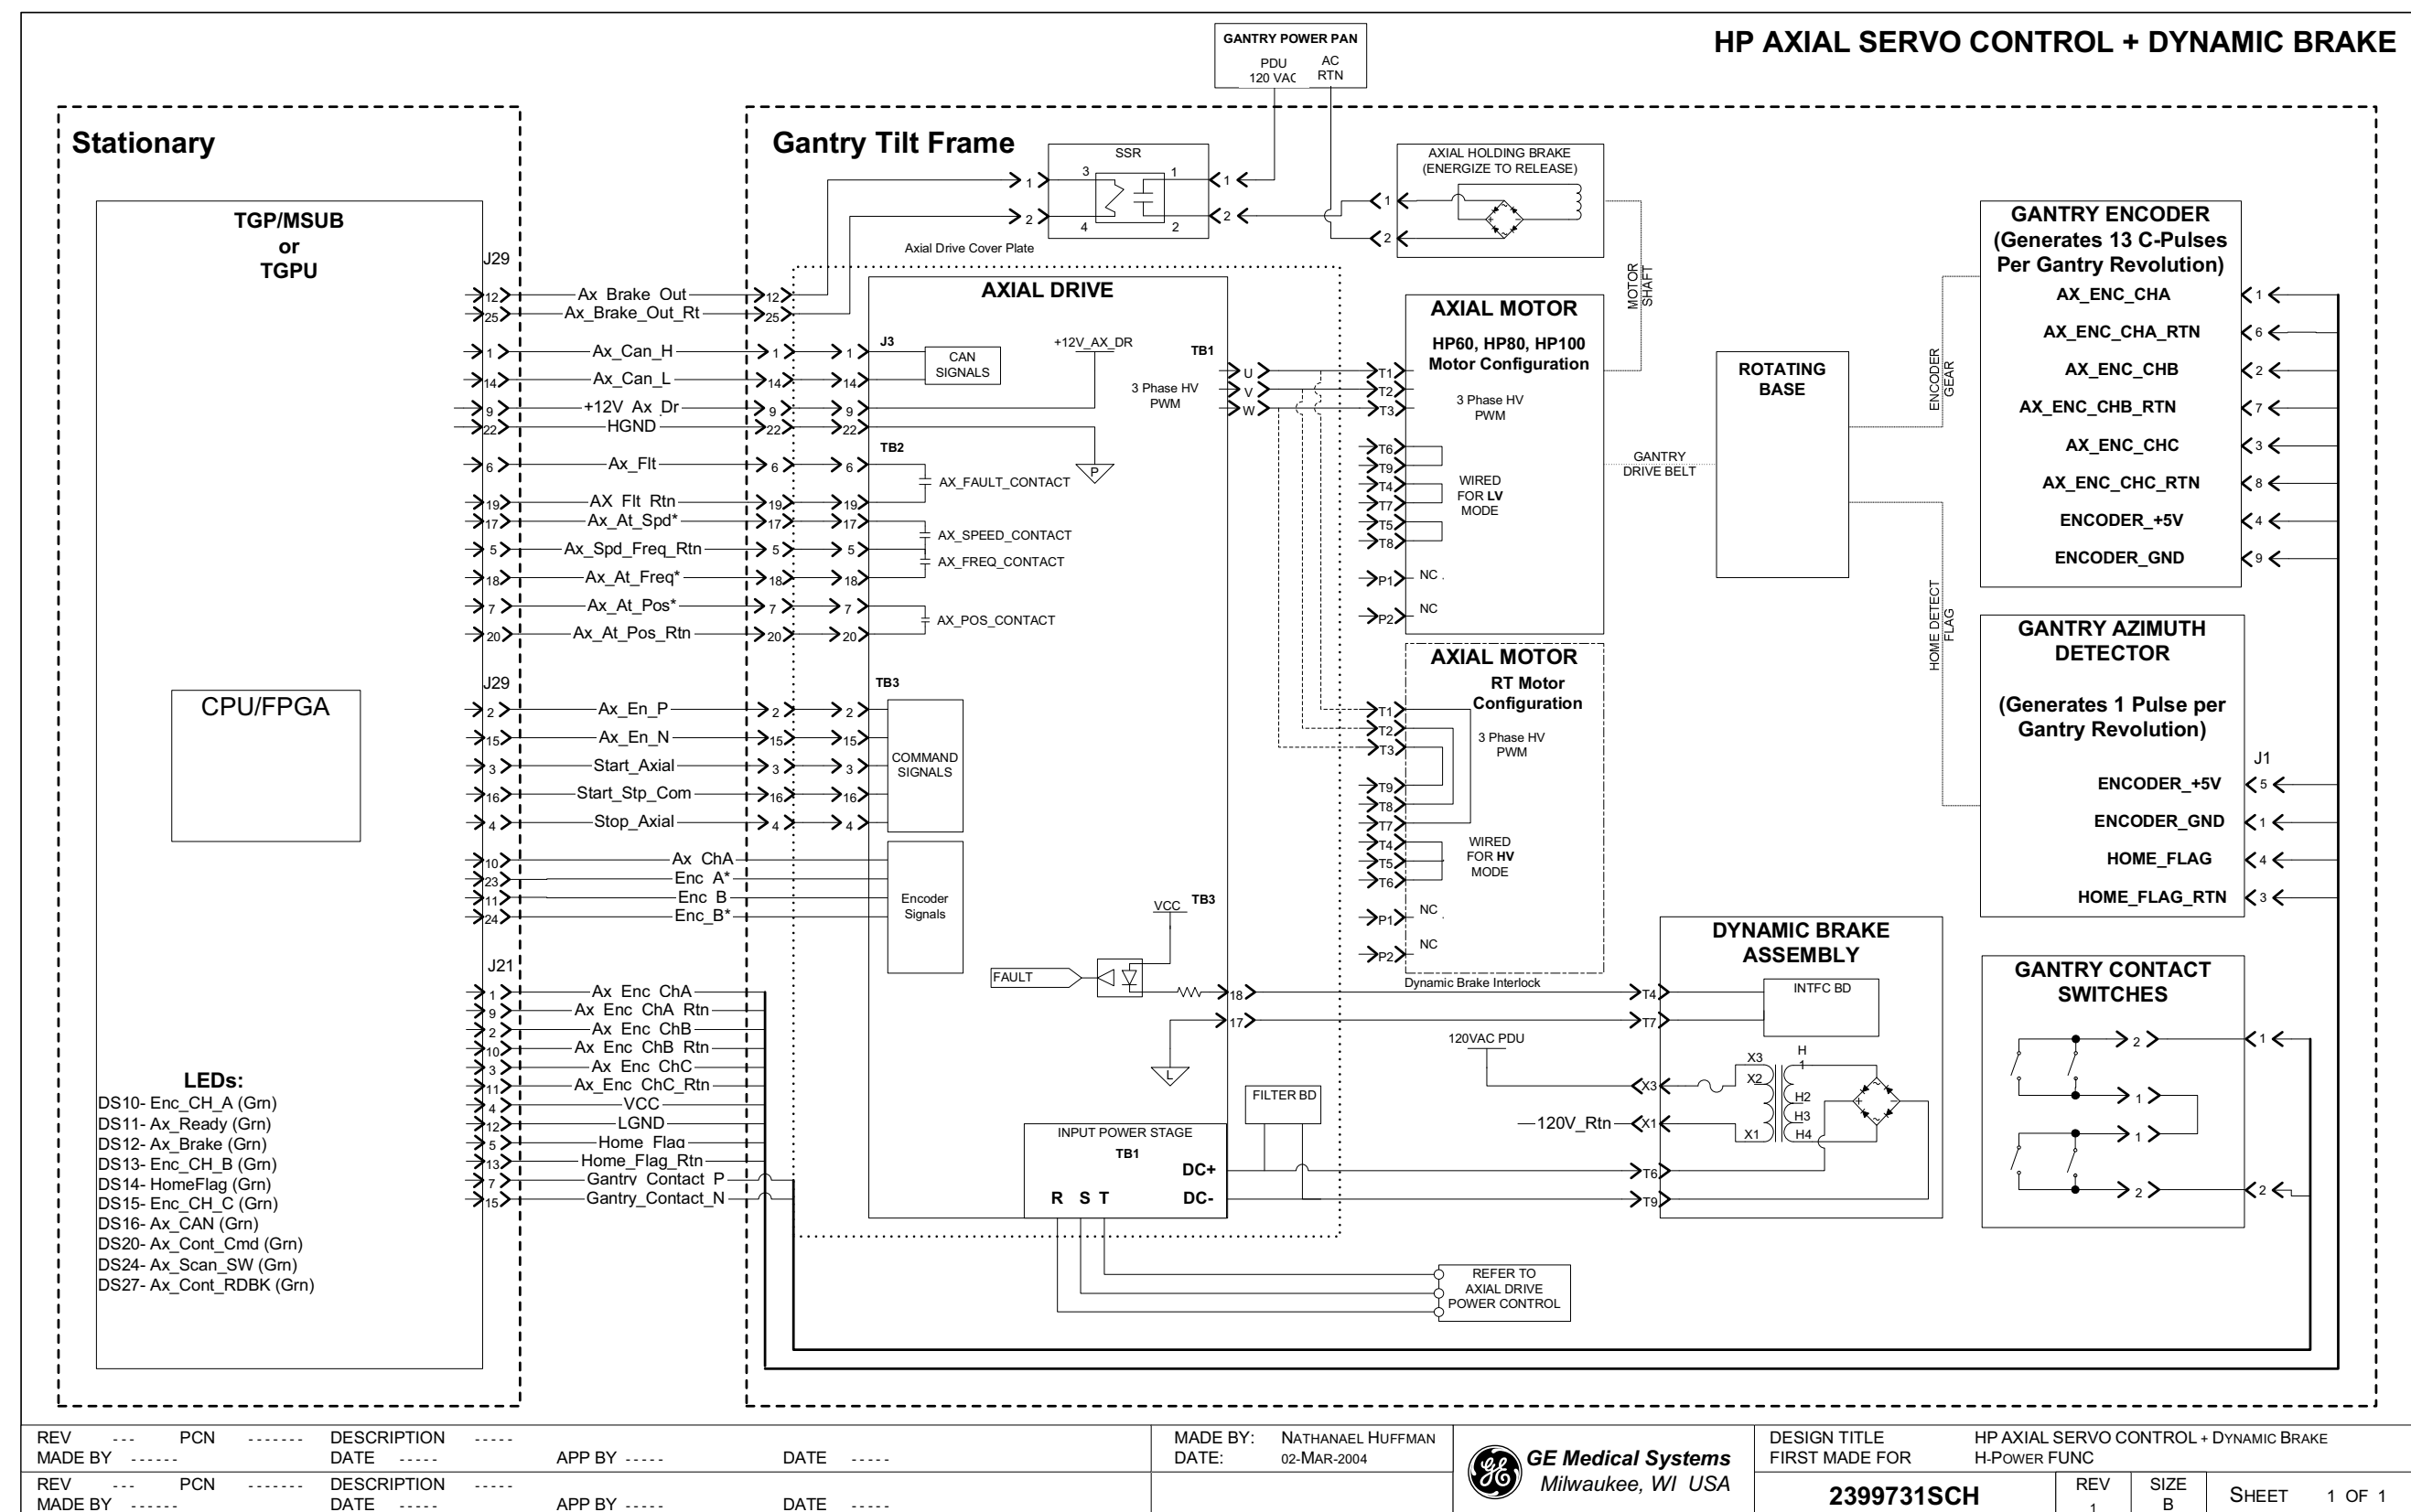


Figure 5-1 2399731 Sheet 1 Rev. 1

Section 2.0 — Axial Power Distribution - 2399732

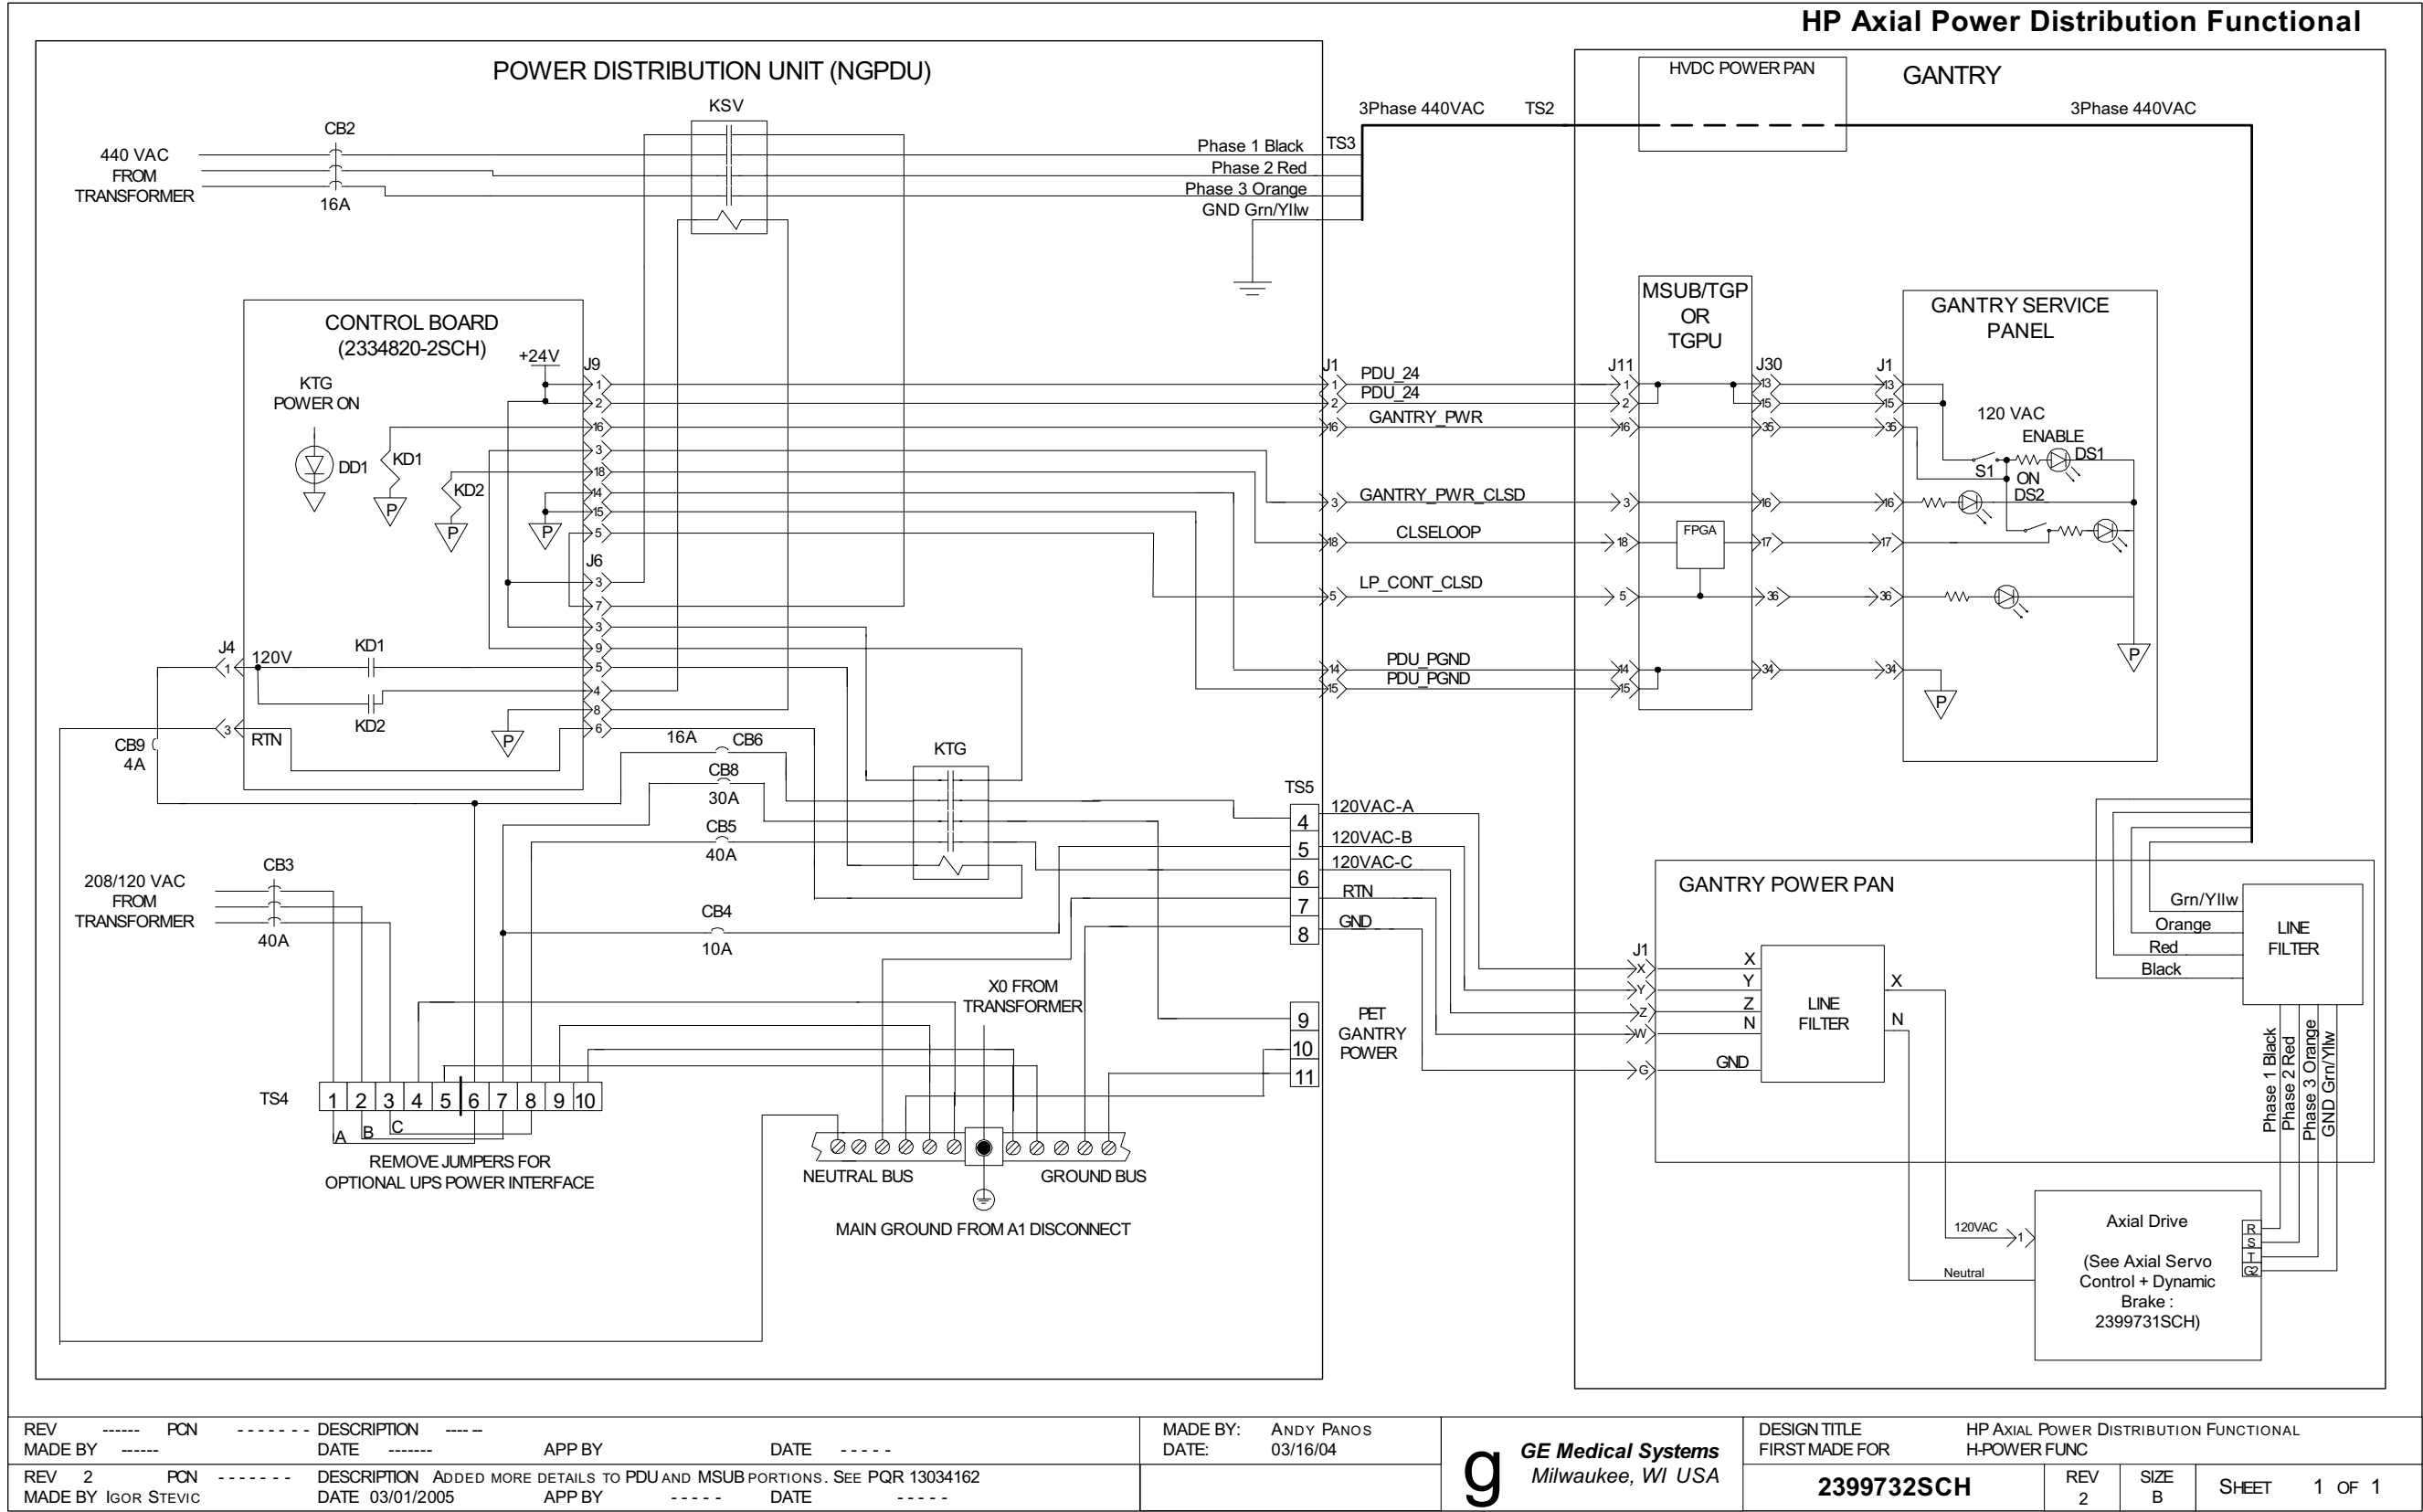


Figure 5-2 2399732 Sheet 1 Rev. 2

THIS PAGE INTENTIONALLY BLANK.

Chapter 6

Operator I/O

Section 1.0 — Gantry Operator Interface and Displays - 2399733

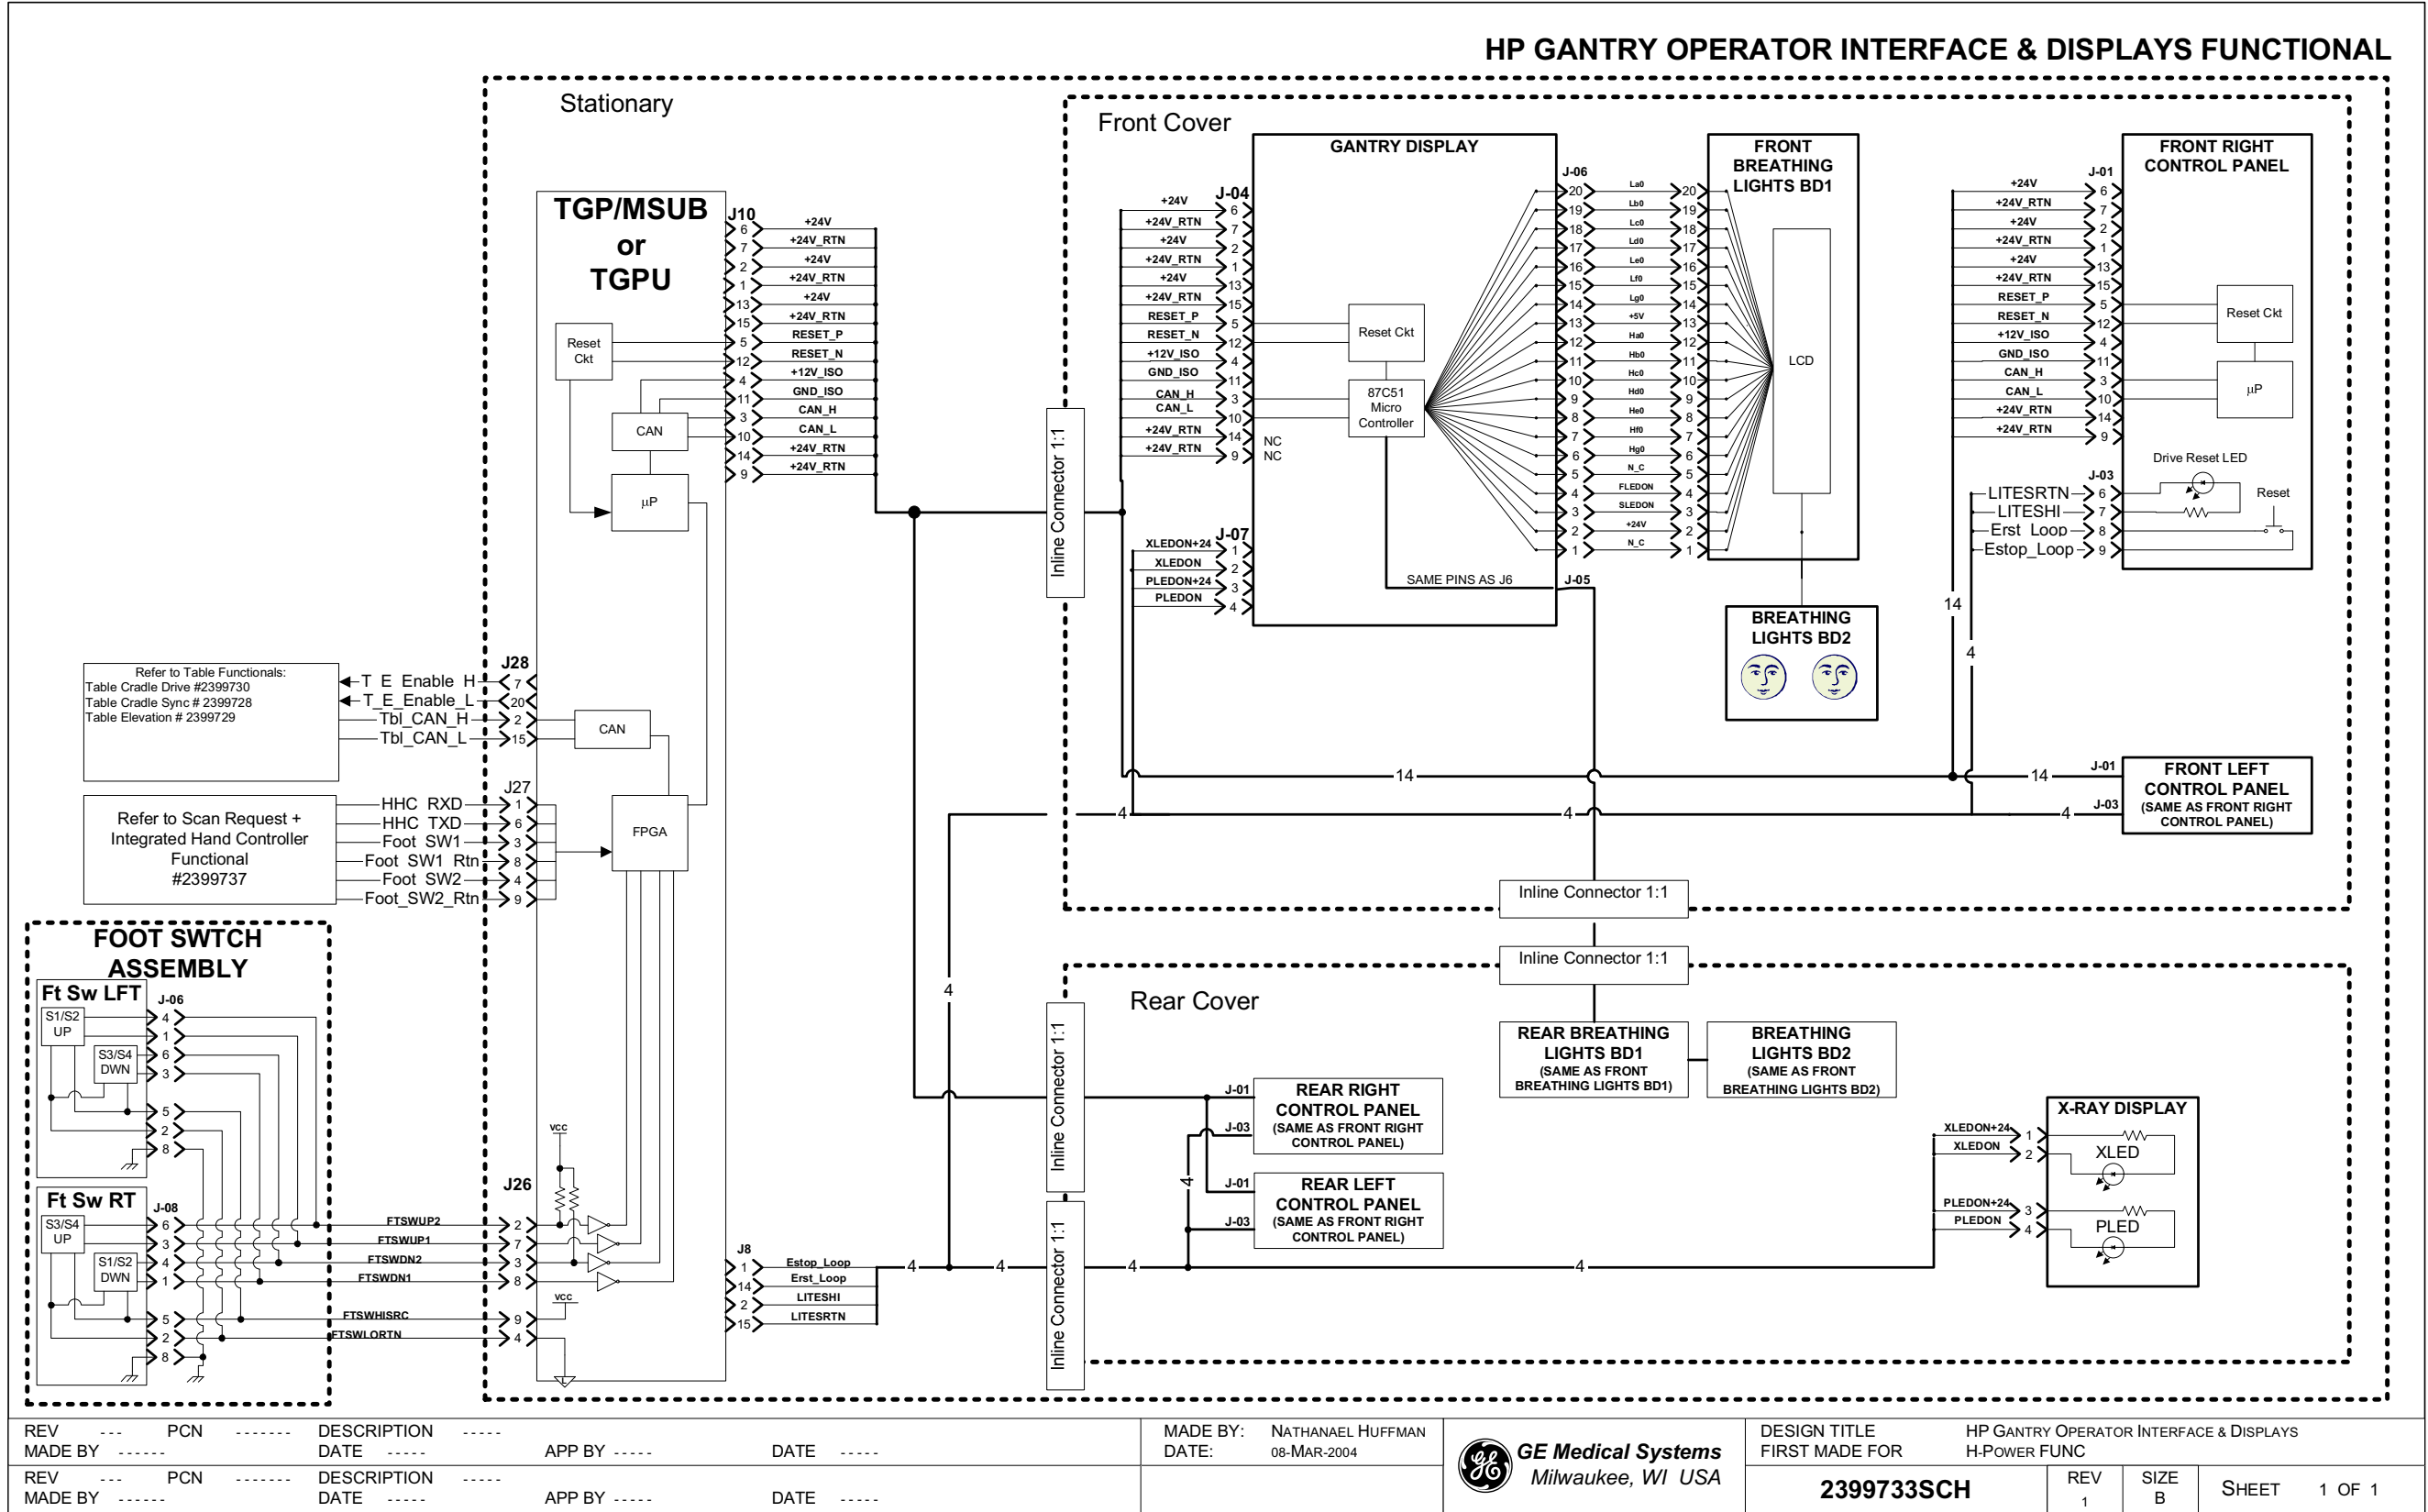


Figure 6-1 2399733 Sheet 1, Rev. 1

Section 2.0 — Gantry Reset from Console


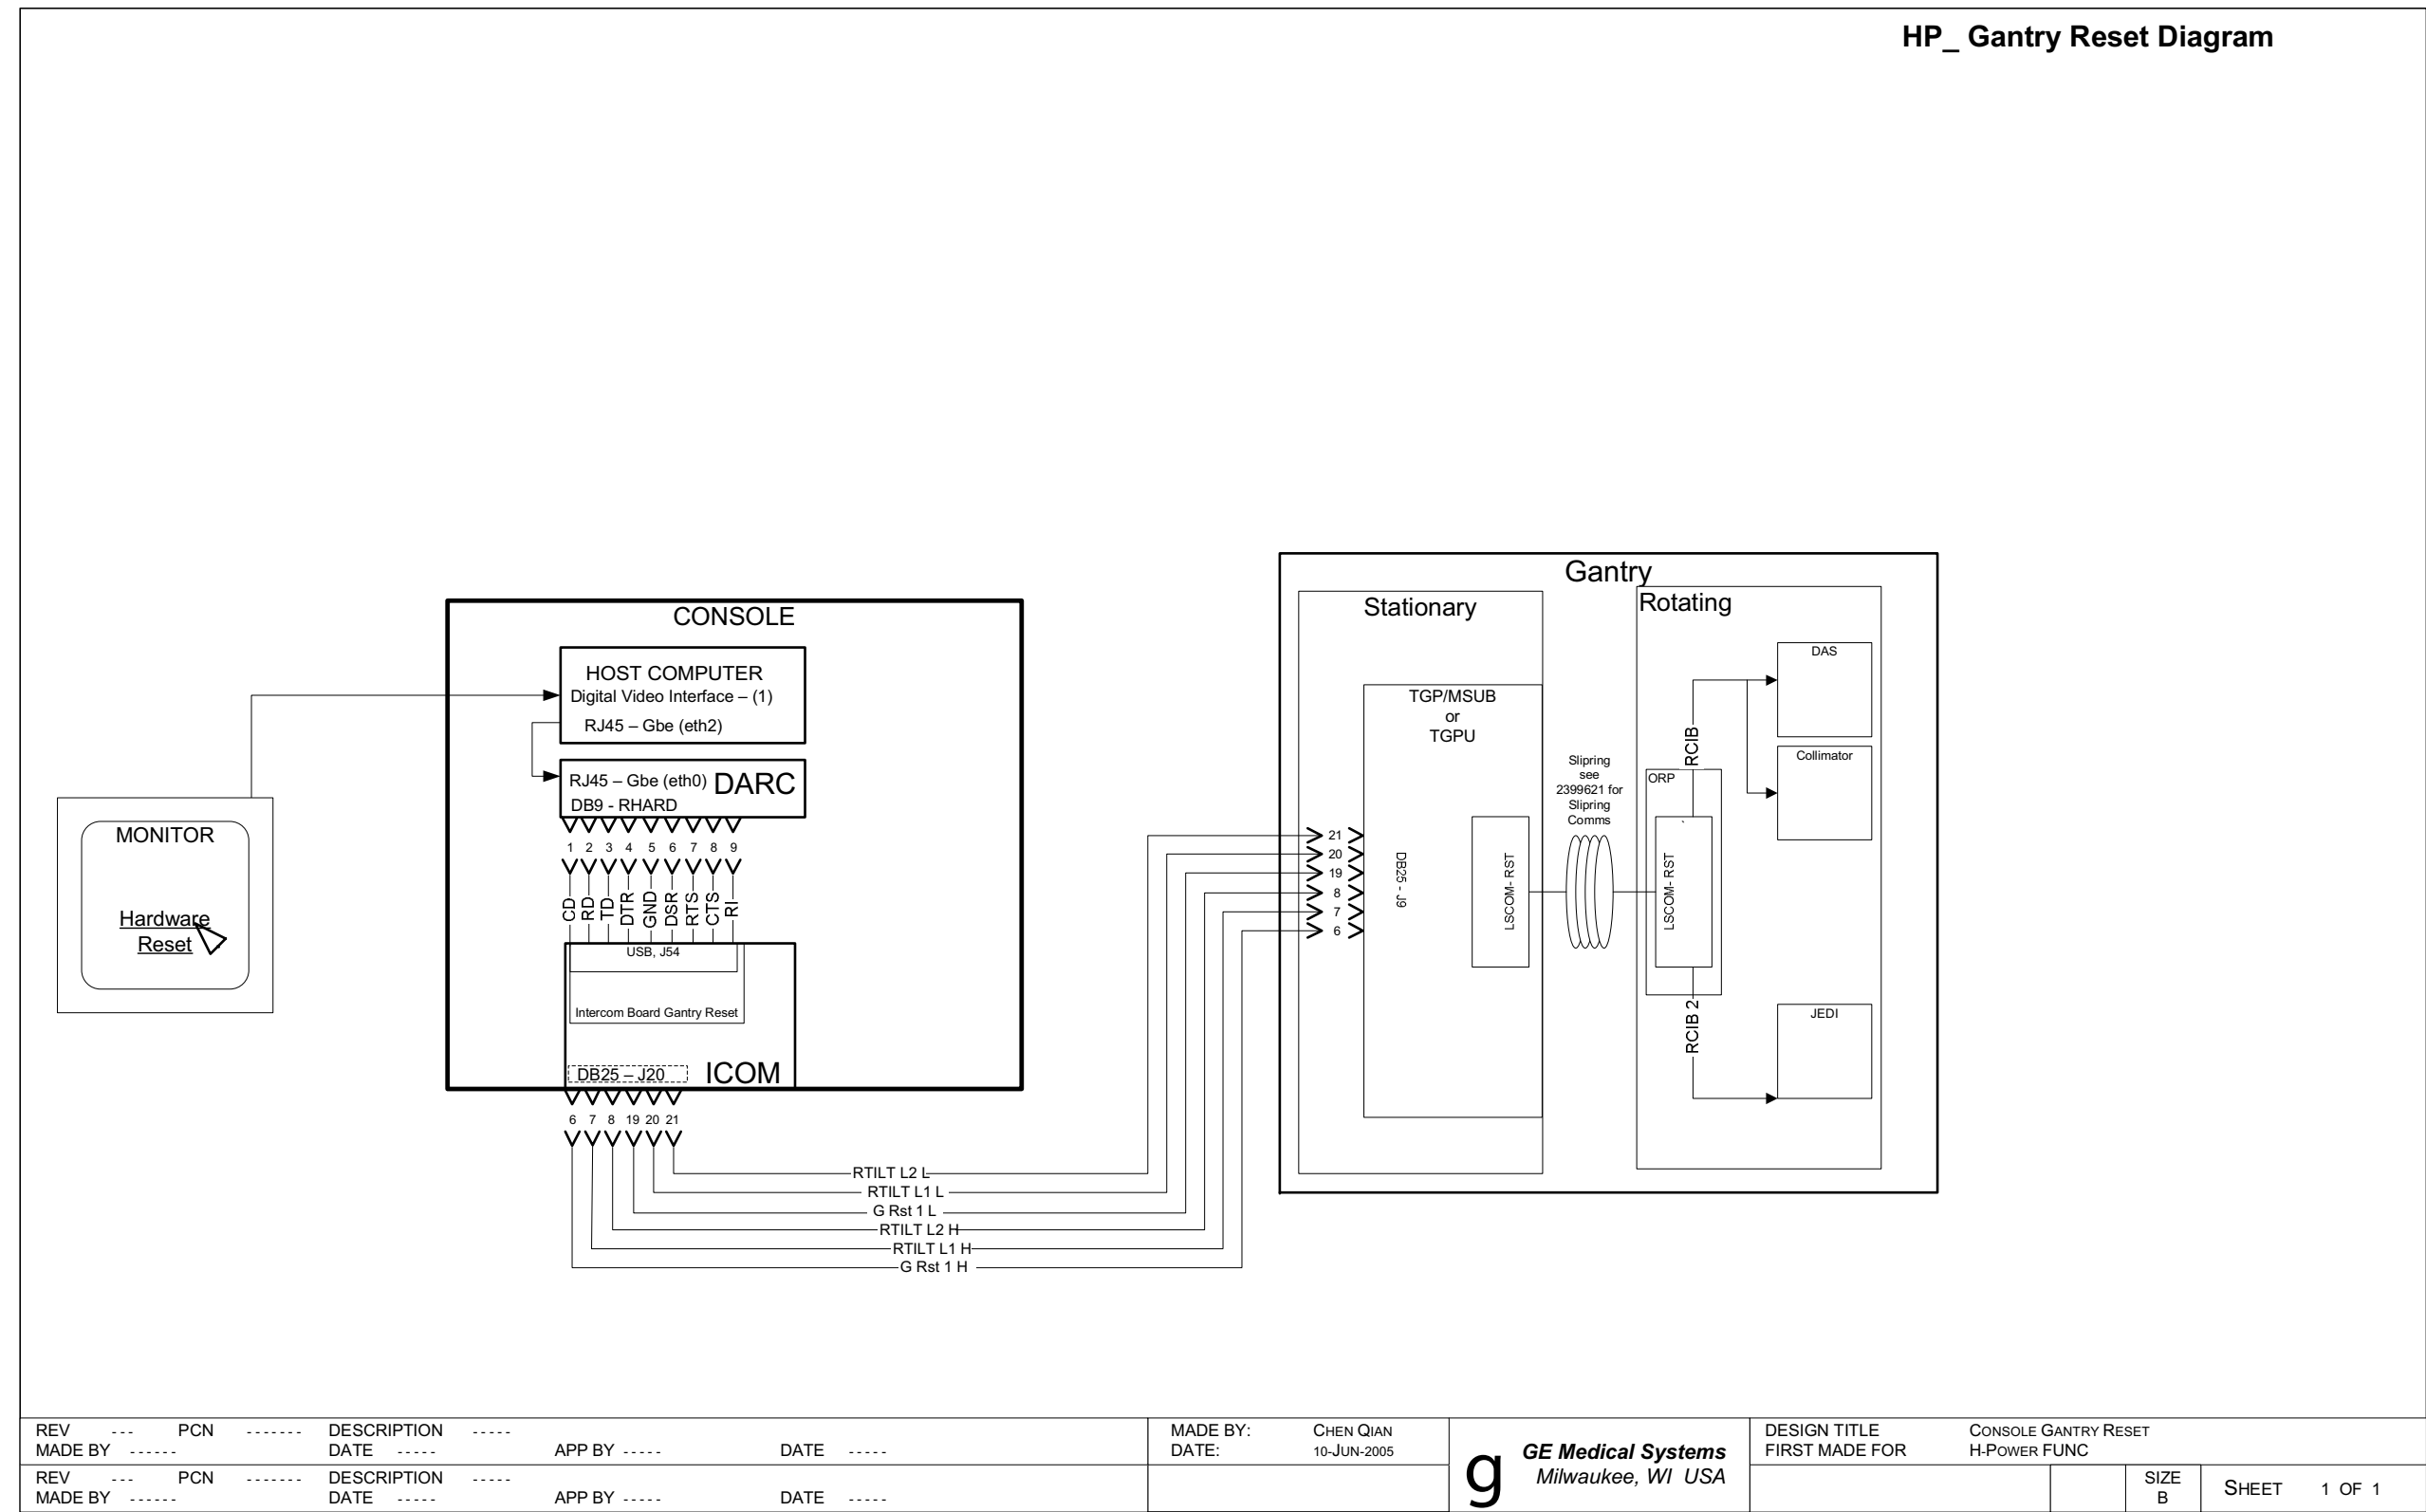


Figure 6-2 2399734 Sheet 1, Rev. 1

Section 3.0 — Gantry Reset from Console (All-In-One)

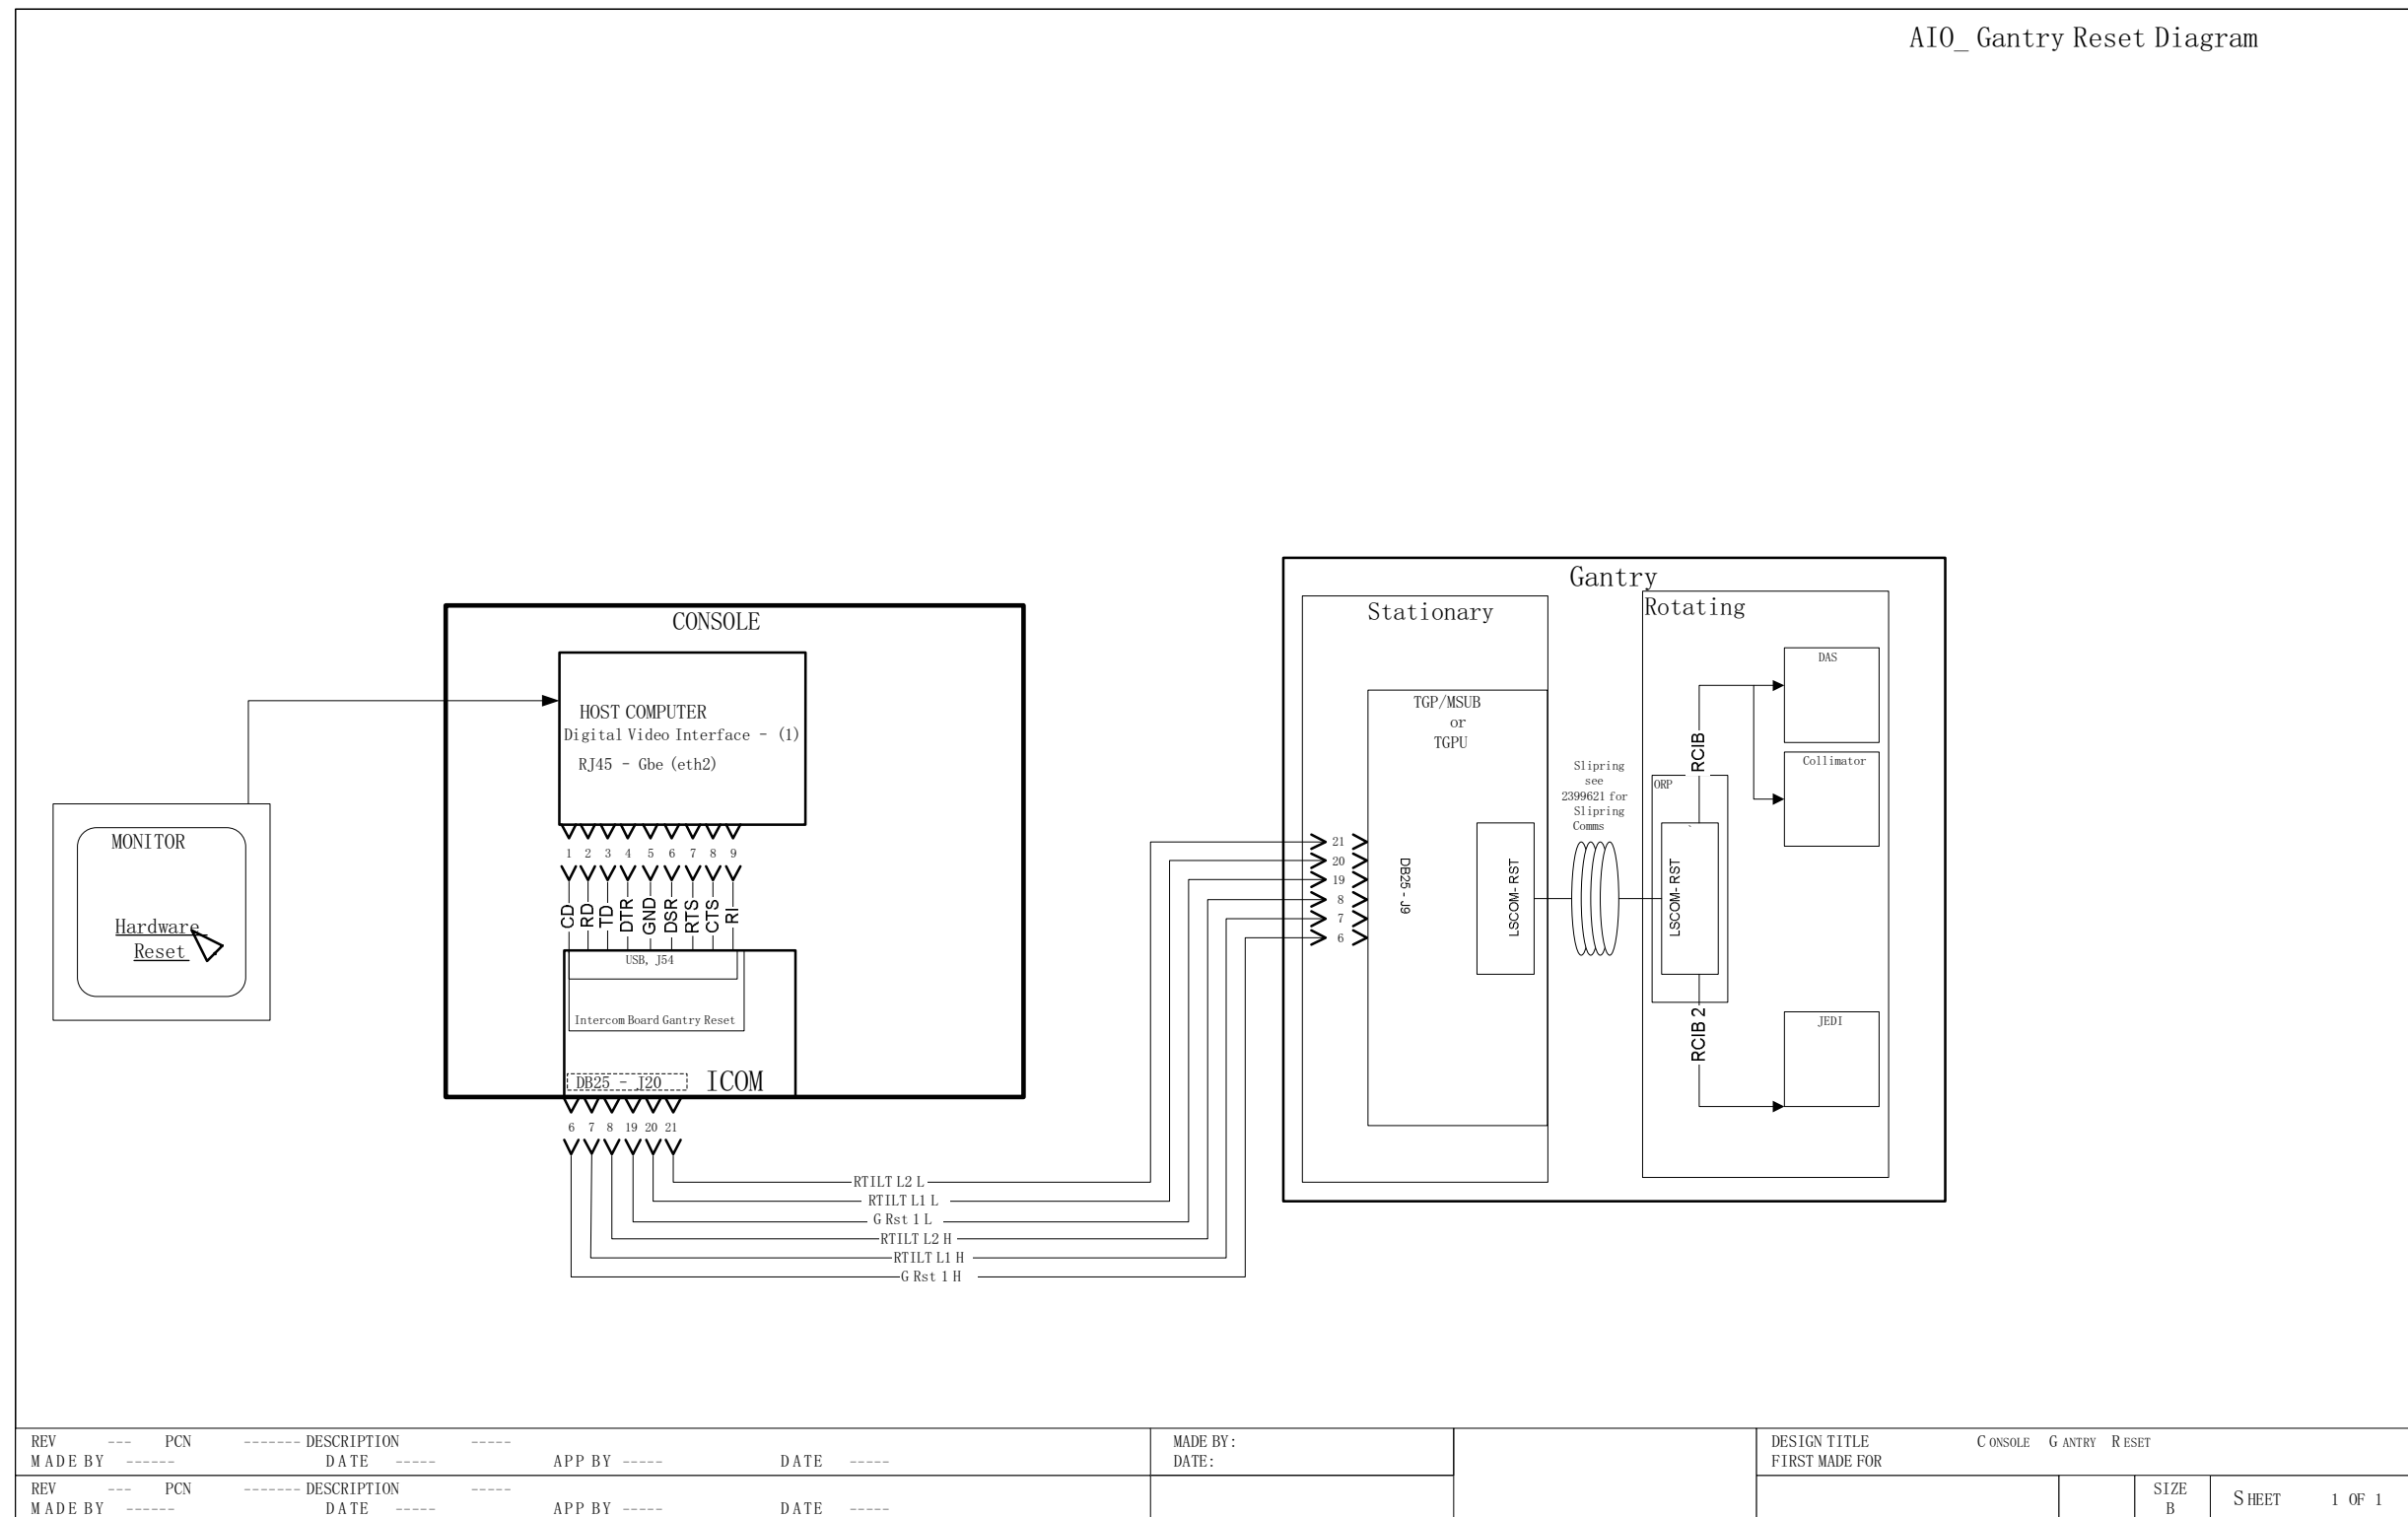

Section 4.0 — Cardiac Options - 2399735


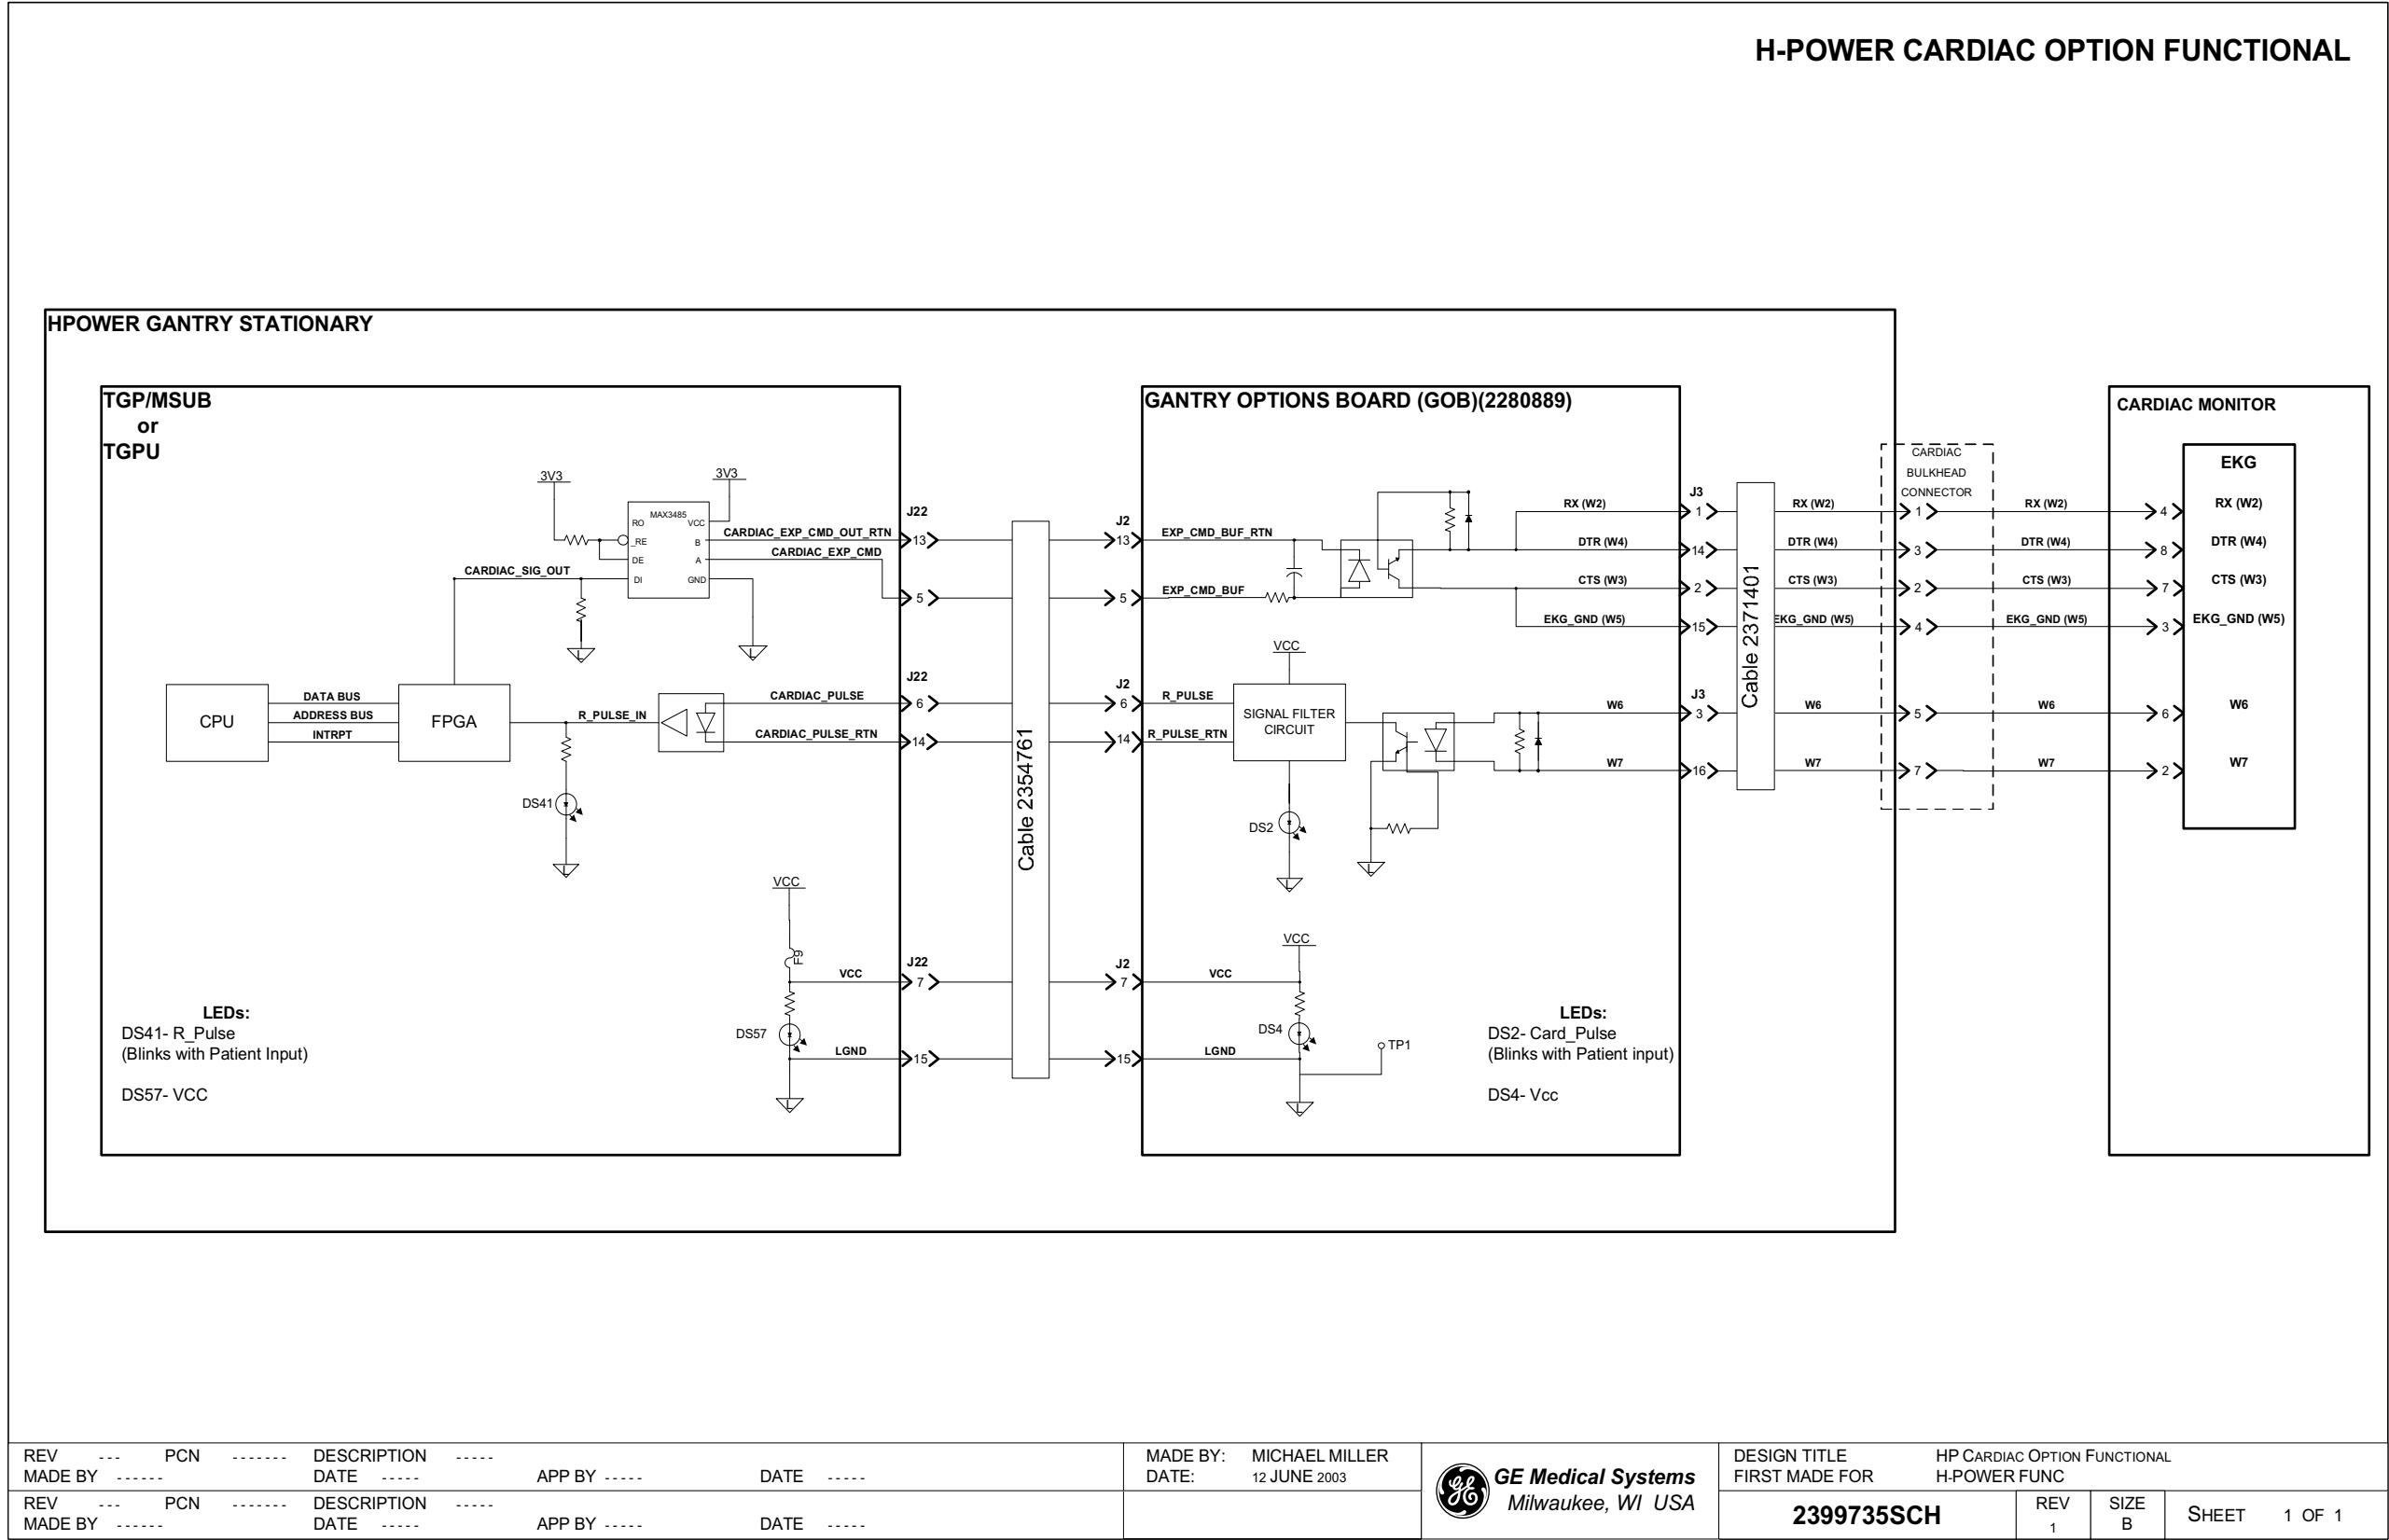


Figure 6-3 2399735 Sheet 1, Rev. 1

H-POWER PULMONARY OPTION FUNCTIONAL

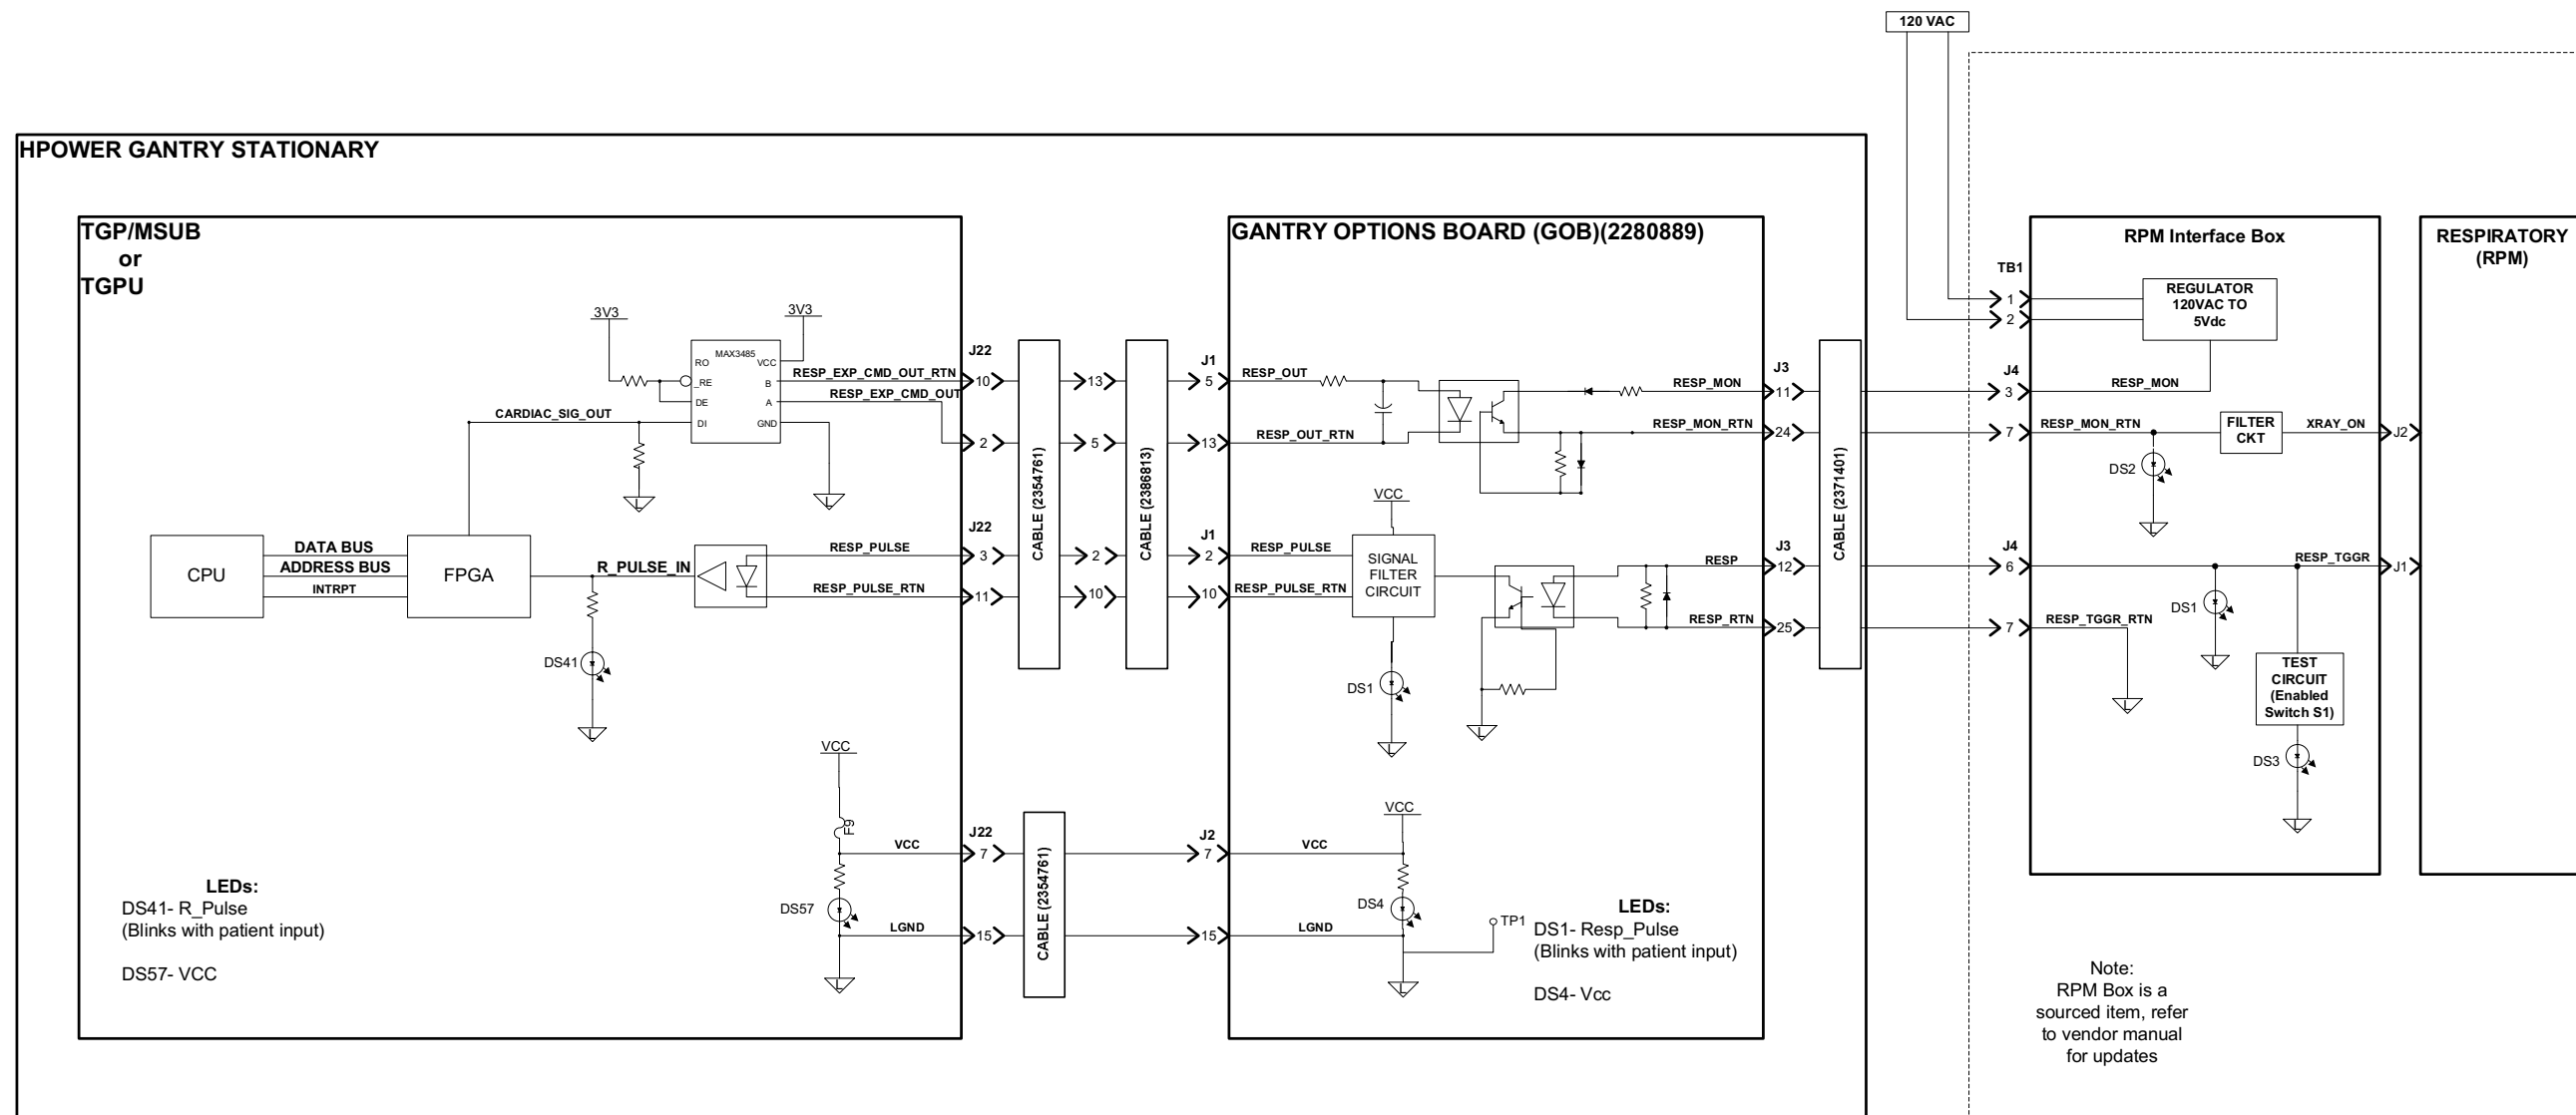

REV --- PCN -----	DESCRIPTION -----	MADE BY: MICHAEL MILLER	 GE Medical Systems Milwaukee, WI USA				DESIGN TITLE		HP PULMONARY OPTION FUNCTIONAL		
MADE BY -----	DATE -----	DATE: 12 JUNE 2003					FIRST MADE FOR		H-POWER FUNC		
REV --- PCN -----	DESCRIPTION -----						2399736SCH		REV 1	SIZE B	SHEET 1 OF 1

Figure 6-4 2399736 Sheet 1, Rev. 1

Section 6.0 — Site X-Ray Light, System Light - 2399738


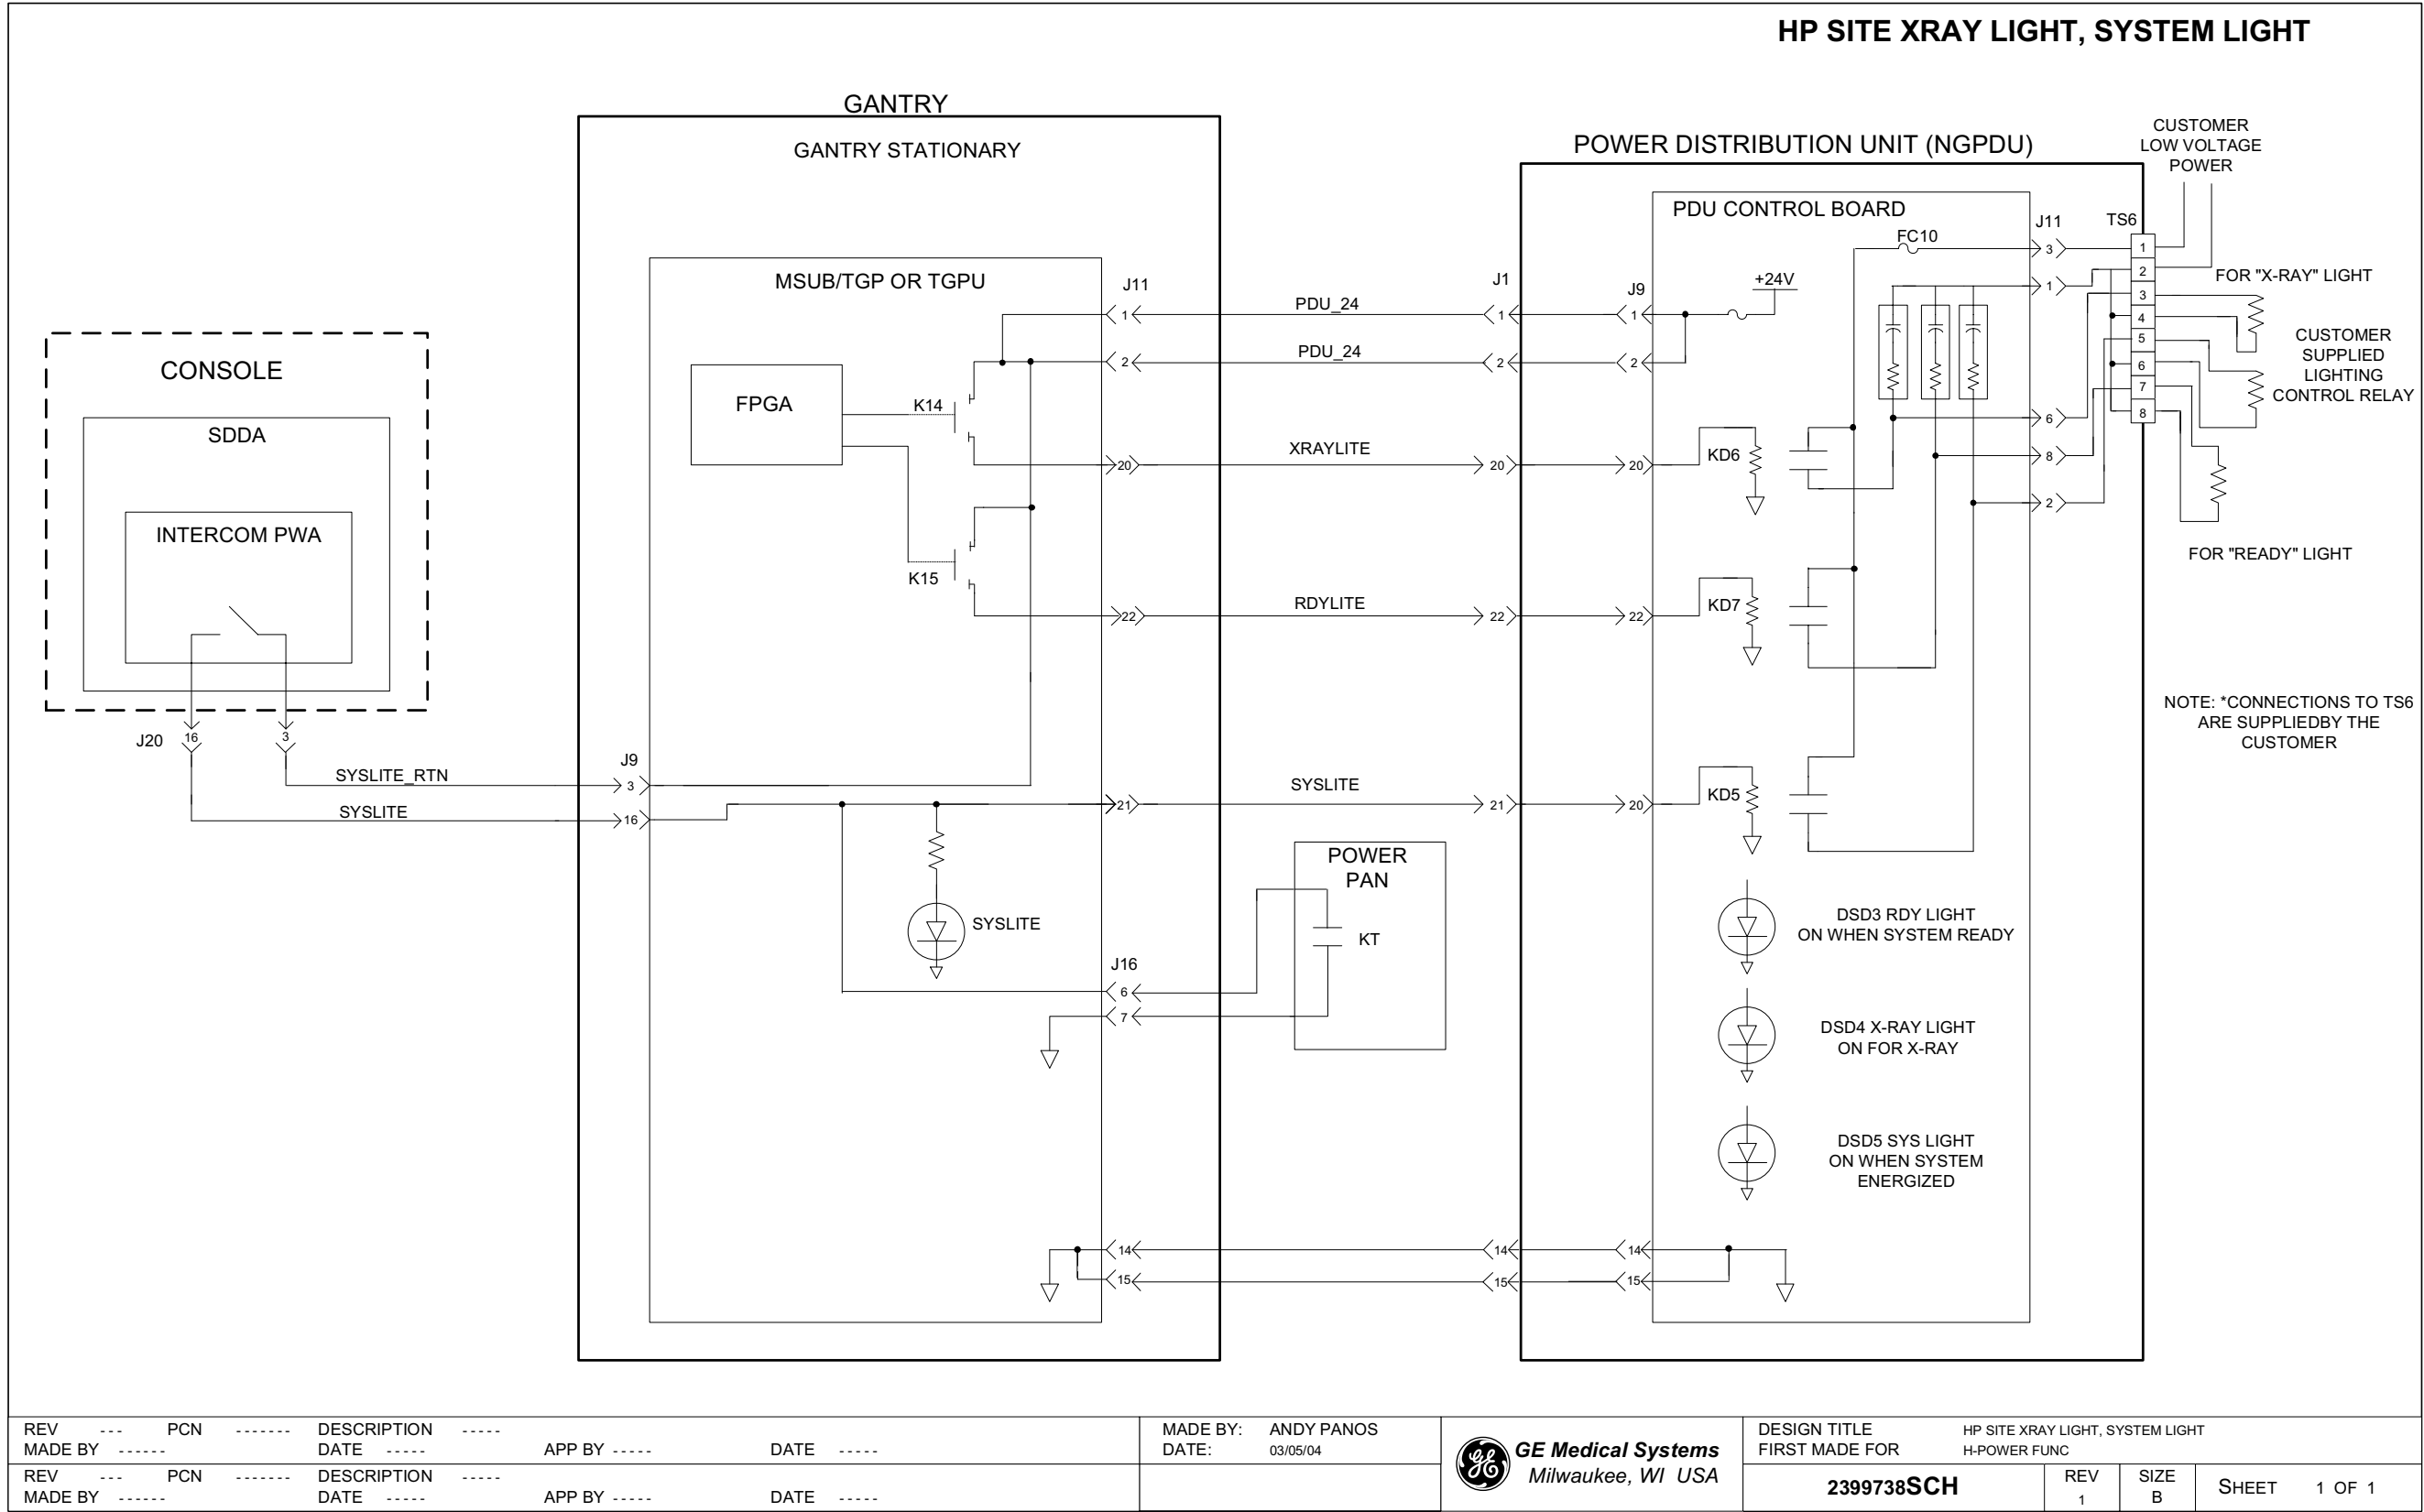


Figure 6-5 2399738 Sheet 1, Rev. 1

Section 7.0 — Autovoice / Intercom - 2399739

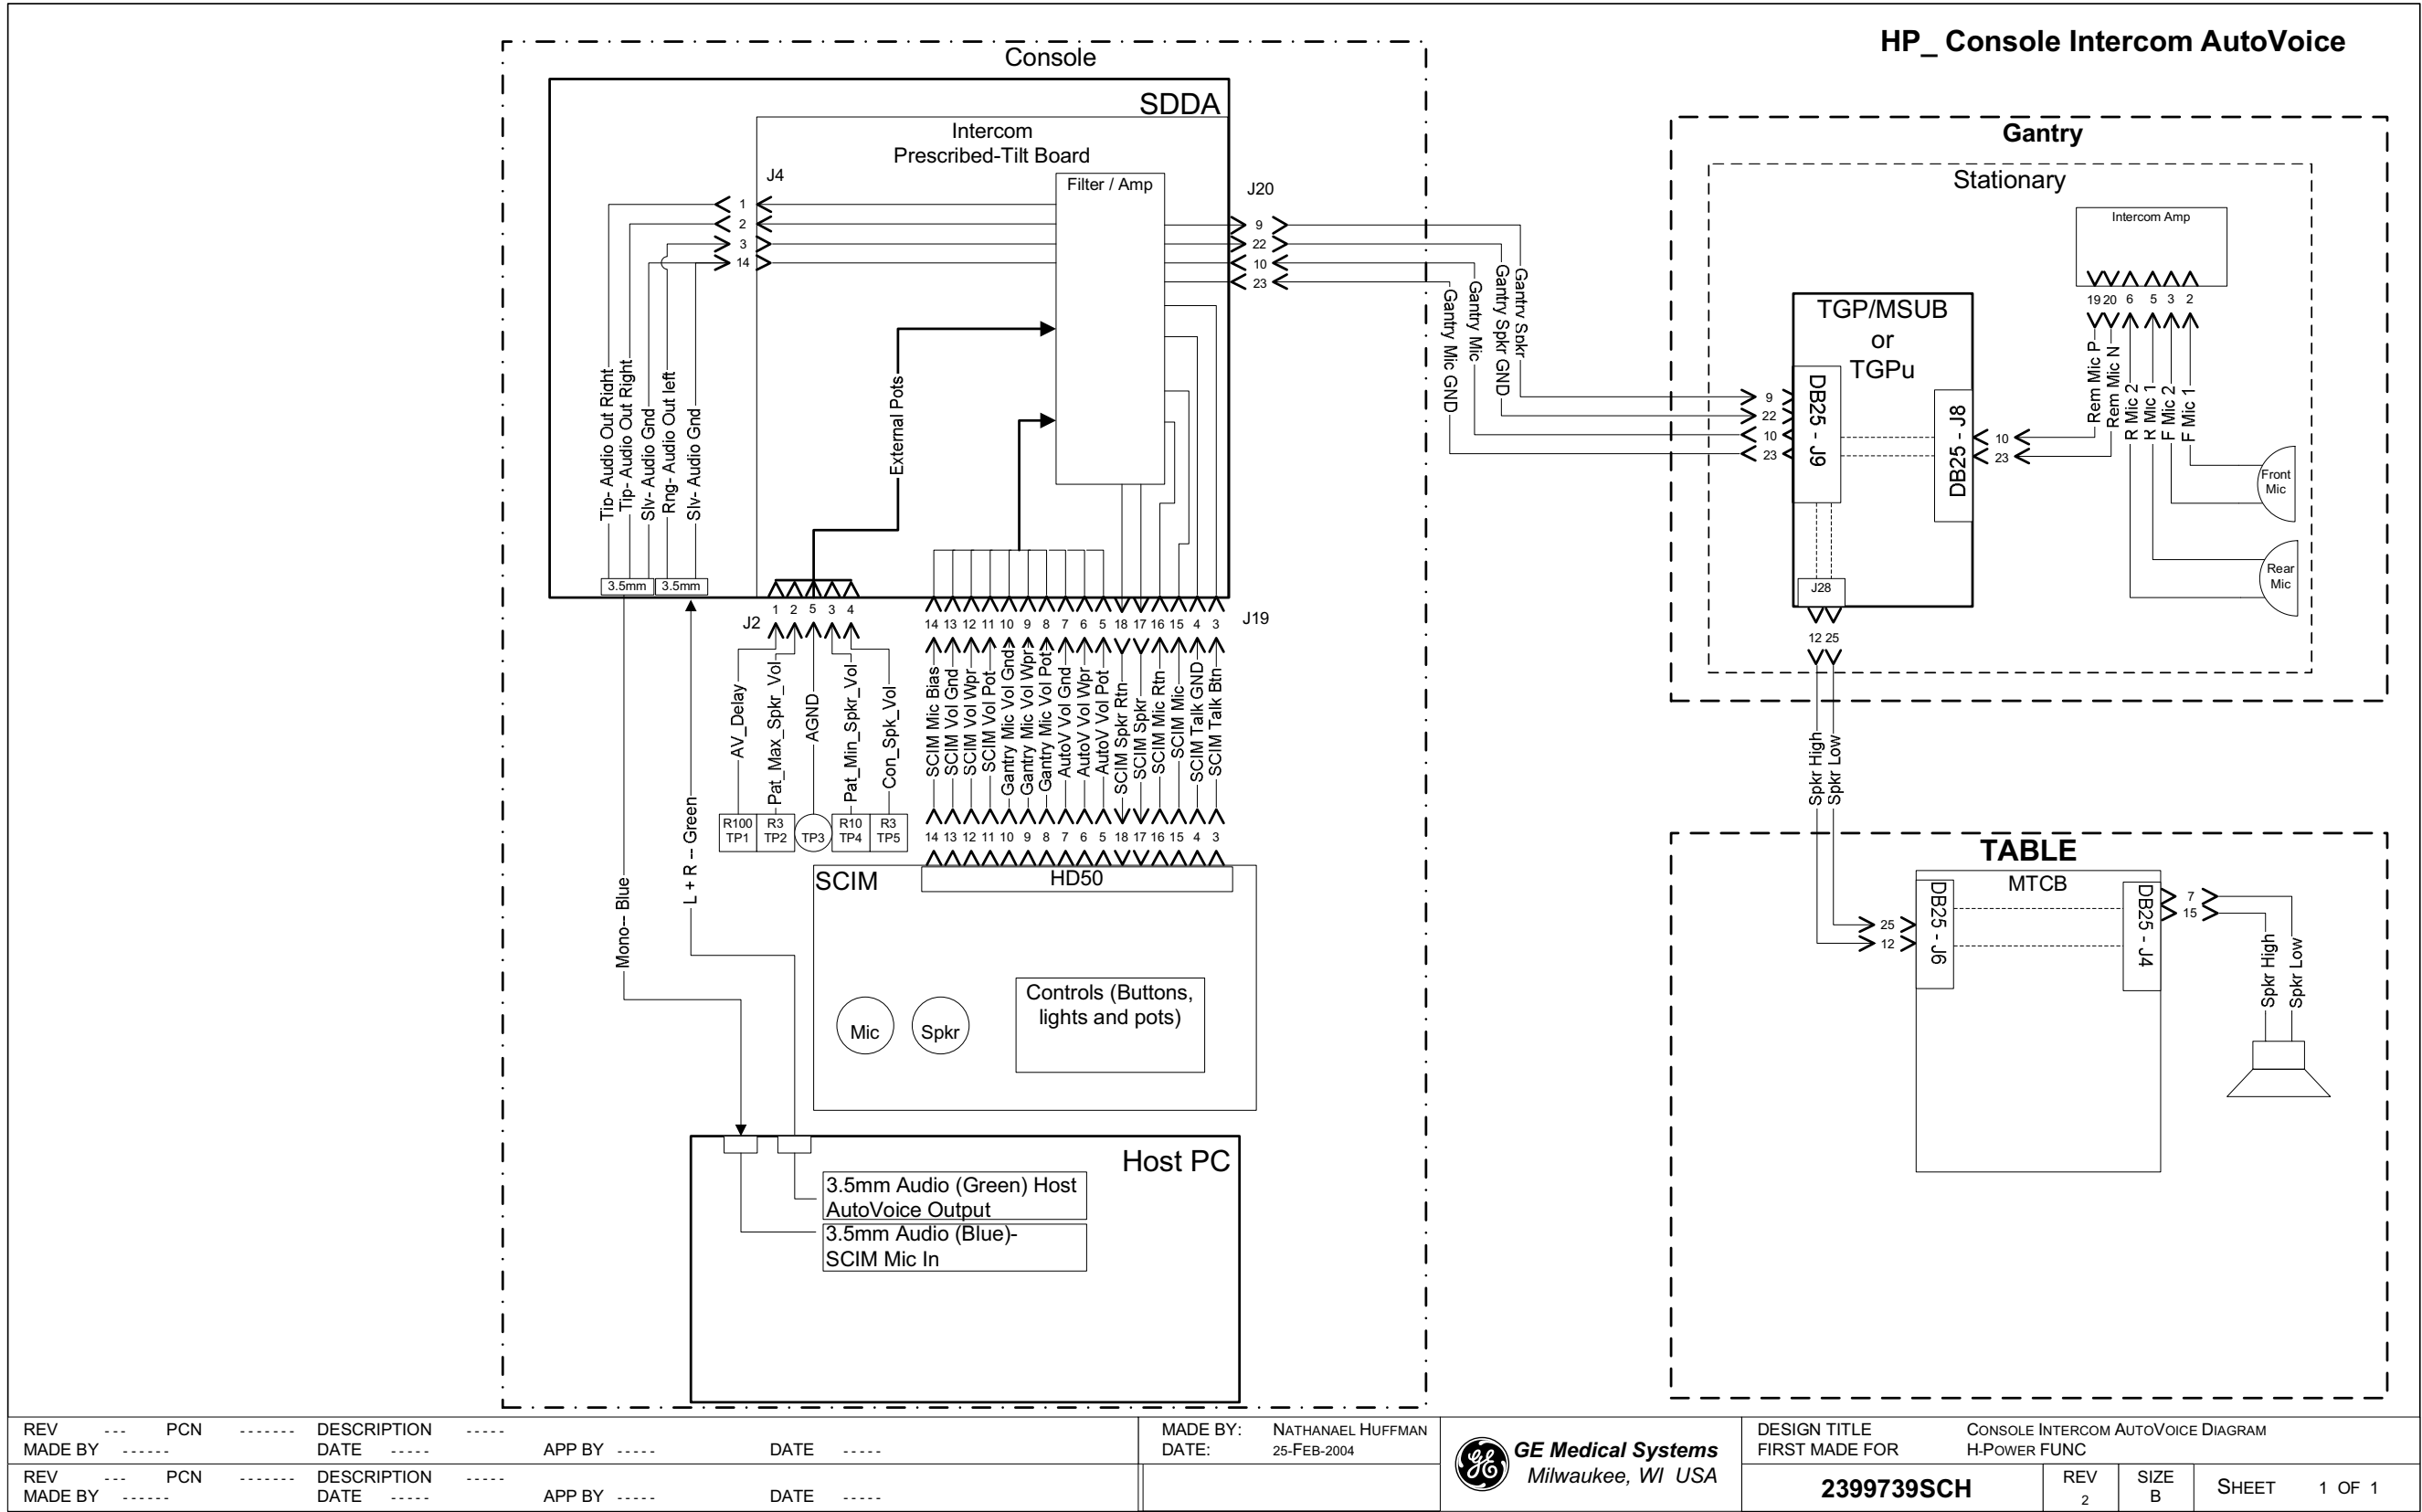

REV --- PCN --- DESCRIPTION --- MADE BY --- DATE ---	APP BY --- DATE ---	MADE BY: NATHANAEL HUFFMAN DATE: 25-FEB-2004	DESIGN TITLE FIRST MADE FOR	CONSOLE INTERCOM AUTOVOICE DIAGRAM H-POWER FUNC	REV 2	SIZE B	SHEET 1 OF 1
REV --- PCN --- DESCRIPTION --- MADE BY --- DATE ---	APP BY --- DATE ---		2399739SCH				

Figure 6-6 2399739 Sheet 1, Rev. 2

Chapter 7

System Monitoring

Section 1.0 — Gantry Temperature and Balance Sensors - 2399740

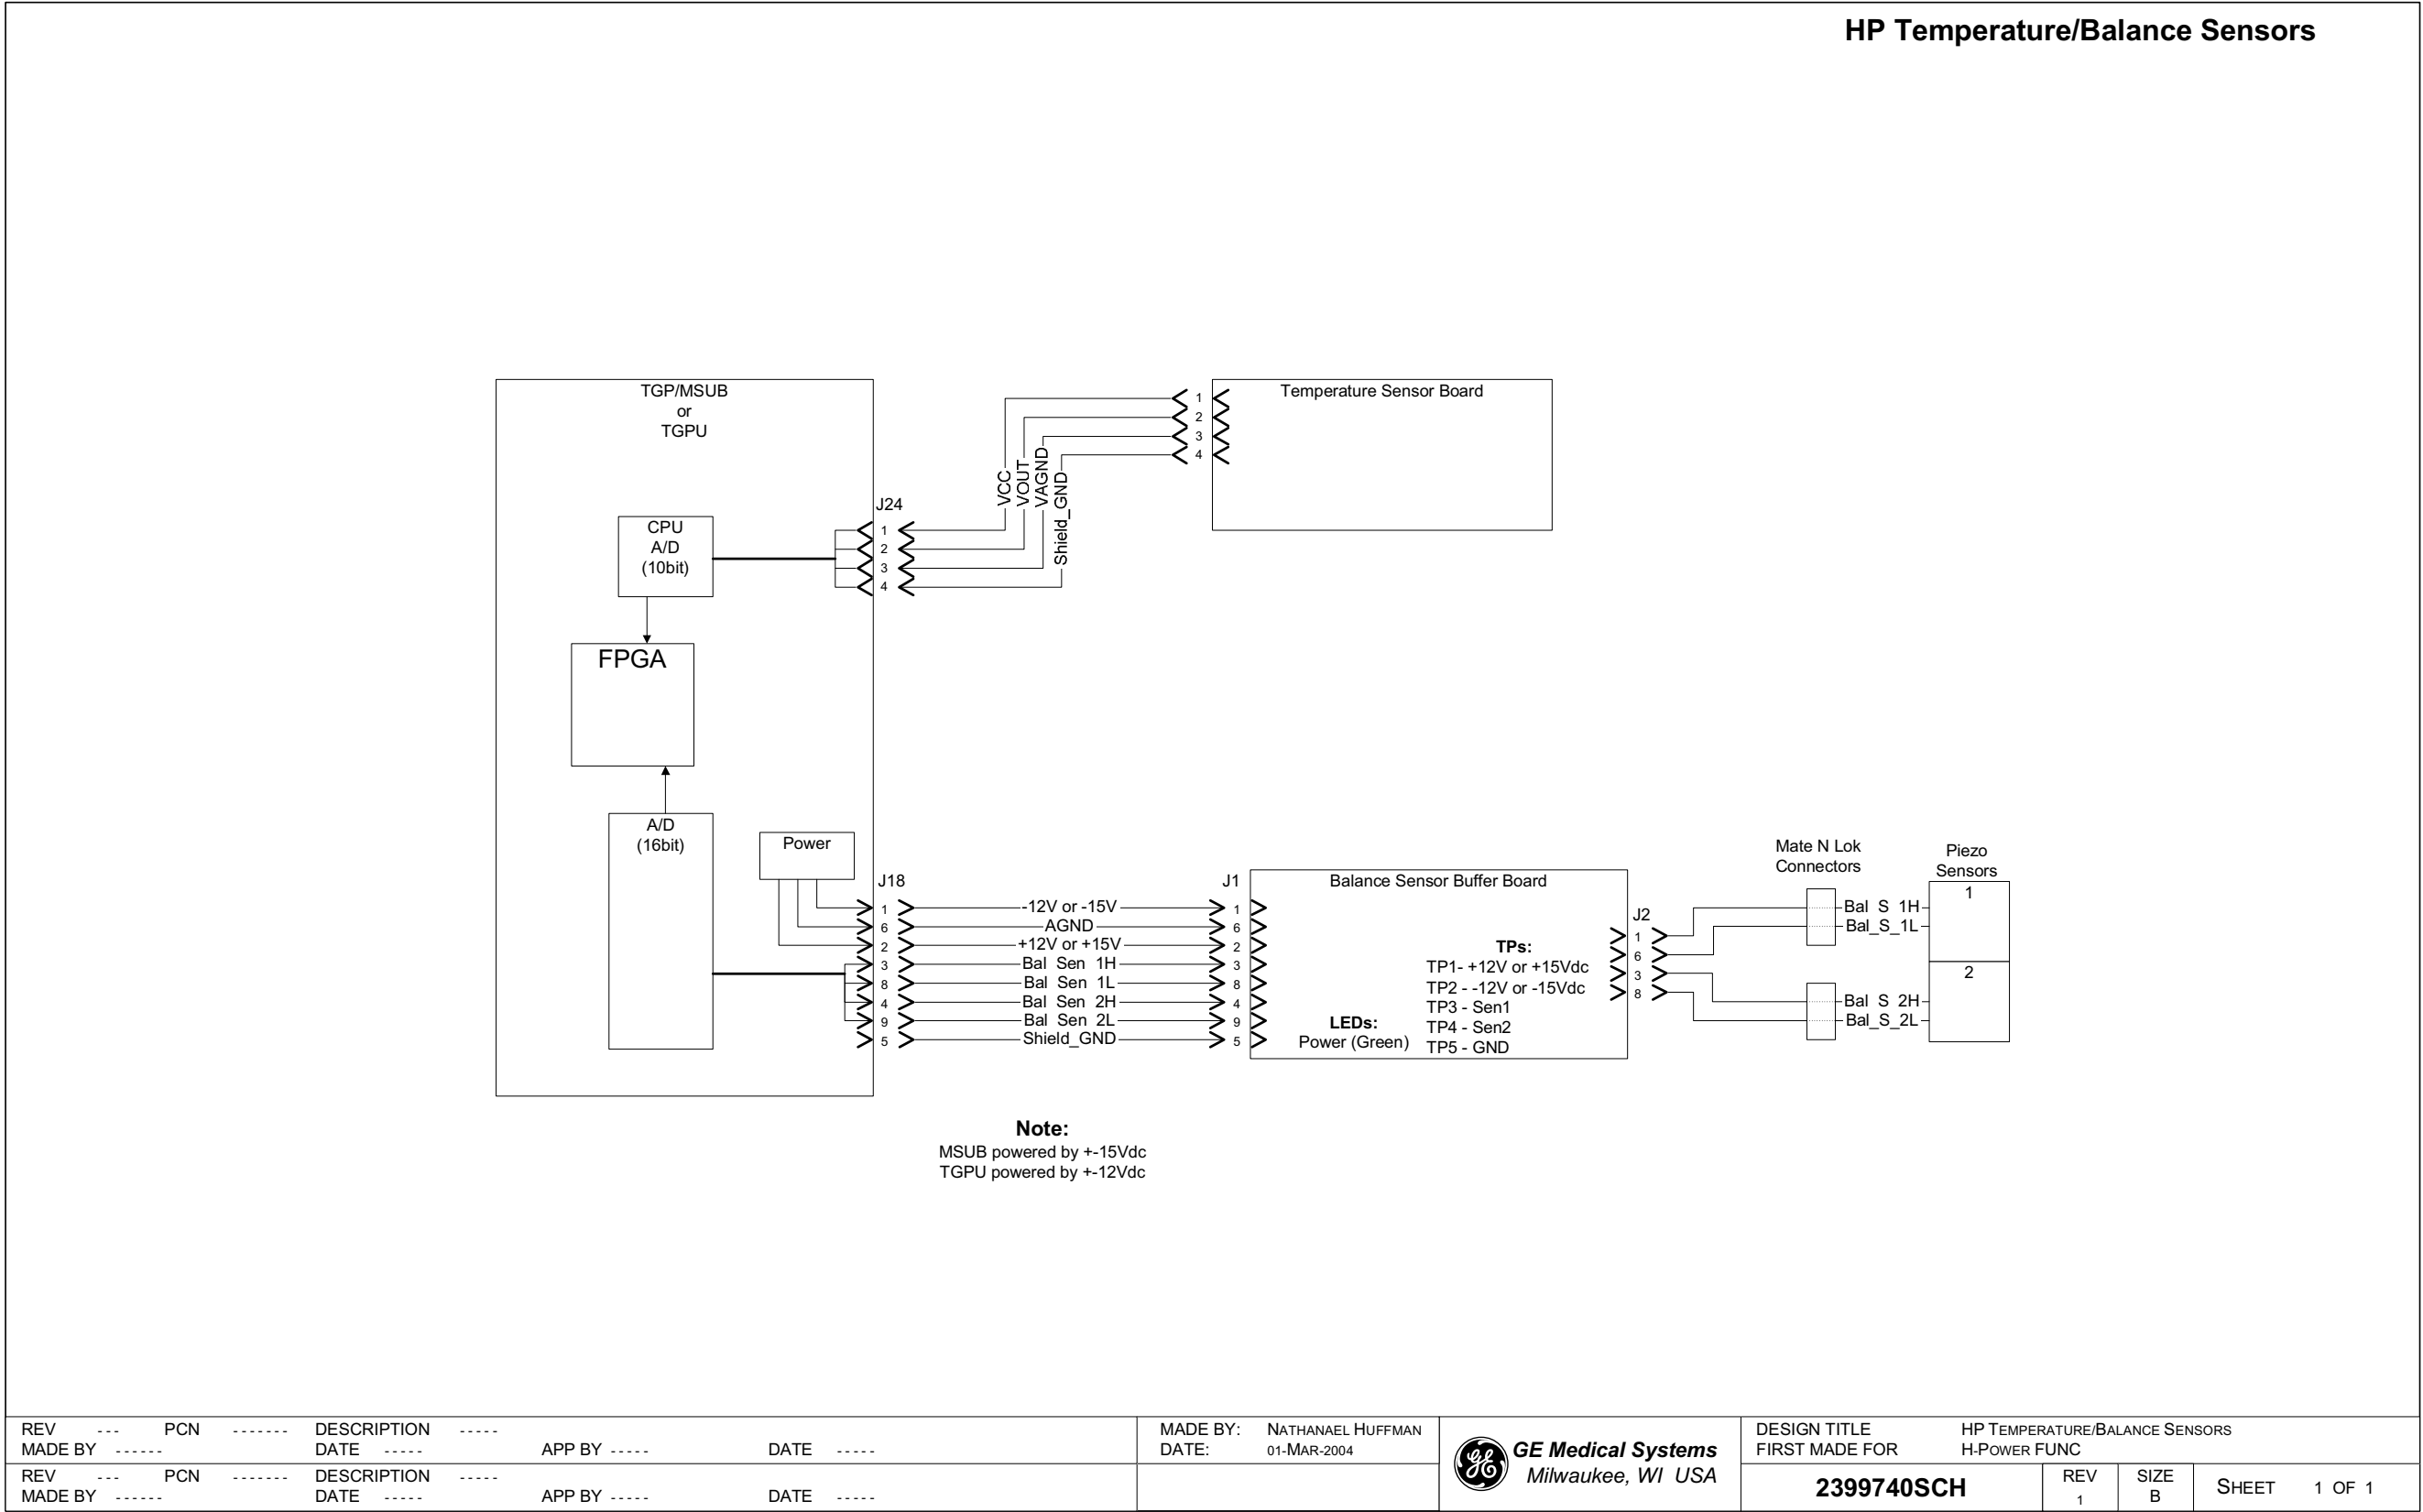


Figure 7-1 2399740 Sheet 1, Rev. 1

Section 2.0 — Gantry Cover Fans - 2399741

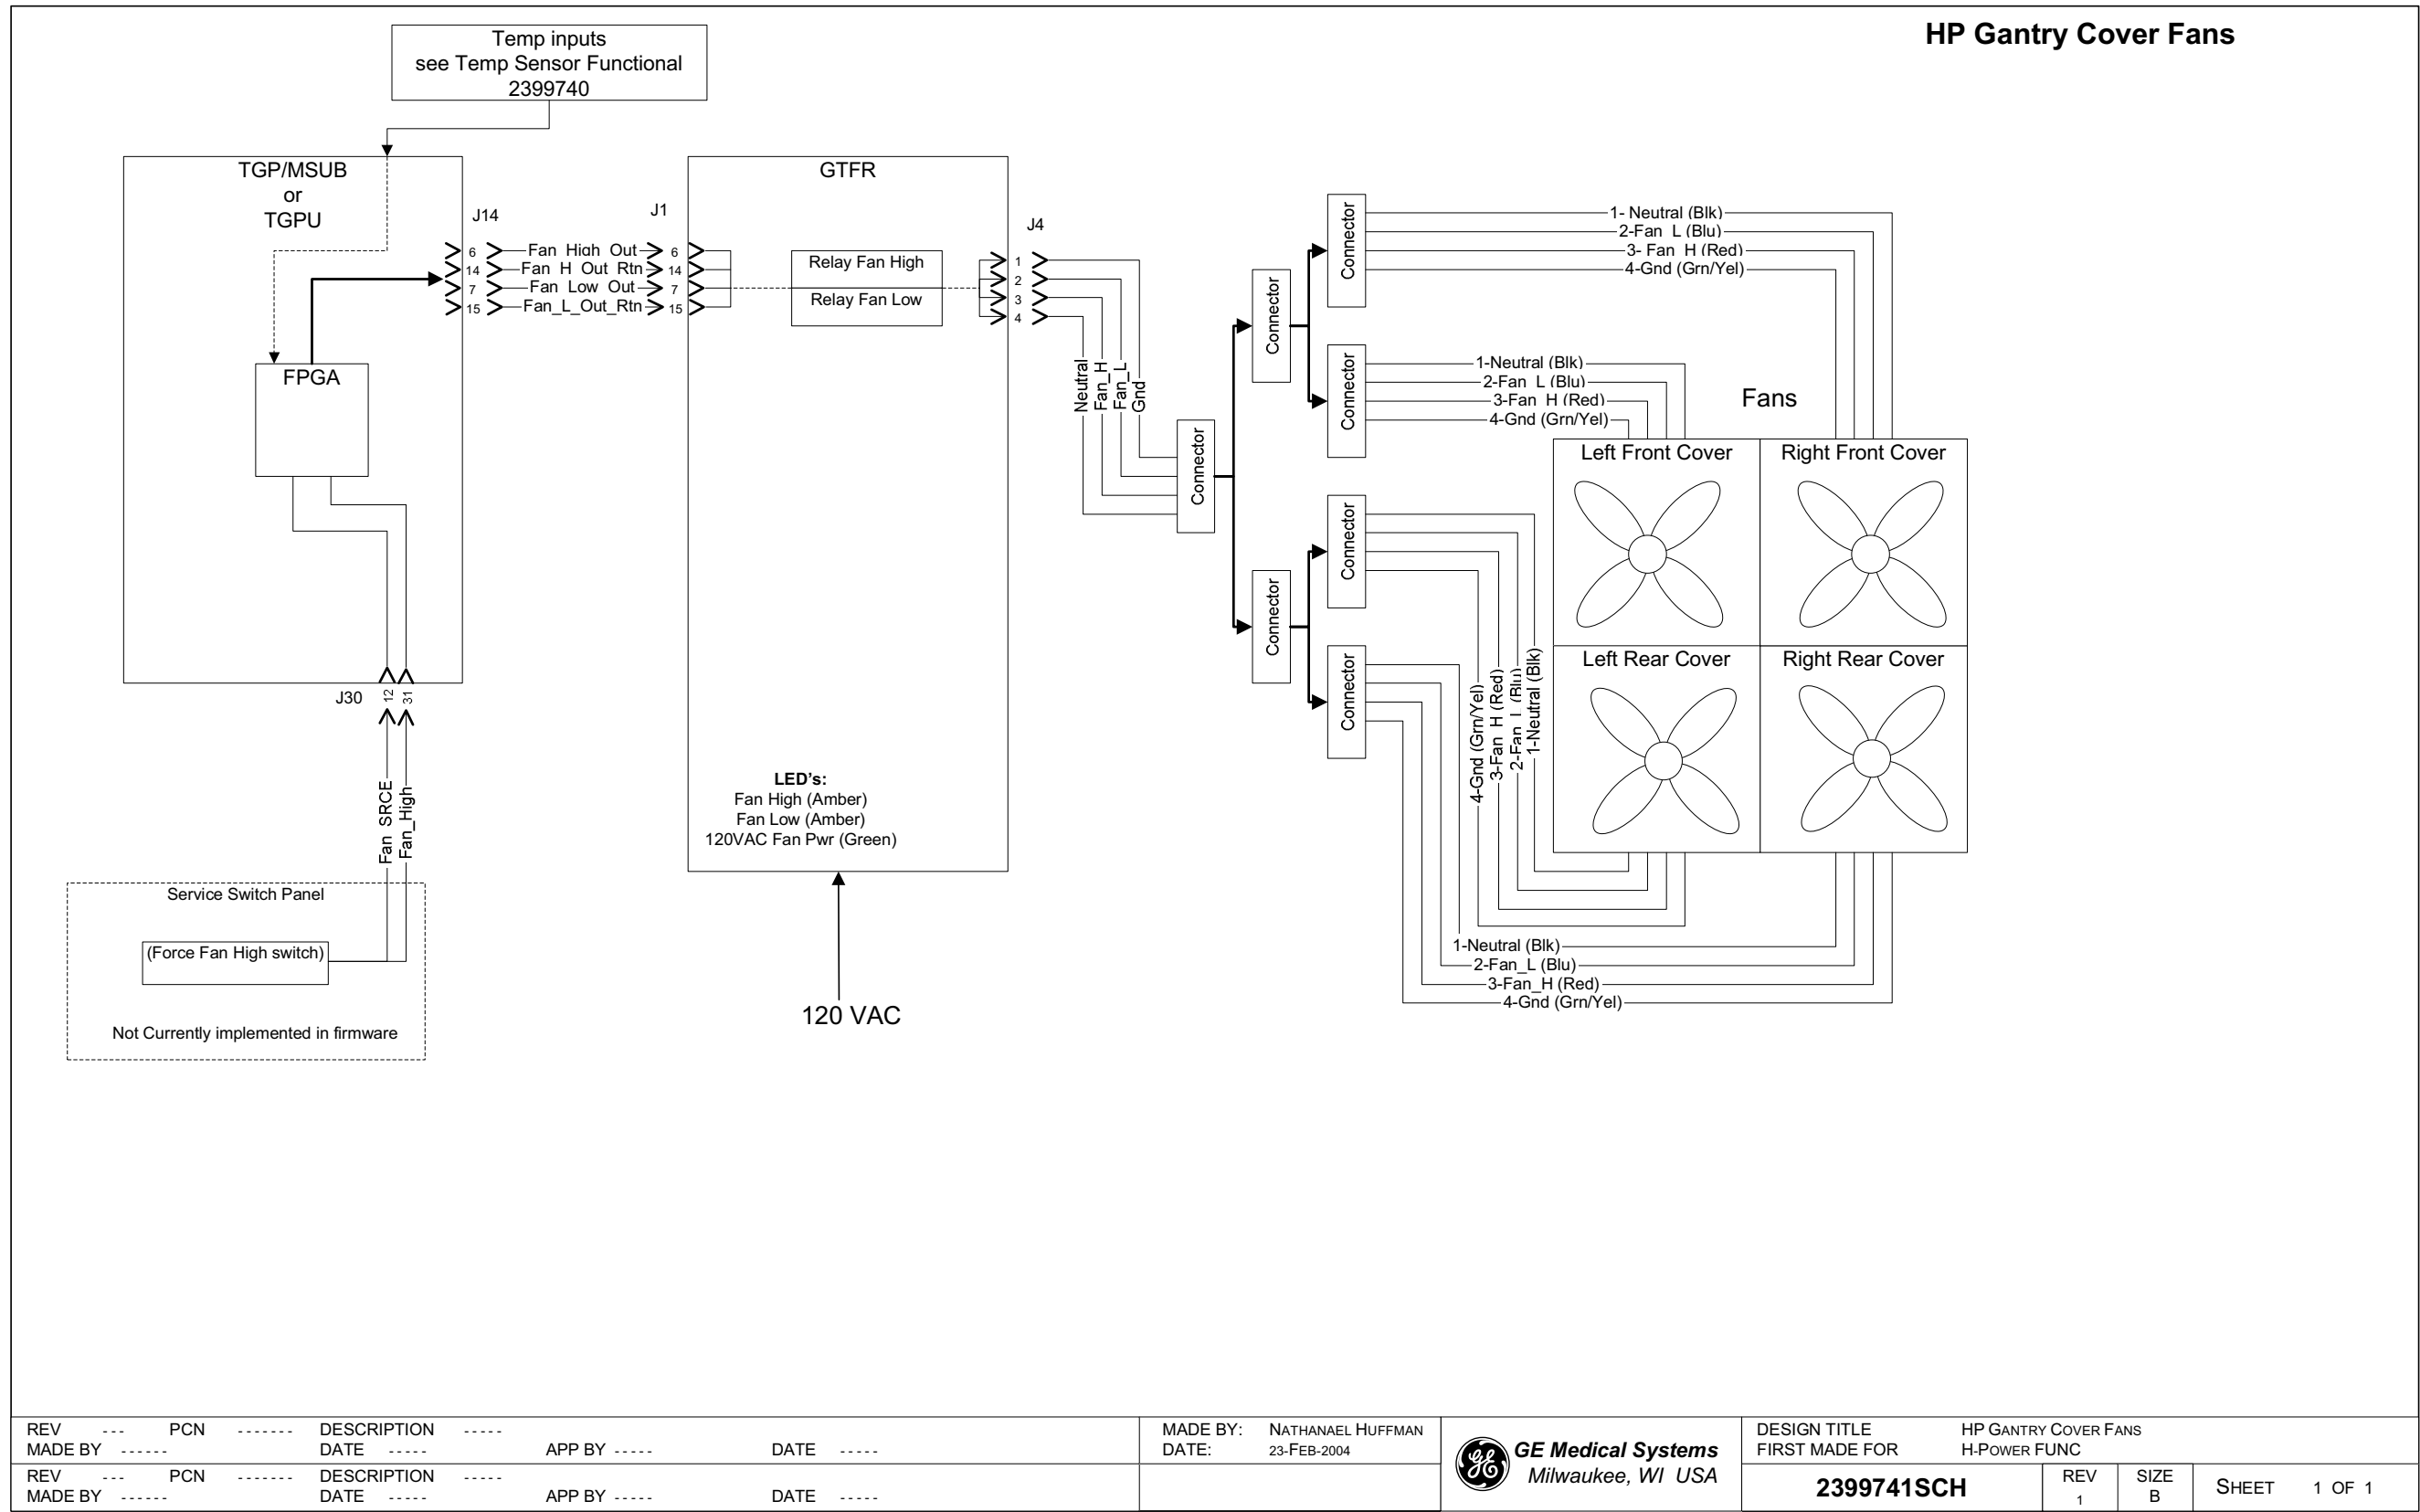


Figure 7-2 2399741 Sheet 1, Rev. 1

THIS PAGE INTENTIONALLY BLANK.

Chapter 8

System Power Control

Section 1.0 — System E-Stop and Power Interlocks - 2399742


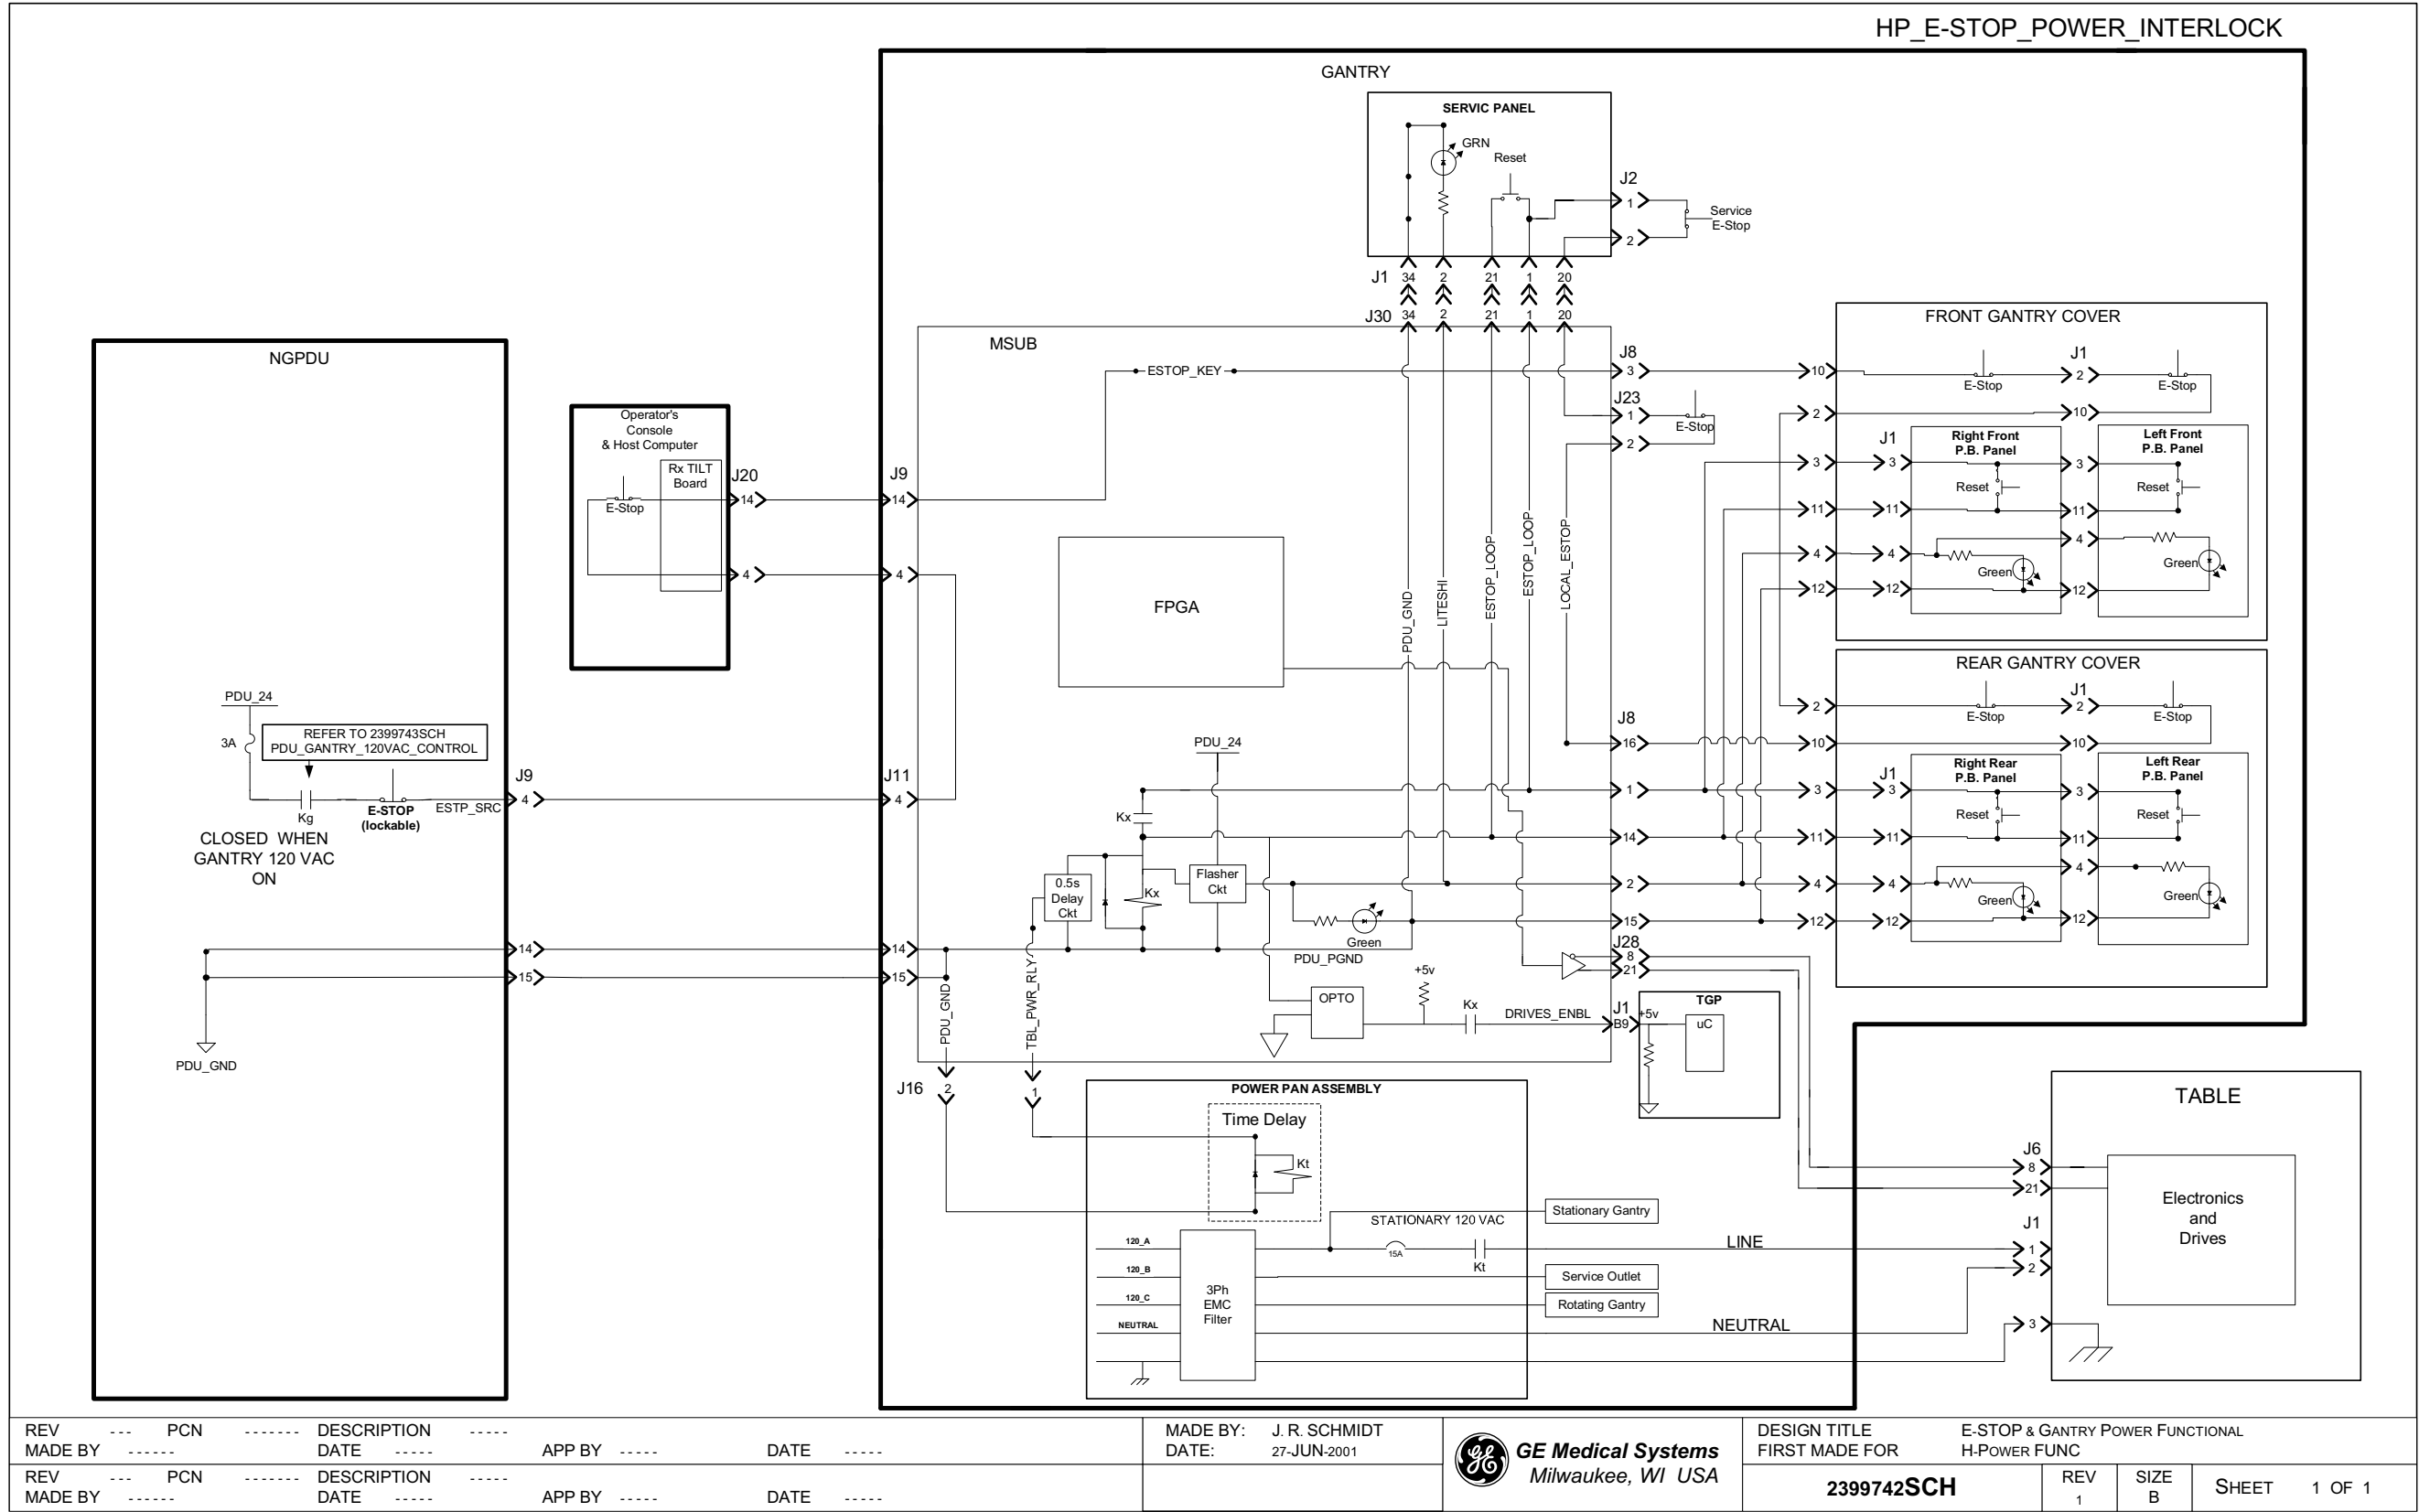


Figure 8-1 2399742 Sheet 1, Rev. 1

Section 2.0 — PDU - Gantry 120 VAC Control - 2399743

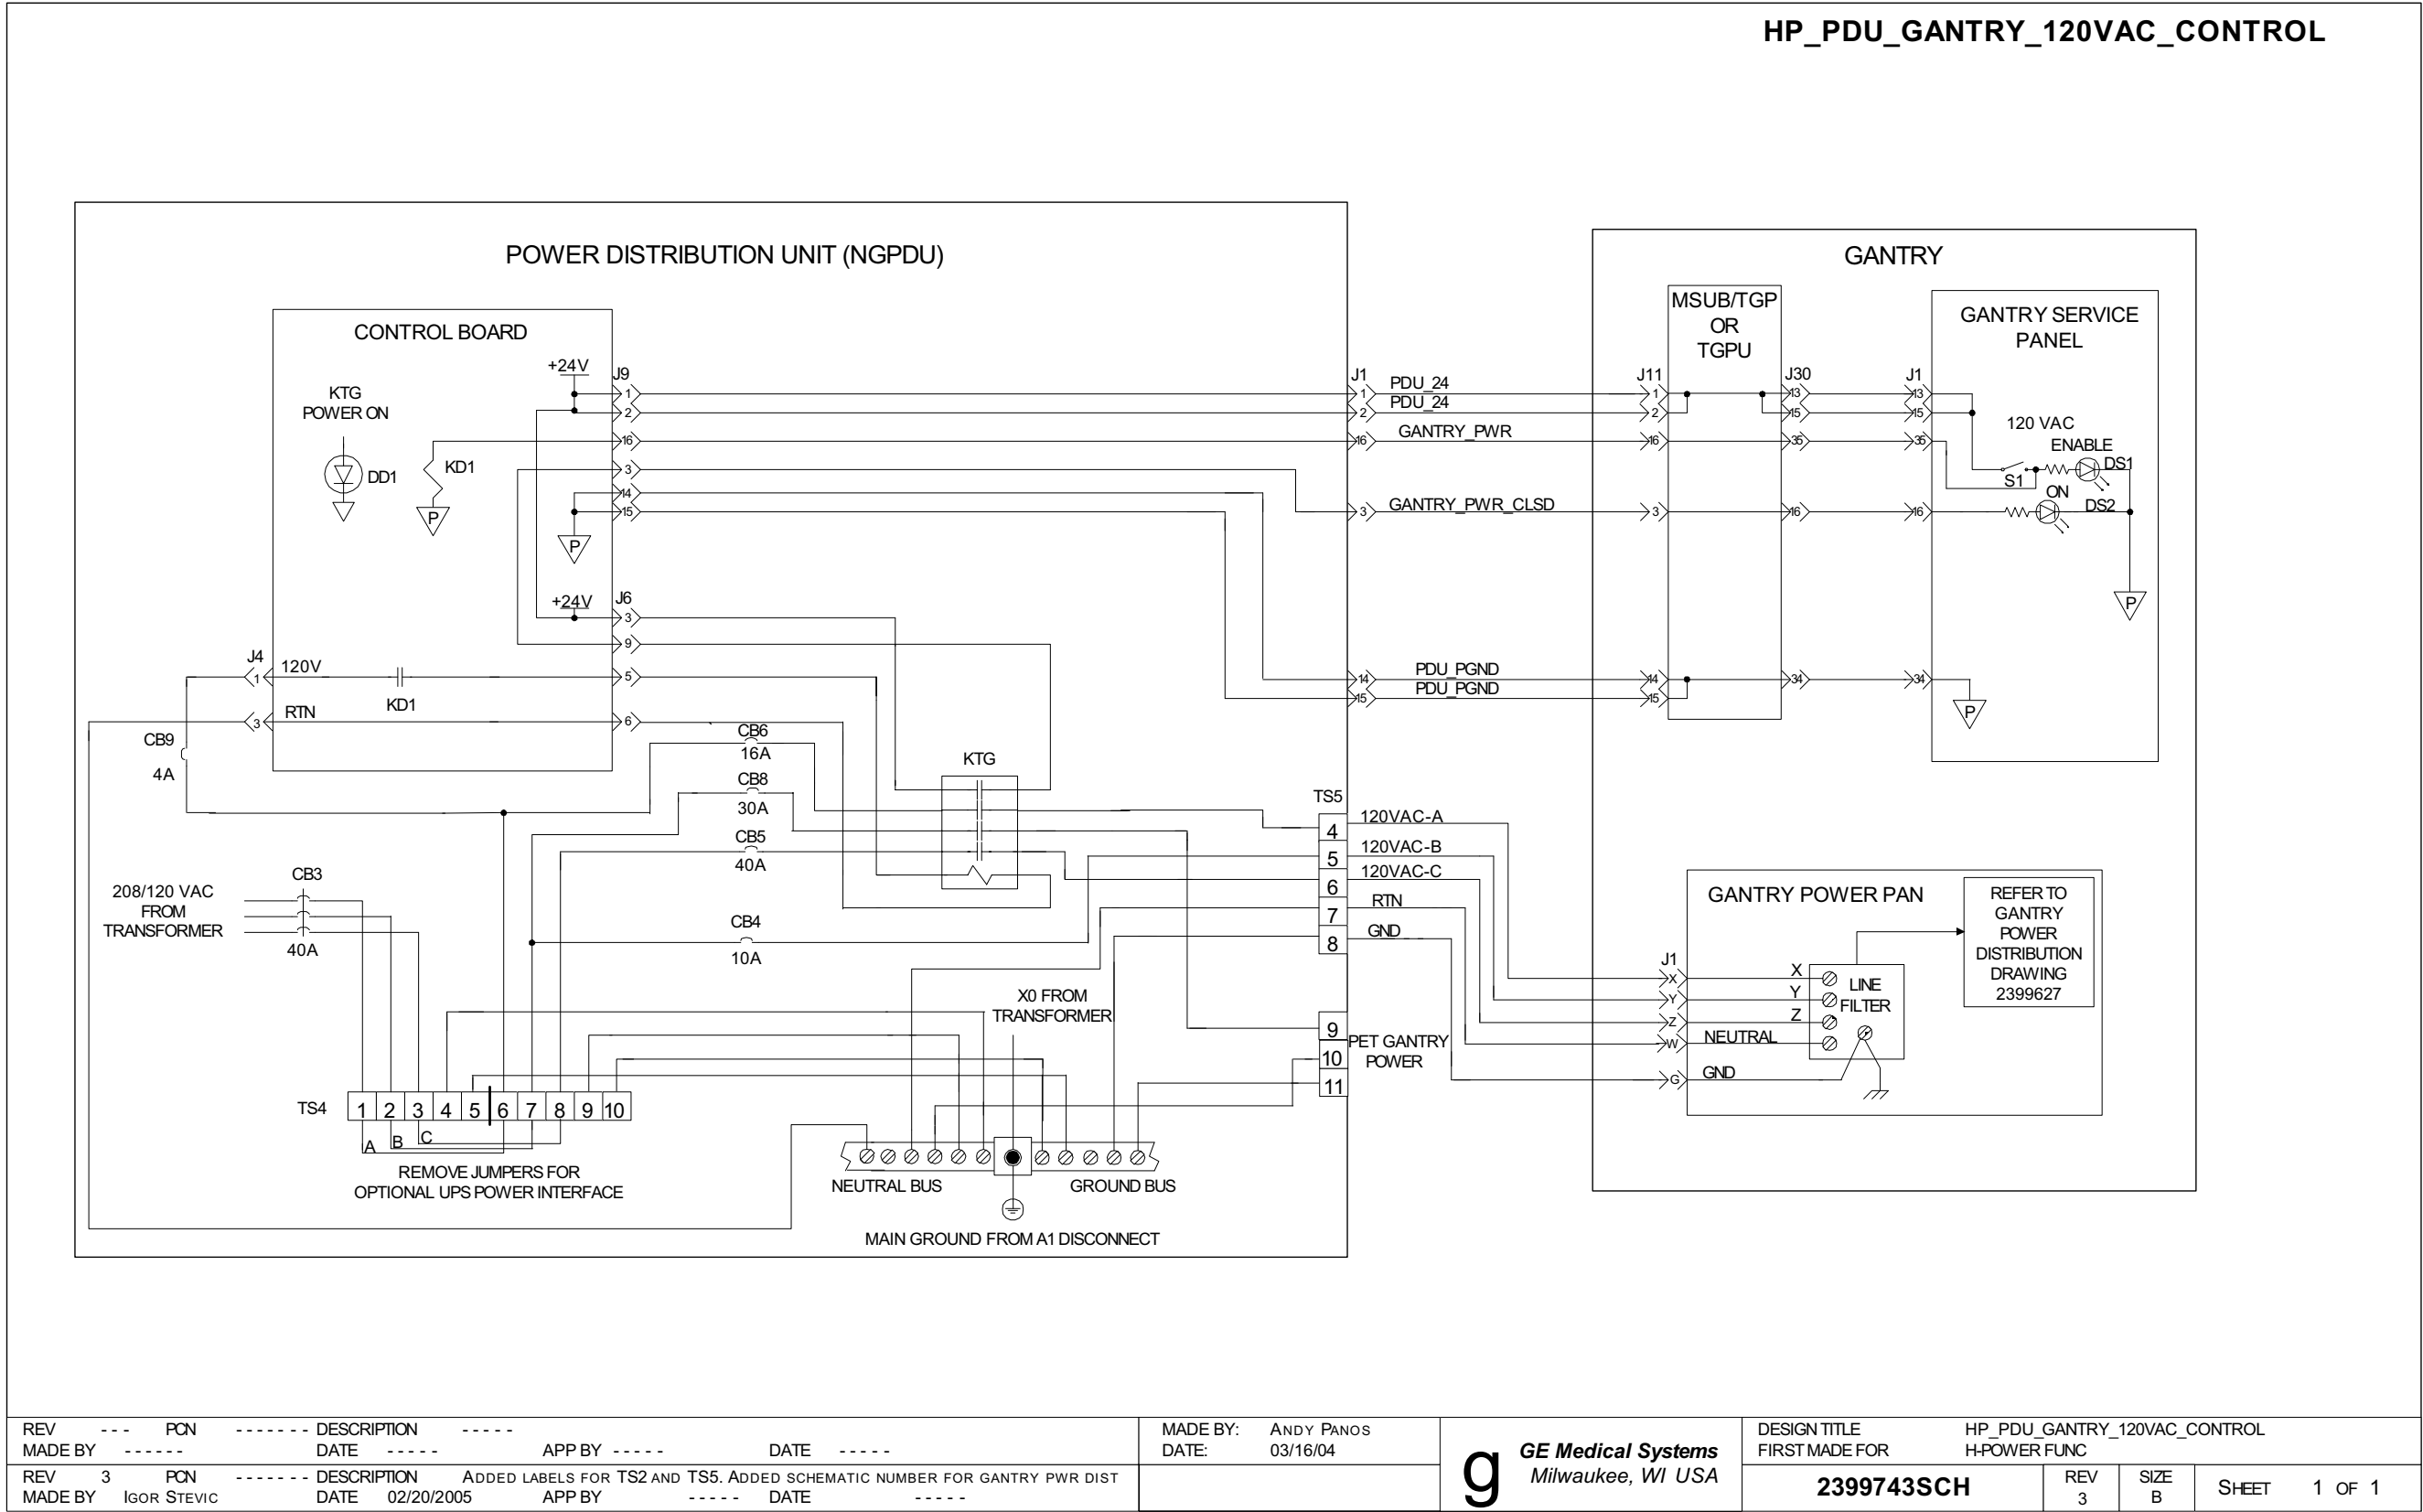

REV	---	PCN	-----	DESCRIPTION	-----	APP BY	-----	DATE	-----
MADE BY	-----			DATE	-----				
REV	3	PCN	-----	DESCRIPTION	ADDED LABELS FOR TS2 AND TS5. ADDED SCHEMATIC NUMBER FOR GANTRY PWR DIST				
MADE BY	IGOR STEVIC			DATE	02/20/2005	APP BY	-----	DATE	-----

MADE BY:	ANDY PANOS
DATE:	03/16/04

g

GE Medical Systems
Milwaukee, WI USA

DESIGN TITLE	HP_PDU_GANTRY_120VAC_CONTROL
FIRST MADE FOR	H-POWER FUNC
2399743SCH	REV 3
SIZE B	SHEET 1 OF 1

Figure 8-2 2399743 Sheet 1, Rev. 3

Section 3.0 — HV_DC_Control - 2399744

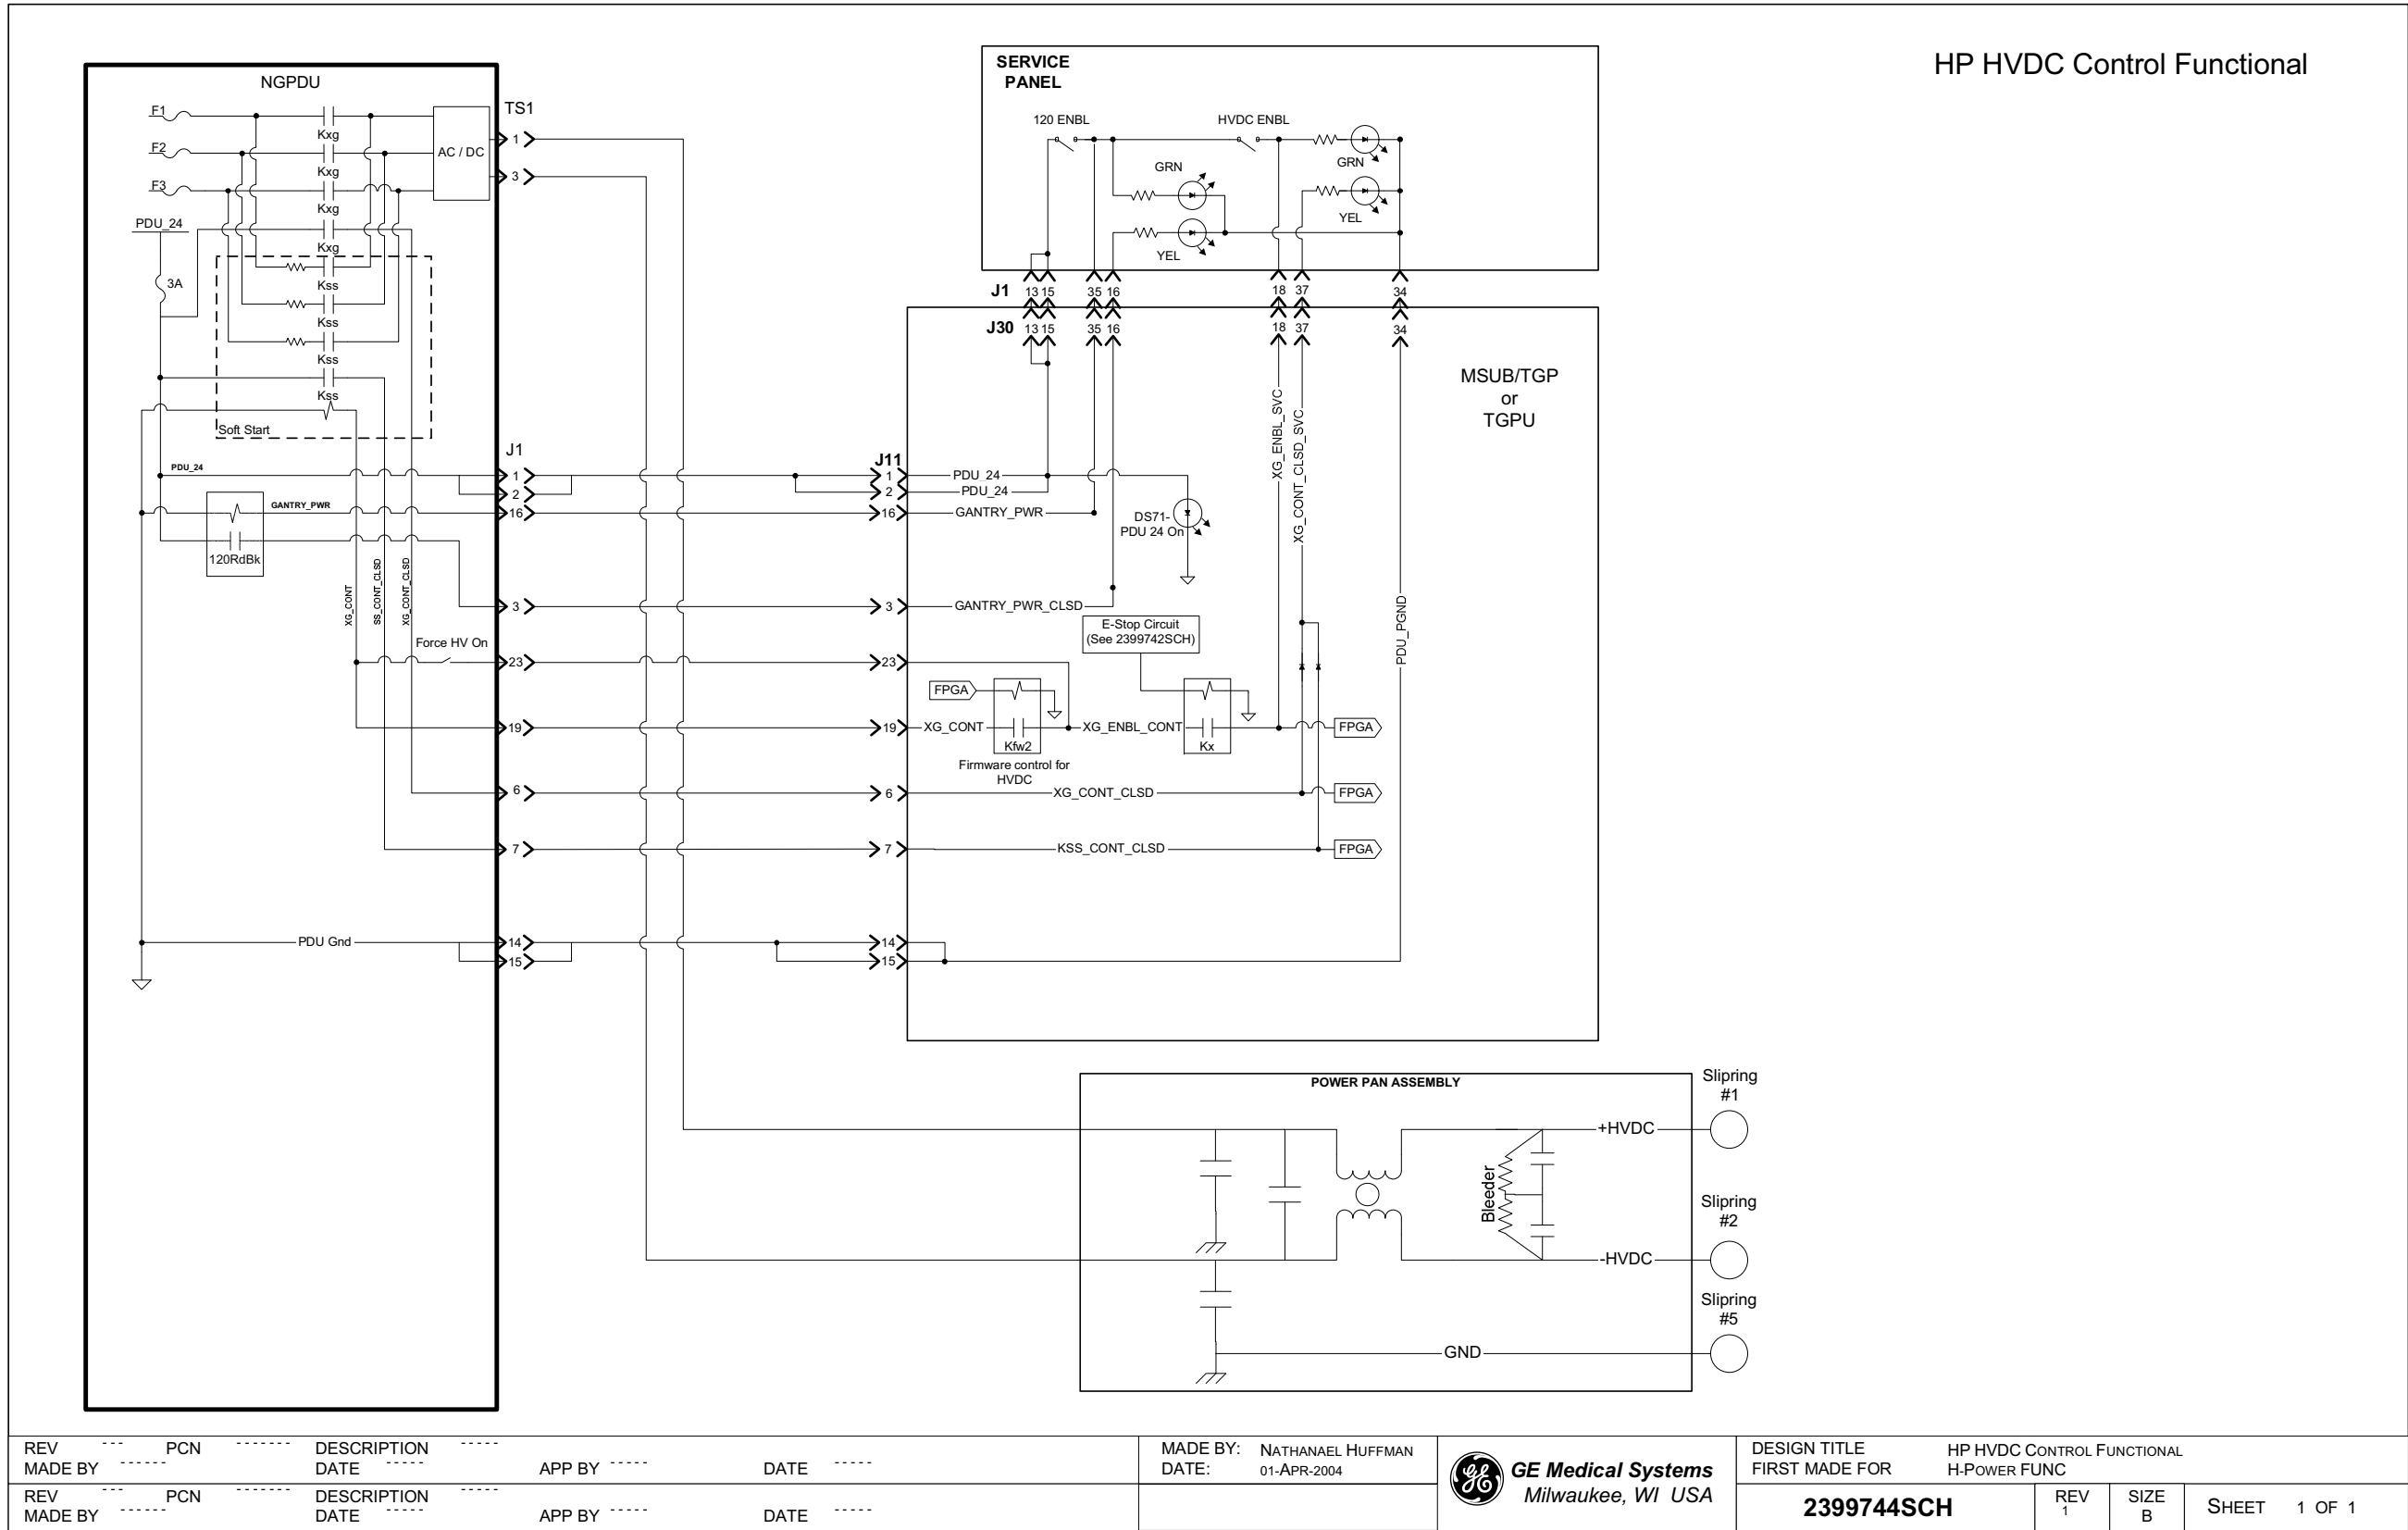


Figure 8-3 2399744 Sheet 1, Rev. 1

THIS PAGE INTENTIONALLY BLANK.