



GE Medical Systems

Technical Publications

Direction 2138247

Revision 14

Signa® Illustrated Parts List (Releases 5.x, 8.x, 9.x, and 10.x)

**Copyright© 1995 – 2004 by General Electric Company, Inc.
All Rights Reserved**

Operating Documentation

DAMAGE IN TRANSPORTATION

All packages should be closely examined at time of delivery. If damage is apparent, have notation "**damage in shipment**" written on **all** copies of the freight or express bill **before** delivery is accepted or "signed for" by a General Electric representative or a hospital receiving agent. Whether noted or concealed, damage **MUST** be reported to the carrier immediately upon discovery, or in any event, within 14 days after receipt, and the contents and containers held for inspection by the carrier. A transportation company will not pay a claim for damage if an inspection is not requested within this 14 day period.

Immediately complete "**Damage Loss Claim Form**" after damage is found. Form is available via MS Exchange Mail at Outlook/Public Folder/All Public Folders/Medical Systems/!Global Initiatives/Information Management/Forms/Common Forms/Damage Loss Claim Form. Send completed form to e-mail address listed on form.

For more information about the Transportation Claim Procedure, access the GE Medical Systems Intranet and enter the following URL address:

<ftp://3.87.40.2/globepro/qualsys/Docs/190016ME.PDF>

Rev. 11/15/2000



GE Medical Systems

GE Medical Systems: Telex 3797371
P.O. Box 414, Milwaukee, Wisconsin 53201 U.S.A.
(Asia, Pacific, Latin America, North America)

GE Medical Systems — Europe: Telex 261794
Shortlands, Hammersmith, London W6 8BX U.K.

WARNING

- THIS SERVICE MANUAL IS AVAILABLE IN ENGLISH ONLY.
- IF A CUSTOMER'S SERVICE PROVIDER REQUIRES A LANGUAGE OTHER THAN ENGLISH, IT IS THE CUSTOMER'S RESPONSIBILITY TO PROVIDE TRANSLATION SERVICES.
- DO NOT ATTEMPT TO SERVICE THE EQUIPMENT UNLESS THIS SERVICE MANUAL HAS BEEN CONSULTED AND IS UNDERSTOOD.
- FAILURE TO HEED THIS WARNING MAY RESULT IN INJURY TO THE SERVICE PROVIDER, OPERATOR OR PATIENT FROM ELECTRIC SHOCK, MECHANICAL OR OTHER HAZARDS.

AVERTISSEMENT

- CE MANUEL DE MAINTENANCE N'EST DISPONIBLE QU'EN ANGLAIS.
- SI LE TECHNICIEN DU CLIENT A BESOIN DE CE MANUEL DANS UNE AUTRE LANGUE QUE L'ANGLAIS, C'EST AU CLIENT QU'IL INCOMBE DE LE FAIRE TRADUIRE.
- NE PAS TENTER D'INTERVENTION SUR LES ÉQUIPEMENTS TANT QUE LE MANUEL SERVICE N'A PAS ÉTÉ CONSULTÉ ET COMPRIS.
- LE NON-RESPECT DE CET AVERTISSEMENT PEUT ENTRAÎNER CHEZ LE TECHNICIEN, L'OPÉRATEUR OU LE PATIENT DES BLESSURES DUES À DES DANGERS ÉLECTRIQUES, MÉCANIQUES OU AUTRES.

WARNUNG

- DIESES KUNDENDIENST-HANDBUCH EXISTIERT NUR IN ENGLISCHER SPRACHE.
- FALLS EIN FREMDER KUNDENDIENST EINE ANDERE SPRACHE BENÖTIGT, IST ES AUFGABE DES KUNDEN FÜR EINE ENTSPRECHENDE ÜBERSETZUNG ZU SORGEN.
- VERSUCHEN SIE NICHT, DAS GERÄT ZU REPARIEREN, BEVOR DIESES KUNDENDIENST-HANDBUCH ZU RATE GEZOGEN UND VERSTANDEN WURDE.
- WIRD DIESE WARNUNG NICHT BEACHTET, SO KANN ES ZU VERLETZUNGEN DES KUNDENDIENSTTECHNIKERS, DES BEDIENERS ODER DES PATIENTEN DURCH ELEKTRISCHE SCHLÄGE, MECHANISCHE ODER SONSTIGE GEFAHREN KOMMEN.

AVISO

- ESTE MANUAL DE SERVICIO SÓLO EXISTE EN INGLÉS.
- SI ALGÚN PROVEEDOR DE SERVICIOS AJENO A GEMS SOLICITA UN IDIOMA QUE NO SEA EL INGLÉS, ES RESPONSABILIDAD DEL CLIENTE OFRECER UN SERVICIO DE TRADUCCIÓN.
- NO SE DEBERÁ DAR SERVICIO TÉCNICO AL EQUIPO, SIN HABER CONSULTADO Y COMPRENDIDO ESTE MANUAL DE SERVICIO.
- LA NO OBSERVANCIA DEL PRESENTE AVISO PUEDE DAR LUGAR A QUE EL PROVEEDOR DE SERVICIOS, EL OPERADOR O EL PACIENTE SUFRAN LESIONES PROVOCADAS POR CAUSAS ELÉCTRICAS, MECÁNICAS O DE OTRA NATURALEZA.

ATENÇÃO

- ESTE MANUAL DE ASSISTÊNCIA TÉCNICA SÓ SE ENCONTRA DISPONÍVEL EM INGLÊS.
- SE QUALQUER OUTRO SERVIÇO DE ASSISTÊNCIA TÉCNICA, QUE NÃO A GEMS, SOLICITAR ESTES MANUAIS NOUTRO IDIOMA, É DA RESPONSABILIDADE DO CLIENTE FORNECER OS SERVIÇOS DE TRADUÇÃO.
- NÃO TENHA TENTADO REPARAR O EQUIPAMENTO SEM TER CONSULTADO E COMPREENDIDO ESTE MANUAL DE ASSISTÊNCIA TÉCNICA.
- O NÃO CUMPRIMENTO DESTA AVISO PODE POR EM PERIGO A SEGURANÇA DO TÉCNICO, OPERADOR OU PACIENTE DEVIDO A CHOQUES ELÉTRICOS, MECÂNICOS OU OUTROS.

AVVERTENZA

- IL PRESENTE MANUALE DI MANUTENZIONE È DISPONIBILE SOLTANTO IN INGLESE.
- SE UN ADDETTO ALLA MANUTENZIONE ESTERNO ALLA GEMS RICHIEDE IL MANUALE IN UNA LINGUA DIVERSA, IL CLIENTE È TENUTO A PROVVEDERE DIRETTAMENTE ALLA TRADUZIONE.
- SI PROCEDA ALLA MANUTENZIONE DELL'APPARECCHIATURA SOLO DOPO AVER CONSULTATO IL PRESENTE MANUALE ED AVERNE COMPRESO IL CONTENUTO.
- NON TENERE CONTO DELLA PRESENTE AVVERTENZA POTREBBE FAR COMPIERE OPERAZIONI DA CUI DERIVINO LESIONI ALL'ADDETTO ALLA MANUTENZIONE, ALL'UTILIZZATORE ED AL PAZIENTE PER FOLGORAZIONE ELETTRICA, PER URTI MECCANICI OD ALTRI RISCHI.

警告

- ・ このサービスマニュアルには英語版しかありません。
- ・ GEMS以外でサービスを担当される業者が英語以外の言語を要求される場合、翻訳作業はその業者の責任で行うものとさせていただきます。
- ・ このサービスマニュアルを熟読し理解せずに、装置のサービスを行わないで下さい。
- ・ この警告に従わない場合、サービスを担当される方、操作員あるいは患者さんが、感電や機械的又はその他の危険により負傷する可能性があります。

注意：

- 本维修手册仅存有英文本。
- 非 GEMS 公司的维修员要求非英文本的维修手册时，客户需自行负责翻译。
- 未详细阅读和完全了解本手册之前，不得进行维修。
- 忽略本注意事项会对维修员，操作员或病人造成触电，机械伤害或其他伤害。

REVISION HISTORY

REV	DATE	PRIMARY REASON FOR CHANGE
0	 Jul., 1995 ...	Initial release for pre-production systems.
1	 Oct. 23, 1995 ...	Removed information that is now provided on Rev 1 of MR CD-ROM <i>Direction 2124201</i> , <i>MR Release 5.x Service Methods</i> . Changed the title of this Direction to reflect those procedures which are not provided on the MR CD-ROM yet (Release 5.5 renewal parts, and EPI calibration).
2	 May, 24, 1996 ...	Removed Tab 1 Calibration information. These procedures are now found on MR CD-ROM <i>Direction 2124201</i> .
3	 Feb. 14, 1997 ...	Changed manual title from Supplemental Service Methods to Renewal Parts. Added sections 3 and 7. Revised all sections to include new LX information. Added True Mobile, Relocatable and Transportable catalogs and related parts information. Added and expanded section 11 with new LX options. Section 9 was divided and the GRAM information, 9A, was moved to new section 12. New section 13, Operator Workspace, was added. Calibration tab and information was removed.
4	 Aug. 24, 1997 ...	Added Cx Magnet Enclosure, SGD Gradient Cabinet, and RF/PEN II catalog information in Section 1, along with other changes. Added Cx Magnet Enclosure parts information to Section 2. Added revised part changes to Section 8, System Cabinet. Added SGD Hi-Slew Gradient information to Section 9. Added RF/PEN II Cabinet information to Section 10. Revised and added parts in Section 13, Operator Workspace. Also made general corrections and changes in other parts of the manual.
5	 Jun 12, 1998 ...	Section 1 – Added Octane computer catalog information along with other changes and additions. Section 2 – Added parts and other update information via CQA referrals. Section 3 – Updated Patient Table information to reflect latest configuration. Section 9 – Added SGD Base Gradient Cabinet information. Section 11 – Updated Accessories and Options to include latest product offerings and other changes and revisions. Section 13 – Added Octane Computer information and updated Indigo computer area to reflect latest revisions and additions.
6	 Sep 30, 1998 ...	Changed the name of the manual to Signa Renewal Parts Release 5.x and 8.x to encompass new CVMR and other future product lines. Section 1 – Added LCC and CVMR catalog information. Section 2 – Added LCC and CVMR magnet enclosure structures and other miscellaneous corrections and additions. Section 8 – Added CVMR system cabinet. Section 11 – Added new Torso Phased Array and Cardiac coils. Section 13 – Added CVMR Octane system computer information and other changes and additions through out the section. Section 14 – New RF/PDU tab and 1.0T RF/PDU cabinet to be added to manual.
7	 Apr 30, 1999 ...	Section 1 – Added MR/i and CV/i catalog information. Section 2 – Added MR/i and CV/i wide-open enclosure and other minor changes and additions. Section 4 – Added Mobile & T/R Penetration Panel cover. Section 8 – Updated section to add IPG II info. Section 9 – Minor corrections. Section 10 – Added several new options. Section 13 – Corrected part numbers and other minor revisions.
8	 Oct 21, 1999 ...	Section 1 – Added 8.s s/w, UCERD, and 1.5T RF/PDU catalog information. Section 7 – Added 46–320144g6 (CQA994035). Section 8 – Added new System cabinets with UCERD, new BIT3 and other changes. Section 9 – Added fuses to 8645 amps (CQA993726). Added MiniGram replacement information. Section 11 – Added 8.3 Option catalogs. Section 13 – Added Release 8.3 configurations and other minor corrections. Section 14 – Added 1.5T RF/PDU cabinet.
9	 Feb 18, 2000 ...	Section 2 – Updated hardware part numbers. Added missing spring to Dock asm (CQA995405) and updated gear-motor part number. Added replacement lamp and lead for Bore Light Asm (CQA997944). Updated WideOpen enclosure assemblies to reflect latest product structure. Section 8 – Added optional Bit3 module, 2149852–2. Highlighted FRU Ones on Page 8–82. Corrected UCERD illustration on Page 8–83. Section 13 – Corrected DASM fru codes. Added SCSI expansion box model 2199817–8.
10	 Nov 10, 2000 ...	Tab 13 – Removed muffin fan as FRU from auxiliary power supply in OW cabinet. Added Section 15, ACGD/PDU Cabinet, and Section 16, SRF Cabinet.
11	 Jun 27, 2001 ...	Tab 2 – Added ASP2 laser information to front Cx and LCC front covers. Corrected Dock Asm part numbers (CQA1012003). Tab 5 – Corrected compression ring part number (SPR#MRlge60072). Tab 8 – Added 34MHz ReFlex AP modules. Tab 13 – Updated cable collectors, added new LCD monitors, added new software collector. Tab 16 – Changed 2160200–43 to 2160200–45
12	 Mar 19, 2002 ...	Tab 13 – Added system software information for TwinSpeed, CNV4, 9.0, and Octane2 10.0. Added SCIM/Keyboard parts information. Updated 18 inch monitor and LCD display monitor part numbers. Revised Octane computer information by updating existing Octane 225MHz & 270MHz system parts (MRlge72954) and adding Octane2 parts. Updated network hub information. Added Granite SCSI box. Tab 15 – Added Control Board (MRlge73502), TVSS Module, & motor/fan information. Updated module part numbers. Tab 16 – Corrected SSM part number (MRlge73082) and added circuit breaker (MRlge67275). Updated other module part numbers.

CONTINUED ON NEXT PAGE

REVISION HISTORY (Continued)

REV	DATE	PRIMARY REASON FOR CHANGE
13	Apr 18, 2003	Changed title of manual to <i>Signa Illustrated Parts List</i> . All pages have been updated with new headers. Tab 1 – Updated all existing M-cats and related structures. Added ACGD, EXCITE, and TwinSpeed catalogs. Updated gradient coils and RF coils with FRU information. Tab 2 – Updated all structures and added TwinSpeed and INFINITY structures. Tab 3 – Updated all parts lists and added WideOpen and INFINITY parts lists. Tab 4 – Updated all parts lists and added TwinSpeed and EXCITE information. Tab 5 – Updated pages with new headers. Tab 6 – Added Full-size PDU cabinets which were used on WideOpen upgrades. Tab 7 – Updated pages with new headers. Tab 8 – Updated all System cabinet structures and added EXCITE System cabinet illustrations and part lists. Tab 9 – Updated pages with new headers. Tab 10 – Updated pages with new headers. Tab 11 – Updated existing Option catalogs and added new ones including Brainwave, APA, EXCITE, and others. Tab 12 – Updated pages with new headers. Tab 13 – Updated all structures as needed. Added Octane II and EXCITE part lists. Tab 14 – Updated pages with new headers. Tab 15 – Updated section with more parts lists and illustrations. Tab 16 – Updated section with more parts lists and illustrations. Added Tab 17, TAC Cabinet, and related illustrations and parts lists.
14	Mar 22, 2004	Tab 1 – Corrected Head Coil Mirror replacement note for ordering of parts (Resolved MRlge89662, 90111, 90553, and 91137). Tab 13 – Changed part # for Indigo zytec power supply (MRlhc03789) Deleted Octane dual processor module, 2169940–20 (MRlge77333)

LIST OF EFFECTIVE PAGES

PAGE	REV	PAGE	REV	PAGE	REV	PAGE	REV	PAGE	REV
Title Page	13	2-1 to 2-346	13	TAB 7 COMPUTER		10-1 to 10-18	13	13-30	14
Damage in Trans.	—	TAB 3 PATIENT TABLE		MR238	—	TAB 11		13-31 to 13-36	13
Direction 2128126	1*	MR233	—	7-1 to 7-8	13	ACCESSORIES AND		TAB 14 RF/PDU	
A to B	13	3-1 to 3-44	13	TAB 8 SYSTEM		OPTIONS		CABINET	
i to x	13	TAB 4 PENETRATION		CABINET		MR241	—	2207068	—
TAB 1 SYSTEM		PANEL		MR238	—	11-1 to 11-116	13	14-1 to 14-15	13
MR231	—	2132238-100	—	8-1 to 8-100	13	TAB 12 GRAM		TAB 15 ACGD/PDU	
1-1 to 1-83	13	4-1 to 4-26	13	TAB 9 GRADIENT		2132240-100	—	CABINET	
1-84	14	TAB 5 CONSOLES		CABINET		12-1 to 12-9	13	2285569	—
1-85 to 1-86	13	MR235	—	MR239	—	TAB 13 OPERATOR		15-1 to 15-10	13
1-87	14	5-1 to 5-20	13	9-1 to 9-22	13	WORKSPACE		TAB 16 SRF CABINET	
1-88 to 1-219	13	TAB 6 POWER DIST.		TAB 10 RF/PEN		13-11	14	2285570	—
TAB 2 MAGNET		UNIT		CABINET		13-12 to 13-27	13	16-1 and 16-14	13
ENCLOSURE		MR236	—	2132239-100	—	13-28	14	TAB 17 TAC CABINET	
MR232	—	6-1 to 6-33	13			13-29	13	2308172	—
								17-1 and 17-5	13

* This revision number/letter corresponds to the indicated document's revision control system.

TABLE OF CONTENTS

SIGNA 5.x, 8.x, 9.x, AND 10.x CATALOG STRUCTURE


The contents of this Direction include assemblies and parts that were delivered with Signa Release 5.x, 8.x, 9.x, or 10.x manufactured systems. For those systems which are modified to a Signa Upgrade configuration, refer to *Direction 15020, Signa Renewal Parts, Direction 15304, Signa Advantage Renewal Parts*, or MR Service Methods CD-ROM 2124201-3 (5.x) or 2160623-3 (LX) for *Direction 15404, Signa Advantage 1.5T, 1.0T, & 0.5T Renewal Parts*. These manuals/CD-ROMs identify those parts used on a system upgraded to a latest version Signa System that are different than a manufactured system.

SECTION


PAGE

Section 1 SIGNA HORIZON 5.x & 8.x SYSTEMS


Includes M-catalogs, most cables, and the following:




Head Coil
and Adapters



Body Coils



Phantoms & Holders

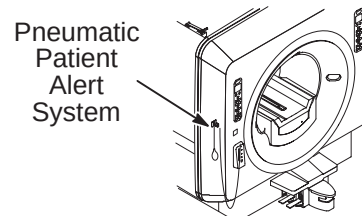


Pneumatic
Patient
Alert
System

1-1	5.x SYSTEM CATALOGS	1-3
	Contains information on Horizon 5.x systems using S-series magnet	
1-2	8.x SYSTEM CATALOGS	1-10
	Contains information on Horizon 8.x systems using S-series magnet and Indigo computer	
1-3	LX SGD SYSTEM CATALOGS	1-16
	Contains information on Signa LX systems using S-series magnet with SGD gradients and Indigo computer	
1-4	LX SGD/OCTANE SYSTEM CATALOGS	1-21
	Contains information on Signa LX systems with Cx or LCC magnets with SGD gradients and Octane computer	
1-5	Cx LX SGD SYSTEM CATALOGS	1-24
	Contains information on Signa LX systems using Cx magnet	
1-6	LCC LX SGD SYSTEM CATALOGS	1-32
	Contains information on Signa LX systems using LCC magnet	
1-7	WideOpen LX SGD SYSTEM CATALOGS	1-39
	Contains information on Signa LX systems with WideOpen enclosure and SGD Gradients	
1-8	WideOpen ACGD SYSTEM CATALOGS	1-49
	Contains information on Signa LX systems with WideOpen enclosure and ACGD Gradients	
1-9	TwinSpeed ACGD SYSTEM CATALOGS	1-64
	Contains information on Signa LX systems with TwinSpeed enclosure and ACGD Gradients	
1-10	MOBILE AND T/R COLLECTORS	1-72
	Contains information on parts for Mobile and T/R installations	
1-11	SYSTEM ACCESSORIES AND PHANTOMS	1-73
	Contains information on phantoms, pads, ECG, PPG, Coil Adapters, Head Coils, Patient Alert systems	
1-12	WideOpen ENCLOSURES	1-94
	Contains information on WideOpen enclosures and Body Coil mounting kit	

TABLE OF CONTENTS (CONT'D)

SECTION	PAGE
1-13 BODY COILS	1-111
Contains information on Gradient and RF Body Coils and replacement coils	
1-14 SYSTEM COMPUTER AND CABINET COLLECTORS	1-134
Contains information on collectors with Indigo or Octane computers and System, RF, and ACGD/PDU cabinets	
1-15 SYSTEM CABINET OPTIONS	1-146
Contains information on Reconstruction Processor options for System cabinet	
1-16 OPERATOR WORKSPACE CATALOGS	1-148
Contains information on DASM's, Keyboards, Monitors, Table, and SOI long cables	
1-17 PDU CATALOGS	1-152
Contains information on Compact PDU's	
1-18 MAGNET MONITOR AND MODEM	1-153
Contains information on Magnet Monitor equipment and cables, and Modem kits	
1-19 SYSTEM CABLE COLLECTORS	1-158
Contains information on system cables, hoses, and heat exchanger	
1-20 PDU CABLES	1-198
Contains information on PDU cables for all systems	
1-21 RF AND HELIAX CABLES	1-206
Contains information on RF and Helix cables, and Penetration Panel adapters	
1-22 GRADIENT CABLES	1-212
Contains information on Gradient and GRAM cables for all systems	
1-23 FIBER OPTIC CABLES	1-215
Contains information on Fiber Optic cables for all systems	

Section 2 MAGNET ENCLOSURE

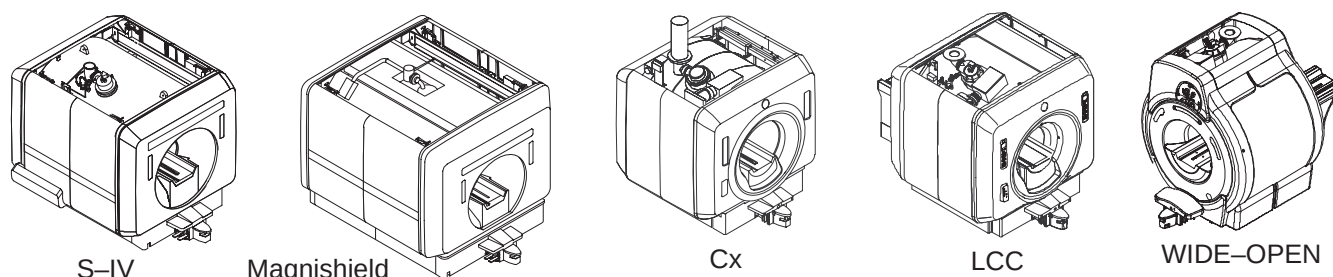

2-1 S-SERIES MAGNET ENCLOSURES	2-5
Contains information on Fixed, T/R, and Mobile enclosures for non-Magnishield magnet enclosures	
1.5T FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2118422-3 2-7
1.5T FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2118422-5 2-9
1.0T FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2118422-7 2-11
1.0T FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2118422-9 2-13
1.5T MOBILE & T/R MAGNET ENCLOSURE w/o MULTICOIL	2118422-2 2-28
1.5T MOBILE & T/R MAGNET ENCLOSURE with MULTICOIL	2118422-4 2-30
1.0T MOBILE & T/R MAGNET ENCLOSURE w/o MULTICOIL	2118422-6 2-32
1.0T MOBILE & T/R MAGNET ENCLOSURE with MULTICOIL	2118422-8 2-34


TABLE OF CONTENTS (CONT'D)

<u>SECTION</u>	<u>PAGE</u>
2-2 MAGNISHIELD MAGNET ENCLOSURES	2-65
Contains information on Magnishield magnet enclosures	
1.5T MAGNISHIELD ENCLOSURE w/o MULTICOIL	2118423 2-67
1.5T MAGNISHIELD ENCLOSURE with MULTICOIL	2118423-2 2-69
2-3 SRI AND PAC ASSEMBLIES	2-96
2-4 BLOWER CABINETS	2-100
2-5 S-SERIES AND MAGNISHIELD REAR PEDESTALS	2-105
2-6 BODY HYBRID SPLITTER ASSEMBLIES	2-128
2-7 STANDARD AND MAGNISHIELD BRIDGES WITH CARRIAGE ASSEMBLIES	2-130
2-8 BRM INSTALLATION KIT FOR S-SERIES MAGNETS	2-153
2-9 Cx HORIZON MAGNET ENCLOSURES	2-154
Contains information on Cx Fixed and Mobile magnet enclosures	
1.0T Cx FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2142000 2-155
1.0T Cx FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2142000-2 2-155
1.0T Cx MOBILE MAGNET ENCLOSURE w/o MULTICOIL	2142000-3 2-156
1.0T Cx MOBILE MAGNET ENCLOSURE with MULTICOIL	2142000-4 2-156
1.5T Cx FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2142000-5 2-157
1.5T Cx FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2142000-6 2-157
1.5T Cx MOBILE MAGNET ENCLOSURE w/o MULTICOIL	2142000-7 2-158
1.5T Cx MOBILE MAGNET ENCLOSURE with MULTICOIL	2142000-8 2-158
1.5T Cx CRM FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2142000-9 2-158
2-10 LCC HORIZON MAGNET ENCLOSURES	2-173
Contains information on LCC Horizon Fixed and Mobile magnet enclosures	
1.0T LCC FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2142000-11 2-174
1.0T LCC FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2142000-12 2-174
1.5T LCC FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2142000-13 2-175
1.5T LCC FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2142000-14 2-175
1.0T LCC MOBILE MAGNET ENCLOSURE w/o MULTICOIL	2142000-15 2-176
1.0T LCC MOBILE MAGNET ENCLOSURE with MULTICOIL	2142000-16 2-176
1.5T LCC MOBILE MAGNET ENCLOSURE w/o MULTICOIL	2142000-17 2-177
1.5T LCC MOBILE MAGNET ENCLOSURE with MULTICOIL	2142000-18 2-177
1.5T LCC CVMR FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2142000-19 2-178
LCC MOBILE MAGNET FRAME KIT	2204359 2-191
LCC FIXED SITE MAGNET FRAME KIT	2204359-2 2-192
2-11 Cx AND LCC HORIZON BRIDGE AND CARRIAGE ASSEMBLIES	2-193
2-12 Cx AND LCC HORIZON BRIDGE AND LOW PROFILE CARRIAGE COVER (LPCC) ASSEMBLIES	2-205
2-13 Cx AND LCC HORIZON REAR PEDESTALS	2-220
2-14 Cx AND LCC HORIZON ENCLOSURE COVERS, END BELLS, AND BORE LAMP	2-229
2-15 Cx AND LCC HORIZON DOCK ASSEMBLY	2-243

TABLE OF CONTENTS (CONT'D)

SECTION	PAGE
2-16 WideOpen MAGNET ENCLOSURES	2-246
Contains information on WideOpen Fixed and Mobile magnet enclosures	
1.0T WideOpen FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2202900 2-247
1.0T WideOpen FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2202900-2 2-247
1.0T WideOpen MOBILE MAGNET ENCLOSURE w/o MULTICOIL	2202900-3 2-247
1.5T WideOpen MOBILE MAGNET ENCLOSURE with MULTICOIL	2202900-4 2-248
1.0T WideOpen FIXED SITE MAGNET ENCLOSURE w/o MULTICOIL	2202900-5 2-248
1.0T WideOpen FIXED SITE MAGNET ENCLOSURE with MULTICOIL	2202900-6 2-248
1.5T WideOpen MOBILE MAGNET ENCLOSURE w/o MULTICOIL	2202900-7 2-249
1.5T WideOpen MOBILE MAGNET ENCLOSURE with MULTICOIL	2202900-8 2-249
1.5T WideOpen CARDIAC FIXED SITE MAGNET ENCLOSURE w/MULTICOIL	2202900-9 2-249
2-17 WideOpen ENCLOSURE COVERS AND END BELLS FOR LONG BRIDGE	2-260
2-18 WideOpen CARDIAC ENCLOSURE COVERS AND END BELLS FOR LONG BRIDGE	2-272
2-19 WideOpen LONG BRIDGE AND CARRIAGE ASSEMBLIES	2-280
2-20 WideOpen ENCLOSURE COVERS AND END BELLS WITH SPLIT BRIDGE	2-287
2-21 WideOpen REAR PEDESTALS	2-313
2-22 WideOpen DOCK ASSEMBLIES	2-327
2-23 TwinSpeed ENCLOSURE COVERS AND END BELLS WITH SPLIT BRIDGE	2-332
Contains information on INFINITY TwinSpeed Fixed, T/R, and Mobile magnet enclosures	
INFINITY TwinSpeed FIXED AND T/R MAGNET ENCLOSURE	2297122 2-337
INFINITY TwinSpeed MOBILE MAGNET ENCLOSURE	2297122-2 2-339

Section 3 PATIENT TABLE




Lightweight
Patient Transport

3-1 HORIZON PATIENT TABLE	46-265300G1 ... 3-3
Contains information on Patient Table with original colors	
3-2 WideOpen PATIENT TABLE	46-265300G2 ... 3-3
Contains information on Patient Table with WideOpen colors	
3-3 INFINITY PATIENT TABLE	46-265300G3 ... 3-3
Contains information on Patient Table with INFINITY colors	
HORIZON TABLE/BASE ASSEMBLY	2135993 3-5
WideOpen TABLE/BASE ASSEMBLY	2135993-2 3-6
INFINITY TABLE/BASE ASSEMBLY	2135993-3 3-7
HORIZON TABLE BASE KIT	2127700 3-14
WideOpen TABLE BASE KIT	2127700-2 3-17
INFINITY TABLE BASE KIT	2127700-3 3-20
HYDRAULIC PUMP ASSEMBLY	46-265779G1 ... 3-23
HYDRAULIC CYLINDER ASM	46-265780G1 ... 3-24
HYDRAULIC CYLINDER ASM	2323995 3-24

TABLE OF CONTENTS (CONT'D)

<u>SECTION</u>	<u>PAGE</u>
TABLE TOP	2135992 3-30
TABLE TOP – INFINITY	2135992-2 3-32
TABLE TOP ASSEMBLY	46-265991G1 ... 3-33
TABLE LATCH ASSEMBLY	46-317191G1 ... 3-34
DETACHABLE, TELESCOPING IV SUPPORT	46-271551G1 ... 3-35
ARMBOARD ASSEMBLY	46-271012G1 ... 3-37
ARMBOARD ASSEMBLY – INFINITY	46-271012G2 ... 3-37
CRADLE ASSEMBLY w/TWIST TO RELEASE	46-301222G1 ... 3-39
FRONT SECTION ASSEMBLY	46-301543G1 ... 3-40
MID SECTION ASSEMBLY	46-301544G1 ... 3-40
HORIZON TABLE COVER KIT	2127699 3-41
WideOpen TABLE COVER KIT	2127699-2 3-41
INFINITY TABLE COVER KIT	2127699-3 3-41
OUTER COVER FOR MRTBL2	2145822 3-42
OUTER COVER FOR MRTBL2 – WideOpen	2145822-2 3-43
OUTER COVER FOR MRTBL2 – INFINITY	2145823 3-44

Section 4 PENETRATION CABINET/PANEL

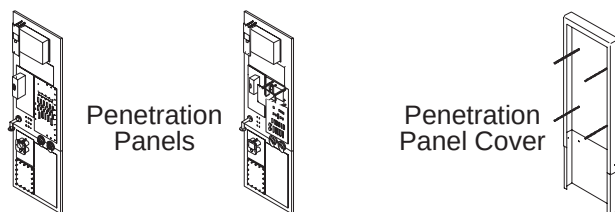

4-1 PENETRATION PANELS	3-3
Contains information on non-EXCITE, EXCITE, and TwinSpeed Penetration Panels	
PENETRATION PANEL w/o MULTICOIL	46-301383G12 .. 4-3
PENETRATION PANEL w/o MULTICOIL	46-301383G18 .. 4-4
PENETRATION PANEL w/MULTICOIL	46-301383G13 .. 4-6
PENETRATION PANEL w/MULTICOIL	46-301383G19 .. 4-7
EXCITE PENETRATION PANEL w/MULTICOIL	46-301383G22 .. 4-9
TwinSpeed PENETRATION PANEL w/MULTICOIL	46-301383G17 .. 4-11
TwinSpeed EXCITE PENETRATION PANEL w/MULTICOIL	46-301383G21 .. 4-13
4-2 PENETRATION PANEL COVERS	4-26
Contains information on Fixed, T/R, and Mobile covers	
PENETRATION PANEL COVER – FIXED	46-317126G3 ... 4-26
PENETRATION PANEL COVER – MOBILE & T/R	46-317126G4 ... 4-26

TABLE OF CONTENTS (CONT'D)



SECTION	PAGE
Section 5 CONSOLES	
 Operator Console	
 Low and High Profile Kits	
3-1 HORIZON OPERATOR CONSOLE	3-3
Contains information on Horizon 5.x Operator Console	
EMC OPERATOR CONSOLE	2119590 5-4
LOW PROFILE KIT	46-287997G1 ... 5-19
HI PROFILE KIT	46-287998G1 ... 5-20
Section 6 POWER DISTRIBUTION UNIT	
 Compact PDU	
 Full-Size PDU	
6-1 COMPACT PDU	6-2
Contains information on Horizon 5.x and LX Compact PDU	
5.x 60Hz 480V REGULATED & FILTERED	46-317099P10 .. 6-4
5.x 50/60Hz 380/400/415V REGULATED & FILTERED	46-317099P11 .. 6-8
LX COMPACT PDU – 60Hz 480V REGULATED & FILTERED	46-317099P20 .. 6-12
LX COMPACT PDU – 50/60Hz 380/400/415V REGULATED & FILTERED	46-317099P21 .. 6-16
6-2 FULL-SIZE PDU	6-18
Contains information on Horizon 5.x and LX Full-size PDU	
FULL-SIZE PDU	46-282368G3 ... 6-20
FULL-SIZE PDU UPGRADE TO LX	46-306985G4 ... 6-33
FULL-SIZE PDU UPGRADE TO WideOpen	2246052 6-33
Section 7 COMPUTER	
 Stealth Computer	
7-1 STEALTH COMPUTER	7-2
Contains information on Horizon 5.x Computer	
7-2 STEALTH COMPUTER INTERFACE KIT	7-8

TABLE OF CONTENTS (CONT'D)




<u>SECTION</u>		<u>PAGE</u>
Section 8	SYSTEM CABINET	
	 5.x System Cabinet	
	 8.x System Cabinet	
	 EXCITE System Cabinet	
8-1	HORIZON 5.x SYSTEM CABINETS	8-3
	Contains information on Horizon 5.x various System Cabinet configurations	
	5.x 1.5T ECHOSPEED with MULTI-COIL & FAST RECEIVER	2117956 8-4
	5.x 1.5T HISPEED with MULTI-COIL & w/o FAST RECEIVER	2117958 8-7
	5.x 1.0T HISPEED with MULTI-COIL & w/o FAST RECEIVER	2117958-2 8-9
	5.x 1.5T ECHOSPEED with FAST RECEIVER & w/o MULTI-COIL	2117960 8-12
	5.x 1.5T w/o MULTI-COIL or FAST RECEIVER	2117962 8-15
	5.x 1.0T w/o MULTI-COIL or FAST RECEIVER	2117962-2 8-17
8-2	HORIZON LX SYSTEM CABINETS	8-50
	Contains information on Horizon 5.x various System Cabinet configurations	
	LX 1.5T with MULTI-COIL & FAST RECEIVER	2138300-2 8-51
	LX 1.5T with MULTI-COIL & w/o FAST RECEIVER	2138300-3 8-53
	LX 1.5T w/o MULTI-COIL or FAST RECEIVER	2138300-4 8-55
	LX 1.0T w/o MULTI-COIL	2138300-6 8-57
	LX 1.0T with MULTI-COIL	2138300-9 8-59
	LX 1.5T CRM with MULTI-COIL & FAST RECEIVER	2138300-16 8-61
	LX 1.5T EchoSpeed with MULTI-COIL & FAST RECEIVER	2138300-19 8-63
	LX 1.5T BASE & HiSpeed with MULTI-COIL	2138300-20 8-65
	LX 1.5T BASE w/o MULTI-COIL	2138300-21 8-67
	LX 1.0T BASE & HiSpeed with MULTI-COIL	2138300-23 8-70
8-3	EXCITE SYSTEM CABINET	8-89
	EXCITE 1.5T SYSTEM CABINET	2294302 8-90

TABLE OF CONTENTS (CONT'D)

SECTION


PAGE

Section 9 GRADIENT CABINET

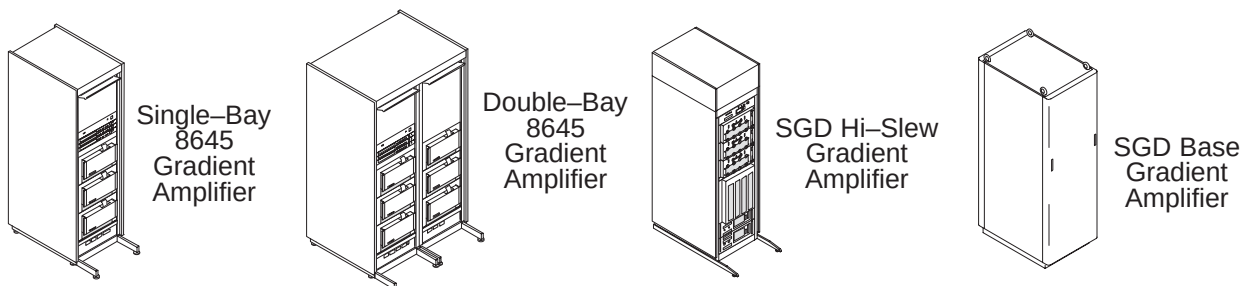

9-1 HORIZON 8645 GRADIENT CABINETS	9-2
Contains information on Horizon single and double bay 8645 Gradient Cabinet configurations	
SINGLE-BAY 8645 GRADIENT CABINET	2108800 9-2
DOUBLE-BAY 8645 GRADIENT CABINET	2108800-2 9-7
9-2 SGD GRADIENT CABINETS	9-12
Contains information on Hi-Slew and Base SGD Gradient Cabinets	
SGD HI-SLEW GRADIENT CABINET	2169944 9-13
SGD BASE GRADIENT CABINET	2172035 9-20

Section 10 RF AMPLIFIER CABINET

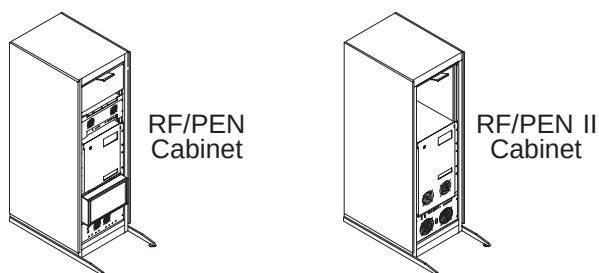

10-1 RF/PENETRATION CABINET	10-2
1.5T RF/PENETRATION CABINET	2109930 10-4
1.0T RF/PENETRATION CABINET	2109930-2 10-8
10-2 RF/PENETRATION II CABINET	10-14
1.5T RF/PENETRATION II CABINET	2160200 10-17
1.0T RF/PENETRATION II CABINET	2160200-3 10-18

Section 11 ACCESSORIES AND OPTIONS

Section includes Surface Coils, Pads and Holders, Multi-coil Options, Software Keys Computer Options, Laser Cameras, E-catalogs, and R-catalogs

11-1 SIGNA OPTION CATALOGS	11-7
11-2 ACCESSORY PACKAGES	11-110
11-3 FACILITY OPTIONS	11-116

TABLE OF CONTENTS (CONT'D)











<u>SECTION</u>	<u>PAGE</u>
Section 12 GRAM CABINET	
	
12-1 GRAM CABINET	12-2
Contains information on GRAM Cabinet	
Section 13 OPERATOR WORKSPACE	
	
	
	
	
13-1 INDIGO COMPUTER	13-2
Contains information on Indigo Computer, Cabinet and related components	
INDIGO OPERATOR WORKSPACE TABLE COMPONENTS – BLACK & WHITE MONITOR	13-2
INDIGO OPERATOR WORKSPACE TABLE COMPONENTS – COLOR MONITOR	13-2
INDIGO OPERATOR WORKSPACE CABINET	13-6
13-2 OCTANE COMPUTER	13-14
Contains information on Octane and Octane II Computers, Cabinets and related components	
OCTANE OPERATOR WORKSPACE TABLE COMPONENTS	13-14
OCTANE OPERATOR WORKSPACE CABINET	13-15
Section 14 RF/PDU CABINET	
	
14-1 1.0T RF/PDU CABINET	14-2
Contains information on 1.0T RF/PDU Cabinet	
14-2 1.5T RF/PDU CABINET	14-10
Contains information on 1.5T RF/PDU Cabinet	

TABLE OF CONTENTS (CONT'D)

SECTION	PAGE
Section 15 ACGD/PDU CABINET	
	
15-1 ACGD/PDU CABINET	15-2
Contains information on ACGD/PDU Cabinet	
ACGD/PDU CABINET	2284300 15-2
ACGD/PDU CABINET	2238915 15-4
Section 16 SRF CABINET	
  SRF Cabinet SRFD II Cabinet	
16-1 SRF CABINET	16-2
Contains information on Solid State RF Cabinets	
1.5T SRF CABINET	2296300 16-2
1.0T SRF CABINET	2296300-2 16-2
1.5T SRF CABINET	2174500 16-4
1.0T SRF CABINET	2174500-2 16-7
16-2 SRFD II CABINET	16-9
Contains information on Solid State RF Cabinets	
1.5T SRFD II CABINET	2275000 16-11
Section 17 TAC CABINET	
 TAC Cabinet	
17-1 TAC CABINET	17-2
Contains information on TwinSpeed Accessory Cabinet (TAC)	
TAC CABINET	2239500 17-3