



**GE Medical Systems**

## Technical Publications

**Direction 2345481**

**Revision 13**

### Signa<sup>®</sup> EXCITE & EXCITE PLUS Field Replaceable Units (FRU)

Copyright © 2002 –2009 by General Electric Company, Inc.

All Rights Reserved



**GE Medical Systems**

GE Medical Systems: Telex 3797371  
P.O. Box 414, Milwaukee, Wisconsin 53201 U.S.A.  
(Asia, Pacific, Latin America, North America)

GE Medical Systems – Europe: Telex 261794  
Shortlands, Hammersmith, London W6 8BX U.K.



**COVER  
BOTTOM  
CROP LINE**

**COVER  
BOTTOM  
CROP LINE**

**5/16" RADIUS  
CORNER TRIM  
TYPICAL**



**COVER  
LEFT  
CROP LINE**

**COVER  
FOLD  
LINE** | **(2) CENTER STAPLES  
FOR BINDING**

**COVER  
RIGHT  
CROP LINE**



**5/16" RADIUS  
CORNER TRIM  
TYPICAL**

# INTRODUCTION TO FIELD REPLACEABLE UNIT (FRU)

This direction is a guide to the FRU's.

Parts designated as a FRU are critical to maintain the safety and/or functionality of the system. FRU's are available on a Priority 1 basis from Service Parts Operation.

As a reference aid, the FRU's are listed under an upper-level part number where they are used. In most cases the upper-level part number is not a FRU. In some cases the parts listed under an upper-level assembly may have been nested in intermediate sub-assemblies which are not shown.

Where possible, FRU's which are part of Option Catalogs are shown under the area where they would be installed, rather than being listed in the Coils or Options Sections (SEE TABLE OF CONTENTS).

## SEND COMMENTS ABOUT THIS MANUAL TO:

GE MEDICAL SYSTEMS  
MANAGER, SERVICE ENGINEERING, W-808  
3200 N. GRANDVIEW BLVD.  
WAUKESHA, WISCONSIN 53188  
USA

This manual belongs to:

---

---

---

## REVISION HISTORY

### REV DATE REASON FOR CHANGE

|    |             |                                                                                                                                                                                                                                                                                                                                               |
|----|-------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 0  | Jul 19, '02 | Initial release                                                                                                                                                                                                                                                                                                                               |
| 1  | Oct 30, '02 | Corrected Touch-up Paint Numbers. Octane I & II – Corrected part numbers and added WARNING message. Added SRFD II Cabinet. General part & format changes throughout to match current production.                                                                                                                                              |
| 2  | Aug 1, '03  | Changed title of manual from <i>10.x MGD</i> to <i>EXCITE I &amp; EXCITE II</i> . Added EXCITE II product to Operator Workspace, System Cabinet, Coils, and Options. Added (4) LPCA FRUs. Updated Octane I & II section.                                                                                                                      |
| 3  | Oct 1, 03   | Added additional EXCITE II parts for Enclosure, System Cabinet, Coils, and added EXCITE II Options                                                                                                                                                                                                                                            |
| 4  | Jan 18, 04  | Added AirSys chillers and other chiller parts. Added ReportCARD Hardware FRU's.                                                                                                                                                                                                                                                               |
| 5  | Jan 27, 04  | Added LPCC parts (MRIge83842). Added Lytron Chiller parts (MRIge90211). Corrected System Cabinet option names (MRige90403). Added 1.5T 8 Ch NV Array Coil (MRIge90388).                                                                                                                                                                       |
| 6  | Jan 10, 05  | Added cable replacement information. Revised Service. Tools and Options. Added GOC AA to OW. Added 2nd TAC. Added BrainWave parts. Corrected part information per CQA's.                                                                                                                                                                      |
| 7  | Mar 18, 05  | Added cable Run 1035 FRU. Corrected Host monitor and SCSI tower part numbers. Added vacuum upgrade kit to TAC.                                                                                                                                                                                                                                |
| 8  | Dec 30, 05  | Added SRI parts. Updated OW monitor info. Updated RRF module part #'s.                                                                                                                                                                                                                                                                        |
| 9  | Jan 19, 07  | Added RF Shield Change Out Kit, Speaker Grill nylon screw, LPCA Wheel Housing FRU kit (MRIhc21559), & Dock pedal FRU parts (MRIhc17629). Updated SRI/PAC FRU's (MRIhc19214). Added Patient Table FRU's. Updated Host monitor FRU. Removed all OW Octane parts. For System cabinet, added RRF Module MUX2 board and Term Server cable FRU kit. |
| 10 | Jun 15, 07  | Added LPCA LED harness (CQA 13099758). Updated ACGD SGA power supply from 2272460–2 to 2317092–2.                                                                                                                                                                                                                                             |
| 11 | May 28, 08  | Changed name of manual to <i>Signa EXCITE &amp; EXCITE Plus FRU's</i> . Added Ground Strap kit part #. Rear Pedestal: Updated Longitudinal Encoder part number (PQR 13175398) and added Encoder board part # 46–226552G2. Chiller: Added E & W mobile Heat Exchanger part #'s (PQR13133952). Added Lytron pump coupler part # (PQR 13136000). |
| 12 | Jun 15, 09  | Added Flexible Coupling (PQR 13206931). Updated Monitor offerings on OW (PCN 290188). Removed DVD–RW kit from OW (PQR 13247342). Also added HP8400 73Gb HDD (ECR 2079589), HP8400 DIMM (ECR 2038518). In RRF Chassis, added 5250028–2 RF–DIF (ECO 2080729).                                                                                   |
| 13 | Nov 3, 09   | Added new GOC AA 2395043–2 (ECO 2084000) and OW cable FRU (ECO 2076722).                                                                                                                                                                                                                                                                      |

## LIST OF EFFECTIVE PAGES

| <u>PAGE</u> | <u>REV</u> | <u>PAGE</u> | <u>REV</u> | <u>PAGE</u> | <u>REV</u> |
|-------------|------------|-------------|------------|-------------|------------|
| Cover Page  | . 13       | 8 to 14     | ..... 11   | 17 to 25    | .... 11    |
| 1 to 2      | ..... 13   | 15          | ..... 12   | 26          | ..... 12   |
| 3 to 6      | ..... 11   | 16          | ..... 13   | 27 to 40    | .... 11    |
| 7           | ..... 12   |             |            |             |            |

## INTRODUCTION

| <b>TITLE</b>                                                            | <b>PAGE</b>             |
|-------------------------------------------------------------------------|-------------------------|
| <b>INTRODUCTION TO FIELD REPLACEABLE UNIT(FRU) . . . . .</b>            | <b>1</b>                |
| <b>MAGNET AND ENCLOSURE (ASSEMBLIES) . . . . 4, 5, 6, 7, 8, &amp; 9</b> |                         |
| BRM & TRM LIST (OF PARTS NOT SHOWN) . . . . .                           | 4                       |
| FRONT COSMETIC COVER & PARTS (BACK VIEW) . . . . .                      | 5                       |
| MAGNET DOCKING PARTS . . . . .                                          | 5                       |
| ENCLOSURE & VACUUM RELATED . . . . .                                    | 6                       |
| FRONT & REAR ENDBELL . . . . .                                          | 6                       |
| COIL ASSEMBLY & BRIDGE SUPPORT . . . . .                                | 6                       |
| REAR PEDESTAL PARTS . . . . .                                           | 7                       |
| COIL ADAPTERS . . . . .                                                 | 7                       |
| SRI/PAC . . . . .                                                       | 7                       |
| LOW PROFILE CARRIAGE COVER . . . . .                                    | 8                       |
| BRIDGE . . . . .                                                        | 8                       |
| TOUCH-UP PAINTS . . . . .                                               | 9                       |
| <b>PATIENT SUPPORT TABLE . . . . .</b>                                  | <b>10</b>               |
| <b>CHILLER . . . . .</b>                                                | <b>12</b>               |
| <b>PENETRATION PANEL . . . . .</b>                                      | <b>13</b>               |
| <b>OPERATOR WORKSPACE – EXCITE II . . . . .</b>                         | <b>15</b>               |
| <b>OPERATOR WORKSPACE COMPUTER CABINET – LINUX . . . . .</b>            | <b>16</b>               |
| <b>WORKSPACE SCIM AND KEYBOARDS . . . . .</b>                           | <b>17</b>               |
| <b>MAIN DISCONNECT PANEL . . . . .</b>                                  | <b>18</b>               |
| <b>SRF CABINET . . . . .</b>                                            | <b>20</b>               |
| <b>SRFD II CABINET . . . . .</b>                                        | <b>21</b>               |
| <b>ACGD/PDU CABINET . . . . .</b>                                       | <b>22</b>               |
| <b>ACGD-Lite CABINET . . . . .</b>                                      | <b>23</b>               |
| <b>SYSTEM CONTROL CABINET . . . . .</b>                                 | <b>24, 25, &amp; 26</b> |
| <b>ACCESSORY CABINET (TWIN<i>SPEED</i> ONLY) . . . . .</b>              | <b>28, 29, &amp; 30</b> |
| <b>REPLACEMENT CABLES . . . . .</b>                                     | <b>31</b>               |
| <b>SERVICE TOOLS . . . . .</b>                                          | <b>32</b>               |
| <b>ACCESSORIES . . . . .</b>                                            | <b>33</b>               |
| <b>COILS . . . . .</b>                                                  | <b>34, 35 &amp; 36</b>  |
| <b>EXCITE OPTIONS . . . . .</b>                                         | <b>38</b>               |
| <b>EXCITE II OPTIONS . . . . .</b>                                      | <b>39</b>               |
| <b>BrainWave OPTIONS . . . . .</b>                                      | <b>40</b>               |






|               |                   |
|---------------|-------------------|
| INTRODUCTION  | PAGE 1            |
| CHILLER PARTS | PAGE 12           |
| CABLES        | PAGE 31           |
| ACCESSORIES   | PAGE 33           |
| COILS         | PAGE 34, 35, & 36 |
| OPTIONS       | PAGE 38, 39, & 40 |

**MAGNET ENCLOSURE:**

|                 |                  |
|-----------------|------------------|
| SUBASSEMBLIES   | PGS 5, 6, 7, & 8 |
| TOUCH-UP PAINTS | PAGE 9           |



SERVICE TOOLS  
PAGE 32

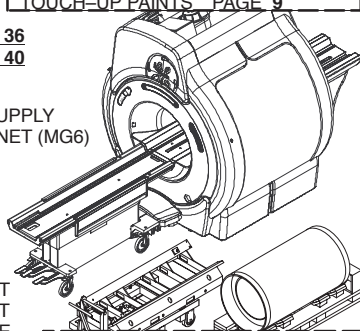**MAGNET ROOM****OPERATOR/EQUIPMENT ROOM****OR****OR****TABLE OF CONTENTS**

**NOTE: The following WideOpen & TwinSpeed common parts Not Shown:**

|           |                                               |
|-----------|-----------------------------------------------|
| 5123812   | BORE TEMPERATURE SENSOR, RUN 1260             |
| 5123813   | OPERATOR DISPLAY CABLE TO SRI-3, RUN 1261     |
| 5133997   | LIQ KIT, contains:                            |
|           | BRIDGE SUPPORT FOR LCC MAGNET ENCLOSURES      |
|           | BRIDGE SUPPORT FOR S-SERIES MAGNET ENCLOSURES |
|           | RADIAL SUPPORTS FOR ALL MAGNETS               |
| 5184777   | RF SHIELD GROUNDING KIT                       |
| 2324086-2 | 5 GALLON PAIL w/ETHYLENE GLYCOL WARNING LABEL |

**NOTE: The following BRM parts Not Shown:**

|            |                                                                                     |
|------------|-------------------------------------------------------------------------------------|
| 2297672    | GLYCOL, 1 GALLON/3.8 LITERS                                                         |
| 5113879*   | RF SHIELD FOR BRM COIL                                                              |
| 2124499-5  | GRAD COIL LCC ONE-PIECE SHIELD                                                      |
| 2144093-3  | BRM GRADIENT COIL W/CART & CRADLE (Cx & S-series)                                   |
| 2144093-5  | BRM-D GRADIENT COIL W/CART & CRADLE (LCC)                                           |
| 2241521    | SPLICE KIT GRADIENT COIL SPLICE KIT                                                 |
| 2208999-3  | SHORT RF COIL & CASE, Order for RF COIL Replacement (LCC)                           |
| 2208999-6  | LONG RF COIL & CASE, Order for RF COIL Replacement (Cx & S-series)                  |
| 2208999-10 | HDx new color SHORT RF COIL & Yellow/Black CASE (Order for RF COIL Replacement-LCC) |
| 5113879*   | RF SHIELD FOR BRM COIL                                                              |

**NOTE: The following TWIN LCC 1.5T FIXED W/TRM & Enclosure related parts Not Shown; MISCELLANEOUS:**



|             |                                          |
|-------------|------------------------------------------|
| 2297760     | VACUUM GREASE, MSDS# 8366442             |
| 2203803     | SPLIT O-RING                             |
| 2242756     | RELIEF VALVE, 3/8 NPT X 7 PSIG, GEN      |
| 2299843     | MAGNET PRESSURE TRANSDUCER, SUNX DP2-41N |
| 46-294231G1 | MAGNET RUNDOWN UNIT                      |
| 46-294231P1 | BUSSMAN, F1, 110VAC .400 GDC             |
| 46-264758G1 | REMOTE INTERCOM BOARD, MG3 A2 A1         |

**TRM:**

|           |                                              |
|-----------|----------------------------------------------|
| 2297672   | GLYCOL, 1 GALLON/3.8 LITERS                  |
| 5113878*  | RF SHIELD FOR TRM COIL                       |
| 5111938   | BORE TEMPERATURE SENSOR CABLE                |
| 2144093-7 | TRM WITH MOUNTING BRACKETS, CART, AND CRADLE |
| 2218148   | COLD SHRINK (FOR REAR ENDBELL AND TRM COIL)  |
| 2208999-8 | RF BODY COIL AND CASE                        |
| 2299498   | COOLING CIRCUIT REPAIR KIT                   |
| 2303520   | DIODE SLOT BOARD                             |
| 2293612   | MALE CONNECTOR 3/4" HOSE TO 3/4" NPT         |

\*2389049 RF Shield Change Out Kit – MUST be ordered for the RF Shield replacement

## 4 MAGNET AND ENCLOSURE (ASSEMBLIES)

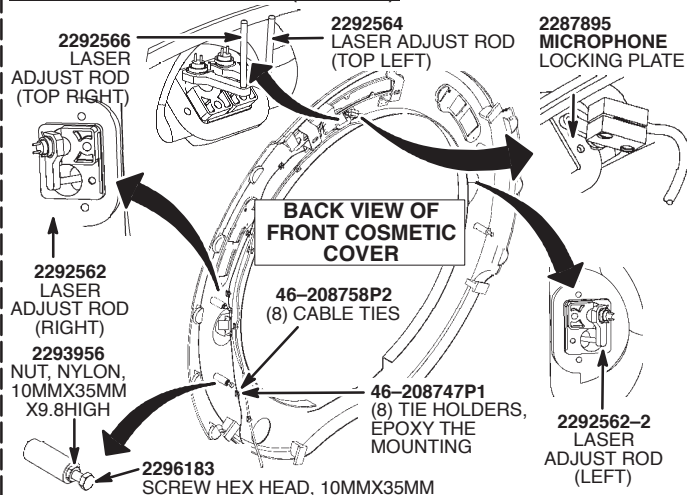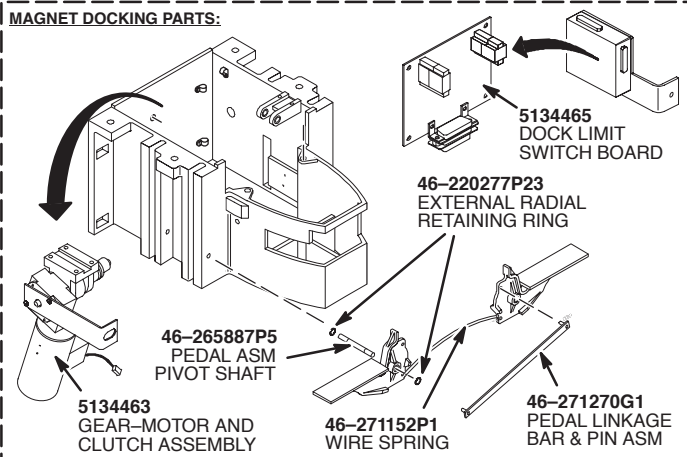**FRONT COSMETIC COVER & PARTS (BACK VIEW):****MAGNET DOCKING PARTS:****MAGNET AND ENCLOSURE (ASSEMBLIES)**


**ENCLOSURE & VACUUM RELATED PARTS:**

**2293323**  
O-RING BETWEEN ENDBELL  
AND ALUMINUM RING

**2293771**  
RADIAL SHIM SPACER, 1.5MM

**2293771-2**  
RADIAL SHIM SPACER, 0.8MM


**2241176**  
RUBBER ISOLATION PAD



**2246966**  
MAGNET  
RING  
GASKET

**FRONT ENDBELL PARTS:  
(TRM ONLY)**


**2295639** GASKET,  
O-RING, ENDBELL  
TO RF TUBE  
ACCESS **2294358**, 4MM  
PANELS **2294358-2**, 6MM



**2297761**  
O-RING, WATERLINE  
FEEDTHROUGH

**COIL ASSEMBLY:  
(TRM ONLY)**

**2131953-5**  
MOUNTING PAD,  
1/4 INCH THICK  
NEOPRENE



**2293535**  
SET SCREW,  
MOUNTING PAD


**BRIDGE SUPPORT PARTS:  
(TRM ONLY)**

**2293539**  
BRIDGE  
SUPPORT  
BUSHING

**2293956**  
NYLON HEX NUT  
M10 X 1.5MM  
X 9.5MM HIGH

**REAR ENDBELL ASSEMBLY  
(TRM ONLY)**

**2284170**  
REAR ENDBELL  
VACUUM ASSEMBLY;  
& **2218148**  
COLD SHRINK  
(FOR REAR ENDBELL &  
TRM COIL)  
& **2218149**  
COMPRESSION  
SPLICER  
(FOR REAR ENDBELL)

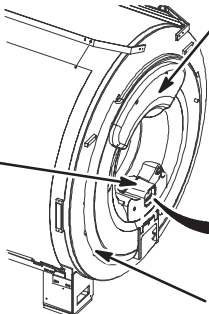

**2284175**  
COMFORT MODULE  
ASSEMBLY

**2206437**  
M4 X 12mm NYLON  
SCREW FOR  
SPEAKER GRILL

**GRADIENT GASKETS:  
(TRM ONLY)**

**2297540**  
(4MM)




**2297540-2**  
(6MM)

**2296182**  
REAR COSMETIC  
COVER ASSEMBLY

**NOTE:** The following parts are **Not Shown**.

**2297760** VACUUM GREASE, MSDS# 8366442

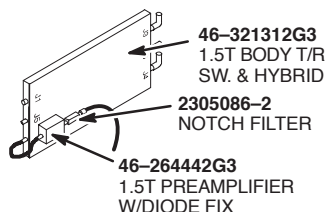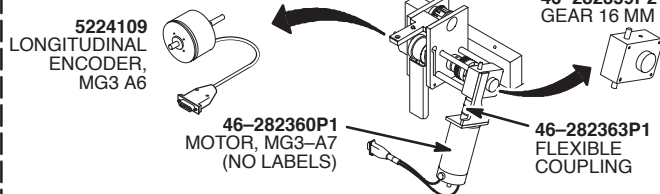

**1.5T SPLITTER BOX:****COIL ADAPTERS:****LONGITUDINAL MOTOR DRIVE PARTS:**


**NOTE:** The following REAR PEDESTAL AREA parts Not Shown:


2362995-2 8 CHANNEL SWITCH ASM - for EXCITE II

2305086-2 BODY RECEIVE IMAGE REJECT FILTER

5250136 REMOTE INTERCOM BOARD


6250012 ENCODER LIMIT SWITCH BOARD

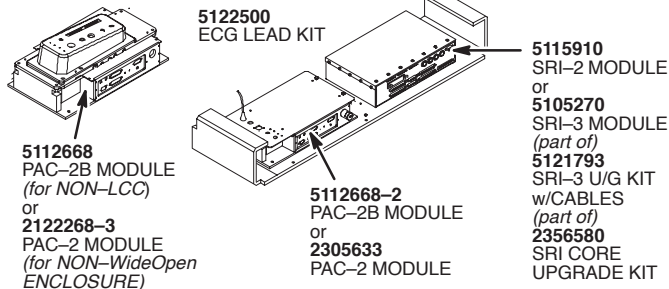**SRI/PAC:**

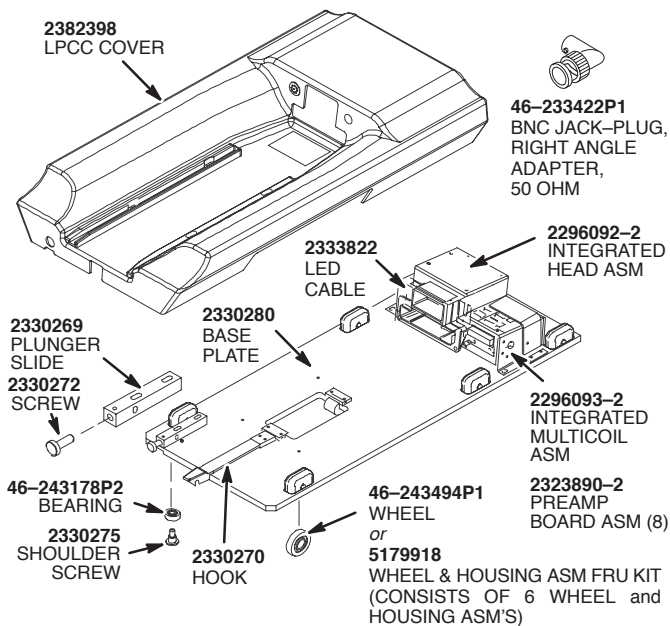**LOW PROFILE CARRIAGE COVER PARTS:**

**NOTE: The following part is Not Shown.**

**5114423-2** HEAD RECEIVE CABLE, RUN 1035

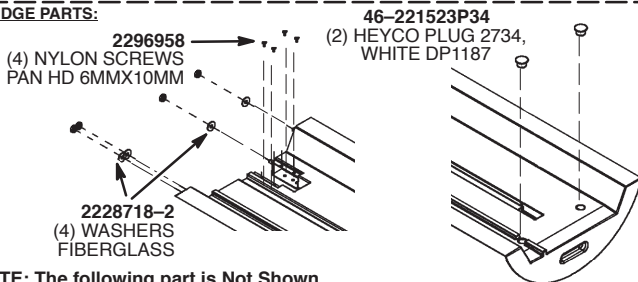
**BRIDGE PARTS:**


**NOTE: The following part is Not Shown.**

**2293538** BRIDGE EDGE FOAM

**TOUCH-UP PAINTS:**

|                    |                        |                            |
|--------------------|------------------------|----------------------------|
| <b>2183491-3</b>   | <b>GRAY #1</b>         | <b>0.6 OZ. NON-AEROSOL</b> |
| <b>46-303460P3</b> | <b>STEEL BLUE</b>      | <b>0.6 OZ. NON-AEROSOL</b> |
| <b>46-303460P4</b> | <b>DARK STEEL BLUE</b> | <b>0.6 OZ. NON-AEROSOL</b> |

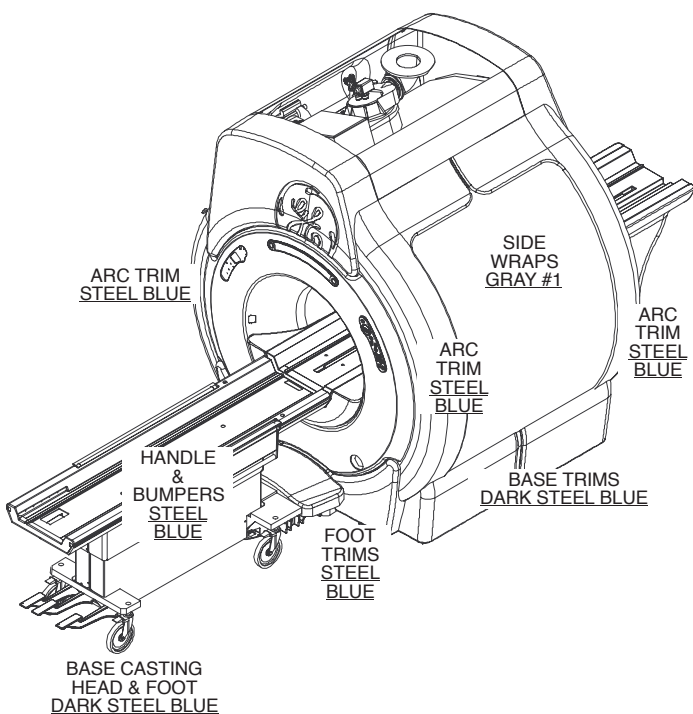**MAGNET AND ENCLOSURE**

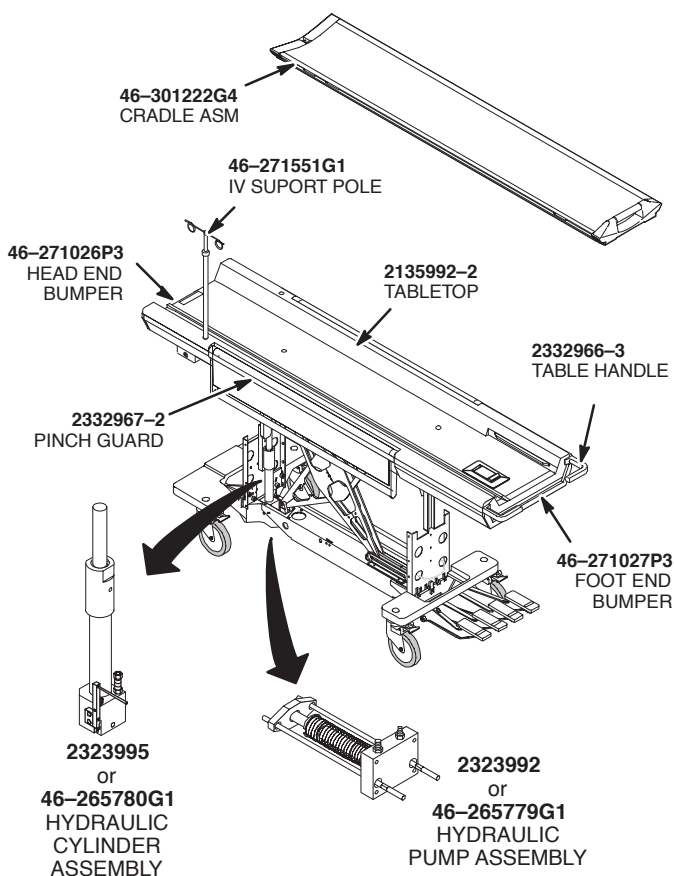
**PATIENT TABLE**

[illegible]

**SYSTEM COOLING CABINETS:**

REFER TO ELLIS & WATTS SERVICE  
MANUALS FOR FRU INFORMATION

REFER TO AIRSYS  
SERVICE MANUALS  
FOR FRU INFORMATION

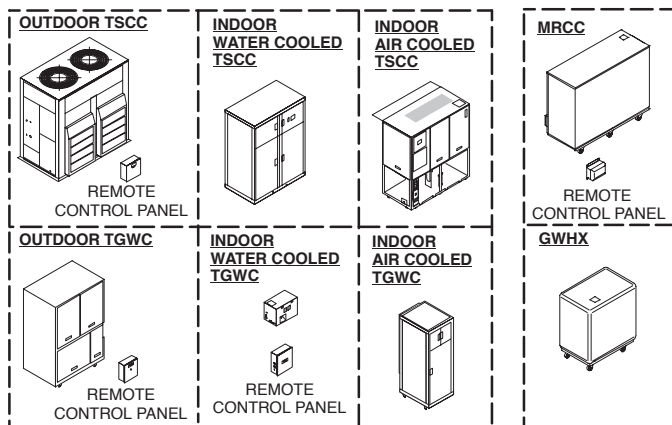

2343325 AIRSYS HEAT EXCHANGER (GWHX)

2341077-2 AIRSYS QUICK DISCONNECT KIT

2341077-3 AIRSYS REMOTE CONTROL PANEL

2230235 E & W MODEL LTL-4 MOBILE HEAT EXCHANGER

2230235-3 E & W PUMP/MOTOR SET

2230235-12 E & W LEVEL SWITCH

2230235-24 QUICK-DISCONNECT FACILITY

2230235-25 QUICK-DISCONNECT COIL

2298100-4 E & W MODEL LTL10 HEAT EXCHANGER CABINET

2298100-5 CONTROL PANEL FOR LTL10 ONLY

2297672 GLYCOL USED WITH E & W OR AIRSYS

**NOTE: The following parts are Not Shown.**

2222564-22 LYTRON CHILLER, 50Hz OR 60Hz

2222564-23 LYTRON CIRCUIT BREAKER

2222564-24 LYTRON PUMP

2222564-25 LYTRON MOTOR

2222564-26 LYTRON KEY PAD


2222564-27 LYTRON FLOW SWITCH

2222564-28 LYTRON HOSE FITTINGS

2222564-29 LYTRON PUMP with NYLON COUPLING


2222564-31 LYTRON NYLON MOTOR COUPLING


2260427 COOLANT (1 GALLON) (LYTRON ONLY)

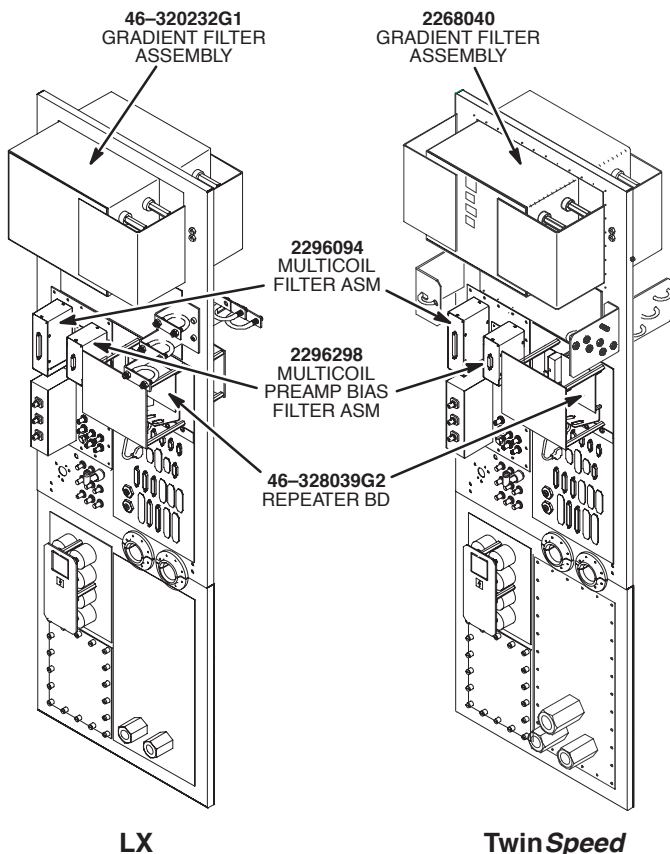

[illegible]

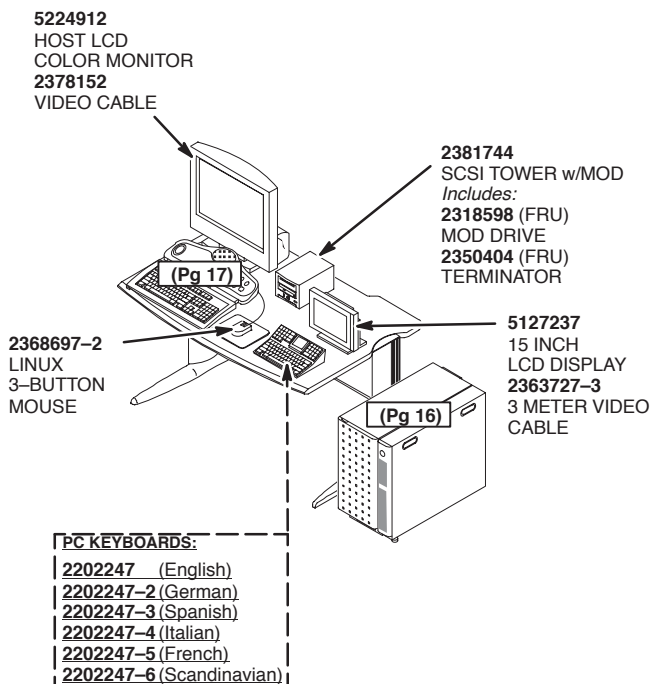


**NOTE: The following parts are Not Shown.****2156158-39** S/W COLLECTOR EXCITE II 11.0**2209991** ECHOSPEED OPTION MEDIA**2385389** SCAN TOOLS MOD**\*2295019** 13W3-DB15 RGB LCD MONITOR DATA CABLE

GOC COMPUTER CABINET – LINUX:


**EXCITE HP8000:**  
**2368697-8** LINUX PC  
**2368697-4**  
 36GB HARD DRIVE  
 FOR LINUX PC  
**2235744-5**  
 BIT3 BD FOR  
 LINUX PC

or

**EXCITE PLUS HP8400:**  
**5183547-31** LINUX PC  
**5183547-15**  
 36GB HARD DRIVE  
 FOR LINUX PC  
**5183547-51**  
 73GB HARD DRIVE  
**5183547-20**  
 SINGLE 1 GB DIMM  
**2235744-5**  
 BIT3 BD FOR  
 LINUX PC  
**5127954**  
 BRKT PC STOPPER  
**5337488**  
 GoldSeal CABLE  
 COLLECTOR FRU

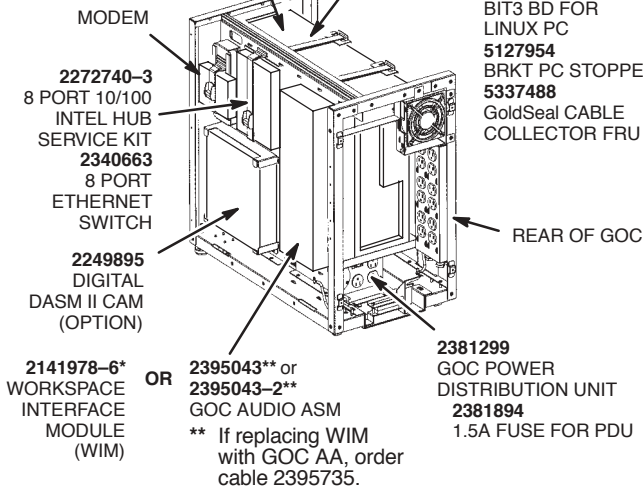**NOTES:**

- \* If WIM is not available, order part 2141978-5 and replace cable between motherboard J1 and CIF J3.

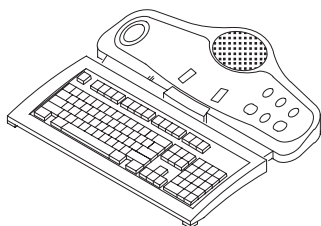**LATEST VERSIONS:****KEYBOARDS ONLY:**

- 2275756 (English)
- \*2275756-2 (French)
- \*2275756-3 (German)
- \*2275756-4 (Scandinavian)
- \*2275756-5 (Italian)
- \*2275756-6 (Portuguese)
- \*2275756-7 (Spanish)

**\* NOTE:**

These types of Keyboard/SCIM Assemblies were not available at the time this book was released, see below for earlier types.

**NOTE: The following parts are Not Shown.**

|           |                                    |
|-----------|------------------------------------|
| 2262158-9 | CABLE, 50 PIN SCIM KEYBOARD        |
| 2289697-2 | SCIM <sup>W</sup> /ENGLISH OVERLAY |
| 2289697-8 | MR SCIM GLOBAL OVERLAY SET         |

**NOTE: Refer to the Directions on CD-2160623 (Signa Service Methods) for additional product information.**





TABLE 1-1


| LOCATION | AMPS | VOLTS | GEMS<br>PART<br>NUMBER | MANUFACTURER |           |
|----------|------|-------|------------------------|--------------|-----------|
|          |      |       |                        | BUSS         | G-S       |
| FUSE F1  | 1.25 | 480   | 2276547-2              | SNQ-R-1-1/4  | ATQR1-1/4 |
| FUSE F2  | 3    | 120   | 2276547-3              | FNQ-R-3      | ATQR3     |
| FUSE F3  | 1    | 12VDC | 2276547-8              | LP-CC-1      | ATDR1     |
| FUSE F4  | 0.12 | 480   | 2276547-9              | SNQ-R-8      | ATQR1/8   |
| FUSE F5  | 125  | 480   |                        | LPJ125       | AJT125    |
| FUSE F6  | 50   | 480   |                        | LPJ-50       | AJT50     |
| FUSE F7  | 20   | 480   | 2276547-7              | LPJ-20       | AJT20     |
| FUSE F8  | 5    | 480   |                        | FRS-R-5      | TRS5R     |
| FUSE F9  | 8    | 400   | 2276547-6              | FRS-R-8      | TRS8R     |
| FUSE F10 | 10   | 120   | 2276547-11             | FNQ-R-10     | ATQR10    |
| FUSE F11 | 10   | 120   | 2276547-11             | FNQ-R-10     | ATQR10    |

2276547-14 12 VDC BATTERY


2276547-16 12 VDC SUPPLY



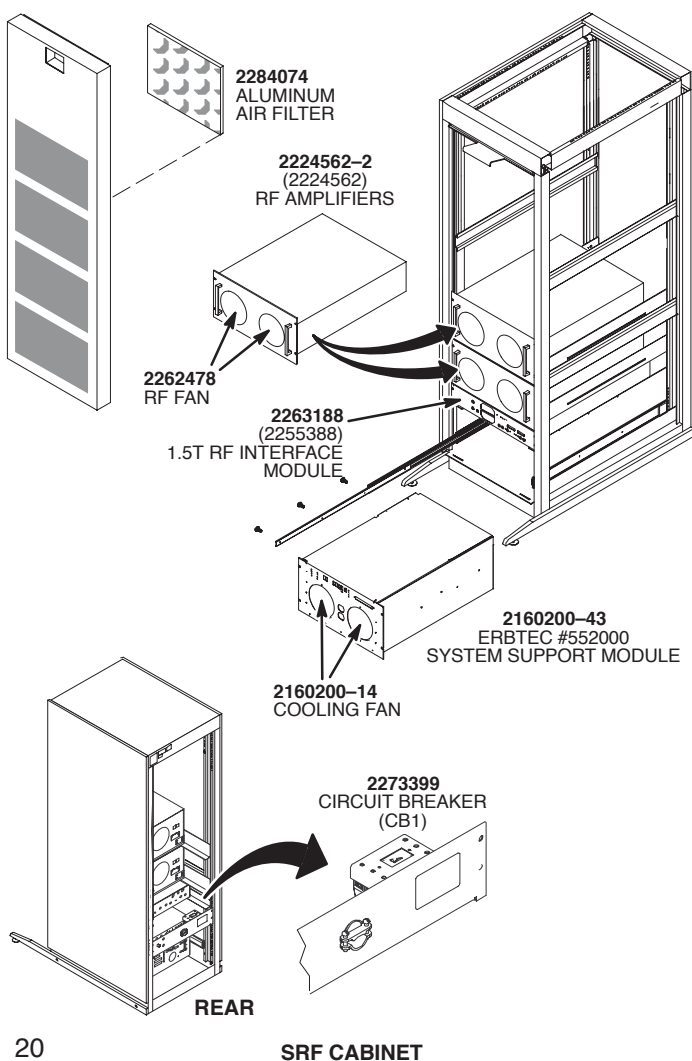

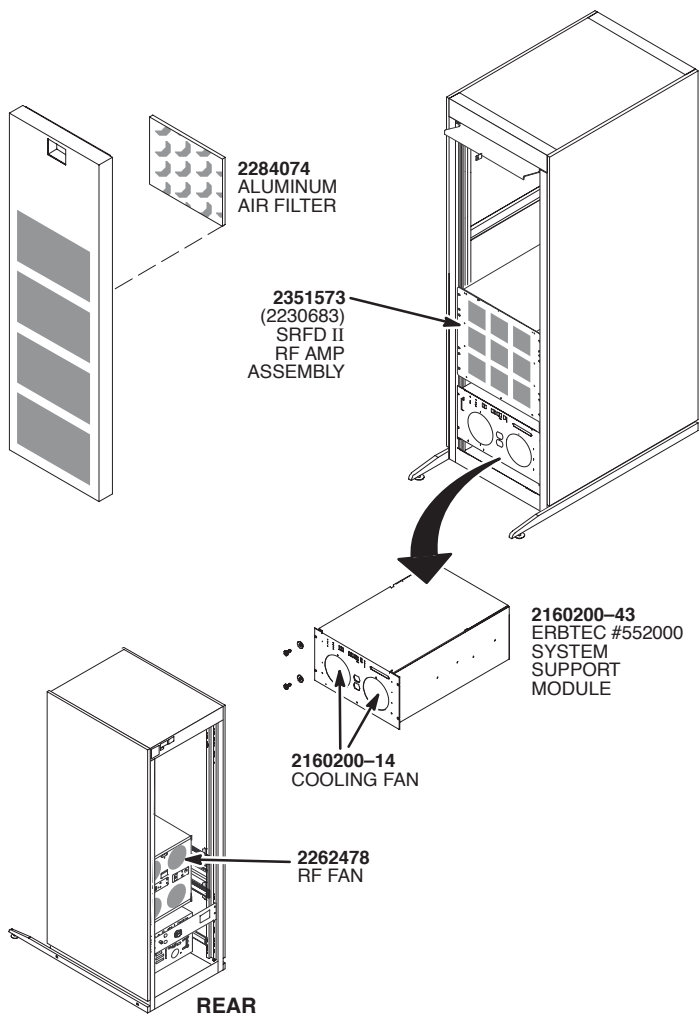


SRFD II CABINET

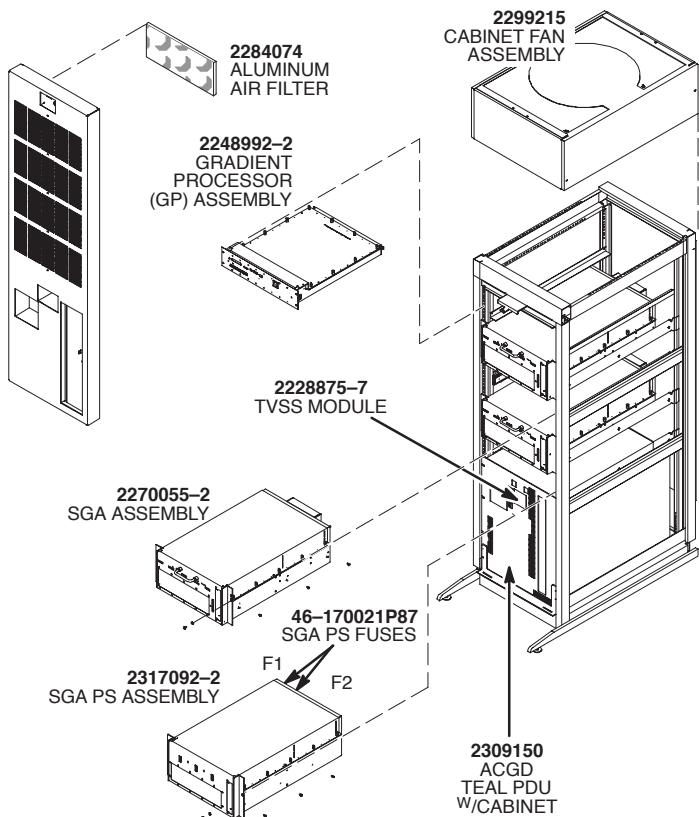
ACGD/PDU CABINET ASSEMBLY W/SGA/SGAPS/GP

**NOTE: The following Part is Not Shown.**

2261124-4 ACGD GRADIENT DATA PDL DOCUMENT

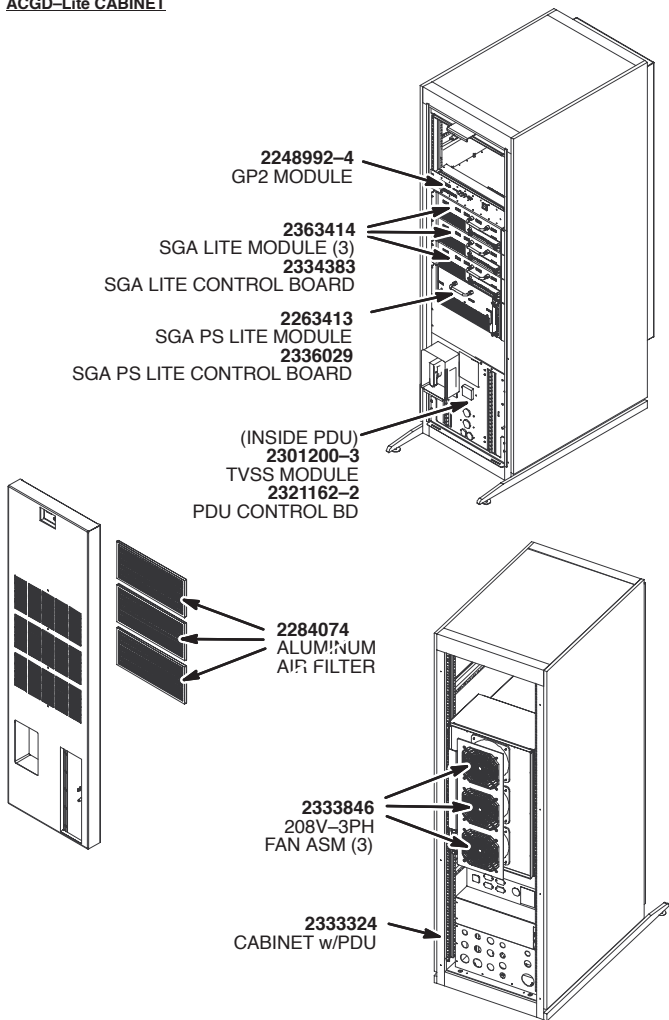


ACGD-Lite CABINETACGD-Lite CABINET

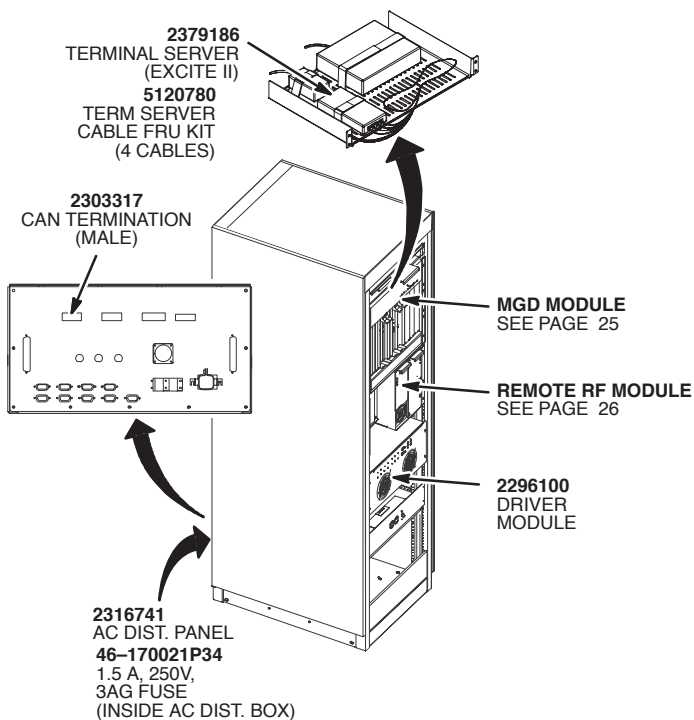

**NOTE: The following System Cabinet Options are Not Shown.**

|                   |                                                          |
|-------------------|----------------------------------------------------------|
| <b>2325947-7</b>  | REFLEX 200 ARRAY PROCESSOR BOARD – EXCITE I              |
| <b>2325947-5</b>  | RIBBON CABLE KIT (2 CABLES/KIT) – EXCITE I               |
| <b>2325947-11</b> | REFLEX 200B MAVERICK II AP (Master or Slave) – EXCITE II |
| <b>2325947-12</b> | MINERVA II AP REFLEX 400B (Master) – EXCITE II           |
| <b>2325947-13</b> | MINERVA II AP REFLEX 400B (Slave) – EXCITE II            |
| <b>2325947-14</b> | PIM FOR REFLEX 200B & 400B – EXCITE II                   |


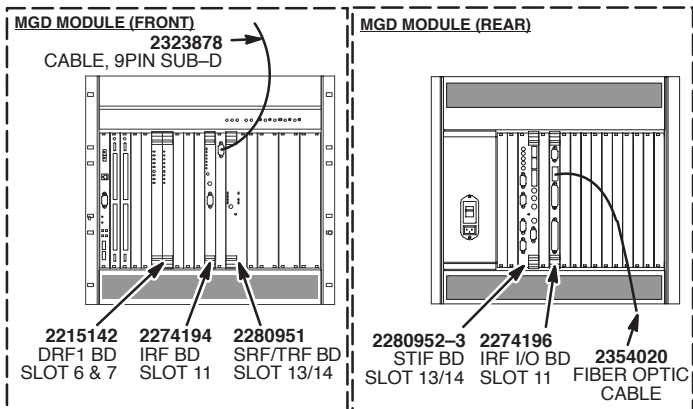


**NOTE: The following MGD Module parts are Not Shown.**

|              |                                                |
|--------------|------------------------------------------------|
| 2294300-2    | SCP BOARD WITH CAN DAUGHTER BD                 |
| 2294300-3    | AGP BOARD                                      |
| 2294300-4    | APS BOARD WITH IT DAUGHTER BD                  |
| 2294300-5    | BRIDGE BOARD                                   |
| 2294300-6    | MGD CHASSIS W/BACKPLANE & AC ENTRY (No Boards) |
| 2294300-7    | MGD FAN                                        |
| 2294300-8 or |                                                |
| 5181495-3    | POWER SUPPLIES                                 |
| 2294300-9    | INDICATOR BOARD                                |
| 2294300-19   | SCP2 BOARD                                     |

**NOTE: The following RRF MODULE (page 26) Parts/Cables are Not Shown.**

|             |                                         |
|-------------|-----------------------------------------|
| 2272740-3   | 8 PORT 10/100 INTEL HUB SERVICE KIT     |
| 46-306565P1 | CABINET FILTER                          |
| 2308729     | BNC TO SMB CABLE (MUX J8 TO CAB I/F J1) |
| 2308728     | 8W8 CABLE ASSEMBLY (MUX J5)             |
| 2322578     | J15/23/25/26 DATA INPUT CABLE (CAB I/F) |
| 2322580     | CABLE J18, UNBLANK (CAB I/F)            |
| 2322581     | CABLE J24, MAGNET MONITOR (CAB I/F)     |
| 2322582     | CABLE J30/31, SERIAL EXP (CAB I/F)      |
| 2322583     | CABLE J62 (15 PIN SUB-D) (CAB I/F)      |
| 2322586     | CABLE J61 (37 PIN SUB-D) (CAB I/F)      |
| 2315093     | ETHERNET CABLE                          |
| 2315093-2   | CABLE J63 ETHERNET (CAB I/F)            |
| 2308729-2   | BNC TO SMB CABLE (MUXJ13 TO CAB I/F J2) |
| 2308729-3   | BNC TO SMB CABLE (MUXJ14 TO CAB I/F J3) |

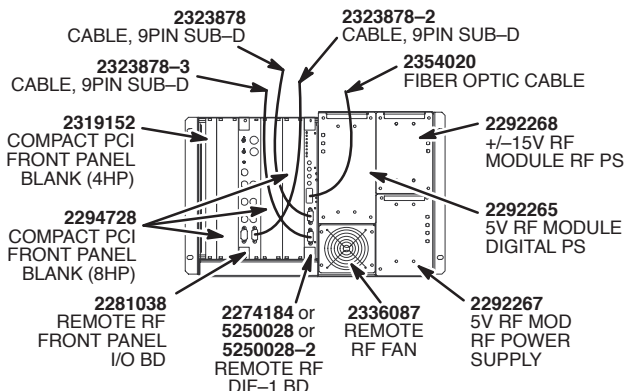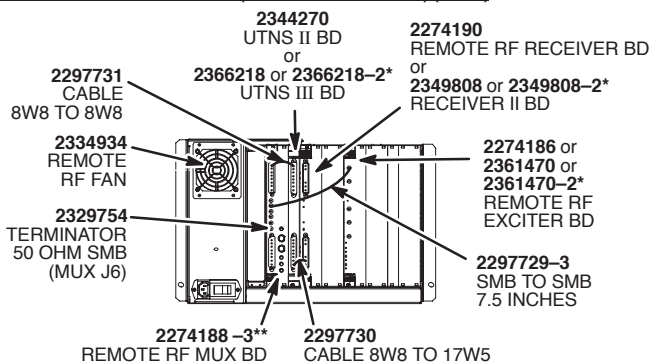
**2305884 REMOTE RF MOD ASM (CHASSIS W/MIDPLANE) (FRONT)****2305884 REMOTE RF MOD ASM (CHASSIS W/MIDPLANE) (REAR)**

**NOTE:** Additional REMOTE RF MOD ASM Parts/Cables are located on page 25.


\* A part that does not have a "-2" or "-3" can be replaced with either the same part number or the same number ending with a "-2" or "-3". If replacing the "-2" or "-3" version, then only the part number with a "-2" or "-3" can be used.


\*\* 2274188 and 2274188-2 are replaced by 2274188-3. Also, all 2274188 series MUX boards can be replaced by backwards compatible MUX2 board, 5250106.

[illegible]

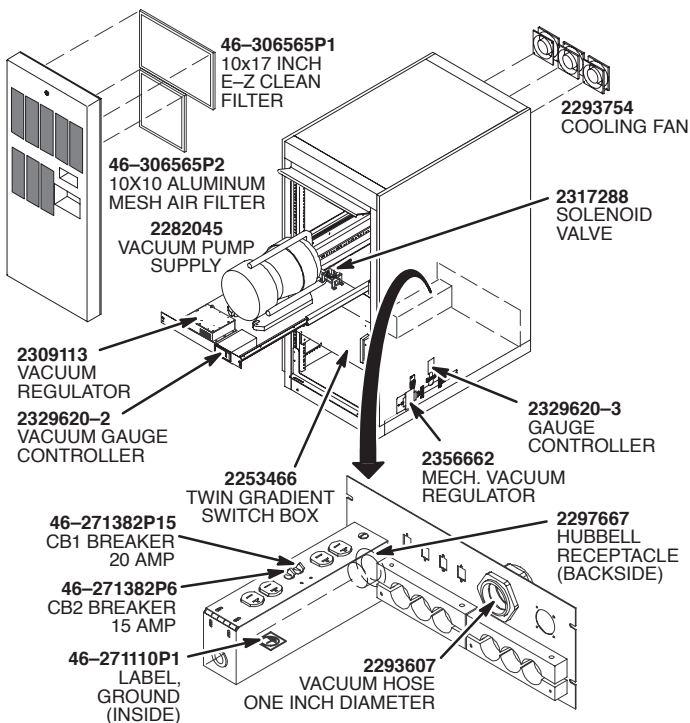**2239500 TAC****NOTE: The following parts are Not Shown.**

|                  |                               |
|------------------|-------------------------------|
| <b>2282045-2</b> | VACUUM PUMP TIP SEAL KIT      |
| <b>2293608</b>   | QF25 CENTERING RING & O-RING  |
| <b>2293608-2</b> | QF16 CENTERING RING & O-RING  |
| <b>2293609</b>   | QF25 VACUUM ELBOW             |
| <b>2293616</b>   | QF25 ADAPTER TO ONE INCH HOSE |
| <b>2293617</b>   | VACUUM REDUCING 'T'           |
| <b>2293618</b>   | QF16 CLAMP                    |
| <b>2293618-2</b> | QF25 CHAIN CLAMP              |
| <b>2294010-3</b> | HOSE CLAMP, SST ONE INCH      |
| <b>2297760</b>   | VACUUM GREASE, MSDS# 8366442  |
| <b>2329620-4</b> | VACUUM GAUGE CONTROLLER CABLE |
| <b>2284301</b>   | VACUUM GAUGE TO TAC J2 CABLE  |

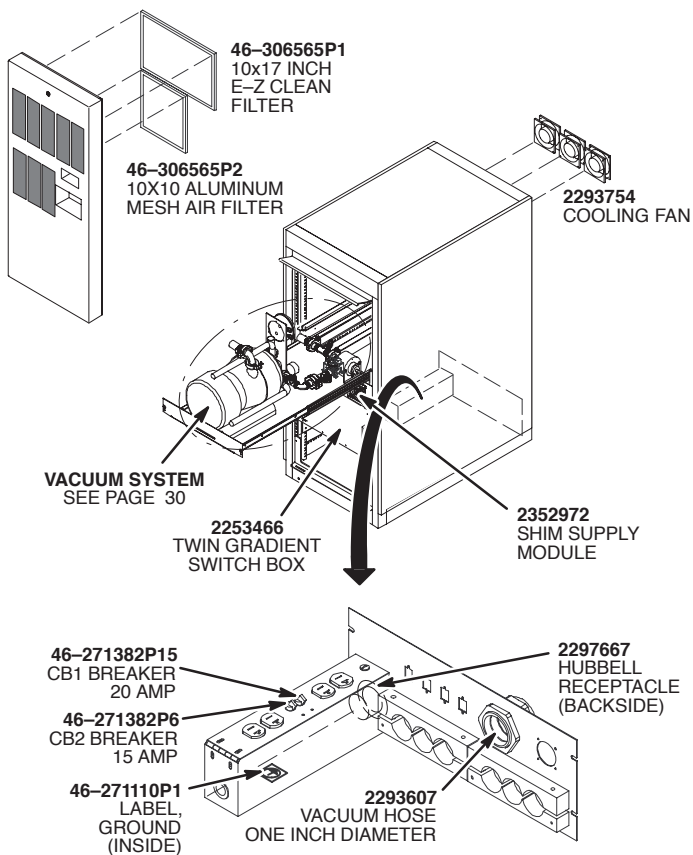
**5118162 TAC****ACCESORY CABINET (TWINSPED ONLY)**

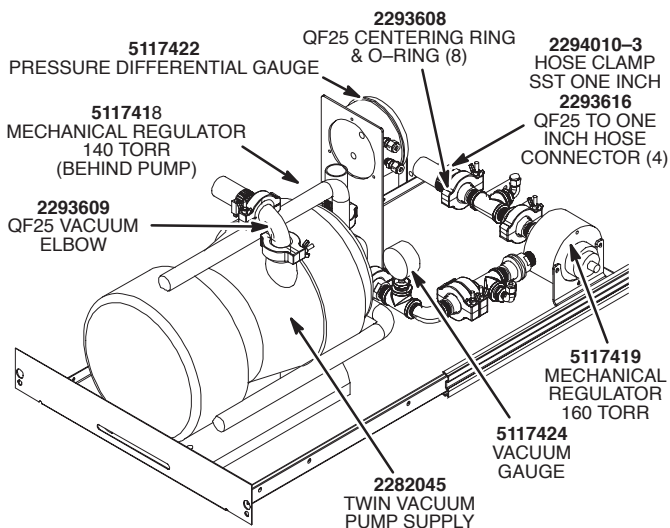

**NOTE: The following parts are Not Shown.**

|                  |                              |
|------------------|------------------------------|
| <b>2282045-2</b> | VACUUM PUMP TIP SEAL KIT     |
| <b>5118818</b>   | CLAMP NW 20-25               |
| <b>2297760</b>   | VACUUM GREASE, MSDS# 8366442 |

**5127147**  
SERVICE KIT FOR TAC VACUUM  
SYSTEM UPGRADE  
(Used to replace old style vacuum  
system, with solenoid)

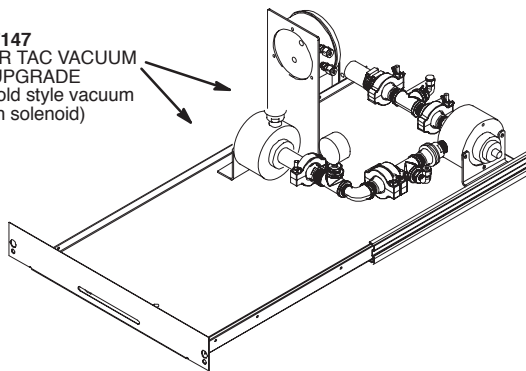



**REPLACEMENT CABLES**


The table below provides information for generic replacement cables. If any of the cables are ordered, make sure to order write-on labels to be used for identifying cable part number and connection designations at the end of each cable.

| Description                                      | Length         |                |
|--------------------------------------------------|----------------|----------------|
|                                                  | 65 Feet        | 100 Feet       |
| 9 Pin Sub-D Male/Female                          | 46-244714G30   | 46-244714G37   |
| 9 Pin Sub-D Female/Female                        | 46-244713G30   | 46-244713G37   |
| 15 Pin Sub-D Male/Female                         | 46-244712G30   | 46-244712G37   |
| 15 Pin Sub-D Female/Female                       | 46-244711G30   | 46-244711G37   |
| 25 Pin Sub-D Male/Female                         | 46-244710G30   | 46-244710G37   |
| 25 Pin Sub-D Female/Female                       | 46-244709G30   | 46-244709G37   |
| 37 Pin Sub-D Male/Female                         | 46-258877G30   | 46-258877G37   |
|                                                  | <b>50 Feet</b> | <b>65 Feet</b> |
| BNC RG 223                                       | 46-251710G1    | 46-251710G18   |
| Cable Write-on Labels<br>(60 labels per booklet) | 46-208781P3    |                |

**2274476**  
LV SHIM PHANTOM  
INNER SPERE


**2306642**  
LV PHANTOM  
SMALL HALF ASM

**2306645**  
LV PHANTOM  
BIG HALF ASM

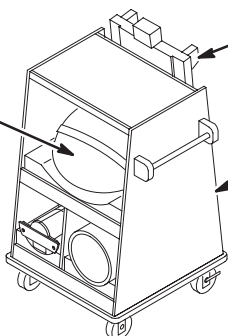

**2125247-13**  
MOLDED SPT  
NESTING PLATE

**2134213**  
SPT PHANTOM  
CART




**2125244**  
SPT SHORT LOADER  
w/SPHERE ASM


For Field Replacement Order:

**2135650-2** – SPT SPHERE


**2135652-2** – SPT LOADER




**2321556**  
DQA PHANTOM  
WITH LOADER



**2131027-2**  
DQA III ASM  
For Field  
Replacement Order:  
**2131027-9**



**2291292**  
EPI HEAD  
POSITIONER



**5110241**  
HEAD LOADER  
POSITIONER



**2170481**  
EPI FOAM  
POSITIONER

**ACCESSORIES:**

The following E-Catalog accessories are available for purchase with M-Catalog Options.

**COLOR POSTSCRIPT PRINTER FOR A/W ..... E7014LA**

|         |                                  |
|---------|----------------------------------|
| 2112346 | POSTSCRIPT COLOR NETWORK PRINTER |
|---------|----------------------------------|

**1.5T VOLUME NECK PA COIL ..... E8800PJ**

|           |                           |
|-----------|---------------------------|
| 2254930-2 | COIL,FRU,VOL NECK PA 1.5T |
| 2254930-3 | ANTERIOR BRIDGE           |
| 2254930-4 | CABLE ASM                 |
| 2254930-5 | ADAPTER BLOCK             |

**PATIENT ECG LEADWIRE SET ..... E8811EC**

|             |                                 |
|-------------|---------------------------------|
| 2219452     | HIGH IMPEDENCE ECG LEAD KIT     |
| 46-306867G1 | PATIENT ECG CABLE ASM (E8811EC) |

**ReportCARD HARDWARE**

|            |                               |
|------------|-------------------------------|
| 2368697-11 | ReportCARD COMPUTER           |
| 2390367-2  | ReportCARD SOFTWARE COLLECTOR |
| 2390369    | ReportCARD OPTON KEY          |

| REVISION 11                                      |                                             | DIRECTION 2345481 |
|--------------------------------------------------|---------------------------------------------|-------------------|
| 1.5T MNS PHOS FLEX COIL .....                    |                                             | M1040PH           |
| 2219090                                          | MNS P31 COIL ASM.                           |                   |
| 2241998                                          | QUICK DISCONNECT BOX W/CABLE TRAP           |                   |
| 46-317287G7                                      | COAXIAL CABLE, 32"                          |                   |
| 1.5T BODY FLEX COIL .....                        |                                             | M1085BE           |
| 46-328215P1                                      | DUAL-COIL CONNECTOR AND SLEEVE              |                   |
| 2151291                                          | ANTERIOR COIL W/CABLE                       |                   |
| 2151291-2                                        | POSTERIOR COIL W/CABLE                      |                   |
| 1.5T GENERAL PURPOSE FLEX COIL .....             |                                             | M1085GR           |
| 2128554                                          | COIL ASM.                                   |                   |
| 2128557                                          | CABLE KIT                                   |                   |
| 1.5T SHOULDER COIL .....                         |                                             | M1085AN           |
| 46-301058P9                                      | MEDRAD SURFACE COIL                         |                   |
| 1.5T SHOULDER ARRAY COIL .....                   |                                             | M1087SD           |
| 2225252-7                                        | SMALL COIL ASM.                             |                   |
| 2225252-6                                        | LARGE COIL ASM.                             |                   |
| 1.5T SHOULDER PHASED ARRAY COIL .....            |                                             | M1087SH           |
| 2100937-17                                       | MEDRAD ANTERIOR COIL W/CABLE                |                   |
| 2100937-18                                       | MEDRAD ANTERIOR CABLE ASM.                  |                   |
| 2100937-19                                       | MEDRAD POSTERIOR COIL W/CABLE               |                   |
| 2100937-20                                       | MEDRAD POSTERIOR CABLE ASM.                 |                   |
| 1.5T BILATERAL BREAST COIL .....                 |                                             | M1085BR           |
| 46-320785P3                                      | MEDRAD BREAST COIL W/O CABLE                |                   |
| 46-320765P2                                      | CABLE TO HEAD PORT                          |                   |
| 46-320756P2                                      | PA CABLE                                    |                   |
| 1.5T OPEN BREAST COIL .....                      |                                             | M1087BT           |
| 2246360                                          | BREAST COIL                                 |                   |
| 2246360-3                                        | CABLE ASM.                                  |                   |
| 1.5T EXTREMITY SURFACE COIL .....                |                                             | M1085AC           |
| 46-265442G1                                      | COIL, CYLINDRICAL                           |                   |
| 46-317278P1                                      | CABLE ASM.                                  |                   |
| 1.5T HIGH RES WRIST ARRAY .....                  |                                             | M1087HW           |
| 2293670-2                                        | HIGH RES WRIST ARRAY W/BASEPLATE ASM.       |                   |
| 2293670-3                                        | WRIST PHANTOM                               |                   |
| 2293670-4                                        | PHANTOM HOLDER                              |                   |
| 1.5T GENERAL PURPOSE COIL CABLE W/COIL ID .....  |                                             | M1085NJ           |
| 2383623                                          | SINGLE CHANNEL RECEIVE ONLY CABLE W/COIL ID |                   |
| 1.5T LINEAR EXTREMITY COIL CABLE W/COIL ID ..... |                                             | M1085PC           |
| 2383622                                          | LINEAR EXTREMITY COIL CABLE W/COIL ID       |                   |
| 1.5T LEGACY HEAD COIL CABLE W/COIL ID .....      |                                             | M1085PJ           |
| 2384268                                          | LEGACY HEAD COIL CABLE W/COIL ID            |                   |
| 1.5T EXTREMITY COIL W/COIL ID .....              |                                             | M1085NA           |
| 2383613-2                                        | MAI QUAD KNEE COIL W/CABLE                  |                   |
| 2383613-3                                        | MAI QUAD KNEE CABLE                         |                   |

COILS CONTINUED ON NEXT PAGE.

REVISION 11

DIRECTION 2345481

|                                                |                       |
|------------------------------------------------|-----------------------|
| 1.5T QUAD EXTREMITY KNEE/FOOT COIL .....       | M1085E                |
| 2225478-7                                      | VELCRO STRAP/LATCH    |
| 2383613-2                                      | COIL ASM.             |
| 2383613-3                                      | CABLE ASM.            |
| 2225478-10                                     | PHANTOM               |
| 1.5T PA KNEE COIL .....                        | M1087AA               |
| 46-320406P1                                    | COIL ASM.             |
| 1.5T PA TR KNEE/FOOT IMAGING OPTION .....      | M1087E                |
| 2293674-14                                     | COIL W/CABLE          |
| 2293674-13                                     | CABLE                 |
| 2293674-3                                      | PHANTOM               |
| 2293674-5                                      | PHANTOM POSITIONER    |
| 1.5T CARDIAC PHASED ARRAY IMAGING OPTION ..... | M1087CA               |
| 2174499                                        | CARDIAC ARRAY         |
| 2189499                                        | COIL ASM. - ANTERIOR  |
| 2189499-2                                      | COIL ASM. - POSTERIOR |
| 2215748                                        | CABLE ASM.            |
| 1.5T CARDIAC PERIPHERAL VASCULAR COIL .....    | M1087PR               |
| 2293676-2                                      | CVNV PV ARRAY COIL    |
| 2293676-3                                      | CABLE ASM.            |
| 2293676-4                                      | PHANTOM               |
| 2192406-7                                      | LOADING PHANTOM       |
| 2293676-6                                      | PHANTOM POSITIONER    |
| 2285178-4                                      | PHANTOM STRAP         |
| 1.5T PERIPHERAL VASCULAR ARRAY COIL .....      | M1087PW               |
| 2192406-2                                      | CABLE ASM             |
| 2192406-12                                     | COIL ASM.             |
| 2192406-5                                      | PIN DIODES            |
| 2192406-6                                      | SNR PHANTOM           |
| 2192406-7                                      | LOADING PHANTOM       |
| 2192406-9                                      | PHANTOM POSITIONER    |
| 1.5T NEUROVASCULAR ARRAY COIL .....            | M1087N                |
| 2225476-2                                      | COIL ASM.             |
| 2225476-3                                      | CABLE ASM.            |
| 2225476-6                                      | COIL LATCHES          |
| 2225476-6                                      | PHANTOM POSITIONER    |
| 1.5T NEUROVASCULAR ARRAY COIL W/ NEW TOP ..... | M1087NB               |
| 2293668-2                                      | COIL W/CABLE          |
| 2225476-3                                      | CABLE ASM.            |
| 2225476-6                                      | COIL LATCHES          |
| 2293668-7                                      | PHANTOM POSITIONER    |
| 1.5T NEUROVASCULAR HEAD/NECK COIL .....        | M1085HN               |
| 2118138-5                                      | COIL ASM.             |
| 2383614                                        | QUAD NV CABLE         |
| 1.5T ANTERIOR NECK COIL .....                  | M1085AK               |
| 46-287396P10                                   | MEDIUM SURFACE COIL   |
| 1.5T POSTERIOR CERVICAL SPINE COIL .....       | M1085AM               |
| 46-287807P12                                   | MEDRAD NECK COIL      |

COILS CONTINUED ON NEXT PAGE.

COILS

35

|                                           |                                      |
|-------------------------------------------|--------------------------------------|
| 1.5T QUADRATURE T/L SPINE COIL .....      | M1085AP                              |
| 46-307387P10                              | MEDRAD COIL W/POSITIONER             |
| 1.5T QUADRATURE CERVICAL SPINE COIL ..... | M1085AR                              |
| 46-320422P1                               | COIL W/CABLE                         |
| 1.5T CTL COIL .....                       | M1087CT                              |
| 2104799                                   | CTL MULTICOIL ASM.                   |
| 1.5T CTL SPINE ARRAY COIL .....           | M1087SP                              |
| 2225545-6                                 | COIL W/CABLE & BRIDGE                |
| 2225545-2                                 | CABLE ASM.                           |
| 2225545-8                                 | ANTERIOR NECK COIL ASM.              |
| 2225545-9                                 | ADAPTER BLOCK                        |
| 1.5T TORSO ARRAY COIL .....               | M1087TB                              |
| 2215261                                   | COIL                                 |
| 2215748-2                                 | CABLE ASM.                           |
| 1.5T PHASED ARRAY PELVIC COIL .....       | M1087PA                              |
| 2144100-2                                 | PELVIC COIL                          |
| 46-307821G1                               | CABLE ASM.                           |
| 2144806                                   | PHASE ADJUST                         |
| 1.5T TORSO PELVIS COIL .....              | M1087TP                              |
| 2298043-2                                 | COIL ASM.                            |
| 2298043-3                                 | CABLE ASM.                           |
| 2298043-4                                 | PHANTOM                              |
| 2298043-5                                 | PHANTOM POSITIONER                   |
| 1.5T HI RES BRAIN COIL .....              | M3087JA                              |
| 2317112-2                                 | 8CHANNEL HR BRAIN CL/BASEPLATE       |
| 2317112-3                                 | 8CHANNEL HR BRAIN PHANTOM POSITIONER |
| 2317112-8                                 | 8CHANNEL HR HEAD CABLE ASSEMBLY      |
| 2317112-12                                | 8CHANNEL HR BRAIN LATCH KIT          |
| 1.5T 8 CHANNEL NV ARRAY COIL .....        | M3087JB                              |
| 2317115-2                                 | 8CHANNEL NV ARRAY                    |
| 2317115-3                                 | 8CHANNEL PHANTOM KIT                 |
| 2317115-10                                | 8CHANNEL RIGHT/LEFT LATCH KIT        |
| 2317115-11                                | 8CHANNEL SUPERIOR LATCH KIT          |
| 1.5T 8 CHANNEL CTL COIL .....             | M3087JC                              |
| 2377426-2                                 | 8CHANNEL COIL W/CABLE                |
| 2377426-3                                 | 8CHANNEL PHANTOM                     |
| 2377426-7                                 | 8CHANNEL CABLE                       |
| 2377426-10                                | 8 CHANNEL PREAMP                     |
| 1.5T 8 CHANNEL CARDIAC COIL .....         | M3087JD                              |
| 2304255-2                                 | 8 CHANNEL CARDIAC ARRAY COIL W/CABLE |
| 2304255-3                                 | 8 CHANNEL CARDIAC ARRAY PHANTOM KIT  |
| 2304255-7                                 | 8 CHANNEL CARDIAC ARRAY CABLE        |
| 2377426-10                                | 8 CHANNEL PREAMP                     |
| 1.5T 8 CHANNEL BODY ARRAY COIL .....      | M3087JE                              |
| 2377425-2                                 | 8 CHANNEL BODY ARRAY COIL W/CABLE    |
| 2377425-3                                 | 8 CHANNEL BODY ARRAY PHANTOM KIT     |
| 2377425-7                                 | 8 CHANNEL BODY ARRAY CABLE           |
| 2377426-10                                | 8 CHANNEL PREAMP                     |



**OPTIONS:**

**NOTE:** Where possible, a FRU which is part of Option Catalog is shown under the area where it would be installed, rather than being listed in this section.

|                                                   |                                  |
|---------------------------------------------------|----------------------------------|
| <b>CLARIVIEW IMAGE FILTERING</b> .....            | <b>M1090PN</b>                   |
| 2203037                                           | AW1.2 CLARIVIEW FLOPPY ASM.      |
| 2203038                                           | AW2.0 CLARIVIEW FLOPPY ASM.      |
| 2203039                                           | SECURITY KEY FLOPPY ASM.         |
| <b>REFLEX 100</b> .....                           | <b>M3000RD</b>                   |
| 2325947-6                                         | EXCITE REFLEX 100                |
| <b>REFLEX 200</b> .....                           | <b>M3000RE</b>                   |
| 2325947-7                                         | EXCITE REFLEX 200                |
| <b>REFLEX 400</b> .....                           | <b>M3000RF</b>                   |
| 2325947-5                                         | RIBBON CABLE (EXCITE REFLEX)     |
| <b>FIESTA-C – EXCITE II</b> .....                 | <b>M3033MB</b>                   |
| 2383494                                           | FIESTA-C S/W KEY                 |
| <b>3D DELAYED ENHANCEMENT – EXCITE II</b> .....   | <b>M3033MD</b>                   |
| 2383495                                           | 3D DELAYED ENHANCEMENT S/W KEY   |
| <b>NAVIGATOR 3D – EXCITE II</b> .....             | <b>M3033ME</b>                   |
| 2383496                                           | NAVIGATOR 3D S/W KEY             |
| <b>3D FATSAT FIESTA CARDIAC – EXCITE II</b> ..... | <b>M3033MF</b>                   |
| 2383497                                           | 3D FATSAT FIESTA CARDIAC S/W KEY |
| <b>TRICKS – EXCITE II</b> .....                   | <b>M3033MH</b>                   |
| 2383498                                           | TRICKS S/W KEY                   |
| <b>BILATERAL BREAST – EXCITE II</b> .....         | <b>M3033MJ</b>                   |
| 2383499                                           | BILATERAL BREAST S/W KEY         |
| <b>BAR CODE READER KIT</b> .....                  |                                  |
| 2180690-2                                         | READER ONLY                      |
| 2180690-3                                         | Y CABLE ONLY                     |



**OPTIONS for EXCITE II:**

|                |                                |
|----------------|--------------------------------|
| <b>2390037</b> | Asset for EXCITE               |
| <b>2390040</b> | ConnectPro for EXCITE          |
| <b>2390075</b> | 3D FRFSE for EXCITE            |
| <b>2390076</b> | PROSE for EXCITE               |
| <b>2390077</b> | 3D FIESTA for EXCITE           |
| <b>2390078</b> | EchoPlus for EXCITE            |
| <b>2390079</b> | Diffusion Tensor EXCITE        |
| <b>2390084</b> | Probe 2000 for EXCITE          |
| <b>2390085</b> | Probe 200 Upgrade for EXCITE   |
| <b>2390086</b> | Sage 7 for EXCITE              |
| <b>2390087</b> | Probe 3D Brain for EXCITE      |
| <b>2390088</b> | 2D FIESTA for EXCITE           |
| <b>2390089</b> | FGRE-ET for EXCITE             |
| <b>2390090</b> | Real-Time FGRE-ET for EXCITE   |
| <b>2390091</b> | 2D Delayed Enhancement EXCITE  |
| <b>2390092</b> | Spiral Hi-Res for EXCITE       |
| <b>2390093</b> | Real-Time Spiral for EXCITE    |
| <b>2390094</b> | iDrive Pro for EXCITE          |
| <b>2390095</b> | iDrive ProPlus for EXCITE      |
| <b>2390096</b> | Cardiac Tagging for EXCITE     |
| <b>2390097</b> | SmartPrep 2000 for EXCITE      |
| <b>2390098</b> | Flouro Trigger MRA for EXCITE  |
| <b>2390103</b> | Performed Proc Step for EXCITE |
| <b>2390340</b> | HiSpeed Option for Linux PC    |
| <b>2390341</b> | EchoSpeed Option for Linux PC  |

**BrainWave OPTIONS:**

|                   |                                                                                                                                                 |
|-------------------|-------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>2363727</b>    | 15" LCD Display with 5 foot VGA Cable for Computer connection                                                                                   |
| <b>2394034-5</b>  | (Cedrus) Response Pad Asm. Left & right hand units with two buttons for each hand. Includes fiber optic cable (20 ft) and optical converter box |
| <b>2394034-6</b>  | (Cedrus) "Lumina" response controller box                                                                                                       |
| <b>2394034-7</b>  | (Cedrus) AC Power module for Lumina Controller Box                                                                                              |
| <b>2394034-9</b>  | FRU usage only Kit containing all cables [Cedrus-4, -5, -6, -7, 2xxxxxx-6, 46-265505P1 (qty 2)]                                                 |
| <b>2394034-10</b> | Penetration Sub-Panel Asm                                                                                                                       |
| <b>2394034-16</b> | PC compatible Keyboard (narrow)                                                                                                                 |
| <b>2394034-17</b> | PC compatible Mouse                                                                                                                             |
| <b>5110767</b>    | BrainWave Application Software CD-ROM                                                                                                           |
| <b>5110736</b>    | EXCITE II Scanner License Key MOD for the BrainWave H/W Option                                                                                  |
| <b>5110946</b>    | PC and Platform Software Asm                                                                                                                    |
| <b>5110968</b>    | Patch CD for BrainWave Stimulus PC                                                                                                              |