

Table of Contents


Chapter 1	
System Communications.....	3
Section 1.0 — Slip Ring Communications Interface - 2399621.....	4
Section 2.0 — Final Scan Control, Console Ethernet - 2399622	5
Section 3.0 — Rotating Controller Interface Bus (RCIB) - 2399623.....	6
 Chapter 2	
X-Ray Generation	7
Section 1.0 — Tube Fans / Pump / SmartID Interface - 2399624.....	8
Section 2.0 — JEDI Interface - kV Loop - 2399625	9
Section 3.0 — JEDI Interface - mA Loop - 2399628.....	10
Section 4.0 — X-Ray Collimation & Filtration - 2399626.....	11
Section 5.0 — Exposure Enable and Final Command - 2399629	12
Section 6.0 — Tube Rotor Control - 2399630.....	13
Section 7.0 — HP X-Ray Tube Coolant Flow - 2399628	14
 Chapter 3	
Data Acquisition	15
Section 1.0 — Trigger Generation - 2399724	16
Section 2.0 — Detector Heater (DAS Item) - 2399725	17
 Chapter 4	
Patient Positioning	19
Section 1.0 — Alignment Lights - 2399726	20
Section 2.0 — Gantry Tilt, from Gantry, Console - 2399727.....	21
Section 3.0 — Table Cradle Sync - 2399728	22
Section 4.0 — Table Cradle Drive - 5127766	23
Section 5.0 — Table Cradle Intermediate Support Drive - 5127766.....	24
Section 6.0 — Table Elevation Drive - 5127766	25
Section 7.0 — Table Interconnect Overview - 5121647.....	26
Section 8.0 — Table Touch Switches - 5121647.....	27
Section 9.0 — Table Footswitch - 5121647	28

Chapter 5	
Axial Control	29
Section 1.0 — Axial Servo Control / Dynamic Brake - 2399731	30
Section 2.0 — Axial Power Distribution - 2399732	31
 Chapter 6	
Operator I/O.....	33
Section 1.0 — Gantry Operator Interface and Displays - 2399733.....	34
Section 2.0 — Gantry Reset from Console - 2399734	35
Section 3.0 — Cardiac Options - 2399735	36
Section 4.0 — Pulmonary Options - 2399736.....	37
Section 5.0 — Scan Footswitch and IHHC Controller - 2399737	38
Section 6.0 — Site X-Ray Light, System Light - 2399738.....	39
Section 7.0 — Autovoice / Intercom - 2399739	40
 Chapter 7	
System Monitoring	41
Section 1.0 — Gantry Temperature and Balance Sensors - 2399740	42
Section 2.0 — Gantry Cover Fans - 2399741.....	43
 Chapter 8	
System Power Control	45
Section 1.0 — System E-Stop and Power Interlocks - 2399742	46
Section 2.0 — PDU - Gantry 120 VAC Control - 2399743	47
Section 3.0 — HV_DC_Control - 2399744.....	48
Section 4.0 — HP MDAS/GDAS Gantry Power Distribution - 2399627	49

THIS PAGE INTENTIONALLY BLANK.

Chapter 1

System Communications

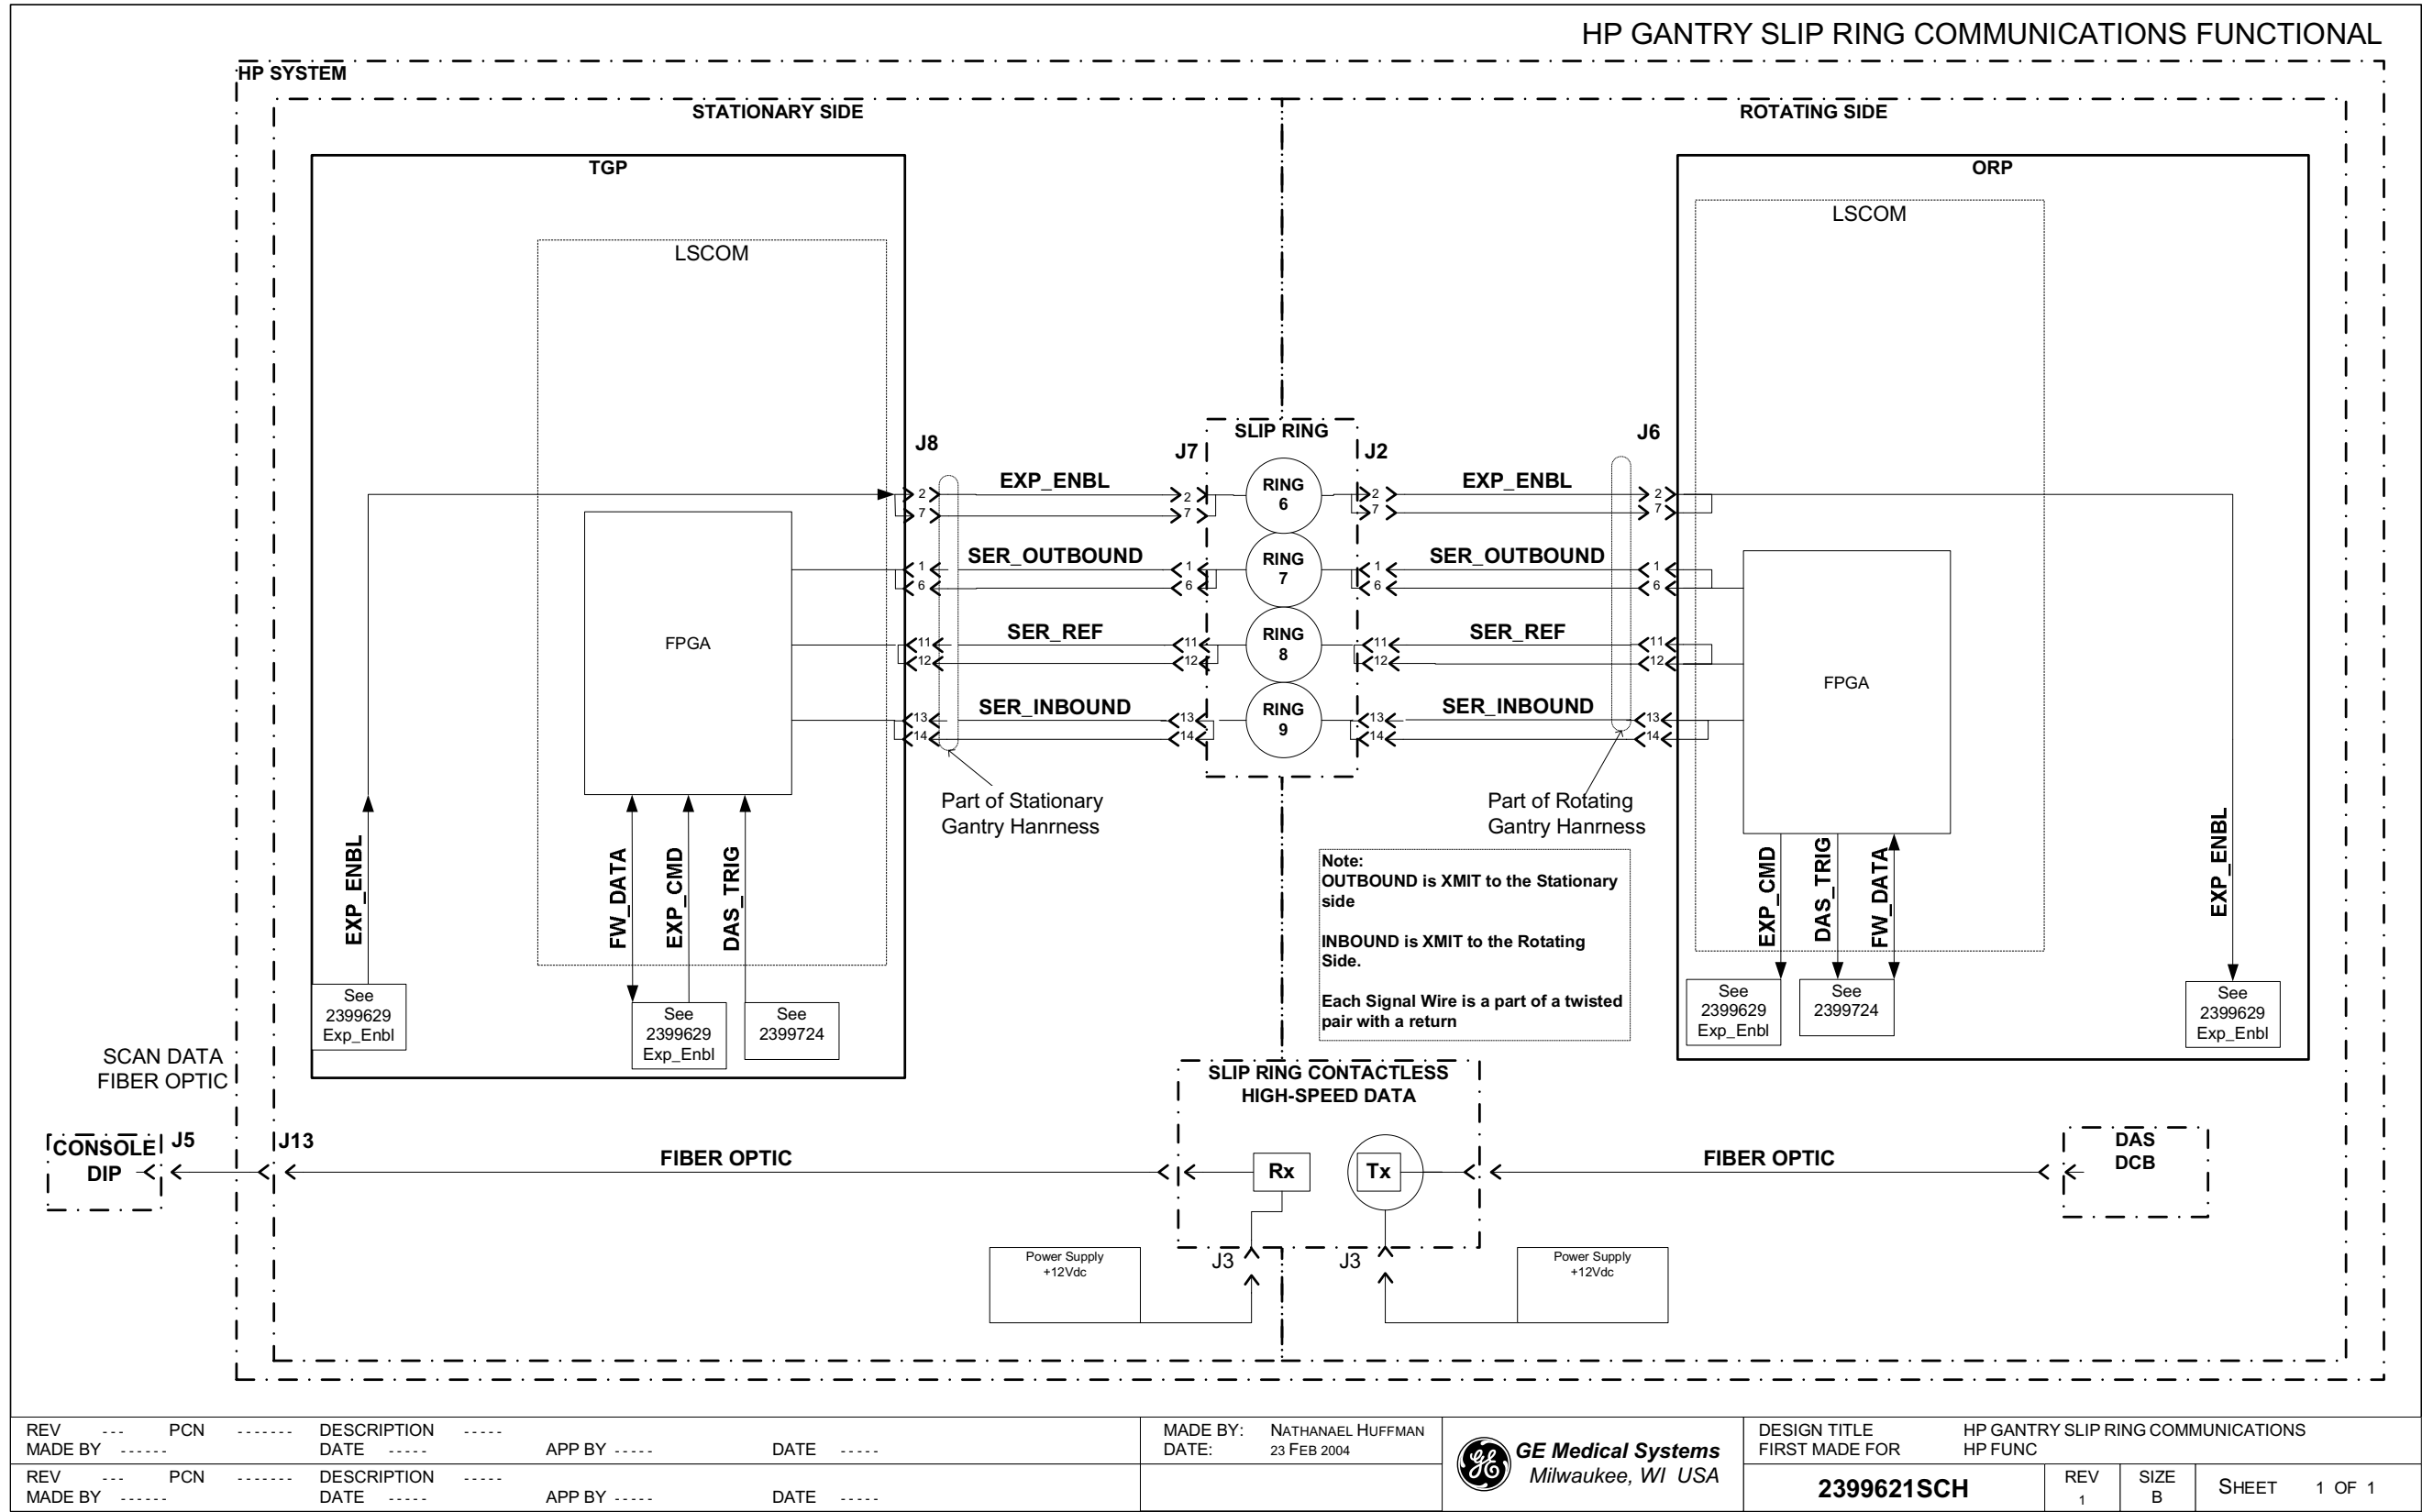

REV	---	PCN	-----	DESCRIPTION	-----	APP BY	-----	DATE	-----	MADE BY:	NATHANAEL HUFFMAN	 GE Medical Systems Milwaukee, WI USA	DESIGN TITLE FIRST MADE FOR				HP GANTRY SLIP RING COMMUNICATIONS HP FUNC				
REV	---	PCN	-----	DESCRIPTION	-----	APP BY	-----	DATE	-----	DATE:	23 FEB 2004		2399621SCH				REV	1	SIZE	B	SHEET

Figure 1-1 2399621 Sheet 1, Rev. 1

Section 2.0 — Final Scan Control, Console Ethernet - 2399622



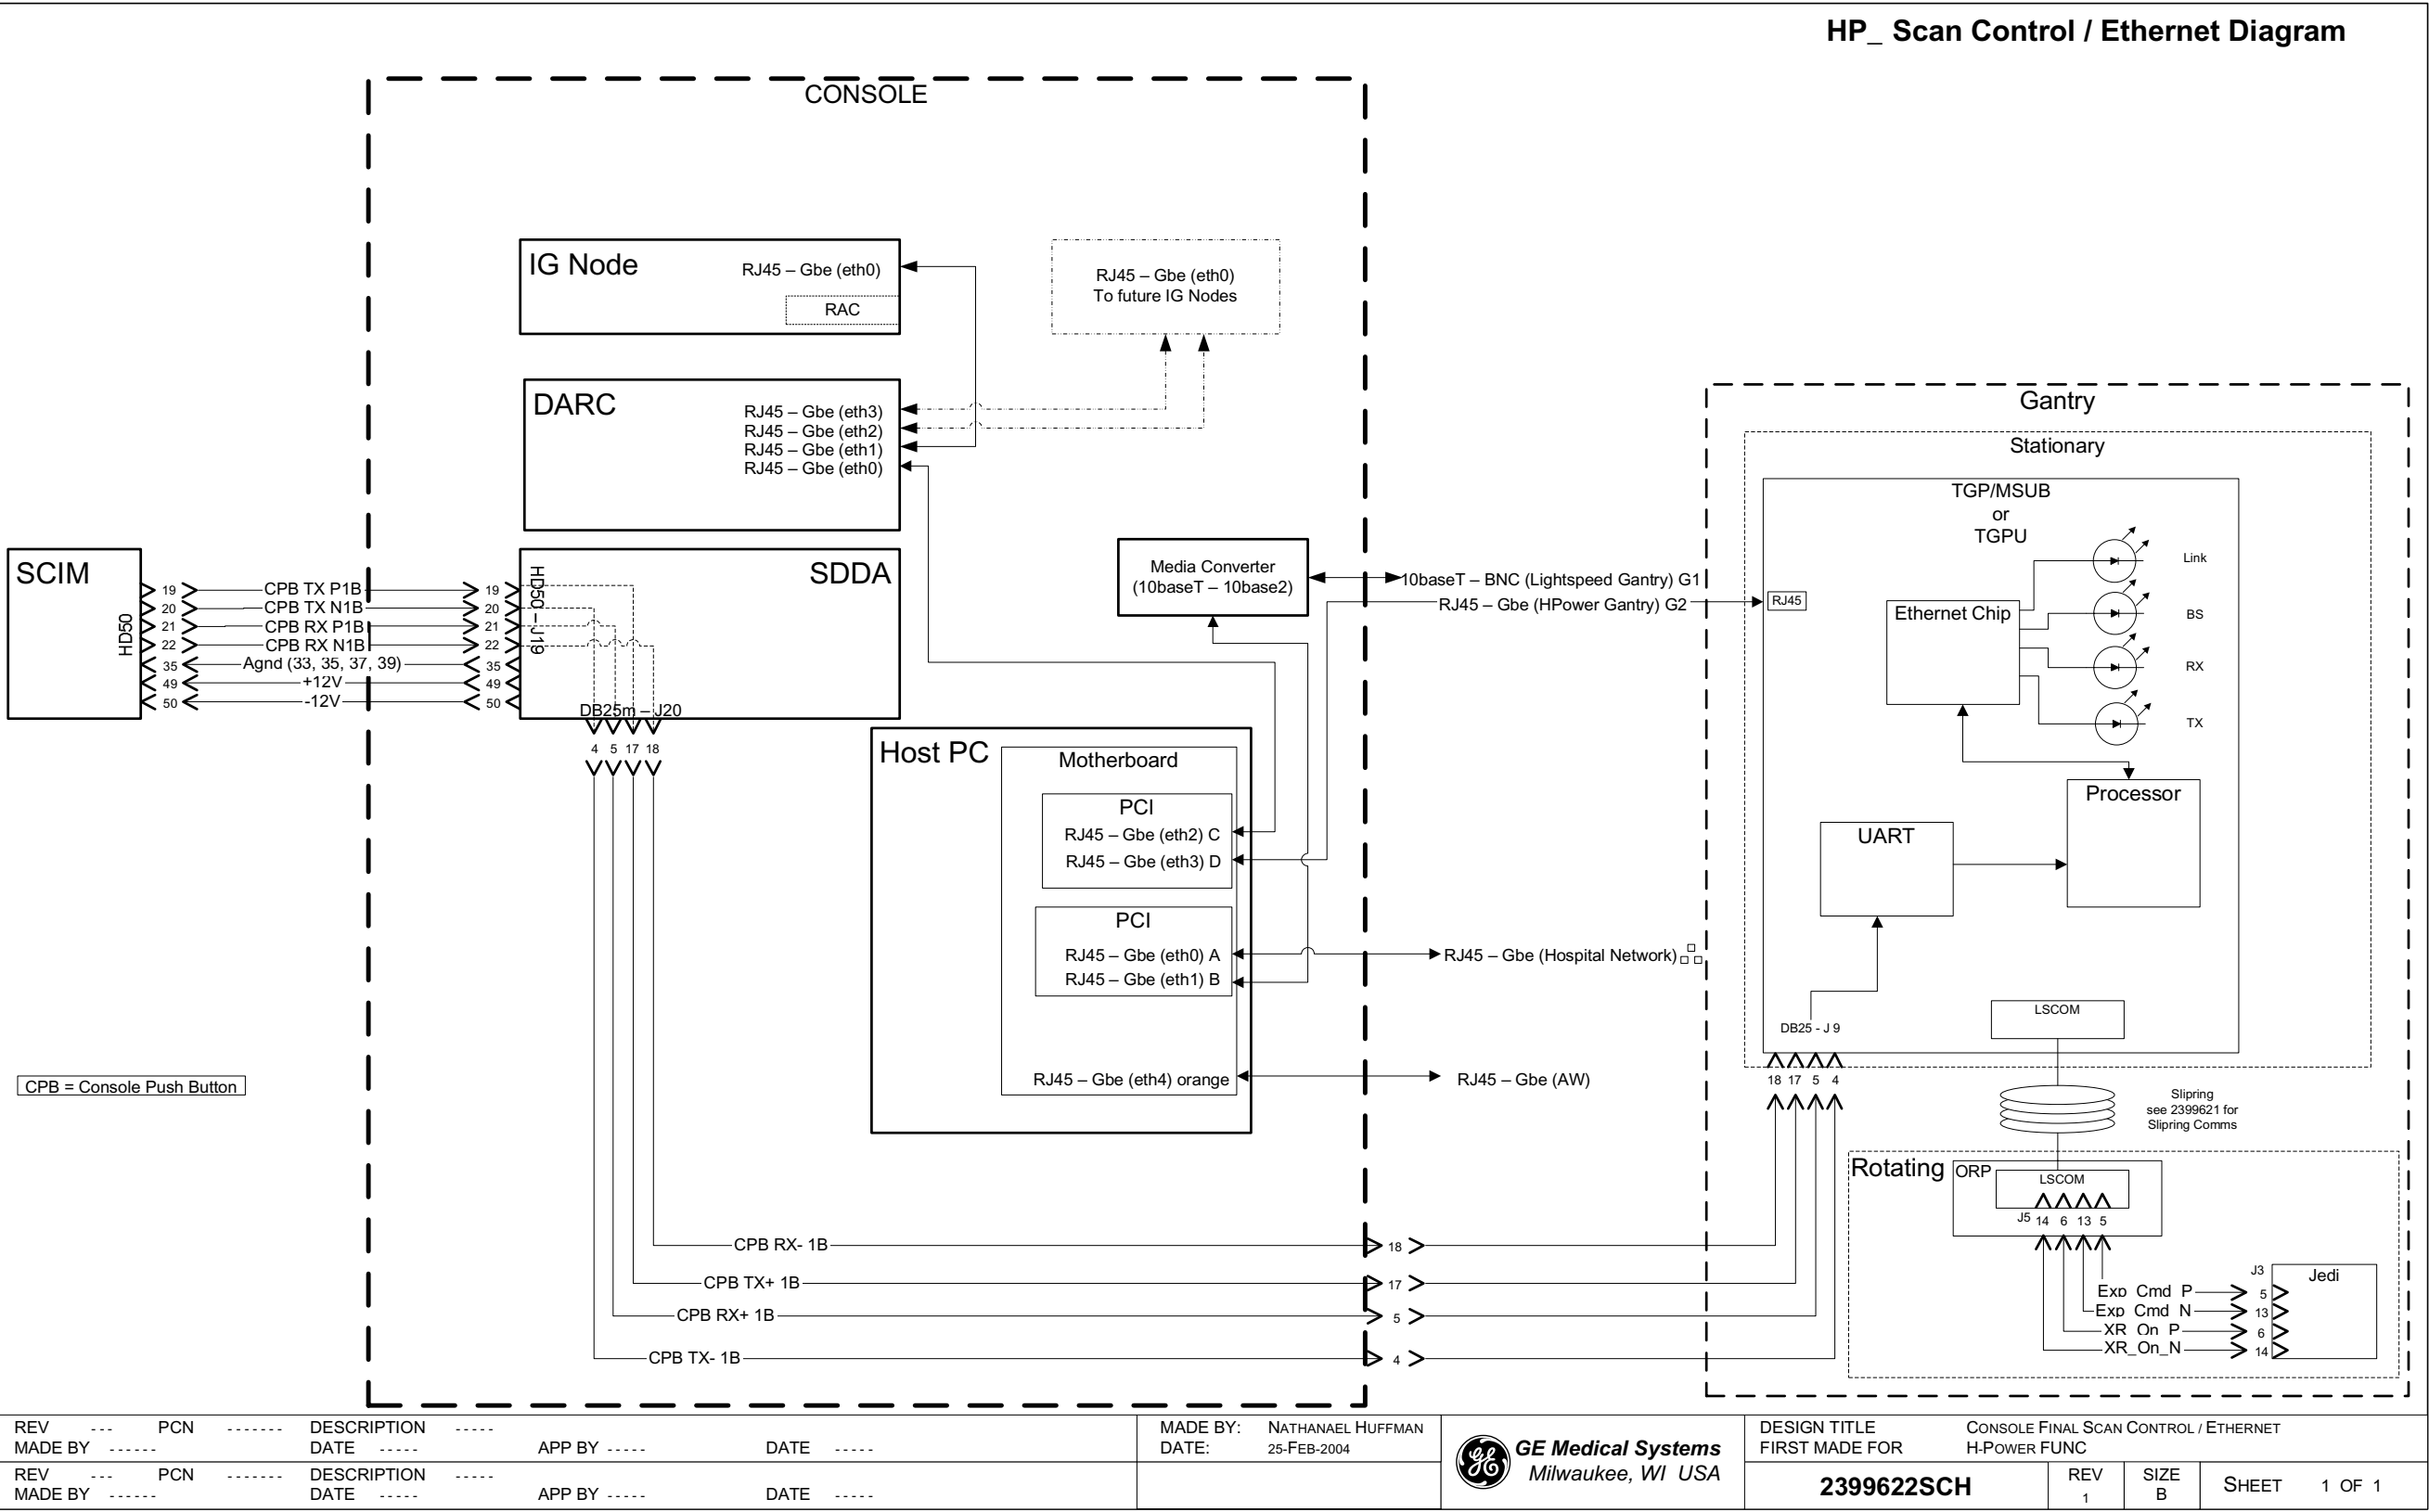


Figure 1-2 2399622 Sheet 1, Rev 1

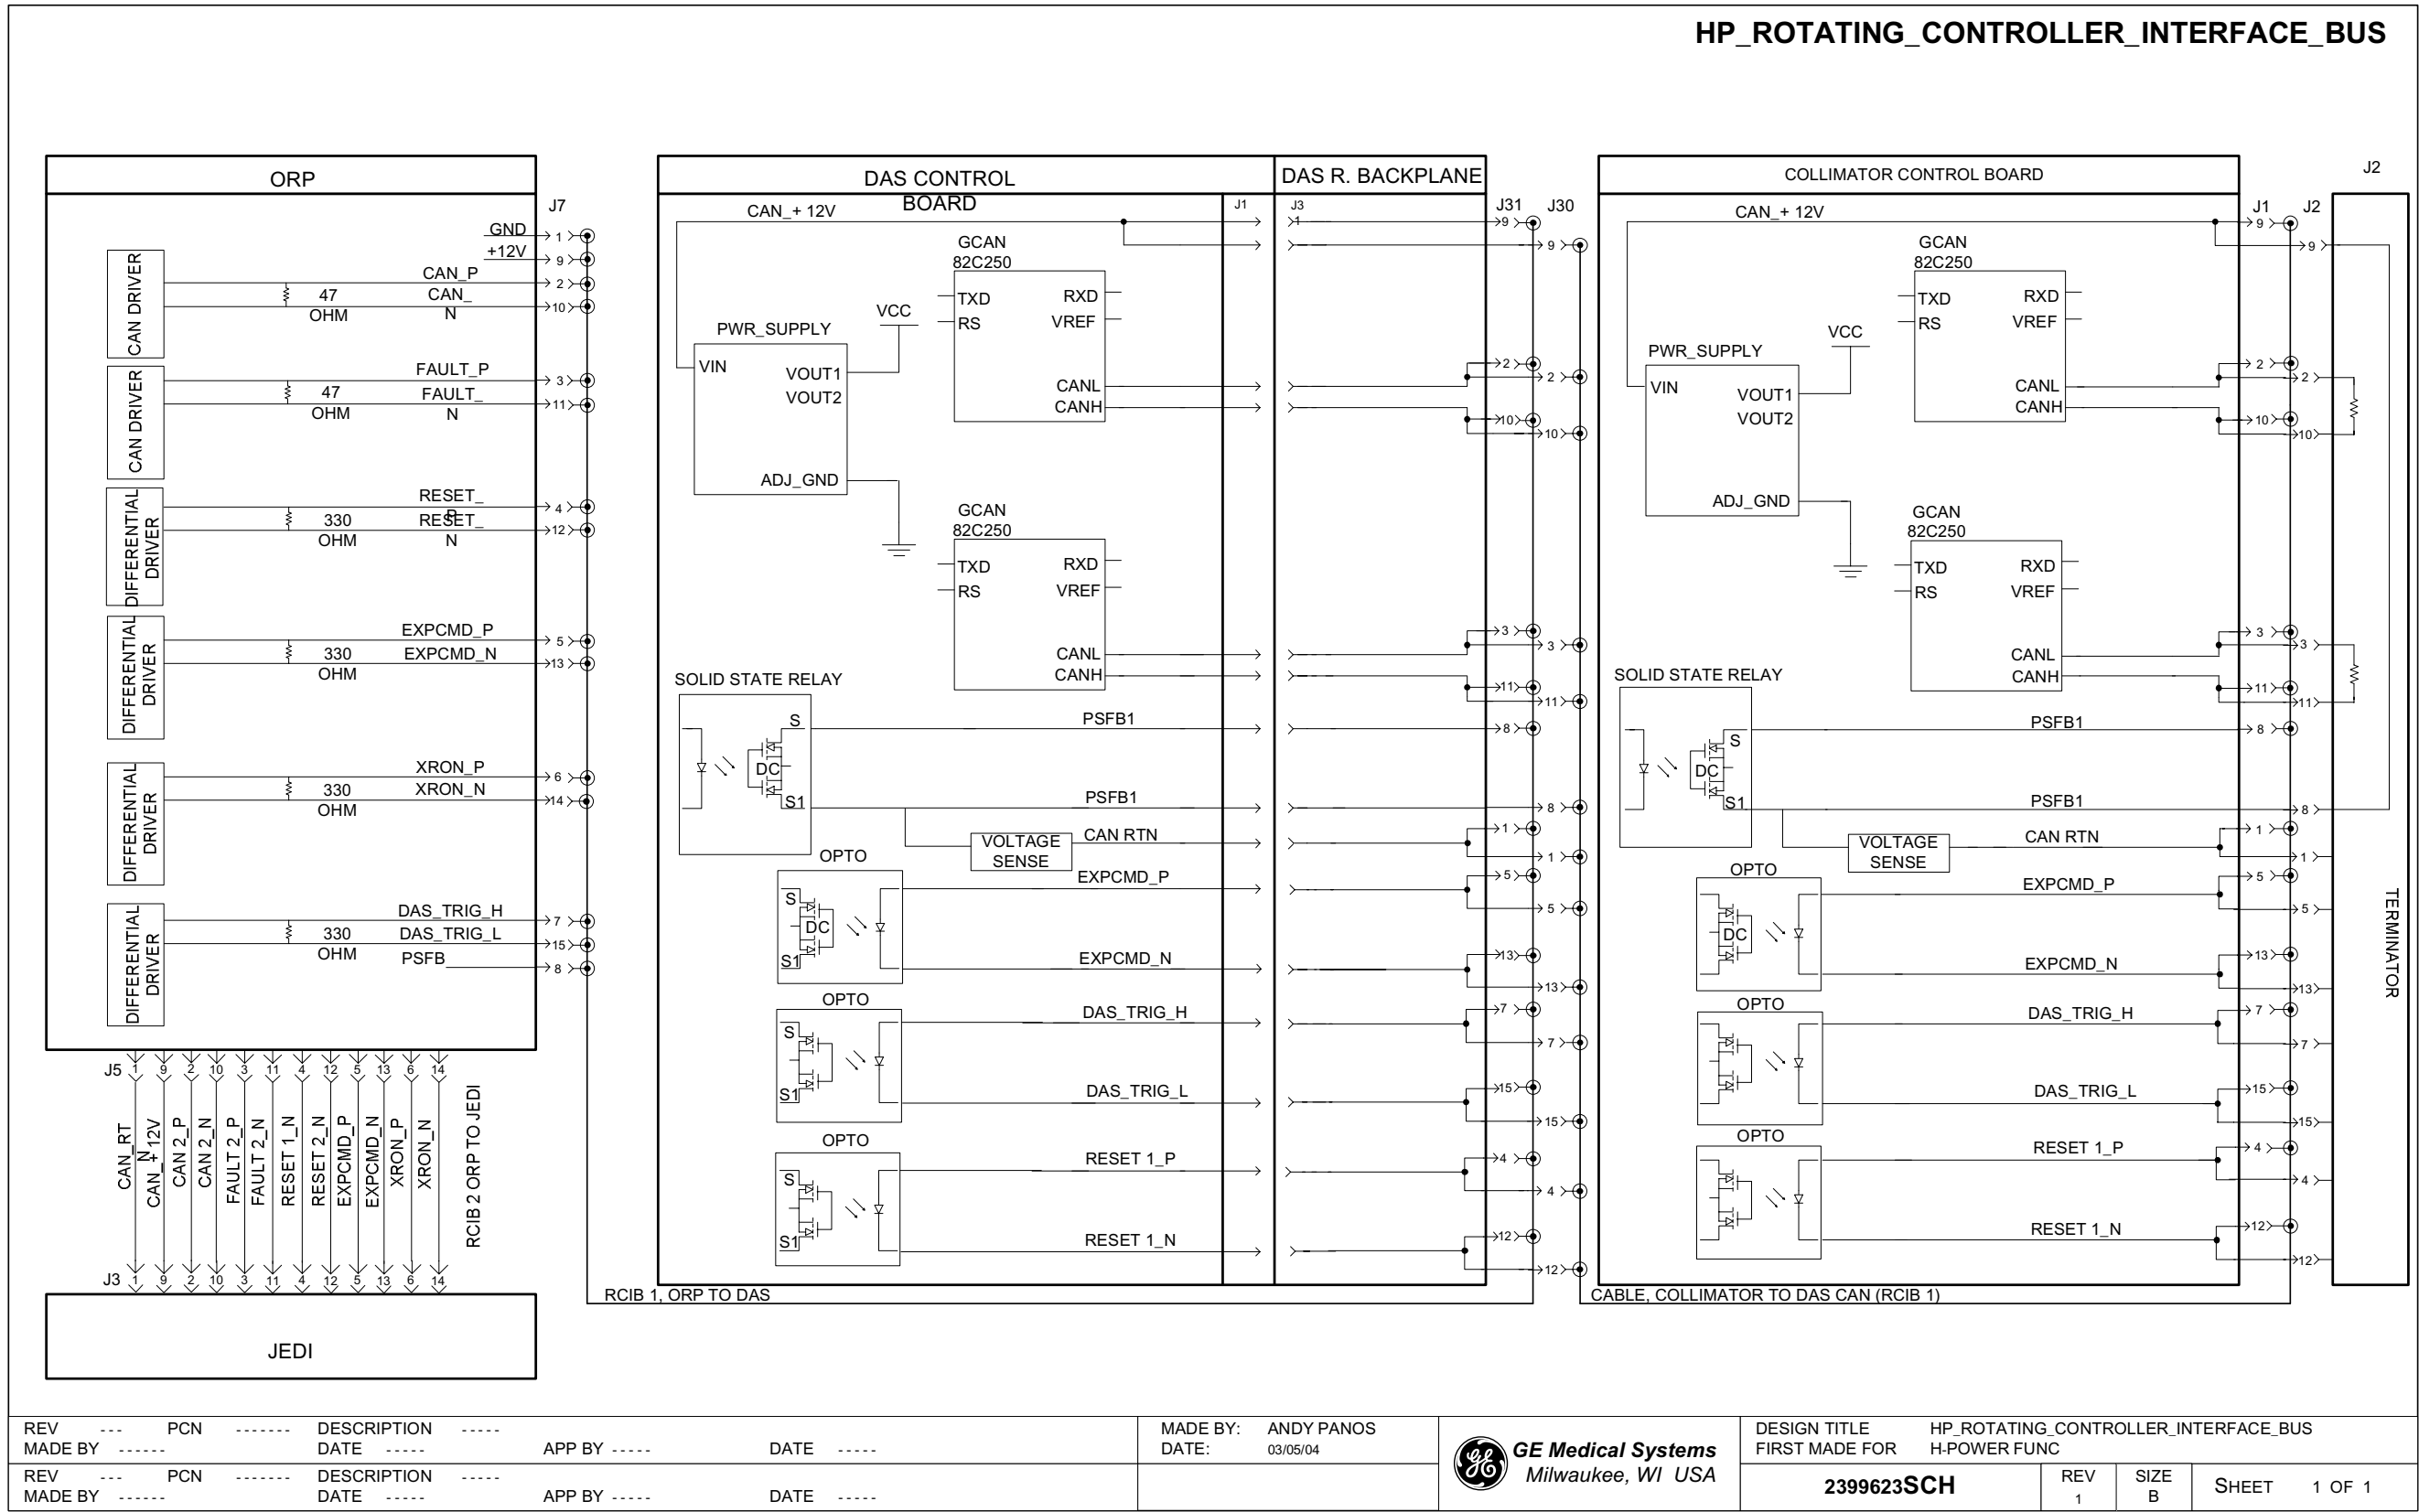


Chapter 2


X-Ray Generation

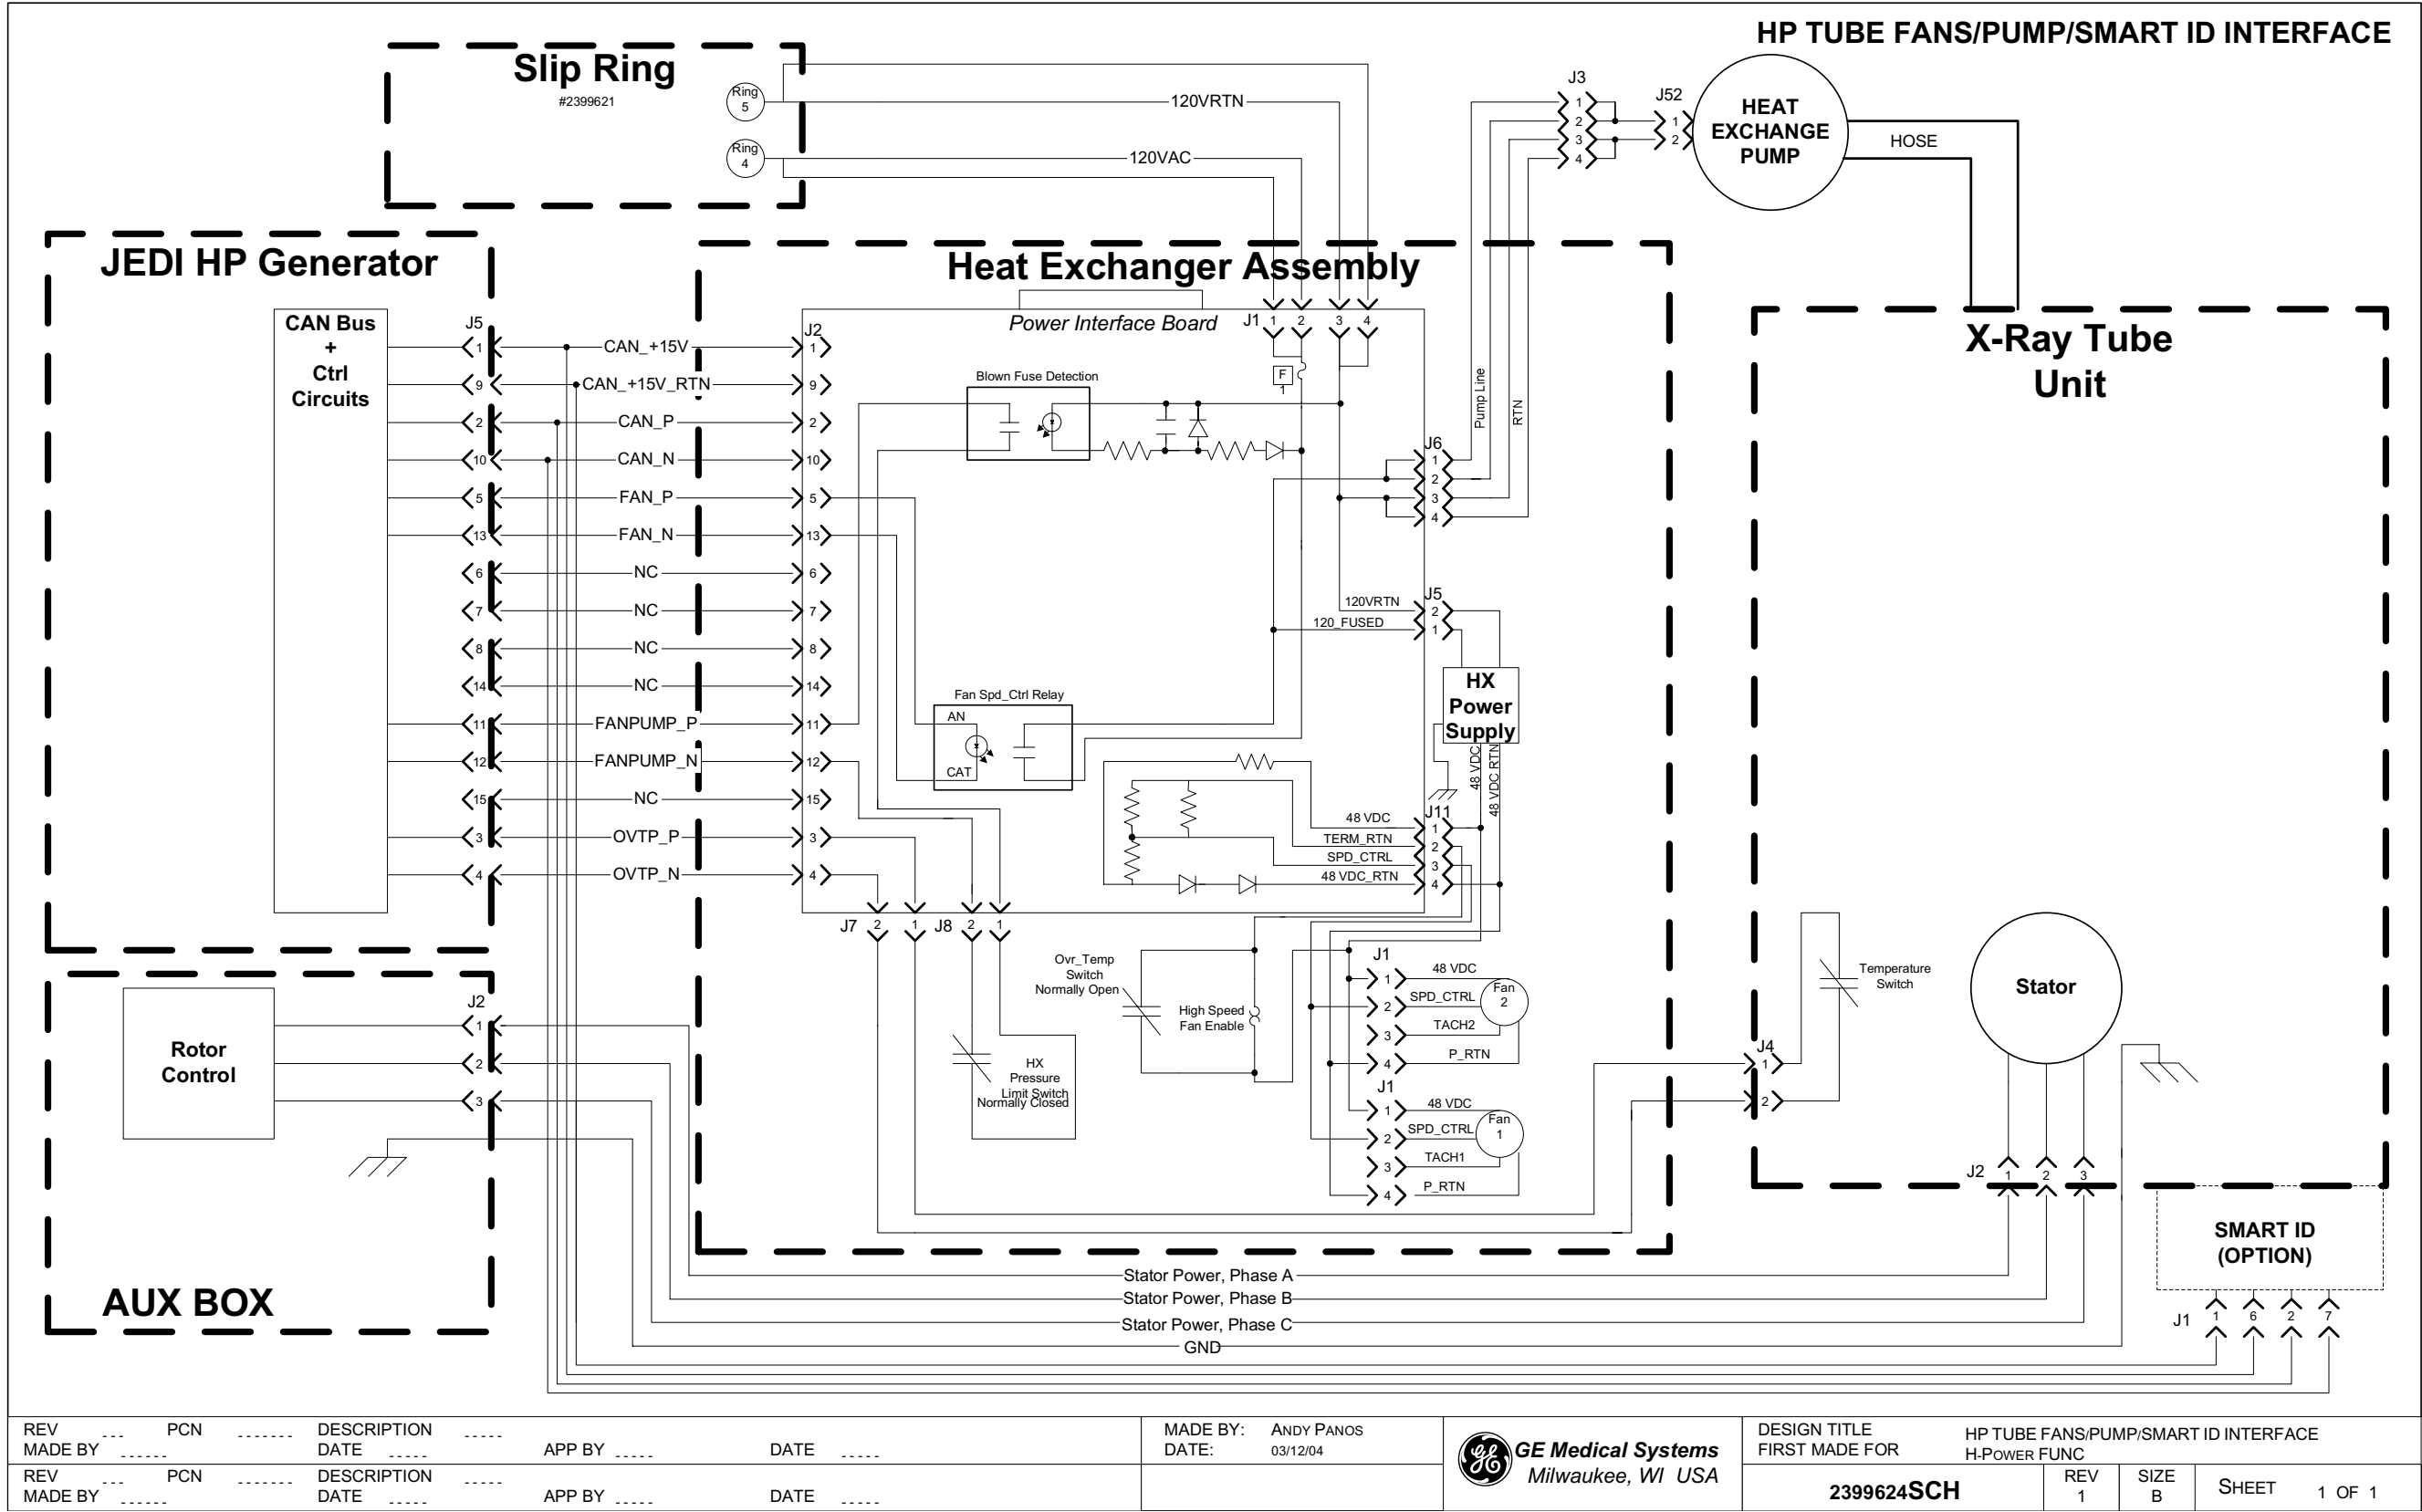

REV MADE BY	PCN	DESCRIPTION DATE	APP BY	DATE	MADE BY: DATE:	ANDY PANOS 03/12/04	 GE Medical Systems Milwaukee, WI USA	DESIGN TITLE FIRST MADE FOR		HP TUBE FANS/PUMP/SMART ID INTERFACE H-POWER FUNC			
REV MADE BY	PCN	DESCRIPTION DATE	APP BY	DATE				2399624SCH		REV 1	SIZE B	SHEET 1 OF 1	

Figure 2-1 2399624 Sheet 1, Rev. 1



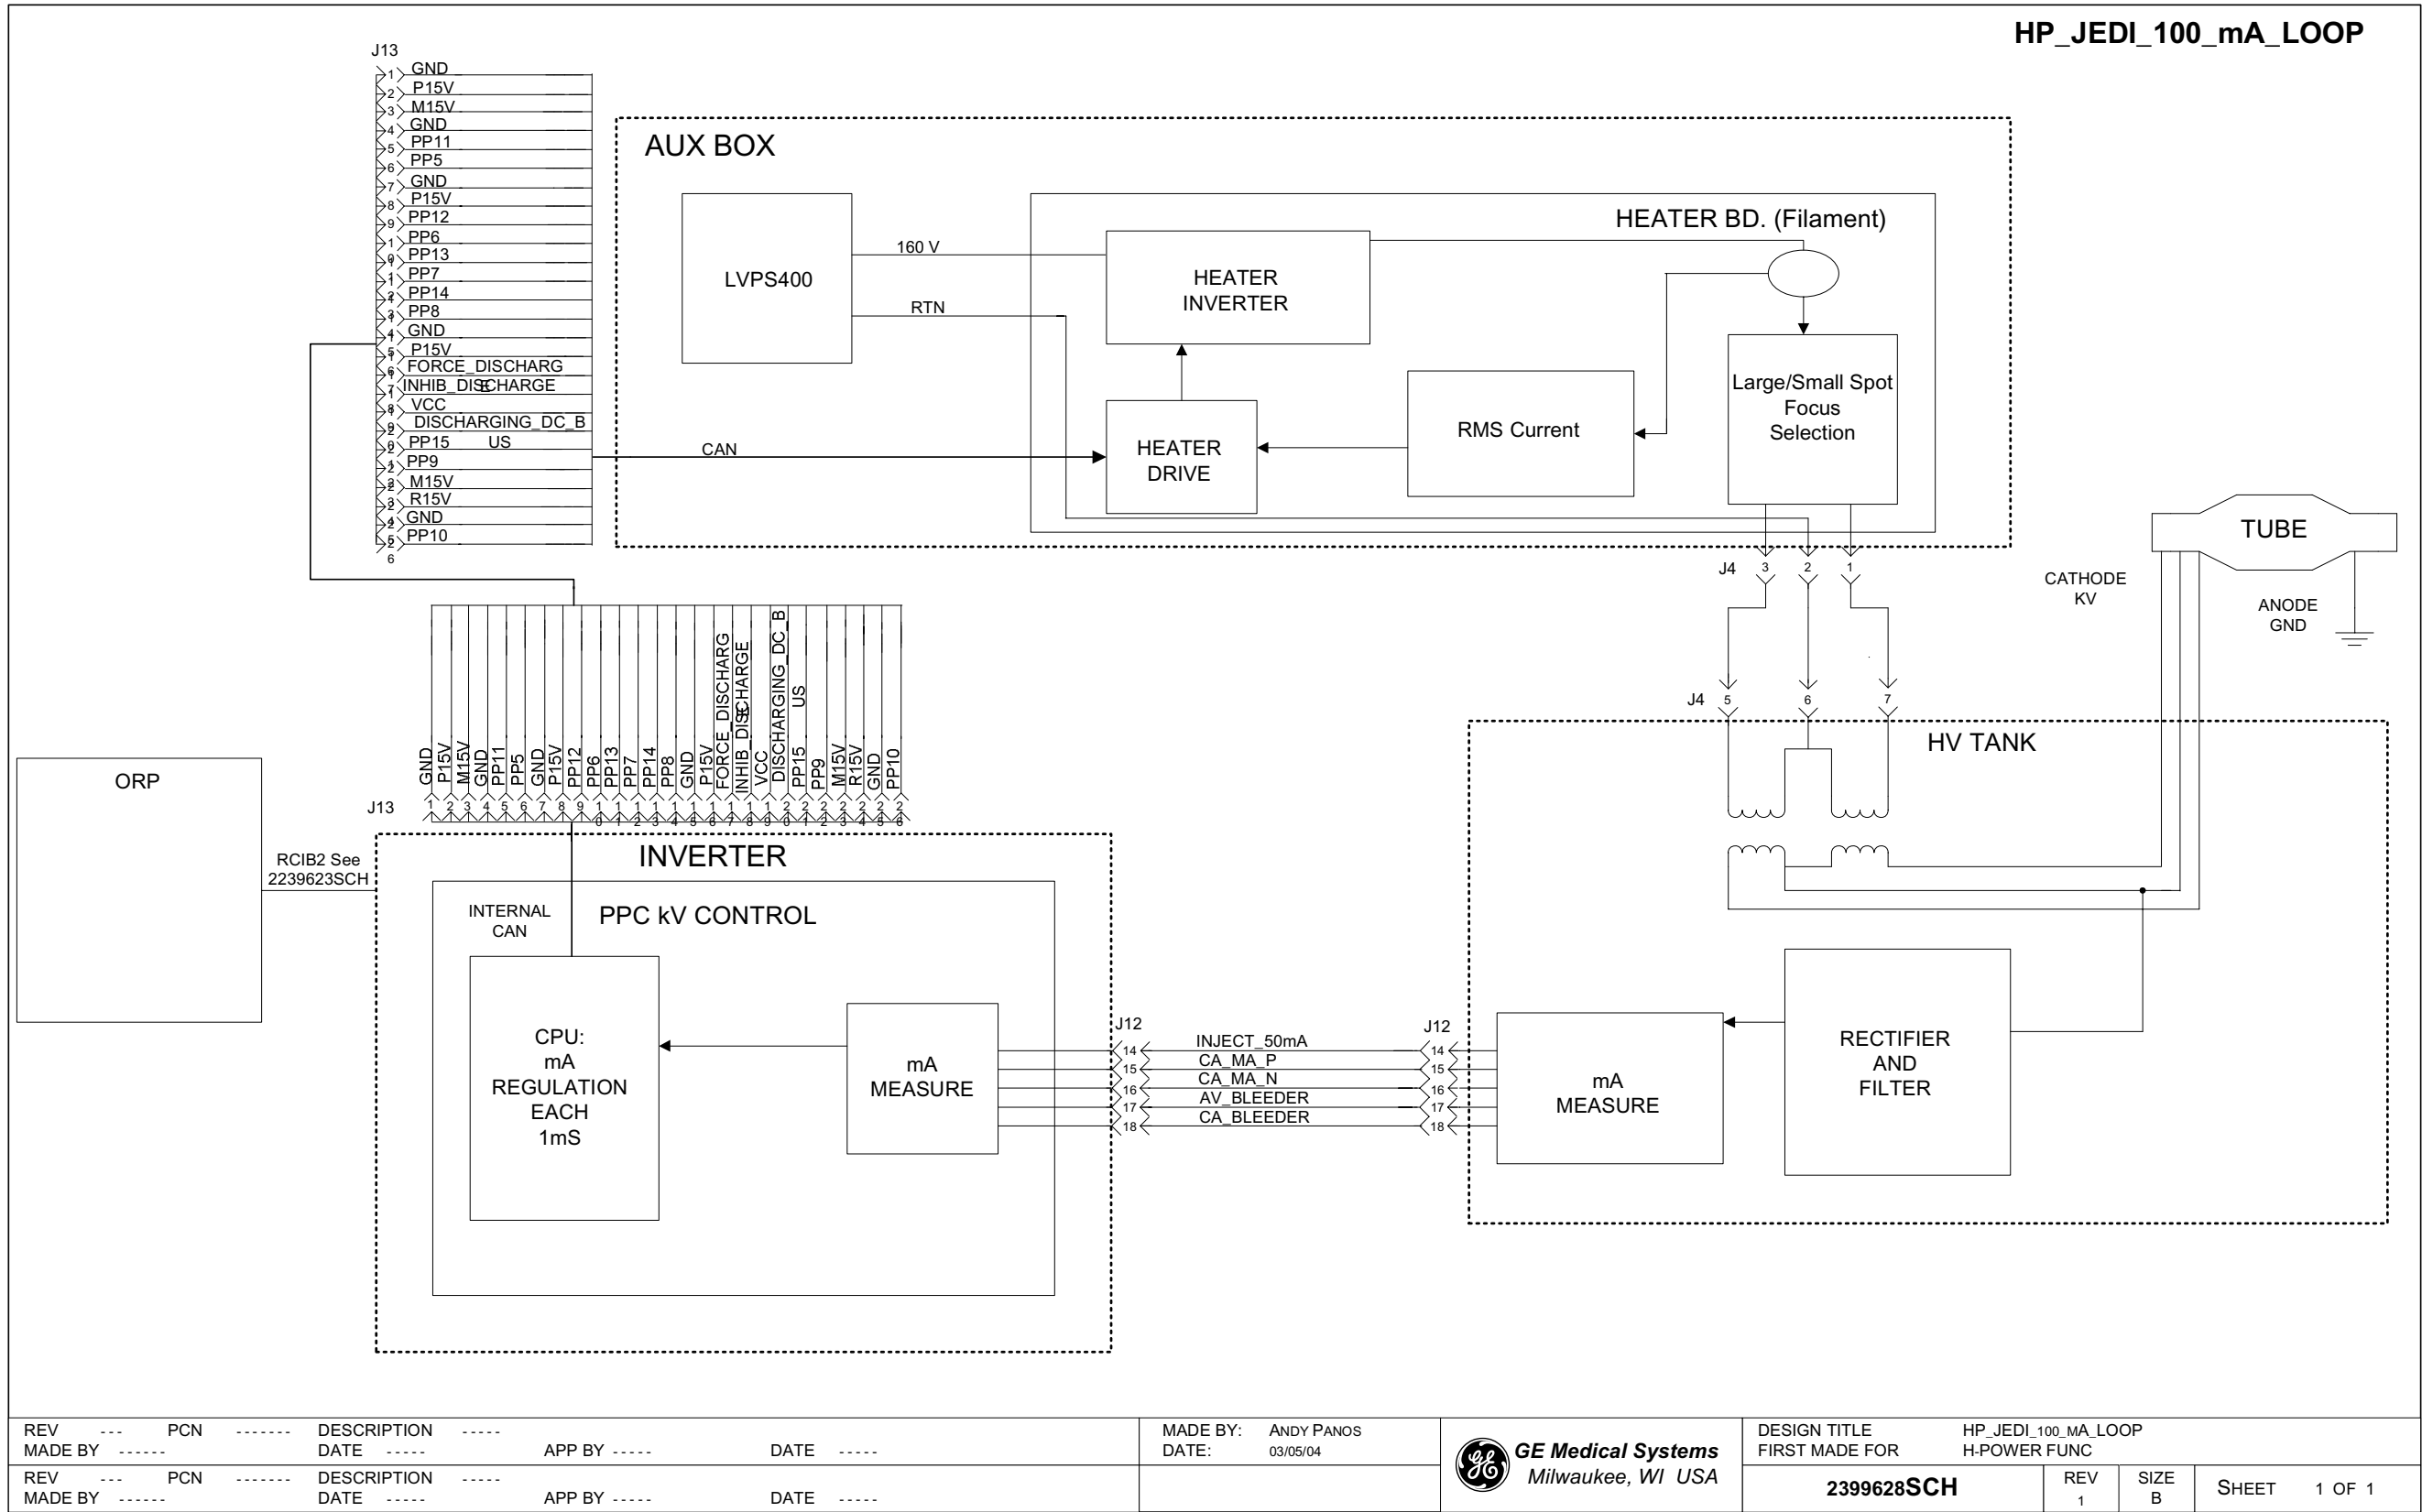

REV ---	PCN -----	DESCRIPTION -----	APP BY -----	DATE -----	MADE BY: ANDY PANOS	DESIGN TITLE HP_JEDI_100_mA_LOOP				
MADE BY -----		DATE -----			DATE: 03/05/04	FIRST MADE FOR H-POWER FUNC				
REV ---	PCN -----	DESCRIPTION -----	APP BY -----	DATE -----	 GE Medical Systems Milwaukee, WI USA	2399628SCH	REV 1	SIZE B	SHEET 1 OF 1	
MADE BY -----		DATE -----								

Figure 2-3 2399628 Sheet 1, Rev. 1

Section 4.0 — X-Ray Collimation & Filtration - 2399626


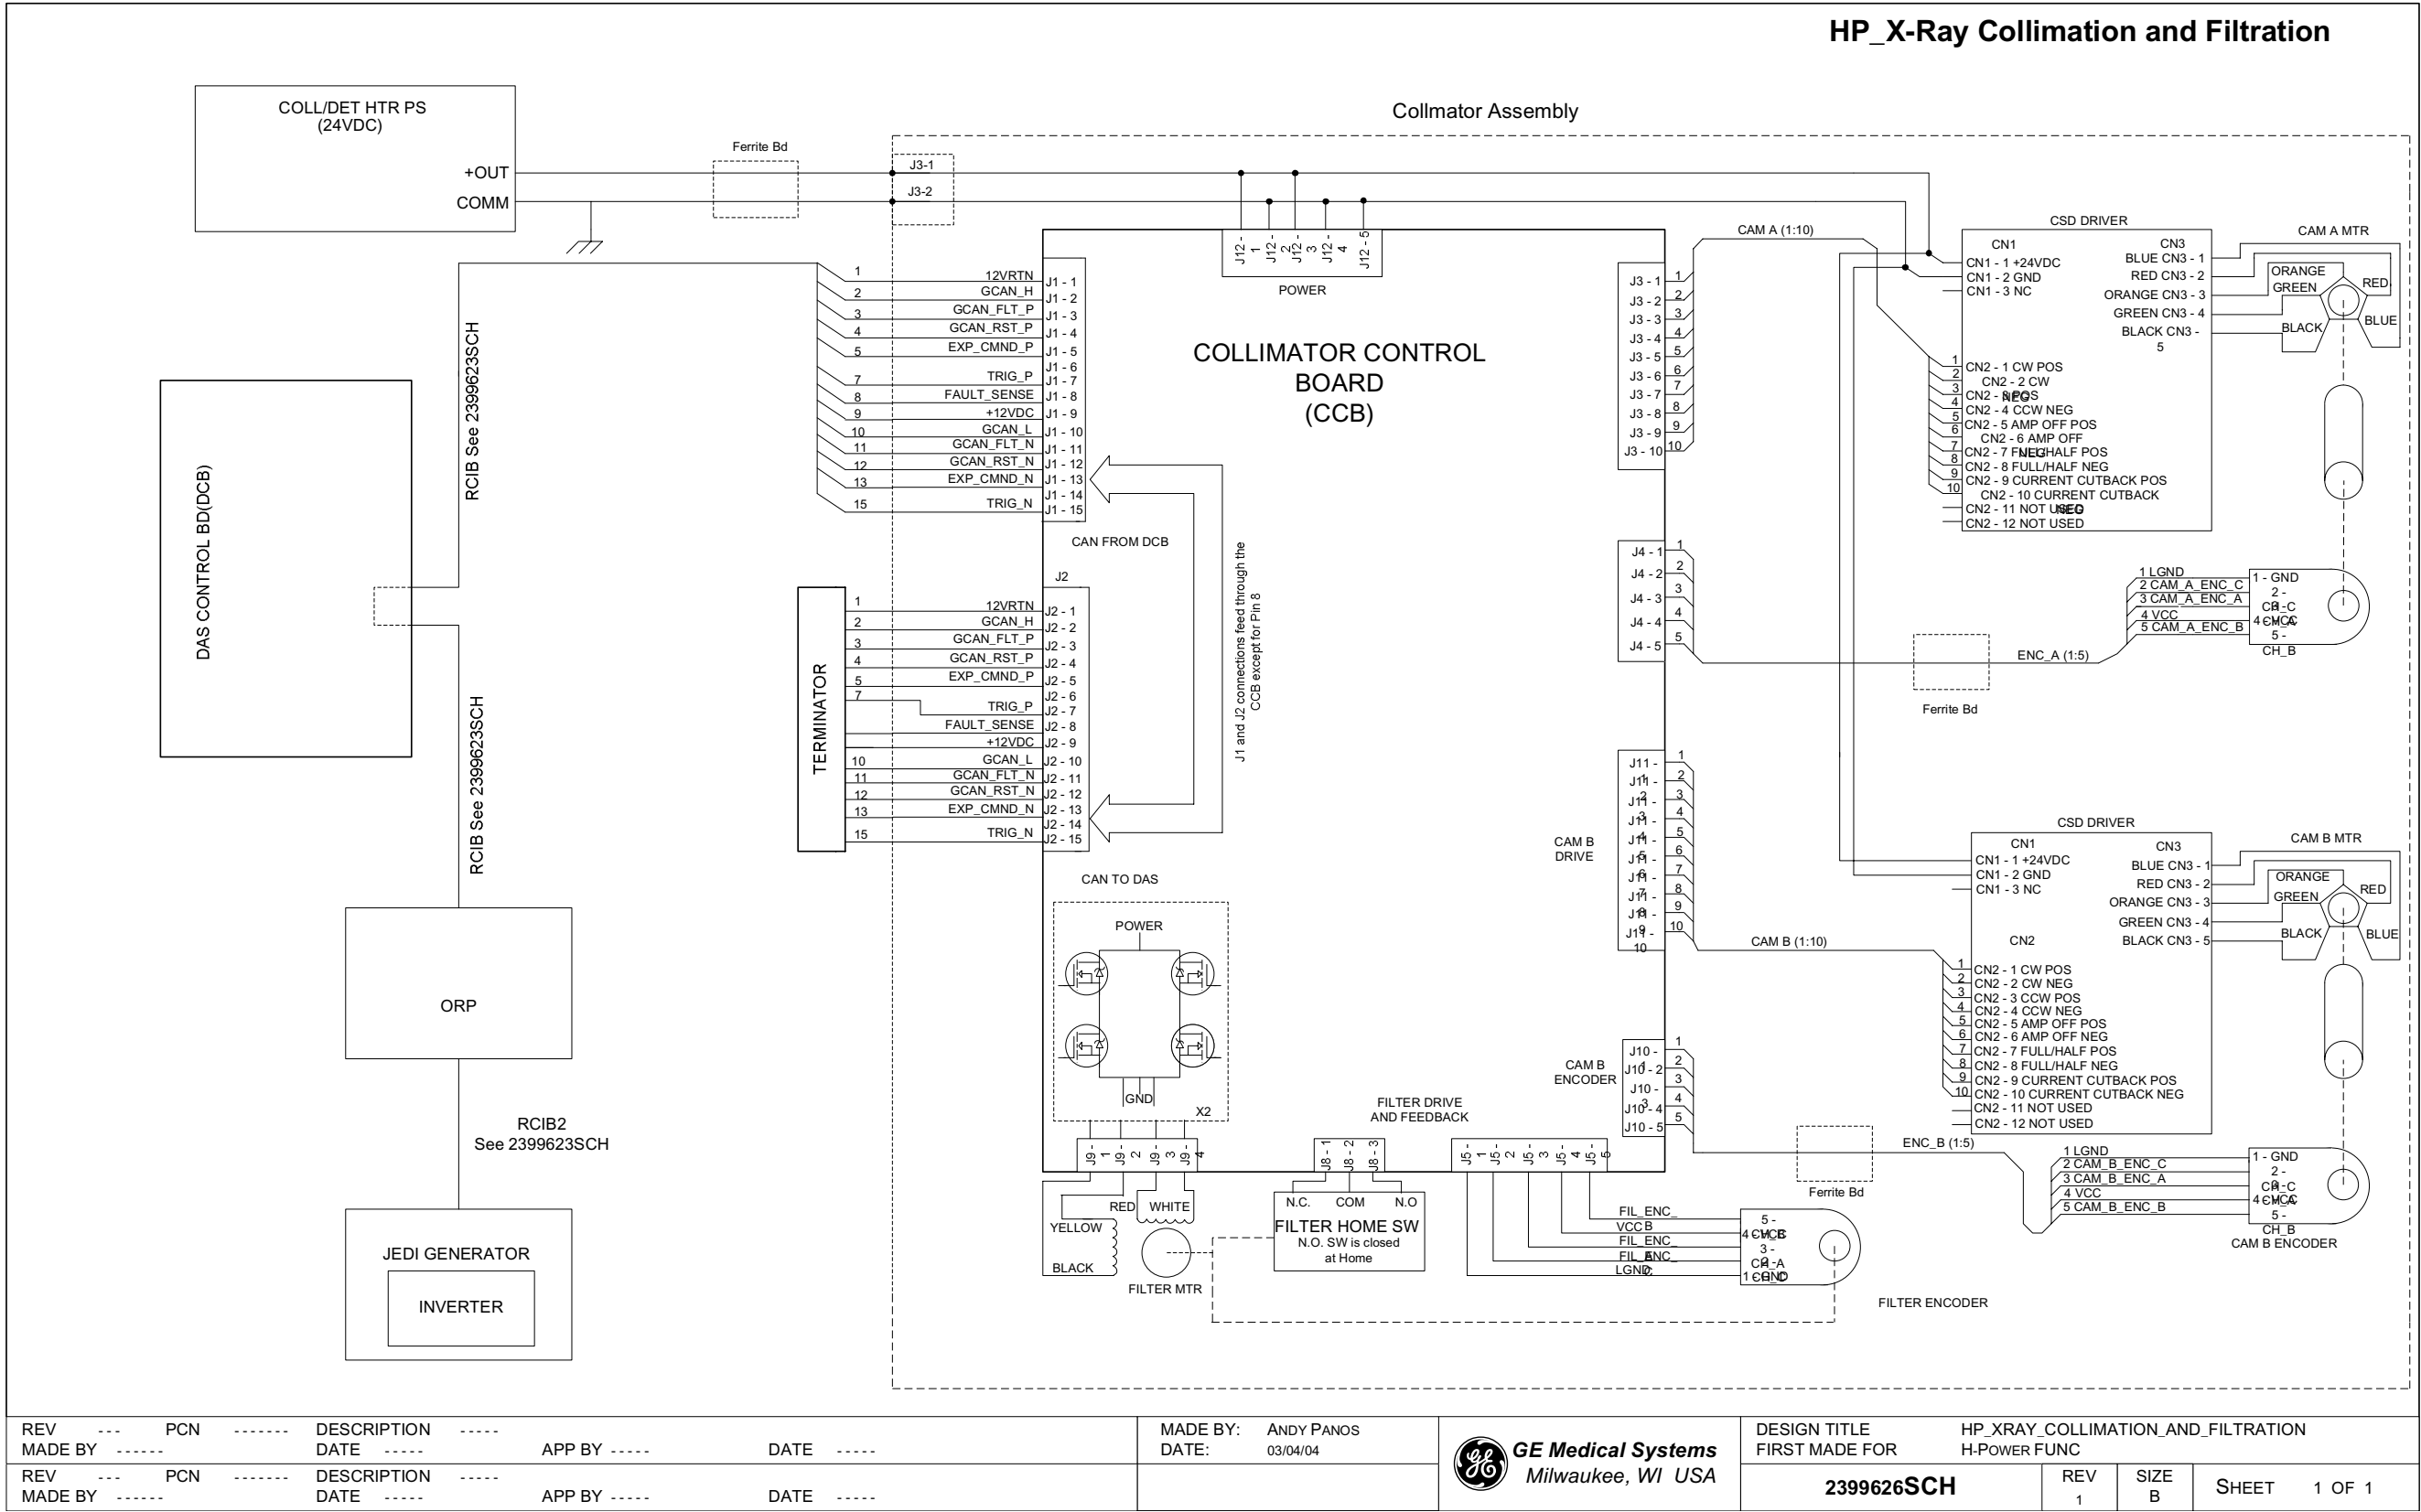



Figure 2-4 2399626 Sheet 1, Rev. 1

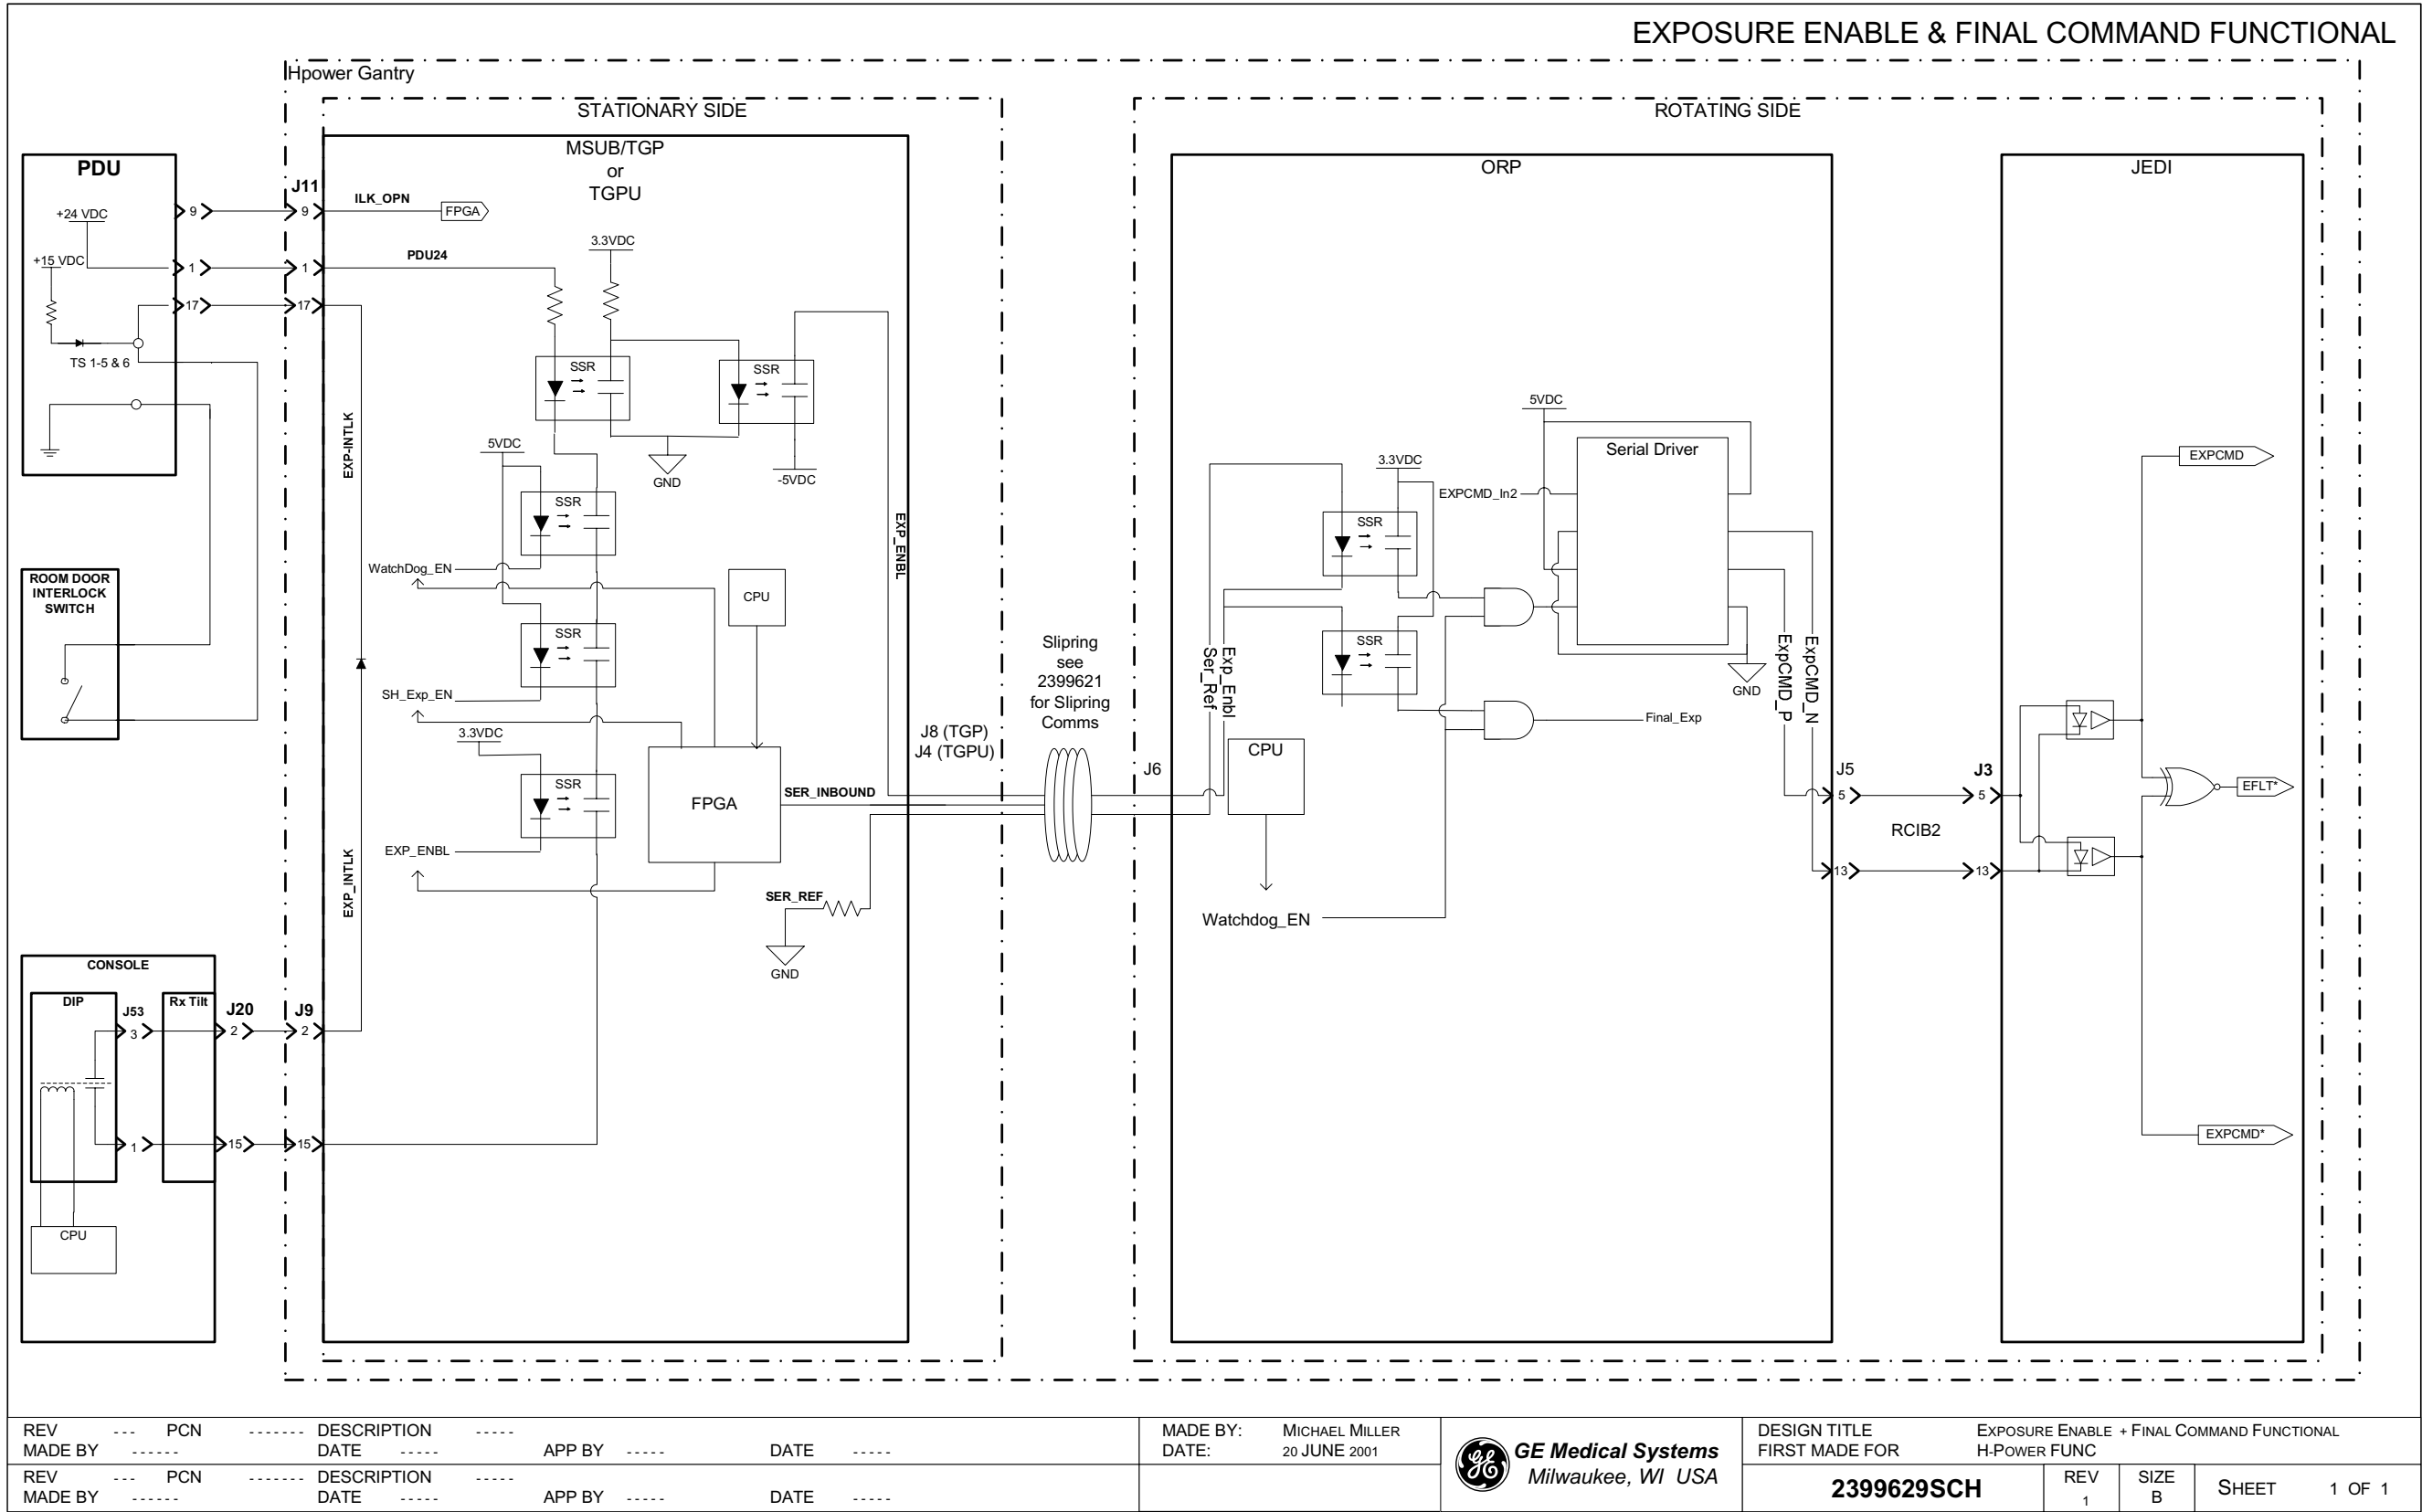

REV	PCN	DESCRIPTION	DATE	APP BY	DATE	MADE BY:	MICHAEL MILLER	 GE Medical Systems Milwaukee, WI USA	DESIGN TITLE	EXPOSURE ENABLE + FINAL COMMAND FUNCTIONAL			
MADE BY						DATE:	20 JUNE 2001		FIRST MADE FOR	H-POWER FUNC			
REV	PCN	DESCRIPTION	DATE	APP BY	DATE				2399629SCH	REV	SIZE	SHEET	1 OF 1
MADE BY										1	B		

Figure 2-5 2399629 Sheet 1, Rev. 1

Section 6.0 — Tube Rotor Control - 2399630

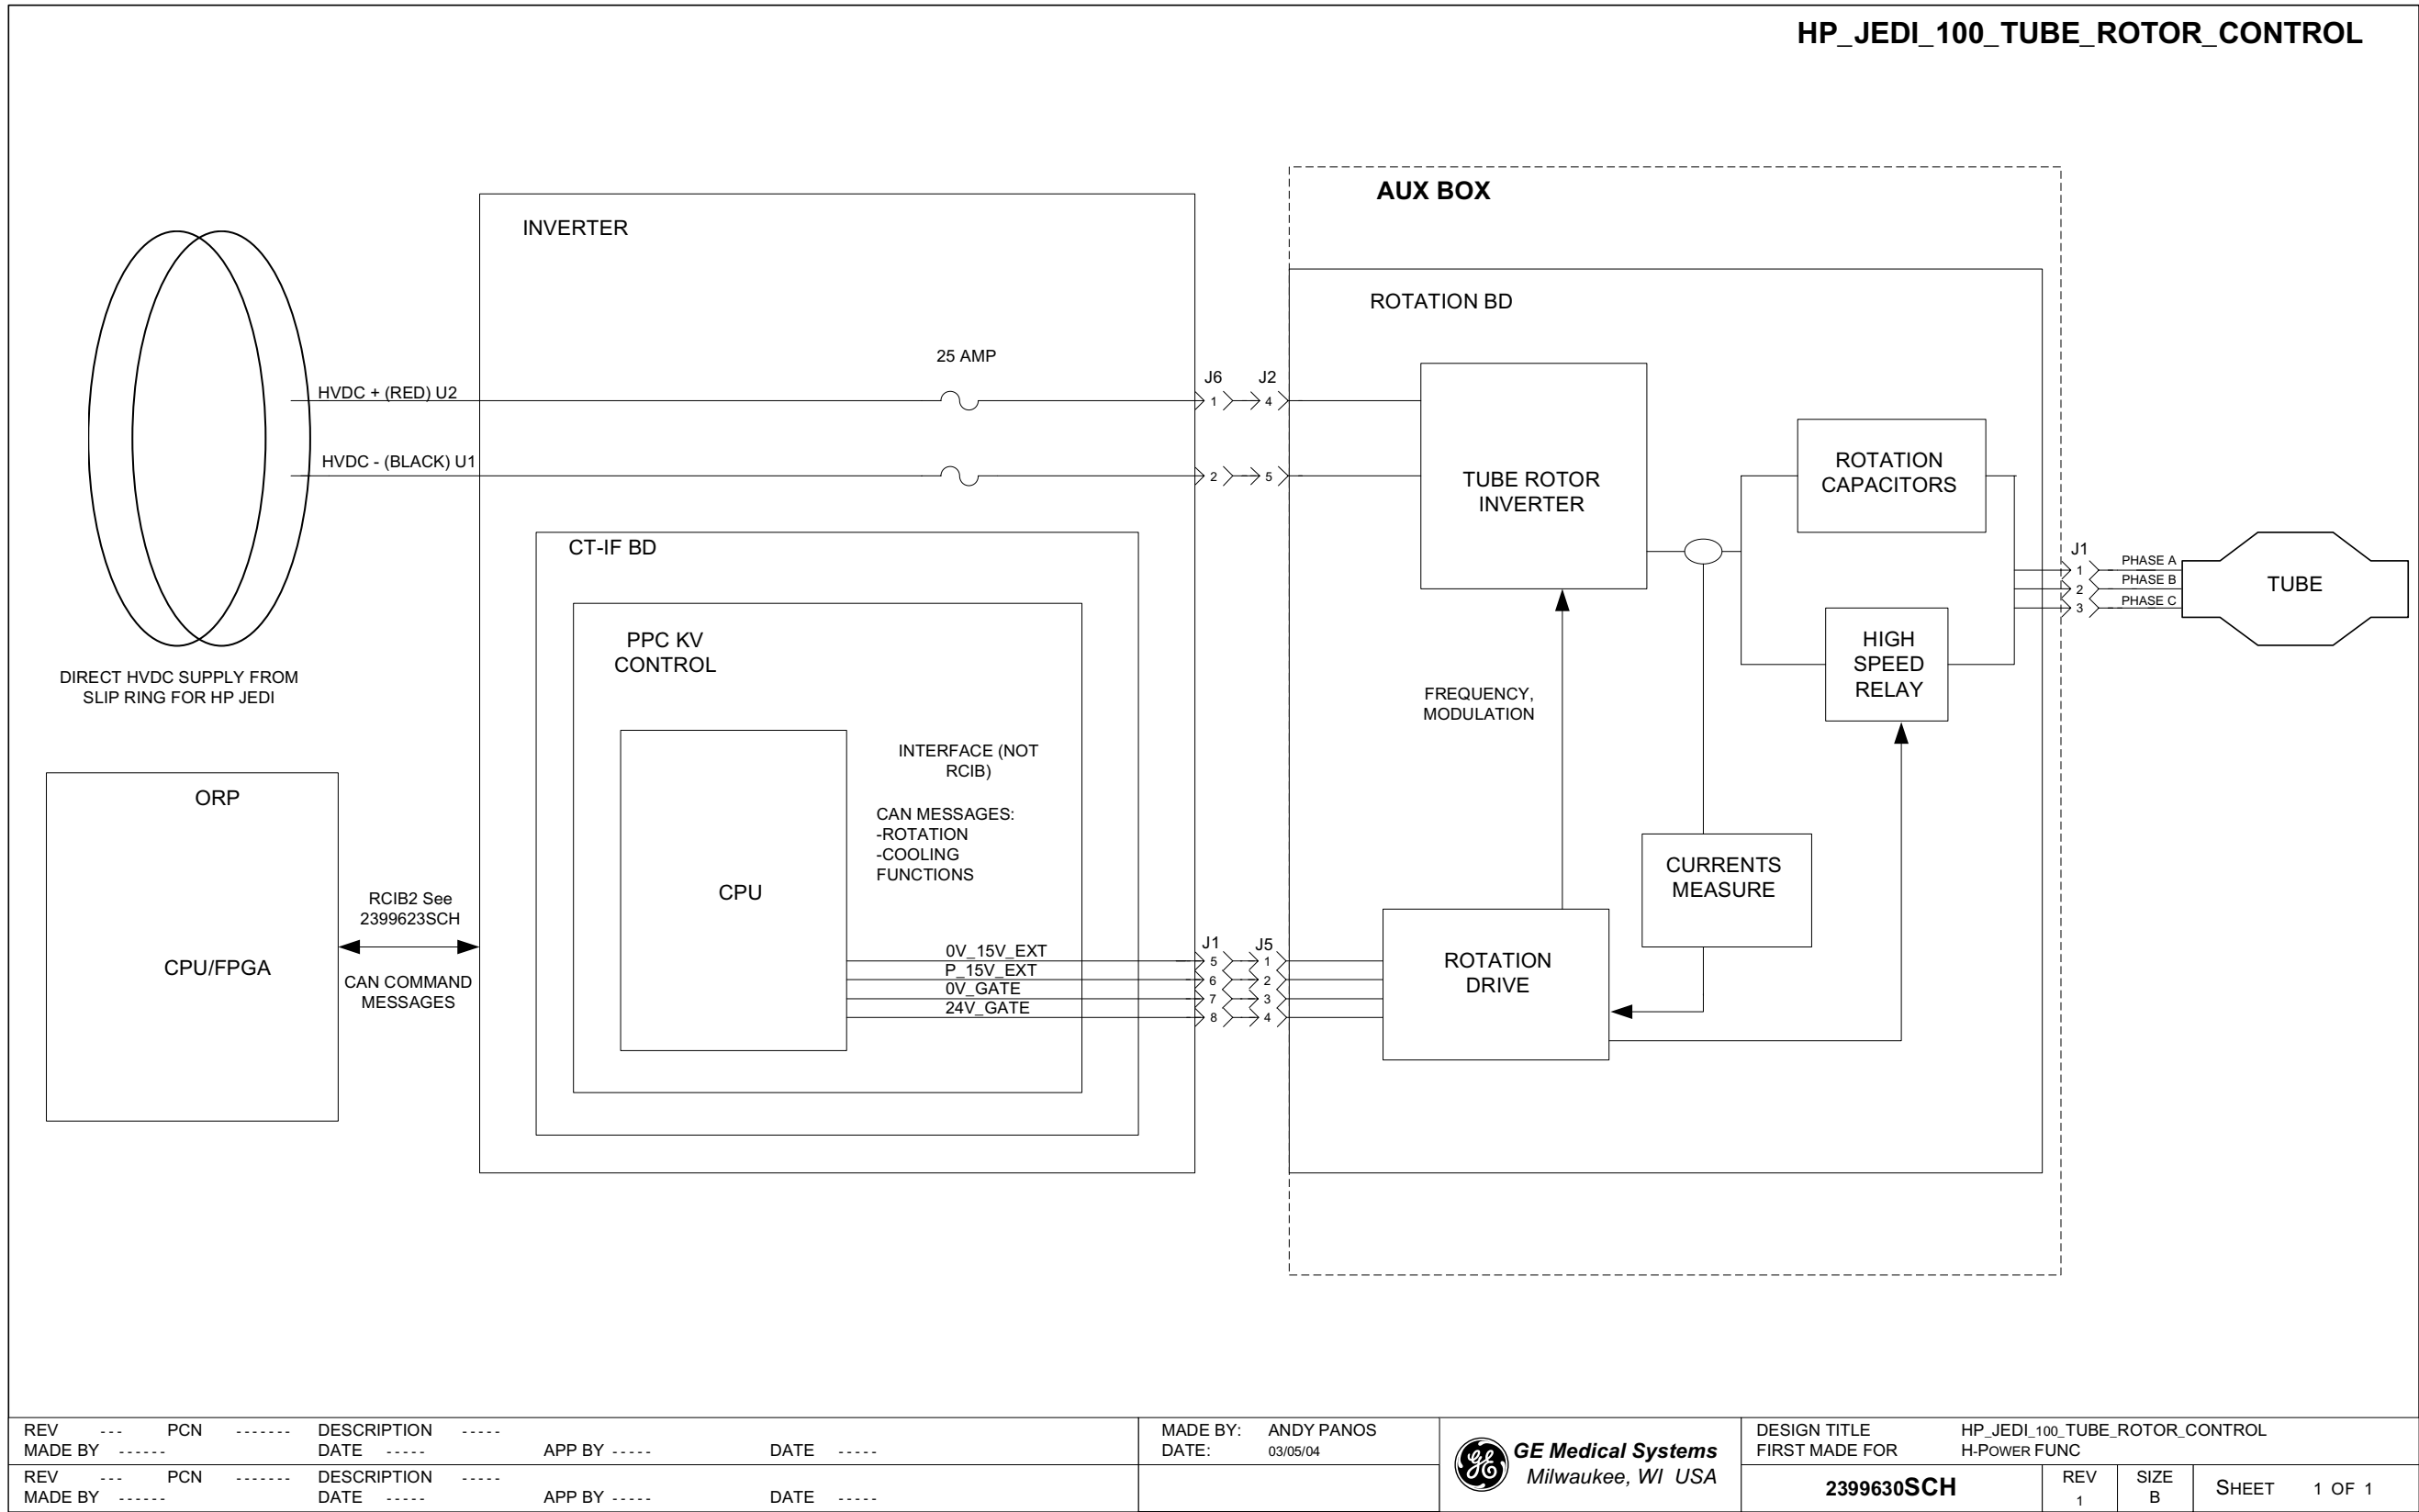

REV --- PCN ----- DESCRIPTION -----	MADE BY: ANDY PANOS	 GE Medical Systems Milwaukee, WI USA	DESIGN TITLE HP_JEDI_100_TUBE_ROTOR_CONTROL				
MADE BY ----- DATE ----- APP BY ----- DATE -----	DATE: 03/05/04		FIRST MADE FOR H-POWER FUNC				
REV --- PCN ----- DESCRIPTION -----			2399630SCH		REV 1	SIZE B	SHEET 1 OF 1
MADE BY ----- DATE ----- APP BY ----- DATE -----							

Figure 2-6 2399630 Sheet 1, Rev. 1

Section 7.0 — HP X-Ray Tube Coolant Flow - 2399628

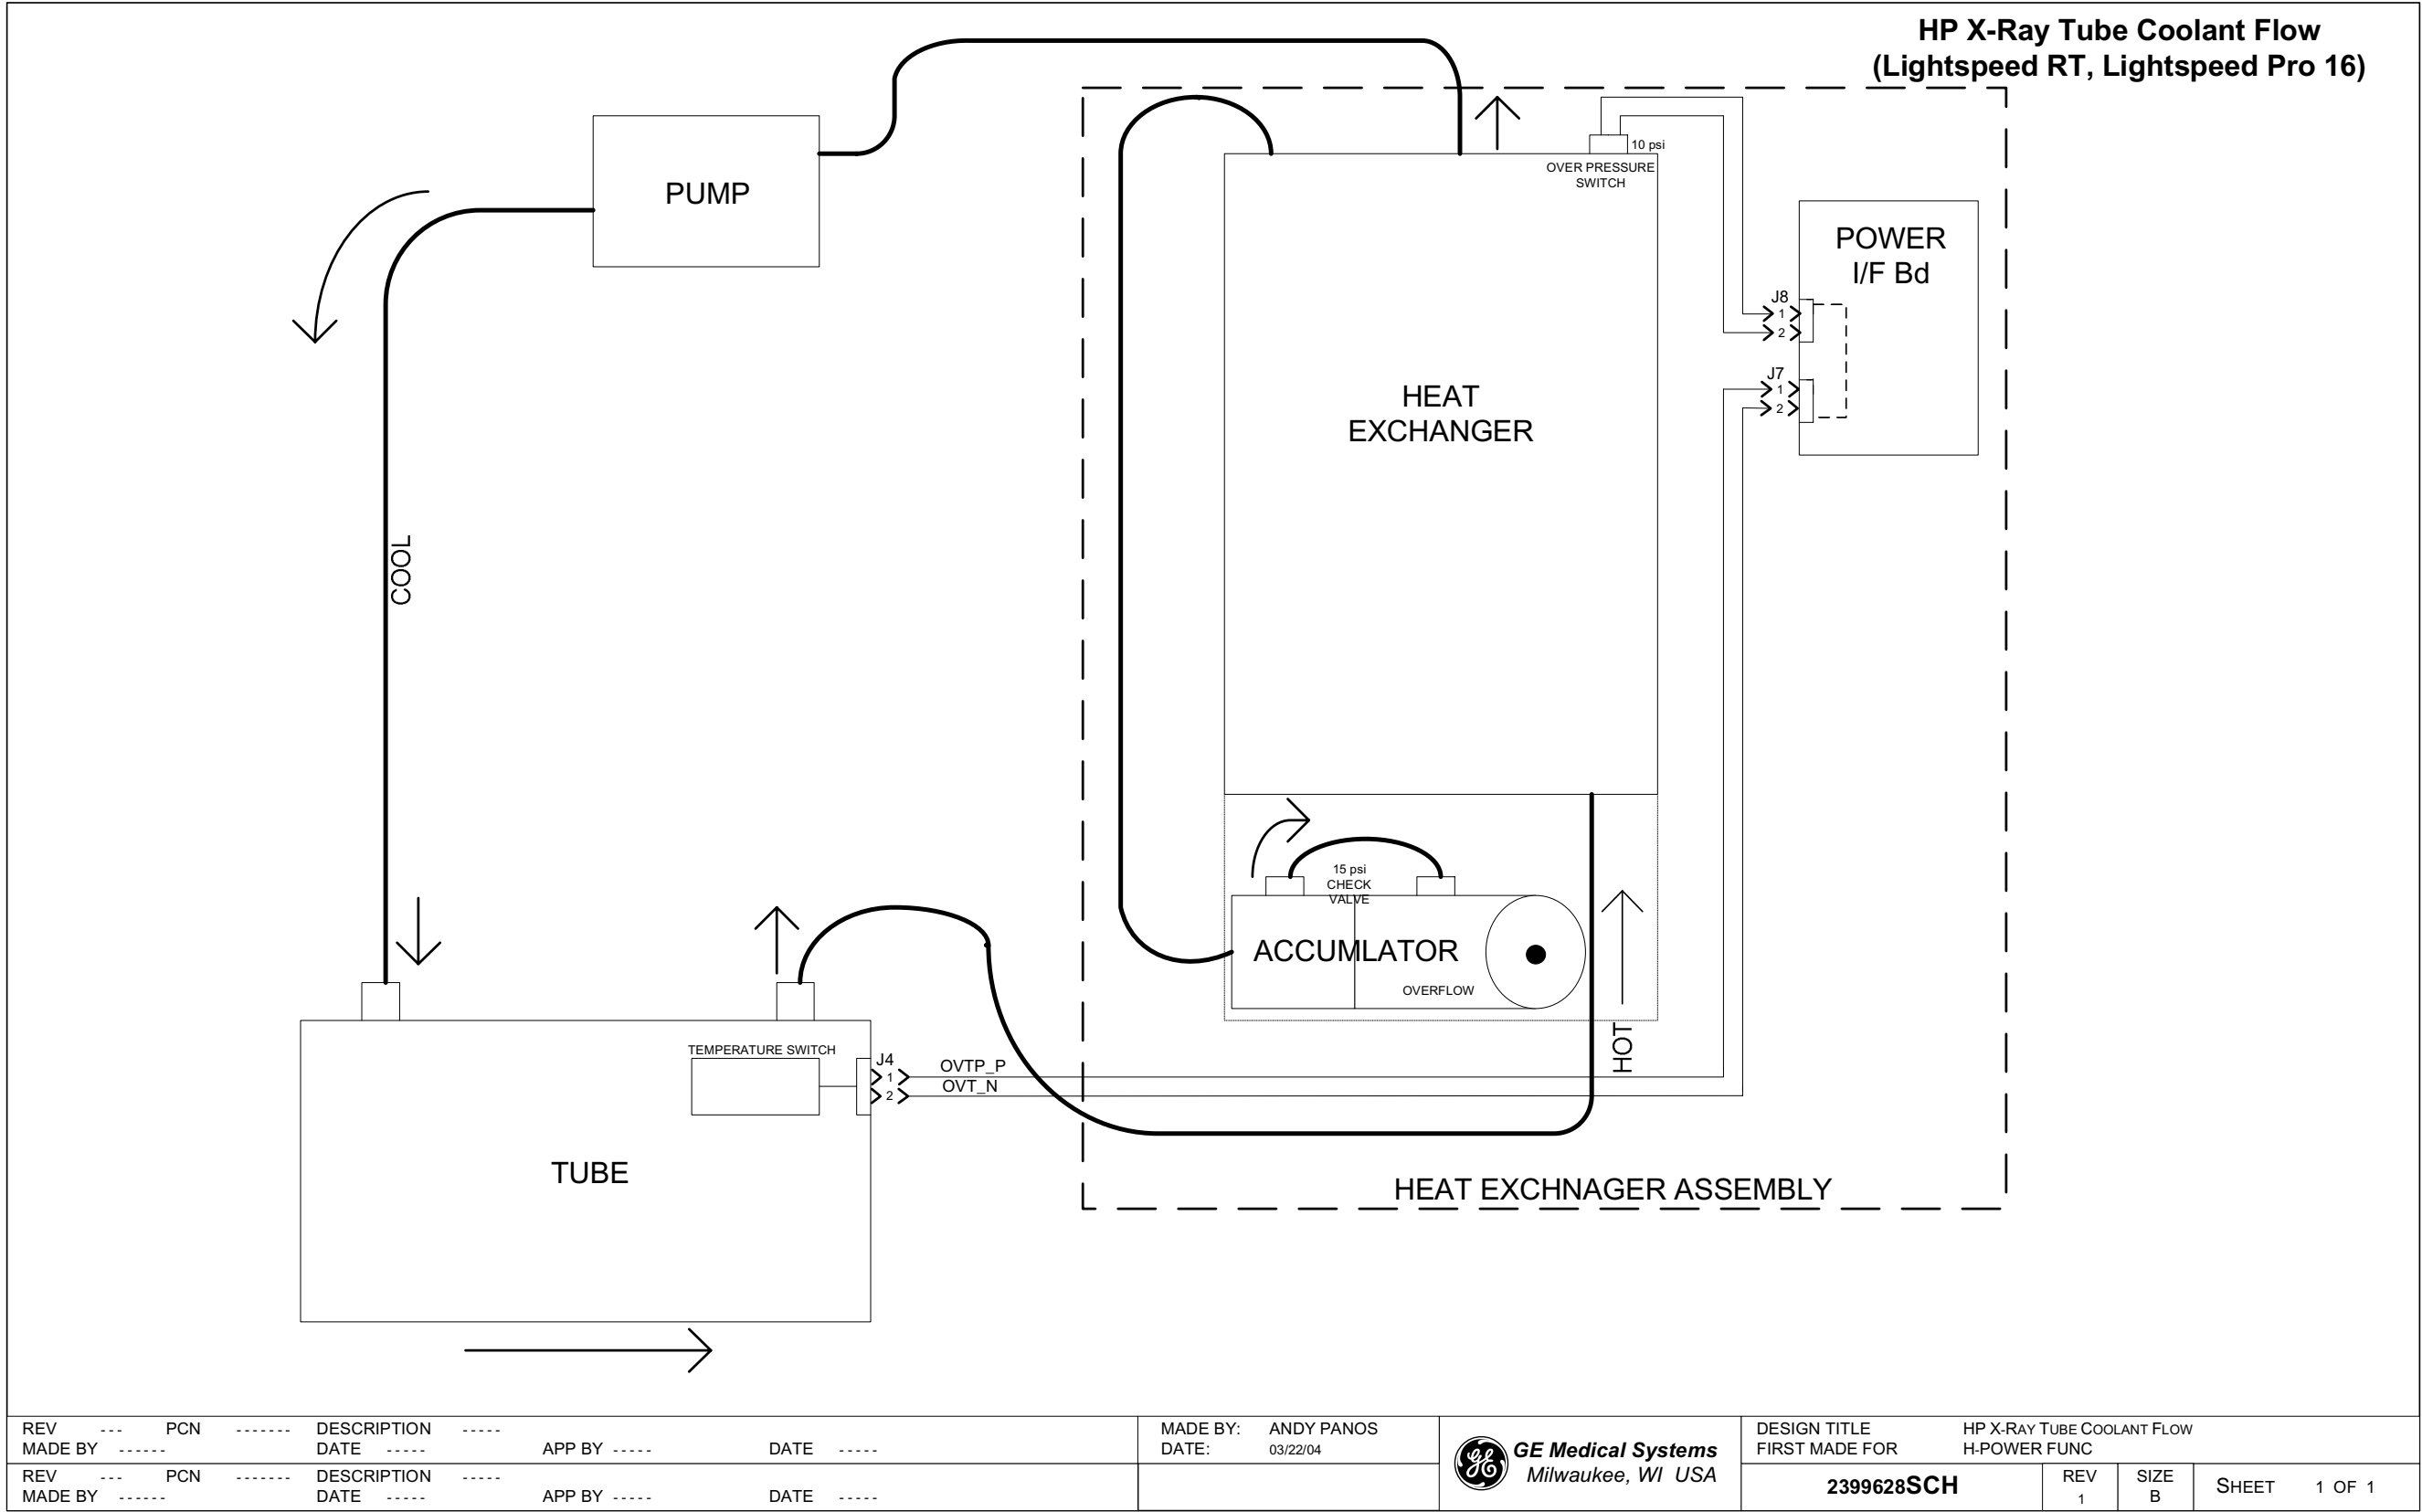


Figure 2-7 2399628 Sheet 1, Rev. 1

Chapter 3

Data Acquisition

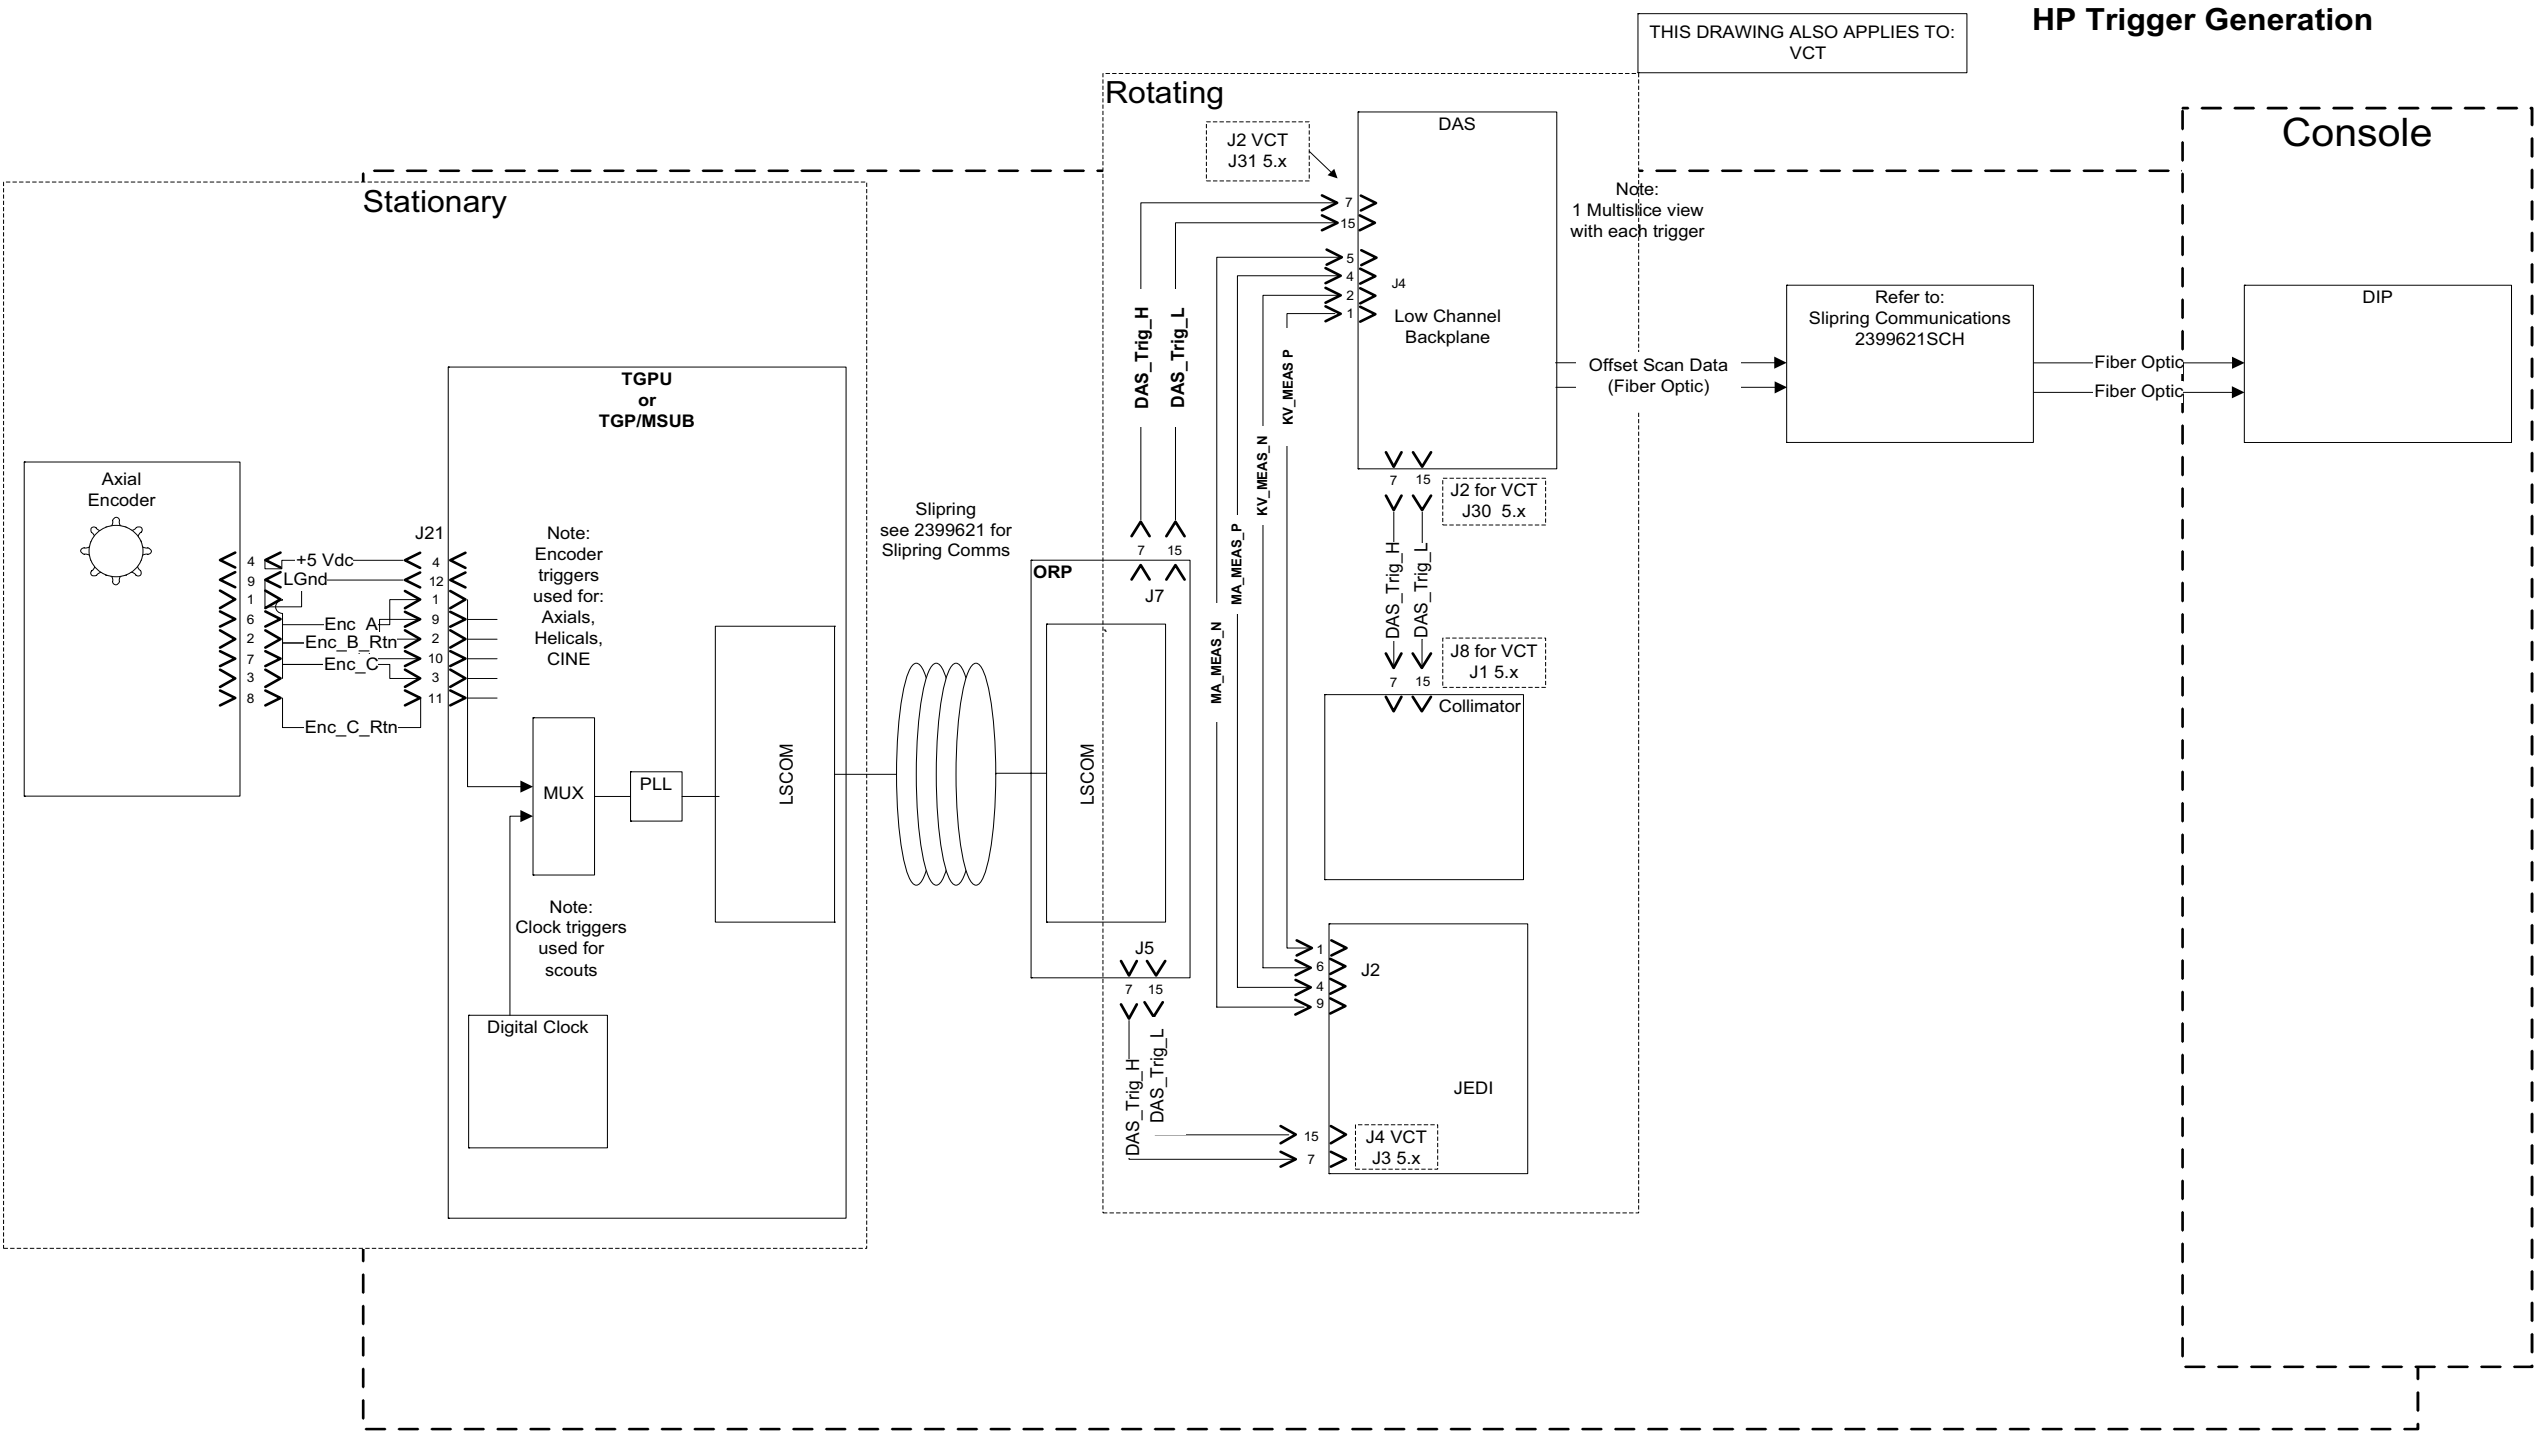


Figure 3-1 2399724 Sheet 1, Rev. 2

Section 2.0 — Detector Heater (DAS Item) - 2399725

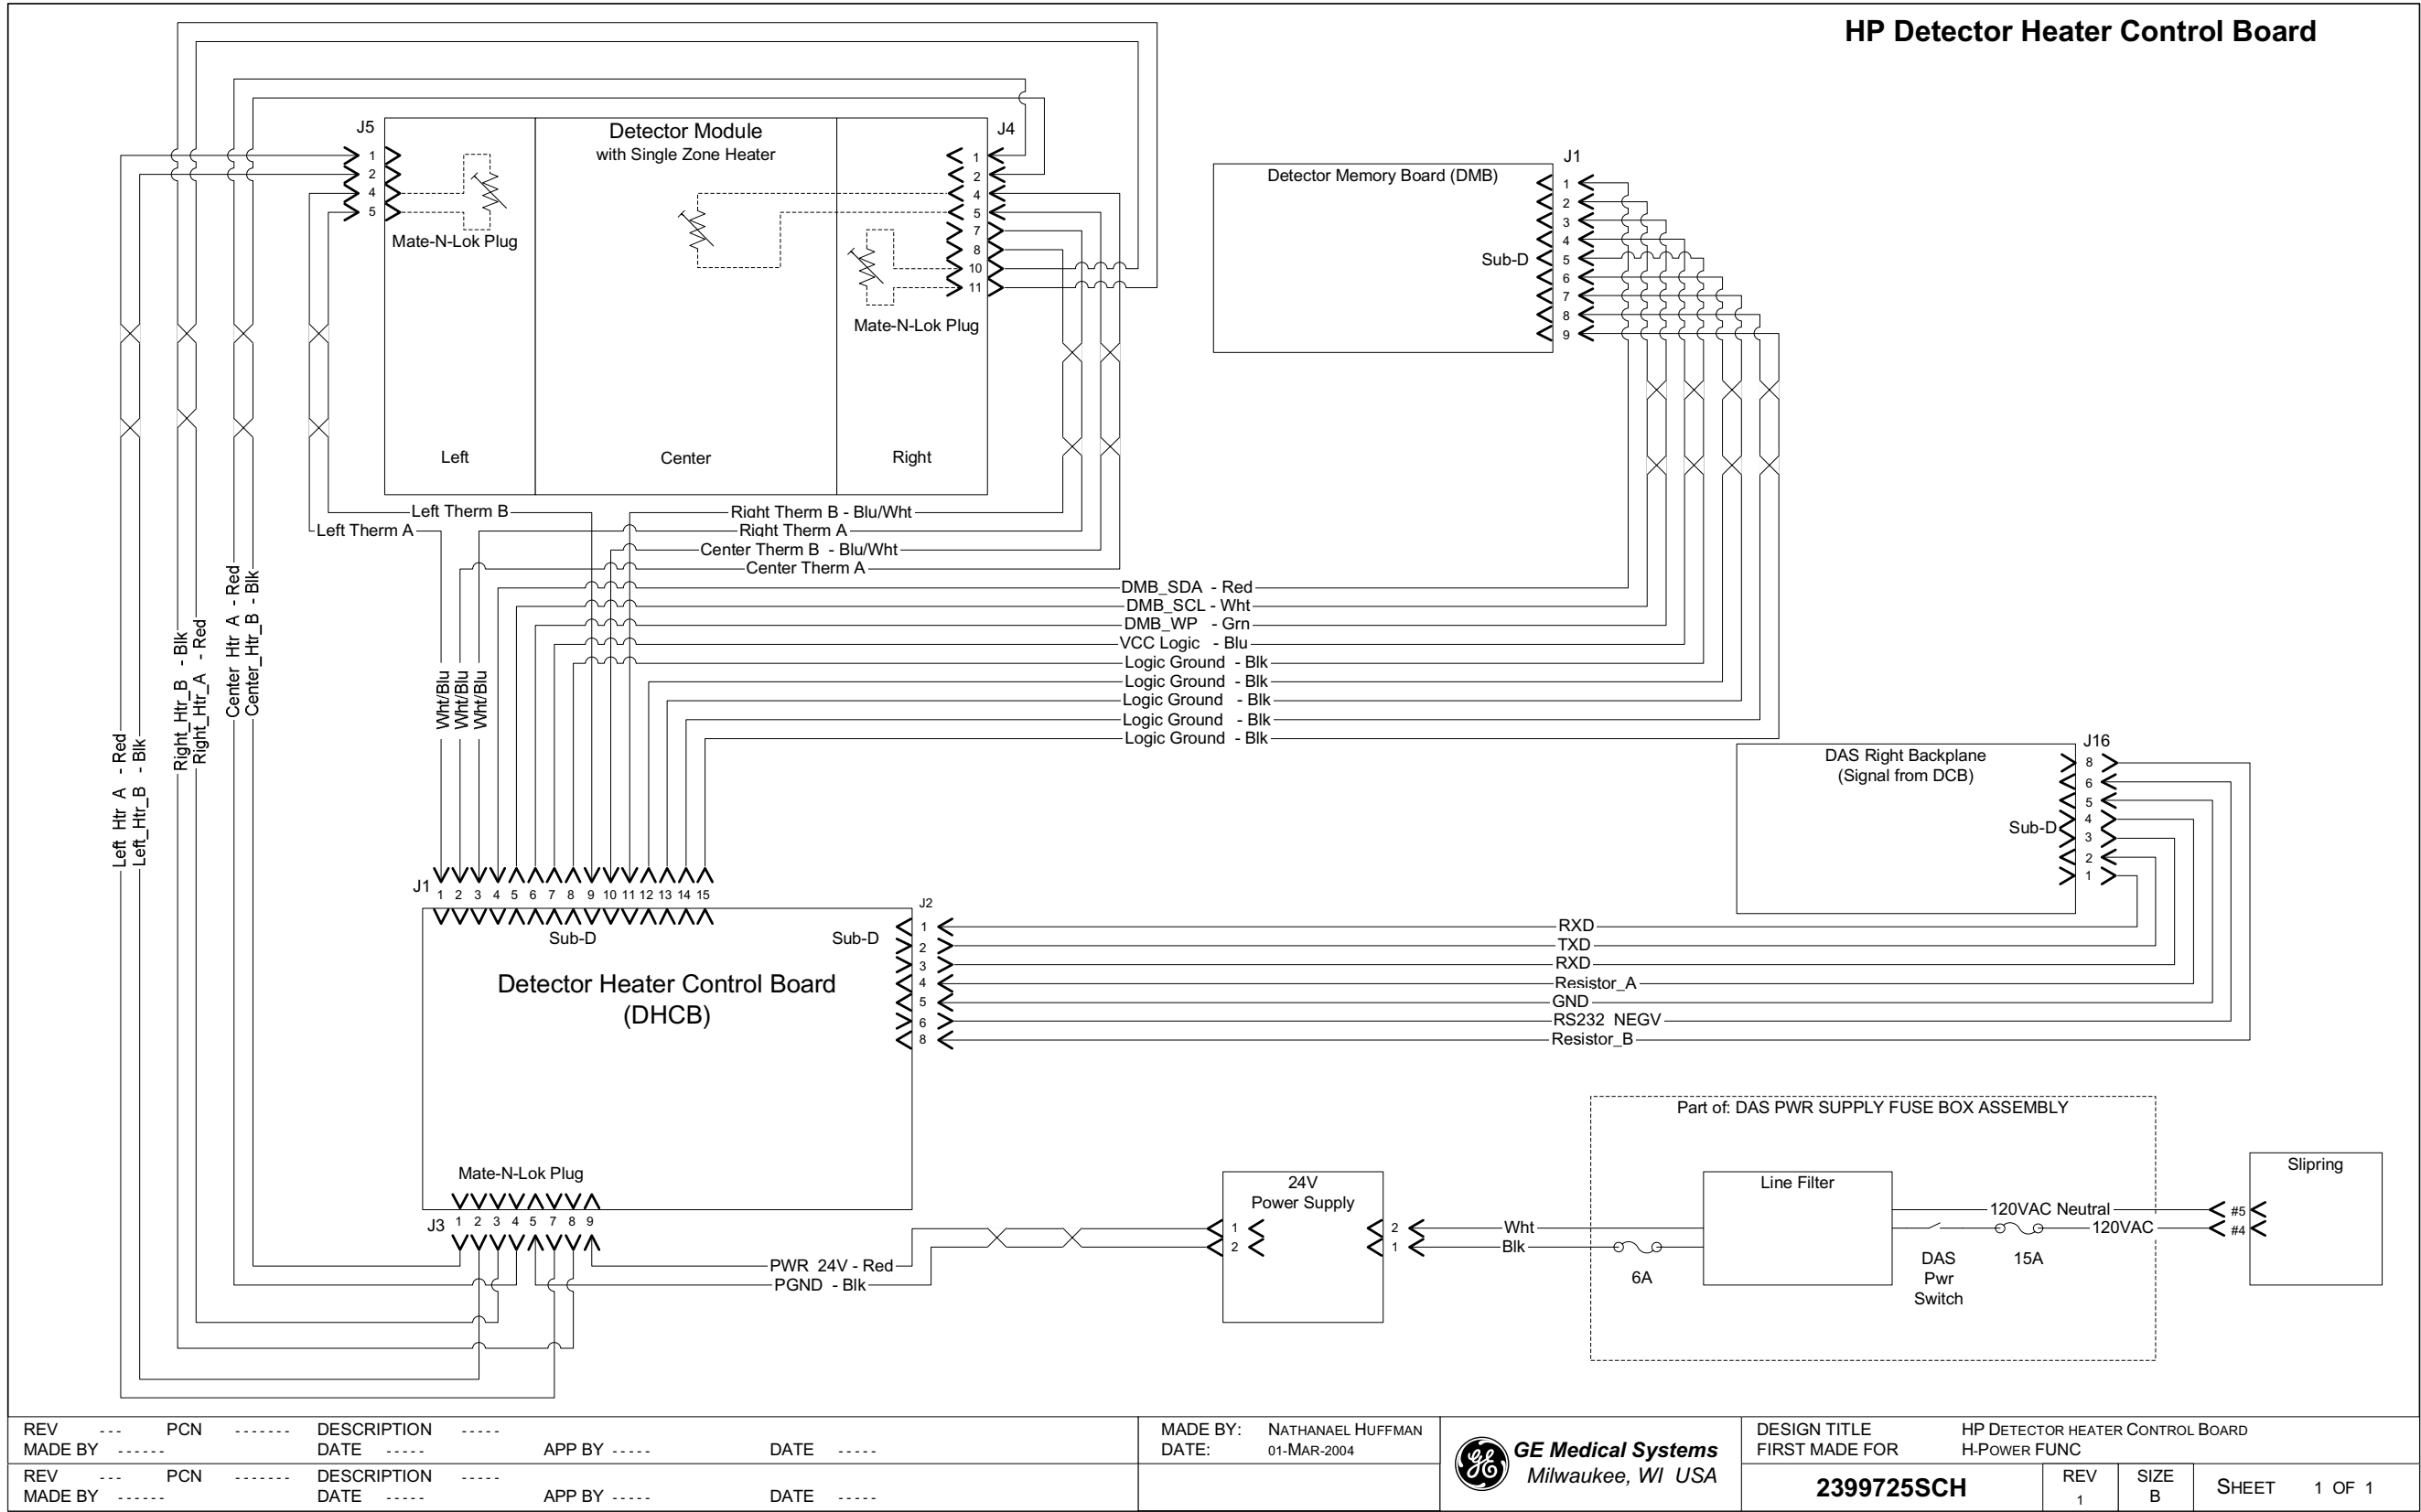



Figure 3-2 2399725 Sheet 1, Rev. 1

THIS PAGE INTENTIONALLY BLANK.

Chapter 4

Patient Positioning

Section 1.0 — Alignment Lights - 2399726

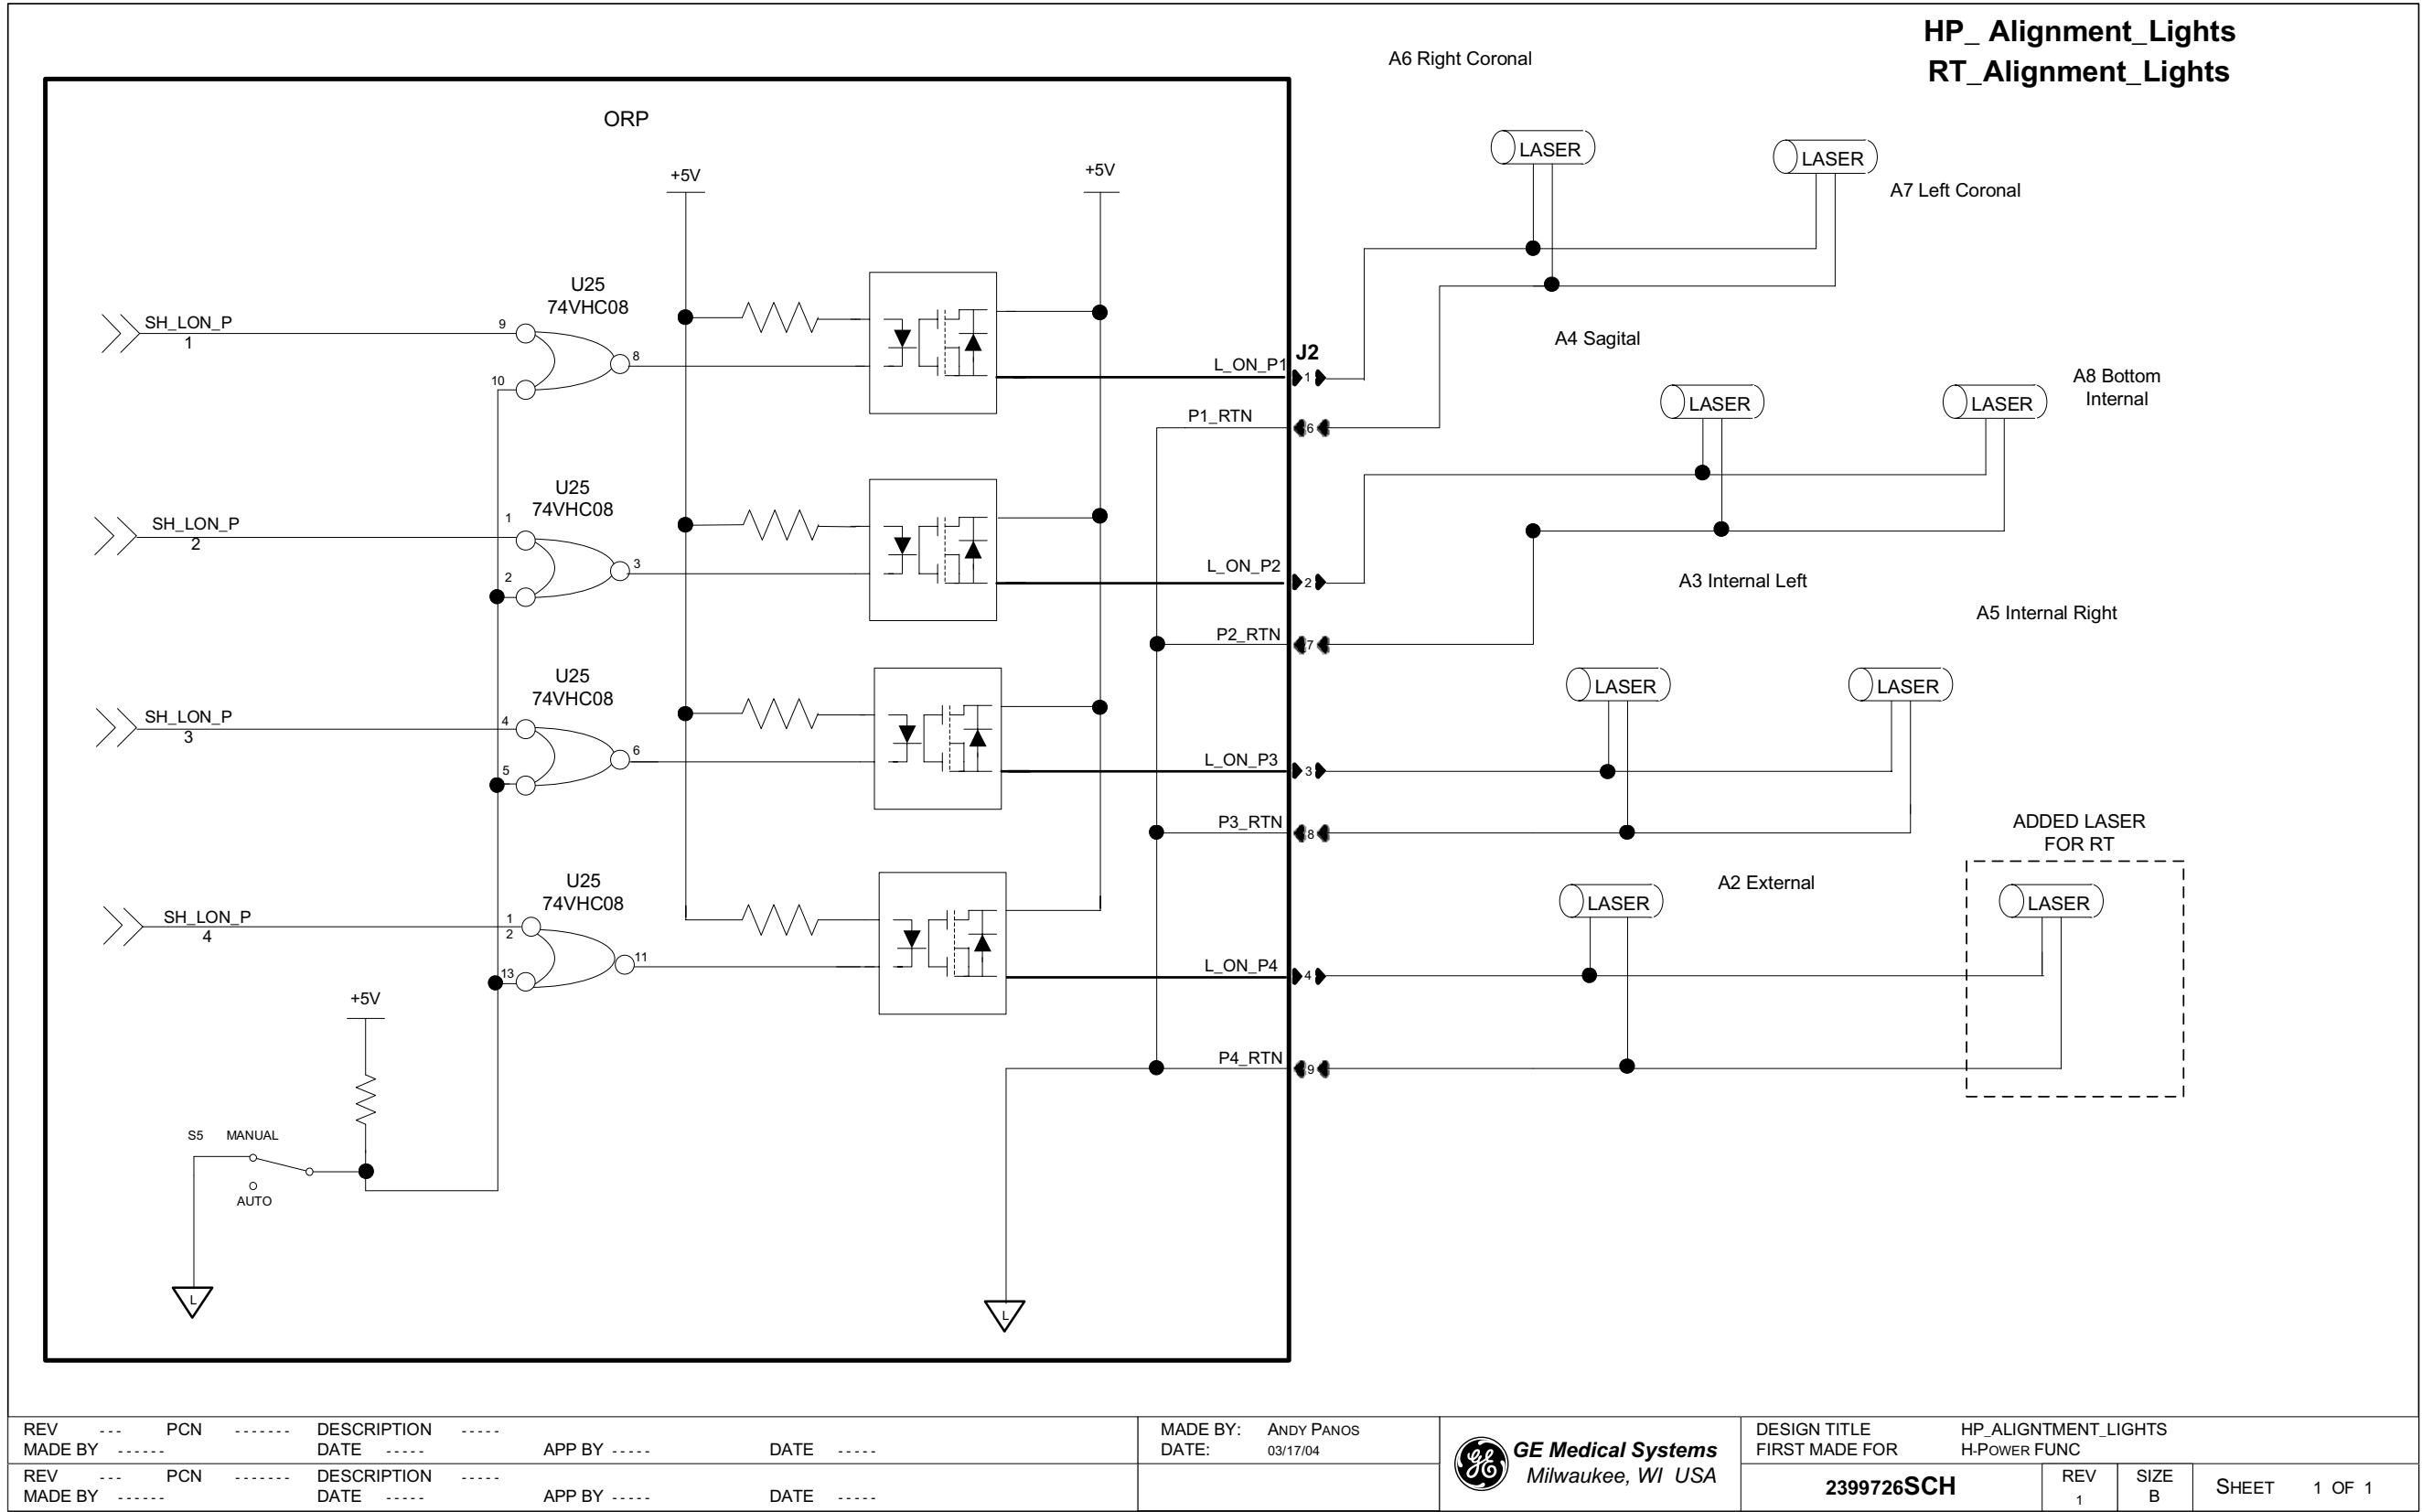


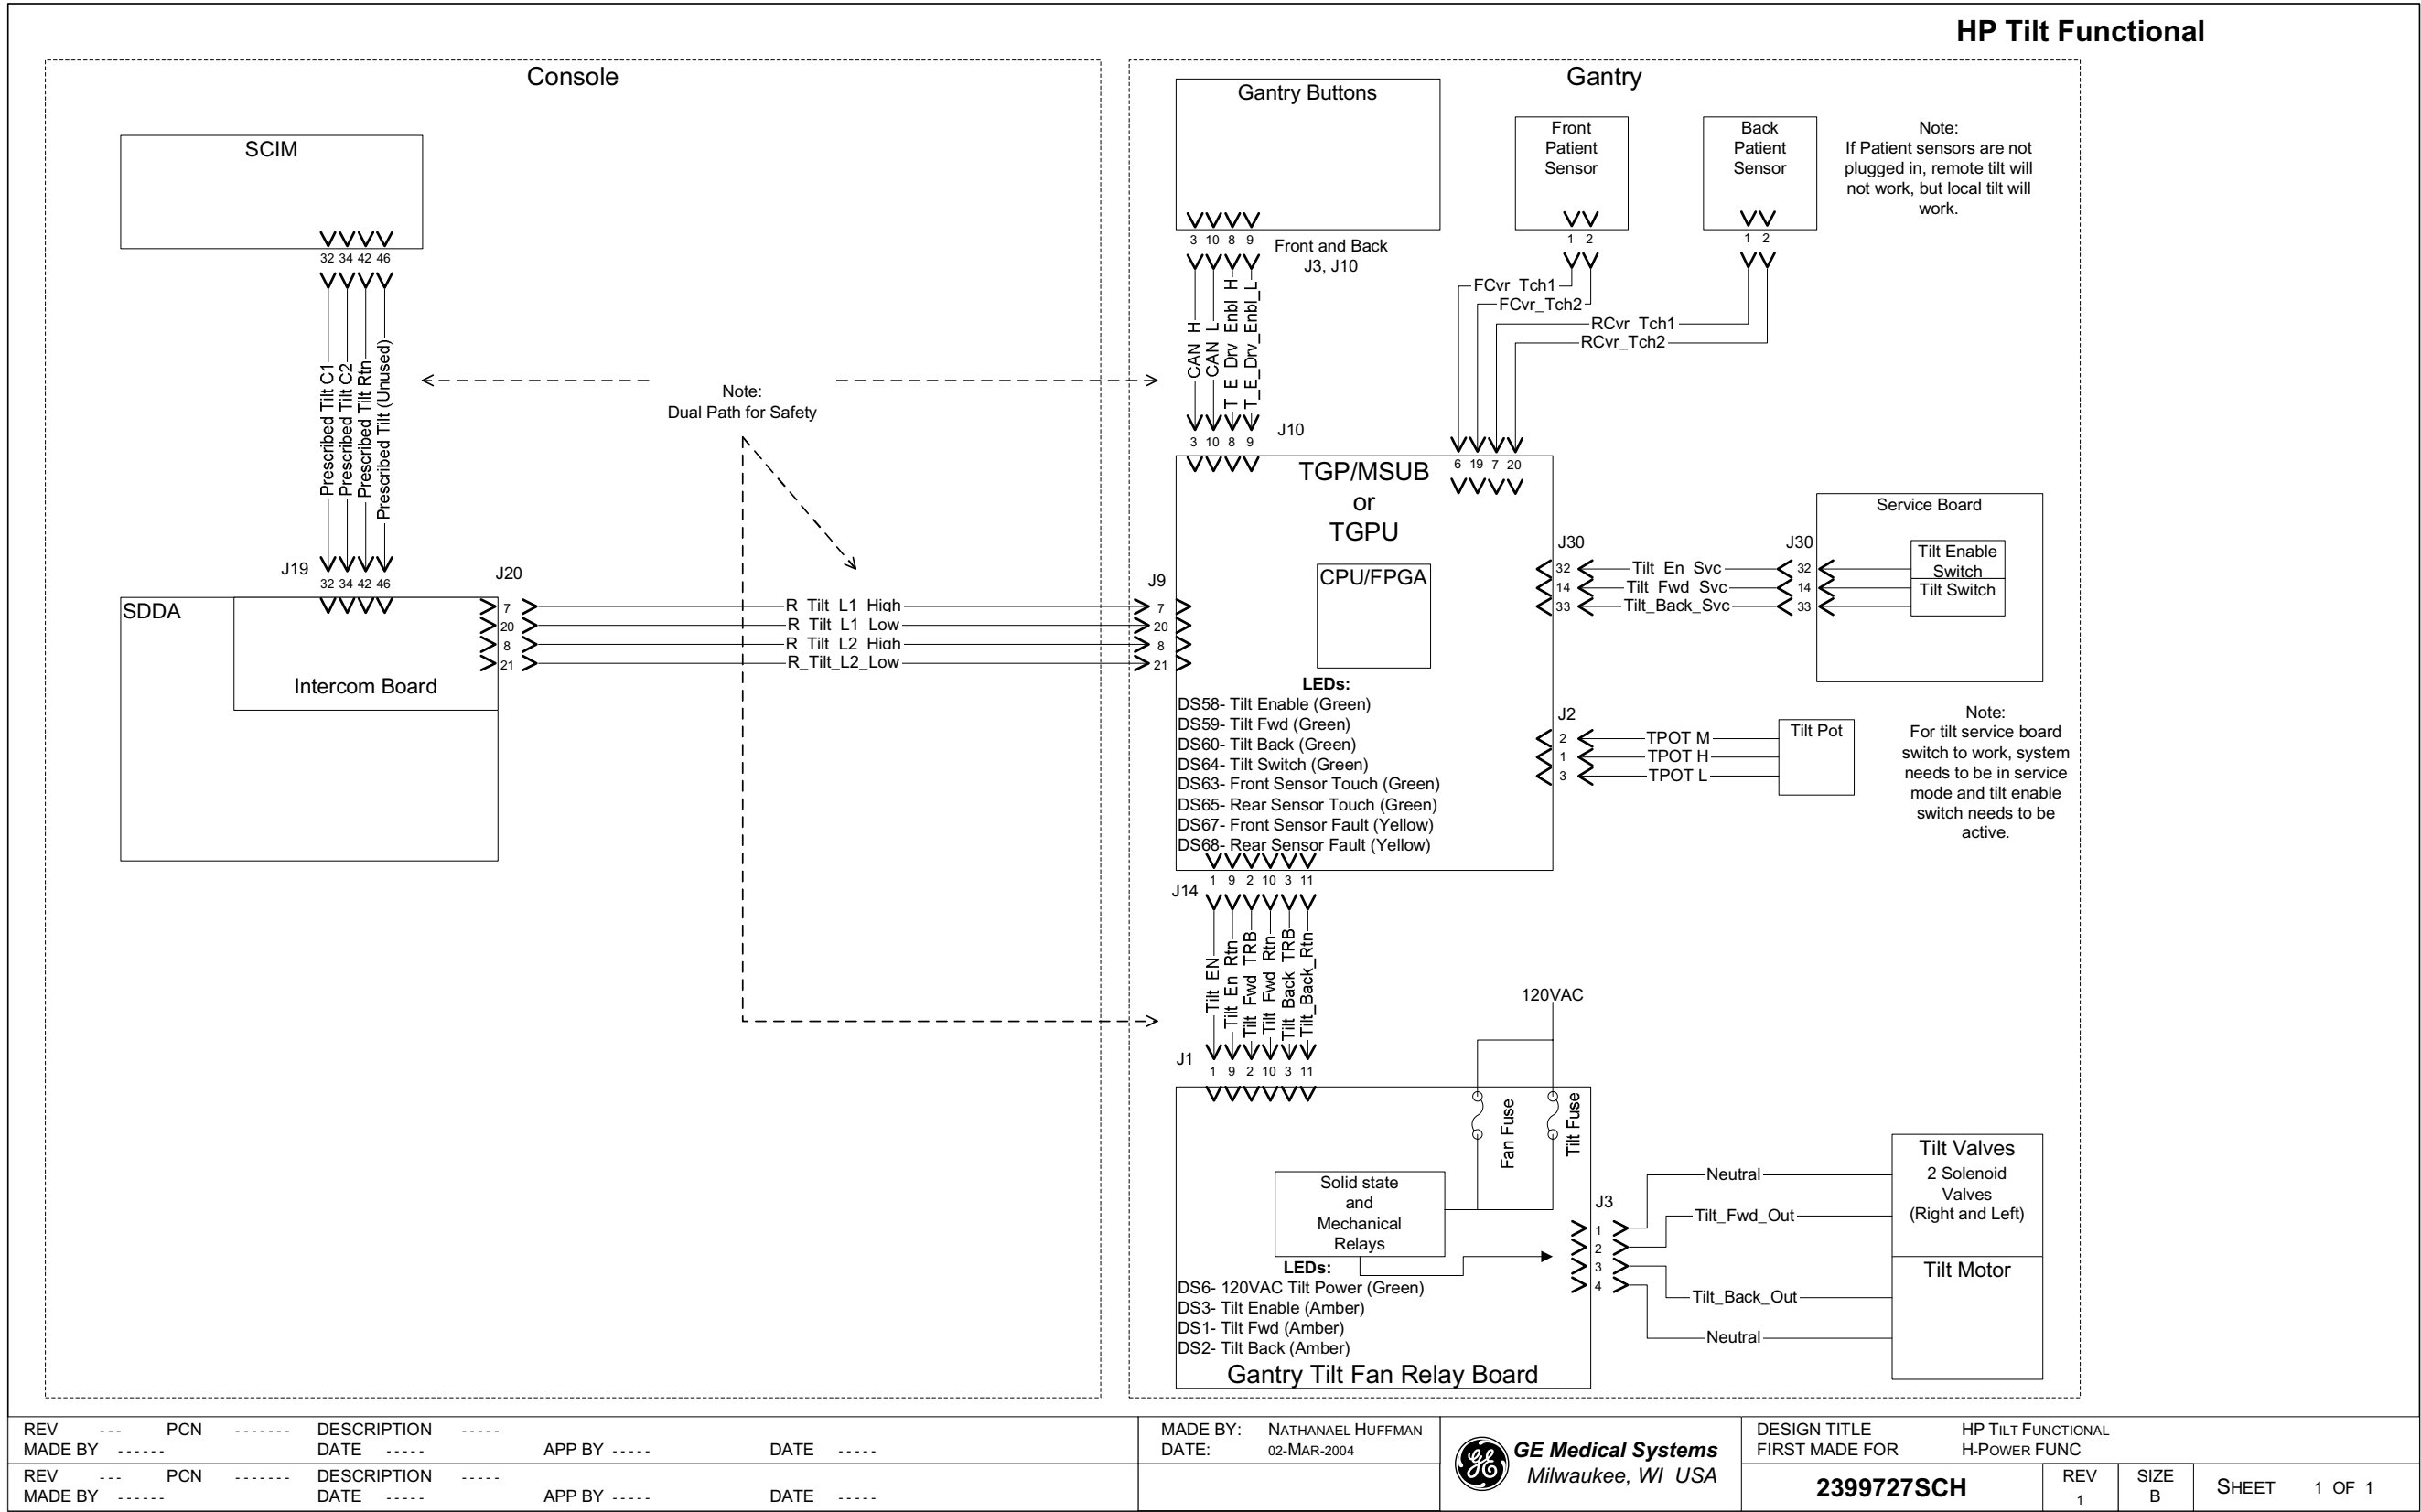


Figure 4-2 2399727 Sheet 1, Rev. 1

H-Power Cradle Sync

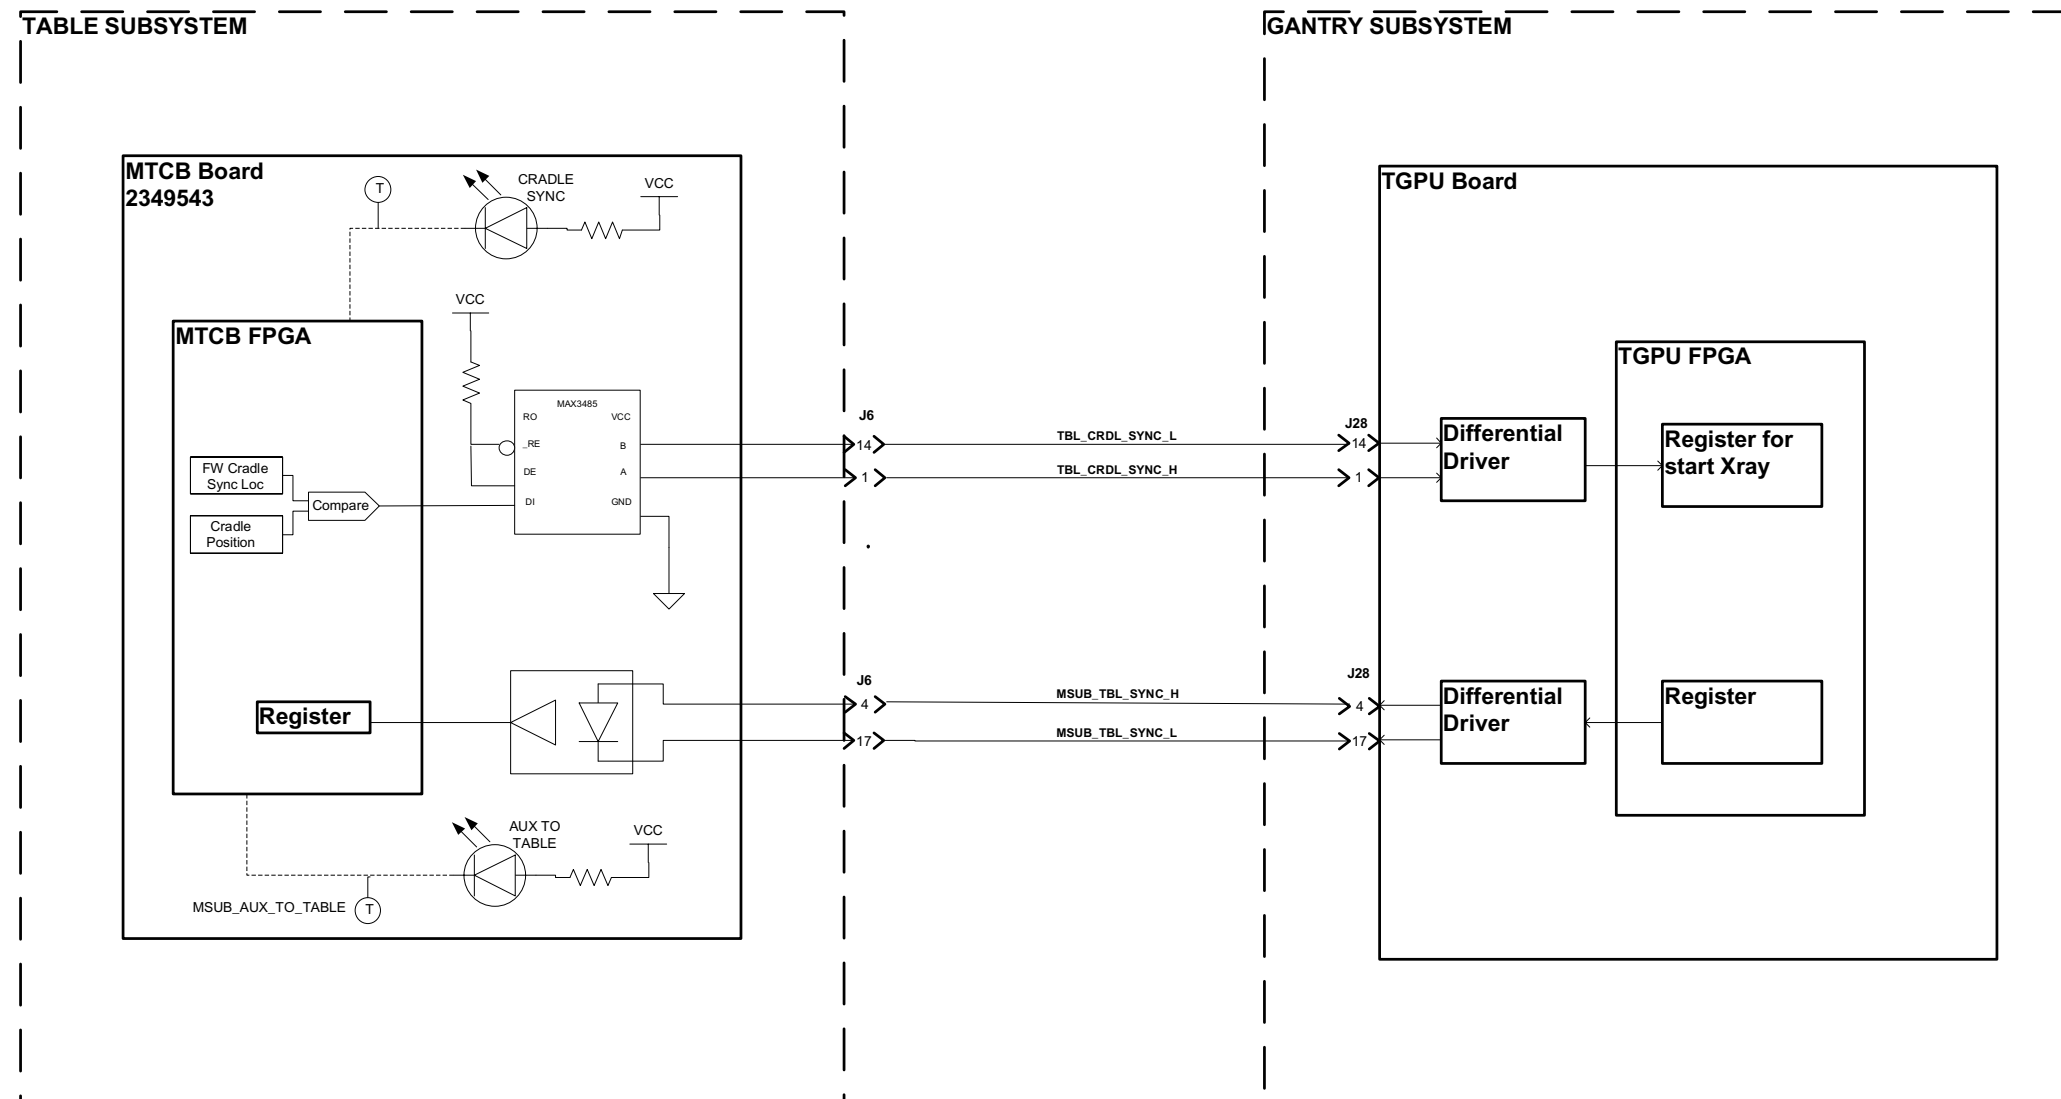

REV --- PCN -----	DESCRIPTION -----	MADE BY: GEORGE CAO	 GE Medical Systems Milwaukee, WI USA	DESIGN TITLE	H-POWER CRADLE SYNC			
MADE BY -----	DATE ----- APP BY ----- DATE -----	DATE: NOV 18, 2003		FIRST MADE FOR	H-POWER FUNC			
REV --- PCN -----	DESCRIPTION -----	ELECTRONIC RELEASE PROCESS	 GE Medical Systems Milwaukee, WI USA	2399728SCH	REV	SIZE	SHEET 1 OF 1	
MADE BY -----	DATE ----- APP BY ----- DATE -----	NOT DESIGN RELEASED			1	B		

Figure 4-3 2399728 Sheet 1, Rev. 1

Section 4.0 — Table Cradle Drive - 5127766

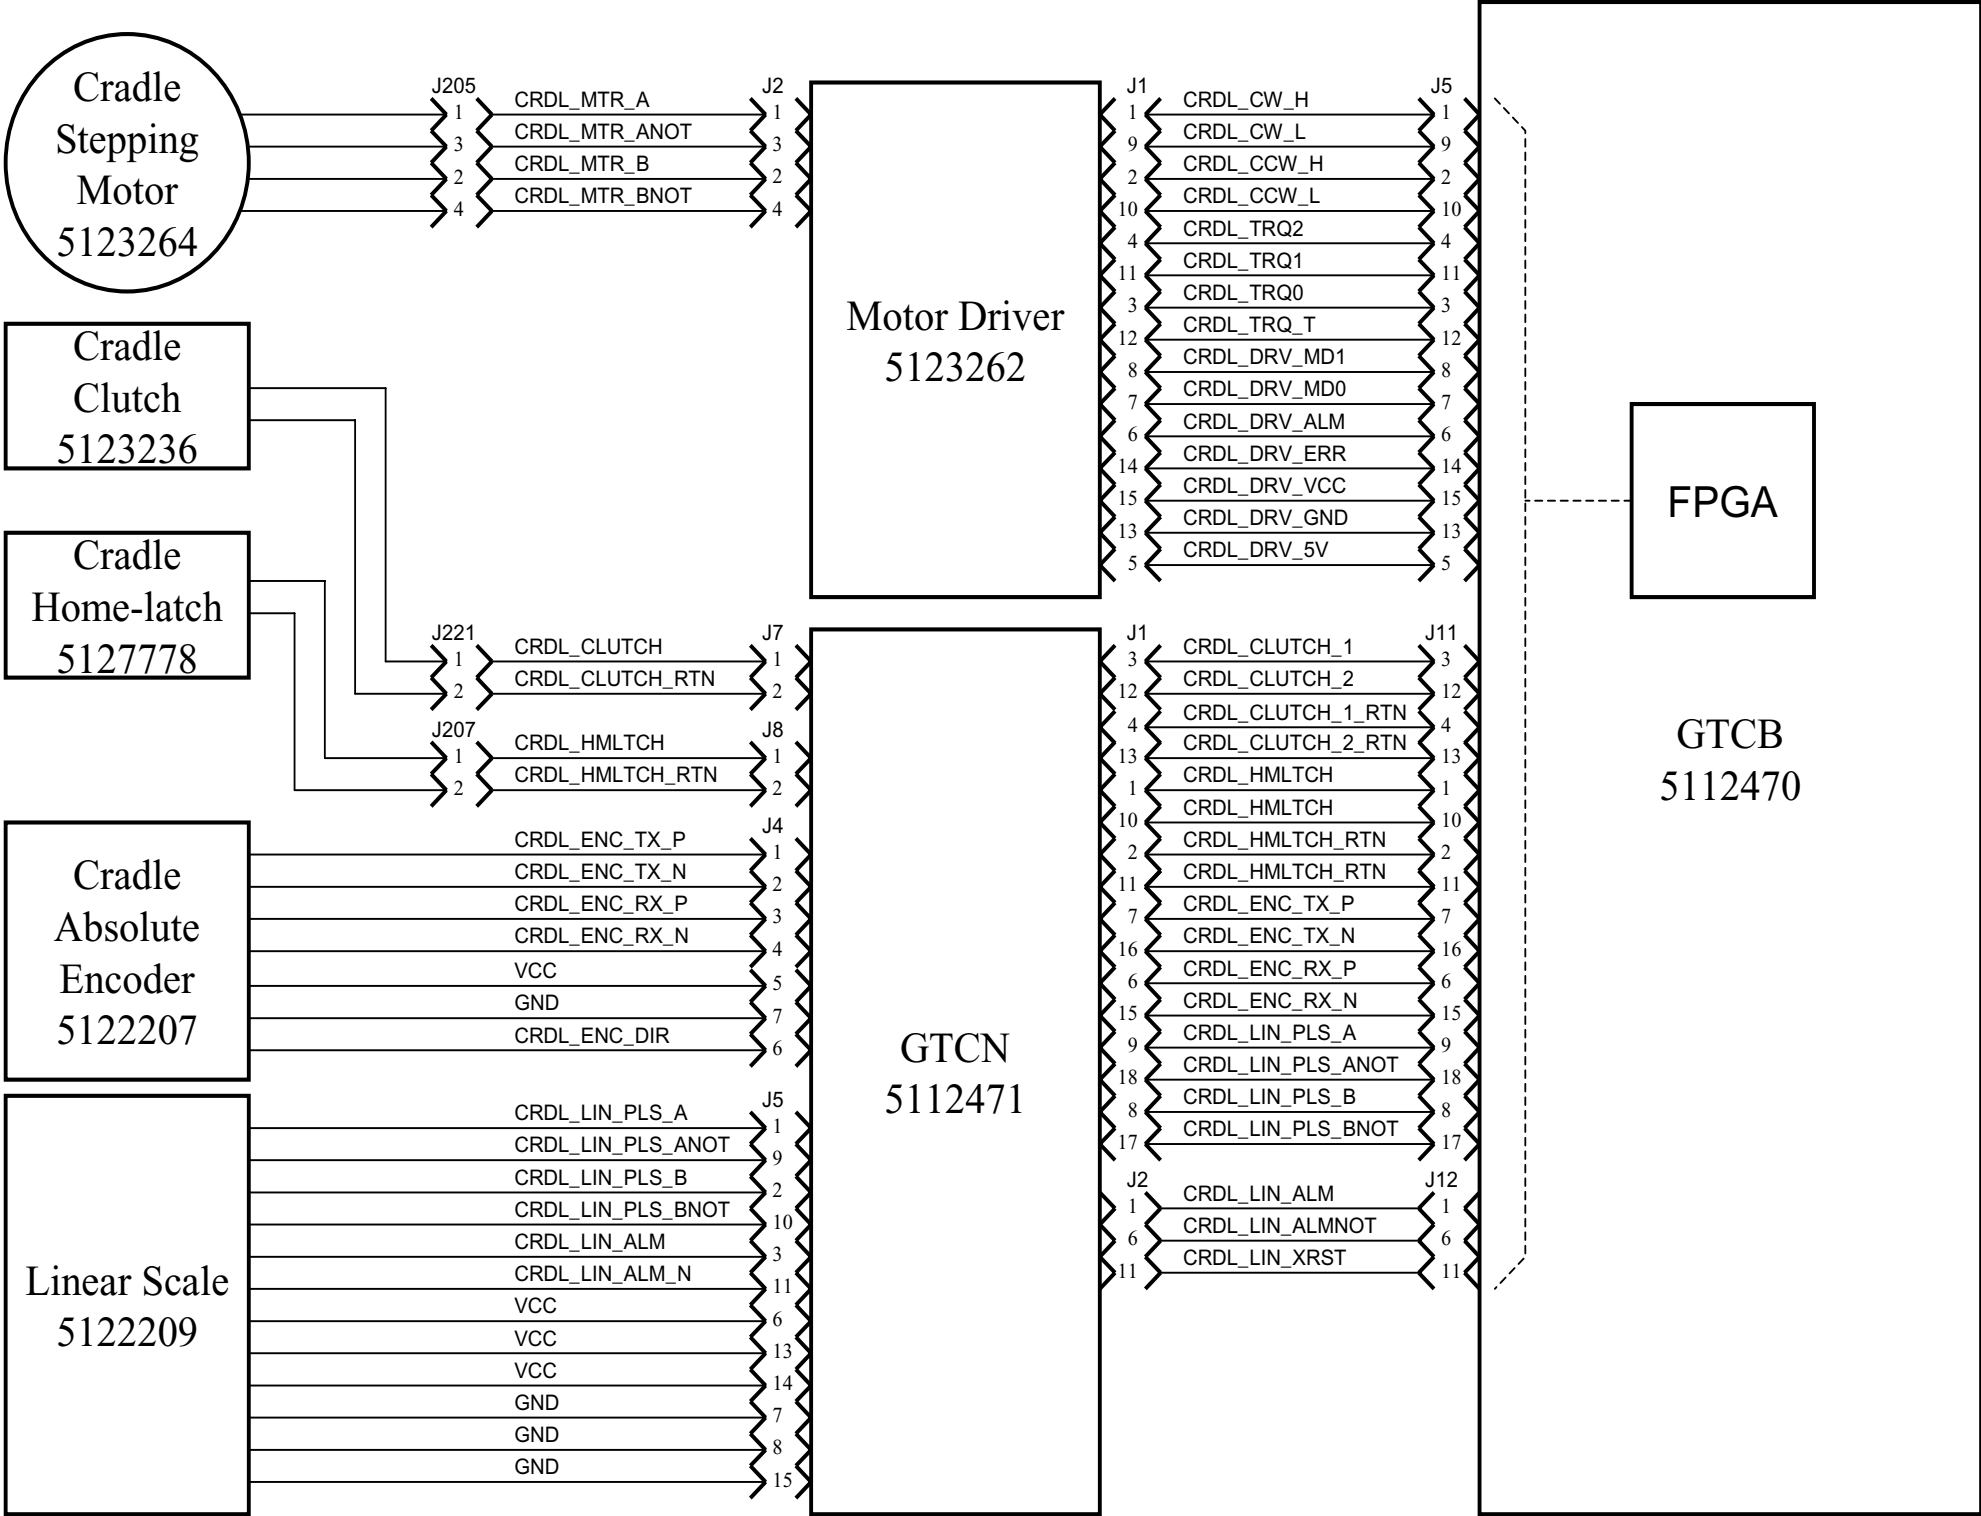


Figure 4-4 5127766 Sheet 1, Rev. 1

Section 5.0 — Table Cradle Intermediate Support Drive - 5127766

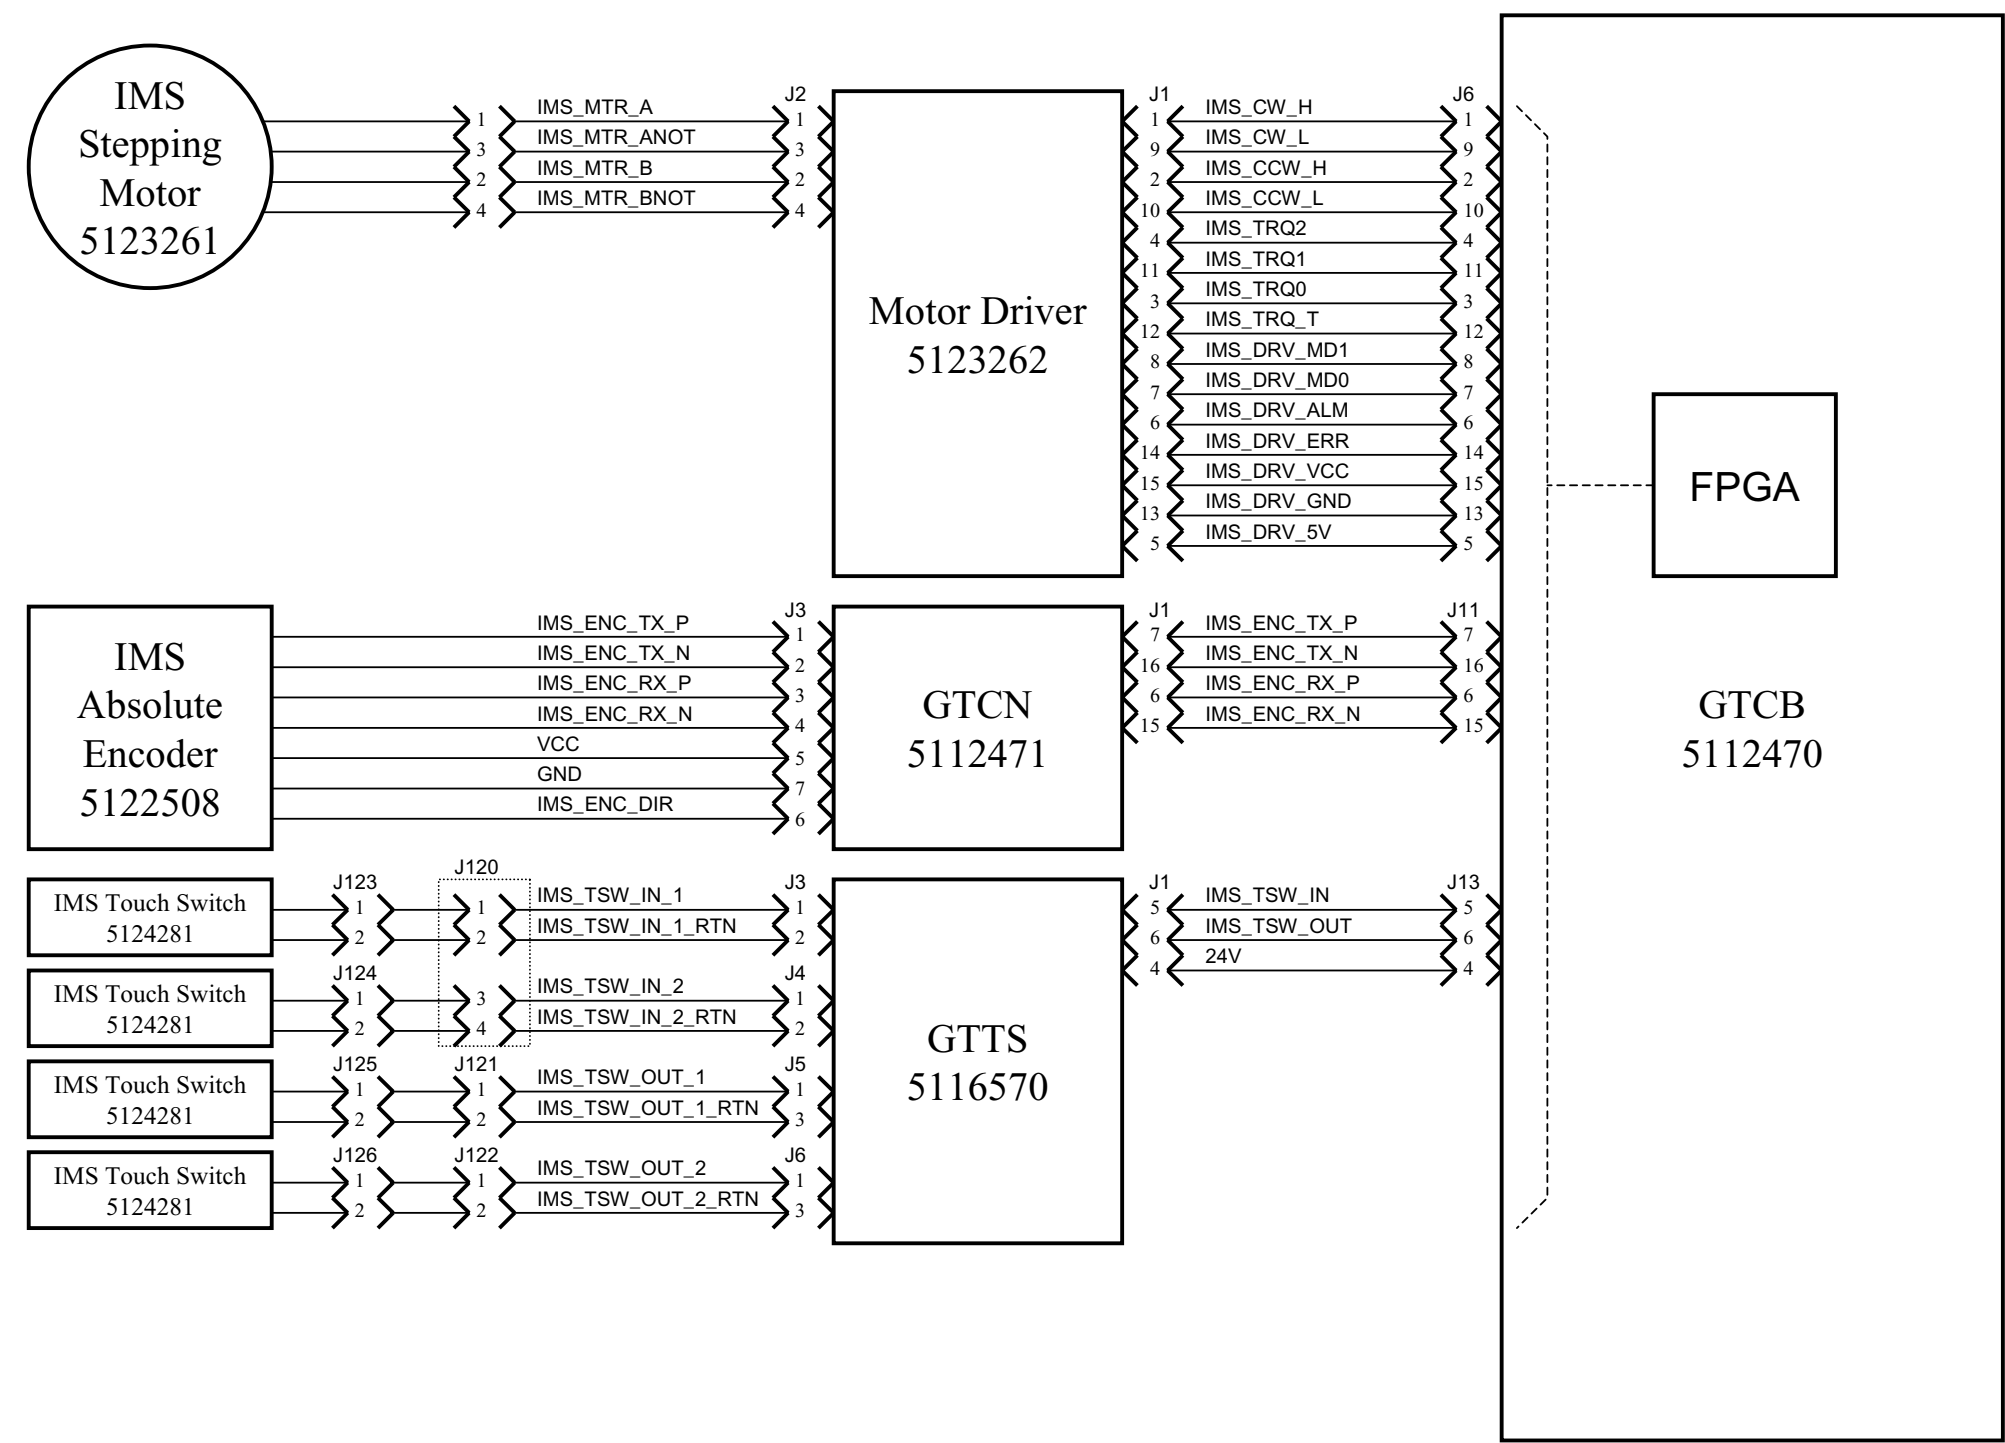


Figure 4-5 5127766 Sheet 2, Rev. 1

Section 6.0 — Table Elevation Drive - 5127766


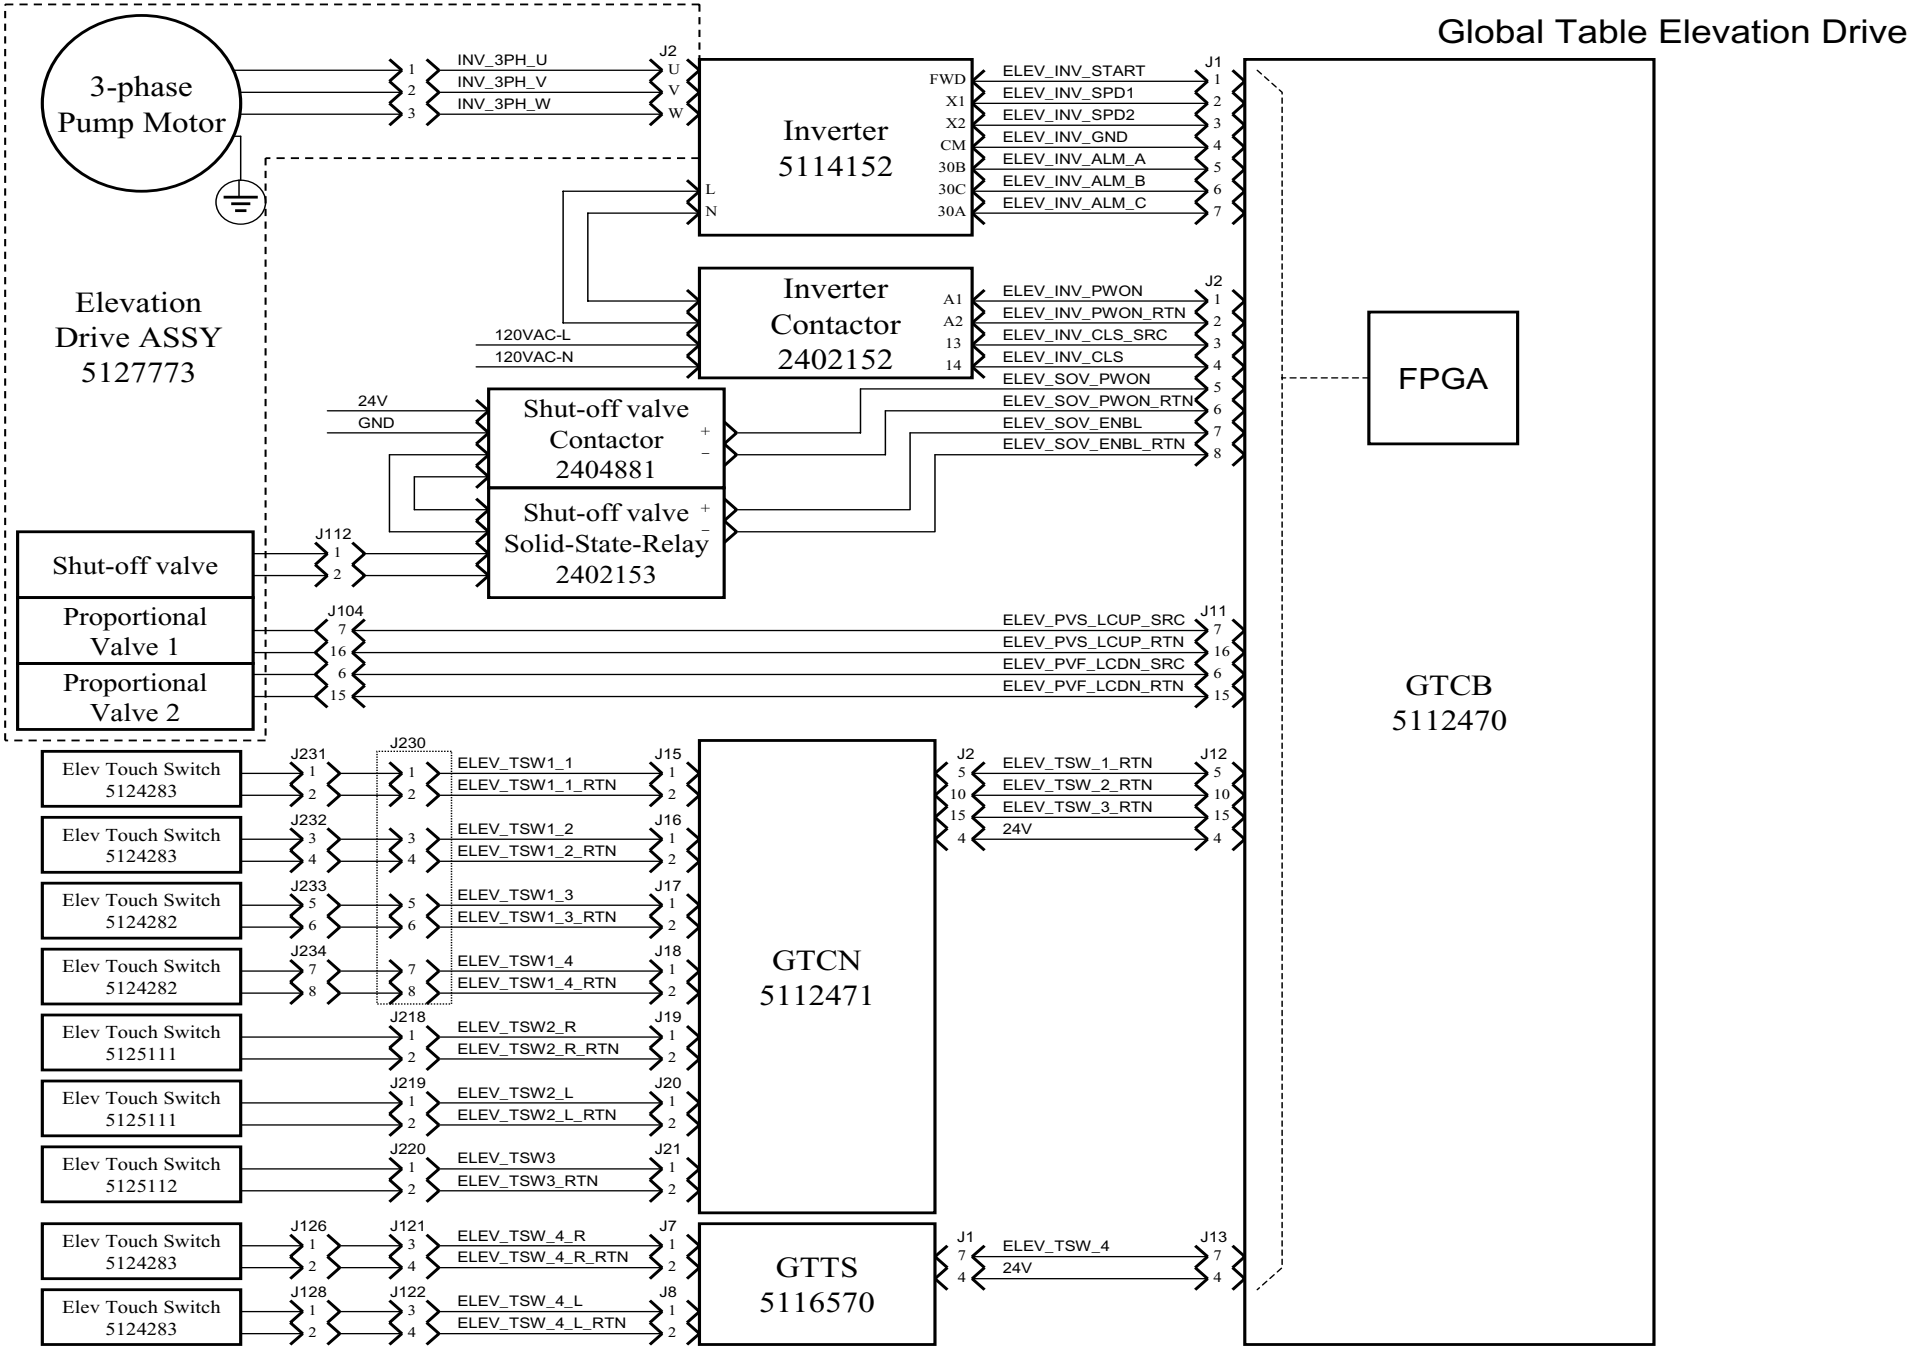


Figure 4-6 5127766 Sheet 3, Rev. 1

DRAWING SHEET - FOR REFERENCE ONLY.
See related Drawing Print for complete definition.



Section 8.0 — Table Touch Switches - 5121647

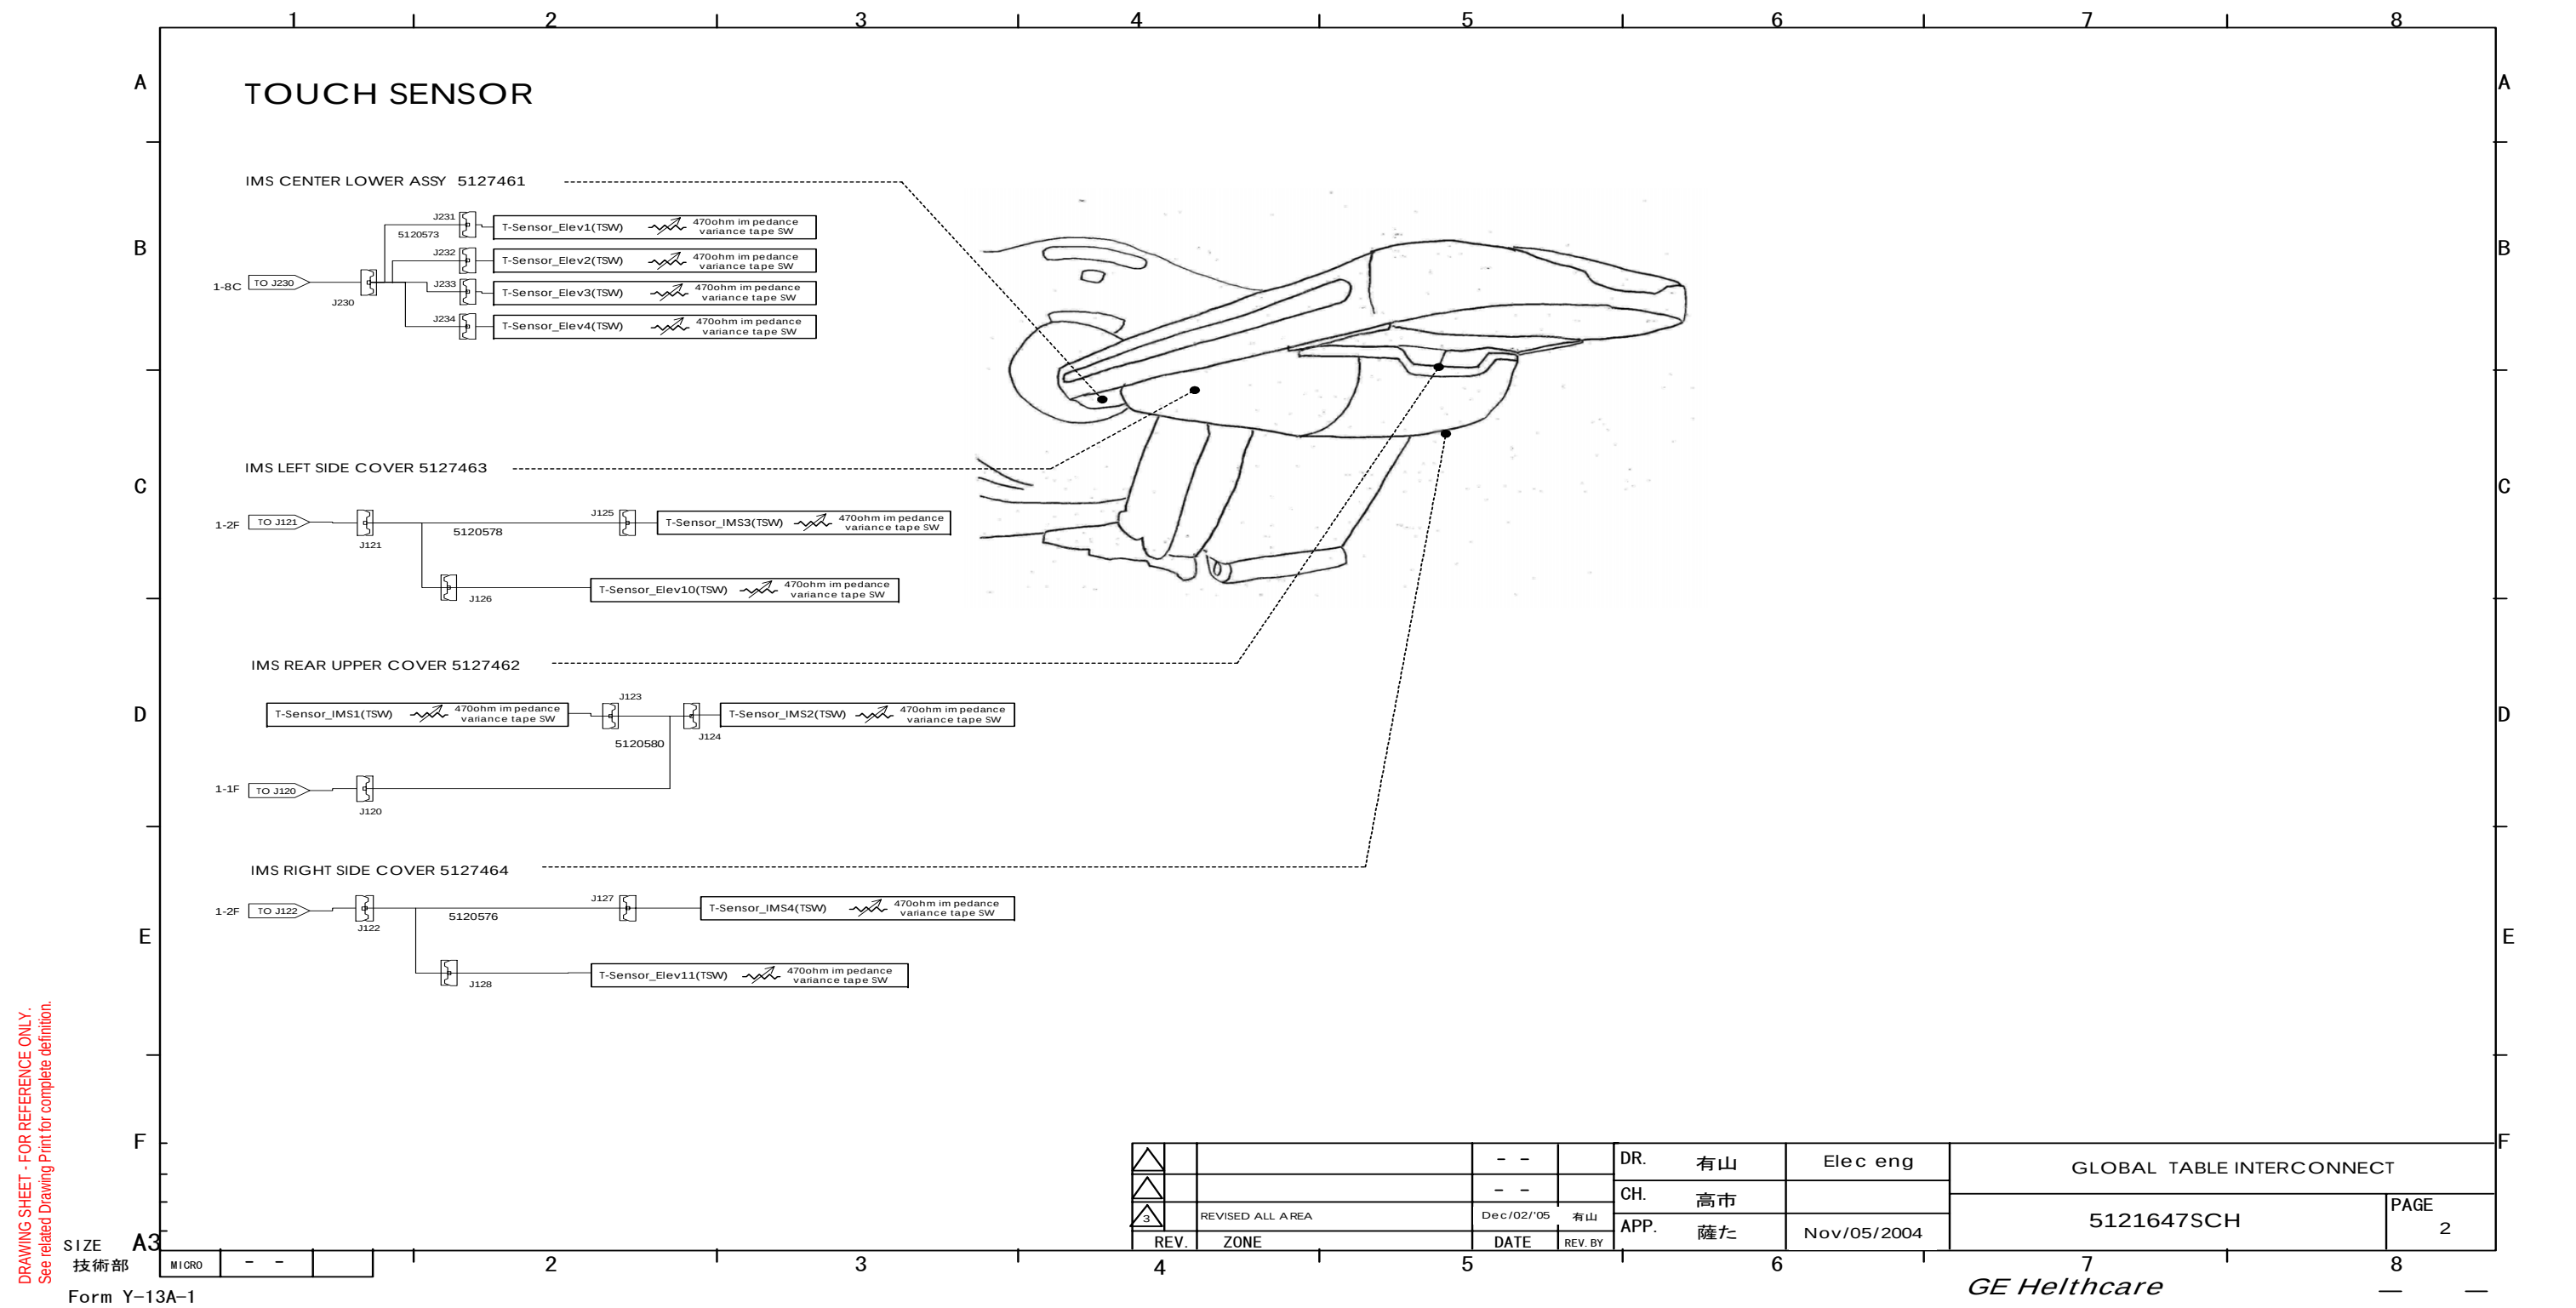


Figure 4-8 5121647 Sheet 2, Rev 3

Section 9.0 — Table Footswitch - 5121647


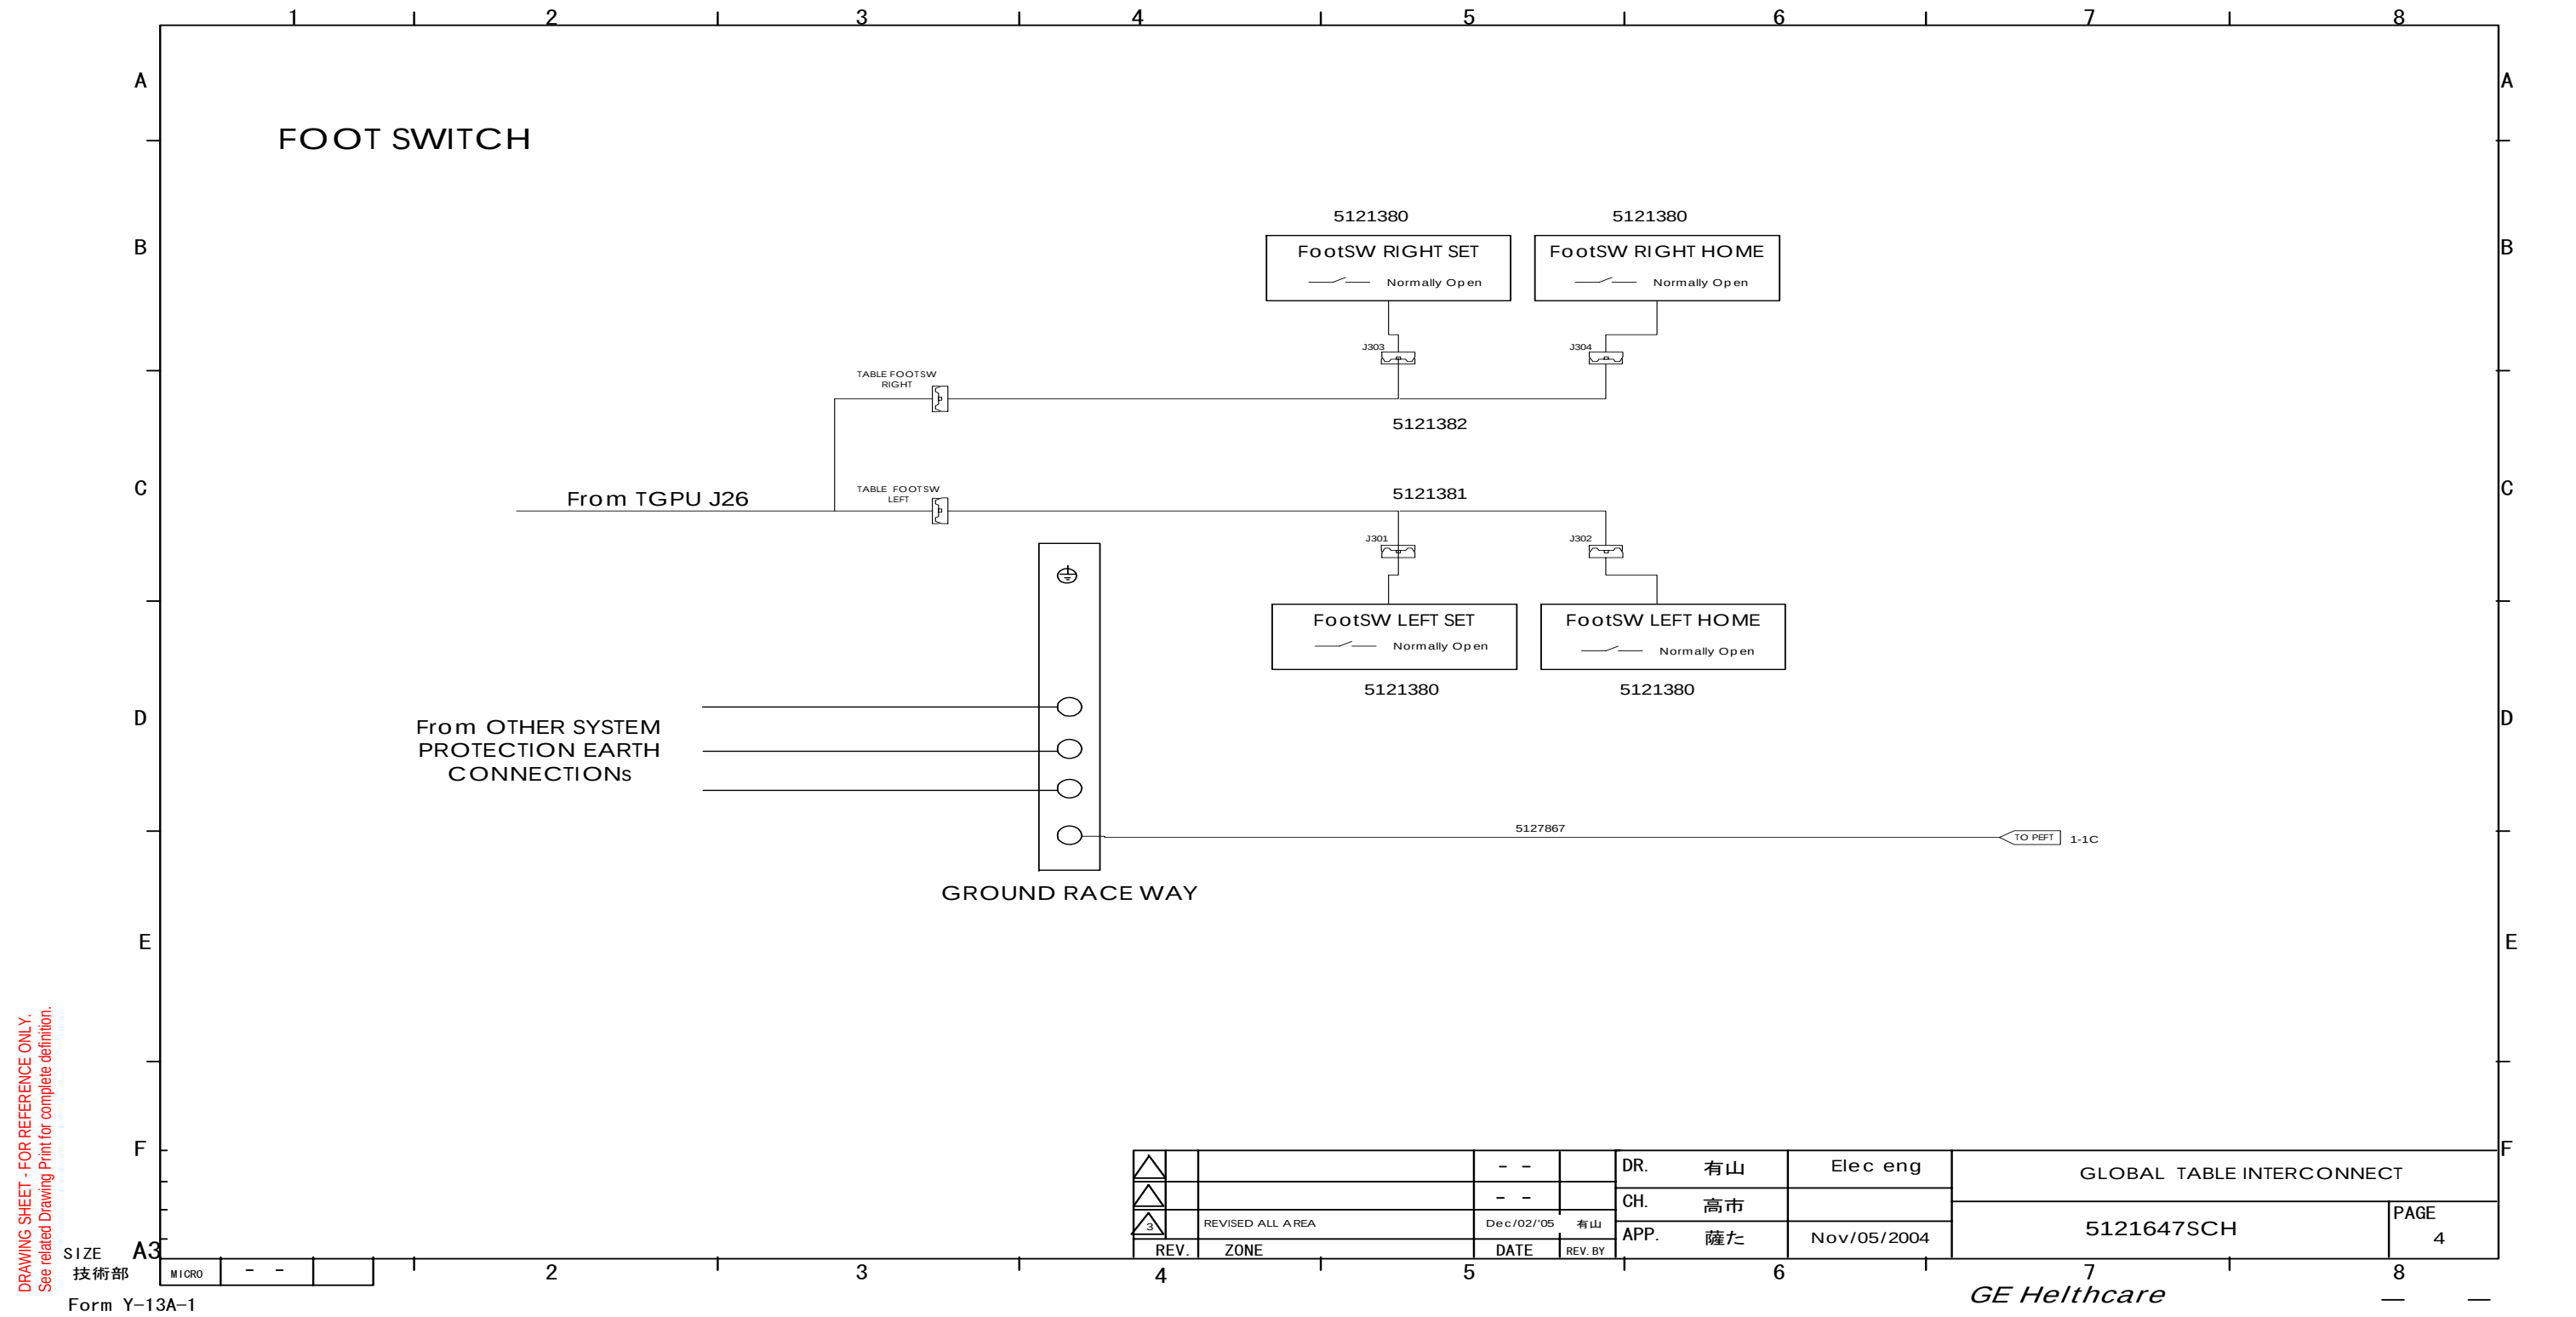


Figure 4-9 5121647 Sheet 4, Rev 3

Chapter 5

Axial Control

Figure 5-1 2399731 Sheet 1 Rev. 1



Section 2.0 — Axial Power Distribution - 2399732

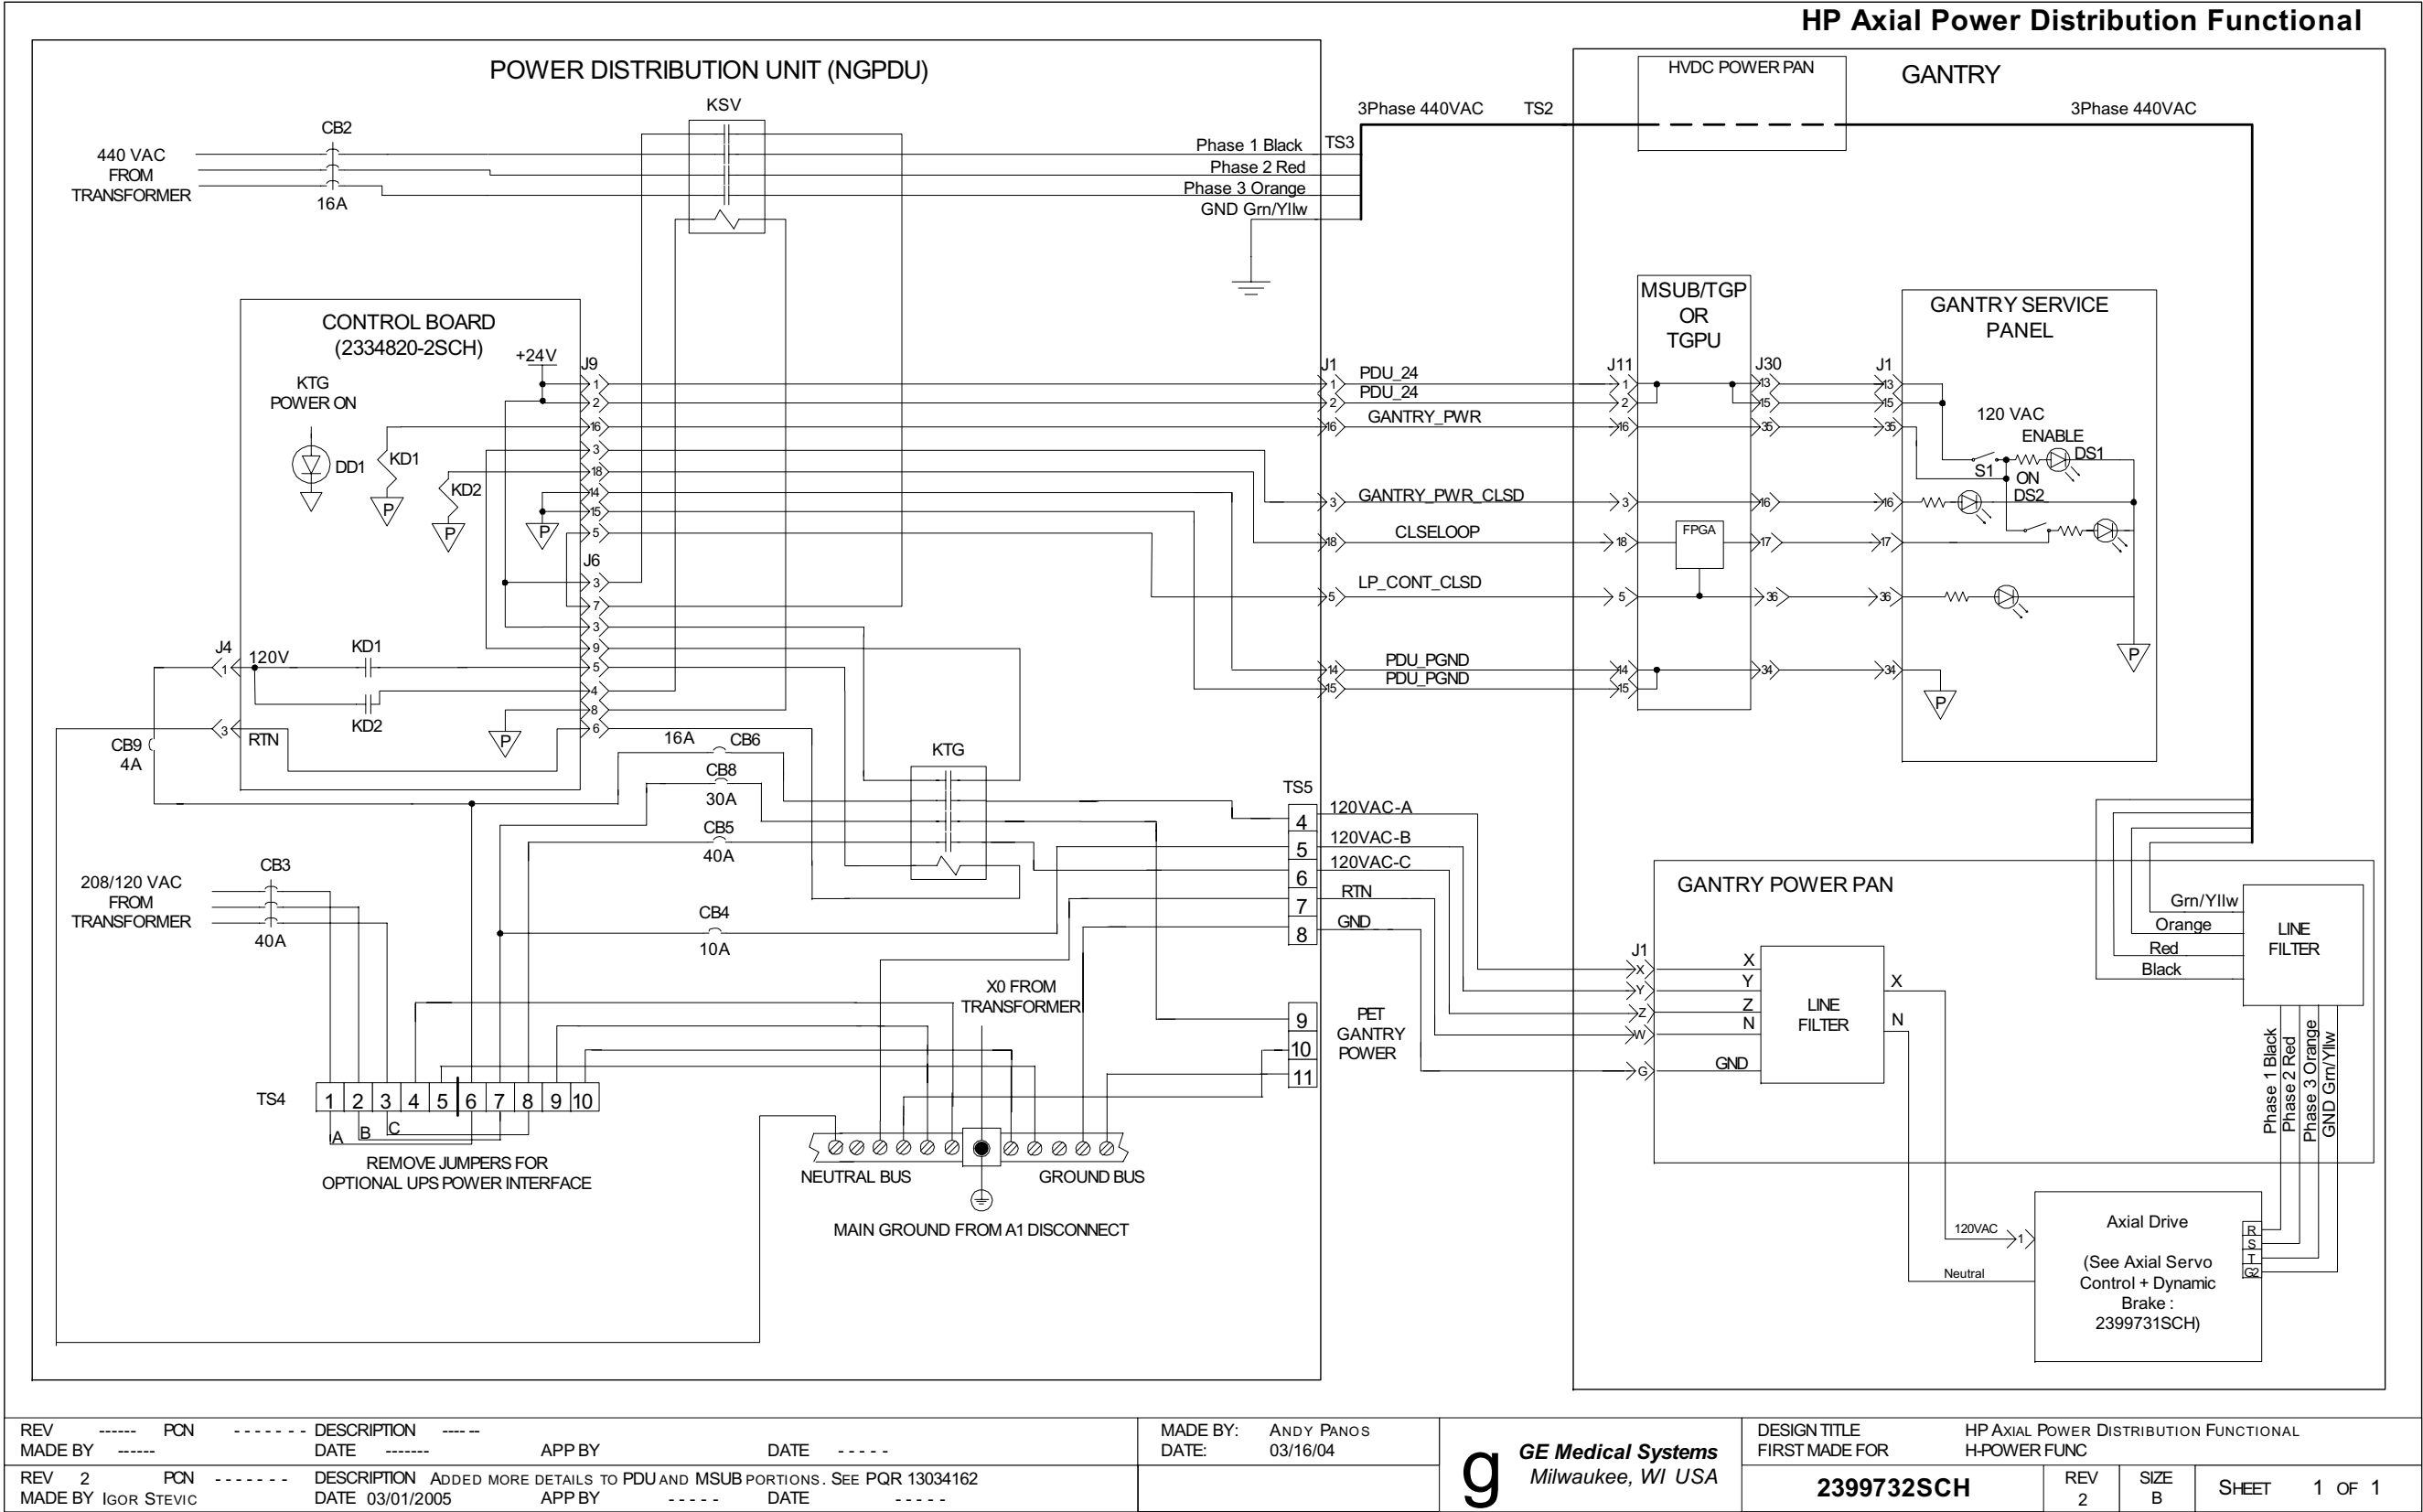


Figure 5-2 2399732 Sheet 1 Rev. 2

THIS PAGE INTENTIONALLY BLANK.

Chapter 6

Operator I/O

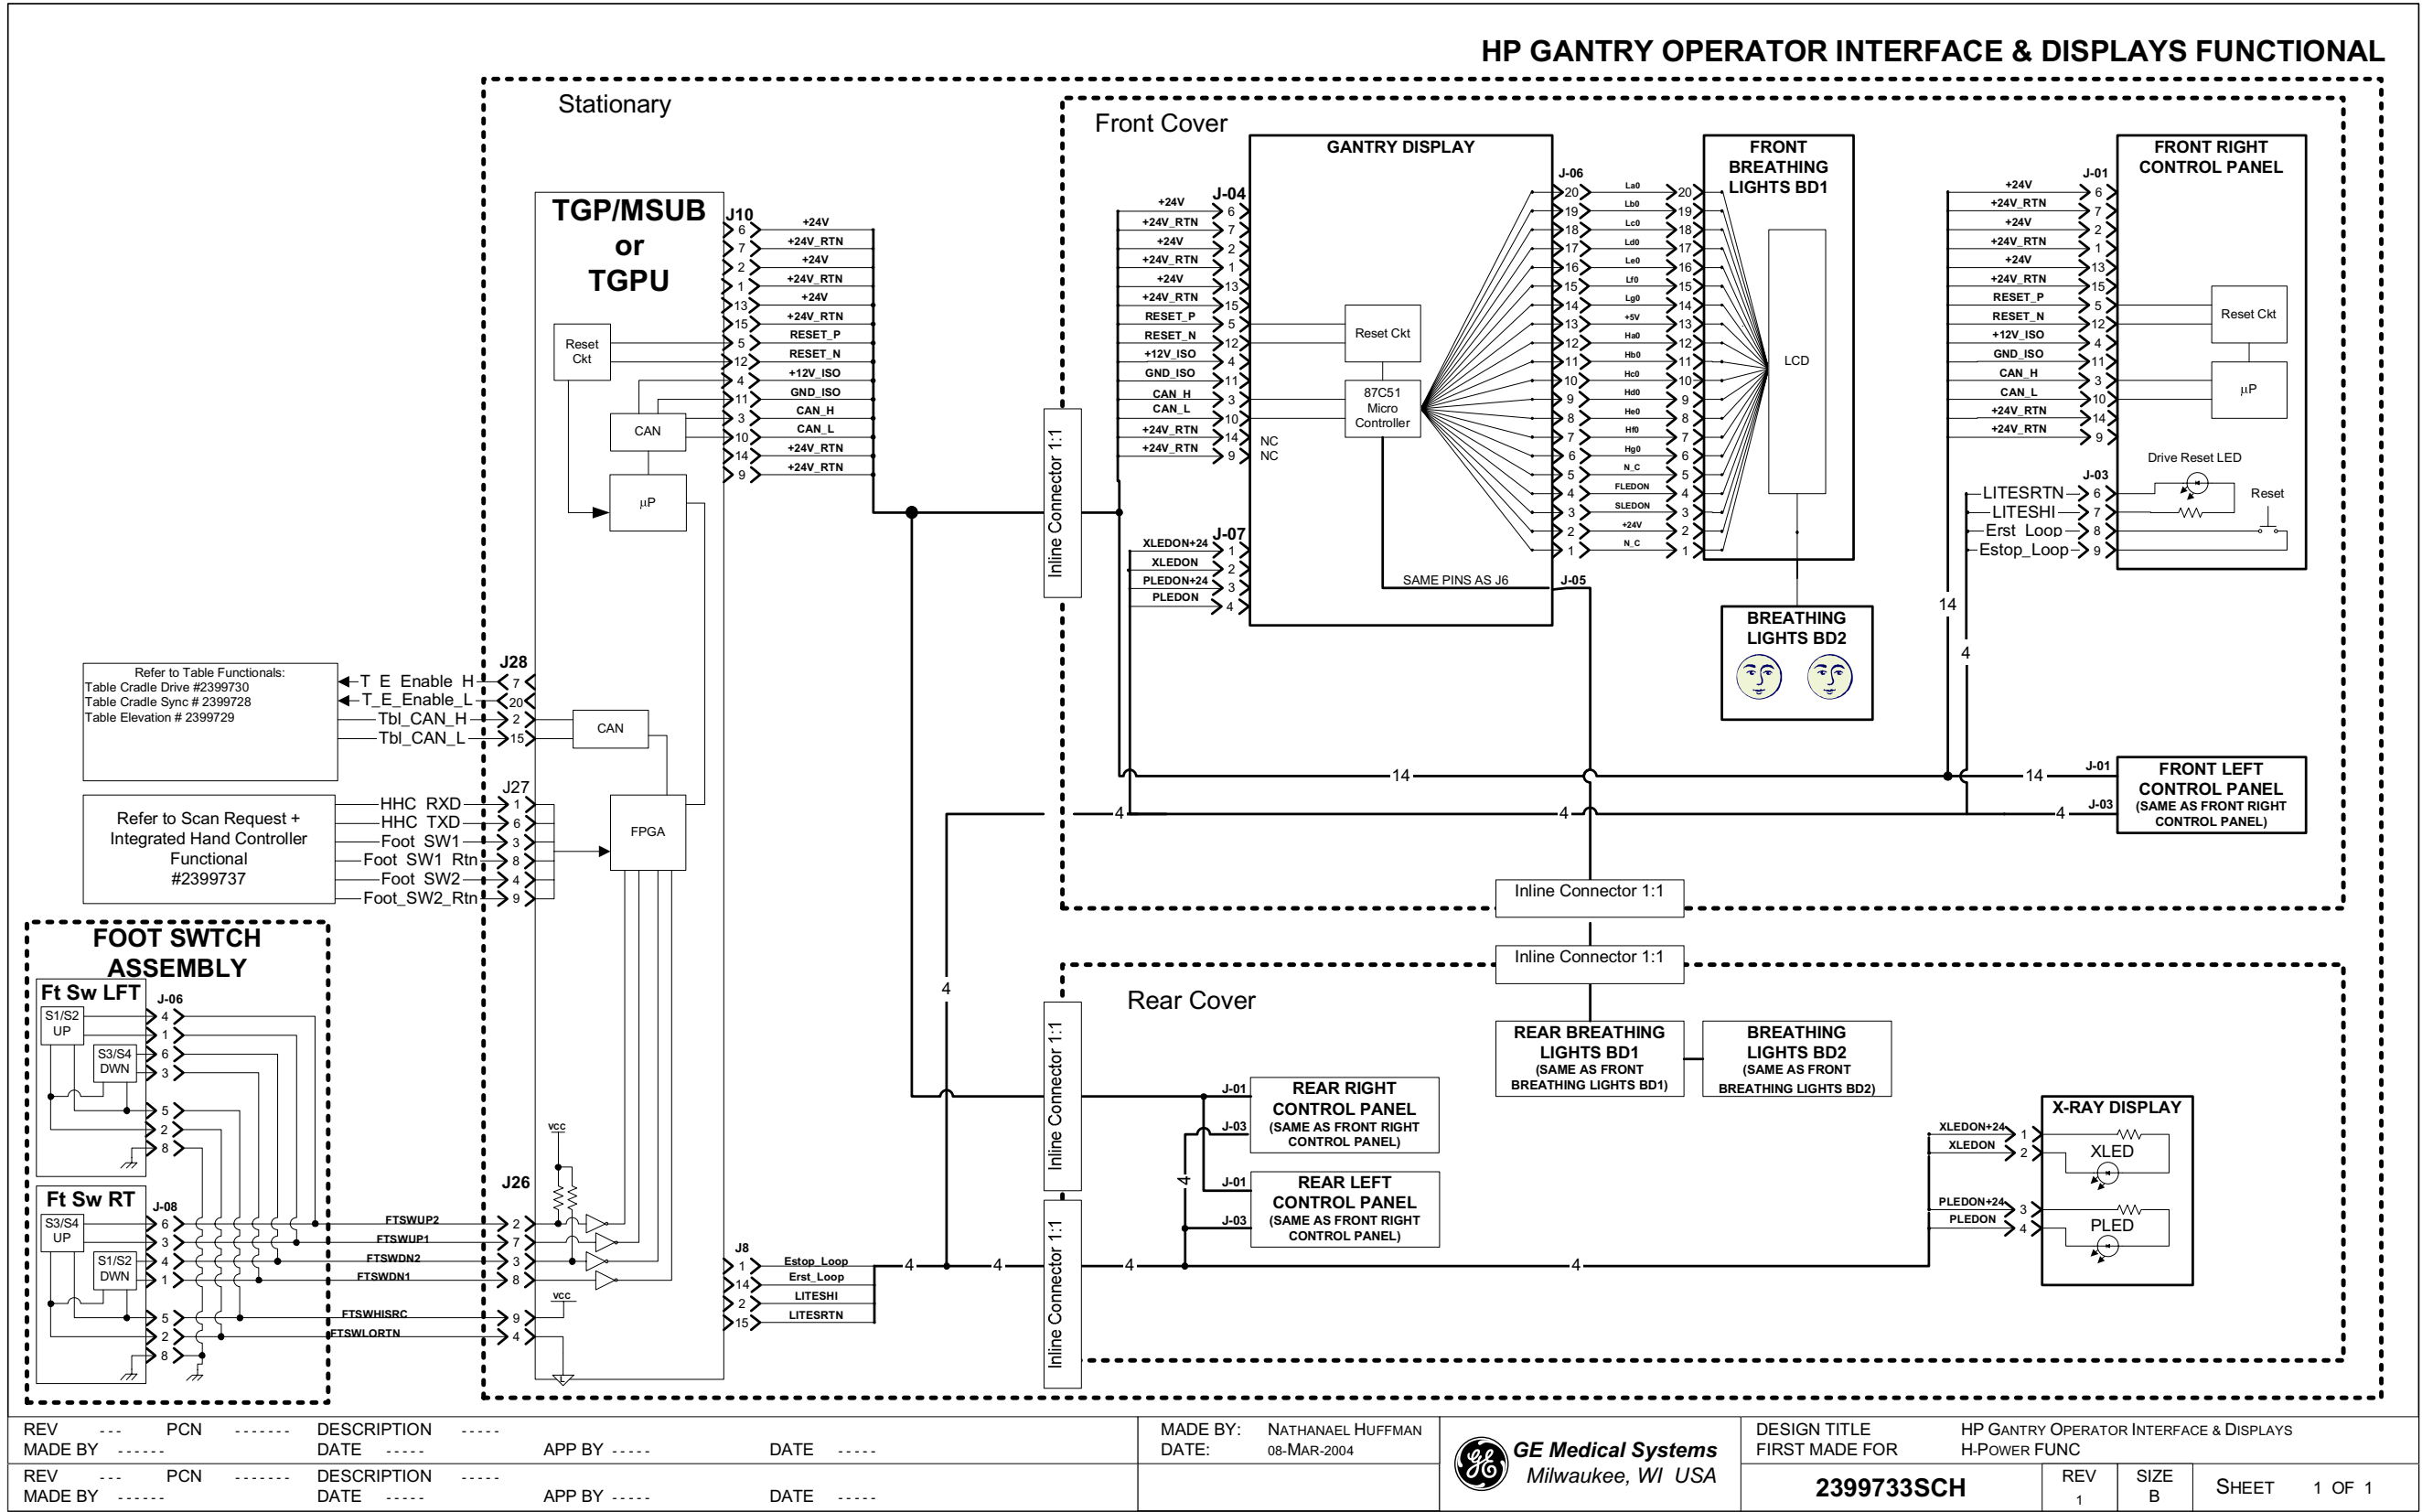


Figure 6-1 2399733 Sheet 1, Rev. 1

Section 2.0 — Gantry Reset from Console - 2399734


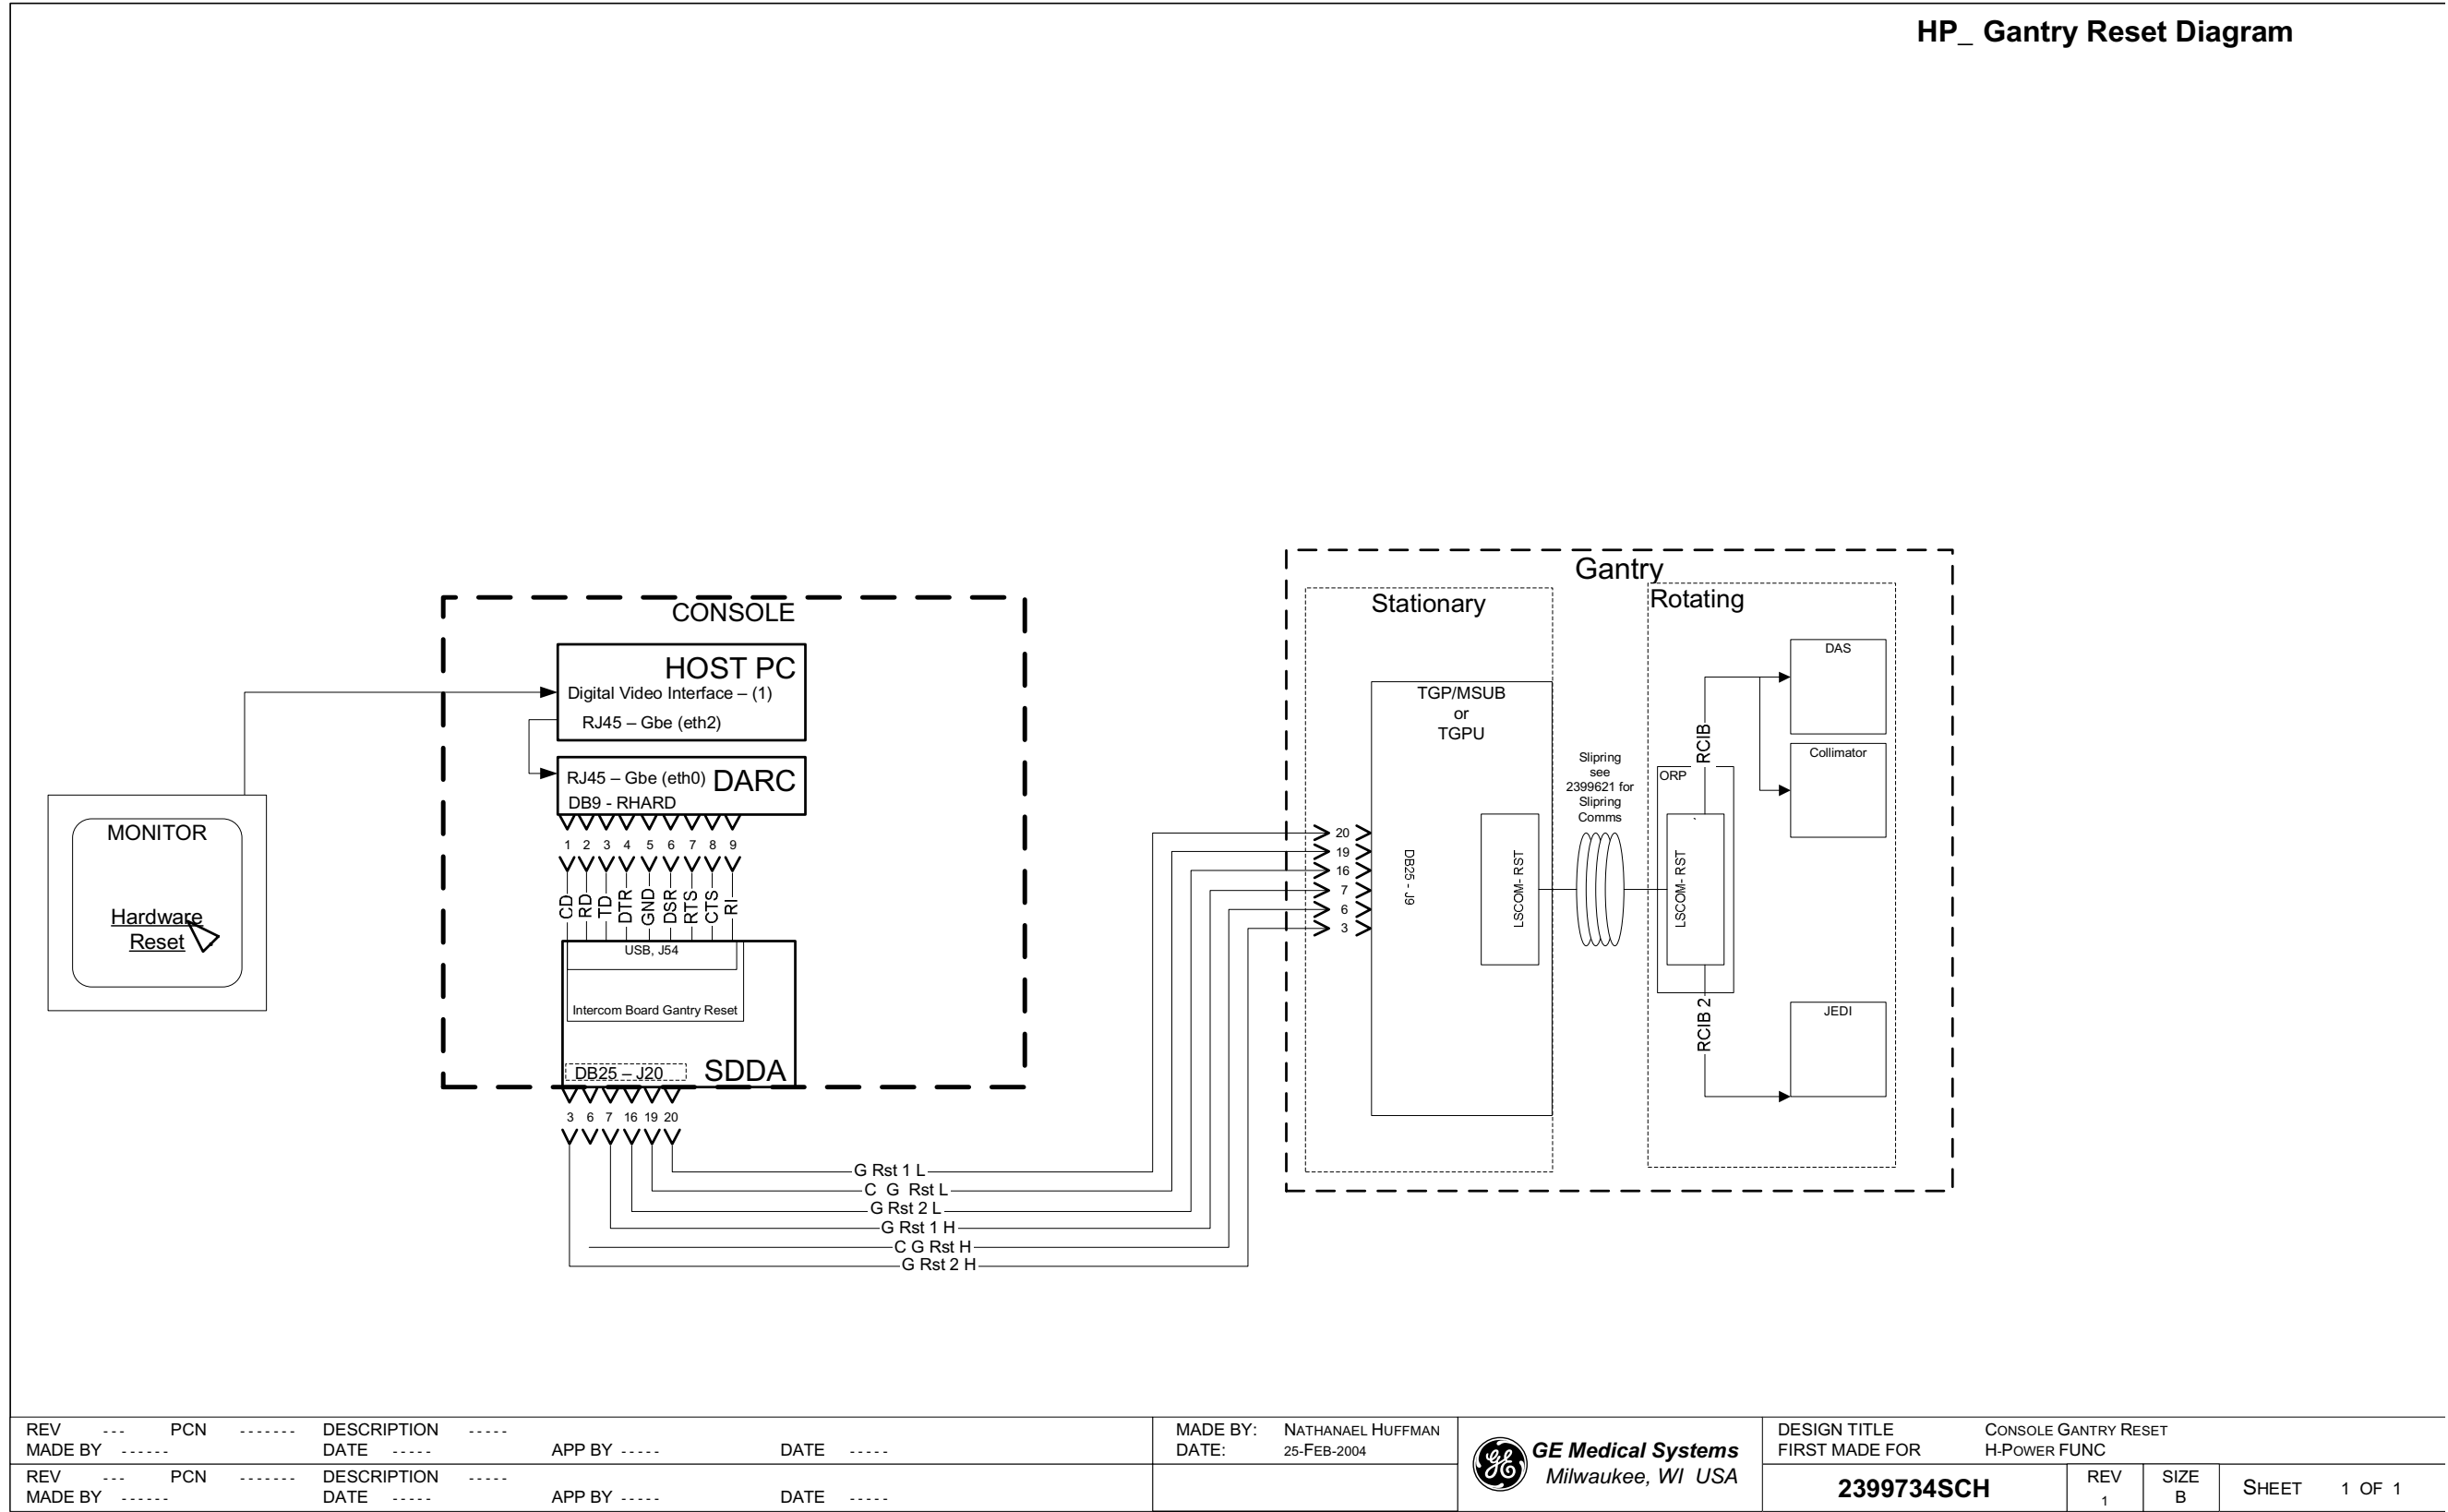


Figure 6-2 2399734 Sheet 1, Rev. 1

H-POWER CARDIAC OPTION FUNCTIONAL

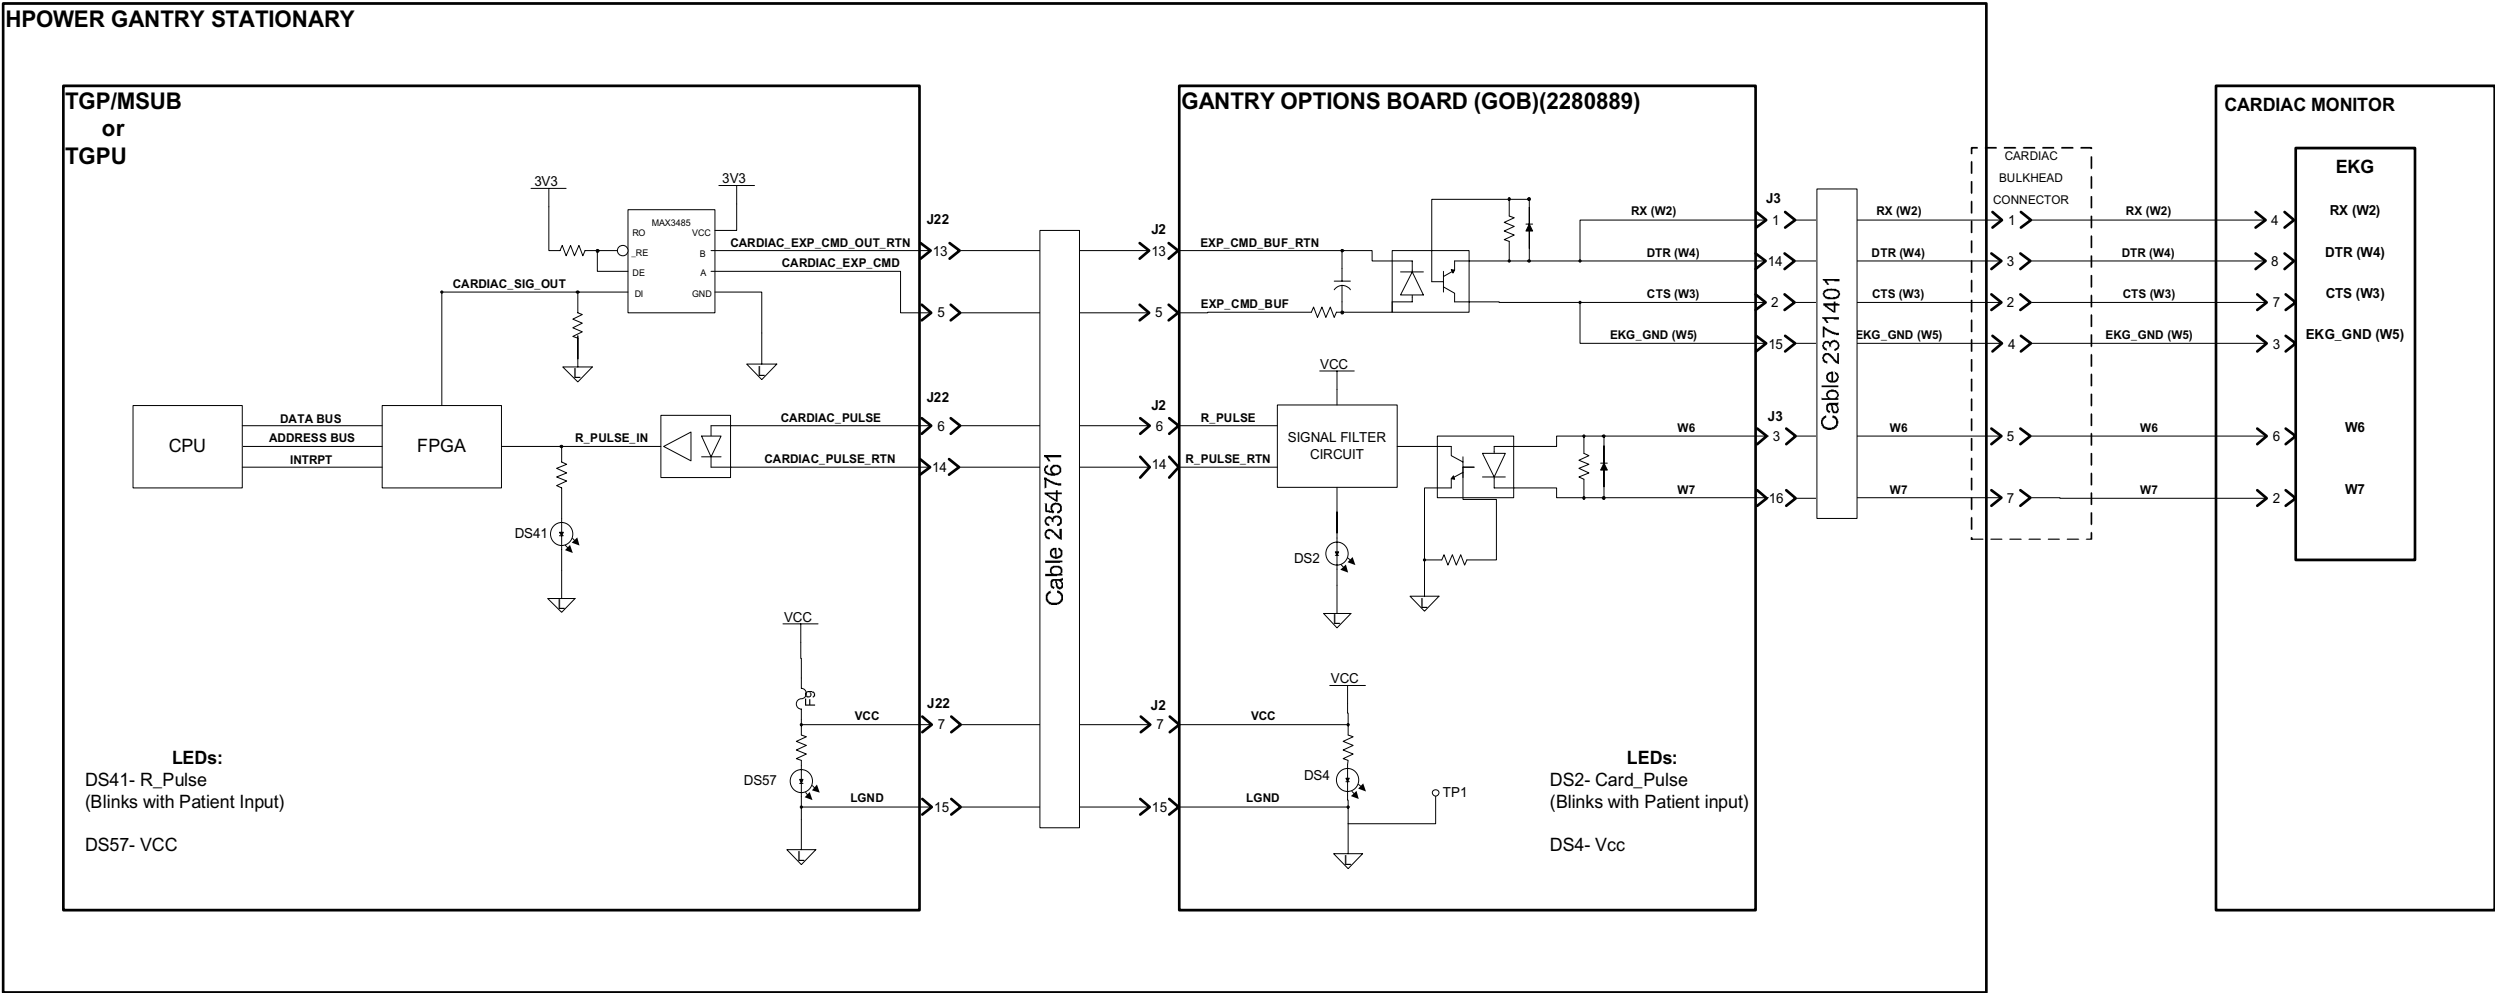

REV --- PCN ----- DESCRIPTION -----	MADE BY: MICHAEL MILLER	DESIGN TITLE HP CARDIAC OPTION FUNCTIONAL			
MADE BY ----- DATE ----- APP BY ----- DATE -----	DATE: 12 JUNE 2003	FIRST MADE FOR H-POWER FUNC			
REV --- PCN ----- DESCRIPTION -----	GE Medical Systems Milwaukee, WI USA		2399735SCH	REV 1	SIZE B
MADE BY ----- DATE ----- APP BY ----- DATE -----				SHEET 1	OF 1

Figure 6-3 2399735 Sheet 1, Rev. 1

Section 4.0 — Pulmonary Options - 2399736


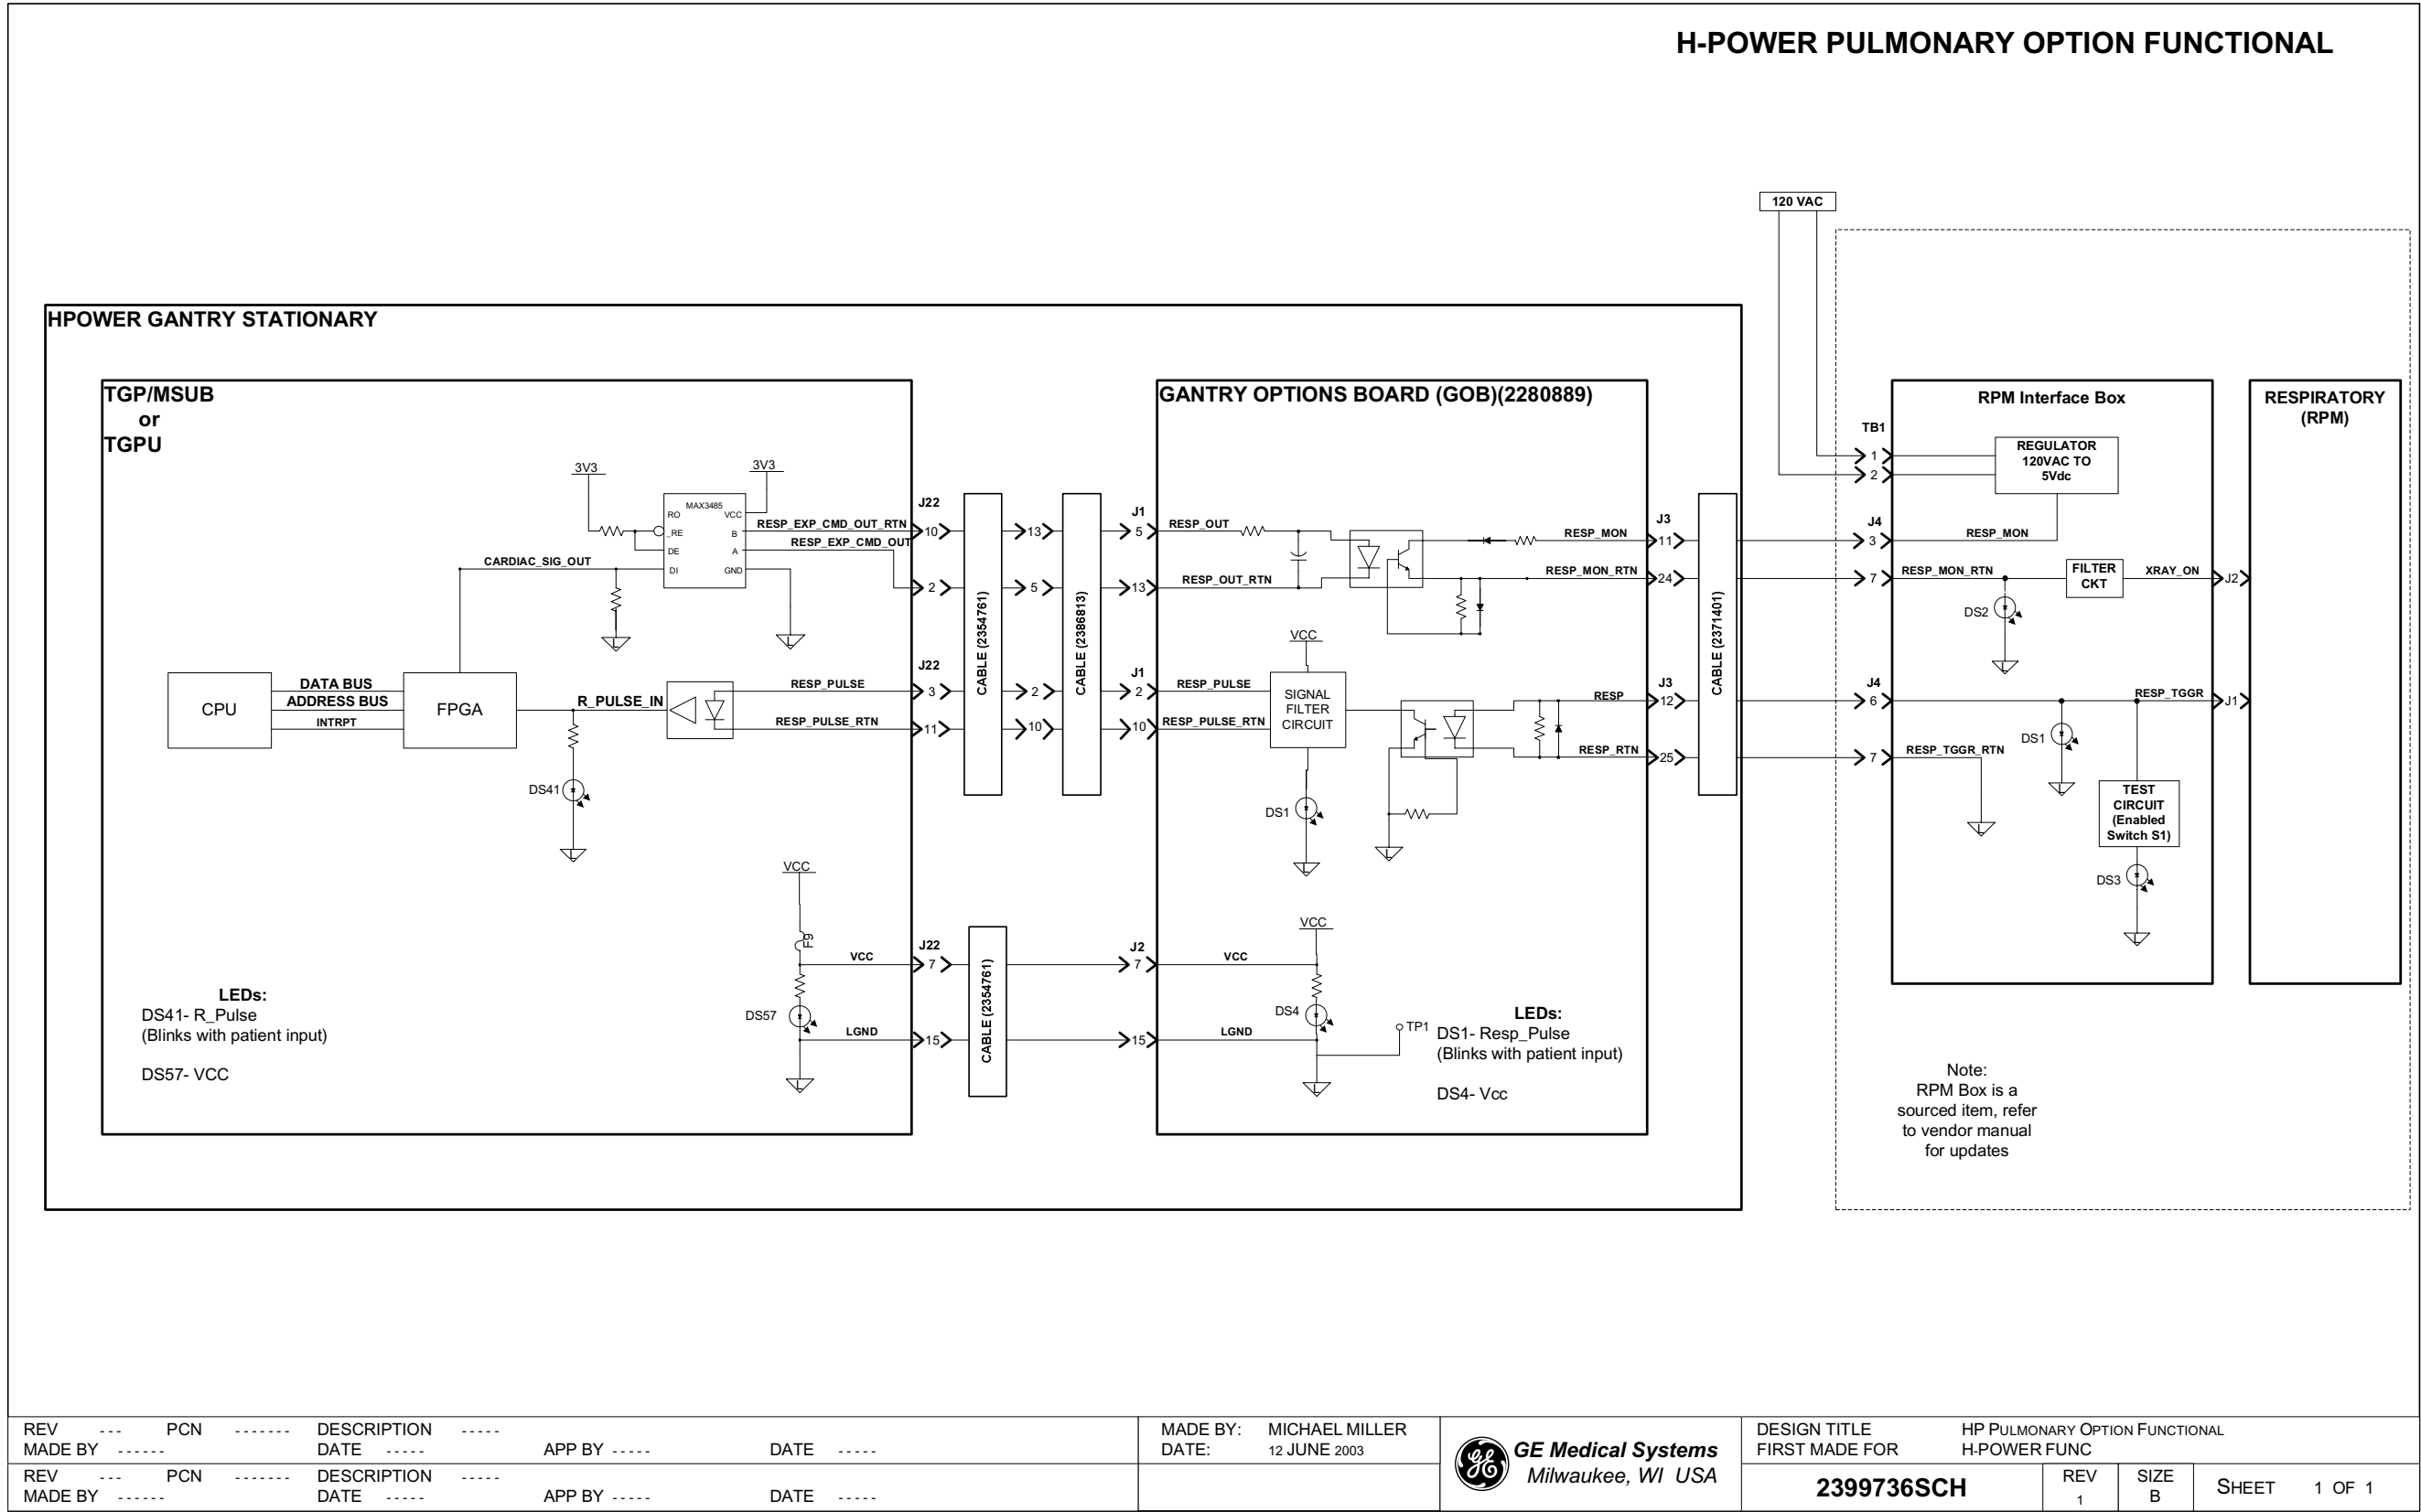


Figure 6-4 2399736 Sheet 1, Rev. 1

Section 5.0 — Scan Footswitch and IHHC Controller - 2399737

HP Scan Request Footswitch & Integrated Hand Held Controller Functional

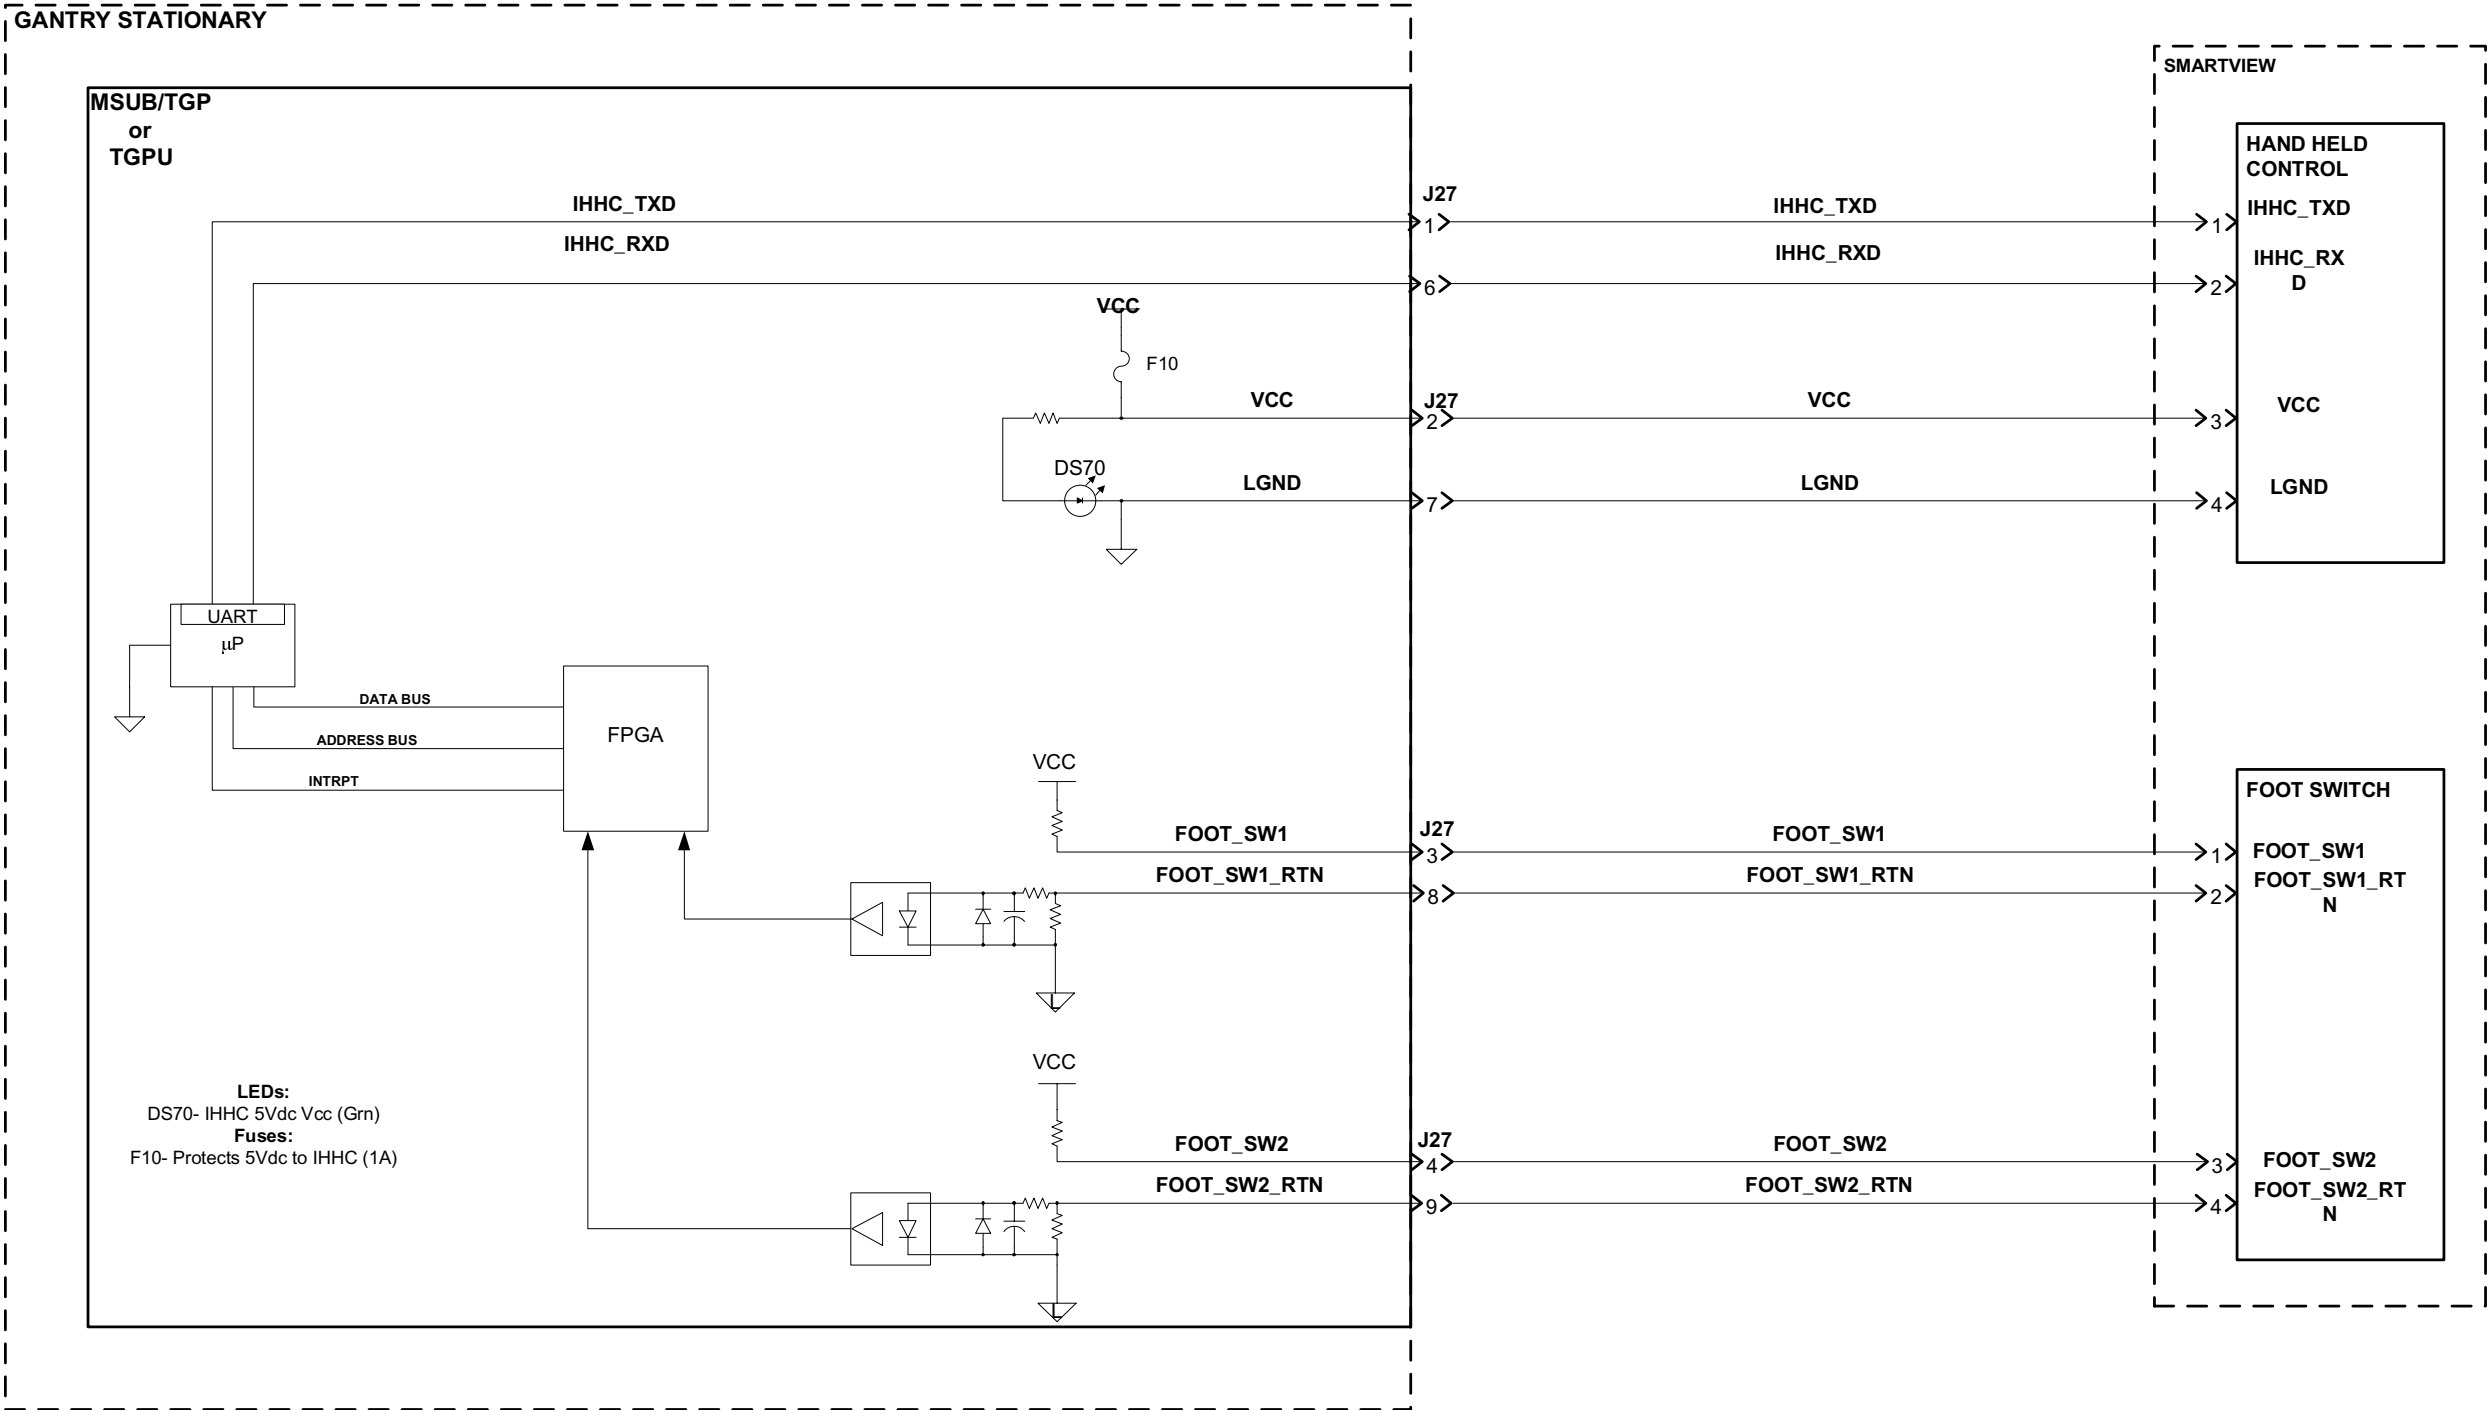

REV --- PCN --- DESCRIPTION --- DATE --- APP BY --- DATE ---	MADE BY: MICHAEL MILLER DATE: 11 JUNE 2001	DESIGN TITLE FIRST MADE FOR	HP Scan Request Footswitch & IHHC FUNCTIONAL H-POWER FUNC	REV 1	SIZE B	SHEET 1 OF 1
REV --- PCN --- DESCRIPTION --- DATE --- APP BY --- DATE ---		2399737SCH				

Figure 6-5 2399737 Sheet 1, Rev. 1

Section 6.0 — Site X-Ray Light, System Light - 2399738

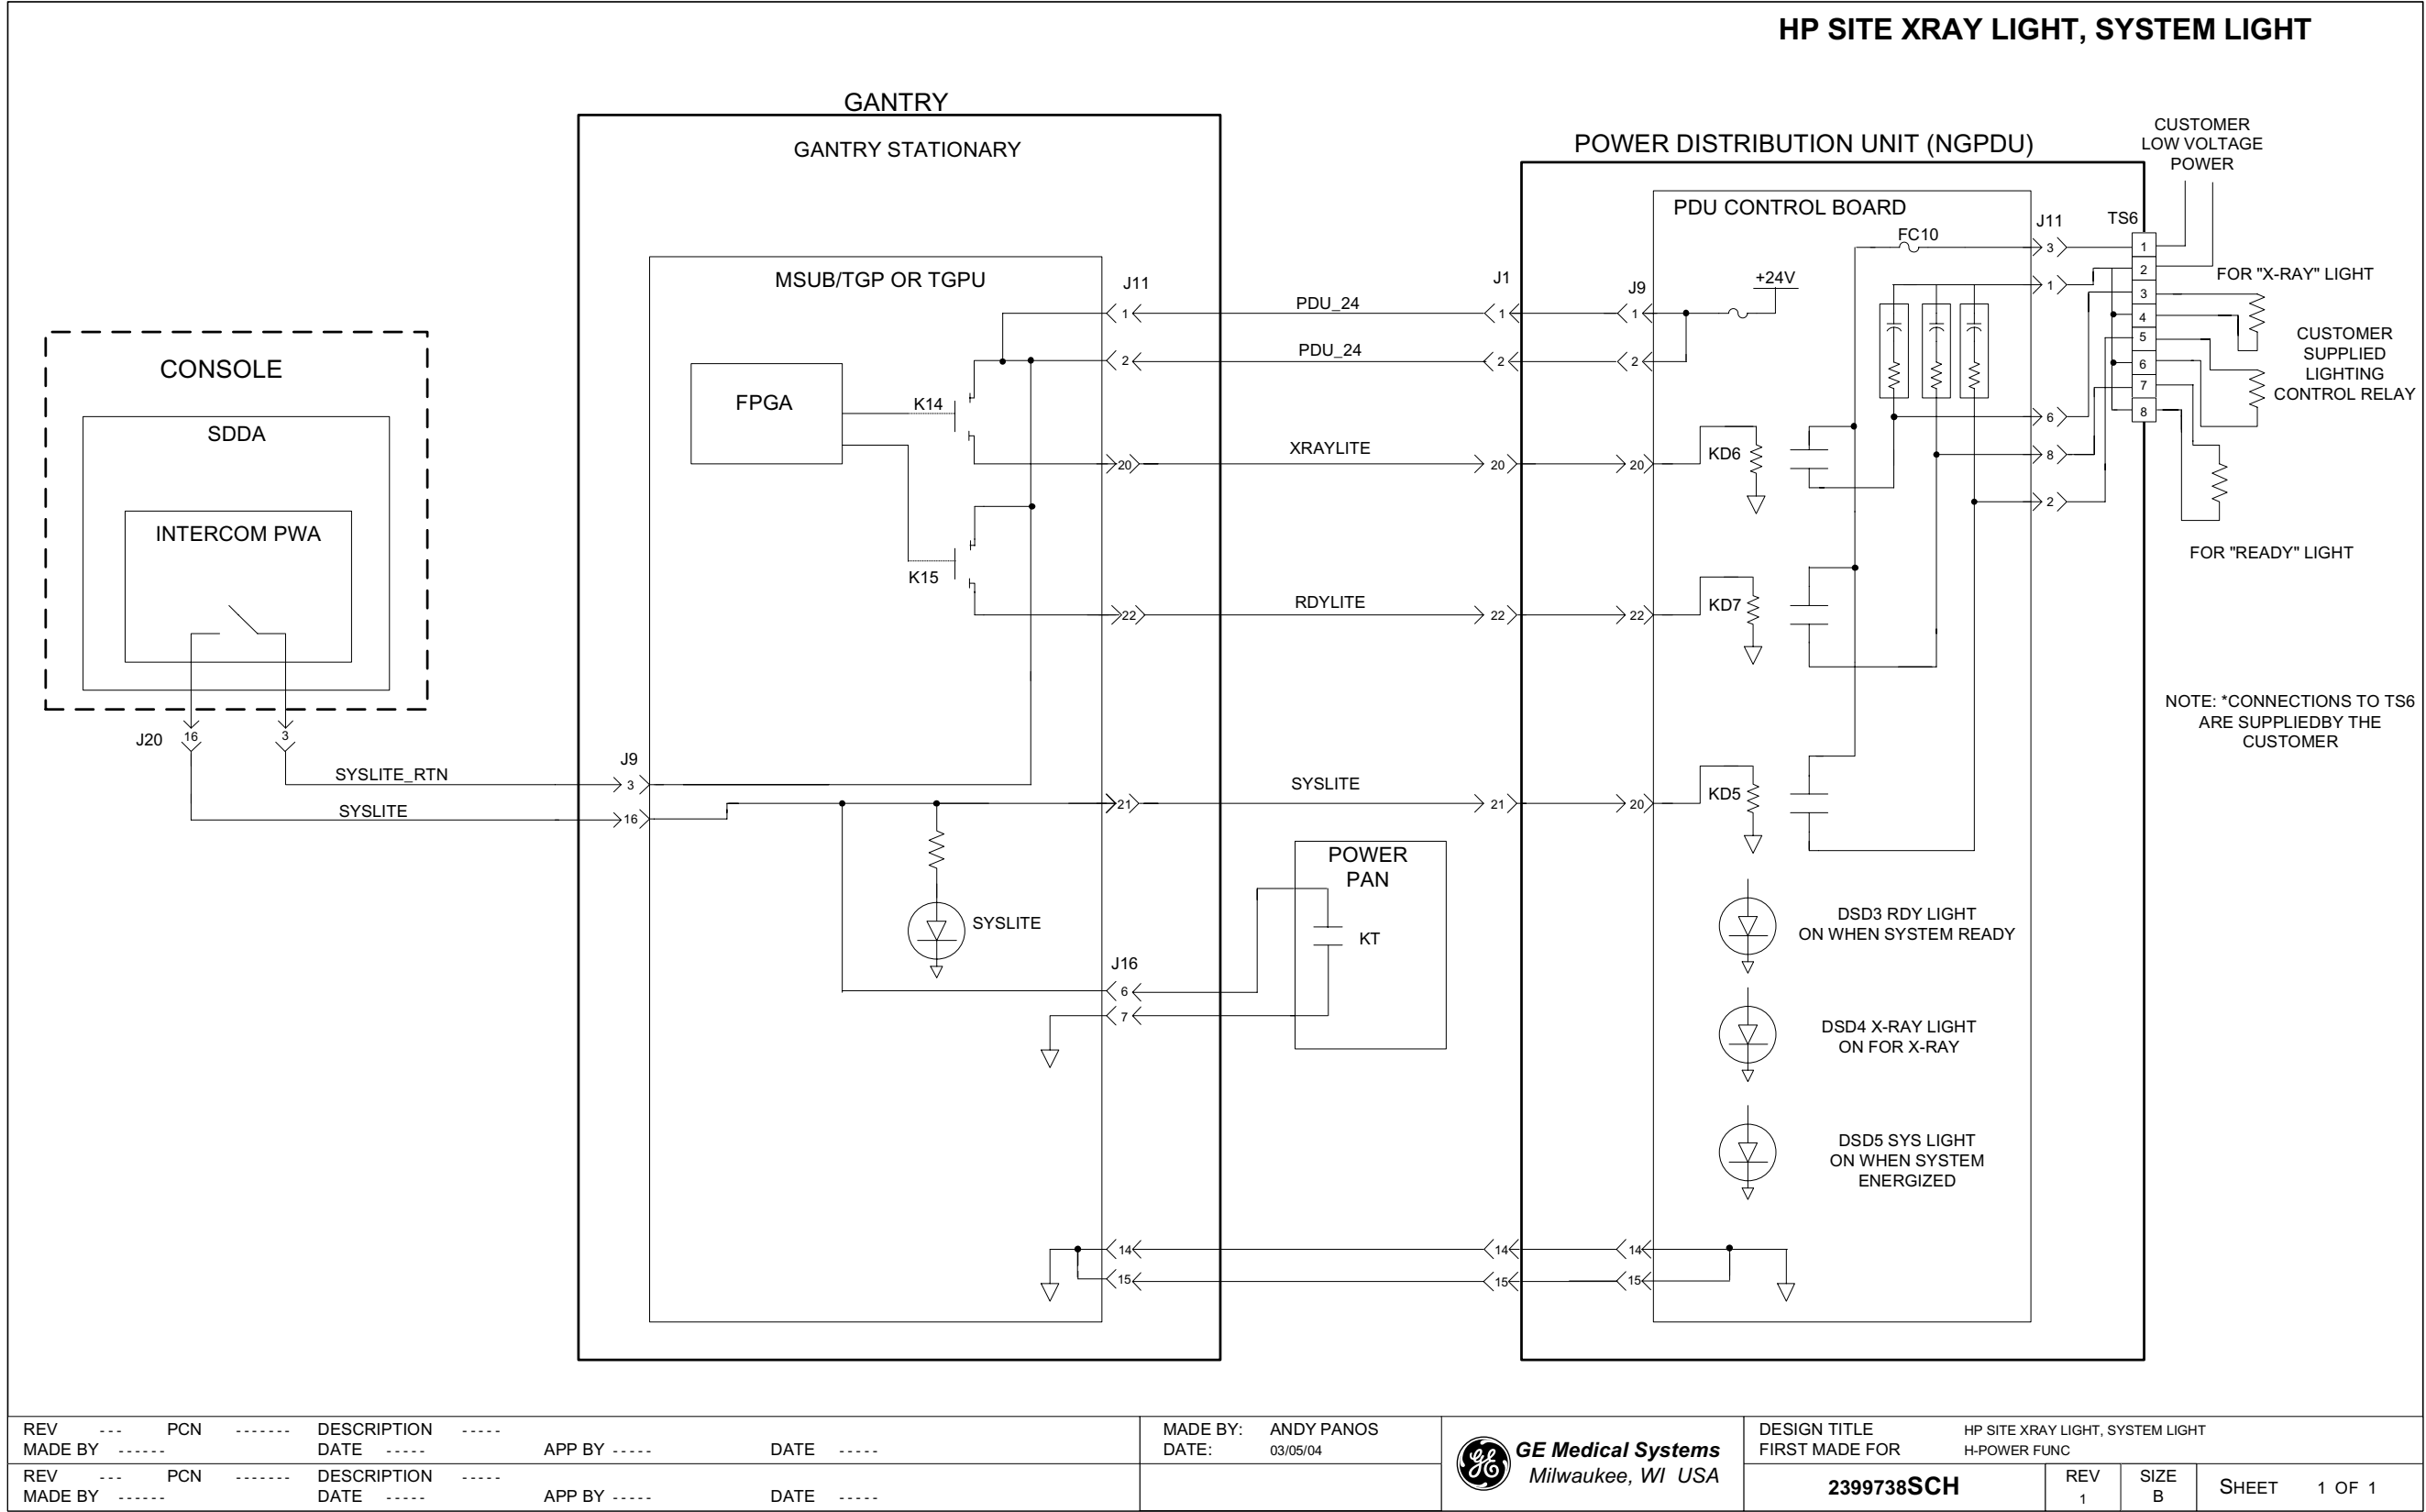


Figure 6-6 2399738 Sheet 1, Rev. 1

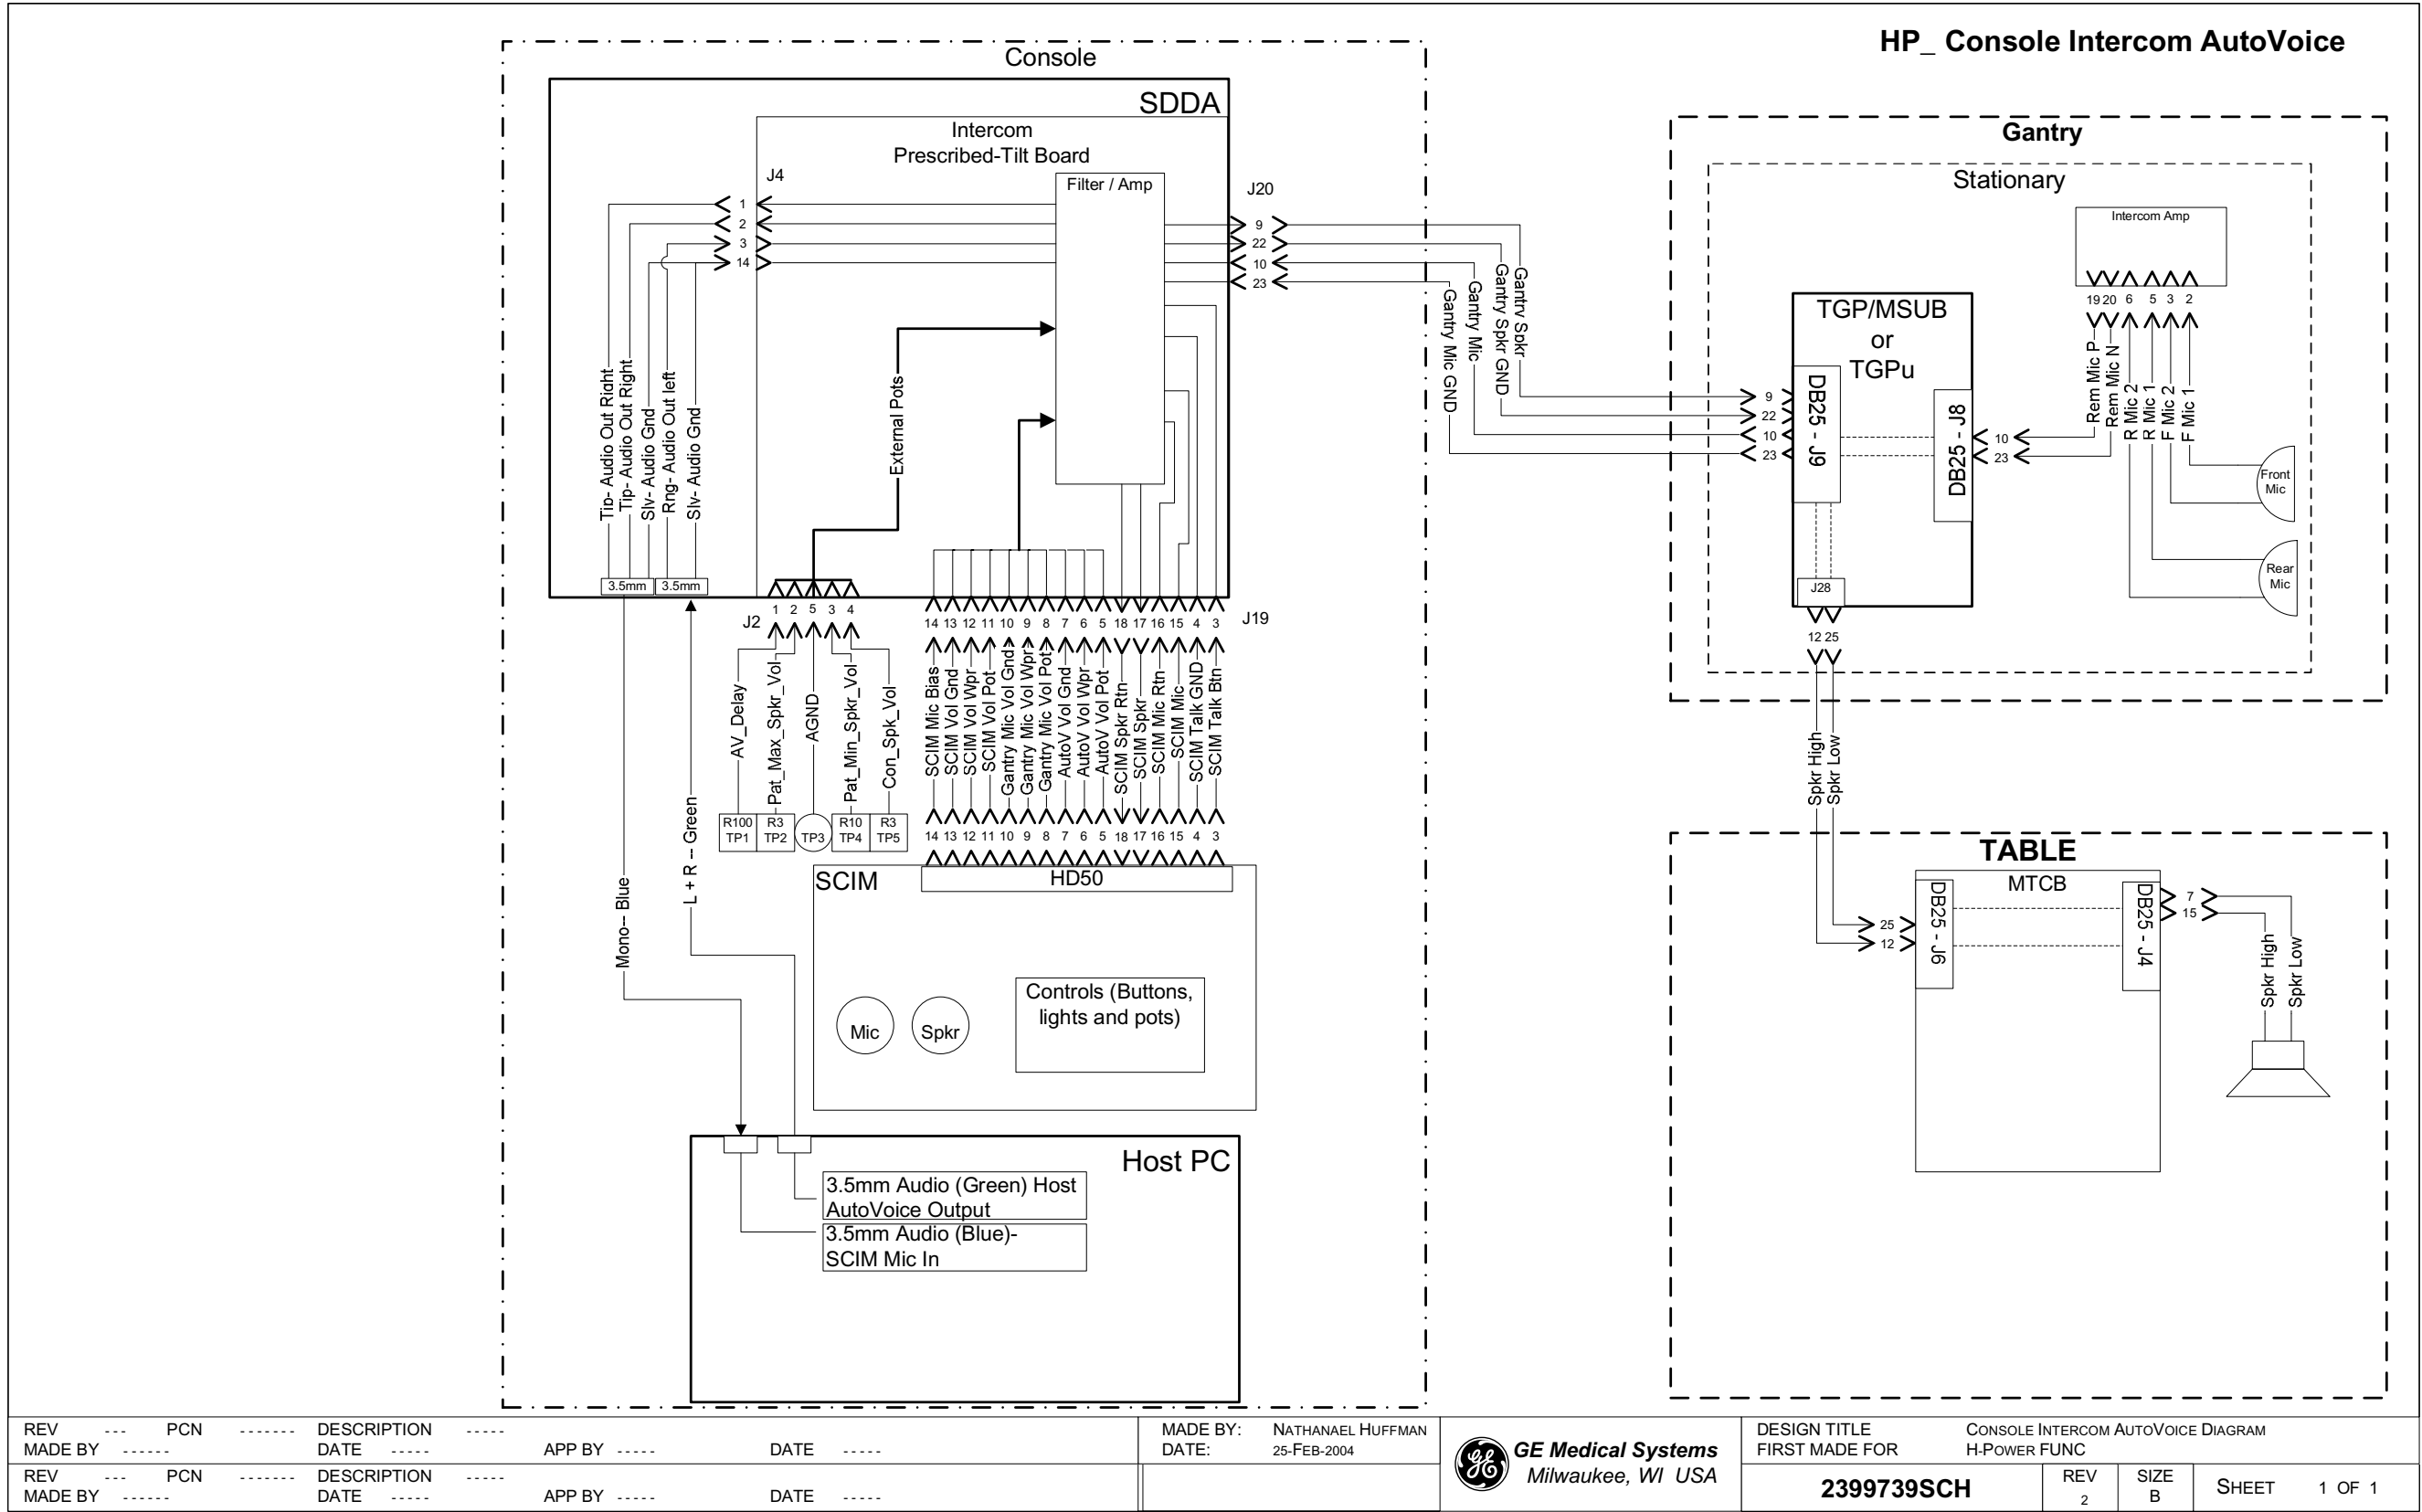


Figure 6-7 2399739 Sheet 1, Rev. 2

Chapter 7

System Monitoring


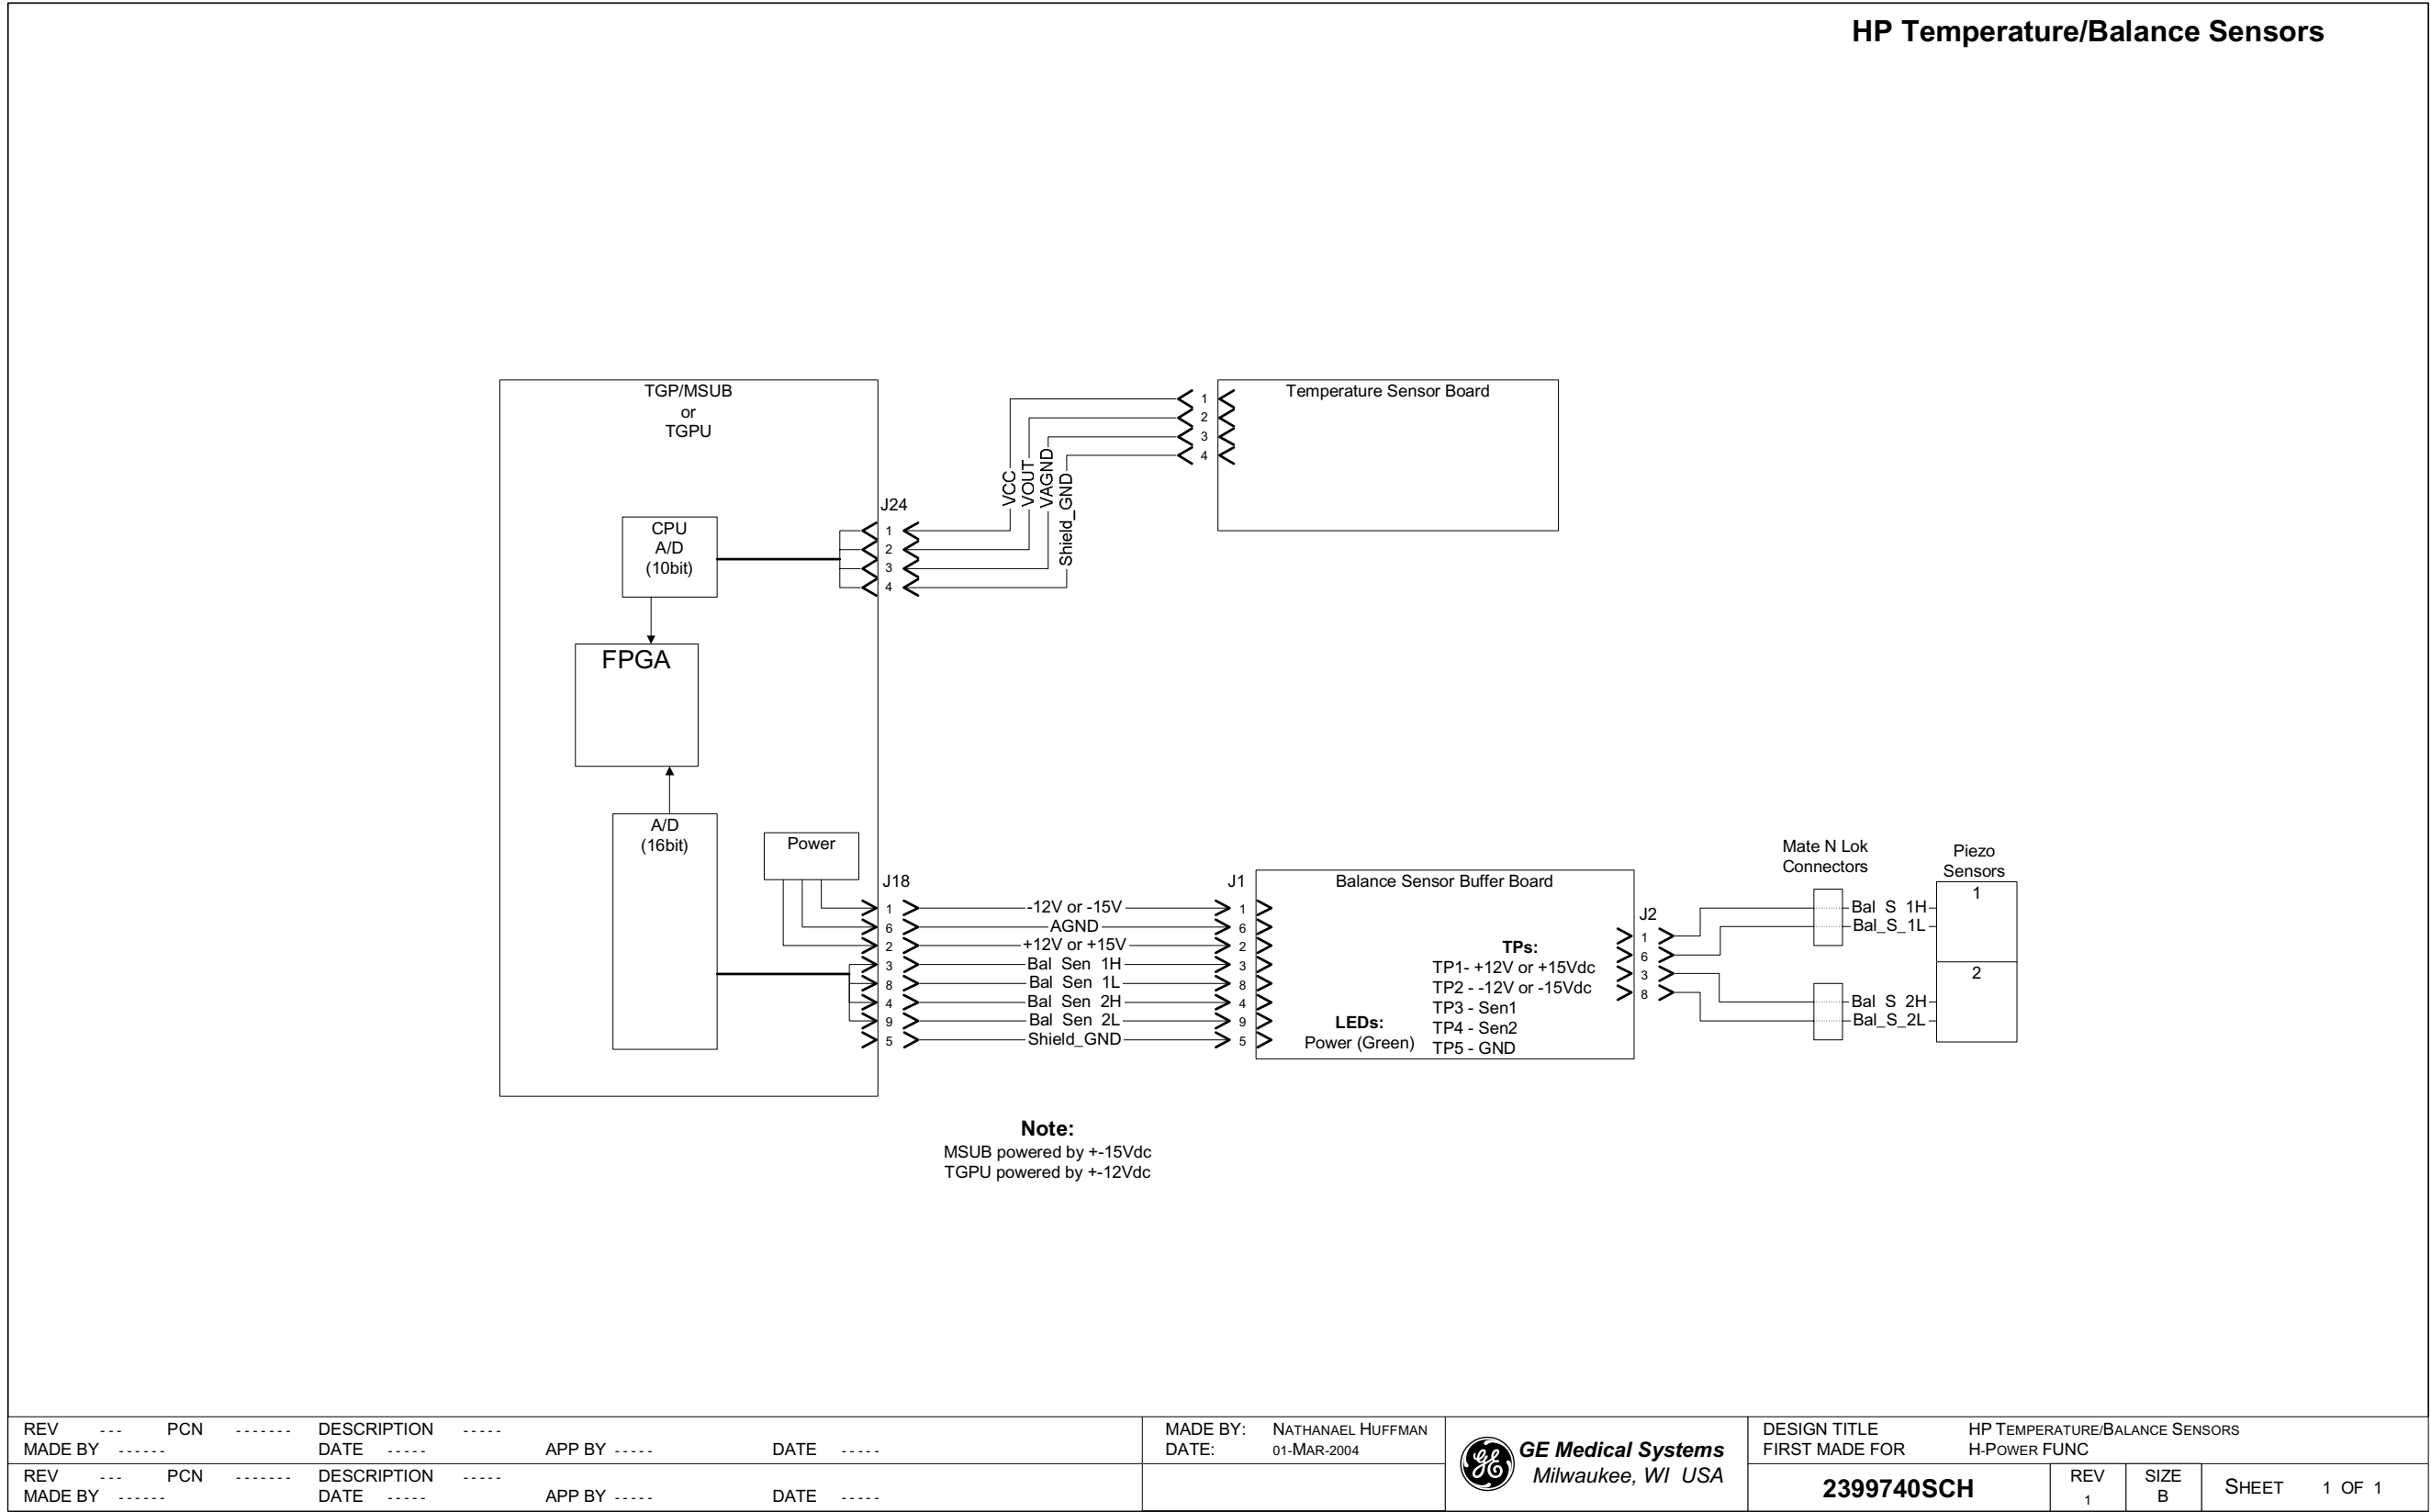


Figure 7-1 2399740 Sheet 1, Rev. 1

Section 2.0 — Gantry Cover Fans - 2399741

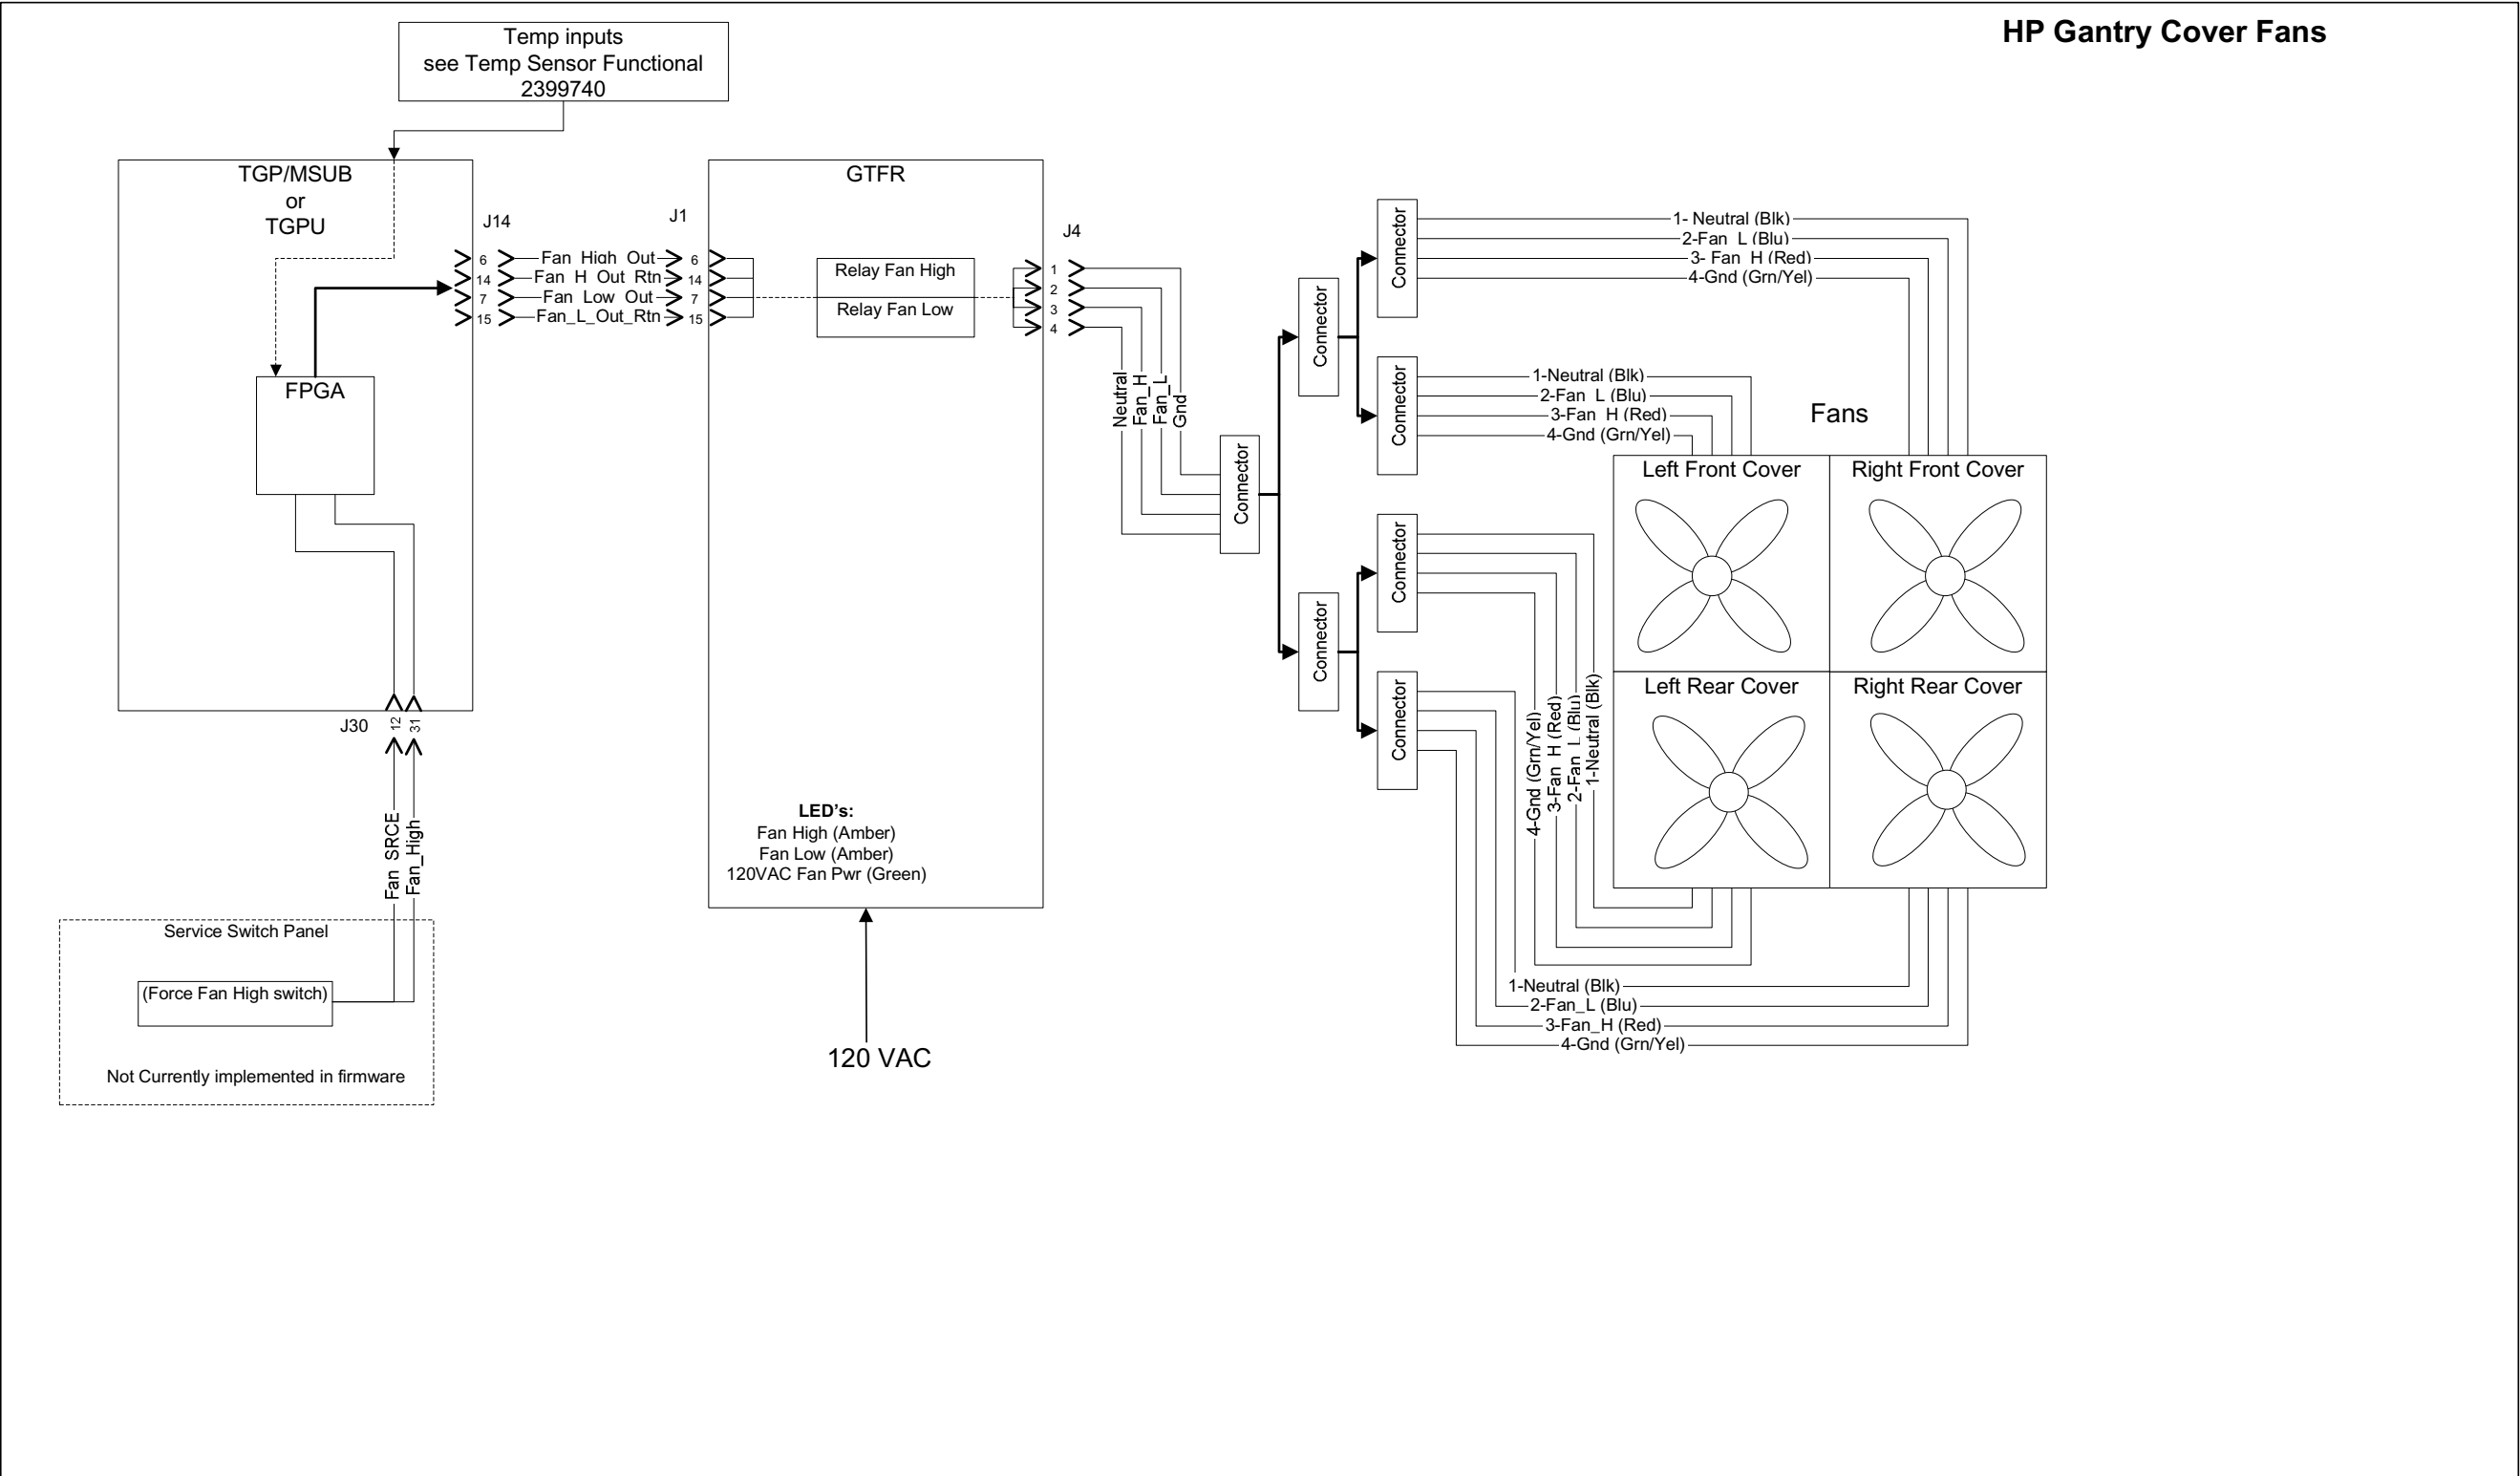

REV --- PCN ----- DESCRIPTION -----	MADE BY: NATHANAEL HUFFMAN	DESIGN TITLE	HP GANTRY COVER FANS			
MADE BY ----- DATE ----- APP BY ----- DATE -----	DATE: 23-FEB-2004	FIRST MADE FOR	H-POWER FUNC			
REV --- PCN ----- DESCRIPTION -----	GE Medical Systems Milwaukee, WI USA	2399741SCH	REV 1	SIZE B	SHEET 1 OF 1	
MADE BY ----- DATE ----- APP BY ----- DATE -----						

Figure 7-2 2399741 Sheet 1, Rev. 1

THIS PAGE INTENTIONALLY BLANK.

Chapter 8

System Power Control

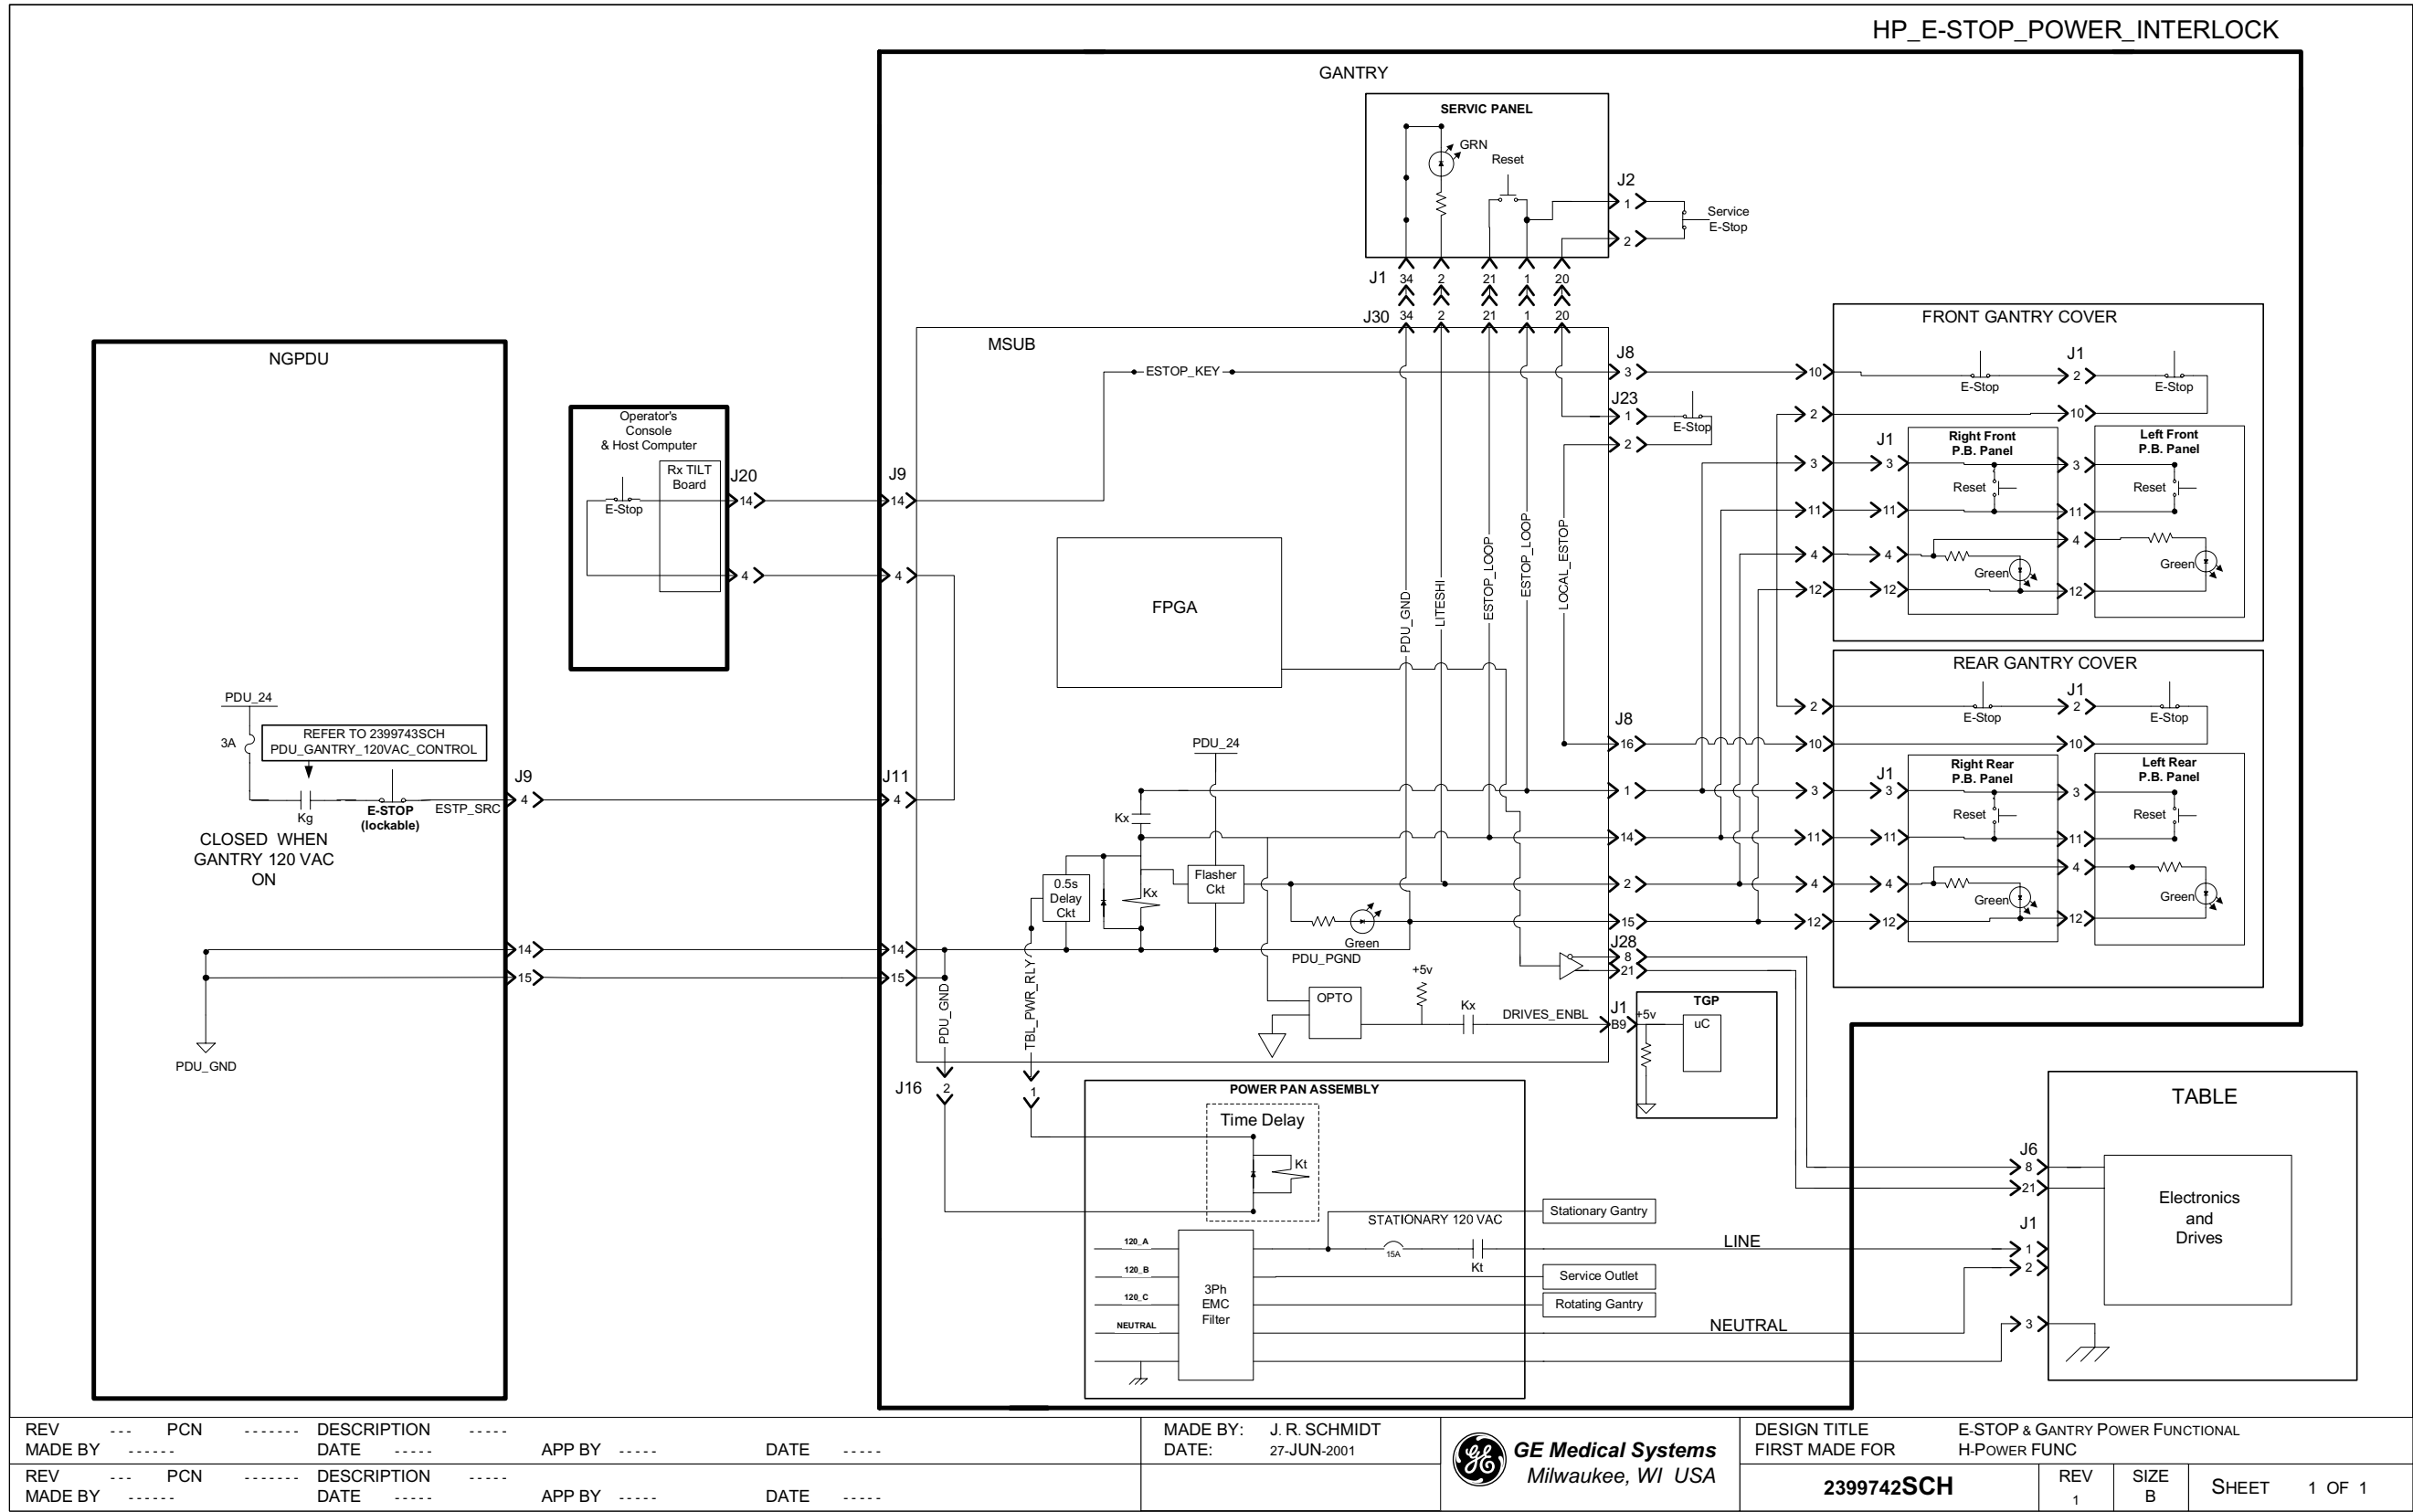


Figure 8-1 2399742 Sheet 1, Rev. 1

Section 2.0 — PDU - Gantry 120 VAC Control - 2399743

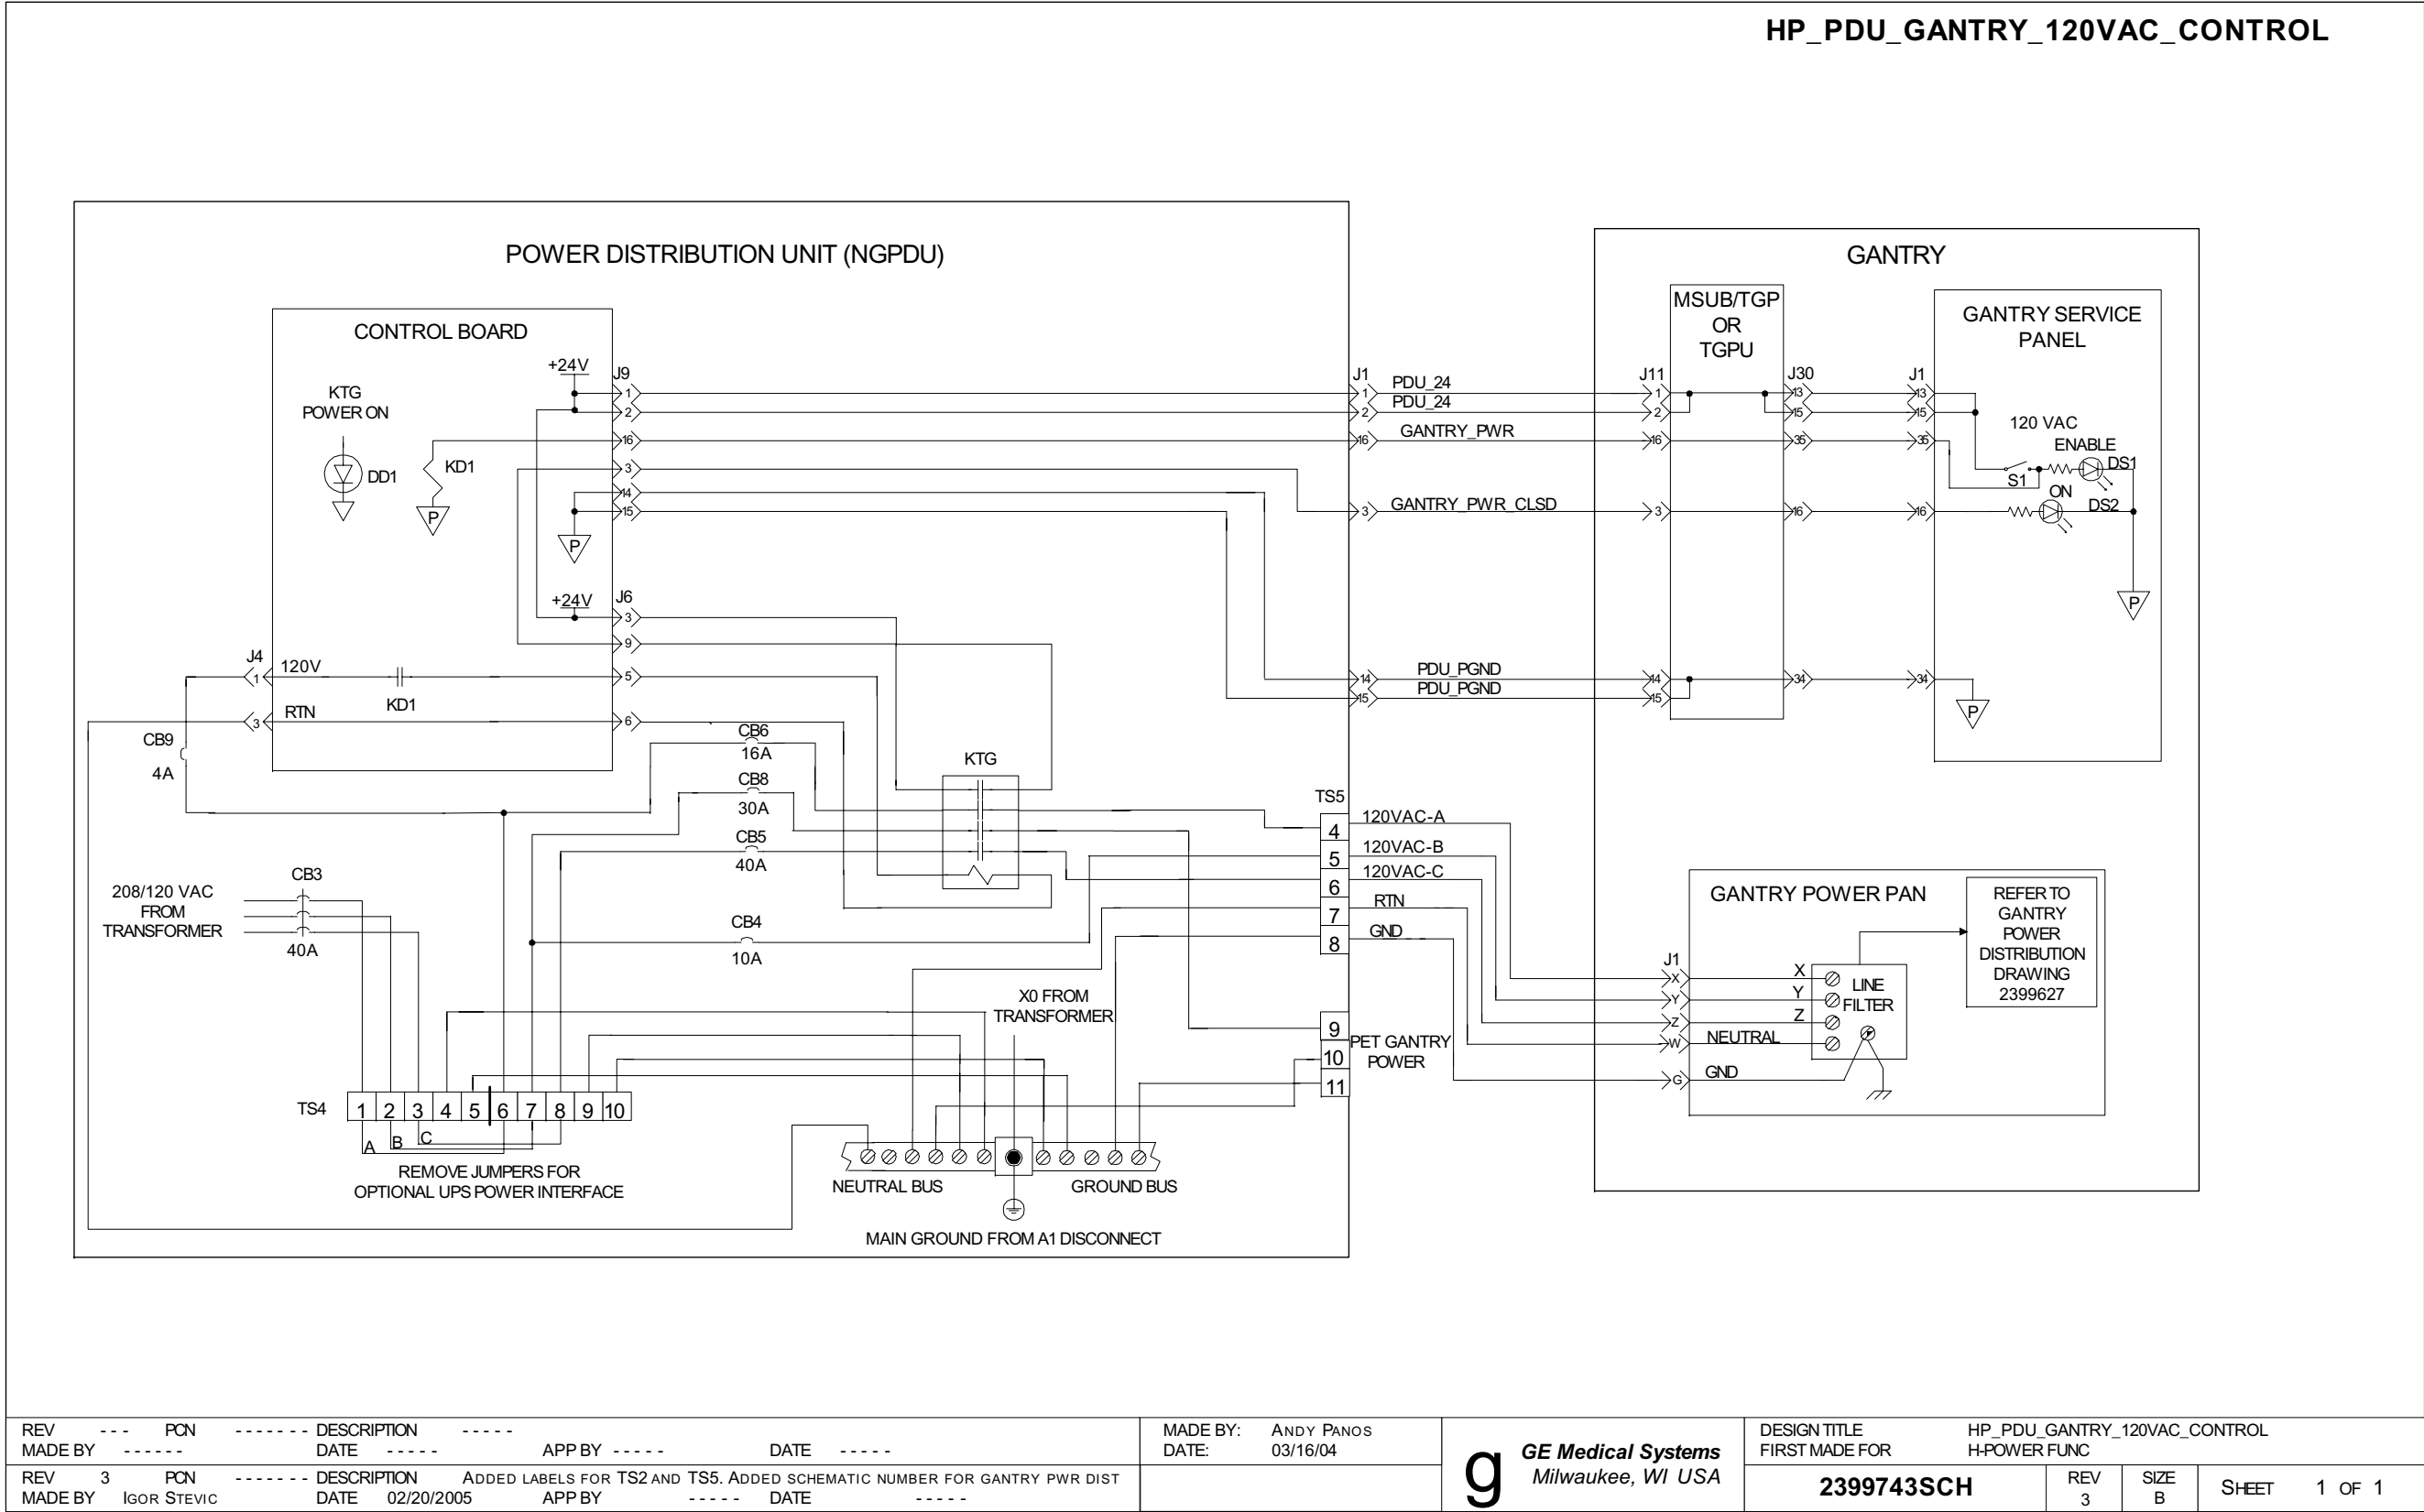


Figure 8-2 2399743 Sheet 1, Rev. 3

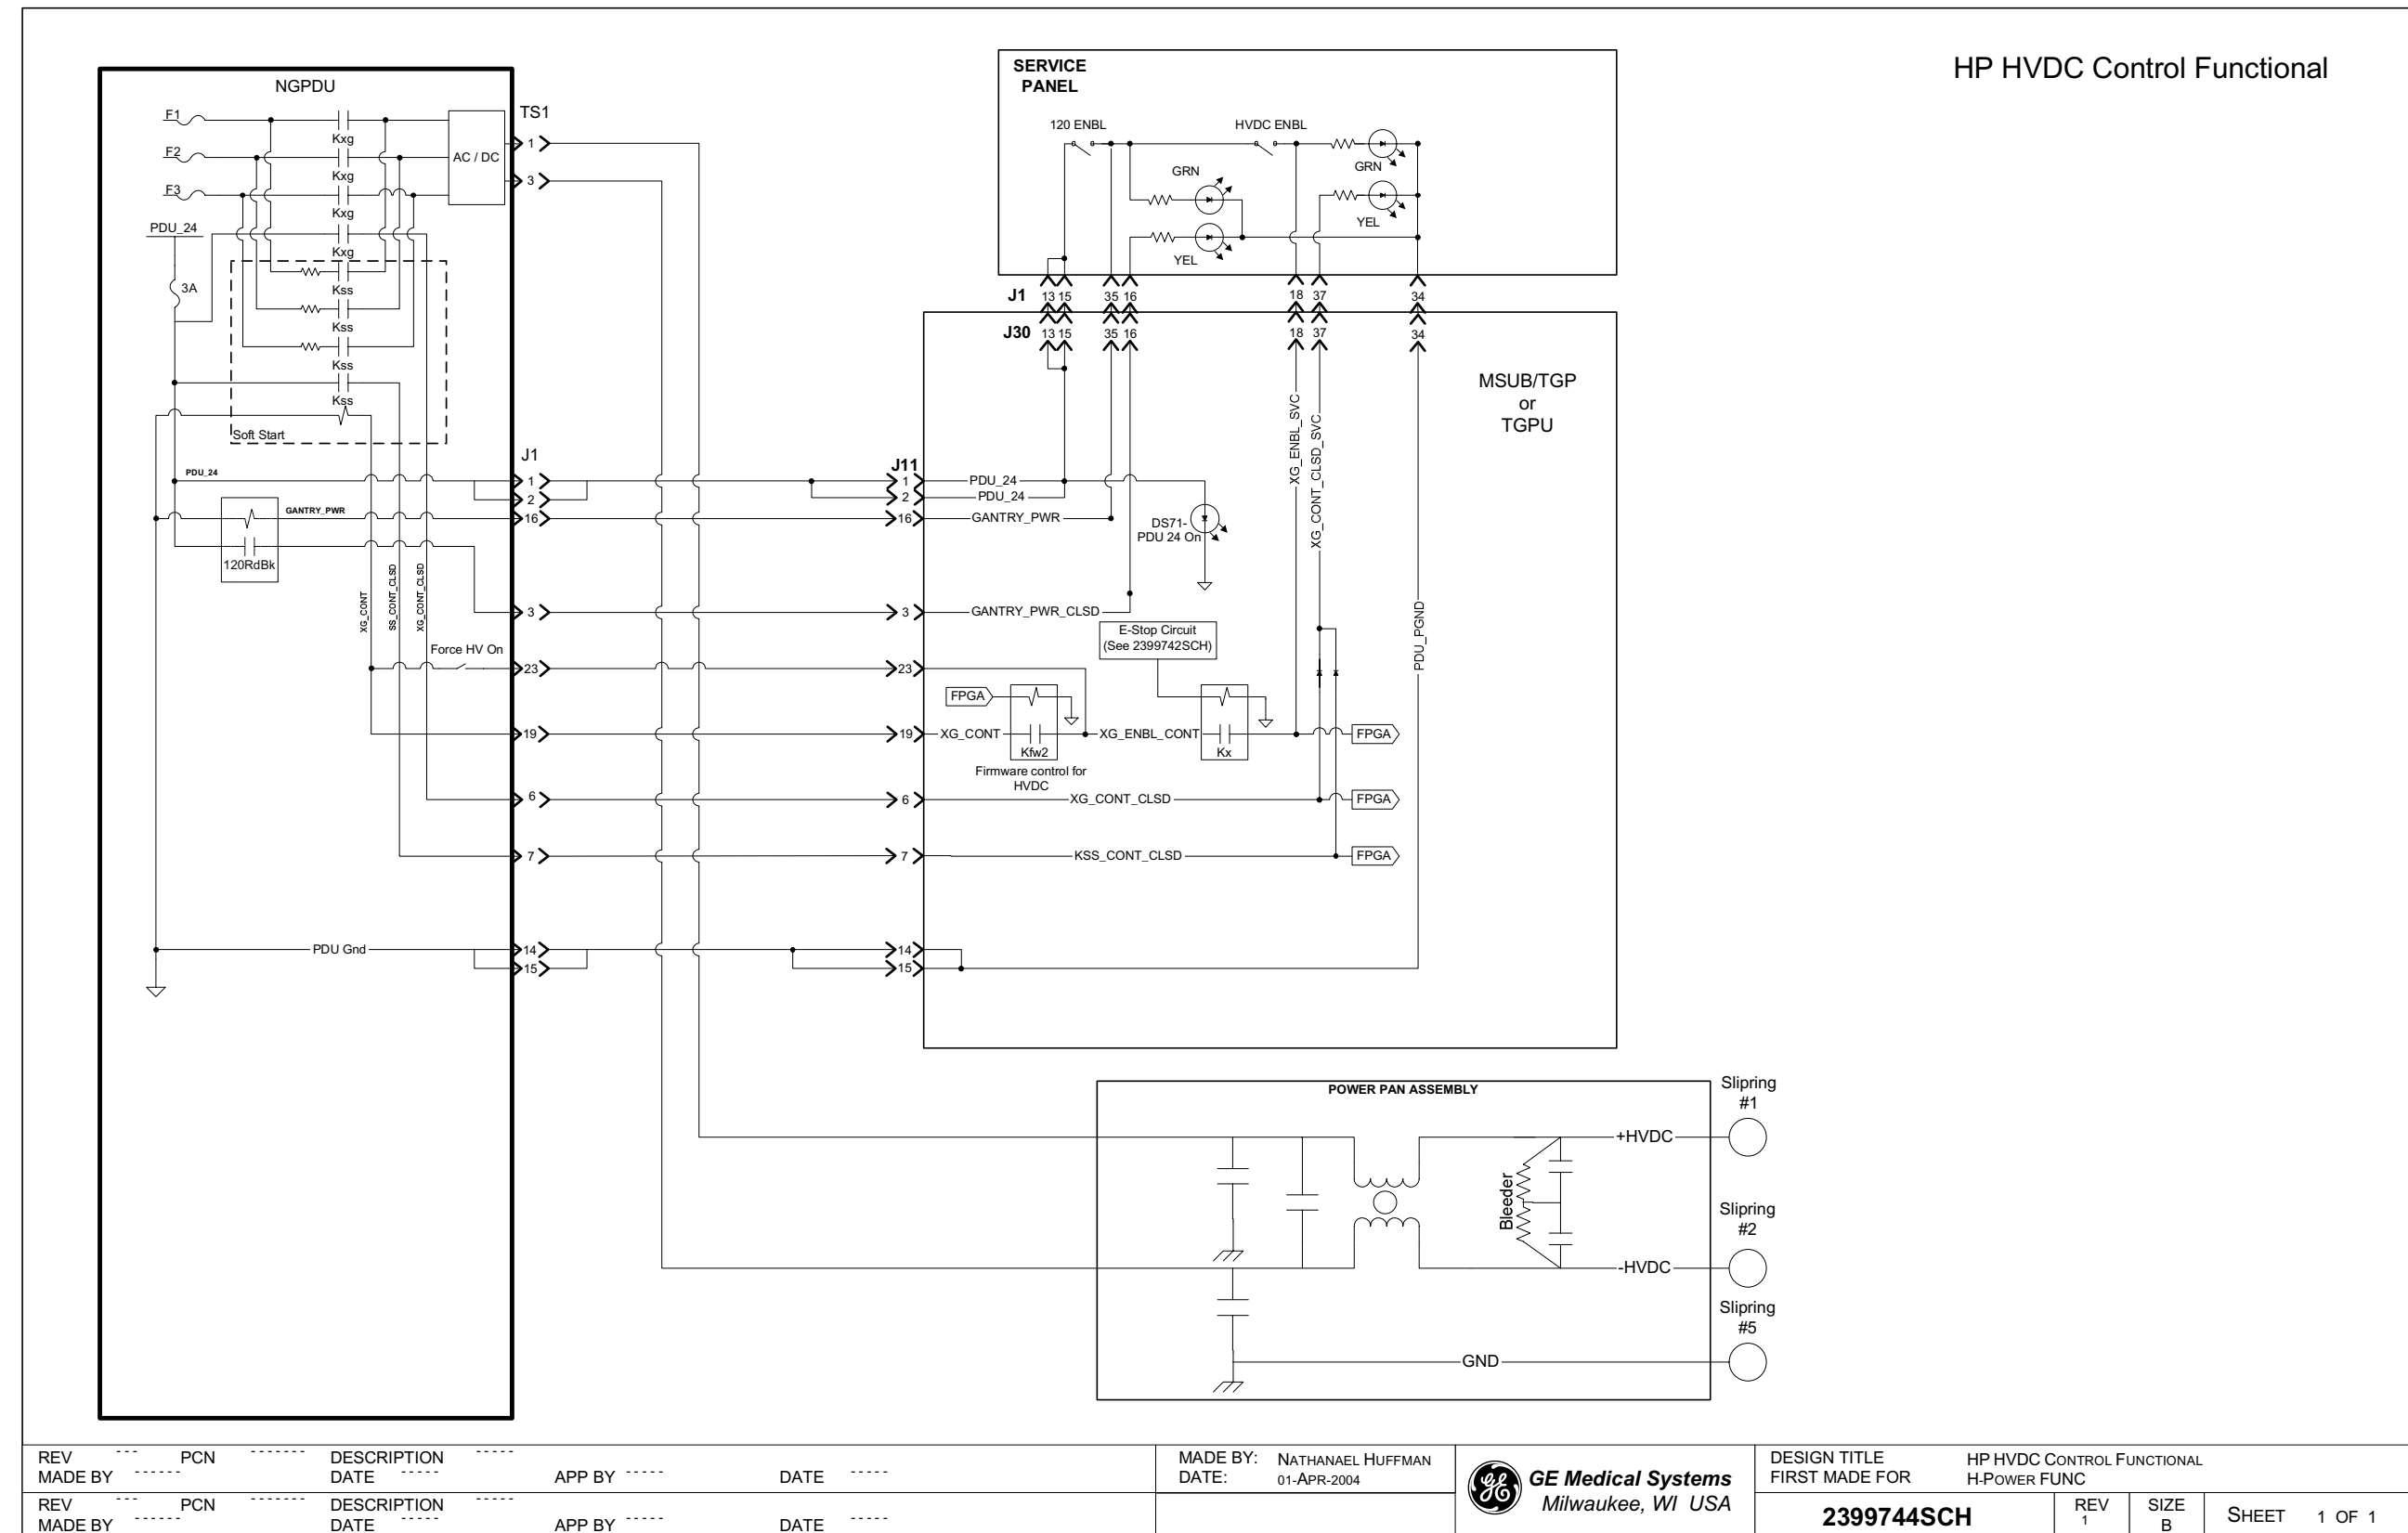


Figure 8-3 2399744 Sheet 1, Rev. 1

Section 4.0 — HP MDAS/GDAS Gantry Power Distribution - 2399627

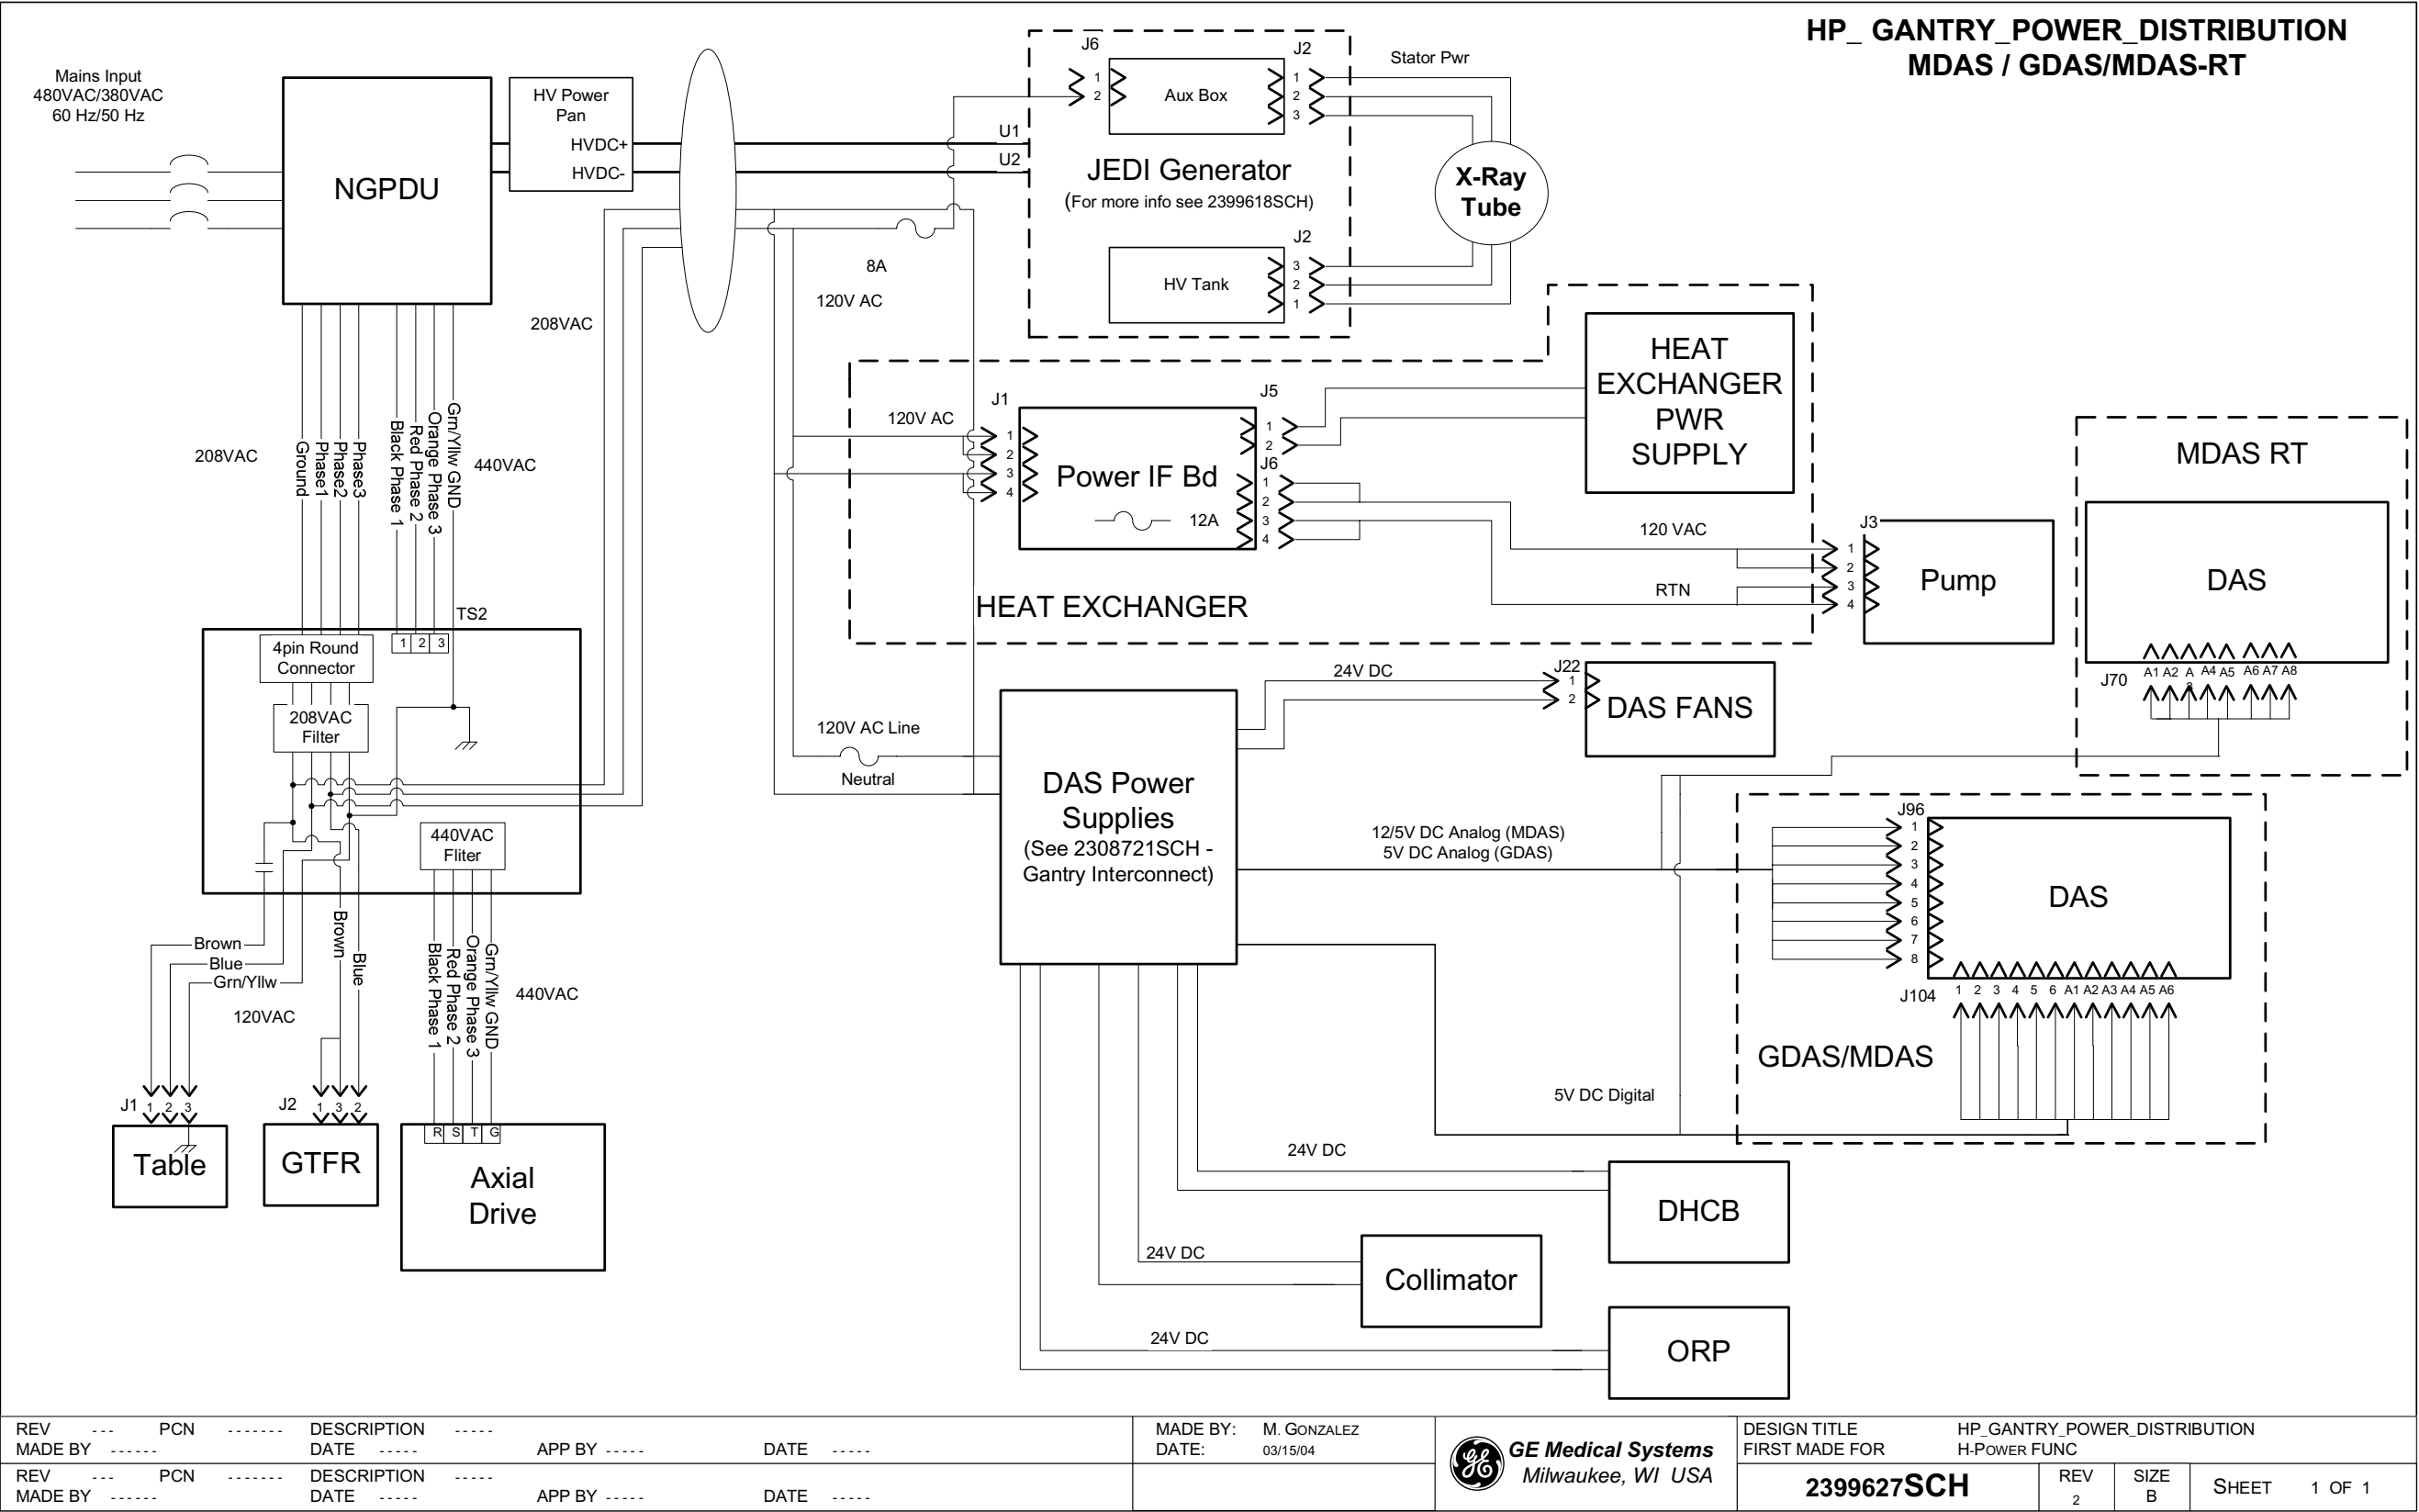


Figure 8-4 2399627 Sheet 1, Rev. 2

THIS PAGE INTENTIONALLY BLANK.