

Technical Publications

**Direction 2191031SNT
Revision 0**

**Service Note: T-1395
Checking ISO Compliance of CT Service Documentation**

Property of GE Medical Systems

**For GE Service Personnel Only
No Rights Licensed.
DO NOT USE OR COPY
Disclosure to Third Parties Prohibited**

Copyright © 1997 by GE Company



Restricted to General Electric Medical Systems (GEMS) personnel only.

Permission to use this Restricted Service Software and related documentation (hereinafter called the "Material") by persons other than GE Medical Systems employees is prohibited. This Material is the property of GEMS and contains information which is restricted to use by GEMS Manufacturing, Engineering and Service personnel. Any reproduction in whole or in part is strictly prohibited. Neither this material nor any information contained herein shall be disclosed to anyone outside of GEMS Manufacturing, Engineering and Service personnel.

If you are not a GE Medical Systems employee, you must exit this material now.

Revision History		
Revision	Date	Reason for Change
0	June, 04, 97	Initial Release

List Of Effective Pages			
PAGE #	PAGE #	PAGE #	PAGE #
0 through 4			

GE Exclusive Use Only
SERVICE NOTE

May 16, 1997

Page 3 of 6

FILE TITLE

Checking ISO Compliance of CT Service Documentation

T-1395

Process to Determine Revision Status of CT Directions

Purpose

Increase GEMS Service effectiveness and efficiency in remaining ISO9000 compliant.

Effectivity


All active and current Directions supporting CT8800, CT9800, HLA, HSA-Z, RP1.x, RP2.x and CT/i systems.

Problem

Different procedures have been used for determining the current revision level of a Direction, some of which are very time consuming and in many cases requiring several phone calls. There is a very simple procedure to locate the current revision level of any Direction, which has been released for distribution.

Procedure

1. Access GEMS' Mainframe (IBM) and enter PCICS.

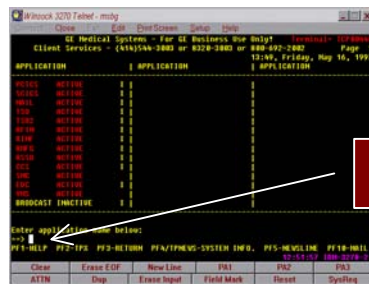

Enter PCICS

GE Exclusive Use Only
SERVICE NOTE

May 16, 1997


Page 4 of 6

FILE TITLE

Checking ISO Compliance of CT Service Documentation


T-1395

2. Enter your name and password.

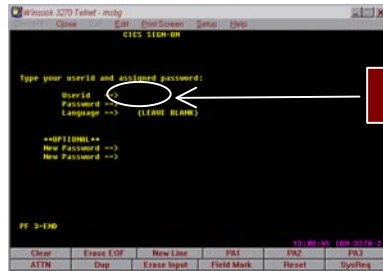


Name & Password

3. On the APPLICATION MENU, select "GLOBAL PRODUCT CONFIGURATION", and press ENTER.

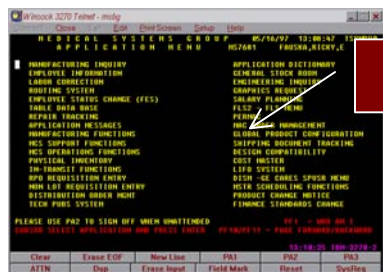

Select GLOBAL PRODUCT CONFIGURATION

4. On the GPS (GLOBAL PRODUCT CONFIGURATION) Main Menu, select "Inquiry Menu", and press ENTER.

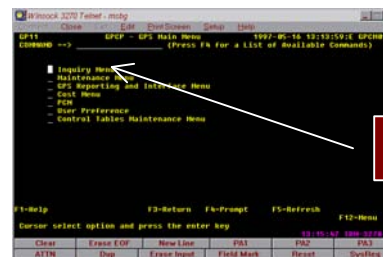

Inquiry Menu

GE Exclusive Use Only
SERVICE NOTE

May 16, 1997

Page 5 of 6

FILE TITLE

Checking ISO Compliance of CT Service Documentation

T-1395

5. On the GIM Inquiry Menu, select “Item Inquiry/ Search Menu”, then press ENTER.



6. Type in the Direction number on the “Number” line as follows:

- Old directions often used abbreviated numbering. For these Directions, such as 18xxx# (e.g. Direction 18301), type in its number preceded by 46–0. In this example, the proper entry would be 46–015301.
- For Directions labeled with the 46# (example: Direction 46–003012) type in the entire number the way it appears on the document’s title page.
- New GEMS-AM & GEMS-A Directions use the new seven digit numbering system. For Directions with a seven digit number (e.g. Direction 2153389), type in the seven number in its entirety.
- For Old YMS Directions, type in the alphanumeric number for the Direction. For example, the proper entry for the Pro-Speed Theory Manual would be P9011CQ.

Note: Entries are not case sensitive.

GE Exclusive Use Only
SERVICE NOTE

May 16, 1997


Page 6 of 6

FILE TITLE


Checking ISO Compliance of CT Service Documentation

T-1395

7. Tab to “Item Inquiry”, then press ENTER.

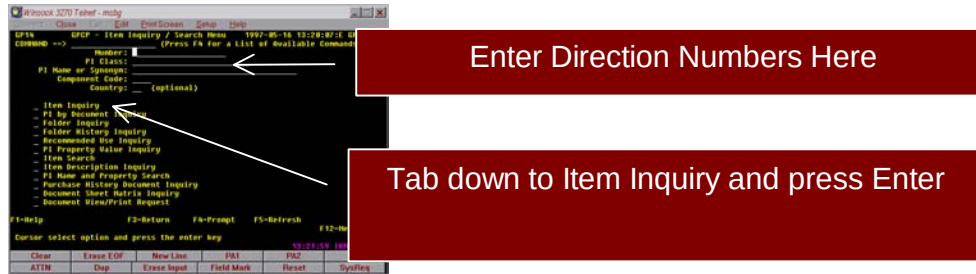

Note: The revision level of the document is displayed in the “Revision:” field (to the right of the “PI Number” field). This number represents the latest revision of the document, which is stocked in the Distribution Center. If you do not have the latest revision to a document, order it immediately via Common Forms. If you are not on the appropriate tab you may need your Manager or ASM signature to order a Proprietary Direction.

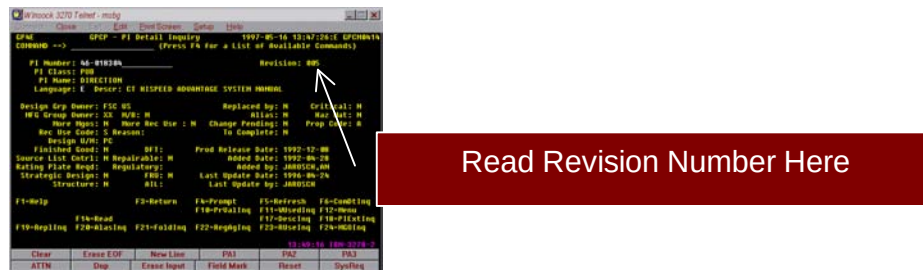

Acknowledgments

Instructions adapted to CT needs from MR SN 60738B, authored by Mike Keber of MR Service Engineering