

IMAGE DATA SHEET

QA Phantom #1


QA#1 MTF and CONTRAST SCALE

QA#1/S/10mm/120KV/170mA/2sec Scan at 0 mm Use this slice data for following Bone Retro.

Exam # # of Slice	MTF	MTF 4 slice average	Contrast Scale	Comments	Scan Tech Aprov.
SPECS	---	0.68 to 1.0	110.0 to 130.0	---	---

Box Size : 17 x 17 pixels

Image Acceptance Date: _____ Image Reviewer: _____

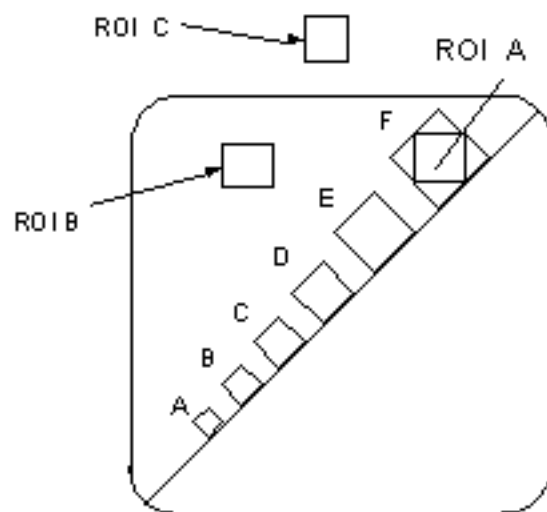

SD_A = Standard deviation of Roi Box over F bar pattern in plexiglass.

SD_{ave} = Average standard deviation of plexiglass and water (i.e., image noise),
 $SD_{ave} = (SD_B + SD_C) / 2$.

Contrast Scale = mean of B - mean of C

Modulation = $(SD_A^2 - SD_{ave}^2)^{1/2}$

MTF = $2.2 \times (\text{Modulation} / \text{Contrast Scale})$

QA#1/S/10mm/120KV/170mA/2sec/ Bone Retro/ DISPLAY FOV=15cm Scan at 0 mm

Exam # # of Slice	Line Patterns Visible	Artifacts	Comments	Scan Tech Aprov.
SPECS	B, C, D, E, F	---	---	---

Image Acceptance Date: _____ Image Reviewer: _____