



GE Medical Systems

Technical Publication

Direction 2370773-100

Revision 3

4.X, 3.X LightSpeed Series

Application Tips and Work-Arounds

Copyrighted © by GE Medical Systems, 2003



Page Left Intentionally Blank

DAMAGE IN TRANSPORTATION

All packages should be closely examined at time of delivery. If damage is apparent write "Damage In Shipment" on ALL copies of the freight or express bill BEFORE delivery is accepted or "signed for" by a GE representative or hospital receiving agent. Whether noted or concealed, damage MUST be reported to the carrier immediately upon discovery, or in any event, within 14 days after receipt, and the contents and containers held for inspection by the carrier. A transportation company will not pay a claim for damage if an inspection is not requested within this 14 day period.

Call Traffic and Transportation, Milwaukee, WI (262) 785 5052 or 8*323 5052 immediately after damage is found. At this time be ready to supply name of carrier, delivery date, consignee name, freight or express bill number, item damaged and extent of damage. Complete instructions regarding claim procedure are found in Section S of the Policy And Procedures Bulletins. 14 July 1993.

CERTIFIED ELECTRICAL CONTRACTOR STATEMENT

All electrical Installations that are preliminary to positioning of the equipment at the site prepared for the equipment shall be performed by licensed electrical contractors. In addition, electrical feeds into the Power Distribution Unit shall be performed by licensed electrical contractors. Other connections between pieces of electrical equipment, calibrations and testing shall be performed by qualified GE Medical personnel. The products involved (and the accompanying electrical installations) are highly sophisticated, and special engineering competence is required. In performing all electrical work on these products, GE will use its own specially trained field engineers. All of GE's electrical work on these products will comply with the requirements of the applicable electrical codes.

The purchaser of GE equipment shall only utilize qualified personnel (i.e., GE's field engineers, personnel of third-party service companies with equivalent training, or licensed electricians) to perform electrical servicing on the equipment.

IMPORTANT...X-RAY PROTECTION

X-ray equipment if not properly used may cause injury. Accordingly, the instructions herein contained should be thoroughly read and understood by everyone who will use the equipment before you attempt to place this equipment in operation. The General Electric Company, Medical Systems Group, will be glad to assist and cooperate in placing this equipment in use.

Although this apparatus incorporates a high degree of protection against x-radiation other than the useful beam, no practical design of equipment can provide complete protection. Nor can any practical design compel the operator to take adequate precautions to prevent the possibility of any persons carelessly exposing themselves or others to radiation.

It is important that anyone having anything to do with x-radiation be properly trained and fully acquainted with the recommendations of the National Council on Radiation Protection and Measurements as published in NCRP Reports available from NCRP Publications, 7910 Woodmont Avenue, Room 1016, Bethesda, Maryland 20814, and of the International Commission on Radiation Protection, and take adequate steps to protect against injury.

The equipment is sold with the understanding that the General Electric Company, Medical Systems Group, its agents, and representatives have no responsibility for injury or damage which may result from improper use of the equipment. Various protective materials and devices are available. It is urged that such materials or devices be used.

OMISSIONS & ERRORS

Customers, please contact your GE Sales or Service representatives. GE personnel, please use the GEMS CQA Process to report all omissions, errors, and defects in this publication.

Page Intentionally Left Blank

LEGAL NOTES

COPYRIGHTS

All Material Copyrighted(c) 2001-2003 by the General Electric Company, All rights reserved.

REVISION HISTORY

Revision	Date	Reason for change
0	3/6/2003	402L.1_H4.1M3 +Patch M3 Pilot Release LightSpeed MDAS 16 306L.1_H3.2M3 +Patch M3 Pilot Release LightSpeed MDAS 4/8
1	3/11/2003	Updates based Feedback 402L.1_H4.1M3 +Patch M3 Pilot Release LightSpeed MDAS 16 306L.1_H3.2M3 +Patch M3 Pilot Release LightSpeed MDAS 4/8
2	09/23/2003	404L.2_H4.2GREM3.1 M3.1 Pilot Release MDAS 16 307L.2_H3.3GREM3 Pilot Release MDAS 4/8
3	12/17/2003	405L.5_H4.2M4 Full Production Release PC Based OC and Xstream based OC 308L.5_H3.3M4 Full Production Release PC Based OC and Xstream based OC

Page Left Intentionally Blank

TABLE OF CONTENTS

Legal Notes.....	5
Table of Contents	7
Features for PC and Xstream Based Operator Console Systems	10
SOFTWARE VERSION.....	10
PC BASED COMPUTER HARDWARE.....	10
GLOBAL RECON ENGINE HARDWARE	10
LINUX OPERATING SYSTEM.....	10
MENU DRIVEN REFORMAT	10
ADDITIONAL ADVANCED APPLICATIONS ON THE CONSOLE	10
HIPPA.....	10
AUTO MA	11
SMARTPREP	11
REPEAT SERIES	11
LOW SIGNAL CORRECTION	12
AUTO FILM COMPOSER DEPOSIT TIME.....	12
AUTO TRANSFER.....	12
ANONYMOUS SCAN DATA SAVE	12
CHANGES TO SHUTDOWN	12
CHANGES TO SHUTDOWN	13
IMAGE ANNOTATION	13
CUSTOM ANNOTATION.....	13
New Precautions 405L.5_H4.2M4/308L.5_H3.3M4	15
SYSTEM.....	15
HIPAA LOG IN	15
SCAN.....	15
PATIENT SCHEDULE	16
PERFORMED PROCEDURE STEP (PART OF CONNECT PRO OPTION)	16
PROTOCOL MANAGEMENT	16
SMARTPREP (PURCHASED OPTION)	17
SMARTSTEP (PURCHASED OPTION)	17
RECONSTRUCTION	18
3000 IMAGE SERIES.....	18
RECON MANAGEMENT	19
DISPLAY (APPLIES TO IMAGE WORKS AND EXAMRX DISPLAY)	19

IMAGE WORKS DISPLAY	19
EXAM RX DISPLAY	19
VARIVIEWER	19
DIRECT3D (OPTION)	20
VOLUME VIEWER (OPTION)	20
CTCOLON (OPTION)	20
CARDIQ (OPTION)	21
ADVANCED VESSEL ANALYSIS (OPTION)	21
REFORMAT	21
CT PERFUSION 2 ON OC – PURCHASED OPTION	21
ADD SUBTRACT	22
ARCHIVE	22
FILMING	22
NETWORK	23
IMAGE MANAGEMENT	23
LEARNING AND REFERENCE GUIDE	23
Legacy Precautions	26
SYSTEM	26
TUBE WARM UP/FAST CAL	27
SCAN	27
SMARTPREP (PURCHASED OPTION)	30
PATIENT SCHEDULE	30
CONNECTPRO (PURCHASED OPTION)	30
PERFORMED PROCEDURE STEP (PART OF CONNECT PRO OPTION)	30
RECONSTRUCTION	31
RETRO RECON	31
RECON MANAGEMENT	32
CT PERFUSION2 ON OC – PURCHASED OPTION	32
SMARTSCORE PRO – PURCHASED OPTION	32
CARDIQ SNAPSHOT – PURCHASED OPTION	33
AUTO TRANSFER	33
DISPLAY	33
EXAM RX DISPLAY	34
IMAGE WORKS DISPLAY	35
EDIT PATIENT DATA	35
REFORMAT	36

FILMING	36
ARCHIVE	38
NETWORK	38
IMAGE MANAGEMENT	40

FEATURES FOR PC AND XTREAM BASED OPERATOR CONSOLE SYSTEMS

SOFTWARE VERSION

LightSpeed¹⁶ 405L.5_H4.2M4 version

LightSpeed QX/i, Plus, Ultra 308L.5_H3.3M4 Release MDAS 4/8

PC BASED COMPUTER HARDWARE

The operator console now uses a PC based computer system running a Linux based operating system. The system provides a gigabyte network port.

GLOBAL RECON ENGINE HARDWARE

The reconstruction hardware has been updated to provide faster reconstruction times. Recon times of 6 images/second can be realized. Time to first image of 2- 3seconds as well as faster time to first image for SmartPrep and SmartStep scans.

LINUX OPERATING SYSTEM

The system now uses the Linux operating system.

MENU DRIVEN REFORMAT

The system now provides a common user interface for reformat with the Advantage Windows in a menu driven format.

ADDITIONAL ADVANCED APPLICATIONS ON THE CONSOLE


The operator console now has the capability to have additional Advance Applications packages such as Volume Viewer, CT Colon, Advanced Vessel Analysis and CardIQ2 on the operator console.

HIPPA

The system provides the option to require users to log in and enter a password to use the system. This capability has been added to enable your institution to comply with HIPAA (Health Insurance Portability and Accountability Act). Users may be assigned to groups of users and permissions may be set for each user. Permissions may also be set to restrict access to the Protocol Management feature. Your field engineer configures log in capability. Login is selected from the shut down button.

AUTO MA

Auto mA is valid with this release. Changes have been made to the user interface to simplify the selections available.

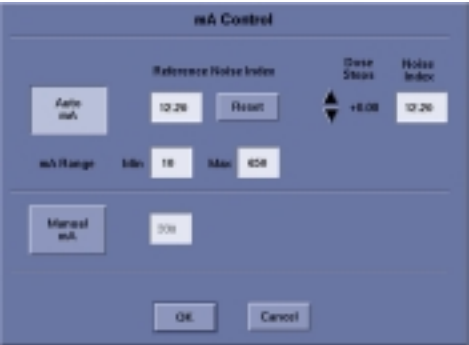

- Reference Noise Index

Default or baseline Noise Index for the given protocol. Any changes to Dose Steps, Slice Thickness or Noise index are referenced to this value. This value can only be prescribed while in protocol management
- Noise Index

The noise level required for the study. As the Noise index increases the required mA decreases and image noise increases.
- Dose Steps

Adjusts Noise Index by steps of 5%. Dose steps can be increased or decreased + values decrease image noise thus increasing required mA. Minus values increase Noise index, thus decreasing required mA. A Dose step value of 0 indicates that the prescribed Noise index is equal to the Reference Noise index for the protocol.
- Reset

Resets the Reference Noise Index to the GE Target Noise Index Default for the anatomical area and slice thickness chosen in the protocol

SMARTPREP

With faster image-to-image times the minimum Monitor ISD has been decreased to 1 sec. This provides faster monitoring of contrast enhancement. The number of Monitor scans has been increased to 40.

REPEAT SERIES

Additional functionality to Repeat Series has been added for this release. Repeat Series now allows you to choose any series that has been scanned. When more than 1 series has been scanned a list of all scanned series will be displayed. Click on the series that you wish to repeat. If only one series has been scanned, Repeat Series will not display the Repeat Series menu.



LOW SIGNAL CORRECTION

Advanced Artifact reduction reconstruction correction has been updated for this release. Reduction in streak artifacts through shoulders and hips should be seen.

AUTO FILM COMPOSER DEPOSIT TIME

The time to deposit an image on the Auto film composer has been reduced to 350ms. This will allow Auto film to take advantage of faster reconstruction times.

AUTO TRANSFER

Auto transfer by iamge has been updated to transfer in larger groups of images. This provides more efficient use of system resources while Auto Transferring by image. Auto transfer by image will transfer the first 50 images in 2 groups of 25, after that images will be transferred in groups of 50.

ANONYMOUS SCAN DATA SAVE

The system now provides the ability to save scan data with patient identifying information removed. This has been added to address HIPAA concerns. Raw data saved anonymously and then restored will reconstruct with patient identifying information removed. The Patient Name and ID will be anonymized.

Select Recon Management

Select Save Scan Data a new choice for Save Selected Annon Data is available.



CHANGES TO SHUTDOWN

When shutdown is selected, you will be presented with 2 choices Restart or Power down. Restart shuts down then automatically restarts the system. Power down brings the system down to the power off prompt. When shutdown is selected you must cycle power to the operator console to reboot the system.

If the HIPAA login feature is enabled you will be presented with 3 choices Logout, Restart or Power down



IMAGE ANNOTATION

Accession Number- Image annotation field Req. No.: has been replaced with annotation that more appropriately identifies it as the field for the accession number entered on the New Patient Screen. The annotation on the image is Acc No.:

CUSTOM ANNOTATION

Custom Annotation-has added an additional group for Accession Number. Selecting group 17 will allow the user to enable or disable display of the Accession Number field on the screen or on film.



This page left intentionally blank

NEW PRECAUTIONS 405L.5_H4.2M4/308L.5_H3.3M4

SYSTEM

- The system may not exit completely out of a pink warning dialog. In most cases a system restart will be needed.
- The system may not show typed information on the New Patient or Viewedit screen. The system will update after a short time
- The system may be slow to respond to keyboard entry and mouse clicks. If the system fails to respond stop and let the events catch up.
- The dyna plan screen may fail to update if Priority Recon is selected during scanning
- Pressing the Space Bar after selecting all fields in New Patient, locks the patient information fields and all the patient information fields become insensitive. Only the delete and backspace key will be active. Press the delete key to recover from this situation.
- Entering a \ and pressing the Enter key in the New Patient can cause the fields to become insensitive.
- Under heavy system operation, the message "Unable to install image in the database" may be seen. Recon for the series will take longer due to unsuccessful install of images to the database.

HIPAA LOG IN

- To move between the user name and password field press the tab key twice.

SCAN

- Show localizer does not show the Scan Field of View when prescribing scans. When scanning head studies, verify that you have your patient centered at ISO center to assure that the entire head is included in the SFOV.
- Show Localizer may fail to display. If toggling the Show Localizer button does not display the scout, then display the scout in a free viewport and use Report Cursor to find your scan locations and A-P and R-L centers, manually enter these on the Viewedit screen.
- The system may not allow changing of the landmark even though no scans have been taken in the series. A landmark that is set at the edge of the scannable range most often causes this. To reset the landmark, choose Select New Protocol.
- The Start End and gantry tilt fields may turn red if Add group is selected too quickly
- A scan abort may occur, resume to continue. These can be caused by the following
 - Taxi link violation due to forward error correction
 - DIP waiting to receive buffer of views
- Always verify the mA table prior to scanning when using Auto mA.
- Auto mA may set the min and the max value to 10 when selecting a protocol or adding a group. Always verify the mA tables prior to confirming the scan to verify the mA values in the table are reasonable for the patient being scanned. If the values do not look reasonable select the mA button and verify the Auto mA parameters.

Scan cont.

- Auto mA may show the max mA from a previous group instead of the max mA prescribed. Always verify that the max mA parameters are correct before confirming a scan.
- Auto mA may set the Max mA to 50. Always verify the mA table prior to scanning.
- The system does not verify the Pediatric protocol number typed in the Protocol number field matches the Patient weight entered on New Patient. When typing in the protocol number always verify that you are entering the correct protocol for the weight category desired.
- If Direct3D or VariViewer are enabled in DirectVIS under the Recon tab, Add Group will display some fields as insensitive as it will be combined with the current Direct3D or VariViewer session. Turn Direct3D or VariViewer off for the added group if you no longer want it to be included as part of the Direct3D or VariViewer session. This will allow changes to any of the acquisition parameters.
- Auto mA should not be used with Gating and Cine acquisitions even though it can be selected.
- The gating button may turn red when the patient experiences a big jump in heart rate such as in a PVC. The system usually will recover and read the signal. Sometimes you may have to toggle the gating button Off/On to get the heart rate signal synched again. Care should be taken in starting the scan if the patient continues to have PVC's

PATIENT SCHEDULE

- The Patient Schedule button may not display the Work List from the HIS/RIS server if the network is slow. Try again.

PERFORMED PROCEDURE STEP (PART OF CONNECT PRO OPTION)

- Complete PPS status for series in the order the series were created. PPS update will fail if done in a different order
- The PPS server may stop and fail to send the request. You may have to select Complete multiple times to get the series to update to the complete state.
- Add Sub does not update images for PPS correctly
- Perfusion2 will not launch if images contain PPS information.

PROTOCOL MANAGEMENT

- The Dose information in protocols used from Most Recent does not reflect the dose actually used for the protocol. If the protocol contains manual mA, retype the mA value to update the dose display. If Auto mA is used, the dose will not be reflected in Protocol Management, but will be updated at scan time for the patient being scanned based off a valid scout image.
- Protocols, which contained a SmartStep series, cannot be selected or copied from the Most Recent selector.
- Protocols can be restored from previous LightSpeed Ultra, LightSpeed Plus or LightSpeed QX/i to LightSpeed¹⁶ systems however any 4-slice protocols will be converted to 16 slice modes. The following conversion will be used:
 - Thin Twin Helical 16 row 0.5625:1 pitch, 5.625 table speed, 0.625 thickness Full mode.

- 75:1 HQ 8 row 0.625:1 pitch, 6.25 table speed, for 4x1.25 and 4x2.5 detector configuration Full mode
 - 75:1 HQ 8 row 1.35:1 pitch, 13.5 table speed for 4x3.75 and 4x5 detector configuration Full mode
 - 1.5:1 HS 8 row 1.35:1 pitch, 1.35 table speed 4x1.25 and 4x2.5 detector configuration Full mode
 - 8 row 1.35:1 pitch, 27 table speed for 4x3.75 and 4x5 detector configuration Full mode Protocol Management cont.
- There is no default protocol for Pediatric areas Neck, Upper Extremity, Chest, Abdomen, Spine, Pelvis, and Lower Extremity.
 - If the weight of a child is at the cross over point of a weight category, due to rounding errors the correct weight category might not be selected. Please check the weight based category selected against the label and the patient's weight.

SMARTPREP (PURCHASED OPTION)

- SmartPrep images may be corrupt when pulled back from some PACS systems.
- The Monitor phase image and graph information will not update if the table height has changed from the Baseline to Monitor phase. Do not change the table height after the baseline scan has been taken to avoid this.
- When transitioning to the Scan Phase from Monitor phase if the XR Auto View layout is selected the upper left viewport will be black. Move your mouse cursor over the viewport to redisplay the image.

SMARTSTEP (PURCHASED OPTION)

- Images may be skipped and get out of sequence if display operations such as WW and WL are in progress as the in room operator steps on the foot pedal. This may cause confusion on the part of the Health Care Professional that is assessing the images. Review the images to be sure about the direction to continue. To avoid this problem Display should be inactive while the in room operator is acquiring images.
- Move to scan from the Hand Held controller will not move to the last scanned location if SmartStep timed out and prep was required again. Always verify that table is positioned at the desired location for the SmartStep scan
- The SmartStep display is not cleared if you return to viewedit and confirm more SmartStep scans. Always be aware of the last image number sequence when reviewing images.
- Measurements will be maintained on images already scanned even after maintain is turned off. Use display normal to remove the measurements.
- The display process may crash if SmartStep is confirmed from a desktop other than the ExamRX desktop. To avoid this always confirm SmartStep from the ExamRx desktop
- The image display during SmartStep may get out of synch and only display a single image.
- SmartStep screen saves may fail to display in the List Select browser while in SmartStep is active. Once you exit SmartStep the screen saves will be shown in the browser.
- Screen Saved images created during a SmartStep session may fail to show up initially in the List Select Browser. The images will appear in the Browser after exiting SmartStep.

RECONSTRUCTION

- Image recon may fail and then shutdown. Select Recon Management, select Pause queue, Restart queue, if this does not restart recon then a Restart of the system will be needed.
- Images may fail to recon. This will be caused by an inadvertent carriage return in the Exam Description field. Avoid carriage returns in the middle of the Exam Description on the New Patient screen.
- Cardiac recon modes of Burst 2 or Burst 4 cannot be selected via column edit. Please select the individual row to edit recon mode selection.
- The dynaplan screen may fail to update if Priority Recon is selected during scanning
- Retro recon may not be able to get the same image locations as prospective recon. This is due to rounding in the start and end location. To avoid this mismatch prescribe start and end locations that are even numbers.
- Retro recon list service exams from Fast Cal. Do not attempt to recon this data, the SRU will shut down. These exams are listed with exams numbers that begin with 50000.
- SmartStep series are listed in Retro Recon but cannot be selected.
- Axial or Helical series will not be listed in retro recon if a scout series is confirmed but not scanned. A reboot will be required to display the series on the Retro Recon List Select screen.
- Anatomy scanned off center from ISO center such as extremities, may have loss of resolution when data is acquired helically. Always make sure to center to anatomy of interest as close to ISO center as possible.
- Cine acquisitions may have retries or image suspension. Un suspend images in recon management.

3000 IMAGE SERIES

Display

- Paging and image review with next prior may slow when reviewing large series.

Archive

- An image series of 3000 images can only fit on one side of a 2.3 gb MOD.
- Auto Store will not save the exam if the media size attached is 1.2 gb.
- If a 1.2 gb media is used for image archive and the image series is greater than 1500 images archive will need to be queued by image. Select a range of images 1500 or less when archiving to 1.2 gb media.
- If greater than 2000 images are queued to save by image you may see the browser disappear and reappear. While this is occurring it will be impossible to access the browser. To avoid this queue less images at a time when saving by image.
- Images may fail to save if saving large groups of images. Verify that all desired images are saved before deleting them from the system disk.

Network

- When queuing a large number of entries are queued for send or receive. Typically this will be seen when 200 or more entries exist. There may be delays seen when accessing the network queue.

DentaScan/Add/Subtract

- These applications can only load 1000 images. Hi-light the desired image range of 1000 images by selecting the first image desired, hold the shift key down and hi-light the last image desired then select the desired range.

RECON MANAGEMENT

- Scan File save is not complete even though the Saved File message has been posted. The problem is due to the time it is taking to unmount the DVD. You may have to wait 5-7 minutes for the DVD to unmount. The write light on the DVD will be green when the DVD is unmounted
- Scan Files restored from a different system will be reconstructed using the product name of the system it is restored on. For example, restore scan files from a H1 SDAS QX/i or a H2 SDAS Plus to a LightSpeed¹⁶ and the product name on the images will be indicated as LightSpeed¹⁶ instead of LightSpeed QX/I or LightSpeed Plus. All other patient and parameter information is correct.

DISPLAY (APPLIES TO IMAGE WORKS AND EXAMRX DISPLAY)

- Plus recon mode is not annotated on the Series Text Page. Refer to the image annotation for the Plus recon mode annotation.
- An active user annotation graphic will not film the box or arrow that is displayed on the screen.

IMAGE WORKS DISPLAY

- The primary focus may change if the space bar is selected multiple times when entering accelerator line commands. Verify that primary focus is on the image desired.

EXAM RX DISPLAY

- The Trackball may fail to initialize properly at system reboot. Try rebooting the system again to recover
- Images reconned with Priority recon are not available in the Auto Link viewport. Redisplay the series to access these images.
- MIROI may fail to produce a graph if next prior is selected while doing MIROI. Redisplay the series and begin again

VARIVIEWER

- Batch film may fail after a system reboot if the format selected is different than the default film format on reboot. An error dialog will be posted informing you of the error. You may have to select filming multiple times to successfully send the request.
- If the scout is taken after the series used for VariViewer operation, the system may be unable to find the scout for graphic batch prescription. Manually enter the range for the batch prescription.
- Any zoom applied to a Variviewer image is not maintained as you page through the images.

VariViewer cont.

- VariViewer session may not be able to be started if there multiple Pause scans during the acquisition of data.
- VariViewer is not compatible with a gantry tilt.
- Switching back from a 768 viewport is VariViewer causes the VariViewer viewport to be forward instead of the Auto View viewport. Use the page turner to toggle back to the auto view Viewport.

DIRECT3D (OPTION)

- The Save State, which allows the user to rebuild the Direct3D model on the AW using the VR algorithm from D3D, does not work on the OC even if Volume Viewer is installed. The user will get an error message informing that the images are missing
- Batch film may fail after a system reboot if the format selected is different than the default film format on reboot. An error dialog will be posted informing you of the error. You may have to select filming multiple times to successfully send the request.
- 768 image size may display split in 2 if resize is selected with the Auto View viewport forward. Always have the D3D viewport forward when selecting resize. To recover from this problem select resize twice.
- If you resize the viewport in Direct3D, the image may not initially be displayed. User the Page Turner in the lower left corner of the viewport to toggle to the time.
- The Direct3D model may not initially build properly. Enter Interactive Review and re-render the model and then the model will build correctly.

VOLUME VIEWER (OPTION)

- Volume Viewer may display on the ExamRx desktop . This will occur if you switch back to the ExamRx desktop quickly after launching Volume Viewer
- Volume Viewer may hang. This occurs due to a error dialog that is hidden. To avoid this don't switch desktops until you start to see the model build in Volume Viewer.
- A 3D model may be missing data when it is initially displayed. Slightly rotate the model to redisplay all of the 3 D data.
- The system may get extremely slow when saving a 3D or VR model. Please be patient for the system to complete saving the model.

CTCOLON (OPTION)

- Rotate and translate is missing in the CTC and Virtual Dissection protocols
- The system may hang and display 3 film composers with no borders, the composers cannot be moved and not selections can be made except for desktop switching. A system reboot will be needed to recover.

CARDIQ (OPTION)

- Multiphase protocols of Vessel Analysis and Heart MP do not load the images correctly. Load the images first using the Tree MP protocol and then select new protocol and change to the desired protocol.
- The Lumen view may display 'Hit space bar to display high resolution view" This will be needed with views 15mm or less.
- WW and WL of screen saved MIP views may not be correct contrast. Adjust the WW and WL to improve the image.
- Batch film will not film images in the Cardiac Short Axis protocol. The images will need to be manually filmed.
- Layout protocols must be created with single phase cardiac data sets. Once saved they can be used with multiphase cardiac data sets.

ADVANCED VESSELL ANALYSIS (OPTION)

- AVA defaults to inferior view instead of Anterior after processing AVA . Use the anatomical buttons to change the view to Anterior
- AVA lumen view may show wavy lines while rotating. When the rotation is stopped the display will update.
- The system may hang and display 3 film composers with no borders, the composers cannot be moved and not selections can be made except for desktop switching. A system reboot will be needed to recover.

REFORMAT

- Sagittal images created from prone direct coronal position are distorted
- Reformat will only allow filming in Batch to the first 30 cameras in the list. If another camera is desired save the batch images to disk and use Print Series to film the images.Reformat cont.
- Images saved from batch mode may appear to have jagged edges or not have optimal Image Quality. Manually save the images to improve image quality.
- Large image series may fail to load when using Reformat detail. This can be caused by small spacing interval between images or image sets greater than 1000 images. Select a sub set of images if this occurs or use Reformat Standard to build the model.
- A series that has more than 1 group with 0.625mm slice thickness will fail to load for reformat or will fail in Volume rendering on the AW. This is due to a mismatch in the spacing between the groups. To avoid this have only one scan group if possible, otherwise selectively highlight the images from the first group for Volume Analysis.

CT PERFUSION 2 ON OC – PURCHASED OPTION

- Computation of perfusion maps and automatic detection of the artery or vein may not function when the data is displayed in Perfusion is initially black and the WW and WL values need to be set to large negative values (WW 40, WL -1020) to make the images viewable. The threshold should be set to the maximum negative value for air to assure that automatic detection of the artery and vein and that Perfusion maps are displayed correctly.
- Perfusion will not launch if the images contain PPS information

- Saving TIFF files of the graph and images is not supported because there is no floppy drive hardware available on the OC.
- Set the color ramp to gray scale for screen saves images if you are going to network the images to another station such as PACS to improve quality of the screen save.
- Initially as CT Perfusio2 is loading, you may see garbage flash along the left side of the screen.
- Processed data does not display if New Protocol is selected within Perfusion2. To avoid this always close Perfusion2 before selecting a new protocol.

ADD SUBTRACT

- Comb images will not contain the e/s/i used for the added image.

ARCHIVE

- Images archived on a Advantage Windows 4.0 or 4.1 system may fail to restore on the LightSpeed system. Use Network to transfer images from the Advantage Windows to the scanner.
- Even though the Sony MOD drive states that it is a 5.3 gb drive. The archive software only supports a maximum size of 2.3 gb. 2.3 gb 512 bytes per sector is the preferred archive media size to utilize on the system.
- Archive may fail and slow the system when more than 200 images are queued by image. Try to archive by series if possible to avoid this.
- The system may report that the media is full even though the media has just been labeled when Save by image is selected. Try selecting a smaller range of images to avoid this.

FILMING

- Image setting such as WW WL and flip rotate, zoom, roam are not maintained across all images when imitating F4 print series from a MID Viewport format. Use a 512 size viewport to initiate F4 Print Series.Filming cont.
- Auto Film may stop and the Continue Same Sheet button will be displayed. The Continue Same Sheet button will be active, but when selected will not restart filming. Use Manual Film to complete filming the exam and reboot the system before starting the next exam
- If the F1 key is used to film the Text Page ROI, Exam Text Page and Series Text Page, the text pages will be filmed to the film composer last selected in the pop-up for text page. Use the filming selections in the text page screens to film the information displayed.
- The message "Film formatting in progress. Please retry." May be seen when filming to the Manual Film composer when the system is busy with other simultaneous operations such as recon, network, auto film and scanning. Retry manual filming when the system is less busy. A system reboot may be required to recover.
- Image annotation may be small or blurry on filmed images when the first image is a scout, which is over 600mm. Place this image on the last space of a film to avoid this.

NETWORK

- The system may create core files that may fill up disk space on the system. Networking color save images from Volume Viewer or CardiacIQ causes these core files. To avoid this save the color images to MOD, remove the color images from the system then restore the color images and then network the images.
- Color Saved images from Volume Viewer or CardiacIQ may fail to transfer. To avoid this save the color images to MOD, remove the color images from the system then restore the color images and then network the images.
- Images that have been edited using Edit Patient networked to a RadStore system will fail to archive to the RadStore DVD. The images must be archived on the CT system MOD.
- The system no longer supports Advantage Net protocol. When sending images DICOM send should be utilized.

IMAGE MANAGEMENT

- Removal of images should be done with the system in an idle state. Failing to remove images at idle times can cause image install timeouts that can then cause recon to shutdown and can cause the browser to fail to respond. The user may also see a blank list in the browser. The system should not be shutdown until the image space has been updated fully from the remove. The length of time to synchronize the database is proportional to the number of images being removed. This will assure that all images are reconstructed, displayed and installed into the database without error and that image space is update correctly.
- Exams that contain SmartStep may fail to remove. Reboot the system to remove the lock on the SmartStep series.

LEARNING AND REFERENCE GUIDE

- After a desktop switch back to Learning Solutions desktop the guide returns to the home page instead of returning to the page they were on when the switch occurred. The document is slightly behind the home page. Left click and drag on the home page border to move the home page so you may access the Learning and Reference Guide pdf file.

Page Left Intentionally Blank

LEGACY PRECAUTIONS

SYSTEM

- Run Shutdown and Restart daily.
- The system may fail to start if system disk space needs to be recovered from unused system files. The following message will be posted in the Disk Management shell window:

```
"The purpose of storelog is to recover system disk space by archiving and then removing core, log, and data files that have been saved for their system troubleshooting diagnostic value. Now they may be taking up too much space for the system to run properly. Removing these "system log" files does not add image space, but should allow the application to start."
```
- You are then directed to answer the following questions (be patient for the messages to display):

Place the mouse cursor inside the black Disk Management window

Q: Do you want to save system log files to removable media?

Type n and hit the enter key

Q: Do you want to remove the system log files?

Type Y and hit the enter key.

You will then see a message "Please be patient, the system is now removing unwanted files." The system will then start normally.

- If the system fails to startup completely, select [Unix Shell] from the tool chest menu in the upper right of the Scan Monitor place your cursor in the blue shell and type st.
- If mouse selections fail, select the [Escape] key to clear backlogged requests.
- If you can no longer type in a field, move the cursor to the field and try clicking the middle mouse to restore functionality. If this does not work, then a system shutdown will be required.
- The cursor may not move between the left and right screen. Wait a few seconds without moving the cursor and try again.
- To install a SMPTE pattern, BRH or Quality assurance images for viewing, select the following. Once installed the images will be available for viewing from the Image Works browser or List Select in Exam RX. Both will be listed as Exam 1000, the patient name will reflect if it is a QA image or a SMPTE pattern.
 - Select Service Desktop
 - Select [Diagnostics]
 - Select [Display Processing]
 - Select [Install SMPTE Image]
- In general, wait for a screen transition to take place before making another selection.
- If the console becomes unresponsive for 2 minutes or more, shutdown the system using the pink shutdown button and restart the system. If you cannot select the pink shutdown button, turn off the console power switch, wait 10 seconds, then turn the console power switch back on. The system should come up normally.
- The system will lock up if the mouse becomes hung on the left monitor. The only known recovery is to cycle power to the console.

System cont.

- You may see a pink warning dialog posted indicating the system has low disk space. This is due to a partition on the system disk getting too full. This can be caused by archive, network or film queues containing too many entries. Make sure that the entries are processed. If the queue is paused, resume it or delete entries as needed.
- Protocol Management may not be selectable. Check that retro recon is selectable. If it is not then the system will need to be rebooted.
- Pop-up screens and menus may appear on the wrong monitor or may be displayed split between the two monitors.
- Windows such as the Film Composer that normally are restrained to the right or left monitor can be dragged to the other monitor. Be careful not to get a Film Composer hidden behind some screen if you move it to the other monitor.
- If a blank viewport is seen where image annotation is displayed and W/L is interactive but no image is seen, shutdown the system, recycle power and reboot the system to clear this display issue.
- If corrupted images are seen after applying an image filter such as enhance, smooth, lung or gray scale, try rebooting the system and see if the image can be displayed correctly. If not contact your GE service representative.

TUBE WARM UP/FAST CAL

- Run Tube Warm up after 2 hours of non-use. It is best to warm the tube as close as possible to the time the next patient will be scanned. Don't warm the x-ray tube and then wait 30 minutes without scanning.
- Always check that the beam is clear when doing Fast Cal. In Fast Cal, the system checks cleanliness of the Mylar Window. If the system suspects the Mylar Window may be dirty to the point that it may cause a beam obstruction, a pop-up message will be displayed. The operator will be instructed to clean the Mylar Window and select [Retry].
- Fast Cal must be run once every 24 hours.
- Complete all portions of Fast Cal, Warm Up 1, Warm Up 2, Gen Cal, Clever Gain and Fast Cal. This assures that the Air calibration and generator calibrations are up to date on the system. Scan aborts may occur during Axial or Helical scanning. Always be aware of the scan progress during an Exam and select Resume as soon as it is posted to continue.

SCAN

- Scan aborts may occur during Axial or Helical scanning. Always be aware of the scan progress during an Exam and select Resume as soon as it is posted to continue.
- Scan may fail to confirm posting a message that not enough image space exists, even though the image space shown in the Feature Status Area indicates there is enough space. This is due to the fact that images are stored on the system disk in more than one partition. Remove consecutive exams to free up image space for confirm to proceed.

Scan cont.

- To terminate an Insite connection on your system. Select [New Patient] a message will be posted informing you that the scan hardware resource is not available. Wait 3 minutes and select [New Patient] again to begin scanning.
- In general, if a scan fails and a [Resume] is posted, press [Resume] to continue. Try [Resume] again if the first [Resume] fails. If a failure still occurs, reset the scanning hardware through System Resets in the Service desktop. If scan still fails to restart, shutdown and Restart the system.
- Auto Voice may fail to function, especially during system simultaneity. Make sure that you can hear the Auto Voice to recognize if Auto Voice has quit, manually breathe the patient when this occurs.
- The Show Localizer scout image may fail to display or images may fail to recon and may become suspended if scanning is started while remove images is in progress. To avoid this **don't** remove images while an exam is in progress or scanning is active. Remove images when the system is idle.
- The Dynaplan screen may report incorrect status (i.e. a scan is removed before it is actually scanned) when stop scan is selected. The screen will reset correctly after Resume or back to view edit is selected.
- Scan groups will not be contiguous if you switch from 2 or more Helical scan groups column or row edit and the scan type is changed to Axial. If this change is made, then verify the Start and End locations of each of your scan groups and adjust if needed.
- The Cine time between images may change when other parameters are modified within a protocol. Check the Cine time between images prior to confirming the scan to verify it is the value you wish.
- Tilt handles will not be visible on the screen if the DFOV is larger than 48. Use a DFOV smaller than 48 to assure that the tilt handles are visible.
- Show Localizer may fail to display the scout image if the Next Series is selected before the scout images are reconstructed. Wait until the scout images are reconstructed before selecting Next Series. If Next Series has already been selected, toggle Show Localizer off and then on again.
- Quickly changing desktops when Show Localizer has been selected for the next series can cause a partial display of the scout in the Graphic Rx window to occur.
- If Page Up or Page Down fails to change the displayed Show Localizer.
Try the following in order:
 1. Turn Show Localizer button off then on.
 2. Move the cursor off the image window and back on to the image to refresh the screen if both of these fail then verify that you have a valid scout for Show Localizer.
- If an R, L or A, P value is more than half of the Display Field of View in mm. The image annotation will not annotate R and L or A and P on the images. For example if the DFOV is 10cm and the R value is 56mm then the image annotation will show R R. Use a R-L or A-P value which is less than half of the DFOV in mm to avoid this.
- A protocol may fail to display. The following message will be posted to the message line on the lower center of the scan monitor "Can't read selected protocol, please choose another protocol". If this occurs the protocol is corrupt and will need to be rebuilt. Delete the protocol and rebuild it.
- The patient history field may be missing the last 9 characters when all 60 characters have been entered and the patient record is either selected as a completed exam or the Patient ID is entered and the system matches a completed exam.

Scan cont.

- Even weights entered in Patient Schedule may be rounded up to the next odd pound. This occurs because weights are stored as kilogram units then converted back to pounds.
- During the acquisition of large data sets (1000-1500), there may be Auto film and reconstruction performance issues. If either stops, check the queues and restart to continue.
- When selecting the Auto Voice field, the selected Auto Voice will be deselected. You must reselect the desired Auto Voice message before exiting the Auto Voice screen.
- When entering birth dates on the New Patient or Schedule Patient screens the following rules apply:
 - 2 digit years can only be entered if the birth year is in the current century for the 21st century - for the year 2000 forward.
 - Birth dates from any other century must be entered as 4 digits for example for the year 1899 –1999 all four digits must be entered.
 - Birth dates can only be entered for 150 years (Current year minus 150 years).
- If InSite is running the “Remote Safety” test, New Patient will not open. New Patient can be made available by either:
 1. Calling InSite and request they abort the test.
 2. Going to the Service Desktop and selecting [CleanUp] option to cancel the test in progress.
- PMR images may fail to recon if disk space is low. To recon the images, remove images and restart the recon queue in Recon Management.
- You may get the message “Duplicate Scan Key”, if a Scout Scan is aborted within the first 20 to 75 mm of table travel or if a the prescribed length of the Scout is less than 75mm. In order to proceed, an End Exam must be done and new exam started.
- It may be possible to prescribe a recon range that is outside the recon 1 boundary. This may occur is the start location is dragged below the recon end location in recon 2 or 3.
- If a large number of scan files are reserved and there is a large recon queue, you may see the message: “Duplicate Scan Key – unable to allocate scan file.” There will be a resume at Start Scan. Either wait a few minutes for the recon queue to decrease or release some of the reserved scan files.
- Bands and lines may be seen in scout images if there is a tube spit or the reference channel is blocked during the acquisition of a scout scan.
- A zero interval axial series, if paused, will add another group equal to the remaining number of images. Make sure to return to the View/Edit screen to delete this group to avoid acquiring additional images.
- Biopsy is not valid for a Thin Twin helical acquisition mode. If Biopsy is selected, the Biopsy window does not open; however a group is added to the series at an inadvertent location. Do not select Biopsy mode with Thin Twin helical scan mode.
- If the message “Can not read Cal Database”, select [End Exam] and re-enter patient information.

SMARTPREP (PURCHASED OPTION)

- Monitor phase scanning will abort if the Monitor ISD is set to less than 3 seconds when the rotation time used is 0.8 sec. Set the Monitor ISD to 3 seconds or greater to avoid this problem.
If this has occurred, do one of the following:
 - Press Monitor Phase to continue monitor scans.
 - Use the graphed data and the clock countdown on the SmartPrep display to determine when to select Scan Phase.
- The film composers will flash and cannot be hidden on the SmartPrep display. This will occur if the Auto Film or Manual Film composer buttons are selected after confirm has been selected for SmartPrep. Don't select the film composer buttons while the SmartPrep display is first coming up or is visible to avoid this.
- If reconstruction fails during SmartPrep, scanning will pause and post a message. Press [Monitor Phase] to resume scanning for the monitor phase.
- SmartPrep may fail to confirm for the Baseline scan. Re –confirm to continue.

PATIENT SCHEDULE

- Close the preferences screen before switching between Patient Schedule and New Patient.
- The Patient Name, Patient ID, Accession Number and Requested Procedure ID can only be edited if “Allow to Edit MWL” is set to yes in the Preference window.

CONNECTPRO (PURCHASED OPTION)

- Bar Codes will fail to be read by the Bar Code reader if the HIS/RIS system the bar code was created on has a different language keyboard than the CT system. For example, if your CT system has a French language keyboard then your HIS/RIS must have a French language keyboard. If it is not possible to have the same language keyboard on each system, then manually enter the Accession or Patient ID number or select the desired patient from the Patient Schedule list to display the patient information on the New Patient screen.
- Patients selected from Modality Work List will be displayed with ^ (carets) to define different DICOM fields. The carets are not displayed on the images.

PERFORMED PROCEDURE STEP (PART OF CONNECT PRO OPTION)

- PPS will post the message “Failed to Start” if the remote server is down.
- Screen Save images created in ExamRx or in the Viewer on the Image Works desktop are not PPS aware in this release of software. Also, images created in Reformat, 3D, and Navigator are not PPS aware. For these image types, “INPR” will be posted in the PPS column in the Browser even though PPS is not enabled.

RECONSTRUCTION

- If images fail to recon the following should be used in order:
 - Select [Recon Management], [Unsuspend Queue]
- If the image still fails to recon
 - Select [Recon Management], [Restart Queue]
- If this still fails Shutdown and reboot the system.
- Lung Algorithm
 - Provides edge enhancement between structures with large density differences, such as calcium and air.
 - Enhances the contrast of small objects. For best viewing and film quality, select a window width of 1000 to 1500 and a window level of -500 to -600.
 - Increases CT number values at the edge of high contrast objects. When planning to take CT number measurements of vessels or nodules in the lung, please check and compare your results with Standard algorithm images. (ROI and Histogram functions use CT numbers.)
 - The edge enhancement provided by Lung Algorithm may not be appropriate in some clinical cases. Please take individual viewing preferences into account when you choose Lung algorithm.

RETRO RECON

- Two decimal points cannot be entered, i.e. 3.75 for image interval if column edit is used. Edit each scan group (row) if an interval with 2 decimals is required.
- If a 1 rotation 4i or 2i axial scan is prescribed using add group in ViewEdit with a Superior to Inferior scan direction is retro reconned, the resulting images will be reconned Inferior to Superior. The image locations are correct, but the image numbers will not match the prospective images.
- If you delete queued Retro images the image space reserved for those retro recons is not given back. You will not get the space back until you reboot the system.
- Only start Retro Recon when scanning is complete. Do not delete queued retros while scanning is active, scanning could stop.
- If maximum A-P or R-L offset is selected in Retro Recon, one image may fail to reconstruct. Select an offset that is 0.5mm less than the maximum value allowed.
- The start/end locations of a retro reconstruction may be different from Recon 1 and 2 and 3 when a PMR with a thicker slice than Recon 1 is prescribed for the series.
- Retro Recon may hang and core. If the Retro recon screen fails to display or queue retrospective images, retro recon has cored. Reboot the system to recover.
- If an R, L or A, P value is more than half of the Display Field of View in mm. The image annotation will not annotate R and L or A and P on the images. For example if the DFOV is 10cm and the R value is 56mm then the image annotation will show R R. Use a R-L or A-P value which is less than half of the DFOV in mm to avoid this.
- It may be possible to confirm a retro recon prescription with an invalid recon start and end location that results in a recon suspend. To avoid this change image thickness before changing image locations.

RECON MANAGEMENT

- Scout queue entries can be selected in Delete Retro queue entries. Only select Scout queue entries to delete if you are sure you do not need the scout image reconstructed.
- Before saving or restoring scan data make sure the system is idle and no Archive, Network or Filming is active. No other features should be accessed until the save or restore is complete.
- Recon Management may hang while trying to display the menu. Finish the current exam if scanning and shutdown and restart the system to correct the problem.
- If you wish to cancel a Save or Restore scan data, the cancel button will cancel only after the current scan file is saved or restored. A helical scan file contains a large amount of data even though it is one scan file, that file can take up to 30 minutes or more to save. You are unable to scan patients while saving or restoring Scan Data.
Make sure that you have ample time to complete the save or restore before beginning.
- Scan data save or restore is active when the dialog message indicating saving or restoring scan file is displayed.
- If saving scan data, after the save is complete select Restore Scan Files to verify the data is stored.

CT PERFUSION2 ON OC – PURCHASED OPTION

- Saving TIFF files of the graph and images is not supported because there is no floppy drive hardware available on the OC.
- The CT Perfusion Control Panel may be displayed on the current desktop if CT Perfusion is launched from the Browser and the desktop is changed before CT Perfusion screens are completely displayed.

SMARTSCORE PRO – PURCHASED OPTION

- Only 0.8 and 0.5 second rotation speeds are valid for Prospective Gating.
- A backslash (/) in the Patient ID for SmartScore exams will cause the patient report to fail to print or be stored to floppy.
- If the Confirm button is not available, select the Gating button and turn gating off and click on Accept. Select Gating button, again, and turn gating on and click on Accept. The Confirm button should now be available. Contact your local service representative if you experience this issue for further investigation.

CARDIQ SNAPSHOT – PURCHASED OPTION

- If a lead falls off during acquisition, the heart rate annotation will be inaccurate for the portion of the acquisition after the lead falls off. Images reconstructed for the complete acquisition using Snapshot Segment will initially display correct BPM for the period of time the leads were connected, and then ungated images will be displayed followed by images annotated with abnormally high heart rate where the leads have fallen off.
- If the Gating button is displayed in red and heart rate is seen, this is most likely due to loose connection of the cable at the connection to the EKG monitor or the scanner. Make sure you see a heart rate before you begin the scout scan.
- CardIQ Snapshot Segment annotation is not displayed on the images displayed on the Advantage Windows workstation. The average heart rate and the percent of R-R interval will not be seen. The Cardiac Helical scan type will be annotated as Axial.
- Snapshot Segment images can be networked to a PACS system, however due to an error in the DICOM header, they can be retrieved from the GE PathSpeed PACS system but the image annotation is wrong.

AUTO TRANSFER

- A series may fail to Auto Transfer if [Next Series] then [Create New Series] is selected after a scout scan is prescribed, but not scanned, i.e.; pause and return to view edit is selected.

DISPLAY

- The Exam Rx List Select and Image Works browsers may in some cases not list an exam, series or image. This may be seen after an interruption of power to the system or the database may be updating slowly. The patient does not need to be rescanned.

Verify the following:

- Type the Exam, Series, Image on the accelerator line to display the image,
- Select another exam in the browser this will cause the browser to update,
- The browser may update after a slight delay,
- Reboot the system,
- A second reboot may be needed if a power fail has occurred.
- The browser may update slowly to reflect Screen Save images created in an exam. If the Screen Save images is not listed in the browser wait for them to appear. The time to appear may be up to 15 minutes if the Automatic Database check and recovery is in progress when the Screen Save images are created.
- In general, wait for a display action to complete before entering in another command.
- With the system configured in French or German language, if a comma is entered in explicit magnify, i.e. 2,3 the comma will not be interpreted as a decimal. The magnification factor is applied without the decimal. In the example shown, 2,3 the image would only be magnified 2X not 2.3X. Always enter a period to designate a decimal and have the correct magnification applied.

Display cont.

- Cross Reference lines will post incorrectly if sort by image location is selected. Make sure that sort by number is selected before posting Cross Reference lines.
- Cross Reference lines may not post with some combinations of DFOV and RAS center. RAS centers at the edge of the DFOV and small DFOV's will exhibit the problem. Retro reconstruct the images to a larger DFOV if posting of the cutlines is desired.
- Image annotation may overlap or not be fully shown if a 32 character patient name is entered for 3D, Navigator, Reformat, MID formats, DentaScan images.
- Text and Series pages only display 24 characters for Patient Name.
- Text pages will not show foreign characters entered using the ALT GR key.
- ROI and STD deviation numbers may be reported as zero after a Zoom is applied to an image with a ROI posted. This is due to partial pixel contained in the ROI. Adjust the size of the ROI to include full pixels and recalculate the ROI.
- No text will be entered in the accelerator line if the mouse cursor is over the film composer.
- Some combinations of E/S/I will fail to display an image, if cap locks are on. To select an exam series and image from the accelerator line use the following format when cap locks is on: For example to select Exam 576 Series 2 image 3 type E576 2 3 on the accelerator line.
- Selection of an exam series or image may fail a second time after an exam series or image is displayed. If the desired exam series or image does not display then select the desired images from the browser.
- Image location seen on the scanner may differ from that seen on an AW 3.1 system for tilted images. LightSpeed reports the image location as iso-center of the image. AW 3.1 reports image location as the image center for the image. With tilted images there will be a difference in the location numbers proportional to the off center distance times the sin of the tilt angle. The image location can be reported as image center on LightSpeed by using the Report Cursor function.

EXAM RX DISPLAY

- Display may reset it's self after a software problem. You may see display stop or not accept your mouse input. Wait for a few seconds and display will automatically reset. You will have to redisplay the images you wish to work on.
- The MIROI pop up may display but will not function. This will occur if an Auto View or Cross reference viewport is in primary focus (blue border) MIROI is not valid in these viewport types. Place a Free or Auto Link viewport in primary focus and reselect the MIROI button to continue.
- Any Report Pixel or MIROI chart that is not screen saved, but is filmed will show the Exam Series and Image as 1000/1/1 on the film composer icon if E/S/I is selected. This is the exam/series/image number the system assigns to this chart display The patients exam number is listed correctly on the filmed image.
- Image selection from the accelerator line will not function if the primary viewport contains a MIROI plot or Report Pixels chart. Use List Select to display a new image.
- Any accelerator commands entered for Series Binding, Annotation levels for display or filming will be saved as defaults
- ExamRx Display may hang. In some cases switching to the Image Works desktop and back to Exam Rx display may clear the problem. If this doesn't work then perform a system shutdown and reboot the system.

ExamRX Display cont.

- With paging active (P in the lower left corner of the image) the trackball may adjust window width and window level in other viewports, verify the image has the correct window level before filming the image.
- The right mouse may fail to roam even when the state is set to roam. A system shutdown may be required to clear this problem.
- Display may crash when selecting a 3D object from the list select browser. When a 3D object is selected, 3D should be selected from the browser.
- Images may not be displayed after a switch between Auto View or Image Review layouts. This is due to a restart in the display process. Redisplay the desired images in the viewport to continue.

IMAGE WORKS DISPLAY

- WW and WL adjustments will only be maintained on individually selected images if the middle mouse button is used. If the accelerator line or Presets are used all images will update regardless of primary or secondary focus of the images.
- Any accelerator commands entered for Series Binding, Annotation levels for display or filming will be applied and not held if the viewer is closed. Use User Preferences in the viewer to save the settings as a default if desired.
- Reference Image may select the wrong scout series, i.e. not the scout series the images were prescribed from, if one or more scout series exists. If the wrong scout is selected place the Reference Image viewport in primary focus and enter the scout series number desired on the accelerator line.
- Window/Level does not display stored value set in the Viewer when +/- series is used. The W/L used is the same as the last series displayed.
- Images created in Add/Sub are displayed with value of WW 4098 and WL 1024.
- If paging is selected while the system is in Compare Mode, the upper left viewport is left blank. Return to the Browser and select the desired series for paging and restart the Viewer.
- Accelerator Command Line entries for E/S/I do not act properly. The first image in the series is always displayed instead of the requested image within the series.
- Cross Reference line numbering along the top of a sagittal scout may be listed in offset manor.
- The new features in User Preferences on the Image Works desktop are not translated.

EDIT PATIENT DATA

- The system may hang if Edit Patient is started while the following operations are in progress:
 - Network Receive
 - Prospective or Retrospective reconstruction is active
 - Archive Restore
- To avoid this, confirm Edit Patient during idle times in network receive, active recon or archive restore.

Edit Patient Data cont.

- Patient age may be seen as zero in Edit Patient Data even though a birth date is entered. Enter the birth date again and patient age will be calculated.
- If duplicate accession numbers exist, Edit Patient Data will not allow the exam to be modified.
- If there is a space at beginning or end of the hospital, Edit Patient Data will fail. Contact your field engineer to update the hospital name correctly in the system reconfiguration.

REFORMAT

- When selecting reformat wait until the % loading dialog is displayed before switching to the Exam RX desktop. This will avoid having to select Load slices to start the reformat model build when returning back to the Image Works desktop.
- The reformat location will not be annotated on images filmed when Printer is selected in Batch Mode. If it is desired to have the reformat location annotated, then use Save in Batch Mode and film the images through Print Series.
- In Batch mode, images reconstructed using "Rotation" or "Oblique" modes will start with number 2 while images created using "First View/Last View" start with 1. In Rotation and Oblique modes, a plan of the reconstructions is screen saved and becomes image 1 for the series.
- Occasionally, the color for the viewports and control panel will change because there is not enough colors available in the resource file to support reformat. To recover, quit reformat and restart the application.
- Window/Level for images are not displayed using the value stored in the image. Use the window/level function keys or selects within Reformat to reset the W/L.

FILMING

- Images or Auto Film control buttons may fail to display in the AutoFilm viewport. This may occur after a switch between desktops. To display the images change to a different AutoView layout, then switch back to your desired layout.
- Don't let the auto film viewport back up with images to be filmed. Start Auto Film as soon as possible to keep caught up on filming.
- Any of the Auto Film control buttons may be activated when the cursor is over the button and the space bar is selected. Place the cursor in the Auto Film viewport only when needed to avoid this problem.
- Auto Film may fail to film. This may occur when the Auto Film viewport selection shows active and the Auto Film status shows paused. Toggle the [Pause] button in the Auto Film viewport and select [Start New Sheet] or [Continue Same Sheet] to restart filming.
- When scanning multiple one rotation axial groups, images are filmed out of order when Auto Film is selected. Turn Auto Film off for these scan groups.
- Intermittently, Auto Film will automatically print the last page when Add Group is selected.
- Occasionally, the last image will not print. Cancel Auto Film and manually film the image to the Auto Film Composer. If scouts and reference lines were prescribed, they will need to be filmed manually.

Filming cont.

- Auto Film may fail to display images if recon is having trouble reconstructing the image or if images have failed to install in the database. This may also occur if a large exam has not reconstructed all images and scanning is started on a new exam. The following dialog will be posted if Auto Film cannot display images:
 - Exam 100
 - Series 2
 - Cannot find 10 images
 - Skip Missing images

Continue
Cancel Film Series

You are presented with 3 choices:

1. Skip Missing images will skip the images that Auto Film cannot find. For example if Auto Film had filmed images 1-10 and you then got the message that 10 images were missing and selected Skip Missing Images, Auto Film would then start filming again with image 21.
 2. Continue will look for the images again, if they are not found then the dialog will be posted again. Before selecting continue verify that recon is active, that the images have been reconstructed, the missing images are not suspended or paused in the Recon Queue and the images are able to be displayed. If the images are suspended or paused in the recon queue, then unsuspend or restart recon to reconstruct the images before selecting Continue.
 3. Cancel Film Series will cancel Auto Film for the series currently being Auto Filmed. The images will then need to be manually filmed.
- If you get this dialog because you have begun an exam while the previous exam still has images to reconstruct, then Select Continue and select Pause Auto Film, resume Auto Film when the Exam Series and Images from the previous exam have reconstructed.
 - When prescribing Mag factor for auto film, scout images if the scout is longer than 500 mm then use a magnification factor less than 1 to display the entire scout.
 - The manual film composer may display when confirm is selected for scanning if the composer had been closed by selecting iconify in the upper right corner of the composer.
 - It's best to run Print Series from only one desktop at a time.
 - It's best to resolve any paused queue entry as soon as possible.
 - Print Series may pause automatically under heavy system load.
 - If Anonymous Patient is selected for an exam where Auto Film is in progress, the system may fail to cross reference the slices on the scout. If Anonymous Patient is required for series that are still active in Auto Film, wait till Auto Film is complete for the series before proceeding with Anonymous Patient.
 - To install a SMPTE pattern select the following . Once installed the images will be available for viewing from the Image Works browser or List Select in Exam RX. And will be listed as Exam 1000. The patient Name will be listed as SMPTE.
 - Select Service Desktop
 - Select [Diagnostics]
 - Select [Display Processing]
 - Select [Install SMPTE Image]

Filming cont.

- Full Annotation instead of partial annotation will be filmed when using F3 (Film MID) in the Image Works desk top when full annotation is selected.
- The format built in a protocol may be changed when the protocol is used with a message that the format was changed due to an invalid format, even though the format is valid. Verify in Auto Film set up is the format you desire before confirming scan.
- For Multi-Image Display (MID) in AutoFilm, filters, gray scale and orientation selections are applied only to the image in the upper left viewport. If there are an odd number of images in the series, the filters, gray scale and image orientation is applied to the first group only.

ARCHIVE

- The feature status area or the browser may report an Exam has saved even though all images have not been saved to MOD. Scroll through the images in the image window. Highlight the images listed as Archive N and resave them.
- Restoring Exam, Series or images that already exist on the system disk will not post a message that the images are restored or that they already exist. If you have restored images, but get no message that they have been restored, verify that they don't already exist on the system disk.
- When the archive media gets close to being full, the system will always look to see if the exam, series or image can fit on the MOD, if it is desired to have exams sequentially on a MOD, place a new MOD in the drive when first notified the disk may be full.
- If Label is selected in Archive, finish the Label process; don't select cancel on the Label pop up. Archive will be non functional, a system reboot will be necessary to recover.
- It's best to resolve any paused queue entry as soon as possible.
- To minimize corruption of MODs, it is extremely important the MOD media be detached and removed from the MOD drive before doing a shutdown or recycling power to the system.
- When restoring from a MOD, it is recommended to write protect the media before placing it in the drive. If the system is unable to read the media, remove the write protect and see if the system is able to perform a recovery of the media to access the data.
- If the MOD can not be detached or will not eject from the drive, do a shutdown and eject the MOD once the message "Hit any key to start the system" is seen. Do not use the screw to eject the disk.
- If you get a timeout message when trying to access the MOD, the MOD drive may no longer recognized by the system. Perform a shutdown to re-establish communication between the system and the MOD drive.

NETWORK

- LightSpeed images will **not** transfer if Advantage Net protocols is used. Always use DICOM protocol to send LightSpeed images.

Network cont.

- LightSpeed images **cannot** be sent to a HiLight Advantage, HiSpeed Advantage or CT Independent console. These systems do not support DICOM receive.
- Some 3rd party workstations may fail to receive LightSpeed scout images. This is due to the matrix size of the scout image. These stations do not support receiving matrix sizes greater than 512. Some LightSpeed scouts images have matrix sizes greater than 512. If it is desired to have the scout image on the workstation, Screen Save the scout and then transfer the screen save image to the workstation.
- If you query a LightSpeed system from a CT/I or Advantage Windows system in Advantage Net, only Advantage format image exams will be displayed, No LightSpeed exams will be shown. Always query a LightSpeed system using DICOM protocol.
- Lateral scouts displayed on an AW 3.1 system will initially display with zero rotation; they should display with a 270-degree rotation. Rotate the image in the left direction using the rl command on the command line to display the scout in the desired format.
- Images networked to a Advantage Windows 3.1 workstation running software versions prior to 3.1_07 will display a DFOV less than what is displayed on the scanner. This is due to the AW not taking in account the pixels under the focus border of the viewport.
- Images networked to a AW 3.1 will have the following annotation missing:
 - Accession number,
 - Date of Birth,
 - 4i, 2i or 1i recon mode on Axial, Retro Axial or Axial Reformatted images,
 - Series type on Retro images,
 - Table Speed on Helical images,
 - Images are annotated +C when Oral Contrast is used. View the Series Text Page to see if IV contrast was used.
 - CardIQ annotation for BPM and percent of R-R interval and scan type will displayed as Axial.
- The number of images indicated in a series may be incorrect on the remote browser when a query is made from an AW or CT/I station.
- Series types may be listed differently when images are networked to an Advantage Windows 1.2, 2.0 or 3.1 system than that shown on the LightSpeed system
- Exams with Swedish, German or French characters in any Patient Info field will not be transferred to an Advantage Windows.
- When using DICOM protocol, the entered host name must match in spelling and case sensitive, otherwise a connection error message will be displayed.
- It's best to resolve any paused queue entry as soon as possible.

IMAGE MANAGEMENT

- Don't let image space fall below 200 images on a single disk system (130,000-image storage). This will ensure there is room on the system disk to confirm scans and to install reconstructed images.
- Remove images when scanning is idle. This will assure that all images are reconstructed, displayed and installed into the database.

This page left intentionally blank

This page left intentionally blank

GE Medical Systems

P.O. BOX 414

MILWAUKEE WISCONSIN 53201-0414 U.S.A.