





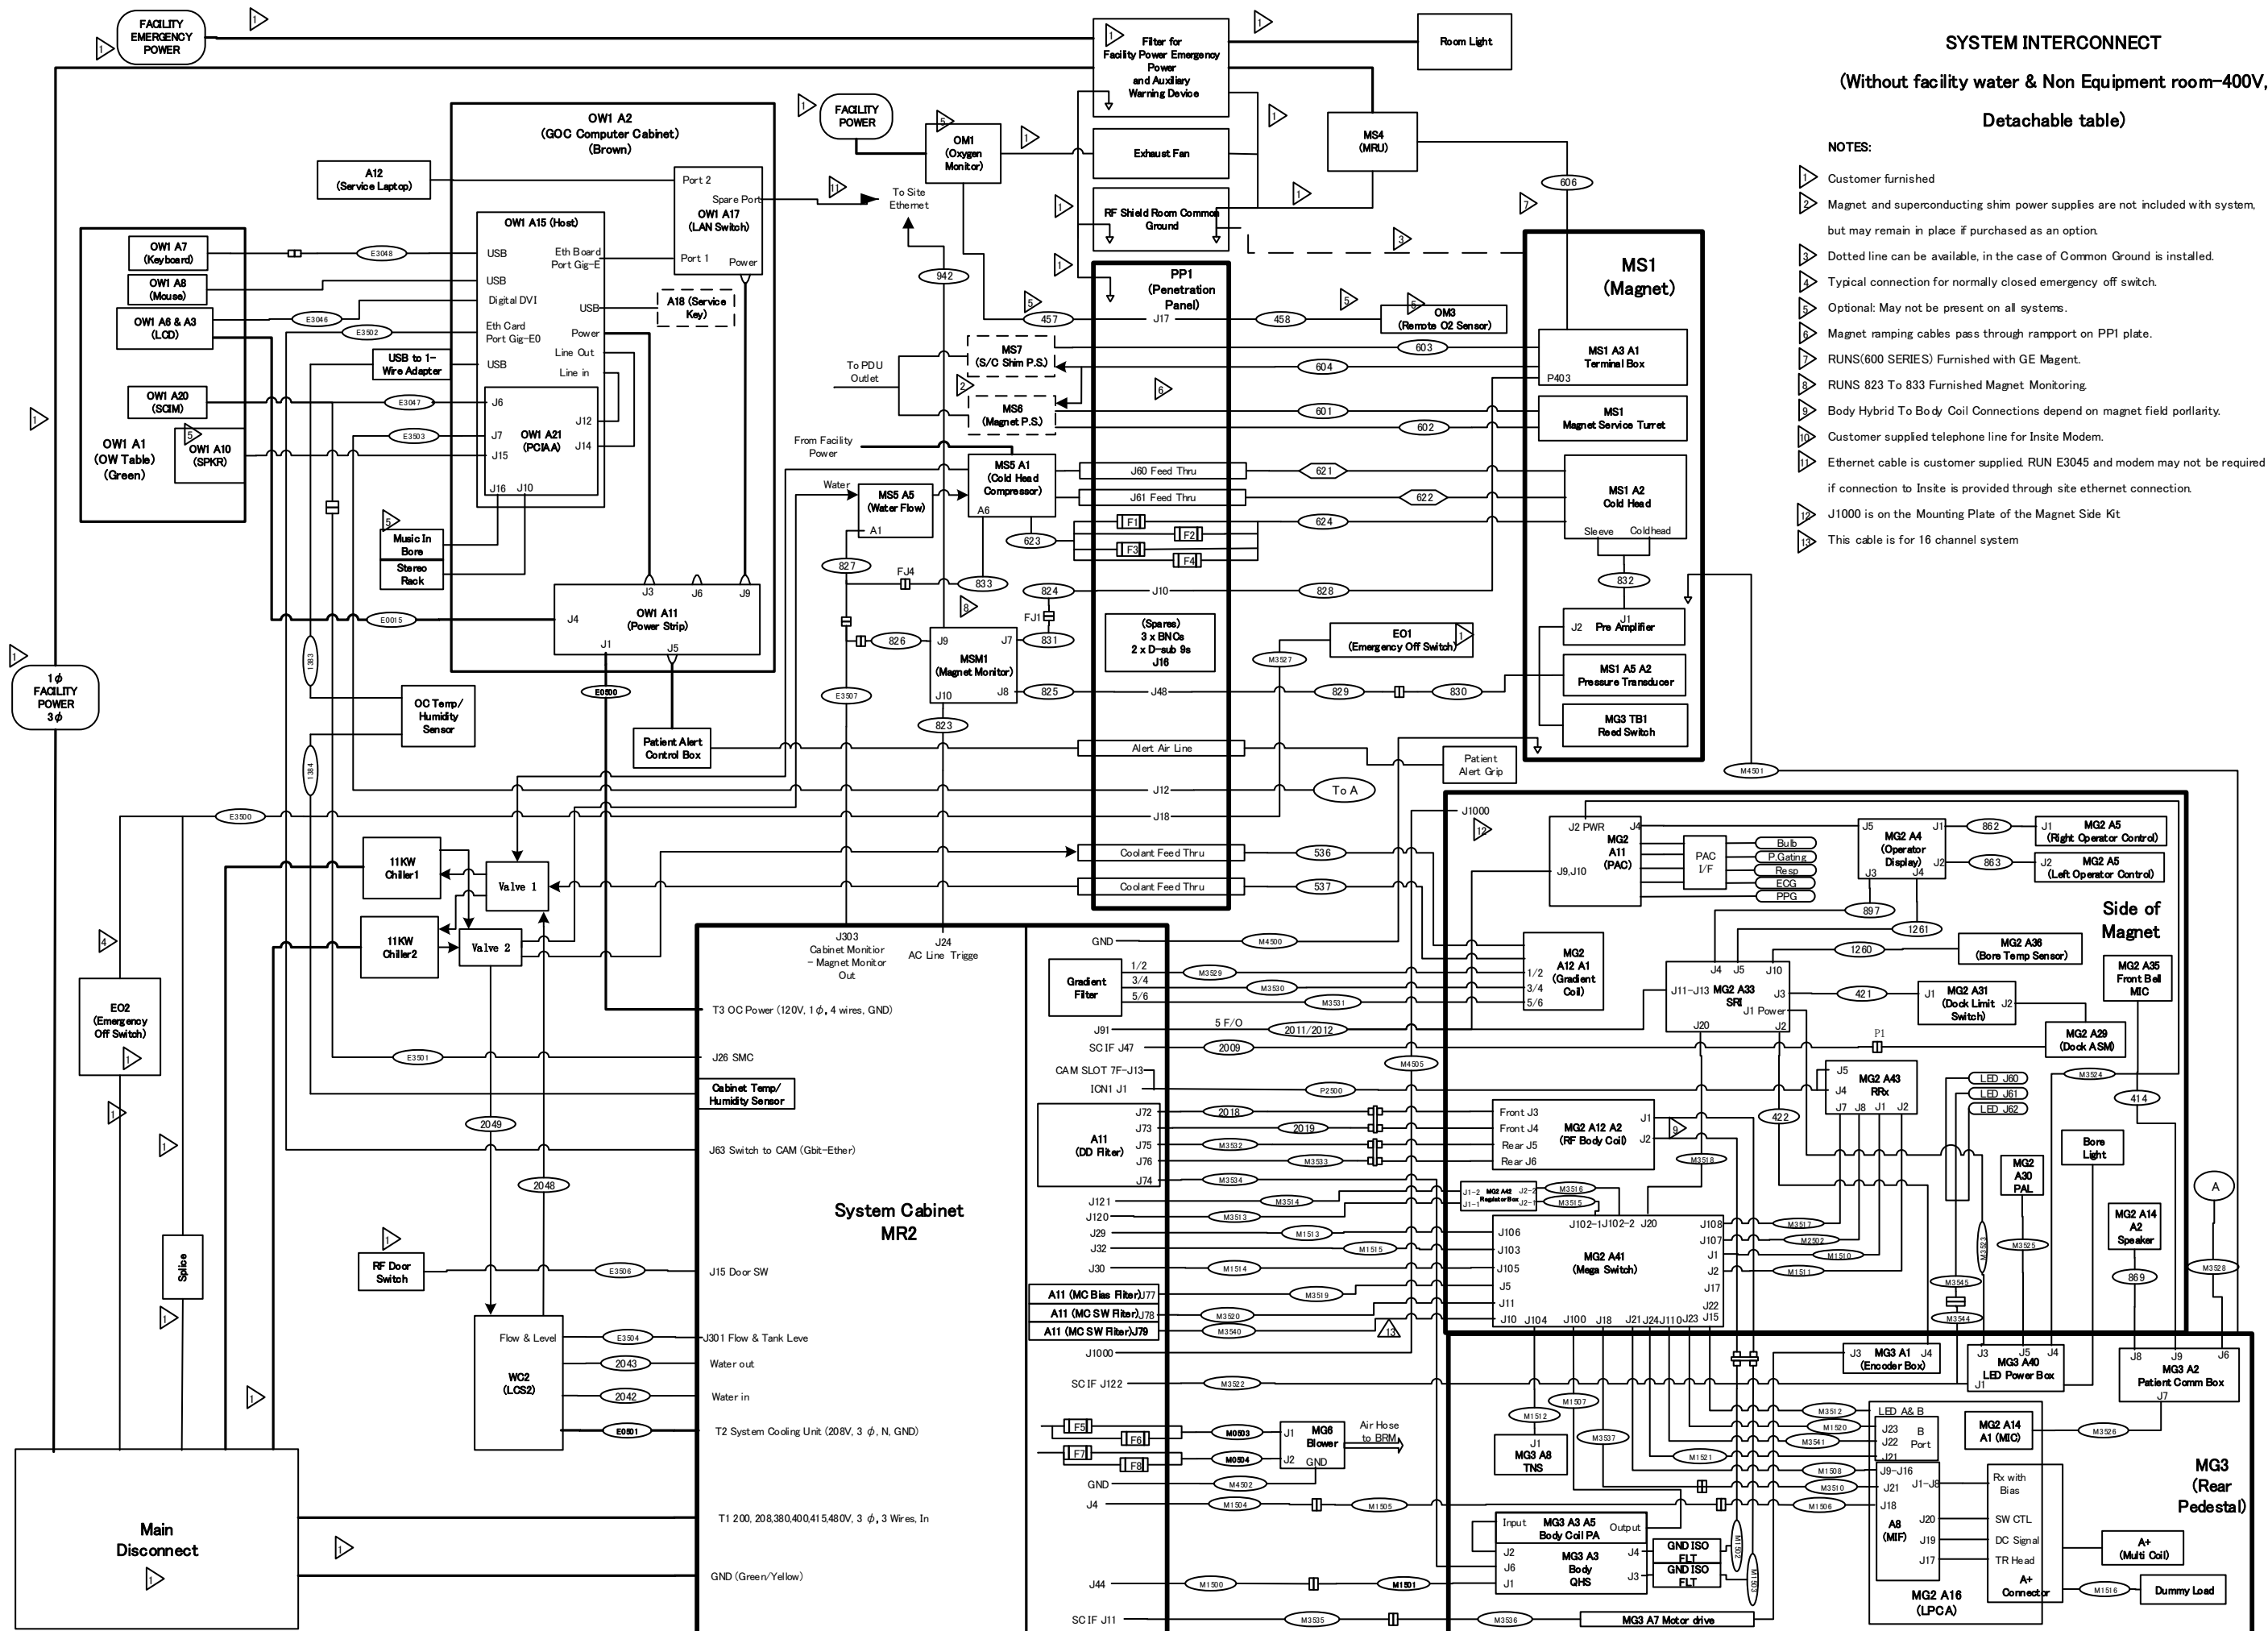

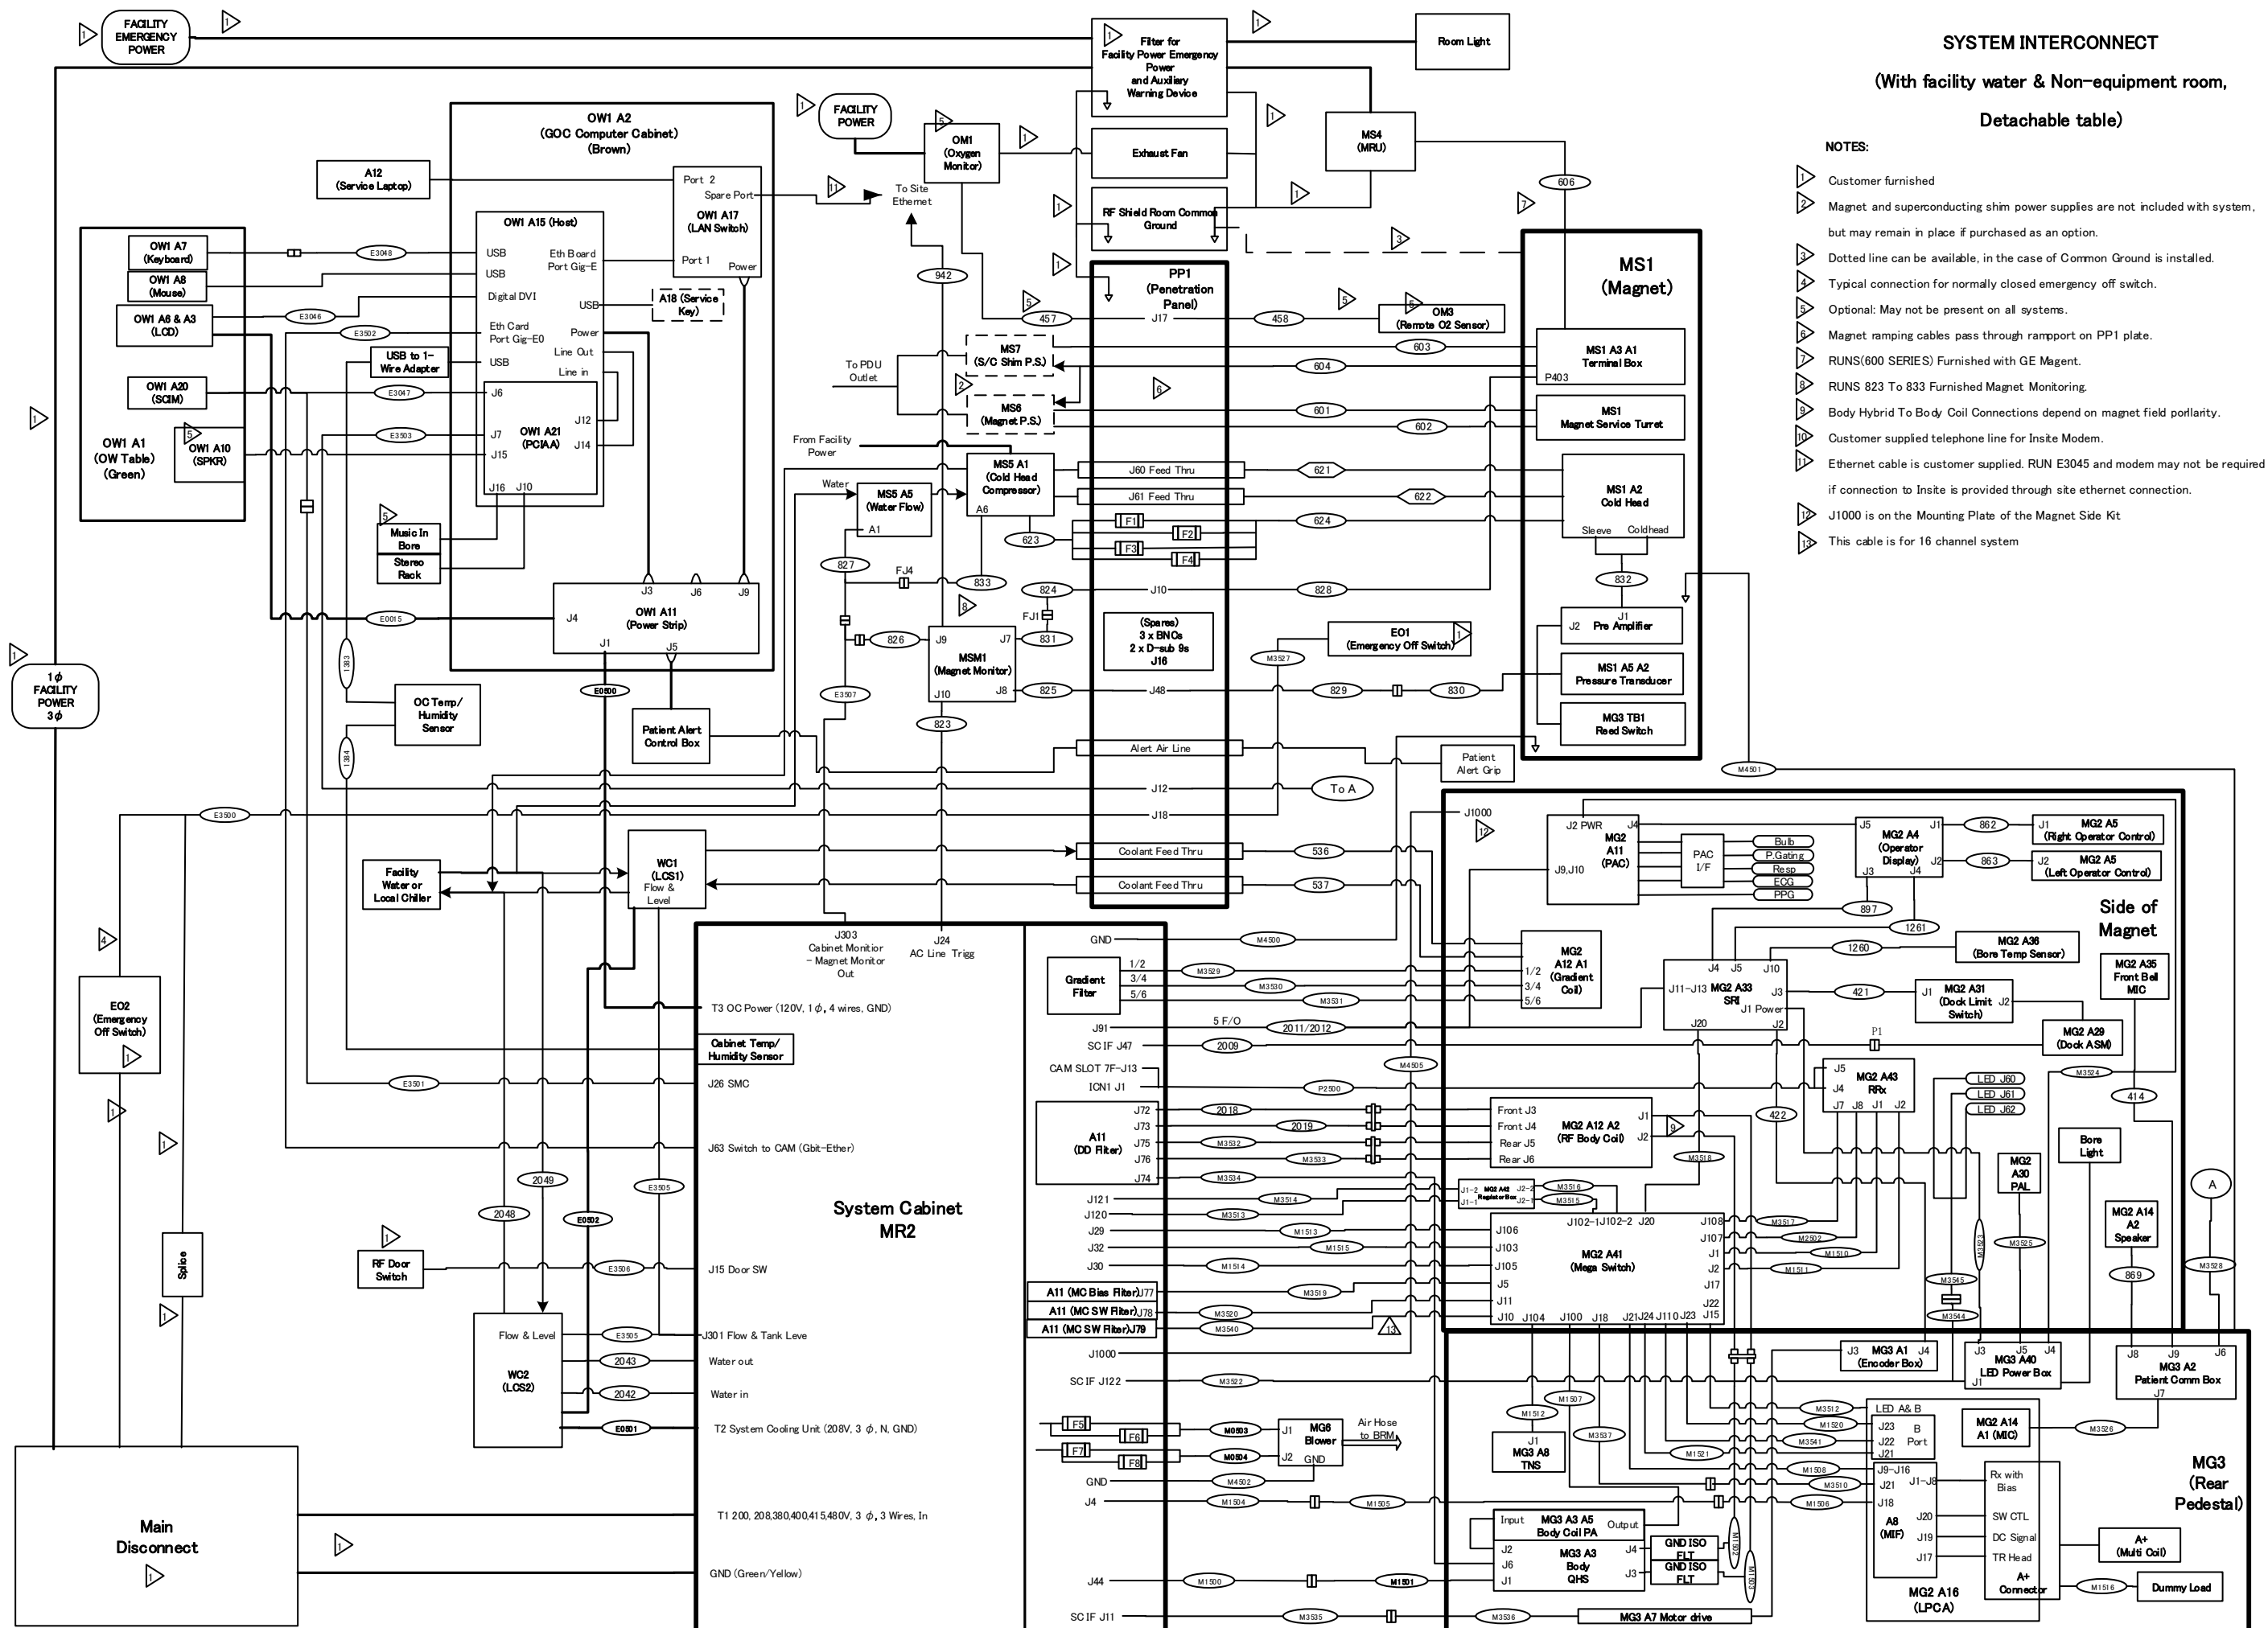

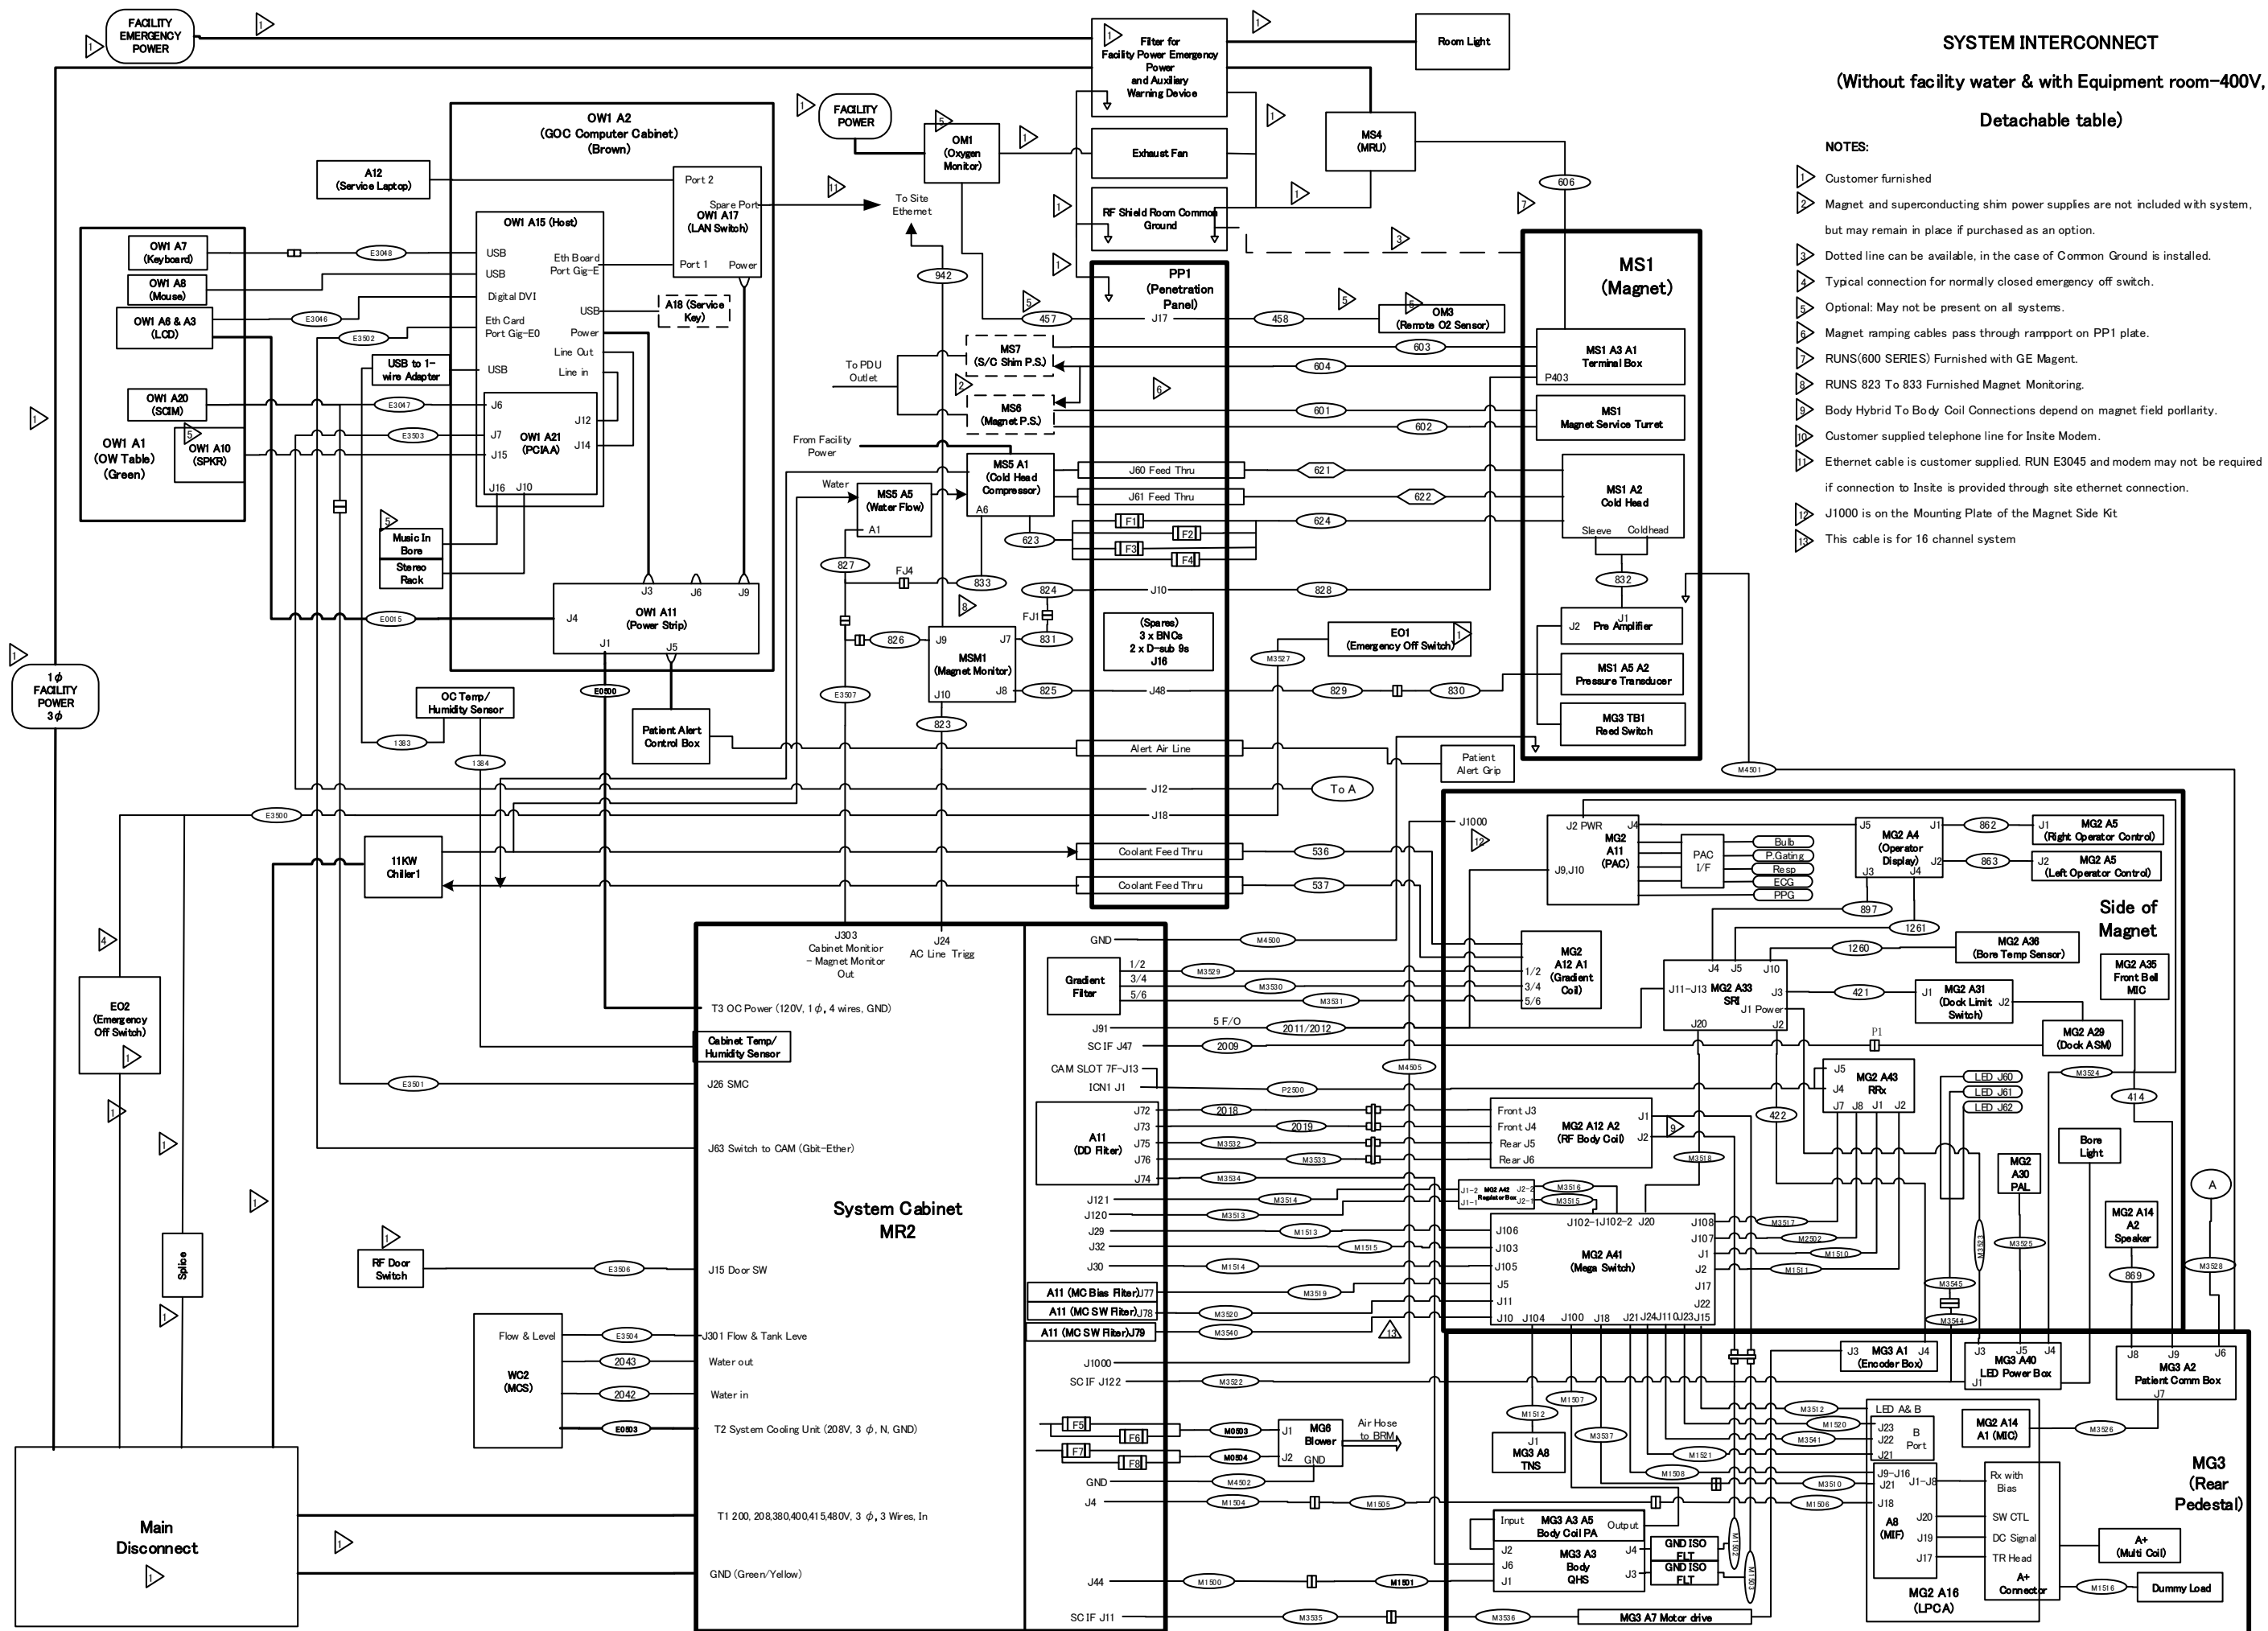

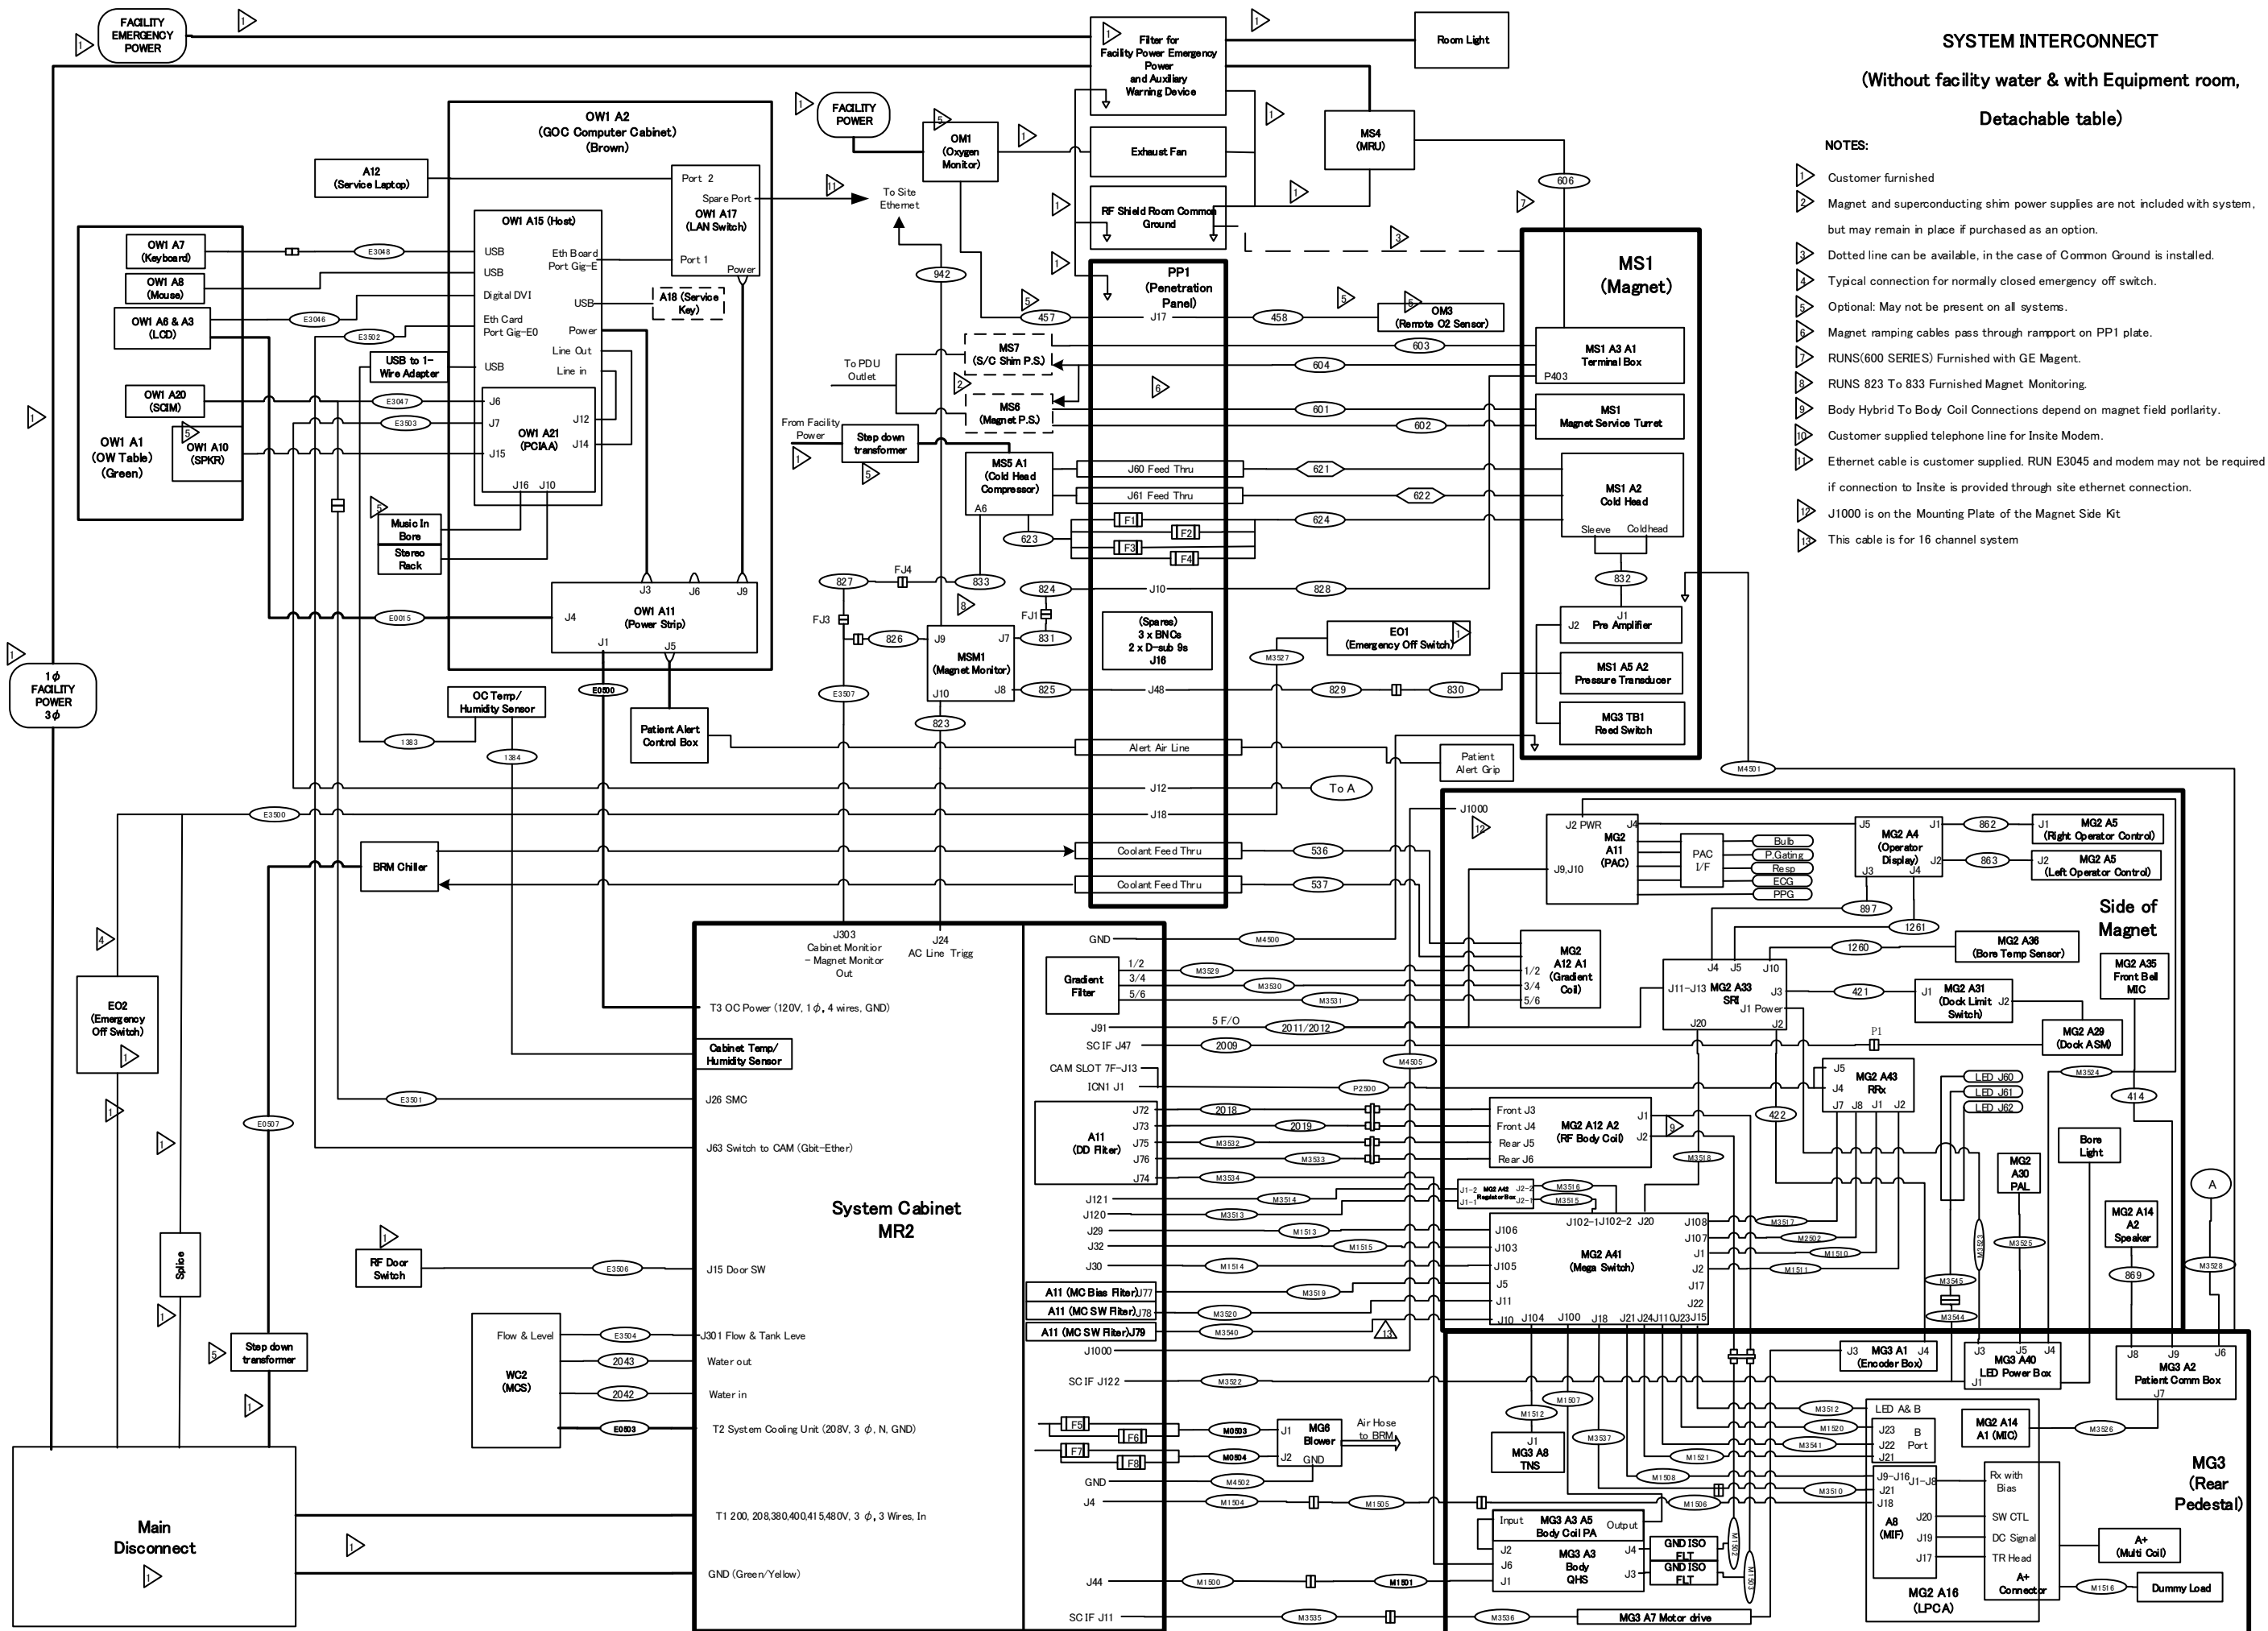

SYSTEM INTERCONNECT

(Without facility water & with Equipment room,
Detachable table)

NOTES:

- Customer furnished
- Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- Dotted line can be available, in the case of Common Ground is installed.
- Typical connection for normally closed emergency off switch.
- Optional: May not be present on all systems.
- Magnet ramping cables pass through rampout on PP1 plate.
- RUNS(600 SERIES) Furnished with GE Magnet.
- RUNS 823 To 833 Furnished Magnet Monitoring.
- Body Hybrid To Body Coil Connections depend on magnet field porlarity.
- Customer supplied telephone line for Insite Modem.
- Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- J1000 is on the Mounting Plate of the Magnet Side Kit
- This cable is for 16 channel system

