




PHILIPS

Philips Medical Systems

GYROSCAN INTERA INSTALLATION

MR/INTERA-SMI-71

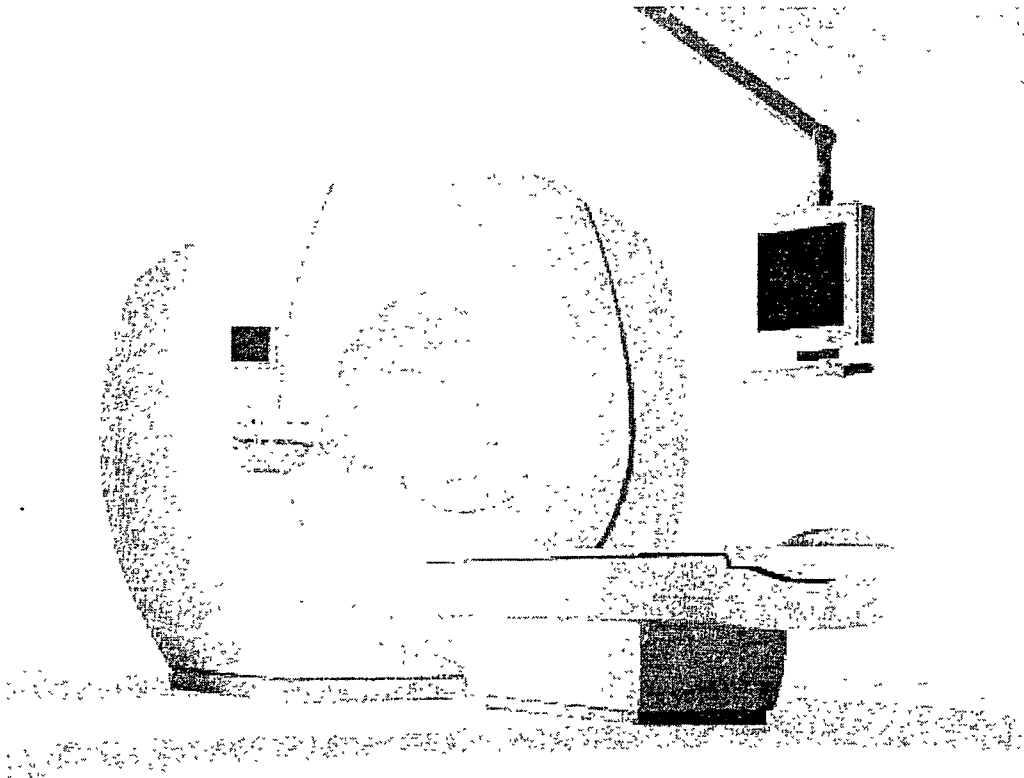

PROPRIETARY NOTICE

This manual and the information contained therein is proprietary to Philips and shall not be reproduced, copied in whole or part, adapted, modified, or disseminated without the written permission of Philips. Use of this manual and the information contained therein is strictly reserved for Philips engineers or persons licensed by Philips. Use of the manual by unauthorized persons is strictly prohibited.

Printed in Best, the Netherlands

Copyright © 1999 Philips Medical Systems Nederland B.V.
ALL RIGHTS RESERVED

CONTENTS OF THE MANUAL

Detailed list of contents
are given at the beginning
of each section.

12. PATIENT SUPPORT	1. GENERAL 
13. COVERS	2. MECHANICAL INSTALLATION (Part 1) 
14. NTDAC	3. CABINET INSTALLATION 
15. RF COILS (0.5T / 1.0T / 1.5T)	4. CRYOGENICS 
16. MAGNET ADJUSTMENT	5. MAINS CABLES 
17. GRADIENT SYSTEM	6. CRYO-COOLER 
18. SYSTEM LEVEL	7. MECHANICAL INSTALLATION (Part 2) 
19. PHYSIOLOGY	8. SIGNAL CABLES 
20. ACCEPTANCE	9. GRADIENT LIQUID COOLING SYSTEM 
21. OPTIONS	10. MAINS DISTRIBUTION 
22. MEASUREMENT RESULTS LIST	11. OPERATOR CONSOLE 

SERVICE MANUAL - INSTALLATION
GYROSCAN Intera
MR/Intera-SMI-71

Serial Number :

Manual Codenumber : 4522 981 05731

LIST OF PAGES AND DRAWINGS :

transparent plastic sheet

MR/INTERA-SMI-71	1	99.0	MR/INTERA-SMI-71	BCD 1.26	99.0
MR/INTERA-SMI-71	2	99.0	MR/INTERA-SMI-71	BCD 1.27	99.0
MR/INTERA-SMI-71	2.1	99.0	MR/INTERA-SMI-71	BCD 1.28	99.0
MR/INTERA-SMI-71	2.2	99.0	MR/INTERA-SMI-71	BCD 1.29	99.0
MR/INTERA-SMI-71	2.3	99.0	MR/INTERA-SMI-71	BCD 1.30	99.0
MR/INTERA-SMI-71	2.4	99.0			
MR/INTERA-SMI-71	2.5	99.0	MR/INTERA-SMI-71	BCD 2a.1	99.0
MR/INTERA-SMI-71	2.6	99.0	MR/INTERA-SMI-71	BCD 2a.2	99.0
MR/INTERA-SMI-71	2.7	99.0	MR/INTERA-SMI-71	BCD 2a.3	99.0
MR/INTERA-SMI-71	2.8	99.0	MR/INTERA-SMI-71	BCD 2a.4	99.0
			MR/INTERA-SMI-71	BCD 2a.5	99.0
MR/INTERA-SMI-71	BCD 1.1	99.0	MR/INTERA-SMI-71	BCD 2a.6	99.0
MR/INTERA-SMI-71	BCD 1.2	99.0	MR/INTERA-SMI-71	BCD 2a.7	99.0
MR/INTERA-SMI-71	BCD 1.3	99.0	MR/INTERA-SMI-71	BCD 2a.8	99.0
MR/INTERA-SMI-71	BCD 1.4	99.0	MR/INTERA-SMI-71	BCD 2a.9	99.0
MR/INTERA-SMI-71	BCD 1.5	99.0	MR/INTERA-SMI-71	BCD 2a.10	99.0
MR/INTERA-SMI-71	BCD 1.6	99.0	MR/INTERA-SMI-71	BCD 2a.11	99.0
MR/INTERA-SMI-71	BCD 1.7	99.0	MR/INTERA-SMI-71	BCD 2a.12	99.0
MR/INTERA-SMI-71	BCD 1.8	99.0	MR/INTERA-SMI-71	BCD 2a.13	99.0
MR/INTERA-SMI-71	BCD 1.9	99.0	MR/INTERA-SMI-71	BCD 2a.14	99.0
MR/INTERA-SMI-71	BCD 1.10	99.0			
MR/INTERA-SMI-71	BCD 1.11	99.0	MR/INTERA-SMI-71	BCD 2b.1	99.0
MR/INTERA-SMI-71	BCD 1.12	99.0		(green)	
MR/INTERA-SMI-71	BCD 1.13	99.0	MR/INTERA-SMI-71	BCD 2b.2	99.0
MR/INTERA-SMI-71	BCD 1.14	99.0	MR/INTERA-SMI-71	BCD 2b.3	99.0
MR/INTERA-SMI-71	BCD 1.15	99.0	MR/INTERA-SMI-71	BCD 2b.4	99.0
MR/INTERA-SMI-71	BCD 1.16	99.0	MR/INTERA-SMI-71	BCD 2b.5	99.0
MR/INTERA-SMI-71	BCD 1.17	99.0	MR/INTERA-SMI-71	BCD 2b.6	99.0
MR/INTERA-SMI-71	BCD 1.18	99.0	MR/INTERA-SMI-71	BCD 2b.7	99.0
MR/INTERA-SMI-71	BCD 1.19	99.0	MR/INTERA-SMI-71	BCD 2b.8	99.0
MR/INTERA-SMI-71	BCD 1.20	99.0	MR/INTERA-SMI-71	BCD 2b.9	99.0
MR/INTERA-SMI-71	BCD 1.21	99.0	MR/INTERA-SMI-71	BCD 2b.10	99.0
MR/INTERA-SMI-71	BCD 1.22	99.0	MR/INTERA-SMI-71	BCD 2b.11	99.0
MR/INTERA-SMI-71	BCD 1.23	99.0	MR/INTERA-SMI-71	BCD 2b.12	99.0
MR/INTERA-SMI-71	BCD 1.24	99.0	MR/INTERA-SMI-71	BCD 2b.13	99.0
MR/INTERA-SMI-71	BCD 1.25	99.0	MR/INTERA-SMI-71	BCD 2b.14	99.0

GYROSCAN Intera

SMI LOPAD

MR/INTERA-SMI-71	BCD 2b.15	99.0	MR/INTERA-SMI-71	BCD 4 11	99.0
MR/INTERA-SMI-71	BCD 2b.16	99.0	MR/INTERA-SMI-71	BCD 4 12	99.0
MR/INTERA-SMI-71	BCD 2b.17	99.0	MR/INTERA-SMI-71	BCD 4.13	99.0
MR/INTERA-SMI-71	BCD 2b.18	99.0	MR/INTERA-SMI-71	BCD 4.14	99.0
MR/INTERA-SMI-71	BCD 2b.19	99.0	MR/INTERA-SMI-71	BCD 4.15	99.0
MR/INTERA-SMI-71	BCD 2b.20	99.0	MR/INTERA-SMI-71	BCD 4.16	99.0
MR/INTERA-SMI-71	BCD 2b.21	99.0			
MR/INTERA-SMI-71	BCD 2b.22	99.0	MR/INTERA/1-SMI-71	BCD 5.1	99.0
MR/INTERA-SMI-71	BCD 2b.23	99.0	MR/INTERA/1-SMI-71	BCD 5 2	99.0
MR/INTERA-SMI-71	BCD 2b.24	99.0	MR/INTERA/1-SMI-71	BCD 5.3	99.0
MR/INTERA-SMI-71	BCD 2b.25	99.0	MR/INTERA/1-SMI-71	BCD 5 4	99.0
			MR/INTERA/1-SMI-71	BCD 5.5	99.0
			MR/INTERA/1-SMI-71	BCD 5.6	99.0
MR/INTERA/1-SMI-71	BCD 3.1	99.0	MR/INTERA/1-SMI-71	BCD 5.7	99.0
MR/INTERA/1-SMI-71	BCD 3.2	99.0	MR/INTERA/1-SMI-71	BCD 5.8	99.0
MR/INTERA/1-SMI-71	BCD 3.3	99.0			
MR/INTERA/1-SMI-71	BCD 3.4	99.0	MR/INTERA/36-SMI-71	BCD 5 1	99.0
MR/INTERA/1-SMI-71	BCD 3.5	99.0	(green)		
MR/INTERA/1-SMI-71	BCD 3.6	99.0	MR/INTERA/36-SMI-71	BCD 5.2	99.0
MR/INTERA/1-SMI-71	BCD 3.7	99.0	MR/INTERA/36-SMI-71	BCD 5.3	99.0
MR/INTERA/1-SMI-71	BCD 3.8	99.0	MR/INTERA/36-SMI-71	BCD 5 4	99.0
MR/INTERA/1-SMI-71	BCD 3.9	99.0	MR/INTERA/36-SMI-71	BCD 5 5	99.0
MR/INTERA/1-SMI-71	BCD 3.10	99.0	MR/INTERA/36-SMI-71	BCD 5.6	99.0
MR/INTERA/1-SMI-71	BCD 3.11	99.0	MR/INTERA/36-SMI-71	BCD 5.7	99.0
MR/INTERA/1-SMI-71	BCD 3.12	99.0	MR/INTERA/36-SMI-71	BCD 5.8	99.0
MR/INTERA/1-SMI-71	BCD 3.13	99.0			
			MR/INTERA-SMI-71	BCD 6.1	99.0
MR/INTERA/36-SMI-71	BCD 3.1	99.0	MR/INTERA-SMI-71	BCD 6.2	99.0
MR/INTERA/36-SMI-71	BCD 3.2	99.0	MR/INTERA-SMI-71	BCD 6.3	99.0
MR/INTERA/36-SMI-71	BCD 3.3	99.0	MR/INTERA-SMI-71	BCD 6 4	99.0
MR/INTERA/36-SMI-71	BCD 3.4	99.0	MR/INTERA-SMI-71	BCD 6.5	99.0
MR/INTERA/36-SMI-71	BCD 3.5	99.0	MR/INTERA-SMI-71	BCD 6.6	99.0
MR/INTERA/36-SMI-71	BCD 3.6	99.0	MR/INTERA-SMI-71	BCD 6.7	99.0
MR/INTERA/36-SMI-71	BCD 3.7	99.0	MR/INTERA-SMI-71	BCD 6.8	99.0
MR/INTERA/36-SMI-71	BCD 3.8	99.0			
MR/INTERA/36-SMI-71	BCD 3.9	99.0	MR/INTERA/1-SMI-71	BCD 7.1	99.0
MR/INTERA/36-SMI-71	BCD 3.10	99.0	(green)		
MR/INTERA/36-SMI-71	BCD 3.11	99.0	MR/INTERA/1-SMI-71	BCD 7.2	99.0
MR/INTERA/36-SMI-71	BCD 3.12	99.0	MR/INTERA/1-SMI-71	BCD 7.3	99.0
MR/INTERA/36-SMI-71	BCD 3.13	99.0	MR/INTERA/1-SMI-71	BCD 7.4	99.0
MR/INTERA/36-SMI-71	BCD 3.14	99.0	MR/INTERA/1-SMI-71	BCD 7.5	99.0
MR/INTERA/36-SMI-71	BCD 3.15	99.0	MR/INTERA/1-SMI-71	BCD 7.6	99.0
MR/INTERA/36-SMI-71	BCD 3.16	99.0	MR/INTERA/1-SMI-71	BCD 7.7	99.0
MR/INTERA/36-SMI-71	BCD 3.17	99.0	MR/INTERA/1-SMI-71	BCD 7.8	99.0
MR/INTERA/36-SMI-71	BCD 3.18	99.0	MR/INTERA/1-SMI-71	BCD 7.9	99.0
MR/INTERA/36-SMI-71	BCD 3.19	99.0	MR/INTERA/1-SMI-71	BCD 7.10	99.0
MR/INTERA/36-SMI-71	BCD 3.20	99.0	MR/INTERA/1-SMI-71	BCD 7.11	99.0
			MR/INTERA/1-SMI-71	BCD 7.12	99.0
MR/INTERA-SMI-71	BCD 4.1	99.0	MR/INTERA/1-SMI-71	BCD 7.13	99.0
MR/INTERA-SMI-71	BCD 4.2	99.0	MR/INTERA/1-SMI-71	BCD 7.14	99.0
MR/INTERA-SMI-71	BCD 4.3	99.0	MR/INTERA/1-SMI-71	BCD 7.15	99.0
MR/INTERA-SMI-71	BCD 4.4	99.0	MR/INTERA/1-SMI-71	BCD 7.16	99.0
MR/INTERA-SMI-71	BCD 4.5	99.0	MR/INTERA/1-SMI-71	BCD 7.17	99.0
MR/INTERA-SMI-71	BCD 4.6	99.0	MR/INTERA/1-SMI-71	BCD 7.18	99.0
MR/INTERA-SMI-71	BCD 4.7	99.0	MR/INTERA/1-SMI-71	BCD 7.19	99.0
MR/INTERA-SMI-71	BCD 4.8	99.0	MR/INTERA/1-SMI-71	BCD 7.20	99.0
MR/INTERA-SMI-71	BCD 4.9	99.0	MR/INTERA/1-SMI-71	BCD 7.21	99.0
MR/INTERA-SMI-71	BCD 4.10	99.0	MR/INTERA/1-SMI-71	BCD 7.22	99.0

GYROSCAN Intera

SMI LOPAD

MR/INTERA/1-SMI-71	BCD 7.23	99.0	MR/INTERA/1-SMI-71	BCD 8.11	99.0
MR/INTERA/1-SMI-71	BCD 7.24	99.0	MR/INTERA/1-SMI-71	BCD 8.12	99.0
MR/INTERA/1-SMI-71	BCD 7.25	99.0	MR/INTERA/1-SMI-71	BCD 8.13	99.0
MR/INTERA/1-SMI-71	BCD 7.26	99.0	MR/INTERA/1-SMI-71	BCD 8.14	99.0
MR/INTERA/1-SMI-71	BCD 7.27	99.0	MR/INTERA/1-SMI-71	BCD 8.15	99.0
MR/INTERA/1-SMI-71	BCD 7.28	99.0	MR/INTERA/1-SMI-71	BCD 8.16	99.0
MR/INTERA/1-SMI-71	BCD 7.29	99.0			
MR/INTERA/1-SMI-71	BCD 7.30	99.0	MR/INTERA/36-SMI-71	BCD 8.1	99.0
MR/INTERA/1-SMI-71	BCD 7.31	99.0	MR/INTERA/36-SMI-71	BCD 8.2	99.0
			MR/INTERA/36-SMI-71	BCD 8.3	99.0
MR/INTERA/36-SMI-71	BCD 7.1	99.0	MR/INTERA/36-SMI-71	BCD 8.4	99.0
	(green)		MR/INTERA/36-SMI-71	BCD 8.5	99.0
MR/INTERA/36-SMI-71	BCD 7.2	99.0	MR/INTERA/36-SMI-71	BCD 8.6	99.0
MR/INTERA/36-SMI-71	BCD 7.3	99.0	MR/INTERA/36-SMI-71	BCD 8.7	99.0
MR/INTERA/36-SMI-71	BCD 7.4	99.0	MR/INTERA/36-SMI-71	BCD 8.8	99.0
MR/INTERA/36-SMI-71	BCD 7.5	99.0	MR/INTERA/36-SMI-71	BCD 8.9	99.0
MR/INTERA/36-SMI-71	BCD 7.6	99.0	MR/INTERA/36-SMI-71	BCD 8.10	99.0
MR/INTERA/36-SMI-71	BCD 7.7	99.0	MR/INTERA/36-SMI-71	BCD 8.11	99.0
MR/INTERA/36-SMI-71	BCD 7.8	99.0	MR/INTERA/36-SMI-71	BCD 8.12	99.0
MR/INTERA/36-SMI-71	BCD 7.9	99.0	MR/INTERA/36-SMI-71	BCD 8.13	99.0
MR/INTERA/36-SMI-71	BCD 7.10	99.0	MR/INTERA/36-SMI-71	BCD 8.14	99.0
MR/INTERA/36-SMI-71	BCD 7.11	99.0	MR/INTERA/36-SMI-71	BCD 8.15	99.0
MR/INTERA/36-SMI-71	BCD 7.12	99.0	MR/INTERA/36-SMI-71	BCD 8.16	99.0
MR/INTERA/36-SMI-71	BCD 7.13	99.0	MR/INTERA/36-SMI-71	BCD 8.17	99.0
MR/INTERA/36-SMI-71	BCD 7.14	99.0	MR/INTERA/36-SMI-71	BCD 8.18	99.0
MR/INTERA/36-SMI-71	BCD 7.15	99.0	MR/INTERA/36-SMI-71	BCD 8.19	99.0
MR/INTERA/36-SMI-71	BCD 7.16	99.0			
MR/INTERA/36-SMI-71	BCD 7.17	99.0	MR/INTERA-SMI-71	BCD 9.1	99.0
MR/INTERA/36-SMI-71	BCD 7.18	99.0	MR/INTERA-SMI-71	BCD 9.2	99.0
MR/INTERA/36-SMI-71	BCD 7.19	99.0	MR/INTERA-SMI-71	BCD 9.3	99.0
MR/INTERA/36-SMI-71	BCD 7.20	99.0	MR/INTERA-SMI-71	BCD 9.4	99.0
MR/INTERA/36-SMI-71	BCD 7.21	99.0	MR/INTERA-SMI-71	BCD 9.5	99.0
MR/INTERA/36-SMI-71	BCD 7.22	99.0	MR/INTERA-SMI-71	BCD 9.6	99.0
MR/INTERA/36-SMI-71	BCD 7.23	99.0	MR/INTERA-SMI-71	BCD 9.7	99.0
MR/INTERA/36-SMI-71	BCD 7.24	99.0	MR/INTERA-SMI-71	BCD 9.8	99.0
MR/INTERA/36-SMI-71	BCD 7.25	99.0	MR/INTERA-SMI-71	BCD 9.9	99.0
MR/INTERA/36-SMI-71	BCD 7.26	99.0	MR/INTERA-SMI-71	BCD 9.10	99.0
MR/INTERA/36-SMI-71	BCD 7.27	99.0	MR/INTERA-SMI-71	BCD 9.11	99.0
MR/INTERA/36-SMI-71	BCD 7.28	99.0	MR/INTERA-SMI-71	BCD 9.12	99.0
MR/INTERA/36-SMI-71	BCD 7.29	99.0	MR/INTERA-SMI-71	BCD 9.13	99.0
MR/INTERA/36-SMI-71	BCD 7.30	99.0			
MR/INTERA/36-SMI-71	BCD 7.31	99.0	MR/INTERA-SMI-71	BCD 10.1	99.0
MR/INTERA/36-SMI-71	BCD 7.32	99.0	MR/INTERA-SMI-71	BCD 10.2	99.0
MR/INTERA/36-SMI-71	BCD 7.33	99.0	MR/INTERA-SMI-71	BCD 10.3	99.0
MR/INTERA/36-SMI-71	BCD 7.34	99.0	MR/INTERA-SMI-71	BCD 10.4	99.0
MR/INTERA/36-SMI-71	BCD 7.35	99.0	MR/INTERA-SMI-71	BCD 10.5	99.0
MR/INTERA/36-SMI-71	BCD 7.36	99.0			
			MR/INTERA-SMI-71	BCD 11.1	99.0
MR/INTERA/1-SMI-71	BCD 8.1	99.0	MR/INTERA-SMI-71	BCD 11.2	99.0
MR/INTERA/1-SMI-71	BCD 8.2	99.0	MR/INTERA-SMI-71	BCD 11.3	99.0
MR/INTERA/1-SMI-71	BCD 8.3	99.0	MR/INTERA-SMI-71	BCD 11.4	99.0
MR/INTERA/1-SMI-71	BCD 8.4	99.0	MR/INTERA-SMI-71	BCD 11.5	99.0
MR/INTERA/1-SMI-71	BCD 8.5	99.0	MR/INTERA-SMI-71	BCD 11.6	99.0
MR/INTERA/1-SMI-71	BCD 8.6	99.0	MR/INTERA-SMI-71	BCD 11.7	99.0
MR/INTERA/1-SMI-71	BCD 8.7	99.0	MR/INTERA-SMI-71	BCD 11.8	99.0
MR/INTERA/1-SMI-71	BCD 8.8	99.0	MR/INTERA-SMI-71	BCD 11.9	99.0
MR/INTERA/1-SMI-71	BCD 8.9	99.0	MR/INTERA-SMI-71	BCD 11.10	99.0
MR/INTERA/1-SMI-71	BCD 8.10	99.0	MR/INTERA-SMI-71	BCD 11.11	99.0

GYROSCAN Intertra

SMI LOPAD

MR/INTERA-SMI-71	BCD 11.12	99.0	MR/INTERA-5/1-SMI-71	BCD 15.7	99.0
MR/INTERA-SMI-71	BCD 11.13	99.0	MR/INTERA-5/1-SMI-71	BCD 15.8	99.0
MR/INTERA-SMI-71	BCD 11.14	99.0	MR/INTERA-5/1-SMI-71	BCD 15.9	99.0
MR/INTERA-SMI-71	BCD 11.15	99.0	MR/INTERA-5/1-SMI-71	BCD 15.10	99.0
MR/INTERA-SMI-71	BCD 11.16	99.0	MR/INTERA-5/1-SMI-71	BCD 15.11	99.0
MR/INTERA-SMI-71	BCD 11.17	99.0	MR/INTERA-5/1-SMI-71	BCD 15.12	99.0
MR/INTERA-SMI-71	BCD 11.18	99.0	MR/INTERA-5/1-SMI-71	BCD 15.13	99.0
MR/INTERA-SMI-71	BCD 11.19	99.0	MR/INTERA-5/1-SMI-71	BCD 15.14	99.0
MR/INTERA-SMI-71	BCD 11.20	99.0	MR/INTERA-5/1-SMI-71	BCD 15.15	99.0
MR/INTERA-SMI-71	BCD 11.21	99.0	MR/INTERA-5/1-SMI-71	BCD 15.16	99.0
MR/INTERA-SMI-71	BCD 11.22	99.0	MR/INTERA-5/1-SMI-71	BCD 15.17	99.0
MR/INTERA-SMI-71	BCD 11.23	99.0	MR/INTERA-5/1-SMI-71	BCD 15.18	99.0
			MR/INTERA-5/1-SMI-71	BCD 15.19	99.0
MR/INTERA-SMI-71	BCD 12.1	99.0	MR/INTERA-5/1-SMI-71	BCD 15.20	99.0
MR/INTERA-SMI-71	BCD 12.2	99.0	MR/INTERA-5/1-SMI-71	BCD 15.21	99.0
MR/INTERA-SMI-71	BCD 12.3	99.0	MR/INTERA-5/1-SMI-71	BCD 15.22	99.0
MR/INTERA-SMI-71	BCD 12.4	99.0	MR/INTERA-5/1-SMI-71	BCD 15.23	99.0
MR/INTERA-SMI-71	BCD 12.5	99.0	MR/INTERA-5/1-SMI-71	BCD 15.24	99.0
			MR/INTERA-5/1-SMI-71	BCD 15.25	99.0
MR/INTERA-SMI-71	BCD 13.1	99.0	MR/INTERA-5/1-SMI-71	BCD 15.26	99.0
MR/INTERA-SMI-71	BCD 13.2	99.0	MR/INTERA-5/1-SMI-71	BCD 15.27	99.0
MR/INTERA-SMI-71	BCD 13.3	99.0	MR/INTERA-5/1-SMI-71	BCD 15.28	99.0
MR/INTERA-SMI-71	BCD 13.4	99.0			
MR/INTERA-SMI-71	BCD 13.5	99.0	MR/INTERA-10/1-SMI-71	BCD 15.1	99.0
MR/INTERA-SMI-71	BCD 13.6	99.0		(green)	
MR/INTERA-SMI-71	BCD 13.7	99.0	MR/INTERA-10/1-SMI-71	BCD 15.2	99.0
MR/INTERA-SMI-71	BCD 13.8	99.0	MR/INTERA-10/1-SMI-71	BCD 15.3	99.0
MR/INTERA-SMI-71	BCD 13.9	99.0	MR/INTERA-10/1-SMI-71	BCD 15.4	99.0
MR/INTERA-SMI-71	BCD 13.10	99.0	MR/INTERA-10/1-SMI-71	BCD 15.5	99.0
MR/INTERA-SMI-71	BCD 13.11	99.0	MR/INTERA-10/1-SMI-71	BCD 15.6	99.0
MR/INTERA-SMI-71	BCD 13.12	99.0	MR/INTERA-10/1-SMI-71	BCD 15.7	99.0
MR/INTERA-SMI-71	BCD 13.13	99.0	MR/INTERA-10/1-SMI-71	BCD 15.8	99.0
MR/INTERA-SMI-71	BCD 13.14	99.0	MR/INTERA-10/1-SMI-71	BCD 15.9	99.0
MR/INTERA-SMI-71	BCD 13.15	99.0	MR/INTERA-10/1-SMI-71	BCD 15.10	99.0
MR/INTERA-SMI-71	BCD 13.16	99.0	MR/INTERA-10/1-SMI-71	BCD 15.11	99.0
MR/INTERA-SMI-71	BCD 13.17	99.0	MR/INTERA-10/1-SMI-71	BCD 15.12	99.0
			MR/INTERA-10/1-SMI-71	BCD 15.13	99.0
MR/INTERA-SMI-71	BCD 14.1	99.0	MR/INTERA-10/1-SMI-71	BCD 15.14	99.0
MR/INTERA-SMI-71	BCD 14.2	99.0	MR/INTERA-10/1-SMI-71	BCD 15.15	99.0
MR/INTERA-SMI-71	BCD 14.3	99.0	MR/INTERA-10/1-SMI-71	BCD 15.16	99.0
MR/INTERA-SMI-71	BCD 14.4	99.0	MR/INTERA-10/1-SMI-71	BCD 15.17	99.0
MR/INTERA-SMI-71	BCD 14.5	99.0	MR/INTERA-10/1-SMI-71	BCD 15.18	99.0
MR/INTERA-SMI-71	BCD 14.6	99.0	MR/INTERA-10/1-SMI-71	BCD 15.19	99.0
MR/INTERA-SMI-71	BCD 14.7	99.0	MR/INTERA-10/1-SMI-71	BCD 15.20	99.0
MR/INTERA-SMI-71	BCD 14.8	99.0	MR/INTERA-10/1-SMI-71	BCD 15.21	99.0
MR/INTERA-SMI-71	BCD 14.9	99.0	MR/INTERA-10/1-SMI-71	BCD 15.22	99.0
MR/INTERA-SMI-71	BCD 14.10	99.0	MR/INTERA-10/1-SMI-71	BCD 15.23	99.0
MR/INTERA-SMI-71	BCD 14.11	99.0	MR/INTERA-10/1-SMI-71	BCD 15.24	99.0
MR/INTERA-SMI-71	BCD 14.12	99.0	MR/INTERA-10/1-SMI-71	BCD 15.25	99.0
MR/INTERA-SMI-71	BCD 14.13	99.0	MR/INTERA-10/1-SMI-71	BCD 15.26	99.0
MR/INTERA-SMI-71	BCD 14.14	99.0	MR/INTERA-10/1-SMI-71	BCD 15.27	99.0
MR/INTERA-5/1-SMI-71	BCD 15.1	99.0	MR/INTERA-10/3-SMI-71	BCD 15.1	99.0
MR/INTERA-5/1-SMI-71	BCD 15.2	99.0		(green)	
MR/INTERA-5/1-SMI-71	BCD 15.3	99.0	MR/INTERA-10/3-SMI-71	BCD 15.2	99.0
MR/INTERA-5/1-SMI-71	BCD 15.4	99.0	MR/INTERA-10/3-SMI-71	BCD 15.3	99.0
MR/INTERA-5/1-SMI-71	BCD 15.5	99.0	MR/INTERA-10/3-SMI-71	BCD 15.4	99.0
MR/INTERA-5/1-SMI-71	BCD 15.6	99.0	MR/INTERA-10/3-SMI-71	BCD 15.5	99.0

GYROSCAN Intertra

SMI LOPAD

MR/INTERA-10/3-SMI-71	BCD 15.6	99.0	MR/INTERA-15/3-SMI-71	BCD 15.6	99.0
MR/INTERA-10/3-SMI-71	BCD 15.7	99.0	MR/INTERA-15/3-SMI-71	BCD 15.7	99.0
MR/INTERA-10/3-SMI-71	BCD 15.8	99.0	MR/INTERA-15/3-SMI-71	BCD 15.8	99.0
MR/INTERA-10/3-SMI-71	BCD 15.9	99.0	MR/INTERA-15/3-SMI-71	BCD 15.9	99.0
MR/INTERA-10/3-SMI-71	BCD 15.10	99.0	MR/INTERA-15/3-SMI-71	BCD 15.10	99.0
MR/INTERA-10/3-SMI-71	BCD 15.11	99.0	MR/INTERA-15/3-SMI-71	BCD 15.11	99.0
MR/INTERA-10/3-SMI-71	BCD 15.12	99.0	MR/INTERA-15/3-SMI-71	BCD 15.12	99.0
MR/INTERA-10/3-SMI-71	BCD 15.13	99.0	MR/INTERA-15/3-SMI-71	BCD 15.13	99.0
MR/INTERA-10/3-SMI-71	BCD 15.14	99.0	MR/INTERA-15/3-SMI-71	BCD 15.14	99.0
MR/INTERA-10/3-SMI-71	BCD 15.15	99.0	MR/INTERA-15/3-SMI-71	BCD 15.15	99.0
MR/INTERA-10/3-SMI-71	BCD 15.16	99.0	MR/INTERA-15/3-SMI-71	BCD 15.16	99.0
MR/INTERA-10/3-SMI-71	BCD 15.17	99.0	MR/INTERA-15/3-SMI-71	BCD 15.17	99.0
MR/INTERA-10/3-SMI-71	BCD 15.18	99.0	MR/INTERA-15/3-SMI-71	BCD 15.18	99.0
MR/INTERA-10/3-SMI-71	BCD 15.19	99.0	MR/INTERA-15/3-SMI-71	BCD 15.19	99.0
MR/INTERA-10/3-SMI-71	BCD 15.20	99.0	MR/INTERA-15/3-SMI-71	BCD 15.20	99.0
MR/INTERA-10/3-SMI-71	BCD 15.21	99.0	MR/INTERA-15/3-SMI-71	BCD 15.21	99.0
MR/INTERA-10/3-SMI-71	BCD 15.22	99.0	MR/INTERA-15/3-SMI-71	BCD 15.22	99.0
MR/INTERA-10/3-SMI-71	BCD 15.23	99.0	MR/INTERA-15/3-SMI-71	BCD 15.23	99.0
MR/INTERA-10/3-SMI-71	BCD 15.24	99.0	MR/INTERA-15/3-SMI-71	BCD 15.24	99.0
MR/INTERA-10/3-SMI-71	BCD 15.25	99.0	MR/INTERA-15/3-SMI-71	BCD 15.25	99.0
MR/INTERA-10/3-SMI-71	BCD 15.26	99.0	MR/INTERA-15/3-SMI-71	BCD 15.26	99.0
MR/INTERA-15/1-SMI-71	BCD 15.1	99.0	MR/INTERA-15/3-SMI-71	BCD 15.27	99.0
	(green)		MR/INTERA-SMI-71	BCD 16.1	99.0
MR/INTERA-15/1-SMI-71	BCD 15.2	99.0	MR/INTERA-SMI-71	BCD 16.2	99.0
MR/INTERA-15/1-SMI-71	BCD 15.3	99.0	MR/INTERA-SMI-71	BCD 16.3	99.0
MR/INTERA-15/1-SMI-71	BCD 15.4	99.0	MR/INTERA-SMI-71	BCD 16.4	99.0
MR/INTERA-15/1-SMI-71	BCD 15.5	99.0	MR/INTERA-SMI-71	BCD 16.5	99.0
MR/INTERA-15/1-SMI-71	BCD 15.6	99.0	MR/INTERA-SMI-71	BCD 16.6	99.0
MR/INTERA-15/1-SMI-71	BCD 15.7	99.0	MR/INTERA-SMI-71	BCD 16.7	99.0
MR/INTERA-15/1-SMI-71	BCD 15.8	99.0	MR/INTERA-SMI-71	BCD 16.8	99.0
MR/INTERA-15/1-SMI-71	BCD 15.9	99.0	MR/INTERA-SMI-71	BCD 16.9	99.0
MR/INTERA-15/1-SMI-71	BCD 15.10	99.0	MR/INTERA-SMI-71	BCD 16.10	99.0
MR/INTERA-15/1-SMI-71	BCD 15.11	99.0	MR/INTERA-SMI-71	BCD 16.11	99.0
MR/INTERA-15/1-SMI-71	BCD 15.12	99.0	MR/INTERA-SMI-71	BCD 16.12	99.0
MR/INTERA-15/1-SMI-71	BCD 15.13	99.0	MR/INTERA-SMI-71	BCD 16.13	99.0
MR/INTERA-15/1-SMI-71	BCD 15.14	99.0	MR/INTERA-SMI-71	BCD 16.14	99.0
MR/INTERA-15/1-SMI-71	BCD 15.15	99.0	MR/INTERA-SMI-71	BCD 16.15	99.0
MR/INTERA-15/1-SMI-71	BCD 15.16	99.0	MR/INTERA-SMI-71	BCD 16.16	99.0
MR/INTERA-15/1-SMI-71	BCD 15.17	99.0	MR/INTERA-SMI-71	BCD 16.17	99.0
MR/INTERA-15/1-SMI-71	BCD 15.18	99.0	MR/INTERA-SMI-71	BCD 16.18	99.0
MR/INTERA-15/1-SMI-71	BCD 15.19	99.0	MR/INTERA-SMI-71	BCD 16.19	99.0
MR/INTERA-15/1-SMI-71	BCD 15.20	99.0	MR/INTERA-SMI-71	BCD 16.20	99.0
MR/INTERA-15/1-SMI-71	BCD 15.21	99.0	MR/INTERA-SMI-71	BCD 16.21	99.0
MR/INTERA-15/1-SMI-71	BCD 15.22	99.0	MR/INTERA-SMI-71	BCD 16.22	99.0
MR/INTERA-15/1-SMI-71	BCD 15.23	99.0	MR/INTERA-SMI-71	BCD 16.23	99.0
MR/INTERA-15/1-SMI-71	BCD 15.24	99.0	MR/INTERA-SMI-71	BCD 16.24	99.0
MR/INTERA-15/1-SMI-71	BCD 15.25	99.0	MR/INTERA-SMI-71	BCD 16.25	99.0
MR/INTERA-15/1-SMI-71	BCD 15.26	99.0	MR/INTERA-SMI-71	BCD 16.26	99.0
MR/INTERA-15/1-SMI-71	BCD 15.27	99.0	MR/INTERA-SMI-71	BCD 16.27	99.0
MR/INTERA-15/1-SMI-71	BCD 15.28	99.0	MR/INTERA-SMI-71	BCD 16.28	99.0
MR/INTERA-15/3-SMI-71	BCD 15.1	99.0	MR/INTERA-SMI-71	BCD 16.29	99.0
	(green)		MR/INTERA-SMI-71	BCD 16.30	99.0
MR/INTERA-15/3-SMI-71	BCD 15.2	99.0	MR/INTERA-SMI-71	BCD 16.31	99.0
MR/INTERA-15/3-SMI-71	BCD 15.3	99.0	MR/INTERA-SMI-71	BCD 16.32	99.0
MR/INTERA-15/3-SMI-71	BCD 15.4	99.0	MR/INTERA-SMI-71	BCD 16.33	99.0
MR/INTERA-15/3-SMI-71	BCD 15.5	99.0	MR/INTERA-SMI-71	BCD 16.34	99.0
			MR/INTERA-SMI-71	BCD 16.35	99.0

GYROSCAN Intera

SMI LOPAD

MR/INTERA-SMI-71	BCD 16.36	99.0	MR/INTERA/36-SMI-71	BCD 17.12	99.0
MR/INTERA-SMI-71	BCD 16.37	99.0	MR/INTERA/36-SMI-71	BCD 17.13	99.0
MR/INTERA-SMI-71	BCD 16.38	99.0	MR/INTERA/36-SMI-71	BCD 17.14	99.0
MR/INTERA-SMI-71	BCD 16.39	99.0	MR/INTERA/36-SMI-71	BCD 17.15	99.0
MR/INTERA-SMI-71	BCD 16.40	99.0	MR/INTERA/36-SMI-71	BCD 17.16	99.0
MR/INTERA-SMI-71	BCD 16.41	99.0	MR/INTERA/36-SMI-71	BCD 17.17	99.0
MR/INTERA-SMI-71	BCD 16.42	99.0	MR/INTERA/36-SMI-71	BCD 17.18	99.0
MR/INTERA-SMI-71	BCD 16.43	99.0	MR/INTERA/36-SMI-71	BCD 17.19	99.0
MR/INTERA-SMI-71	BCD 16.44	99.0	MR/INTERA/36-SMI-71	BCD 17.20	99.0
MR/INTERA-SMI-71	BCD 16.45	99.0	MR/INTERA/36-SMI-71	BCD 17.21	99.0
MR/INTERA-SMI-71	BCD 16.46	99.0	MR/INTERA/36-SMI-71	BCD 17.22	99.0
MR/INTERA-SMI-71	BCD 16.47	99.0	MR/INTERA/36-SMI-71	BCD 17.23	99.0
MR/INTERA-SMI-71	BCD 16.48	99.0	MR/INTERA/36-SMI-71	BCD 17.24	99.0
MR/INTERA-SMI-71	BCD 16.49	99.0	MR/INTERA/36-SMI-71	BCD 17.25	99.0
MR/INTERA-SMI-71	BCD 16.50	99.0	MR/INTERA/36-SMI-71	BCD 17.26	99.0
MR/INTERA-SMI-71	BCD 16.51	99.0	MR/INTERA/36-SMI-71	BCD 17.27	99.0
MR/INTERA-SMI-71	BCD 16.52	99.0	MR/INTERA/36-SMI-71	BCD 17.28	99.0
MR/INTERA-SMI-71	BCD 16.53	99.0	MR/INTERA/36-SMI-71	BCD 17.29	99.0
MR/INTERA-SMI-71	BCD 16.54	99.0	MR/INTERA/36-SMI-71	BCD 17.30	99.0
MR/INTERA-SMI-71	BCD 16.55	99.0	MR/INTERA/36-SMI-71	BCD 17.31	99.0
MR/INTERA-SMI-71	BCD 16.56	99.0	MR/INTERA/36-SMI-71	BCD 17.32	99.0
			MR/INTERA/36-SMI-71	BCD 17.33	99.0
MR/INTERA/1-SMI-71	BCD 17.1	99.0	MR/INTERA/36-SMI-71	BCD 17.34	99.0
MR/INTERA/1-SMI-71	BCD 17.2	99.0	MR/INTERA/36-SMI-71	BCD 17.35	99.0
MR/INTERA/1-SMI-71	BCD 17.3	99.0	MR/INTERA/36-SMI-71	BCD 17.36	99.0
MR/INTERA/1-SMI-71	BCD 17.4	99.0	MR/INTERA/36-SMI-71	BCD 17.37	99.0
MR/INTERA/1-SMI-71	BCD 17.5	99.0	MR/INTERA/36-SMI-71	BCD 17.38	99.0
MR/INTERA/1-SMI-71	BCD 17.6	99.0	MR/INTERA/36-SMI-71	BCD 17.39	99.0
MR/INTERA/1-SMI-71	BCD 17.7	99.0	MR/INTERA/36-SMI-71	BCD 17.40	99.0
MR/INTERA/1-SMI-71	BCD 17.8	99.0	MR/INTERA/36-SMI-71	BCD 17.41	99.0
MR/INTERA/1-SMI-71	BCD 17.9	99.0	MR/INTERA/36-SMI-71	BCD 17.42	99.0
MR/INTERA/1-SMI-71	BCD 17.10	99.0	MR/INTERA/36-SMI-71	BCD 17.43	99.0
MR/INTERA/1-SMI-71	BCD 17.11	99.0	MR/INTERA/36-SMI-71	BCD 17.44	99.0
MR/INTERA/1-SMI-71	BCD 17.12	99.0	MR/INTERA/36-SMI-71	BCD 17.45	99.0
MR/INTERA/1-SMI-71	BCD 17.13	99.0	MR/INTERA/36-SMI-71	BCD 17.46	99.0
MR/INTERA/1-SMI-71	BCD 17.14	99.0	MR/INTERA/36-SMI-71	BCD 17.47	99.0
MR/INTERA/1-SMI-71	BCD 17.15	99.0	MR/INTERA/36-SMI-71	BCD 17.48	99.0
MR/INTERA/1-SMI-71	BCD 17.16	99.0	MR/INTERA/36-SMI-71	BCD 17.49	99.0
MR/INTERA/1-SMI-71	BCD 17.17	99.0	MR/INTERA/36-SMI-71	BCD 17.50	99.0
MR/INTERA/1-SMI-71	BCD 17.18	99.0	MR/INTERA/36-SMI-71	BCD 17.51	99.0
MR/INTERA/1-SMI-71	BCD 17.19	99.0			
MR/INTERA/1-SMI-71	BCD 17.20	99.0	MR/INTERA-SMI-71	BCD 18.1	99.0
MR/INTERA/1-SMI-71	BCD 17.21	99.0	MR/INTERA-SMI-71	BCD 18.2	99.0
MR/INTERA/1-SMI-71	BCD 17.22	99.0	MR/INTERA-SMI-71	BCD 18.3	99.0
MR/INTERA/1-SMI-71	BCD 17.23	99.0	MR/INTERA-SMI-71	BCD 18.4	99.0
			MR/INTERA-SMI-71	BCD 18.5	99.0
MR/INTERA/36-SMI-71	BCD 17.1	99.0	MR/INTERA-SMI-71	BCD 18.6	99.0
	(green)		MR/INTERA-SMI-71	BCD 18.7	99.0
MR/INTERA/36-SMI-71	BCD 17.2	99.0	MR/INTERA-SMI-71	BCD 18.8	99.0
MR/INTERA/36-SMI-71	BCD 17.3	99.0	MR/INTERA-SMI-71	BCD 18.9	99.0
MR/INTERA/36-SMI-71	BCD 17.4	99.0	MR/INTERA-SMI-71	BCD 18.10	99.0
MR/INTERA/36-SMI-71	BCD 17.5	99.0	MR/INTERA-SMI-71	BCD 18.11	99.0
MR/INTERA/36-SMI-71	BCD 17.6	99.0	MR/INTERA-SMI-71	BCD 18.12	99.0
MR/INTERA/36-SMI-71	BCD 17.7	99.0	MR/INTERA-SMI-71	BCD 18.13	99.0
MR/INTERA/36-SMI-71	BCD 17.8	99.0	MR/INTERA-SMI-71	BCD 18.14	99.0
MR/INTERA/36-SMI-71	BCD 17.9	99.0			
MR/INTERA/36-SMI-71	BCD 17.10	99.0	MR/INTERA-SMI-71	BCD 19.1	99.0
MR/INTERA/36-SMI-71	BCD 17.11	99.0	MR/INTERA-SMI-71	BCD 19.2	99.0

GYROSCAN Intera

SMI LOPAD

MR/INTERA-SMI-71	BCD 19.3	99.0	MR/INTERA-SMI-71	BCD 21.8.7	99.0
MR/INTERA-SMI-71	BCD 19.4	99.0	MR/INTERA-SMI-71	BCD 21.8.8	99.0
			MR/INTERA-SMI-71	BCD 21.8.9	99.0
MR/INTERA-SMI-71	BCD 20.1	99.0	MR/INTERA-SMI-71	BCD 21.8.10	99.0
MR/INTERA-SMI-71	BCD 20.2	99.0	MR/INTERA-SMI-71	BCD 21.8.11	99.0
MR/INTERA-SMI-71	BCD 20.3	99.0	MR/INTERA-SMI-71	BCD 21.8.12	99.0
MR/INTERA-SMI-71	BCD 20.4	99.0	MR/INTERA-SMI-71	BCD 21.8.13	99.0
MR/INTERA-SMI-71	BCD 20.5	99.0			
MR/INTERA-SMI-71	BCD 20.6	99.0	MR/INTERA-SMI-71	BCD 21.11.1	99.0
MR/INTERA-SMI-71	BCD 20.7	99.0		(green)	
MR/INTERA-SMI-71	BCD 20.8	99.0	MR/INTERA-SMI-71	BCD 21.11.2	99.0
MR/INTERA-SMI-71	BCD 20.9	99.0	MR/INTERA-SMI-71	BCD 21.11.3	99.0
MR/INTERA-SMI-71	BCD 20.10	99.0	MR/INTERA-SMI-71	BCD 21.11.4	99.0
MR/INTERA-SMI-71	BCD 20.11	99.0	MR/INTERA-SMI-71	BCD 21.11.5	99.0
MR/INTERA-SMI-71	BCD 20.12	99.0			
MR/INTERA-SMI-71	BCD 20.13	99.0	MR/INTERA-SMI-71	BCD 21.12.1	99.0
MR/INTERA-SMI-71	BCD 20.14	99.0		(green)	
MR/INTERA-SMI-71	BCD 20.15	99.0	MR/INTERA-SMI-71	BCD 21.12.2	99.0
MR/INTERA-SMI-71	BCD 20.16	99.0	MR/INTERA-SMI-71	BCD 21.12.3	99.0
			MR/INTERA-SMI-71	BCD 21.12.4	99.0
MR/INTERA-SMI-71	BCD 21.1.1	99.0	MR/INTERA-SMI-71	BCD 21.12.5	99.0
			MR/INTERA-SMI-71	BCD 21.12.6	99.0
MR/INTERA-SMI-71	BCD 21.2.1	99.0	MR/INTERA-SMI-71	BCD 21.12.7	99.0
	(green)		MR/INTERA-SMI-71	BCD 21.12.8	99.0
MR/INTERA-SMI-71	BCD 21.2.2	99.0	MR/INTERA-SMI-71	BCD 21.12.9	99.0
MR/INTERA-SMI-71	BCD 21.2.3	99.0	MR/INTERA-SMI-71	BCD 21.12.10	99.0
MR/INTERA-SMI-71	BCD 21.2.4	99.0	MR/INTERA-SMI-71	BCD 21.12.11	99.0
MR/INTERA-SMI-71	BCD 21.2.5	99.0	MR/INTERA-SMI-71	BCD 21.12.12	99.0
MR/INTERA-SMI-71	BCD 21.2.6	99.0	MR/INTERA-SMI-71	BCD 21.12.13	99.0
MR/INTERA-SMI-71	BCD 21.2.7	99.0	MR/INTERA-SMI-71	BCD 21.12.14	99.0
MR/INTERA-SMI-71	BCD 21.2.8	99.0	MR/INTERA-SMI-71	BCD 21.12.15	99.0
MR/INTERA-SMI-71	BCD 21.2.9	99.0	MR/INTERA-SMI-71	BCD 21.12.16	99.0
MR/INTERA-SMI-71	BCD 21.2.10	99.0	MR/INTERA-SMI-71	BCD 21.12.17	99.0
MR/INTERA-SMI-71	BCD 21.2.11	99.0	MR/INTERA-SMI-71	BCD 21.12.18	99.0
MR/INTERA-SMI-71	BCD 21.2.12	99.0	MR/INTERA-SMI-71	BCD 21.12.19	99.0
MR/INTERA-SMI-71	BCD 21.2.13	99.0	MR/INTERA-SMI-71	BCD 21.12.20	99.0
MR/INTERA-SMI-71	BCD 21.2.14	99.0	MR/INTERA-SMI-71	BCD 21.12.21	99.0
			MR/INTERA-SMI-71	BCD 21.12.22	99.0
MR/INTERA-SMI-71	BCD 21.4.1	99.0	MR/INTERA-SMI-71	BCD 21.12.23	99.0
	(green)		MR/INTERA-SMI-71	BCD 21.12.24	99.0
MR/INTERA-SMI-71	BCD 21.4.2	99.0	MR/INTERA-SMI-71	BCD 21.12.25	99.0
MR/INTERA-SMI-71	BCD 21.4.3	99.0	MR/INTERA-SMI-71	BCD 21.12.26	99.0
MR/INTERA-SMI-71	BCD 21.4.4	99.0	MR/INTERA-SMI-71	BCD 21.12.27	99.0
MR/INTERA-SMI-71	BCD 21.4.5	99.0	MR/INTERA-SMI-71	BCD 21.12.28	99.0
MR/INTERA-SMI-71	BCD 21.4.6	99.0	MR/INTERA-SMI-71	BCD 21.12.29	99.0
MR/INTERA-SMI-71	BCD 21.4.7	99.0	MR/INTERA-SMI-71	BCD 21.12.30	99.0
MR/INTERA-SMI-71	BCD 21.4.8	99.0	MR/INTERA-SMI-71	BCD 21.12.31	99.0
MR/INTERA-SMI-71	BCD 21.4.9	99.0	MR/INTERA-SMI-71	BCD 21.12.32	99.0
MR/INTERA-SMI-71	BCD 21.4.10	99.0	MR/INTERA-SMI-71	BCD 21.12.33	99.0
MR/INTERA-SMI-71	BCD 21.4.11	99.0	MR/INTERA-SMI-71	BCD 21.12.34	99.0
MR/INTERA-SMI-71	BCD 21.4.12	99.0	MR/INTERA-SMI-71	BCD 21.12.35	99.0
			MR/INTERA-SMI-71	BCD 21.12.36	99.0
MR/INTERA-SMI-71	BCD 21.8.1	99.0			
	(green)		MR/INTERA-SMI-71	BCD 21.13.1	99.0
MR/INTERA-SMI-71	BCD 21.8.2	99.0		(green)	
MR/INTERA-SMI-71	BCD 21.8.3	99.0	MR/INTERA-SMI-71	BCD 21.13.2	99.0
MR/INTERA-SMI-71	BCD 21.8.4	99.0	MR/INTERA-SMI-71	BCD 21.13.3	99.0
MR/INTERA-SMI-71	BCD 21.8.5	99.0	MR/INTERA-SMI-71	BCD 21.13.4	99.0
MR/INTERA-SMI-71	BCD 21.8.6	99.0	MR/INTERA-SMI-71	BCD 21.13.5	99.0

MR/INTERA-SMI-71	BCD 21 13.6	99.0
MR/INTERA-SMI-71	BCD 22.1	99.0
MR/INTERA-SMI-71	BCD 22.2	99.0
MR/INTERA-SMI-71	BCD 22.3	99.0
MR/INTERA-SMI-71	BCD 22.4	99.0
MR/INTERA-SMI-71	BCD 22.5	99.0
MR/INTERA-SMI-71	BCD 22.6	99.0
MR/INTERA-SMI-71	BCD 22.7	99.0
MR/INTERA-SMI-71	BCD 22.8	99.0
MR/INTERA-SMI-71	BCD 22.9	99.0
MR/INTERA-SMI-71	BCD 22.10	99.0
MR/INTERA-SMI-71	BCD 22.11	99.0
MR/INTERA-SMI-71	BCD 22.12	99.0
MR/INTERA-SMI-71	BCD 22.13	99.0
MR/INTERA-SMI-71	BCD 22.14	99.0
MR/INTERA-SMI-71	BCD 22.15	99.0
MR/INTERA-SMI-71	BCD 22.16	99.0
MR/INTERA-SMI-71	BCD 22.17	99.0
MR/INTERA-SMI-71	BCD 22.18	99.0