



Regression modality and module ablation


(a) FMA-UE

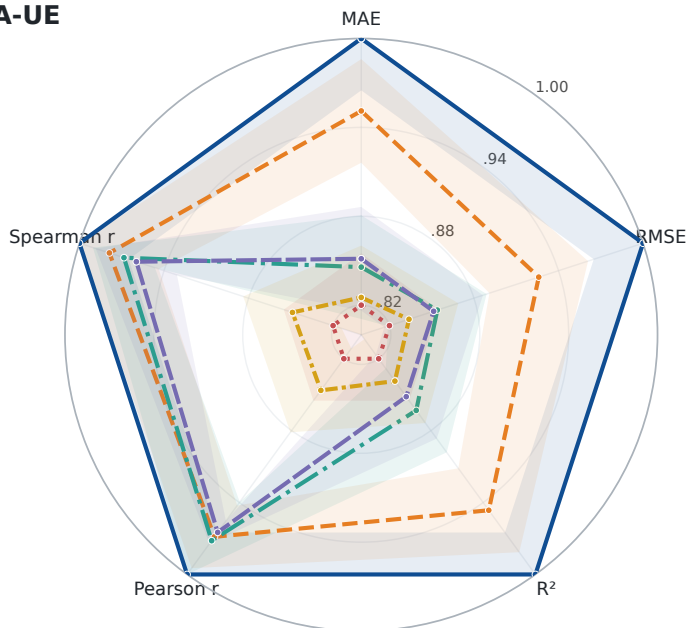


(b) BI

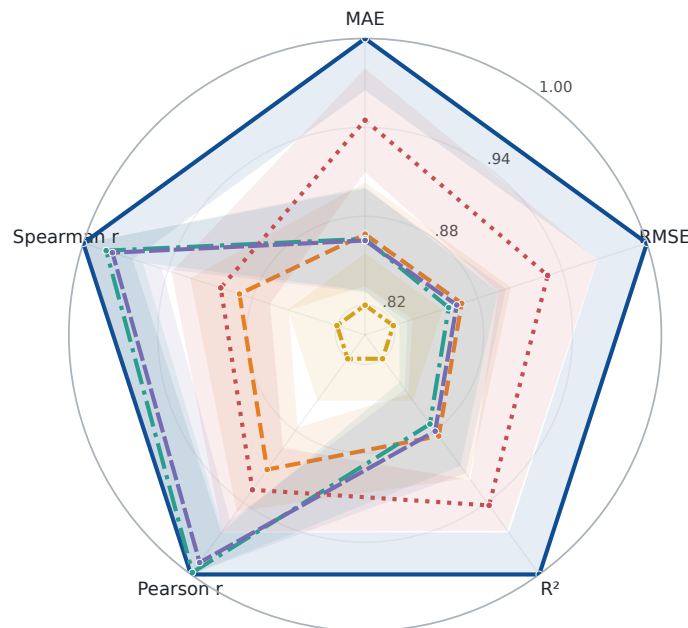

(c) FMA-UE

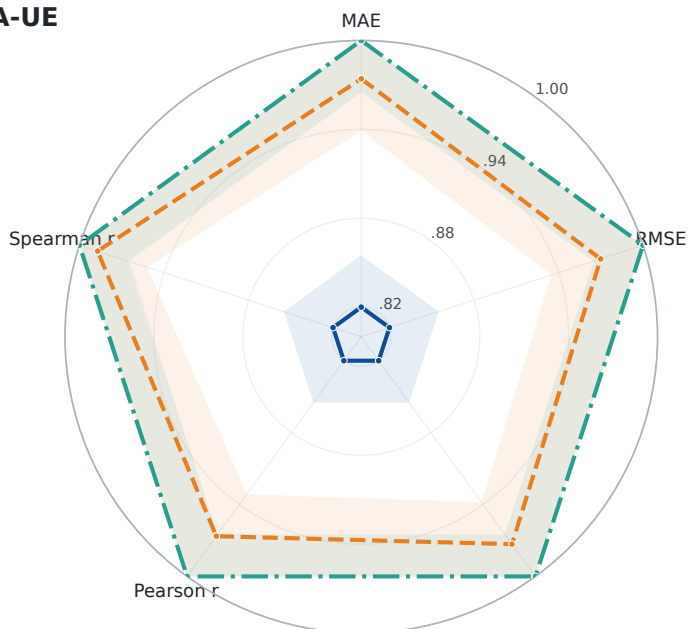

(d) BI

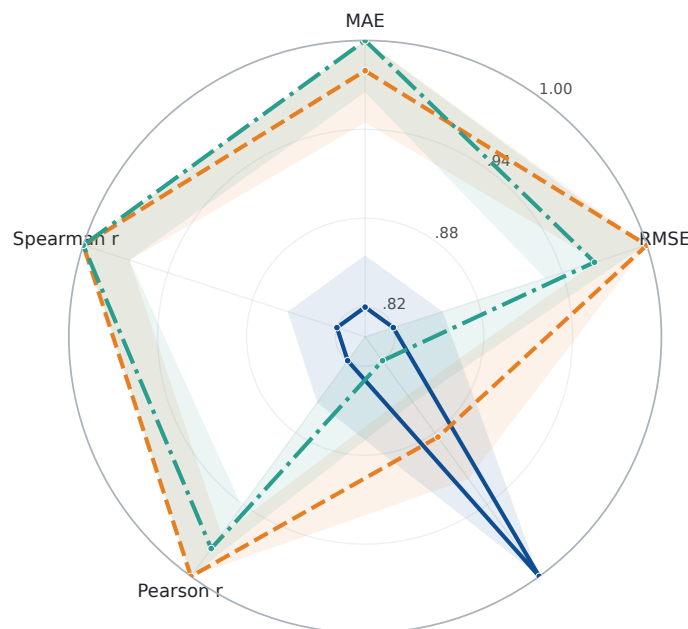

Sensor configurations

- EEG + EMG
- EMG + IMU
- EMG only
- EEG + IMU
- EEG only
- IMU only

Module ablations

- w/o MDFAN
- w/o TriAlign
- w/o W-DTW