



Ordinal-task modality and module ablation


(a) Hand tone

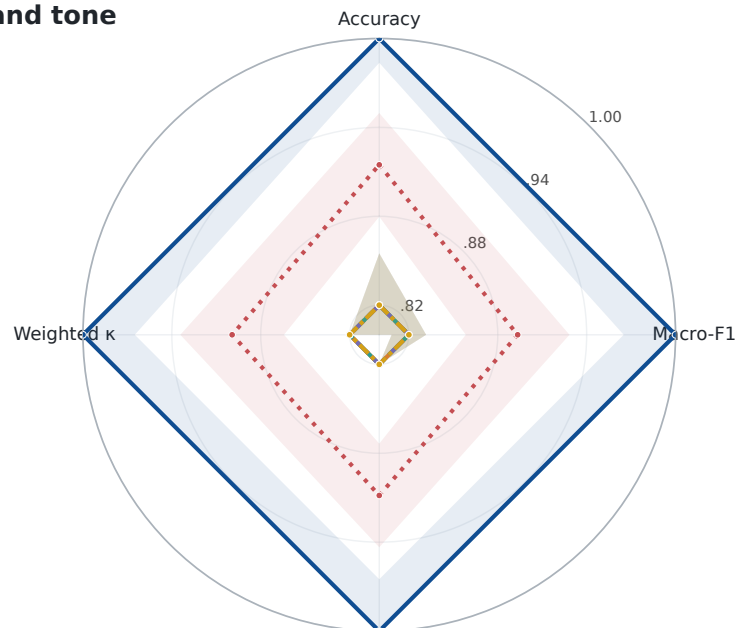


(b) Brunnstrom

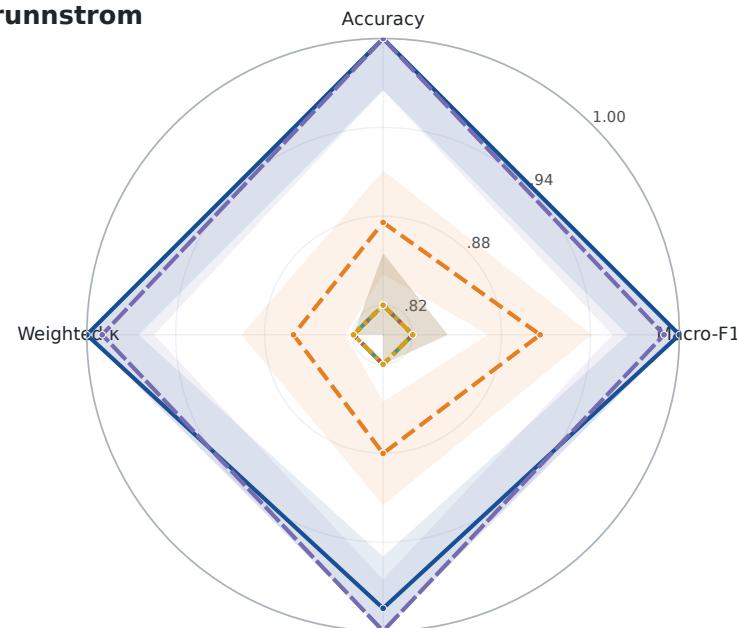

(c) Hand tone

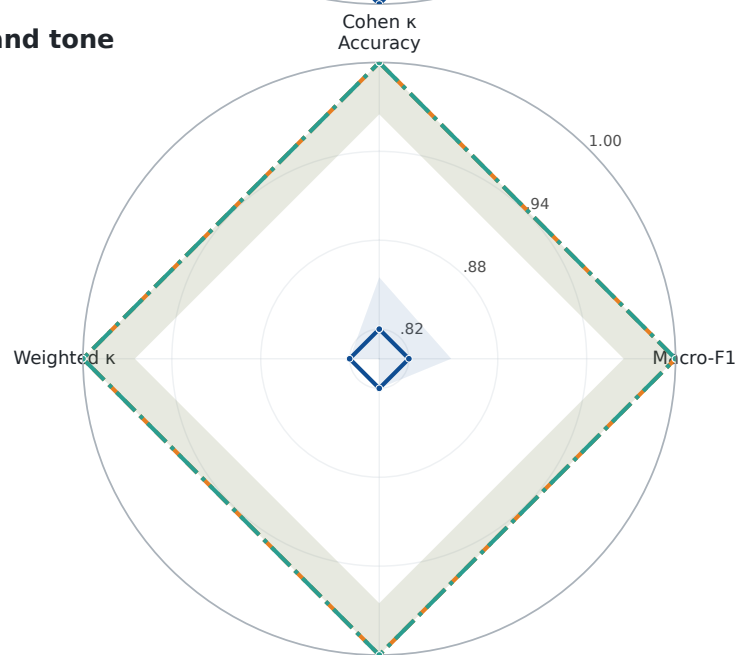

(d) Brunnstrom

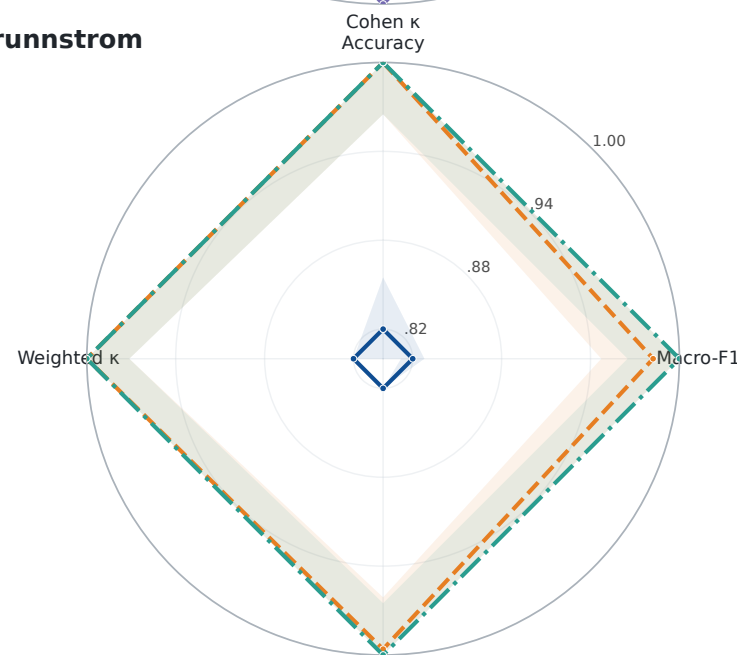

Sensor configurations

- EEG + EMG
- EEG + IMU
- EEG only
- EMG + IMU
- IMU only
- EMG only

Module ablations

- w/o MDFAN
- w/o TriAlign
- w/o W-DTW