

# Protocol of RF Detector Calibration

IAP RAS

September 25, 2025

## 1 Measurement equipment

1. Microwave generator: Rigol DSG830
2. Spectrum analyzer: Rigol RSA5065N
3. Oscilloscope: Tektronix MD034

## 2 Parameters

Parameters from DetCal application settings file.

RF frequencies	1000 to 3000 MHz [3]
RF levels	-5.0 to 14.0 dBm [21]
SPAN wide	2000 kHz
SPAN narrow	100 kHz
RBW wide	10 kHz
RBW narrow	1 kHz
VBW wide	10 kHz
VBW narrow	1 kHz
REF level	10.0 dBm
SWEEP points	1001
SWEEP time	AUTO ON
Precise	True
HOR scale	10 ms/div
High res	True
Impedance 50Ohm	True
Coupling DC	True
Channel	4
Recalc atten	True

Table 1: Measurement parameters

### 3 Results

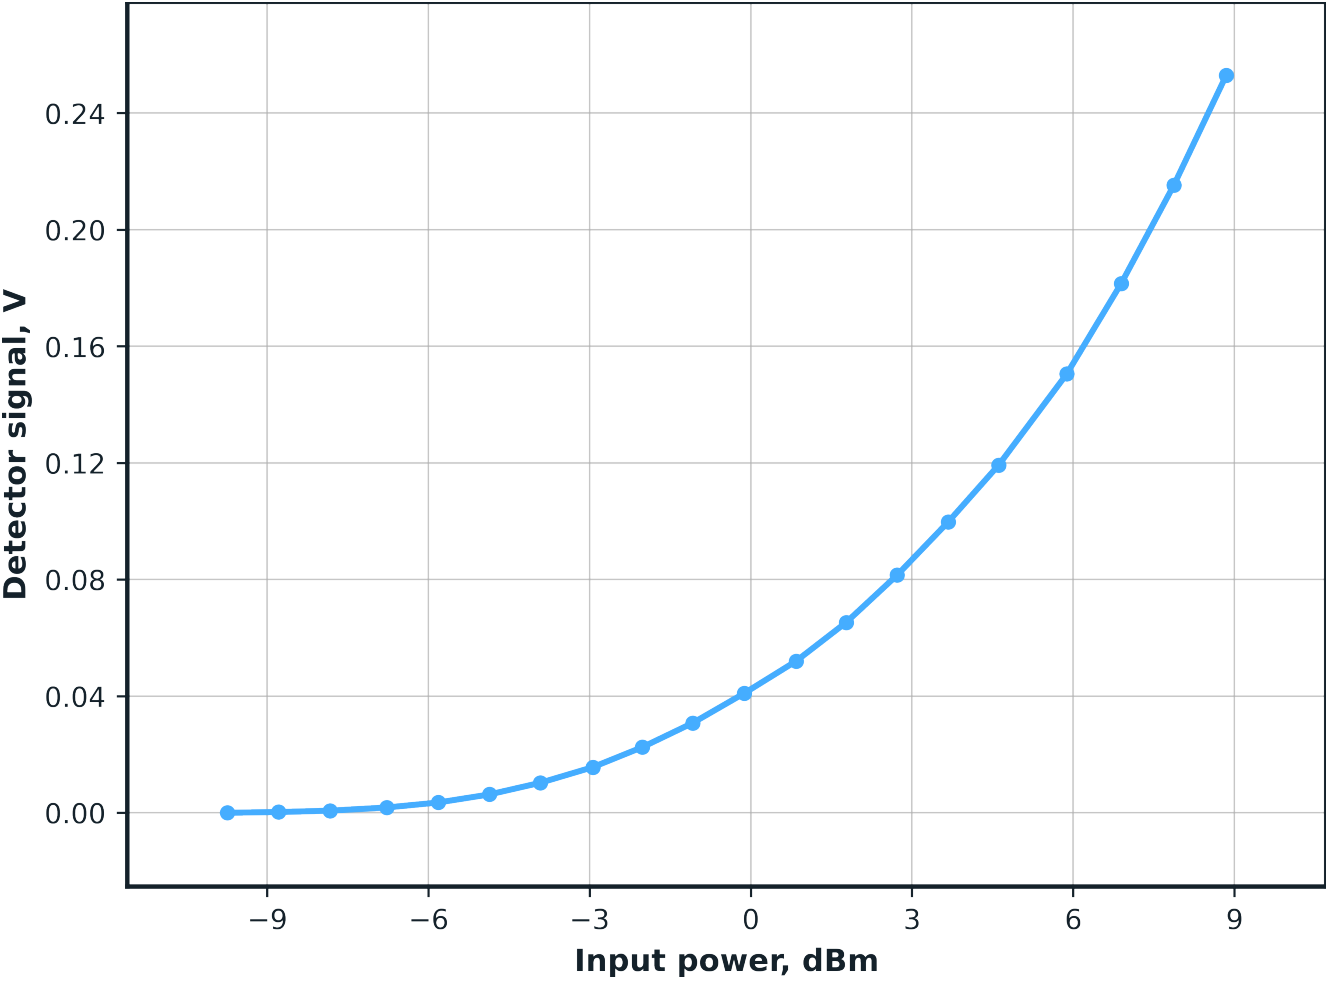


Figure 1: Detector response at 3000 MHz