


Step 1c:
DC logic supply
(10 V DC, 200 mA limit)

Step 2:
DC power supply
(Corresponds to TX power input, 1A limit)

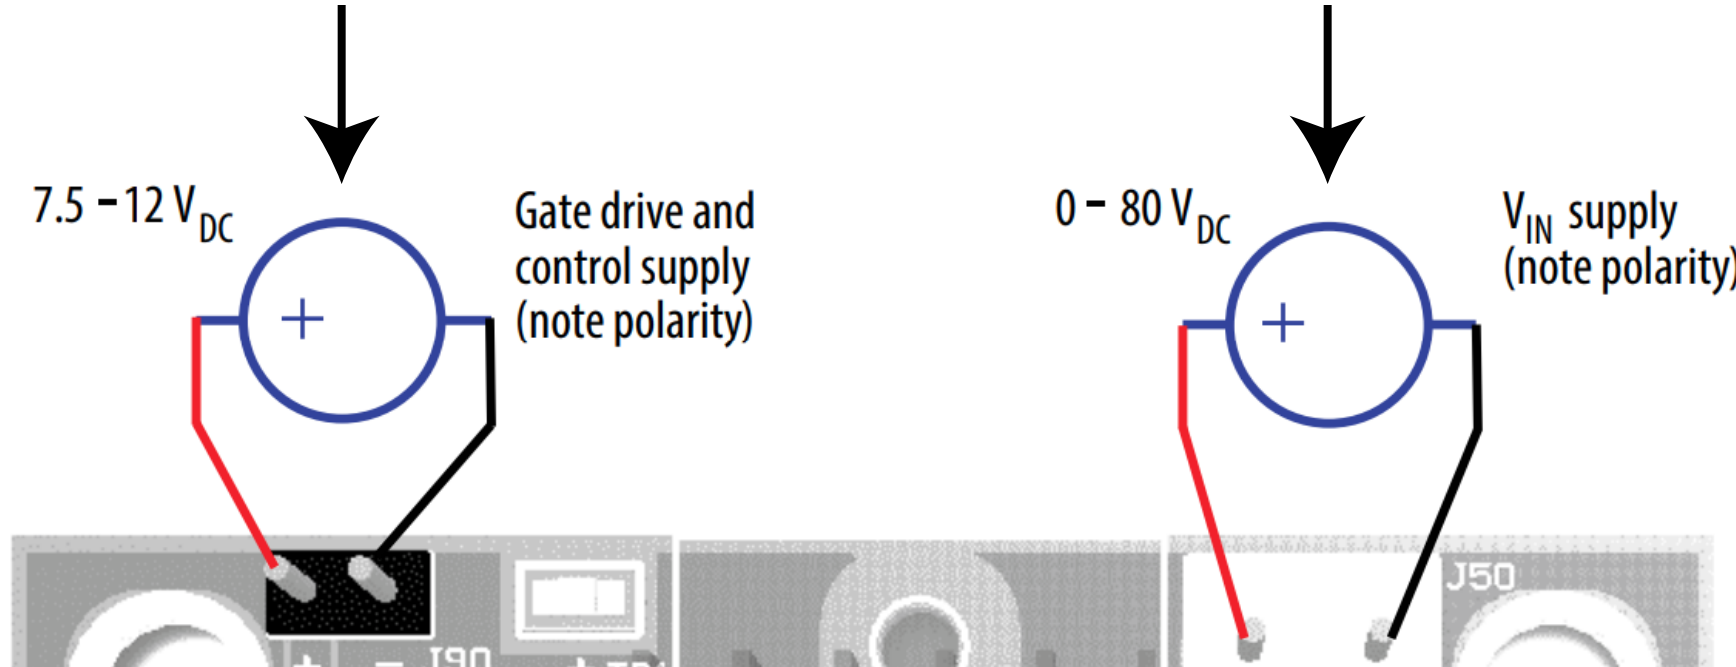


Step 1b:
Input clock signal with signal generator
(5Vpp, square wave, low = 0V)

Amplifier
timing setting
(not installed)

External
oscillator
input
(optional)

Step 1a:
Disable oscillator with jumper
(Data sheet figure is incorrect)

Disable
pre-regulator
jumper

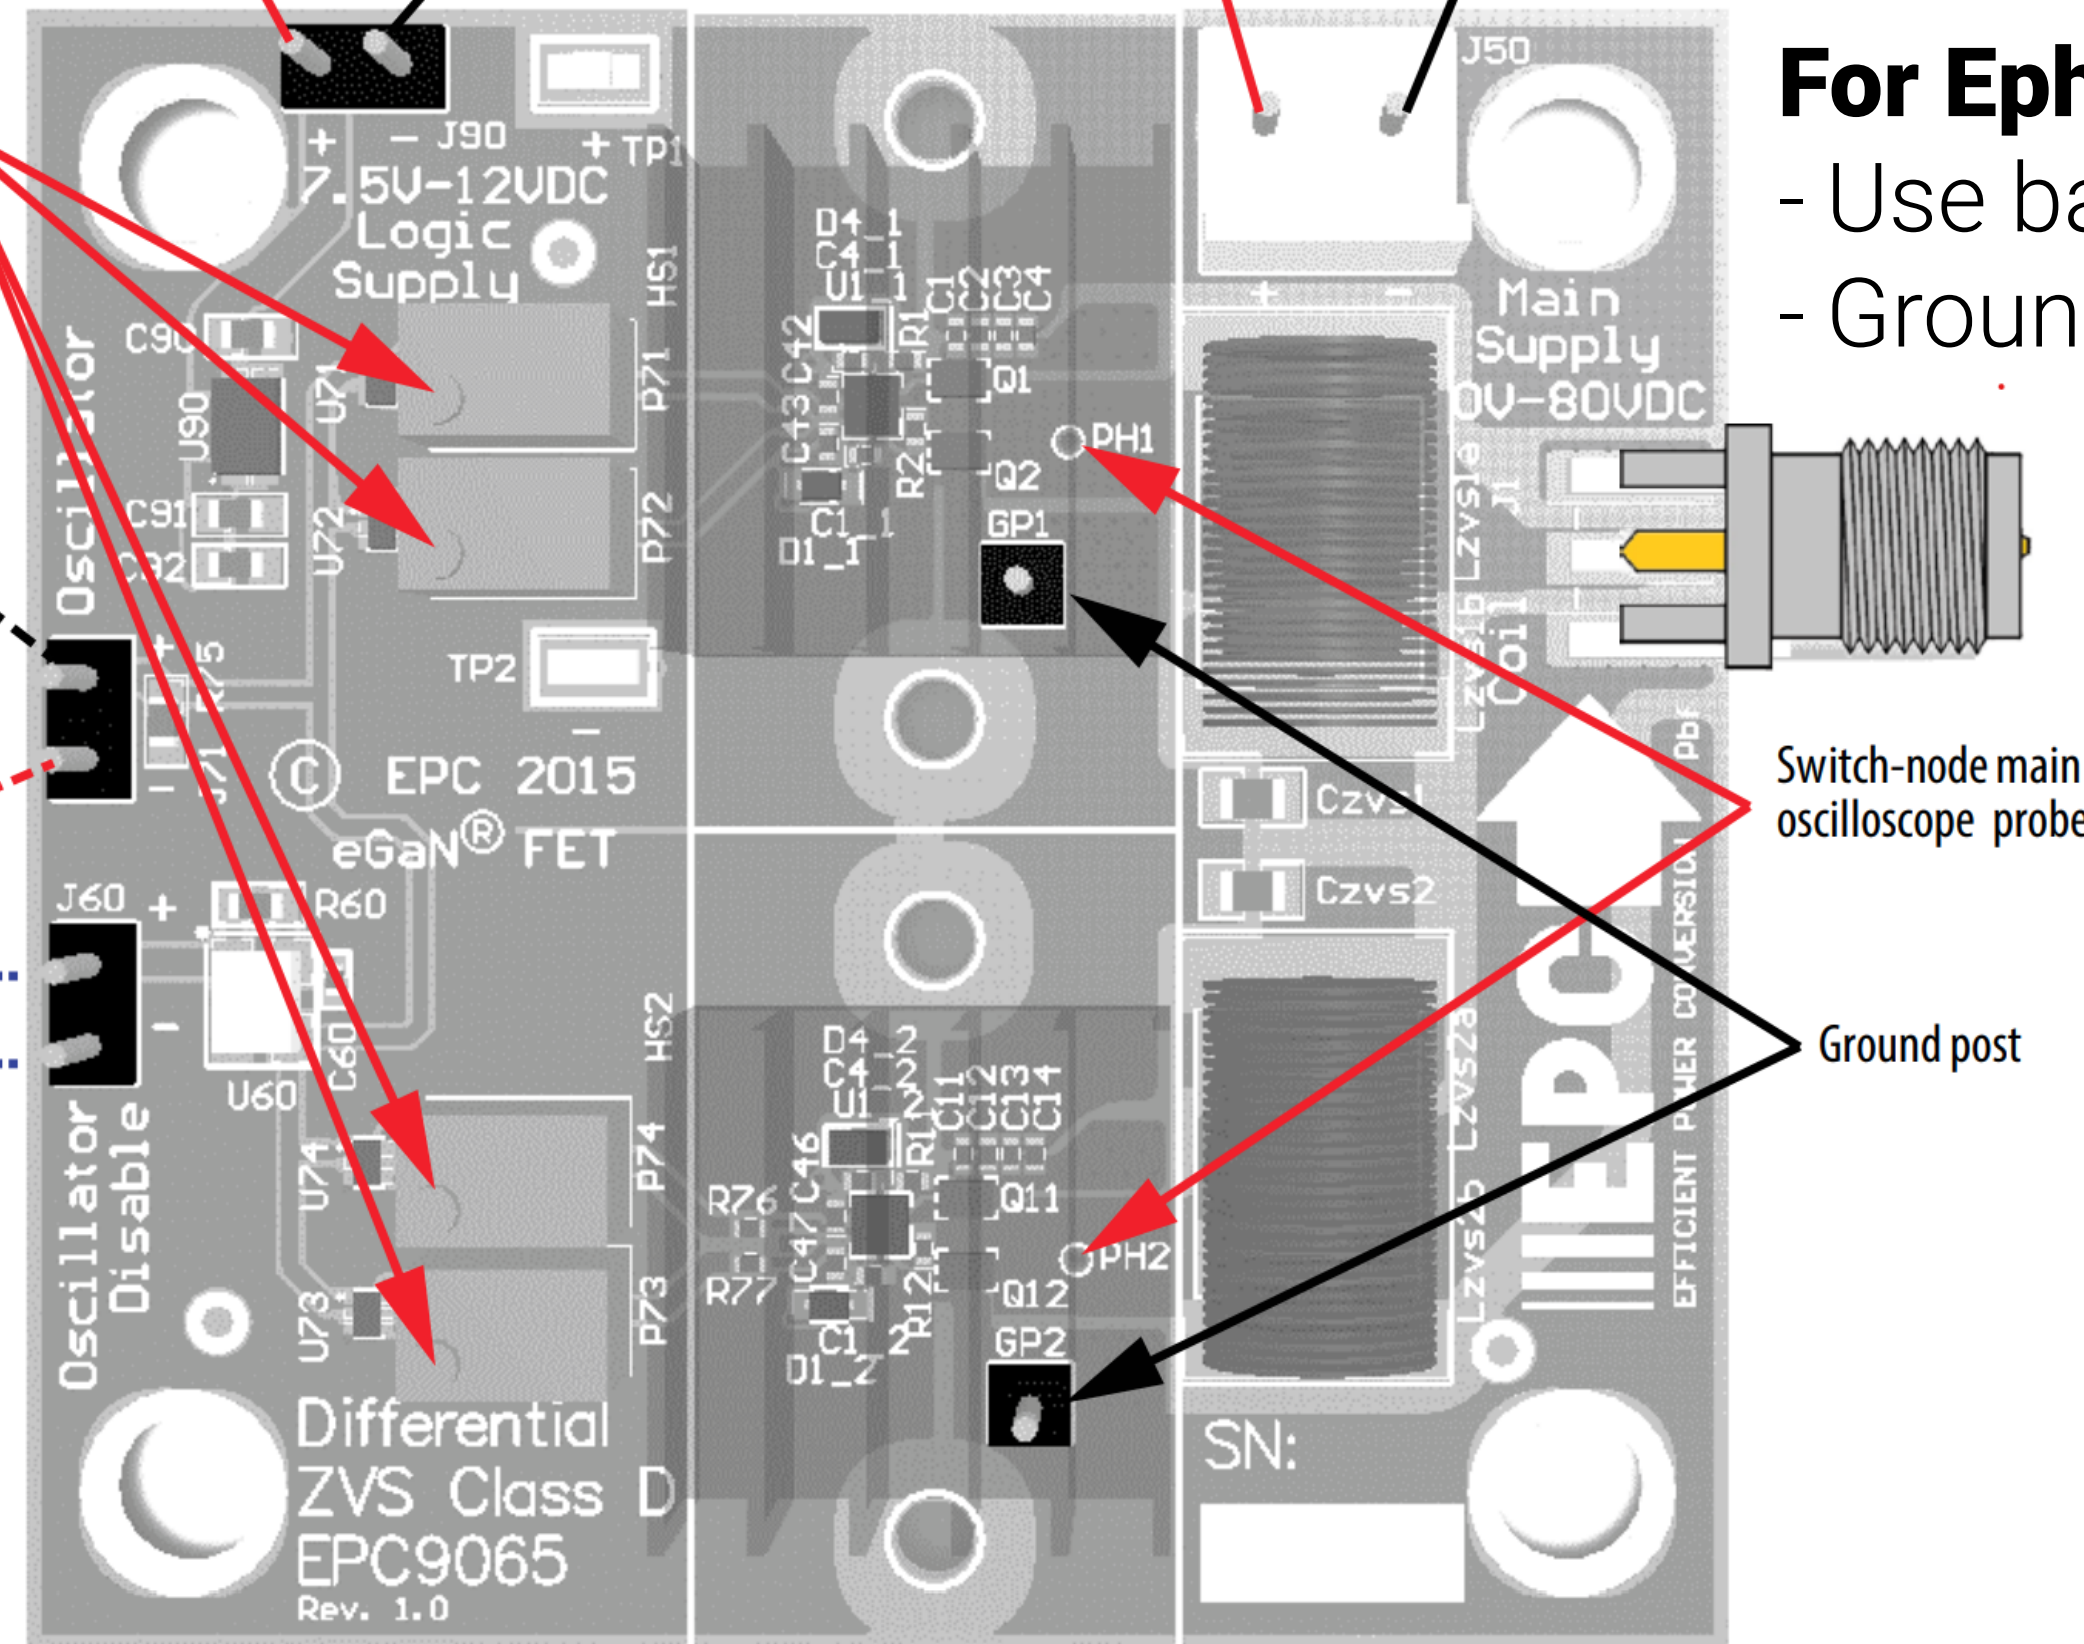

For Ephys (tentative)

- Use battery source for DC supply
- Ground the output coaxial GND

Warning:
SMA connector GND does not match Circuit GND