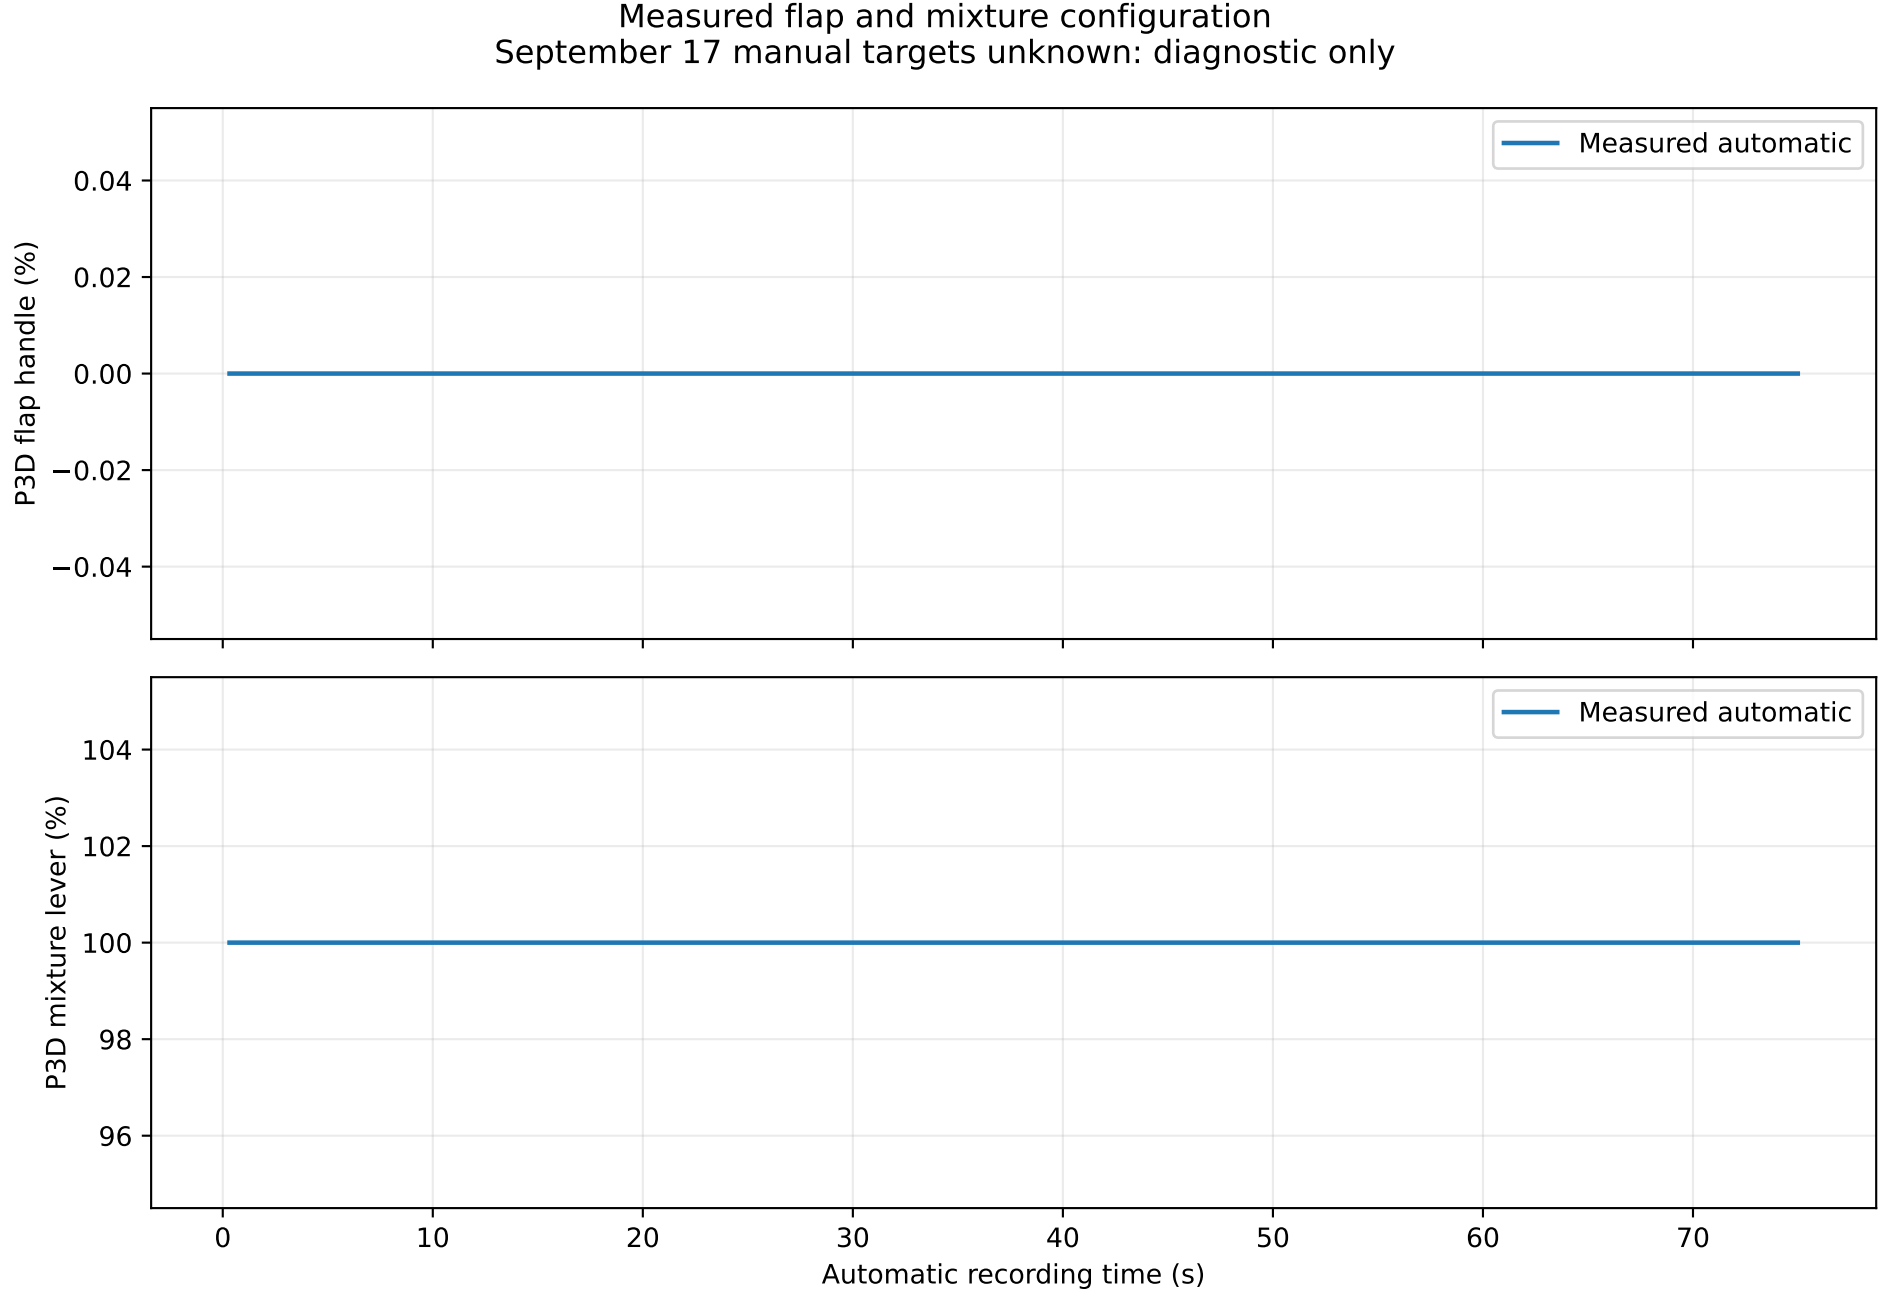
Measured flap and mixture configuration
September 17 manual targets unknown: diagnostic only
Measured automatic
P3D flap handle (%)
0.04
0.02
0.00
−0.02
−0.04
Measured automatic
P3D mixture lever (%)
104
102
100
98
96
0
10
20
30
40
50
60
70
Automatic recording time (s)