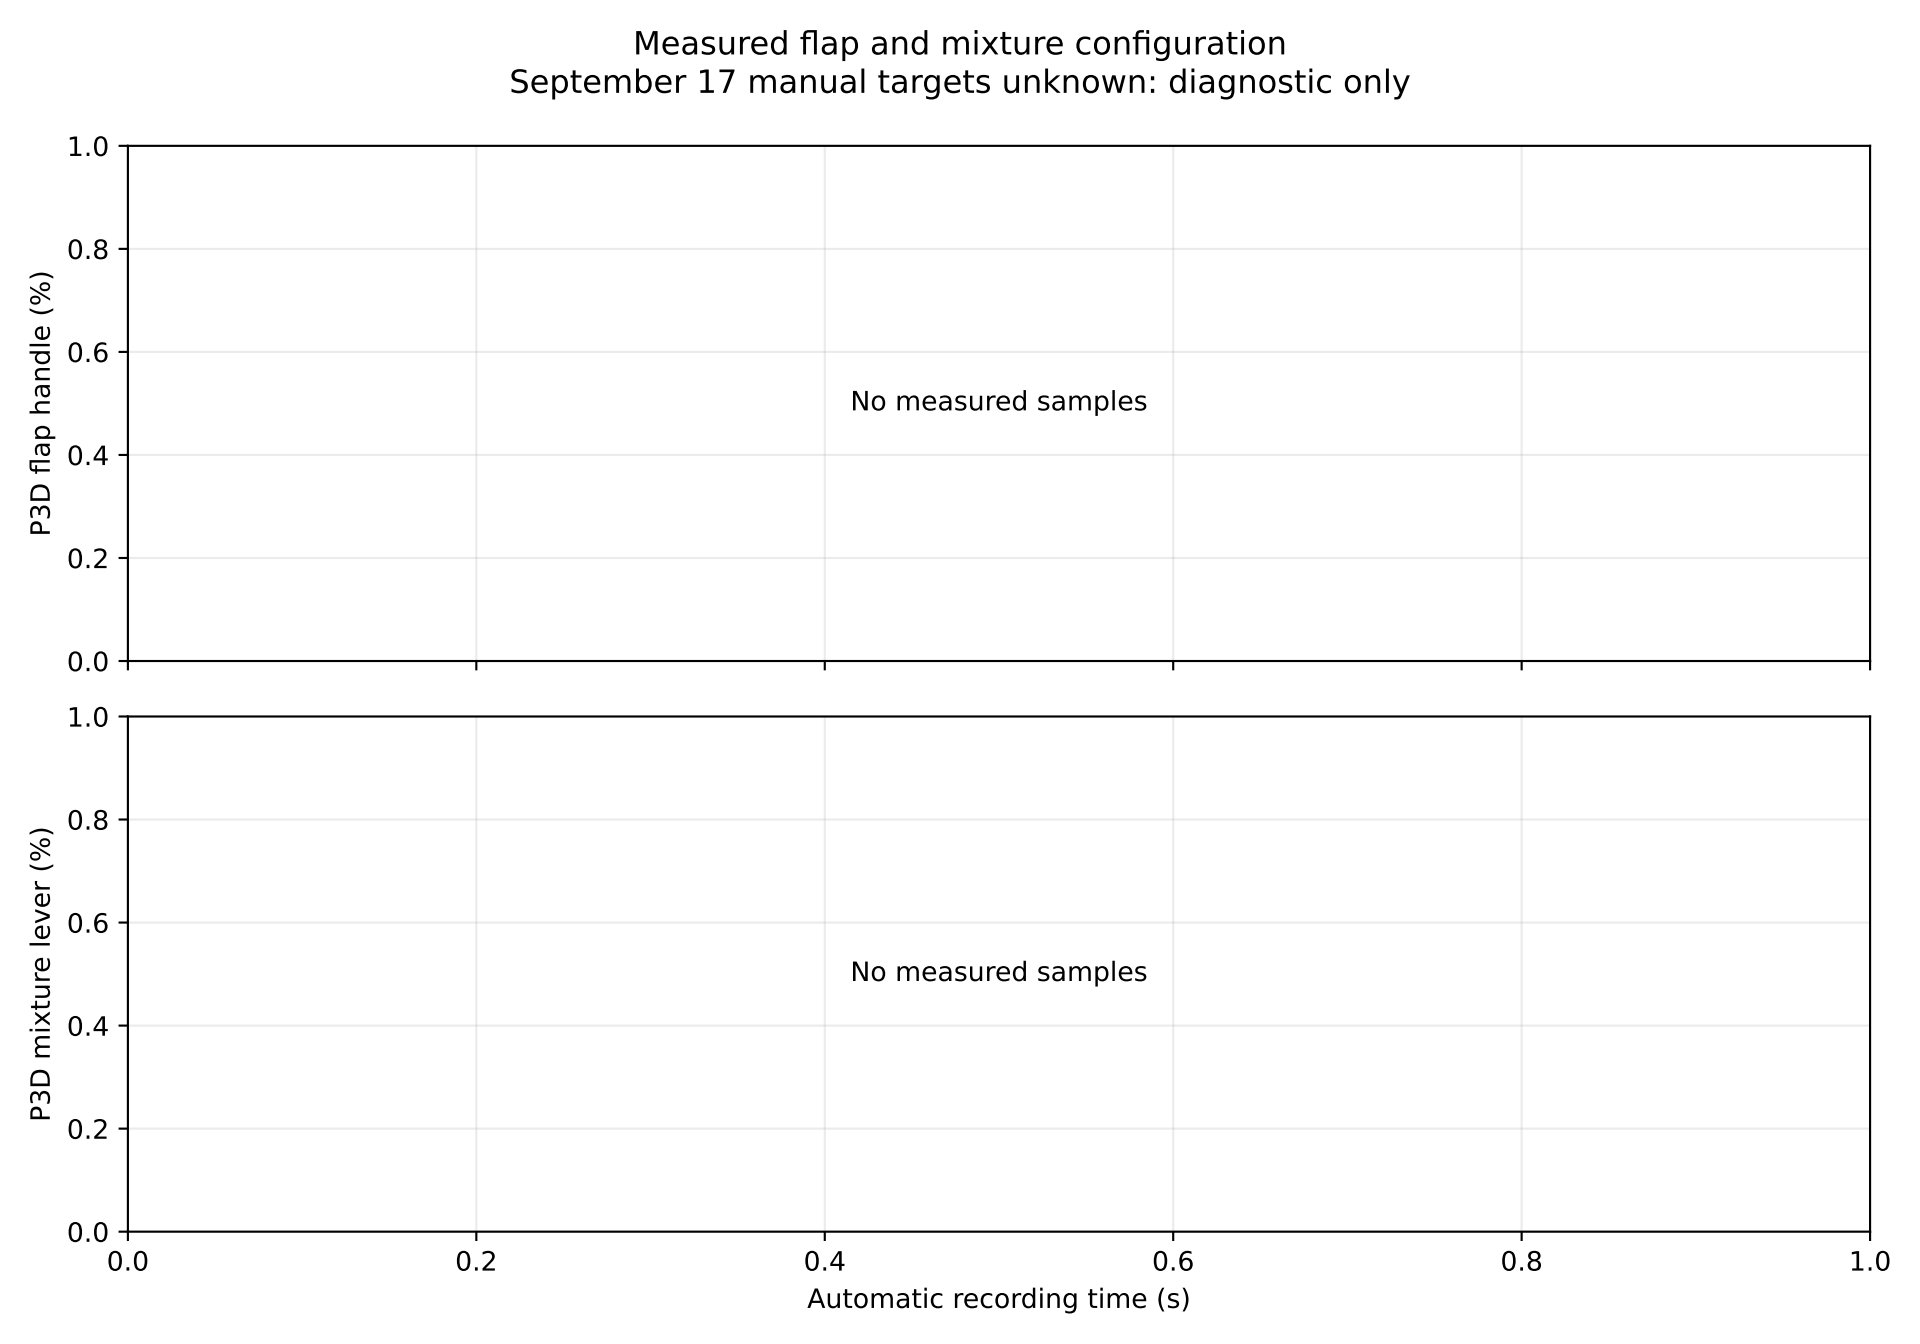
Measured flap and mixture configuration
September 17 manual targets unknown: diagnostic only
P3D flap handle (%)
No measured samples
P3D mixture lever (%)
No measured samples
Automatic recording time (s)
0.0
0.2
0.4
0.6
0.8
1.0