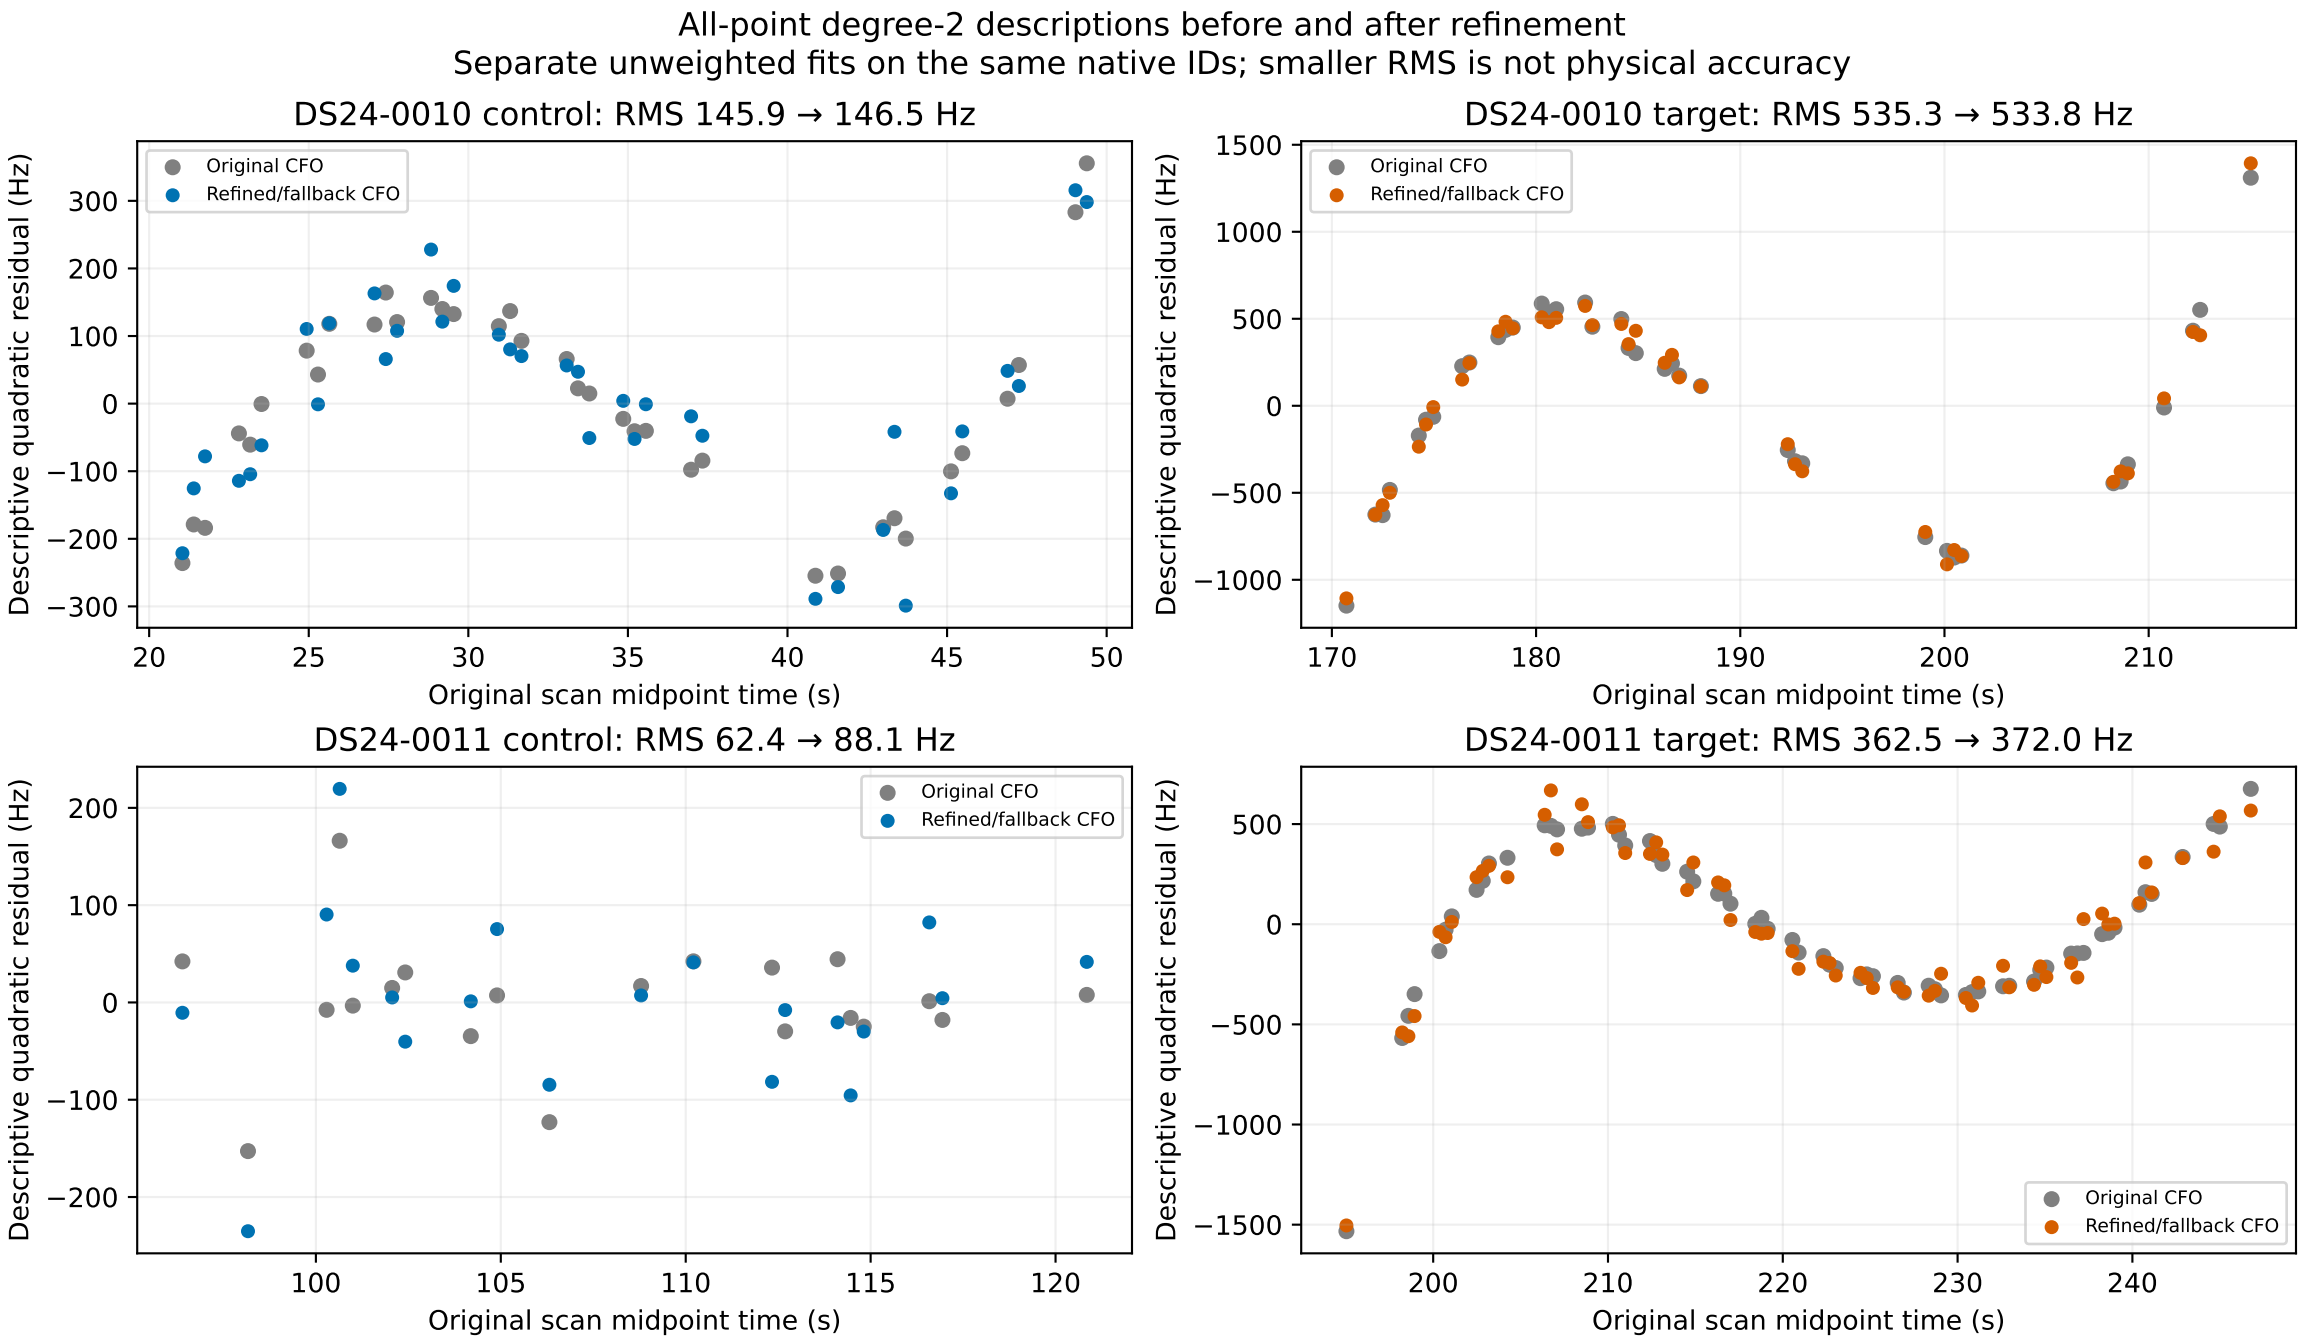
All-point degree-2 descriptions before and after refinement
Separate unweighted fits on the same native IDs; smaller RMS is not physical accuracy
DS24-0010 control: RMS 145.9 → 146.5 Hz
DS24-0010 target: RMS 535.3 → 533.8 Hz
DS24-0011 control: RMS 62.4 → 88.1 Hz
DS24-0011 target: RMS 362.5 → 372.0 Hz
Original CFO
Refined/fallback CFO
Descriptive quadratic residual (Hz)
Original scan midpoint time (s)