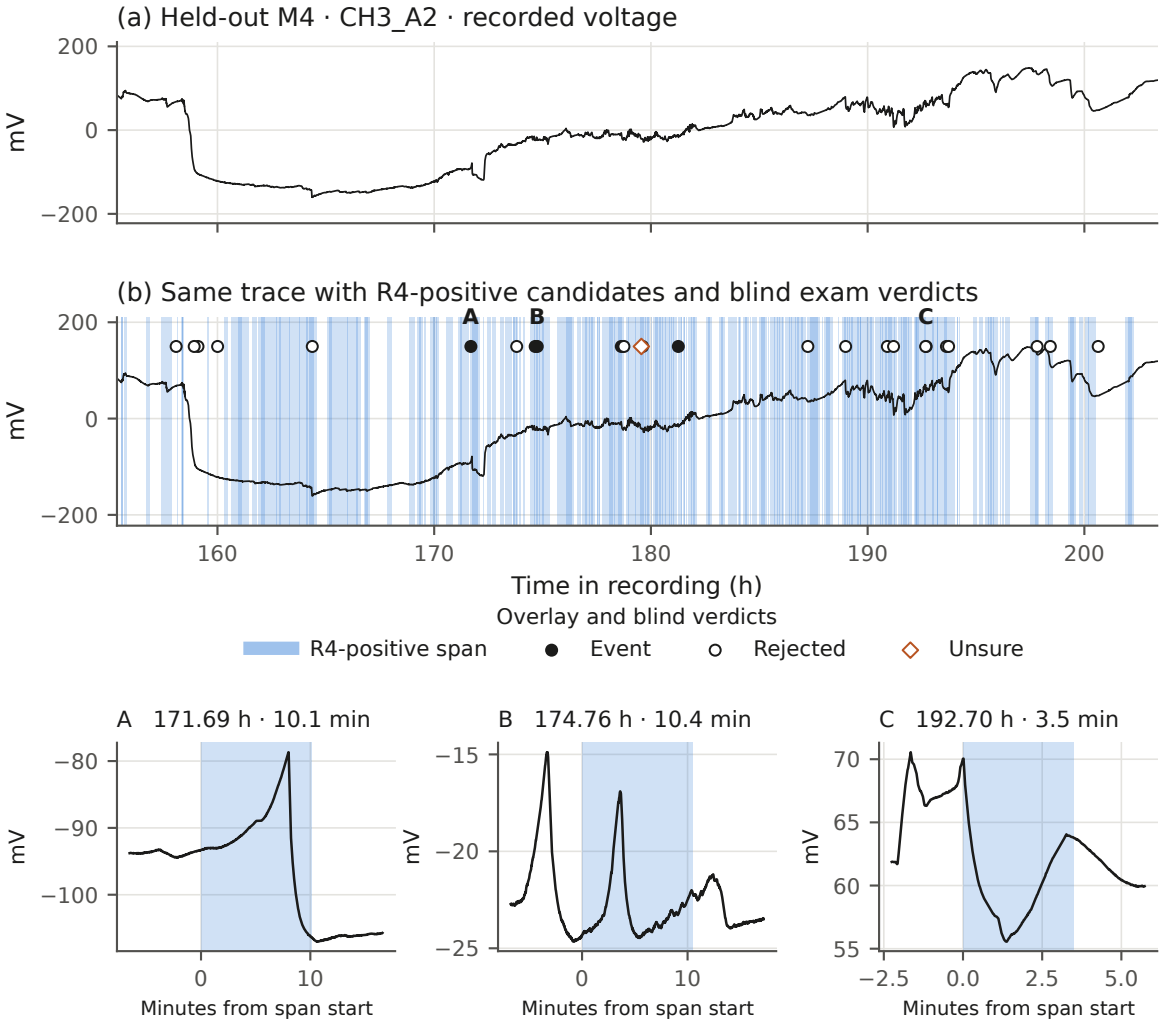

(a) Held-out M4 · CH3_A2 · recorded voltage
mV
200
0
−200
(b) Same trace with R4-positive candidates and blind exam verdicts
A
B
C
160
170
180
190
200
Time in recording (h)
Overlay and blind verdicts
R4-positive span
Event
Rejected
Unsure
A 171.69 h · 10.1 min
B 174.76 h · 10.4 min
C 192.70 h · 3.5 min
Minutes from span start
Minutes from span start
Minutes from span start