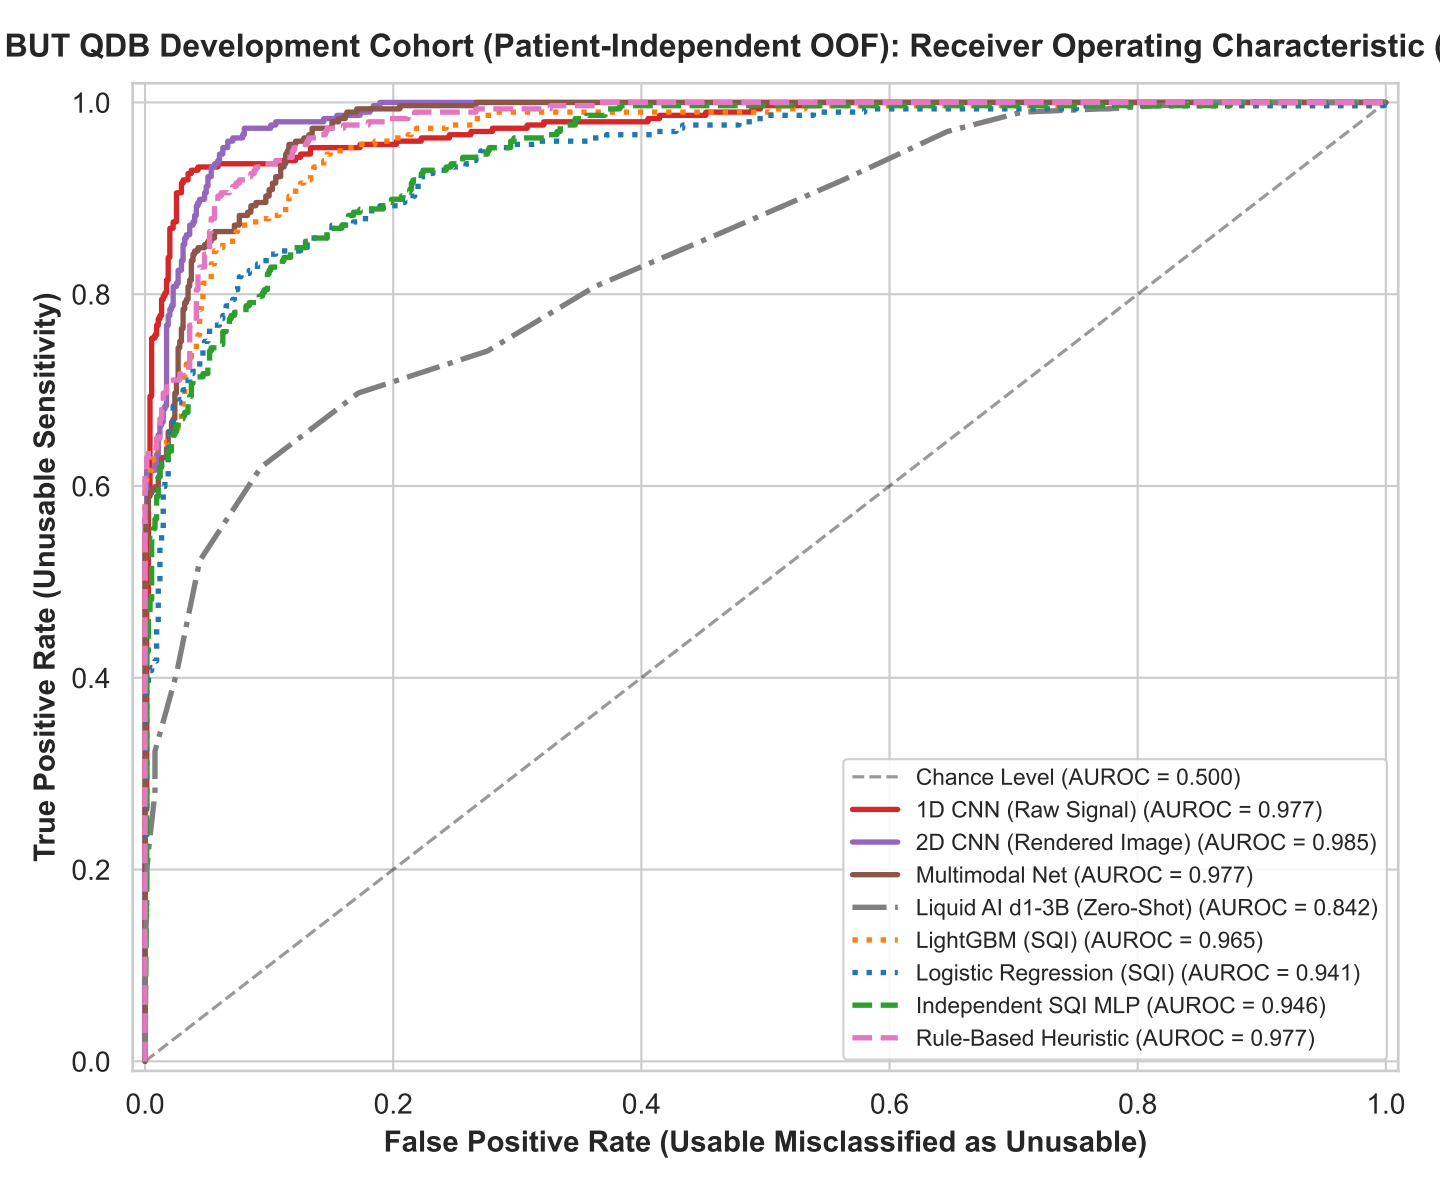
BUT QDB Development Cohort (Patient-Independent OOF): Receiver Operating Characteristic (
True Positive Rate (Unusable Sensitivity)
False Positive Rate (Usable Misclassified as Unusable)
0.0
0.2
0.4
0.6
0.8
1.0
Chance Level (AUROC = 0.500)
1D CNN (Raw Signal) (AUROC = 0.977)
2D CNN (Rendered Image) (AUROC = 0.985)
Multimodal Net (AUROC = 0.977)
Liquid AI d1-3B (Zero-Shot) (AUROC = 0.842)
LightGBM (SQI) (AUROC = 0.965)
Logistic Regression (SQI) (AUROC = 0.941)
Independent SQI MLP (AUROC = 0.946)
Rule-Based Heuristic (AUROC = 0.977)