



Degree Project in Decision and Control Systems

Second cycle, 30 credits

Modeling Nonlinear Insulin-Glucose Dynamics in Critically-ill Patients

Degree Project 2026

MARKUS MULVIHILL

Modeling Nonlinear Insulin-Glucose Dynamics in Critically-ill Patients

Degree Project 2026

MARKUS MULVIHILL

Master's Programme, Information and Network Engineering, 120 credits

Date: July 16, 2026

Supervisor: Martin Lindström

Examiner: Ragnar Thobaben

School of Electrical Engineering and Computer Science

Swedish title: Modellerings av Icke-linjärt Insulin-Glukosdynamik hos Kritiskt Sjuka Patienter

Swedish subtitle: Examensarbete 2026

Abstract

Lorem ipsum dolor sit amet, consectetur adipiscing elit. Ut purus elit, vestibulum ut, placerat ac, adipiscing vitae, felis. Curabitur dictum gravida mauris. Nam arcu libero, nonummy eget, consectetur id, vulputate a, magna. Donec vehicula augue eu neque. Pellentesque habitant morbi tristique senectus et netus et malesuada fames ac turpis egestas. Mauris ut leo. Cras viverra metus rhoncus sem. Nulla et lectus vestibulum urna fringilla ultrices. Phasellus eu tellus sit amet tortor gravida placerat. Integer sapien est, iaculis in, pretium quis, viverra ac, nunc. Praesent eget sem vel leo ultrices bibendum. Aenean faucibus. Morbi dolor nulla, malesuada eu, pulvinar at, mollis ac, nulla. Curabitur auctor semper nulla. Donec varius orci eget risus. Duis nibh mi, congue eu, accumsan eleifend, sagittis quis, diam. Duis eget orci sit amet orci dignissim rutrum. Nam dui ligula, fringilla a, euismod sodales, sollicitudin vel, wisi. Morbi auctor lorem non justo. Nam lacus libero, pretium at, lobortis vitae, ultricies et, tellus. Donec aliquet, tortor sed accumsan bibendum, erat ligula aliquet magna, vitae ornare odio metus a mi. Morbi ac orci et nisl hendrerit mollis. Suspendisse ut massa. Cras nec ante. Pellentesque a nulla. Cum sociis natoque penatibus et magnis dis parturient montes, nascetur ridiculus mus. Aliquam tincidunt urna. Nulla ullamcorper vestibulum turpis. Pellentesque cursus luctus mauris.

Keywords

Canvas Learning Management System, Docker containers, Performance tuning

Sammanfattning

Lorem ipsum dolor sit amet, consectetur adipiscing elit. Ut purus elit, vestibulum ut, placerat ac, adipiscing vitae, felis. Curabitur dictum gravida mauris. Nam arcu libero, nonummy eget, consectetur id, vulputate a, magna. Donec vehicula augue eu neque. Pellentesque habitant morbi tristique senectus et netus et malesuada fames ac turpis egestas. Mauris ut leo. Cras viverra metus rhoncus sem. Nulla et lectus vestibulum urna fringilla ultrices. Phasellus eu tellus sit amet tortor gravida placerat. Integer sapien est, iaculis in, pretium quis, viverra ac, nunc. Praesent eget sem vel leo ultrices bibendum. Aenean faucibus. Morbi dolor nulla, malesuada eu, pulvinar at, mollis ac, nulla. Curabitur auctor semper nulla. Donec varius orci eget risus. Duis nibh mi, congue eu, accumsan eleifend, sagittis quis, diam. Duis eget orci sit amet orci dignissim rutrum. Nam dui ligula, fringilla a, euismod sodales, sollicitudin vel, wisi. Morbi auctor lorem non justo. Nam lacus libero, pretium at, lobortis vitae, ultricies et, tellus. Donec aliquet, tortor sed accumsan bibendum, erat ligula aliquet magna, vitae ornare odio metus a mi. Morbi ac orci et nisl hendrerit mollis. Suspendisse ut massa. Cras nec ante. Pellentesque a nulla. Cum sociis natoque penatibus et magnis dis parturient montes, nascetur ridiculus mus. Aliquam tincidunt urna. Nulla ullamcorper vestibulum turpis. Pellentesque cursus luctus mauris.

Nyckelord

Canvas Lärplattform, Dockerbehållare, Prestandajustering

Acknowledgments

Stockholm, July 2026

Markus Mulvihill

Contents

Acronyms	xi
1 Introduction	1
1.1 Background	2
1.2 Problem	2
1.2.1 Original problem and definition	2
1.2.2 Scientific and engineering issues	2
1.3 Purpose	3
1.4 Goals	3
1.5 Research Methodology	3
1.6 Delimitations	4
1.7 Structure of the thesis	4
2 Background	5
2.1 Intensive Control Insulin-Nutrition-Glucose Model	5
2.2 State Estimation	8
2.2.1 Extended Kalman filter	9
2.2.2 Bootstrap particle filter	10
2.2.3 Observability in Nonlinear Discrete-Time State-Space Models	11
2.2.4 Related Work	13
2.3 Parameter Estimation	13
2.3.1 State Augmentation	14
2.3.2 Related Work	14
2.4 Summary	16
3 Methodology	17
3.1 Synthetic Patient Cohort	17
3.2 Observability of the Intensive Control Insulin-Nutrition- Glucose Model	19

3.3	Nonlinear State Estimation	19
3.4	Parameter Estimation	22
4	Results	25
4.1	Synthetic Patient Cohort	25
4.2	Observability of the Intensive Glucose Insulin-Nutrition- Glucose Model	25
4.3	Nonlinear State Estimation	27
4.4	Parameter Estimation	31
5	Conclusions	35
5.1	Future work	35
5.2	Reflections	35
	References	37

List of Figures

2.1	Example patient's blood glucose and measurement	16
4.1	Virtual Patient Cohort Histograms	26
4.2	Analysis across all calculated empirical observability gramians.	28
4.3	Estimator Comparison	30
4.4	Integral-based method insulin sensitivity estimation performance across varying measurement noise variances.	32
4.5	Mean MSE over time in parameter estimation methods estimating insulin sensitivity.	33

List of Tables

2.1	Assigned parameters in the ICING model. The parameters shaded in gray are derived from fitting methods.	7
4.1	Mean MSE for different estimators and deviations of the initial state. Standard deviations of the MSE are shown in parentheses.	29
4.2	Comparison of the mean MSE in parameter estimation methods estimating insulin sensitivity. Standard deviations of the MSE are shown in parentheses.	34

Acronyms

ICING	Intensive Control Insulin-Nutrition-Glucose
IPI	Integral-based Parameter Identification
MSE	Mean squared error

Chapter 1

Introduction

Patients in the intensive care unit suffering from critical illnesses (e.g. acute myocardial infarction, sepsis, stroke) have been widely documented to undergo hyperglycaemia, even those without a prior diagnosis of diabetes [1]. Acute stress observed in critical illnesses often induces physiological changes, as the secretion of cortisol and catecholamines results in an inflammatory response associated with insulin-resistance [2] [3] [4] [5] [6] [7]. While there is inconclusive evidence pertaining to the causality of stress hyperglycaemia and adverse outcomes, the onset of mortality is far greater in patients with no reported history of hyperglycaemia, in contrast to patients with diabetes [1] [3]. Sustaining glucose concentration under 6.106 mmol/L through insulin infusion has demonstrated a reduction of mortality and morbidity, compared to less-intensive methods of glycaemic control [8], at the subsequent cost of an increase of reported incidences of hypoglycaemia [9]. Further review of intensive insulin therapy and tight glucose control has identified discrepancies in the administration of glycaemic control, mostly corresponding to the risk of moderate to severe hypoglycaemia and glycaemic variability in a critically ill patient is equally detrimental as stress hyperglycaemia, with an increase of mortality and health complications observed [9] [10] [11]. Clinicians aim to maintain blood glucose in a range of 6 mmol/L to 10 mmol/L to account for adverse outcomes in hyperglycaemia and hypoglycaemia. Traditional intensive insulin therapy struggles to fully capture the dynamic fluctuations of blood glucose in critically ill patients. Thus, model-based methods are required to achieve tight glycaemic control.

1.1 Background

The implementation of model-based tight glucose control methods relies on the derivation of insulin-glucose dynamics. Mechanistic insulin-glucose models have been developed with an extensive physiological foundation, and have been validated for gluco-regulation in clinical settings [12] [13] [14] [15] [16]. The insulin-glucose models derived are nonlinear, which requires more advanced numerical methods to properly estimate the current and future insulin-glucose dynamics in patients. In practice, the estimated dynamics from the insulin-glucose models contain process noise from unaccounted dynamics in the model formulation as well as noisy measurements. As a result, the insulin-glucose dynamics in practice struggle to be estimated deterministically. To accommodate modeling of stochastic processes, statistical methods are needed to optimally estimate the dynamics in mechanistic insulin-glucose models.

1.2 Problem

1.2.1 Original problem and definition

There currently exist gaps in research for in-depth analysis of statistical modeling of insulin-glucose dynamics. Previous studies have employed Bayesian filtering methods for this task [17] [18], but they lack necessary evaluation and motivation regarding the patient cohort and the filter design process. While patient inputs differ among institutions due to differing nutrition guidelines and stay times for patients, a systematic virtual patient cohort framework would greatly improve the simulation of diverse patient dynamics and experiment reproducibility, as real patient data are often limited in size and closed-source. Concurrently, concise parameterization and optimization of Bayesian filters will further improve glycaemic control in critically-ill patients.

1.2.2 Scientific and engineering issues

To model the behavior of dynamical systems, experience of statistical modeling is often required to construct assumptions of the system parameters. In the case of the representation insulin-glucose dynamics, there are several unknown parameters, and each has its respective role in modeling gluco-regulation. As a result, on top of estimating nonlinear and time-varying

dynamics, the models must be robust to misalignments of the assigned parameters, which poses an ongoing challenge.

1.3 Purpose

Mechanistic insulin-glucose models are of great benefit to critically ill patients and clinicians, as modeling gluco-regulation allows for necessary glycaemic adjustments to avoid the onset of adverse outcomes. In practice, clinicians only have the ability to base insulin resistance on blood glucose measurements, and thus, state estimators models fill in the gap as a tool for insulin-glucose dynamics estimation. Improvements in the estimation of insulin-glucose dynamics can better capture the evolution of the health of the patient in the intensive care unit to prevent mortality and morbidity.

1.4 Goals

The overall goals of this project has been divided into the following sub-goals:

1. Design a virtual patient cohort
2. Compare performance of varying filtering configurations in estimation of insulin-glucose dynamics
3. Extrapolate the formulation of insulin-glucose estimators to estimate unknown parameters in patients

1.5 Research Methodology

The modeling of the insulin-glucose dynamics found in critically ill patients will be implemented on a virtual patient cohort. Using virtual patients allows the researcher to manually control the insulin-glucose model parameters, which directly improves the evaluation of the outcome of the insulin-glucose control. Previous work will serve as the benchmark to compare how the parameterization of our method performs in estimating insulin-glucose dynamics of virtual patients. The chosen filter design will then be used to estimate additional dynamics not mathematically represented in insulin-glucose models. Fitting metrics and computational complexity of the estimators will be utilized to draw inferences about the performance.

1.6 Delimitations

This study will consist of a virtual patient cohort. Using virtual patients is important for maintaining internal validity in the experimental process, as it verifies the observed outcome of the experiment is due to the manipulation of insulin-glucose model parameters rather than uncontrolled variables. The expense of using virtual patients can be identified in the reduced generalizability of this experiment, since virtual patients are models. While this is a limitation, this study will focus on the foundation of the modeling of insulin-glucose dynamics, and future work can replicate the study with real clinical data.

1.7 Structure of the thesis

Chapter 2 will introduce the existing modeling of insulin-glucose dynamics used, followed by an overview of discretization, state estimation, and related work in parameter estimation. In Chapter 3, the proposed research process used to answer the research questions of this study will be documented and motivated. The results will be presented in Chapter 4 along with the discussion. The key findings and future work of the experiment will be summarized in Chapter 5.

Chapter 2

Background

The background will introduce the theoretical concepts and prior work relevant to the paper. The **ICING** model will be introduced to lay the foundation of insulin-glucose modeling, and how state estimation methods can be applied to estimate dynamics optimally. The chapter will conclude with practical parameter estimation approaches to predict unknown parameters.

2.1 Intensive Control Insulin-Nutrition-Glucose Model

The **ICING** model presented by Lin et al. [14] contains the insulin-glucose dynamics in critically ill patients. The model is constructed as a fusion of two existing models validated for patients in the intensive care unit [12] [13], containing the following ensemble of differential equations

$$\dot{G} = -p_G G(t) - S_I(t) G(t) \frac{Q(t)}{1 + \alpha_G Q(t)} + \frac{P(t) + E_G - C_G}{V_G} \quad (2.1)$$

$$\dot{Q} = n_I(I(t) - Q(t)) - n_C \frac{Q(t)}{1 + \alpha_G Q(t)} \quad (2.2)$$

$$\begin{aligned} \dot{I} = & -n_K I(t) - n_L \frac{I(t)}{1 + \alpha_I I(t)} - n_I(I(t) - Q(t)) + \frac{u_{ex}(t)}{V_I} \\ & + \frac{(1 - x_L)u_{en}(t)}{V_I} \end{aligned} \quad (2.3)$$

$$\dot{P1} = -d_1 P1 + D(t) \quad (2.4)$$

$$\dot{P2} = -\min(d_2 P2, P_{max}) + d_1 P1 \quad (2.5)$$

$$u_{en}(t) = k_1 \exp\left(-\frac{k_2}{k_3} I(t)\right), \quad \text{when C-peptide data is not available} \quad (2.6)$$

$$P(t) = \min(d_2 P_2, P_{max}) + P_N(t). \quad (2.7)$$

Equation (2.1) is the independent insulin glucose removal, with G being the total blood glucose concentration (mmol/L). The whole-body insulin sensitivity $S_I(t)$ gives insight into the metabolic condition of the patient and is a time-varying dynamic. The insulin pharmacodynamics are shown in Equations (2.2) and (2.3), with Q and I being the interstitial insulin concentration (mU/L) and the plasma insulin concentration (mU/L) respectively. The exogenous insulin input is $u_{ex}(t)$ (mU/min), and the endogenous insulin production $u_{en}(t)$ (mU/min) can be measured from C-Peptide, but if measurements are not feasible, the kinetics can model as such in Equation (2.6). The gastric absorption of glucose is defined in Equations (2.4) to (2.7). The dynamics P_1 and P_2 describe the glucose in the stomach and the gut (mmol), with $P(t)$ representing the glucose appearance in the blood (mmol/min). Any enteral food intake given to the patient is accounted for by $D(t)$ (mmol/min), and additional parenteral glucose is described by $P_N(t)$ (mmol/min).

The **ICING** model also involves several parameters alongside the previously defined dynamics, which are detailed in Table 2.1. The majority of the patient model parameters are assigned as general population constants observed from clinical trials, and are validated in relevant insulin-glucose control parameter sensitivity studies [15] [16] [19]. The identification of the remaining parameters was estimated with a data-driven approach by fitting the patient parameters to the observed dynamics in 173 patients, and by assessing the impact of prediction errors [19]. Estimating the endogenous glucose removal p_G and the suppression of endogenous glucose produce E_G constants involved assigning all other patient parameters and the insulin sensitivity to constants, then starting a grid search that covers $p_G = 0.001, 0.002, \dots, 0.1(\text{min}^{-1})$ and $E_G = 0.0, 0.1, \dots, 3.5$ (mmol/min). The joint p_G and E_G value that achieved the lowest fitting and prediction error for blood glucose in Equation (2.1) was chosen. Ultimately, that was $p_G = 0.006(\text{min}^{-1})$ and $E_G = 1.16$, while both falling in the ranges observed physiologically. The glucose distribution rate between the stomach and the gut n_I , and cellular insulin clearance rate in the interstitium were estimated similarly by fitting to Q in the Equation (2.2), a grid search covers a range of $n_I = n_C = 0.0001, \dots, 0.02(\text{min}^{-1})$, with a value of $n_I = 0.003$ resulting in the best predictive performance.

Table 2.1: Assigned parameters in the **ICING** model. The parameters shaded in gray are derived from fitting methods.

Parameter	Notation	Value
Patient endogenous glucose removal	p_G (min^{-1})	0.006
Saturation of insulin-stimulated glucose removal	α_G (L/mU)	0.0154
Suppression of endogenous glucose production	E_G (mmol/min)	1.16
Central nervous system uptake	C_G (mmol/L)	0.3
Glucose distribution volume	V_G (L)	13.3
Glucose distribution rate between the stomach and the gut	n_I (min^{-1})	0.003
Cellular insulin clearance rate in the interstitium	n_C (min^{-1})	$= n_I$
Kidney clearance rate of insulin from plasma	n_K (min^{-1})	0.0542
Liver clearance rate of insulin from plasma	n_L (min^{-1})	0.01578
Saturation of plasma insulin disappearance	α_I (L/mU)	0.0017
Insulin distribution volume	V_I (L)	3.15
Fraction of endogenous insulin hepatic extraction	x_L	0.67
Maximal glucose out flux from the gut	P_{max} (mmol/min)	6.11
Base endogenous insulin production rate	k_1 (mU/min)	45.7
Transport rates between the stomach and the gut	d_1 (min^{-1})	0.0347
	d_2 (min^{-1})	0.0069
Exponential suppression constants	k_2	1.5
	k_3	1000

It should be noted that in the **ICING** model, the nonlinear dynamics are defined in continuous time. Discretization of the dynamic system is necessary as in the following section, the estimation methods presented operate within discrete time, noted as k . If we define the discrete time step as $t_k = t_{k-1} + \Delta$, an example dynamic $F(t)$ can be discretized according to the Euler method

$$\begin{aligned}\dot{F} &\approx \frac{F(t_k) - F(t_k - \Delta)}{\Delta} \\ F_k &\approx F_{k-1} + \Delta \dot{F}.\end{aligned}\tag{2.8}$$

The error of this numerical approximation of differential equations is bounded by the step size Δ . As a result, larger step sizes will introduce greater approximation errors. Thus, a relatively small step size is necessary to prevent errors from propagating in the estimates.

2.2 State Estimation

Within the scope of this paper, discrete-time dynamical systems will be modeled in the state-space representation. A state-space model consists of system variables that describe the state of the system, inputs, and measurements. The states are typically formulated as linear or nonlinear differential equations. A probabilistic representation of the discrete-time state-space can be represented as such

$$\begin{aligned} x_k &\sim p(x_k \mid x_{k-1}, u_{k-1}) \\ y_k &\sim p(y_k \mid x_k), \end{aligned} \quad (2.9)$$

where $p(x_k \mid x_{k-1}, u_k)$ and $p(y_k \mid x_k)$ are the stochastic discrete-time dynamic and measurement models, with $x_k \in \mathbb{R}^n$ representing the states, $u_k \in \mathbb{R}^p$ are the inputs, and $y_k \in \mathbb{R}^m$ are the measurements.

Any dynamic model has intrinsic approximation errors, and the errors should be taken into account. The approximation error for the states can be modeled as a random process, and artificial process noise can be added into x_k at each time step. This step is important to accommodate errors due to unaccounted dynamics. Choices in the specifics regarding the modeling of process noise of insulin-glucose dynamics will be discussed in Chapter 3.

The objective of state estimators can be described as estimating the distribution of the state x_k , given all the measurements up to the current sample $p(x_k \mid y_{1:k})$. In the case of assuming the state estimator is linear and Gaussian, the states and measurements can be written as the difference equations

$$\begin{aligned} x_k &= A_{k-1}x_{k-1} + B_{k-1}u_{k-1} + q_{k-1} \\ y_k &= Hx_k + r_k, \end{aligned} \quad (2.10)$$

where $q_{k-1} \sim \mathcal{N}(0, Q_{k-1})$ is the process noise, $r_k \sim \mathcal{N}(0, R_k)$ is the measurement noise, we can rewrite the Equation (2.9) as the following

$$\begin{aligned} p(x_k \mid x_{k-1}, u_{k-1}) &= \mathcal{N}(x_k \mid A_{k-1}x_{k-1} + B_{k-1}u_{k-1}, Q_{k-1}) \\ p(y_k \mid x_k) &= \mathcal{N}(y_k \mid Hx_k, R_k). \end{aligned} \quad (2.11)$$

The closed-form solution of $p(x_k \mid y_{1:k})$ for linear and Gaussian dynamic and measurement functions is known as the Kalman filter, with a full derivation available from Särkkä and Svensson [20]. The filter contains two key parts: the *prediction step* and the *update step*.

1. Prediction step

$$\begin{aligned} m_k^- &= A_{k-1}x_{k-1} + B_{k-1}u_{k-1} \\ P_k^- &= A_{k-1}P_{k-1}A_{k-1}^\top + Q_{k-1}. \end{aligned} \quad (2.12)$$

2. Update step

$$\begin{aligned} v_k &= y_k - H_k m_k^- \\ S_k &= H_k P_k^- H_k^\top + R_k \\ K_k &= P_k^- H_k^\top S_k^{-1} \\ m_k &= m_k^- + K_k v_k \\ P_k &= P_k^- - K_k S_k K_k^\top. \end{aligned} \quad (2.13)$$

The Kalman filter is recursive, as the filter starts with an estimate of the initial distribution of the state m_0^- and the covariance P_0^- , and iterates sequentially over discrete time steps k . In practice, the Kalman filter is often a great starting point for an estimator because the assumptions of linearity and Gaussianity often hold in many contexts, but as Equations (2.1) to (2.5) are nonlinear, other methods must be considered.

2.2.1 Extended Kalman filter

The extended Kalman filter can accommodate the nonlinearities in the **ICING** model by approximating the dynamic and measurement models as a linear transformation of the states and inputs. The structure of the extended Kalman filter remains the same as the Equations (2.12) and (2.13), but changes are seen in the matrices of the dynamic and measurement models $f(\cdot)$ and $h(\cdot)$. Assuming that the dynamic and measurement models are Gaussian, the prediction and update steps [20] can be defined as

1. Prediction step

$$\begin{aligned} m_k^- &= f(m_{k-1}, u_{k-1}) \\ P_k^- &= F_x(m_{k-1})P_{k-1}F_x^\top(m_{k-1}) + F_q(m_{k-1})Q_{k-1}F_q^\top(m_{k-1}) \end{aligned} \quad (2.14)$$

2. Update step

$$\begin{aligned}
v_k &= y_k - h(m_k^-) \\
S_k &= H_x(m_k^-)P_k^-H_x^\top(m_k^-) + H_r(m_k^-)R_kH_r^\top(m_k^-) \\
K_k &= P_k^-H_k^\top(m_k^-)S_k^{-1} \\
m_k &= m_k^- + K_kv_k \\
P_k &= P_k^- - K_kS_kK_k^\top,
\end{aligned} \tag{2.15}$$

the Jacobian matrices $F_x(m_k^-)$, $F_q(m_k^-)$, $H_x(m_k^-)$, and $H_r(m_k^-)$ are the Taylor series linear approximation of the dynamic and measurement models

$$\begin{aligned}
[F_x(m)]_{j,j'} &= \left. \frac{\partial f_j(x, q)}{\partial x_{j'}} \right|_{x=m_{k-1}, q=0} \\
[F_q(m)]_{j,j'} &= \left. \frac{\partial f_j(x, q)}{\partial q_{j'}} \right|_{x=m_{k-1}, q=0} \\
[H_x(m)]_{j,j'} &= \left. \frac{\partial h_j(x, r)}{\partial x_{j'}} \right|_{x=m_k^-, r=0} \\
[H_r(m)]_{j,j'} &= \left. \frac{\partial h_j(x, r)}{\partial r_{j'}} \right|_{x=m_k^-, r=0}.
\end{aligned} \tag{2.16}$$

The intrinsic bottleneck of the extended Kalman filter can be ascribed to the Gaussian formulation of the state update equations. Any deviations from Gaussianity in the posterior will directly degrade the estimation capabilities of the estimator. Another type of state estimation method is the particle filter, which can accommodate nonlinear and nongaussian dynamic and measurement models by using point estimates from a Monte Carlo approximation of the posterior $p(x_k \mid y_{1:k})$.

2.2.2 Bootstrap particle filter

For state-space modeling, the dynamic and measurement models are run sequentially such that x_k and y_k are represented as a Markov Chain

$$\begin{aligned}
x_k &\sim p(x_k \mid x_{k-1}, u_{k-1}) \\
y_k &\sim p(y_k \mid x_k)
\end{aligned} \tag{2.17}$$

In the Kalman filter case, such dynamic and measurement models were assumed to be linear and Gaussian. As a result, the posterior of the state

$p(x_k | y_k)$ was derived as a linear transformation of the mean and covariance. For the bootstrap particle filter, the posterior of the state is formulated as a Monte Carlo approximation, with $x_k^{(i)}$ denoting a randomly sampled state for N total particles

$$p(x_k | y_k) \approx \frac{\sum_{i=1}^N p(y_k | x_k^{(i)}) p(x_k^{(i)})}{\sum_{j=1}^N p(y_k | x_k^{(j)})}. \quad (2.18)$$

The steps to implement to formulate the bootstrap particle filter iteratively can be summarized in the following algorithm [20] [21] [22]

1. Sample N particles from the dynamic function

$$x_k^{(i)} \sim p(x_k | x_{k-1}^{(i)}, u_{k-1}) \quad i = 1, \dots, N \quad (2.19)$$

2. Update weights from the measurement

$$\begin{aligned} w_k^{*(i)} &\propto p(y_k | x_k^{(i)}) \quad i = 1, \dots, N \\ w_k^{(i)} &= \frac{w_k^{*(i)}}{\sum_{j=1}^N w_k^{*(j)}} \quad i = 1, \dots, N \end{aligned} \quad (2.20)$$

3. Systematically resample particles from a distribution proportional to the weights

$$u_1 \sim \mathbb{U} \left[0, \frac{1}{N} \right] \quad (2.21a)$$

$$u_r = u_1 + \frac{r-1}{N} \quad r = 2, \dots, N \quad (2.21b)$$

$$x_k^{(i)} = \begin{cases} x_k^{(r)} & \text{if } \sum_{j=1}^{i-1} w_k^{(j)} < u_r \leq \sum_{j=1}^i w_k^{(j)} \end{cases} \quad i = 1, \dots, N \quad (2.21c)$$

$$w_k^{(i)} = \frac{1}{N} \quad i = 1, \dots, N \quad (2.21d)$$

2.2.3 Observability in Nonlinear Discrete-Time State-Space Models

Analyzing observability in linear and nonlinear systems assesses how well the dynamics of the model can be inferred from the observations. The observability gramian W_O has traditionally been used in model reduction

of linear dynamic systems, but empirical methods have been adapted to accommodate nonlinear systems [23]. The observability gramian provides insight which states have the most influence on the output of the system by analyzing the rank condition of the observability gramian matrix, which in return allows for analytically evaluating observability.

To empirically calculate the observability gramian, we first generate 2^n unique combinations of the initial state $x_0 \in \mathbb{R}^n$, with n denoting the numbers of states [18] [23] [24]. The initial condition x_0 will be assigned as perturbations $\delta_i \in \mathbb{R}^n$ around a nominal value $x_{nom} \in \mathbb{R}^n$

$$\begin{aligned} x_{0,i} &= x_{nom} + \delta_i \\ \delta_i &= c \cdot S \cdot t_i, \quad \text{with } S = \text{diag}(x_{\max}). \end{aligned} \quad (2.22)$$

The scalar constant c corresponds to the magnitude of deviation, $S \in \mathbb{R}^{n,n}$ is the diagonal matrix of the maximum of each state and parameter. The row vector $t_i \in \mathbb{R}^n$ is the specified perturbation i from the orthonormal matrix

$$\begin{aligned} T &= [t_1 \ t_2 \ \dots \ t_{2^n}] \in \mathbb{R}^{n,2^n} \\ t_1^T &= \frac{1}{\sqrt{2^n}} [-1 \ -1 \ \dots \ -1] \\ t_2^T &= \frac{1}{\sqrt{2^n}} [-1 \ -1 \ \dots \ 1] \\ &\vdots \\ t_{2^n}^T &= \frac{1}{\sqrt{2^n}} [1 \ 1 \ \dots \ 1]. \end{aligned} \quad (2.23)$$

After calculating the 2^n perturbations of the initial state, the output can be derived sequentially with Equations (2.9) from time step $k = 1, \dots, K$ beginning with $x_{0,i}$ to generate $y_{1:K,i}$. Then, the empirical observability with discrete time steps $t = k \, dt$ can be expressed as such

$$W_O = (cS)^{-1} \sum_{k=1}^K T \Psi[k] T^T dt (cS)^{-1}, \quad (2.24)$$

with the positive definite matrix $\Psi[k]$ being assigned as the following

$$\Psi_{i,j}[k] = |y_i[k] - y_0[k]| |y_j[k] - y_0[k]|. \quad (2.25)$$

If the states have varying magnitudes of scale, it is recommended

[18] to rerun the observability gramian algorithm again with the following transformations

$$x_s = \sqrt{\text{diag}(W_O)} \quad T_s = \text{diag}^{-1}(x_s). \quad (2.26)$$

The new state perturbations are now assigned as the transformation $\bar{x} = T_s x$. To make inferences about of the observability gramian, one can check the rank condition of the matrix by analyzing the nonzero singular values of W_0 . If there exists singular values near zero (e.g. < 0.1), a subset of the dynamics of the system can not be observed from the measurements.

2.2.4 Related Work

Nonlinear state estimation of the **ICING** model has been investigated in a previous study by Aguirre-Zapata et al. [17]. The study incorporated an additional measurement and dynamic due to their clinical facility having a continuous glucose machine that can measure the patient's interstitial glucose, but the formulation of patient dynamics otherwise remained the same. In the methodology of the paper, all tests regarding estimation performance are tested on deviations from one virtual patient, with each deviation being assigned the same exogenous insulin input per deviation, and food intake is generally not considered. Overall, their virtual patients do not constitute a reasonable patient model in comparison to real patients.

The study includes three state estimators: the extended Kalman filter, the unscented Kalman filter, and the particle filter. The majority of the study uses discrete time-steps of 5 minutes. While the dynamics of patients develop relatively slowly, such a large time step can introduce approximation errors in the discretization of the **ICING** model. Another notable design choice of their particle filter is that it contains 5000 particles. Further analysis of various sized particle filters would motivate the overall trade-off estimation performance compared to the time complexity. State estimation remained in the scope of dynamics represented in the **ICING** model and an additional interstitial glucose dynamic. As a result, there exists further development of state estimators to predict unrepresented **ICING** model parameters as well.

2.3 Parameter Estimation

As previously mentioned, there exists unrepresented **ICING** model parameters. Additionally, these parameters contain time-varying characteristics. The

whole-body insulin sensitivity S_I or the endogenous insulin u_{en} dynamically fluctuates over time depending on the patient's metabolic condition. As a result, naively assigning either as a general population constant can hinder the performance of the estimators. The unknown time-varying parameters of interest will be denoted as θ in preparation for the next section.

2.3.1 State Augmentation

A practical method to handle unknown parameters is to augment them to the existing state variables $\tilde{x}_k = [x_k, \theta_k]^\top$, such that Equation (2.9) can be redefined as

$$\begin{aligned}\tilde{x}_k &\sim p(\tilde{x}_k \mid \tilde{x}_{k-1}, u_{k-1}) \\ y_k &\sim p(y_k \mid \tilde{x}_k).\end{aligned}\tag{2.27}$$

An important distinction in Equation (2.27) is that the unknown parameters are treated as stochastic variables with singularity in the process noise. This can be problematic as all models often have approximation errors, and this can drive the extended Kalman filter to ultimately diverge in the Gaussian approximation, as well as introduce sample impoverishment in particle filters [20].

One method to compensate for singularity is to also add artificial process noise Q_k to the unknown parameters to allow for random walking in the state space, thus, accounting for errors in the dynamic function

$$\theta_k = \theta_{k-1} + \epsilon_{k-1}, \quad \text{with } \epsilon_{k-1} \sim \mathcal{N}(0, Q_{k-1}).\tag{2.28}$$

With this method, you inherently add another unknown parameter Q_k , but such a parameter can be tuned with prior knowledge of the parameters θ_k .

2.3.2 Related Work

The **IPI** method is a nonlinear and nonconvex parameter identification method that has been introduced that can estimate patient-specific parameters as a least squares solution [15]. By linearly interpolating between the blood glucose measurements in times $[t_0, t_1]$,

$$\tilde{G}(t) = \frac{G(t_1) - G(t_0)}{t_1 - t_0}(t - t_0) + G(t_0),\tag{2.29}$$

the Equation (2.1) can be rearranged as such for a piecewise constant S_I

$$\begin{aligned} \int_{t_0}^{t_1} \dot{G} dt &\approx -p_G \int_{t_0}^{t_1} \tilde{G}(t) dt - S_I \int_{t_0}^{t_1} \tilde{G}(t) \frac{Q(t)}{1 + \alpha_G Q(t)} dt \\ &\quad + \frac{1}{V_G} \int_{t_0}^{t_1} (P(t) + E_G - C_G) dt \\ G(t_1) - G(t_0) &\approx -p_G \int_{t_0}^{t_1} \tilde{G}(t) dt - S_I \int_{t_0}^{t_1} \tilde{G}(t) \frac{Q(t)}{1 + \alpha_G Q(t)} dt \\ &\quad + \frac{1}{V_G} \int_{t_0}^{t_1} (P(t) + E_G - C_G) dt, \end{aligned} \quad (2.30)$$

and S_I can be expressed as a linear equation

$$\underbrace{\int_{t_0}^{t_1} \tilde{G}(t) \frac{Q(t)}{1 + \alpha_G Q(t)} dt}_{A(t_0, t_1)} S_I \approx \underbrace{\left(G(t_0) - G(t_1) - p_G \int_{t_0}^{t_1} \tilde{G}(t) dt + \frac{1}{V_G} \int_{t_0}^{t_1} (P(t) + E_G - C_G) dt \right)}_{b(t_0, t_1)}. \quad (2.31)$$

It is often the case with longer measurement periods ($t_1 - t_0$), that identifying multiple S_I values within the time period may be necessary. For instance, if every 120 minutes glucose measurements are taken from the patient, but every 60 minutes a patient's insulin sensitivity should be identified $S_I \in \mathbb{R}^2$. Both insulin sensitivity parameters at 60 minutes S_I^{60} and 120 minutes S_I^{120} can be derived as the least squares solution from the system of linear equations

$$\begin{bmatrix} A(t_0, t_0 + 30) & 0 \\ A(t_0 + 30, t_0 + 60) & 0 \\ 0 & A(t_0 + 60, t_0 + 90) \\ 0 & A(t_0 + 90, t_0 + 120) \end{bmatrix} \begin{bmatrix} S_I^{60} \\ S_I^{120} \end{bmatrix} = \begin{bmatrix} b(t_0, t_0 + 30) \\ b(t_0 + 30, t_0 + 60) \\ b(t_0 + 60, t_0 + 90) \\ b(t_0 + 90, t_0 + 120) \end{bmatrix}. \quad (2.32)$$

The fundamental flaw of the **IPI** method is the assumption of linear blood glucose dynamics between measurements of times $[t_0, t_1]$. If we closely analyze the Figure 2.1, linearly interpolating blood glucose introduces residuals, due to fitting errors. Consequently, the residuals will propagate into the integrals in the Equation (2.31), resulting in errors in the parameter calculation. Other methods not relying on linearization of the measurements must be explored to allow for realistic estimation of parameters, thus giving

better insight of the patient's health status to clinicians.

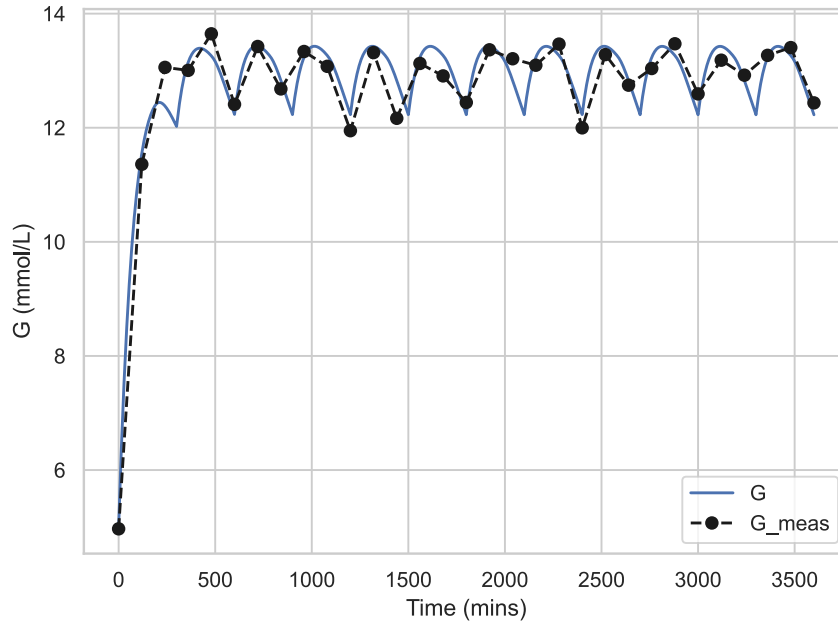


Figure 2.1: Blood glucose and its' corresponding measurements from an example patient trajectory from the **ICING** model.

2.4 Summary

The **ICING** model provides a foundation to model glucose removal, insulin pharmacokinetics, and gastric absorption of glucose for tight glucose control in critically ill patients. Utilizing nonlinear state estimators such as the extended Kalman filter and the bootstrap particle filter allows for optimal estimation of the dynamics over time with consideration of model approximation errors and measurement noise. Consideration of realistic virtual patients and systematically motivated parameterization of filters will improve generalizability of the estimators. The current method of **IPI** is formulated with strict assumptions of blood glucose measurements, which limits the ability for clinicians to infer the health of the patient from the approximated patient-specific parameters. More in-depth parameter estimation methods can improve model identifiability for glucoregulation in critically ill patients.

Chapter 3

Methodology

The necessary methodology to achieve the goals introduced in Section 1.4 will be presented in this chapter. It begins with the design of the virtual patient cohort used for simulation of patients in this paper. The observability of the ICING model is analyzed to learn if the dynamics can be inferred from the measurements. Based on the observed performance, nonlinear state estimators are utilized to assess the model's ability to estimate unmeasured dynamics. Finally, the parameter estimation methods used to estimate unknown constant and time-varying insulin sensitivity are introduced.

3.1 Synthetic Patient Cohort

A virtual patient cohort will be simulated to model clinical insulin-glucose data observed in patients in the intensive care unit. A patient model consists of simulated insulin-glucose dynamics (G , Q , I , $P1$, $P2$, u_{en} , P) represented in Equations (2.1) to (2.7), known insulin sensitivity S_I , exogenous insulin u_{ex} , enteral feed D , and parenteral feed P_N . The population constants listed in Table 2.1 are assigned to the constant parameters for all virtual patients. To introduce variance between patients, a virtual patient is given a random constant input observed from doses given to patients in the Karolinska University Hospital

$$\begin{aligned} u_{ex} &\sim \mathcal{U}[0, 166] \text{ mU/min} \\ D &\sim \mathcal{U}[0.2, 0.4] \text{ mmol/min} \\ P_N &\sim \mathcal{U}[0.2, 0.4] \text{ mmol/min.} \end{aligned} \tag{3.1}$$

The insulin sensitivity has been shown to follow a log-normal distribution [25]. Sampling the insulin sensitivity from a log-normal is important to adhere to the physiological constraints typically observed in patients, as the insulin sensitivity is small in magnitude, and sampling from a normal distribution may shift the value to negative or too large in magnitude, which can possibly result in poor estimation. The values chosen within this study will be drawn from the distribution*

$$S_I = \exp(X), \quad \text{with } X \sim \mathcal{N}(-8.05, 0.70^2). \quad (3.2)$$

To simulate patient data given the inputs and parameters, each virtual patient needs to be assigned a unique initial state[†] for the dynamics

$$x_0 = [G_0 \quad I_0 \quad Q_0 \quad P1_0 \quad P2_0 \quad u_{en0}] . \quad (3.3)$$

If it assumed that the patient model begins at a steady state, it is possible to derive the initial states with the given input and parameter values by solving for the roots of the Differential Equations (2.1) to (2.6). This can be computed with the solver function `scipy.optimize.fsolve`[‡] for each patient.

Given all the initial states x_0 , known insulin sensitivity S_I , and the patient inputs u_{ex} , D , and PN , the patient cohort can be generated by solving the differential equations (2.1) to (2.5) with a time step of $dt = 1$ min for each patient, and the results will be inputs to Equations (2.6) and (2.7). The ODE solver `scipy.integrate.solve_ivp`[§] function in python will be applied with the Explicit Runge-Kutta of order 5(4) integration method [26] to solve for the necessary dynamics.

*These parameters are approximated according to previous work from Davidson et al. [25]

[†]The glucose appearance in the blood P is not included as an initial state in the state-space model. This is a result of patients not reaching the maximum glucose out flux from the gut $P_{\max}$ at the beginning of the simulation. Thus, it simplifies to a deterministic equation.

[‡]<https://docs.scipy.org/doc/scipy/reference/generated/scipy.optimize.fsolve.html>

[§]https://docs.scipy.org/doc/scipy/reference/generated/scipy.integrate.solve_ivp.html

3.2 Observability of the Intensive Control Insulin-Nutrition-Glucose Model

In Chapter 3.1, virtual patients were created by first randomly sampling initial dynamics, and then utilizing an ODE solver to solve the dynamics according to the ICING model. For the ICING model to be classified as observable, it must be possible to infer the insulin-glucose dynamics, given a sufficient number of observations. To establish if the formulation of the ICING model is observable, a mathematical analysis can determine the relationship of the insulin-glucose dynamics and the observations as previously discussed in Section 2.2.3.

1000 patient models will be randomly sampled to investigate the observability of the ICING model across various permutations of each random nominal state vector. The maximum value of each state* x_{max} will be chosen as the maximum values of the patient cohort dynamics found in the previous Section 3.1

$$S = \text{diag}(x_{max}) \quad (3.4)$$

as well with a maximum perturbation constant of $c = 0.1$. With the following defined inputs, the observability gramian W_O can be derived to analyze the singular values of all the calculated matrices using single value decomposition. To also analyze which states are the most observable respectively to each other, the diagonals of the observability gramian can be used to propose that the diagonal entries that are greater in magnitude, those states provide more information in relation to the observations. Formulating an approximation of the observability will provide insight into the performance of the estimators in the following section.

3.3 Nonlinear State Estimation

The extended Kalman filter and the particle filter are two different nonlinear state estimation methods presented in Section 2.2. To compare each estimator with the ICING model, the computational complexity $\mathcal{C}$ of estimating all states over the total time and the MSE of the blood glucose concentration estimates will be recorded for all patients and filters in the given virtual patient cohort. The simulations will span 12 hours to allow each estimator to converge, as

*For this calculation, u_{en} and P are omitted. This is due to the fact that these dynamics are deterministic at $t = 0$.

well as a discrete time-step of 1 minute, with glucose measurements corrupted with additive Gaussian noise ($\mathcal{N}(0, 0.125)$) sampled every 120 minutes. There will be offsets in the initial states of $\pm 2\%$, $\pm 10\%$, $\pm 25\%$, with each iteration having a virtual cohort of 500 patients. Adding an offset to the initial state will gauge how well each estimator can adapt to various initial perturbations in the estimate.

If it is assumed that the model approximation errors can be modeled as a random process, artificial process noise can be added to the state estimates for both the extended Kalman filter and the particle filter. Due to the discrete time-step to measurement time-step ratio being 120:1, the process noise per sample was chosen as an expected amount of deviation between measurements divided by 120. The process noise w will be sampled at each discrete time-step for both the extended Kalman filter and the particle filter roughly according to the following normal distribution

$$w \sim \mathcal{N}\left(0, \frac{1}{120} \text{diag} \begin{pmatrix} \left(\frac{\text{med}(G)}{100}\right)^2 \\ \left(\frac{\text{med}(I)}{100}\right)^2 \\ \left(\frac{\text{med}(Q)}{100}\right)^2 \\ \left(\frac{\text{med}(P1)}{100}\right)^2 \\ \left(\frac{\text{med}(P2)}{100}\right)^2 \\ 1.0 \times 10^{-8} \end{pmatrix}\right). \quad (3.5)$$

The variance for the dynamics G , I , Q , $P1$, $P2$ are chosen as the scaled median for the population statistics found in Section 3.1. The process noise for the enteral insulin is assigned as a relatively small value in comparison to the other states. This is a design to choose to have the insulin sensitivity absorb more of the uncertainty of the glucose distribution between the gut and the stomach, instead of the endogenous insulin. The covariance between states is assigned as zero, as model approximation errors are assumed to be independent of states.

The extended Kalman filter parameters will be defined as

1. Initial covariance matrix of

$$P_0 = \text{diag} \left(\begin{bmatrix} \log_{10}(\text{med}(G)) \\ \log_{10}(\text{med}(I)) \\ \log_{10}(\text{med}(Q)) \\ \log_{10}(\text{med}(P1)) \\ \log_{10}(\text{med}(P2)) \\ \log_{10}(\text{med}(u_{en})) \end{bmatrix} \right) \quad (3.6)$$

2. Process noise covariance matrix of

$$Q = \frac{1}{120} \text{diag} \left(\begin{bmatrix} \left(\frac{\text{med}(G)}{100} \right)^2 \\ \left(\frac{\text{med}(I)}{100} \right)^2 \\ \left(\frac{\text{med}(Q)}{100} \right)^2 \\ \left(\frac{\text{med}(P1)}{100} \right)^2 \\ \left(\frac{\text{med}(P2)}{100} \right)^2 \\ 10^{-8} \end{bmatrix} \right) \quad (3.7)$$

3. Measurement noise covariance matrix of

$$R = [0.125] \quad (3.8)$$

Particle filters containing (100, 200, 300, 400, 500, 750, 1000, 1500, 2000) particles will be used to compare the relationship of the estimation performance over an increasing number of particles. The notation of the extended Kalman filter will be abbreviated as EKF and for a particle filter with N particles, it will be represented as PF N . The particle filter will be initialized by sampling particles from a multivariate Gaussian distribution with a mean of the initial state, and a covariance equal to the extended Kalman filter's Q .

To define the computational complexity of the estimators given the experimental setup, let τ_i denote the average total time to run each particle filter and the extended Kalman filter in seconds, with N being the total number

of filters

$$\begin{aligned}\tau_{\min} &= \min(\tau) \\ \mathcal{C}_i &= \frac{\tau_i}{\tau_{\min}} \quad i = 1, \dots, N.\end{aligned}\tag{3.9}$$

The total time complexity is relative to the machine running the particle simulation. Hence, using a normalized scale for τ maintains repeatability across different environments, as each particle filter is designed in software such that the time complexity is linearly dependent on the amount of particles. The error of the estimators will be represented as the mean squared error **MSE** of the true blood glucose concentration sequence G and an estimated blood glucose concentration sequence $\hat{G}$ of length L

$$\text{MSE}_i = \frac{1}{L} \sum_{j=1}^L \left(G_i[j] - \hat{G}_i[j] \right)^2 \quad i = 1, \dots, K.\tag{3.10}$$

A Pareto curve can be utilized to visualize the "optimal" number of particles in terms of the trade-off between computational complexity and error. The resulting number of particles needed per dimension will be calculated to gauge the rough number of particles needed to include additional parameters in the state-space in the following section.

3.4 Parameter Estimation

The **IPI** method introduced in Section 2.3.2 will be the baseline implementation of estimating insulin sensitivity S_I in patients and will be compared against the extended Kalman filter and the particle filter with state augmentation. Each method will try to estimate a constant insulin sensitivity and a piecewise insulin sensitivity that steps to a new value twice throughout the experiment to draw conclusions on the limitations of each estimator. The simulation will last for 60 hours, as changes in S_I are relatively slow in time, with discrete time-steps of 1 minute. There will be 500 total patients, and each filter will get an initial state with a $\pm 10\%$ deviation from the true initial state. At 20 and 40 hours, the piecewise insulin sensitivity will be randomly assigned a new value $S_{I,1}$ represented from the current value $S_{I,0}$

$$\begin{aligned}q &\sim \mathbb{U}[0.75, 0.95] \\ S_{I,1} &= \begin{cases} S_{I,0}(1 - q), & \text{with probability 0.5,} \\ S_{I,0}(1 + q), & \text{with probability 0.5.} \end{cases}\end{aligned}\tag{3.11}$$

To ensure the insulin sensitivity is constrained to a physiologically relevant value, $S_{I,1}$ will be clamped to the minimum and maximum insulin sensitivity observed from Equation 3.2. Due to an additional state being included in the state space, the process noise in Equation (3.5) needs to be appended to consider the uncertainty of S_I . As previously mentioned in Section 3.1, insulin sensitivity has been observed to be log-normal, which would translate to process noise that is multiplicative, not additive. Multiplicative noise follows a similar structure to Equation (3.11), such that

$$\begin{aligned} S_{I,k} &= f(S_{I,k-1}, u_{k-1}) w_{S_I,k-1}, & \text{with } w_{S_I,k-1} &\sim \mathcal{N}(1, \sigma_{S_I}^2) \\ &= S_{I,k-1} w_{S_I,k-1}. \end{aligned} \quad (3.12)$$

The multiplicative noise variance $\sigma_{S_I}^2$ will be chosen for the desired coefficient of variation CV for a constant or time-varying insulin sensitivity

$$\begin{aligned} CV &= \frac{\sigma_{S_I}}{\mu} \\ \sigma_{S_I} &= CV. \end{aligned} \quad (3.13)$$

Each estimate in the extended Kalman filter and the particle filter will include sampling from the additive process noise distribution from Equation (3.5), but the insulin sensitivity estimate is multiplied with a sampled random variable in Equation (3.12).

The extended Kalman filter configuration for this section will roughly be the following

1. Initial covariance matrix of

$$P_0 = \text{diag} \left(\begin{bmatrix} \log_{10}(\text{med}(G)) \\ \log_{10}(\text{med}(I)) \\ \log_{10}(\text{med}(Q)) \\ \log_{10}(\text{med}(P1)) \\ \log_{10}(\text{med}(P2)) \\ \log_{10}(\text{med}(u_{en})) \\ \max(S_I)^2 \end{bmatrix} \right) \quad (3.14)$$

2. Process noise matrix of

$$Q = \frac{1}{120} \text{diag} \left(\begin{bmatrix} \left(\frac{\text{med}(G)}{100} \right)^2 \\ \left(\frac{\text{med}(I)}{100} \right)^2 \\ \left(\frac{\text{med}(Q)}{100} \right)^2 \\ \left(\frac{\text{med}(P1)}{100} \right)^2 \\ \left(\frac{\text{med}(P2)}{100} \right)^2 \\ 10^{-8} \\ CV^2 \end{bmatrix} \right) \quad (3.15)$$

3. Measurement noise of

$$R = 0.125. \quad (3.16)$$

For a constant insulin sensitivity, the coefficient of variation can be assigned a smaller magnitude, as the estimator doesn't need to accommodate for larger deviations in the estimate. The initial covariance of the particles in the particle filter has the same value as Equation (3.15). The particle filter will contain the extrapolated "optimal" number of particles chosen from the previous section to accommodate another dimension in the state-space. Assessing the estimation of the insulin sensitivity will be evaluated using the **MSE** of the true insulin sensitivity S_I and the estimated insulin sensitivity $\hat{S}_I$ for a given patient i , and a insulin sensitivity measurement of length L

$$\text{MSE}_i = \frac{1}{L} \sum_{j=1}^L \left(S_{Ii}[j] - \hat{S}_{Ii}[j] \right)^2. \quad (3.17)$$

In the next chapter, the results of the virtual patient cohort generation, observability, state estimation, and parameter estimation will be presented and analyzed.

Chapter 4

Results


4.1 Synthetic Patient Cohort

Approximating probability mass functions was used to analyze the characteristics of the target population of critically-ill patients in the Karolinska University Hospital. Figure 4.1 is divided into two subfigures, with Figure 4.1a consisting of the probability mass functions of the inputs u_{ex} , D , and PN , as well as the insulin sensitivity parameter S_I , and Figure 4.1b is visualizing the probability mass functions of the derived initial dynamics G , I , Q , P_1 , P_2 , P , u_{en} .


When numerous virtual patients were sampled, the figures present a diverse distribution of realistic initial dynamics from the randomly assigned inputs and insulin sensitivity. This allowed for sampling of many unique variations of patient dynamics over time without relying on manual interventions. Previous work in virtual patient cohorts in glycaemic control was often limited to perturbations in previously recorded clinical data [13] or from integral-fitting [14] [15], but in this approach, a clear computational method towards reproducible generation of patient data was made feasible to analyze and compare the methods in the following sections.

4.2 Observability of the Intensive Glucose Insulin-Nutrition-Glucose Model

To investigate the observability of the ICING model, two methods were investigated. In Figure 4.2a, a probability mass function of eigenvalues from the 1000 calculated empirical observability gramians were plotted. The

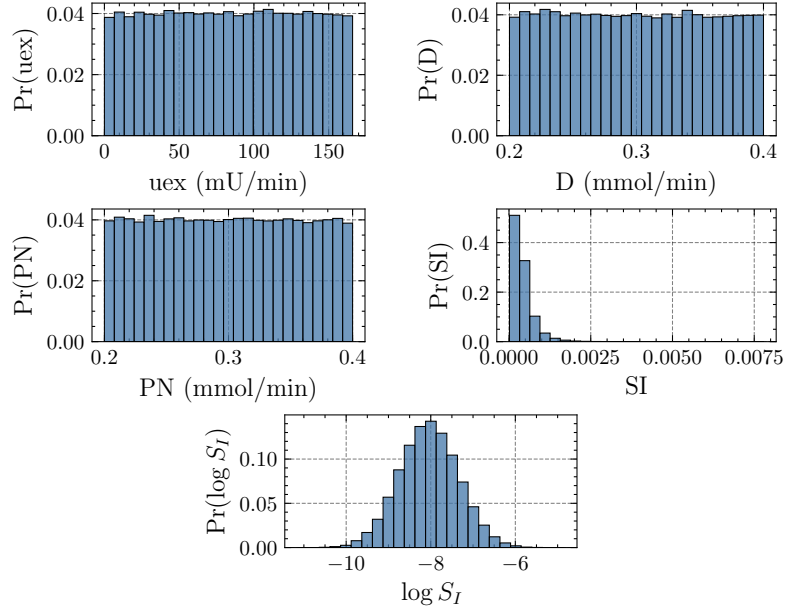

(a) Inputs and parameters

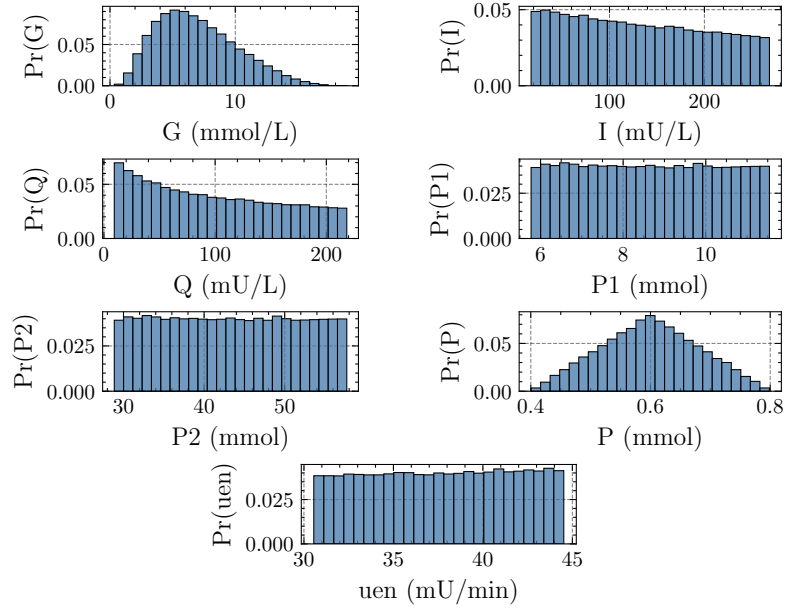

(b) Initial Dynamics

Figure 4.1: Histograms of the generated virtual patient cohort characteristics.

eigenvalues are transformed in a log-scale to easier visualize the spread of values. The red dotted line denotes the threshold chosen to distinguish the eigenvalues that are considered observable (> 0.10) or unobservable (≤ 0.10). The eigenvalues range from 10^{-15} to 10^2 . The number of states with eigenvalues considered observable is approximately 2, which would suggest that, given all available measurements, about a quarter of the states provide insight into the observations. The other Figure 4.2b, a box plot for each dynamic in the empirical observability gramian is plotted to show the respective locality of the empirical observability matrix diagonal $\text{diag}(W_O)$ over all patients. As a result of scaling all dynamics in the empirical observability gramian, the diagonal values are comparable amongst the dynamics.

The blood glucose concentration G is the most observable. This is to be expected as the observations in our state-space model are noisy blood glucose measurements. The blood glucose appearance in the stomach and the gut are the next observable states, with a median roughly of 2.95×10^{-2} and 3.07×10^{-2} , as well as an approximate interquartile range of 4.33×10^{-2} and 4.35×10^{-2} respectively. In Equation (2.1), the change in G is dependent on a constant consisting of a scaled multiple of the total glucose appearance P , which is a function of both the glucose appearance in the stomach and gut P_1, P_2 . Thus, this representation can be attributed to why P_1 and P_2 are more observable compared to the plasma insulin I and the interstitial insulin Q , as the fraction $\frac{Q}{1+\alpha_G Q}$ is being multiplied by a relatively small value S_I , and changes in I take time to propagate to Equation (2.1).

Overall, the ICING model can not be classified as observable. For a system that is not observable, the performance of the state estimates may be hindered, as for each observation sampled, only the blood glucose and possibly the total glucose appearance can be uniquely identified. In practice, you could add more observations to increase the observability, but in the context of insulin-glucose dynamics, most institutions only have access to blood glucose measurements and not plasma insulin or C-peptide data. While poor observability is a limitation in state-space models, the following sections show that the model has capabilities, albeit imperfect, to estimate insulin-glucose dynamics.

4.3 Nonlinear State Estimation

In the first stage of comparing different nonlinear state estimators, each estimator is given an initial state that has a deviation in each state from the true initial state. The MSE is averaged among all patients for each deviation

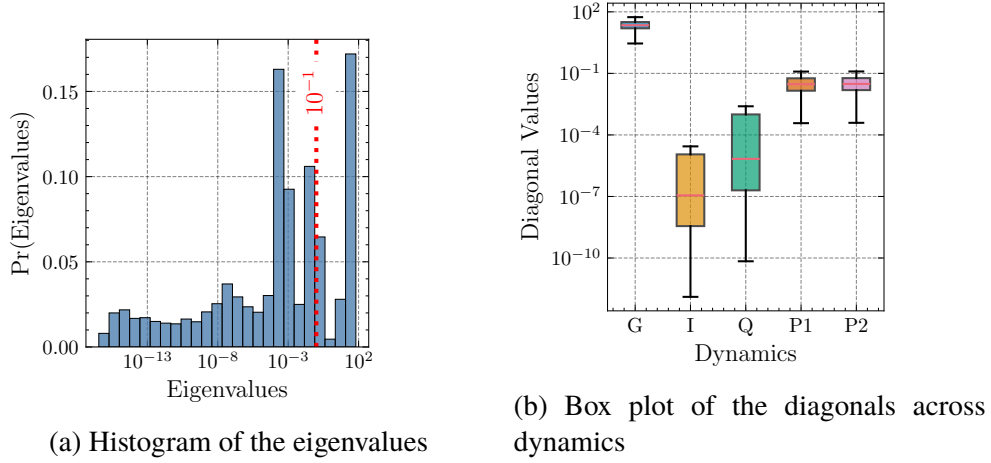


Figure 4.2: Analysis across all calculated empirical observability gramians.

in Table 4.1, as well as the standard deviation SD of the error, and an average **MSE** across all deviations is calculated. The distribution of dynamics from Section 4.1 allows for the corresponding initial and process noise covariance matrices

$$P_0 = \text{diag} \begin{pmatrix} 1.00 \\ 3.00 \\ 3.00 \\ 1.00 \\ 2.00 \\ 1.00 \end{pmatrix} \quad (4.1)$$

$$Q = \frac{1}{120} \text{diag} \begin{pmatrix} 5.00 \times 10^{-3} \\ 1.00 \\ 1.00 \\ 5.00 \times 10^{-3} \\ 2.50 \times 10^{-2} \\ 1.00 \times 10^{-8} \end{pmatrix}.$$

The extended Kalman filter overall performs the worst compared to the particle filters. When there are large deviations in the initial state of $\pm 25\%$, the **MSE** (0.265, 0.117) and the standard deviation (0.85, 0.55) are large

Table 4.1: Mean MSE for different estimators and deviations of the initial state. Standard deviations of the MSE are shown in parentheses.

Estimator	Deviations						Avg
	-25%	-10%	-2%	+2%	+10%	+25%	
EKF	0.265 (0.85)	0.087 (0.23)	0.040 (0.11)	0.028 (0.08)	0.030 (0.10)	0.117 (0.55)	0.095
PF 100	0.057 (0.17)	0.031 (0.08)	0.035 (0.09)	0.037 (0.10)	0.035 (0.10)	0.038 (0.12)	0.039
PF 200	0.055 (0.16)	0.033 (0.08)	0.035 (0.09)	0.036 (0.10)	0.035 (0.10)	0.037 (0.12)	0.038
PF 300	0.051 (0.14)	0.033 (0.08)	0.035 (0.09)	0.035 (0.10)	0.035 (0.10)	0.036 (0.12)	0.037
PF 400	0.046 (0.13)	0.033 (0.08)	0.034 (0.09)	0.035 (0.10)	0.035 (0.10)	0.036 (0.11)	0.037
PF 500	0.046 (0.13)	0.033 (0.08)	0.034 (0.09)	0.035 (0.09)	0.035 (0.10)	0.036 (0.11)	0.037
PF 750	0.046 (0.13)	0.033 (0.08)	0.034 (0.09)	0.034 (0.09)	0.035 (0.10)	0.035 (0.11)	0.036
PF 1000	0.038 (0.10)	0.033 (0.08)	0.034 (0.09)	0.035 (0.09)	0.035 (0.10)	0.036 (0.12)	0.035
PF 1500	0.036 (0.09)	0.034 (0.08)	0.034 (0.09)	0.035 (0.10)	0.036 (0.10)	0.036 (0.12)	0.035
PF 2000	0.037 (0.09)	0.033 (0.08)	0.035 (0.09)	0.035 (0.10)	0.036 (0.10)	0.037 (0.12)	0.035

respectively in comparison to a particle filter with only 100 particles (MSEs of 0.057 and 0.038, SDs of 0.17 and 0.12). Such improvements in performance with only using 100 particles, highlight the particle filter's ability to adapt quickly to errors in the state estimates when resampling after the initial measurement, compared to the extended Kalman filter that is dynamically propagating a point estimate of states. In the deviations of $\pm 2\%$ and $+10\%$, the extended Kalman filter outperforms or is comparable to the particle filters. It is a possibility that when resampling happens at the beginning of the simulation, regardless of the deviation, that the particle filter may be over-correcting because of the error till it adjusts after receiving another measurement.

To compare the overall performance of the filters, it is helpful to analyze Figure 4.3. The x-axis is the computational complexity of each estimator.

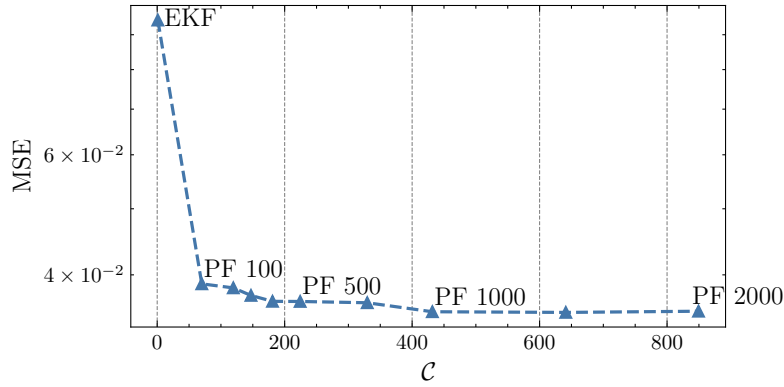


Figure 4.3: Comparison of the total average computational complexity and error across all estimators.

The minimum time to run amongst all the estimators was the extended filter. Thus, its computational complexity is 1. The computational complexity of the rest of the estimators is the multiple of time to run relative to the extended Kalman filter. The y-axis is the average **MSE** for all deviations of the initial states, plotted in the log-domain. In terms of error, there is a plateau in improvements in performance after 750 particles. The subjective "optimum" number of particles was chosen as 750 particles, as there is a balance of moderate performance and lower computational cost. It was assumed that for each dimension in the state space (total of 6), the number of particles needed P grows exponentially with a power of 2, which allows P to be estimated using the determined "optimal" number of particles

$$\begin{aligned}
 750 &= P \times 2^6 \\
 P &= \frac{750}{64} \\
 P &\approx 11.7.
 \end{aligned} \tag{4.2}$$

For the next section, the insulin sensitivity will be included in the state-space. Consequently, the state space increases to 7. To have a rough range of the number of particles needed to accommodate a larger dimension in the state space, the approximate number of particles N was calculated as such

$$\begin{aligned}
 N &= P \times 2^7 \\
 N &\approx 1500.
 \end{aligned} \tag{4.3}$$

The chosen "optimal" number of particles is much less computationally

expensive compared to previous work [17] that used 5000 particles for a state-space with the same number of dimensions. Although the Aguirre et al. study did contain non-Gaussian measurement noise, the number of particles to estimate the posterior distribution with a known measurement model prior likely does not require that many particles. If we decided to choose 5000 particles, there would likely be little marginal gain in the performance and would result in 5 times the computational complexity. For a system that may require an estimator to run in approximately real-time, an estimator with 5000 particles would require lots of computational resources. Hence, our approach is more practical in clinical settings. If very limited computational resources are allotted, smaller sized particle filters or the extended Kalman filter can be utilized instead.

4.4 Parameter Estimation

State augmentation of insulin sensitivity in the extended Kalman filter and the particle filter was implemented to compare the estimation performance of the existing state estimators against the Integral-based Patient Identification method. To accommodate the inclusion of the insulin sensitivity in the state-space, the initial and process noise covariance is appended as such

$$P_0 = \text{diag} \left(\begin{bmatrix} 1.00 \\ 3.00 \\ 3.00 \\ 1.00 \\ 2.00 \\ 1.00 \\ 1.00 \times 10^{-5} \end{bmatrix} \right)$$

$$Q_{\text{constant } S_I} = \frac{1}{120} \text{diag} \left(\begin{bmatrix} 5.00 \times 10^{-3} \\ 1.00 \\ 1.00 \\ 5.00 \times 10^{-3} \\ 2.50 \times 10^{-2} \\ 1.00 \times 10^{-8} \\ 8.00 \times 10^{-4} \end{bmatrix} \right) \quad (4.4)$$

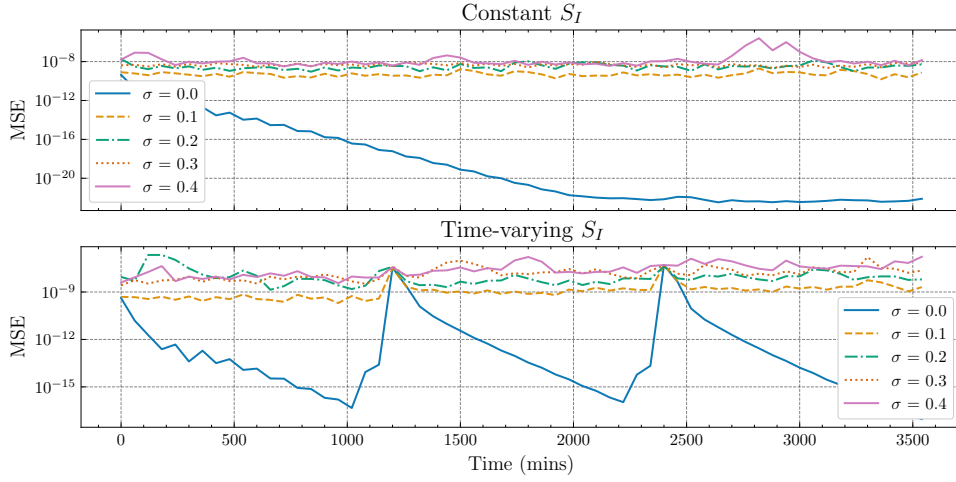


Figure 4.4: Integral-based method insulin sensitivity estimation performance across varying measurement noise variances.

$$Q_{\text{time-varying } S_I} = \frac{1}{120} \text{diag} \left(\begin{bmatrix} 5.00 \times 10^{-3} \\ 1.00 \\ 1.00 \\ 5.00 \times 10^{-3} \\ 2.50 \times 10^{-2} \\ 1.00 \times 10^{-8} \\ 0.33 \end{bmatrix} \right).$$

Both constant and time-varying insulin-sensitivity were used to investigate how characteristics of the parameter affect estimation. Figures 4.4 and 4.5 display the performance of each method according to the time dependency of the parameter. MSE in these figures depicts the mean error for each time step, not the length of the sequence.

The **IPI** method in Figure 4.4 illustrates how the estimation accuracy degrades if measurement noise is present in the calculation. Therefore, the performance is dependent on the quality of the measurements. Any estimation of the insulin sensitivity from the **IPI** method does not provide any information on the insulin sensitivity, as the output never converges towards the true value(s) in a practical setting with noisy measurements. For this reason, the **IPI** method is taken out of the comparison of the extended Kalman filter and particle filter in the following section.

In Figure 4.5, both the extended Kalman filter and the particle filter converge towards the true insulin sensitivity for a constant insulin sensitivity.

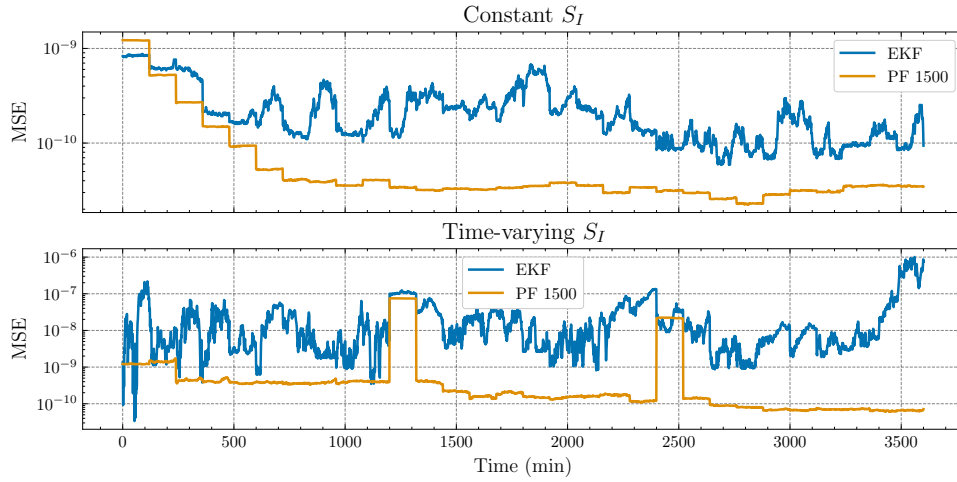


Figure 4.5: Mean MSE over time in parameter estimation methods estimating insulin sensitivity.

The extended Kalman filter on average plateaus in the estimation of the insulin sensitivity around a MSE of 10^{-10} , while the particle filter with 1500 particles on average roughly converges closer to the true value with roughly a MSE close to 10^{-11} . The extended Kalman filter often has higher variance in the estimate because particle filters average the variance over all the particles. Thus, the extended Kalman filter can also converge to the true value, but on average performs worse than the particle filter.

In the time-varying parameter estimation case, it can be seen in Figure 4.5 that the extended Kalman filter struggles to converge compared to the particle filter. This can be attributed to the extended Kalman filter's linearization approximation in the dynamic models, as when having a parameter transition to a new value quickly, the mismatch in the Jacobian linearization causes the filter to diverge. About 30% of the extended Kalman filter runs (150 patients) diverged, and had to be discarded entirely. Consequently, the extended Kalman filter is unreliable regarding unaccounted for changes in the parameters of interest. The particle filter can be seen to adapt when the insulin sensitivity steps to a new value at 1200 and 2400 mins. The particle filter largely remains unaffected by the stationarity of the insulin-sensitivity due to the particle filter's ability to approximate nonlinear and nongaussian dynamic models, unlike the extended Kalman filter. To conclude, the overall performance in parameter estimation is shown in Table 4.2, with the particle filter achieving the lowest MSE in estimating both constant and time-varying insulin sensitivity.

(a) Constant S_I			
Method	Deviation		Avg
	-10%	+10%	
EKF	9.57×10^{-10} (3.26×10^{-9})	5.03×10^{-9} (2.82×10^{-8})	3.00×10^{-9} (2.02×10^{-8})
PF 1500	7.21×10^{-10} (3.64×10^{-9})	7.02×10^{-10} (3.65×10^{-9})	7.11×10^{-10} (3.65×10^{-9})
(b) Time-varying S_I			
Method	Deviation		Avg
	-10%	+10%	
EKF	8.66×10^{-5} (2.61×10^{-3})	9.73×10^{-5} (2.64×10^{-3})	9.19×10^{-5} (2.63×10^{-4})
PF 1500	2.73×10^{-8} (1.82×10^{-7})	2.71×10^{-8} (1.79×10^{-7})	2.72×10^{-8} (1.80×10^{-7})

Table 4.2: Comparison of the mean MSE in parameter estimation methods estimating insulin sensitivity. Standard deviations of the MSE are shown in parentheses.

Chapter 5

Conclusions

5.1 Future work

5.2 Reflections

References

- [1] K. M. Dungan, S. S. Braithwaite, and J.-C. Preiser, “Stress hyperglycaemia,” *The Lancet*, vol. 373, no. 9677, pp. 1798–1807, May 2009. doi: 10.1016/S0140-6736(09)60553-5. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0140673609605535> [Page 1.]
- [2] P. Paolisso, A. Foà, L. Bergamaschi, F. Donati, M. Fabrizio, C. Chiti, F. Angeli, S. Toniolo, A. Stefanizzi, M. Armillotta, P. Rucci, G. Iannopollo, G. Casella, C. Marrozzini, N. Galiè, and C. Pizzi, “Hyperglycemia, inflammatory response and infarct size in obstructive acute myocardial infarction and MINOCA,” *Cardiovascular Diabetology*, vol. 20, no. 1, p. 33, Feb. 2021. doi: 10.1186/s12933-021-01222-9. [Online]. Available: <https://doi.org/10.1186/s12933-021-01222-9> [Page 1.]
- [3] G. Song, X. Liu, Z. Lu, J. Guan, X. Chen, Y. Li, G. Liu, G. Wang, and F. Ma, “Relationship between stress hyperglycaemic ratio (SHR) and critical illness: a systematic review,” *Cardiovascular Diabetology*, vol. 24, no. 1, p. 188, May 2025. doi: 10.1186/s12933-025-02751-3. [Online]. Available: <https://doi.org/10.1186/s12933-025-02751-3> [Page 1.]
- [4] C. H. Lang, C. Dobrescu, and K. Mészáros, “Insulin-mediated glucose uptake by individual tissues during sepsis,” *Metabolism*, vol. 39, no. 10, pp. 1096–1107, Oct. 1990. doi: 10.1016/0026-0495(90)90172-9. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/0026049590901729> [Page 1.]
- [5] R. C. ANDREWS and B. R. WALKER, “Glucocorticoids and insulin resistance: old hormones, new targets,” *Clinical Science*, vol. 96, no. 5, pp. 513–523, Apr. 1999. doi: 10.1042/cs0960513. [Online]. Available: <https://doi.org/10.1042/cs0960513> [Page 1.]

- [6] R. E. Shangraw, F. Jahoor, H. Miyoshi, W. A. Neff, C. A. Stuart, D. N. Herndon, and R. R. Wolfe, "Differentiation between septic and postburn insulin resistance," *Metabolism*, vol. 38, no. 10, pp. 983–989, Oct. 1989. doi: 10.1016/0026-0495(89)90010-3. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/0026049589900103> [Page 1.]
- [7] T. Heise, L. Heinemann, and A. A. R. Starke, "Simulated postaggression metabolism in healthy subjects: Metabolic changes and insulin resistance," *Metabolism*, vol. 47, no. 10, pp. 1263–1268, Oct. 1998. doi: 10.1016/S0026-0495(98)90334-1. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0026049598903341> [Page 1.]
- [8] G. V. d. Berghe, P. Wouters, F. Weekers, C. Verwaest, F. Bruyninckx, M. Schetz, D. Vlasselaers, P. Ferdinande, P. Lauwers, and R. Bouillon, "Intensive Insulin Therapy in Critically Ill Patients," *New England Journal of Medicine*, vol. 345, no. 19, pp. 1359–1367, Nov. 2001. doi: 10.1056/NEJMoa011300_eprint: <https://www.nejm.org/doi/pdf/10.1056/NEJMoa011300>. [Online]. Available: <https://www.nejm.org/doi/full/10.1056/NEJMoa011300> [Page 1.]
- [9] F. M. Brunkhorst, C. Engel, F. Bloos, A. Meier-Hellmann, M. Ragaller, N. Weiler, O. Moerer, M. Gruendling, M. Oppert, S. Grond, D. Olthoff, U. Jaschinski, S. John, R. Rossaint, T. Welte, M. Schaefer, P. Kern, E. Kuhnt, M. Kiehntopf, C. Hartog, C. Natanson, M. Loeffler, and K. Reinhart, "Intensive Insulin Therapy and Pentastarch Resuscitation in Severe Sepsis," *New England Journal of Medicine*, vol. 358, no. 2, pp. 125–139, Jan. 2008. doi: 10.1056/NEJMoa070716_eprint: <https://www.nejm.org/doi/pdf/10.1056/NEJMoa070716>. [Online]. Available: <https://www.nejm.org/doi/full/10.1056/NEJMoa070716> [Page 1.]
- [10] NICE-SUGAR Study Investigators, S. Finfer, B. Liu, D. R. Chittock, R. Norton, J. A. Myburgh, C. McArthur, I. Mitchell, D. Foster, V. Dhingra, W. R. Henderson, J. J. Ronco, R. Bellomo, D. Cook, E. McDonald, P. Dodek, P. C. Hébert, D. K. Heyland, and B. G. Robinson, "Hypoglycemia and risk of death in critically ill patients," *The New England Journal of Medicine*, vol. 367, no. 12, pp. 1108–1118, Sep. 2012. doi: 10.1056/NEJMoa1204942 [Page 1.]

- [11] L. Evans, A. Rhodes, W. Alhazzani, M. Antonelli, C. M. Coopersmith, C. French, F. R. Machado, L. McIntyre, M. Ostermann, H. C. Prescott, C. Schorr, S. Simpson, W. J. Wiersinga, F. Alshamsi, D. C. Angus, Y. Arabi, L. Azevedo, R. Beale, G. Beilman, E. Belley-Cote, L. Burry, M. Cecconi, J. Centofanti, A. Coz Yataco, J. De Waele, R. P. Dellinger, K. Doi, B. Du, E. Estenssoro, R. Ferrer, C. Gomersall, C. Hodgson, M. H. Møller, T. Iwashyna, S. Jacob, R. Kleinpell, M. Klompas, Y. Koh, A. Kumar, A. Kwizera, S. Lobo, H. Masur, S. McGloughlin, S. Mehta, Y. Mehta, M. Mer, M. Nunnally, S. Oczkowski, T. Osborn, E. Papathanassoglou, A. Perner, M. Puskarich, J. Roberts, W. Schweickert, M. Seckel, J. Sevransky, C. L. Sprung, T. Welte, J. Zimmerman, and M. Levy, “Surviving sepsis campaign: international guidelines for management of sepsis and septic shock 2021,” *Intensive Care Medicine*, vol. 47, no. 11, pp. 1181–1247, Nov. 2021. doi: 10.1007/s00134-021-06506-y. [Online]. Available: <https://doi.org/10.1007/s00134-021-06506-y> [Page 1.]
- [12] J. G. Chase, G. M. Shaw, T. Lotz, A. LeCompte, J. Wong, J. Lin, T. Lonergan, M. Willacy, and C. E. Hann, “Model-Based Insulin and Nutrition Administration for Tight Glycaemic Control in Critical Care,” *Current Drug Delivery*, vol. 4, no. 4, pp. 283–296. doi: 10.2174/156720107782151223. [Online]. Available: <https://www.eurekaselect.com/article/4990> [Pages 2 and 5.]
- [13] T. F. Lotz, J. G. Chase, K. A. McAuley, G. M. Shaw, X.-W. Wong, J. Lin, A. LeCompte, C. E. Hann, and J. I. Mann, “Monte Carlo analysis of a new model-based method for insulin sensitivity testing,” *Computer Methods and Programs in Biomedicine*, vol. 89, no. 3, pp. 215–225, Mar. 2008. doi: 10.1016/j.cmpb.2007.03.007. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0169260707000582> [Pages 2, 5, and 25.]
- [14] J. Lin, N. N. Razak, C. G. Pretty, A. Le Compte, P. Docherty, J. D. Parente, G. M. Shaw, C. E. Hann, and J. Geoffrey Chase, “A physiological Intensive Control Insulin-Nutrition-Glucose (ICING) model validated in critically ill patients,” *Computer Methods and Programs in Biomedicine*, vol. 102, no. 2, pp. 192–205, May 2011. doi: 10.1016/j.cmpb.2010.12.008. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0169260710003007> [Pages 2, 5, and 25.]

- [15] C. E. Hann, J. G. Chase, J. Lin, T. Lotz, C. V. Doran, and G. M. Shaw, “Integral-based parameter identification for long-term dynamic verification of a glucose–insulin system model,” *Computer Methods and Programs in Biomedicine*, vol. 77, no. 3, pp. 259–270, Mar. 2005. doi: 10.1016/j.cmpb.2004.10.006. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0169260704002123> [Pages 2, 6, 14, and 25.]
- [16] A. L. Compte, J. G. Chase, A. Lynn, C. Hann, G. Shaw, X.-W. Wong, and J. Lin, “Blood Glucose Controller for Neonatal Intensive Care: Virtual Trials Development and First Clinical Trials,” *Journal of Diabetes Science and Technology*, vol. 3, no. 5, pp. 1066–1081, Sep. 2009. doi: 10.1177/193229680900300510. [Online]. Available: <https://journals.sagepub.com/doi/10.1177/193229680900300510> [Pages 2 and 6.]
- [17] E. Aguirre-Zapata, J. Cardenas-Cartagena, and J. Garcia-Tirado, “Glycemic Monitoring in Critical Care using Nonlinear State Estimators,” *IFAC-PapersOnLine*, vol. 50, no. 1, pp. 4430–4435, Jul. 2017. doi: 10.1016/j.ifacol.2017.08.369. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S2405896317307127> [Pages 2, 13, and 31.]
- [18] C. Eberle and C. Ament, “Identifiability and online estimation of diagnostic parameters with in the glucose insulin homeostasis,” *Biosystems*, vol. 107, no. 3, pp. 135–141, Mar. 2012. doi: 10.1016/j.biosystems.2011.11.003. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0303264711001857> [Pages 2, 12, and 13.]
- [19] J. G. Chase, G. M. Shaw, J. Lin, C. V. Doran, C. Hann, M. B. Robertson, P. M. Browne, T. Lotz, G. C. Wake, and B. Broughton, “Adaptive bolus-based targeted glucose regulation of hyperglycaemia in critical care,” *Medical Engineering & Physics*, vol. 27, no. 1, pp. 1–11, Jan. 2005. doi: 10.1016/j.medengphy.2004.08.006. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S1350453304001420> [Page 6.]
- [20] S. Särkkä and L. Svensson, “Bayesian Filtering and Smoothing.” [Pages 8, 9, 11, and 14.]

- [21] J. S. Liu, *Monte Carlo Strategies in Scientific Computing*, ser. Springer Series in Statistics. New York, NY: Springer, 2004. ISBN 978-0-387-76369-9 978-0-387-76371-2. [Online]. Available: <http://link.springer.com/10.1007/978-0-387-76371-2> [Page 11.]
- [22] C. Kuptamete and N. Aunsri, “A review of resampling techniques in particle filtering framework,” *Measurement*, vol. 193, p. 110836, Apr. 2022. doi: 10.1016/j.measurement.2022.110836. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0263224122001312> [Page 11.]
- [23] J. Hahn and T. F. Edgar, “An improved method for nonlinear model reduction using balancing of empirical gramians,” *Computers & Chemical Engineering*, vol. 26, no. 10, pp. 1379–1397, Oct. 2002. doi: 10.1016/S0098-1354(02)00120-5. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0098135402001205> [Page 12.]
- [24] D. Geffen, R. Findeisen, M. Schliemann, F. Allgower, and M. Guay, “Observability Based Parameter Identifiability for Biochemical Reaction Networks,” in *2008 American Control Conference*, Jun. 2008. doi: 10.1109/ACC.2008.4586807. ISSN 2378-5861 pp. 2130–2135, iSSN: 2378-5861. [Online]. Available: <https://ieeexplore.ieee.org/abstract/document/4586807> [Page 12.]
- [25] S. Davidson, C. Pretty, V. Uyttendaele, J. Knopp, T. Desai, and J. G. Chase, “Multi-input stochastic prediction of insulin sensitivity for tight glycaemic control using insulin sensitivity and blood glucose data,” *Computer Methods and Programs in Biomedicine*, vol. 182, p. 105043, Dec. 2019. doi: 10.1016/j.cmpb.2019.105043. [Online]. Available: <https://www.sciencedirect.com/science/article/pii/S0169260718314342> [Page 18.]
- [26] J. Dormand and P. Prince, “A family of embedded Runge-Kutta formulae,” *Journal of Computational and Applied Mathematics*, vol. 6, no. 1, pp. 19–26, Mar. 1980. doi: 10.1016/0771-050X(80)90013-3. [Online]. Available: <https://linkinghub.elsevier.com/retrieve/pii/0771050X80900133> [Page 18.]

€€€€ For DIVA €€€€

```
{
  "Author1": { "Last name": "Mulvihill",
    "First name": "Markus",
    "Local User Id": "u100001",
    "E-mail": "mulvkth.se",
    "organisation": { "L1": "School of Electrical Engineering and Computer Science",
      }
    },
  "Cycle": "2",
  "Course code": "EA260X",
  "Credits": "30.0",
  "Degree1": { "Educational program": "Master's Programme, Information and Network Engineering, 120 credits"
    , "programcode": "TINNM"
    , "Degree": "Master's"
    , "subjectArea": "Decision and Control Systems"
    },
  "Title": {
    "Main title": "Modeling Nonlinear Insulin-Glucose Dynamics in Critically-ill Patients",
    "Subtitle": "Degree Project 2026",
    "Language": "eng" },
    "Alternative title": {
      "Main title": "Modellering av lcke-linjärt Insulin-Glukosodynamik hos Kritiskt Sjuka Patienter",
      "Subtitle": "Examensarbete 2026",
      "Language": "swe"
    },
  },
  "Supervisor1": { "Last name": "Lindström",
    "First name": "Martin",
    "Local User Id": "u15dfclv",
    "E-mail": "martin12@kth.se",
    "organisation": { "L1": "School of Electrical Engineering and Computer Science",
      "L2": "Teknisk informationsvetenskap" }
    },
  "Examiner1": { "Last name": "Thobaben",
    "First name": "Ragnar",
    "Local User Id": "u1rs7mp9",
    "E-mail": "ragnart@kth.se",
    "organisation": { "L1": "School of Electrical Engineering and Computer Science",
      "L2": "Teknisk informationsvetenskap" }
    },
  },
  "National Subject Categories": "10201, 10206",
  "Other information": { "Year": "2026", "Number of pages": "xi,43" },
  "Copyrightleft": "copyright",
  "Series": { "Title of series": "TRITA-EECS-EX" , "No. in series": "2022:00" },
  "Opponents": { "Name": "A. B. Normal & A. X. E. Normalè" },
  "Presentation": { "Date": "2022-03-15 13:00"
    , "Language": "eng"
    , "Room": "via Zoom https://kth-se.zoom.us/j/ddddddd"
    , "Address": "Isafjordsgatan 22 (Kistagången 16)"
    , "City": "Stockholm" },
  "Number of lang instances": "2",
  "Abstract[eng ]": €€€€
  Lorem ipsum dolor sit amet, consectetur adipiscing elit. Ut purus elit, vestibulum ut, placerat ac, adipiscing vitae, felis. Curabitur dictum gravida mauris. Nam arcu libero, nonummy eget, consectetur id, vulputate a, magna. Donec vehicula augue eu neque. Pellentesque habitant morbi tristique senectus et netus et malesuada fames ac turpis egestas. Mauris ut leo. Cras viverra metus rhoncus sem. Nulla et lectus vestibulum urna fringilla ultrices. Phasellus eu tellus sit amet tortor gravida placerat. Integer sapien est, iaculis in, pretium quis, viverra ac, nunc. Praesent eget sem vel leo ultrices bibendum. Aenean faucibus. Morbi dolor nulla, malesuada eu, pulvinar at, mollis ac, nulla. Curabitur auctor semper nulla. Donec varius orci eget risus. Duis nibh mi, congue eu, accumsan eleifend, sagittis quis, diam. Duis eget orci sit amet orci dignissim rutrum. Nam dui ligula, fringilla a, euismod sodales, sollicitudin vel, wisi. Morbi auctor lorem non justo. Nam lacus libero, pretium at, lobortis vitae, ultricies et, tellus. Donec aliquet, tortor sed accumsan bibendum, erat ligula aliquet magna, vitae ornare odio metus a mi. Morbi ac orci et nisl hendrerit mollis. Suspendisse ut massa. Cras nec ante. Pellentesque a nulla. Cum sociis natoque penatibus et magnis dis parturient montes, nascetur ridiculus mus. Aliquam tincidunt urna. Nulla ullamcorper vestibulum turpis. Pellentesque cursus luctus mauris. €€€€,
  "Keywords[eng ]": €€€€
  Canvas Learning Management System, Docker containers, Performance tuning €€€€,
  "Abstract[swe ]": €€€€
  Lorem ipsum dolor sit amet, consectetur adipiscing elit. Ut purus elit, vestibulum ut, placerat ac, adipiscing vitae, felis. Curabitur dictum gravida mauris. Nam arcu libero, nonummy eget, consectetur id, vulputate a, magna. Donec vehicula augue eu neque. Pellentesque habitant morbi tristique senectus et netus et malesuada fames ac turpis egestas. Mauris ut leo. Cras viverra metus rhoncus sem. Nulla et lectus vestibulum urna fringilla ultrices. Phasellus eu tellus sit amet tortor gravida placerat. Integer sapien est, iaculis in, pretium quis, viverra ac, nunc. Praesent eget sem vel leo ultrices bibendum. Aenean faucibus. Morbi dolor nulla, malesuada eu, pulvinar at, mollis ac, nulla. Curabitur auctor semper nulla. Donec varius orci eget risus. Duis nibh mi, congue eu, accumsan eleifend, sagittis quis, diam. Duis eget orci sit amet orci dignissim rutrum. Nam dui ligula, fringilla a, euismod sodales, sollicitudin vel, wisi. Morbi auctor lorem non justo. Nam lacus libero, pretium at, lobortis vitae, ultricies et, tellus. Donec aliquet, tortor sed accumsan bibendum, erat ligula aliquet magna, vitae ornare odio metus a mi. Morbi ac orci et nisl hendrerit mollis. Suspendisse ut massa. Cras nec ante. Pellentesque a nulla. Cum sociis natoque penatibus et magnis dis parturient montes, nascetur ridiculus mus. Aliquam tincidunt urna. Nulla ullamcorper vestibulum turpis. Pellentesque cursus luctus mauris. €€€€,
  "Keywords[swe ]": €€€€
  Canvas Lärplattform, Dockerbehållare, Prestandajustering €€€€,
```

