


Figure 6: Real DICOM Metadata & CT Windowing Demo

CT Image (raw)



MRI Image (raw)

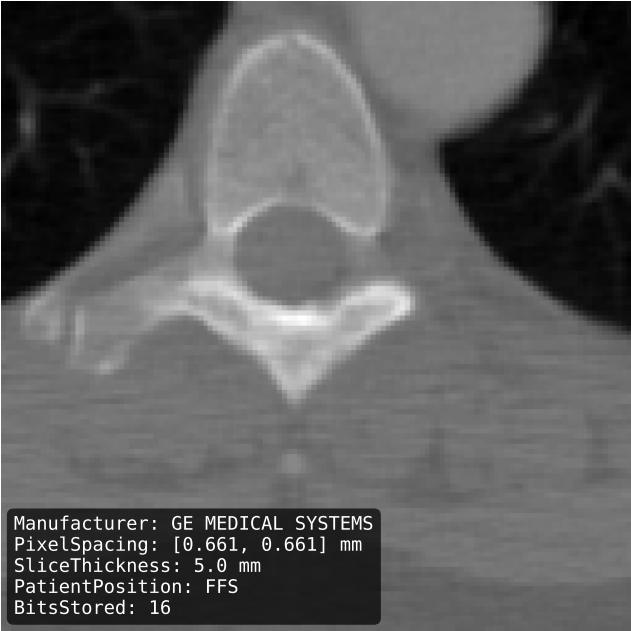


DICOM Metadata Comparison

Field	CT (GE)	MR (Toshiba)
PixelSpacing	0.661 mm	0.3125 mm
SliceThickness	5.0 mm	0.8 mm
Resolution	128×128	64×64
Intensity	Hounsfield (std)	Arbitrary (!)
Position	FFS	HFS

Lung Window
C=-600, W=1500



Soft Tissue Window
C=40, W=400

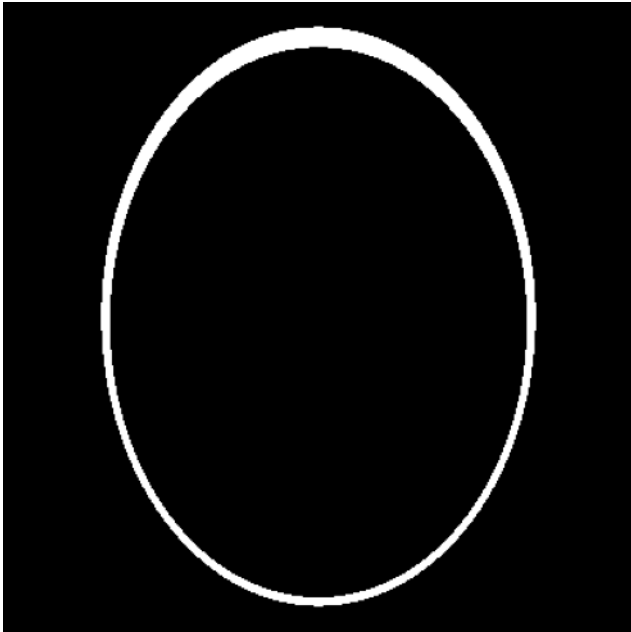

Bone Window
C=400, W=1800

