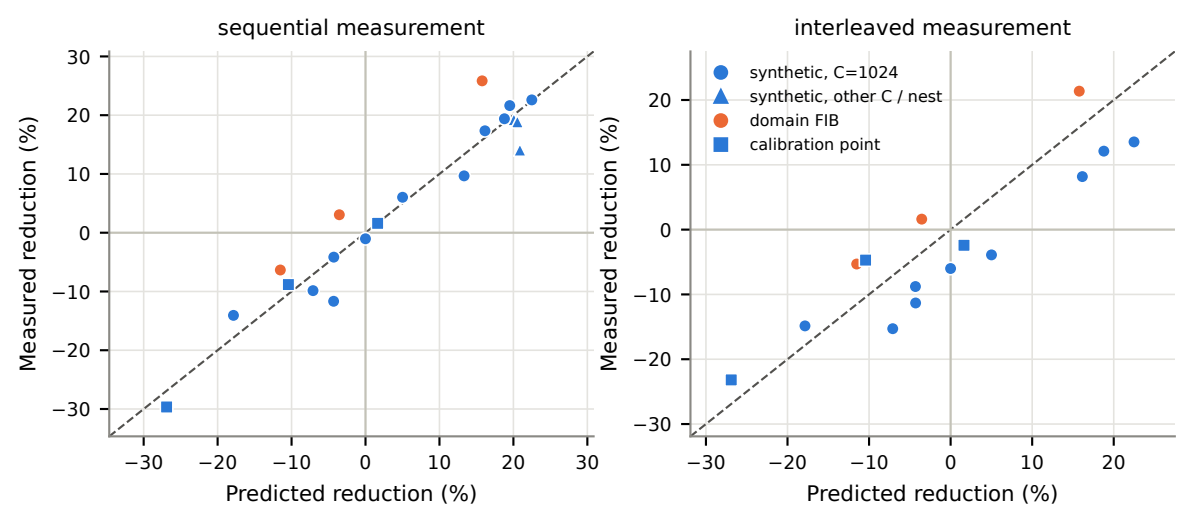
sequential measurement
interleaved measurement
Measured reduction (%)
Predicted reduction (%)
synthetic, C=1024
synthetic, other C / nest
domain FIB
calibration point
30
20
10
0
−10
−20
−30