Adapting the MRIQC structural workflow for estimation of FLAIR scan quality

We have developed a modified version of the MRIQC workflow for FLAIR scans and validated it across multiple sites and head-motion degraded scans

Molly Ireland[1], Heath Pardoe[1], Perchyonok Yuliya[2], Ricky Lu[2], Greg Fitt[2], David N Vaughan[1,2], Chris Tailby[1,3], David F Abbott[1] and Graeme D Jackson[1,2] for the Australian Epilepsy Project Investigators

1. Florey Institute of Neuroscience and Mental Health, Melbourne, Australia
2. Department of Neurology, Austin Health, Melbourne, Australia
3. Department of Neuropsychology, Austin Health, Melbourne, Australia

Background

MRIQC is a widely used tool to generate **automated assessments of MRI scan quality**; however its structural workflow does not include FLAIR scans

FLAIR-specific challenges:

- Low signal-to-noise (SNR) due to CSF suppression
- White-matter (WM) hyperintensities

This work **adapted the MRIQC tool** for assessment of 3D isotropic **FLAIR** scans
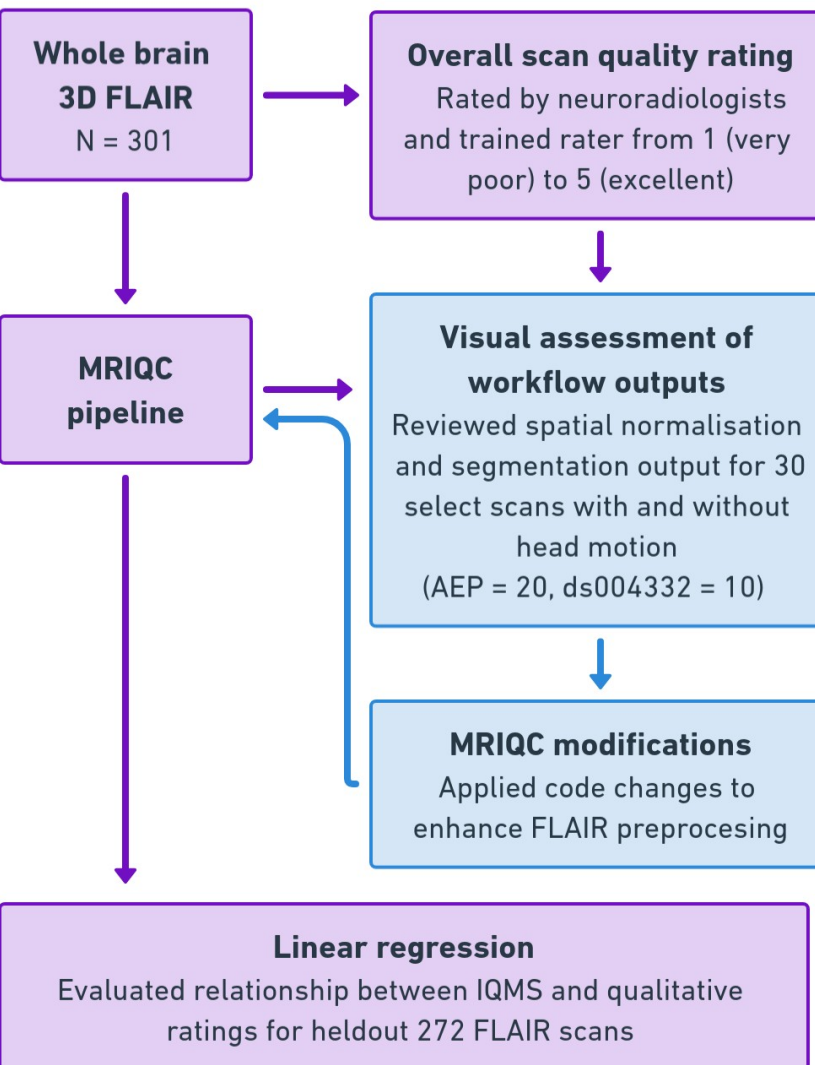
Methods

Iteratively modified the MRIQC workflow to process FLAIR scans from the Australia Epilepsy Project (AEP) and OpenNeuro ds004332 dataset.

| Dataset	N	Age	Multi-site
AEP	272	37y (18-67y)	Yes (235/25/7/3/2)
ds004332	29	23.5y (19-36y)	No
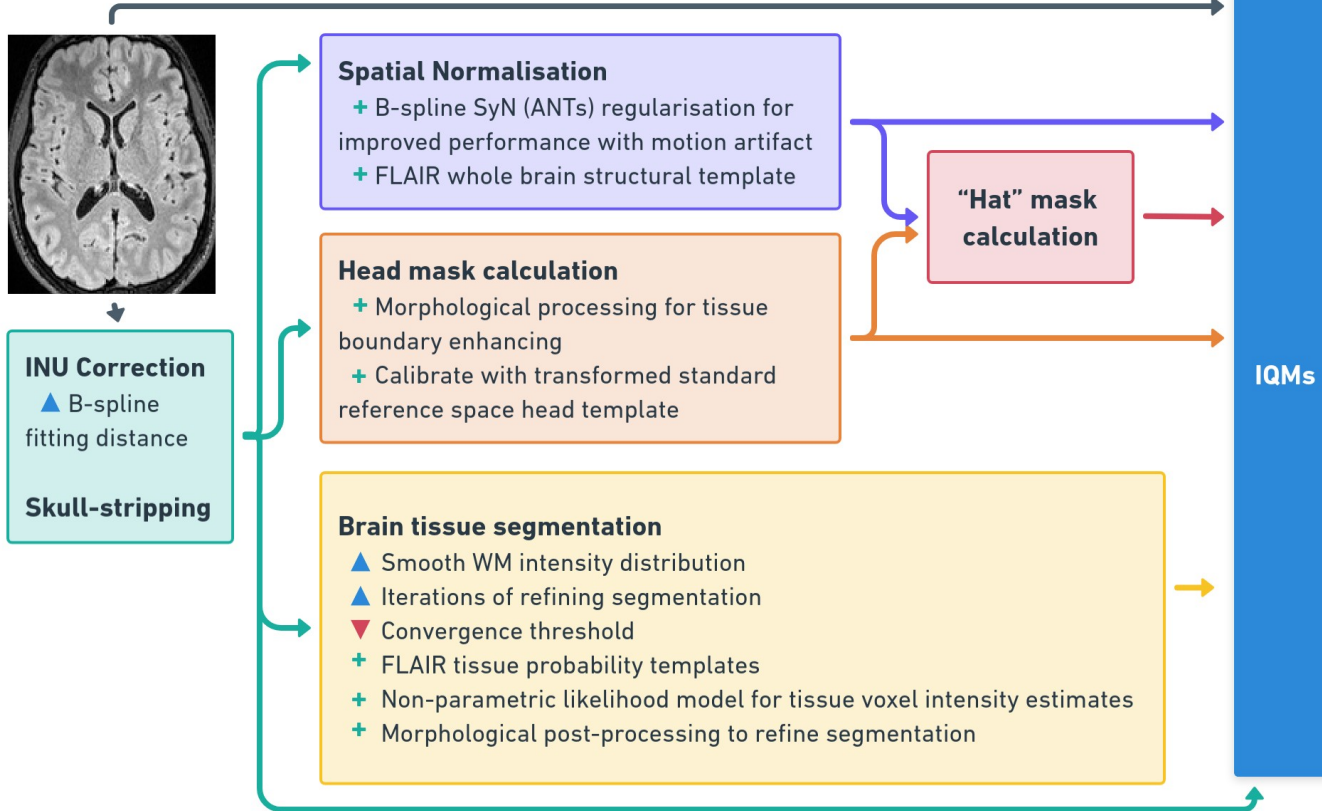
Figure 1: Adapted MRIQC structural workflow for FLAIR scans. Modifications to the workflow are embedded within preexisting processing modules. Changes: ▲= increase, ▼ = decrease, + = addition.

Spatial Normalisation
+ B-spline SyN (ANTs) regularisation for improved performance with motion artifact
+ FLAIR whole brain structural template

Head mask calculation
+ Morphological processing for tissue boundary enhancing
+ Calibrate with transformed standard reference space head template

"Hat" mask calculation

INU Correction
▲ B-spline fitting distance

Skull-stripping

Brain tissue segmentation
▲ Smooth WM intensity distribution
▲ Iterations of refining segmentation
▼ Convergence threshold
+ FLAIR tissue probability templates
+ Non-parametric likelihood model for tissue voxel intensity estimates
+ Morphological post-processing to refine segmentation

IQMs

Whole brain 3D FLAIR
N = 301

Overall scan quality rating
Rated by neuroradiologists and trained rater from 1 (very poor) to 5 (excellent)

MRIQC pipeline

Visual assessment of workflow outputs
Reviewed spatial normalisation and segmentation output for 30 select scans with and without head motion
(AEP = 20, ds004332 = 10)

MRIQC modifications
Applied code changes to enhance FLAIR preprocesing

Linear regression
Evaluated relationship between IQMS and qualitative ratings for heldout 272 FLAIR scans

To evaluate our FLAIR pipeline, the relationship between expert neuroradiological ratings and output image quality metrics (IQMs) was assessed with linear regression.

Finally, we compared these relationships with the same analyses applied to output from T1w scans from the unmodified MRIQC pipeline.

Results

Three changes significantly improved overall preprocessing for FLAIR:
1. Spatial transforms using FLAIR templates in MNI space
2. Registration with ANTs B-spline symmetric normalization (SyN) algorithm showed significant improvements for motion-affected FLAIR scans relative to default SyN
3. Tissue segmentation with a nonparametric likelihood model
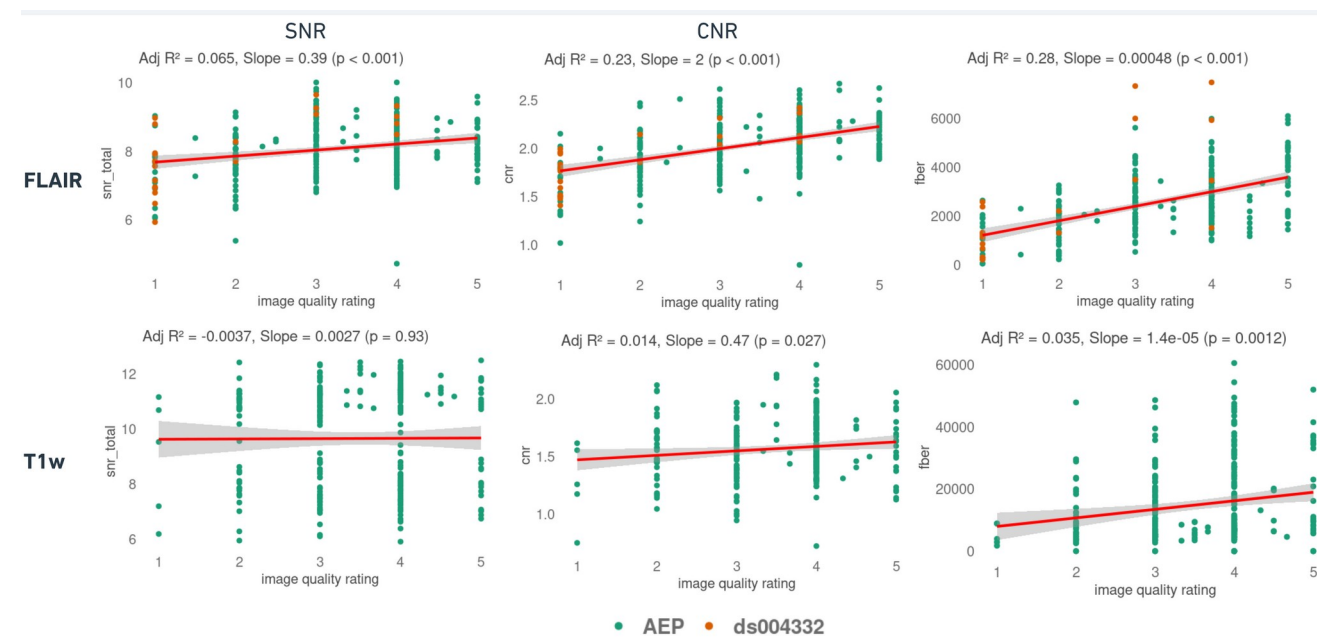
Figure 2: Comparisons of overall scan quality ratings against selected IQMs (snr_total, cnr and fber) for T1w and FLAIR scans.

- Many more IQMs correlated with visual ratings for FLAIR (N = 44) compared to T1 (N = 18)
- FLAIR and T1w IQMs were consistent with each other. Same direction for 13/15 IQMs with statistically significant associations for both modalities
- Mean adjusted R^2 higher for FLAIR (0.2) than T1w (0.04)

Conclusions

- Modified MRIQC workflow to estimate image quality metrics for 3D isotropic FLAIR
- Validated relationship between FLAIR IQMS from multisite, motion-affected and motion-free scans against neuroradiologist visual image quality ratings
- Predominantly developed with standardised Australian Epilepsy Project data meaning more multiside data required to validate performance

References
1. Esteban, O., et al. (2017b, June 25-29). MRIQC: Automatic prediction of quality and visual reporting of MRI scans [Poster Abstract]. 23rd Annual Meeting of the Organization for Human Brain Mapping (OHBM), Vancouver, BC, Canada. https://doi.org/10.7490/
2. Ganz, M., et al. (2022). Datasets with and without deliberate head movements for evaluating the performance of markerless prospective motion correction and selective reacquisition in ageneral clinical protocol for brain MRI [Dataset]. OpenNeuro. https://doi.org/10.18112/ openneuro.ds004332.v1.0.0
3. Tustison, N. J., et al. (2021). The ANTsX ecosystem for quantitative biological and medical imaging. Scientific Reports, 11(1), 9068. https://doi.org/10.1038/s41598-021-87564-6
4. Winkler, A. M., et al. (2019). FLAIR templates [Data set]. Brainder. https://brainder.org/download/flair/

The Florey
Advancing Brain Research

THE UNIVERSITY OF MELBOURNE

AUSTRALIAN EPILEPSY PROJECT
CHANGING LIVES | SUPERCHARGING MEDTECH