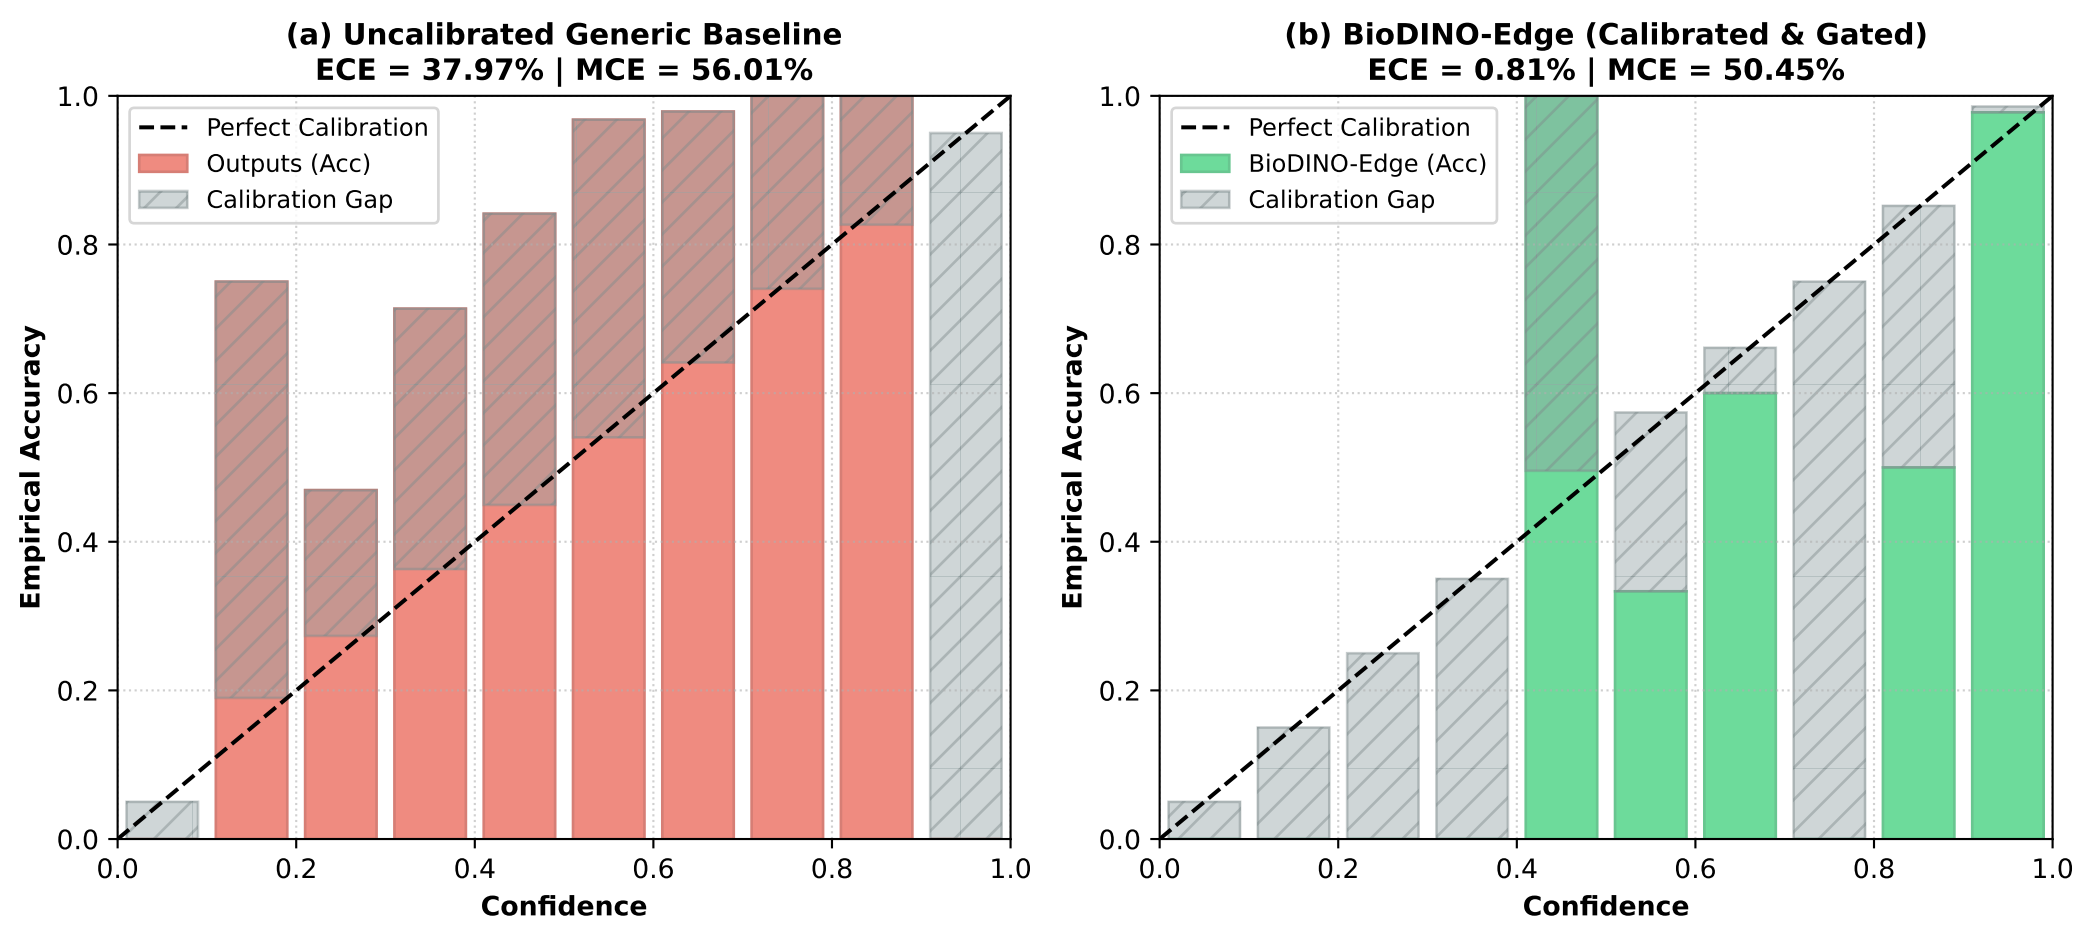
(a) Uncalibrated Generic Baseline
ECE = 37.97% | MCE = 56.01%
Perfect Calibration
Outputs (Acc)
Calibration Gap
Empirical Accuracy
Confidence
0.0
0.2
0.4
0.6
0.8
1.0
(b) BioDINO-Edge (Calibrated & Gated)
ECE = 0.81% | MCE = 50.45%
Perfect Calibration
BioDINO-Edge (Acc)
Calibration Gap
Empirical Accuracy
Confidence