

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 170626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	17/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
 (Suspension of ISO MTD in MIL-H-5606)
 No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	74	1056340	1061375	5035	0.48%
>6	178	459350	456941	-2409	-0.52%
>14	960	36410	37250	840	2.31%
>21	1992	10940	10752	-188	-1.72%
>25	2972	5210	4846	-364	-6.99%
>38	9926	612	515	-97	-15.81%
>**50	15882	145	135	-	-
>**70	24367	25	14	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
32	42	2.31

630/0072

Actual versus target calibration level

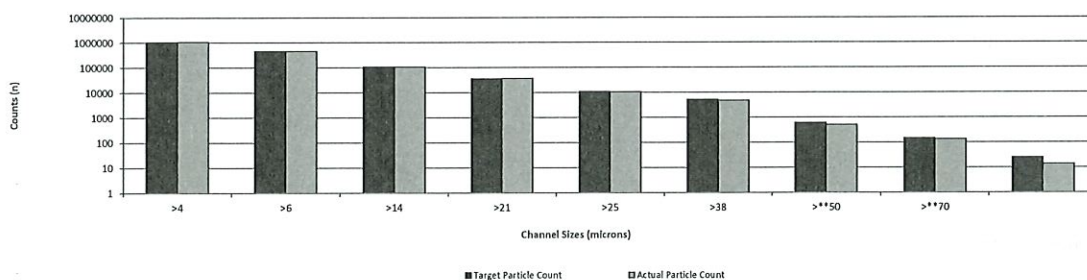

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
 Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
 Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 170626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	17/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	80	1056340	1065116	8776	0.83%
>6	194	459350	459710	360	0.08%
>14	1032	36410	37720	1310	3.60%
>21	2064	10940	11889	949	8.67%
>25	3012	5210	5538	328	6.30%
>38	10314	612	525	-87	-14.18%
>**50	16352	145	112	-	-
>**70	25228	25	18	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
31	49	2.58

63010073

Actual versus target calibration level

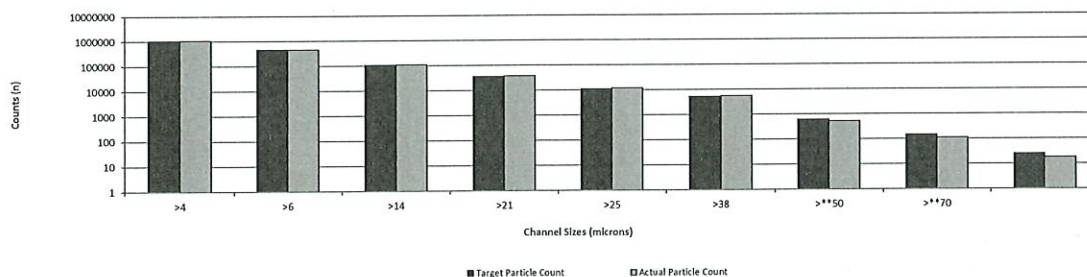

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	12345671
CERTIFICATE NUMBER	12345671 050526

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	05/05/26
CALIBRATION RIG NUMBER	00304

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	112	1037710	1047870	10160	0.98%
>6	176	432580	431351	-1229	-0.28%
>14	714	31970	32014	44	0.14%
>21	1314	9870	9858	-12	-0.12%
>25	1794	5300	5300	0	0.00%
>38	4348	1180	1181	1	0.08%
>**50	6298	640	637	-	-
>**70	14290	140	139	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
54	58	2.07

630/0074

Actual versus target calibration level

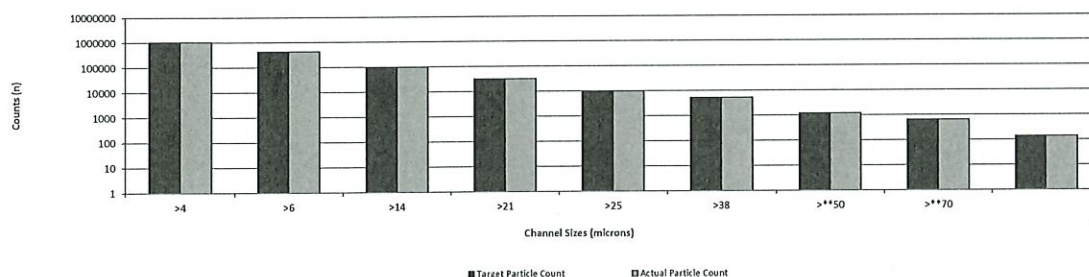

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	84	1056340	1070049	13709	1.30%
>6	204	459350	473353	14003	3.05%
>14	1090	36410	38842	2432	6.68%
>21	2214	10940	11869	929	8.49%
>25	3260	5210	5852	642	12.32%
>38	9853	612	761	149	24.46%
>**50	16228	145	145	-	-
>**70	25551	25	14	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
32	52	2.63

63010075

Actual versus target calibration level

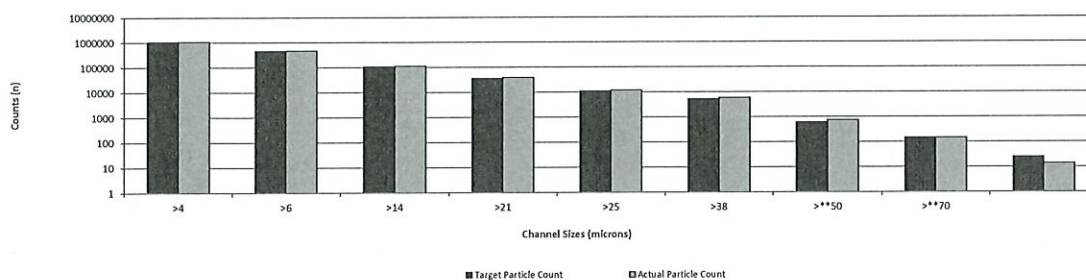

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
 (Suspension of ISO MTD in MIL-H-5606)
 No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	90	1056340	1043509	-12831	-1.21%
>6	220	459350	456440	-2910	-0.63%
>14	1052	36410	43205	6795	18.66%
>21	1882	10940	16417	5477	50.06%
>25	2634	5210	8965	3755	72.07%
>38	10217	612	1948	1336	218.45%
>**50	16276	145	800	-	-
>**70	24441	25	201	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
30	60	3.00

63010076

Actual versus target calibration level

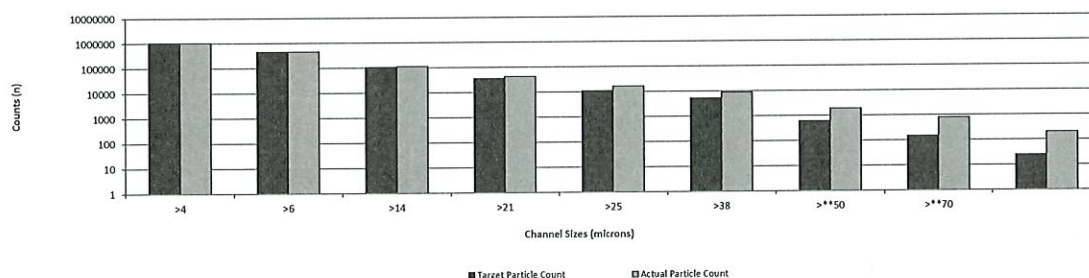

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
 Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
 Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000