

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	94	1056340	1053891	-2449	-0.23%
>6	228	459350	462774	3424	0.75%
>14	1224	36410	37427	1017	2.79%
>21	2462	10940	11838	898	8.21%
>25	3592	5210	5709	499	9.59%
>38	9874	612	699	87	14.27%
>**50	15648	145	130	-	-
>**70	25061	25	27	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
37	57	2.54

63010077

Actual versus target calibration level

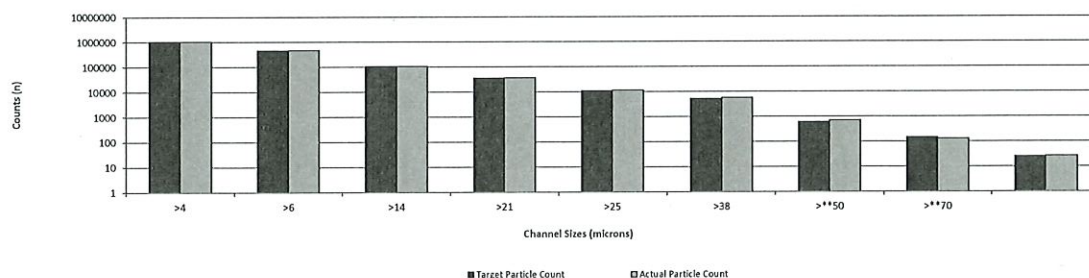

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	82	1056340	1062517	6177	0.58%
>6	198	459350	459007	-343	-0.07%
>14	1080	36410	35999	-411	-1.13%
>21	2220	10940	10547	-393	-3.59%
>25	3204	5210	5119	-91	-1.75%
>38	10296	612	593	-19	-3.08%
>**50	16082	145	126	-	-
>**70	25407	25	37	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
35	47	2.34

63010078

Actual versus target calibration level

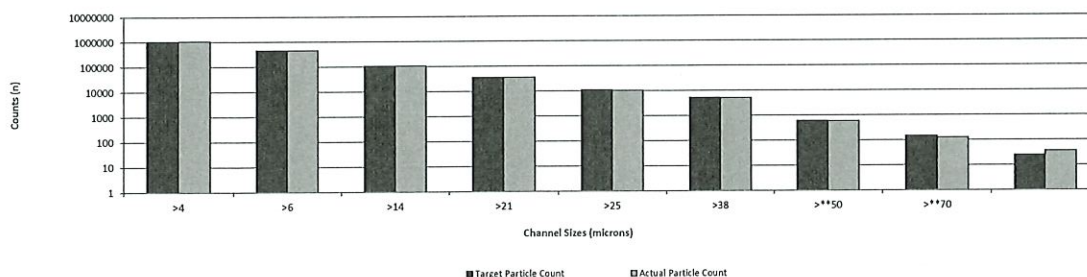

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
 (Suspension of ISO MTD in MIL-H-5506)
 No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	78	1056340	1066968	10628	1.01%
>6	188	459350	465752	6402	1.39%
>14	1018	36410	37095	685	1.89%
>21	2074	10940	11283	343	3.14%
>25	2990	5210	5545	335	6.43%
>38	10008	612	731	119	19.50%
>**50	16418	145	150	-	-
>**70	24602	25	14	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
32	46	2.44

630/0079

Actual versus target calibration level

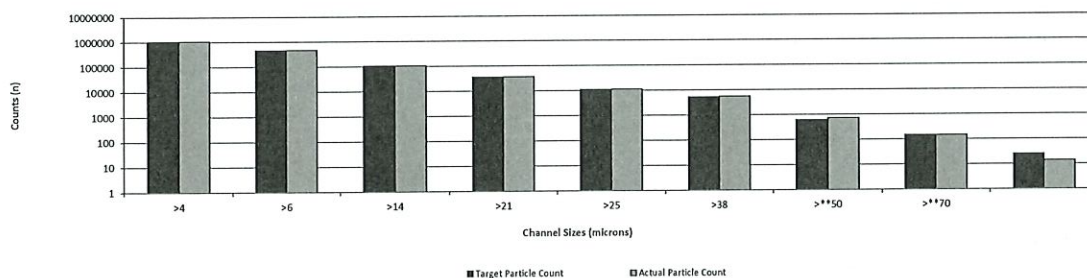

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
 Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
 Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	82	1056340	1070933	14593	1.39%
>6	204	459350	465044	5694	1.24%
>14	1092	36410	37039	629	1.73%
>21	2158	10940	12118	1178	10.77%
>25	3182	5210	5651	441	8.48%
>38	10154	612	586	-26	-4.20%
>**50	15872	145	153	-	-
>**70	25309	25	23	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
32	50	2.56

63010080

Actual versus target calibration level

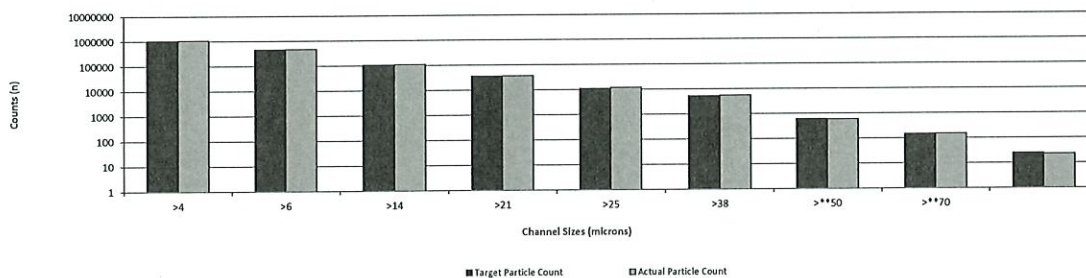

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5608)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	86	1056340	1061754	5414	0.51%
>6	216	459350	454811	-4539	-0.99%
>14	1126	36410	35888	-522	-1.43%
>21	2254	10940	10365	-575	-5.23%
>25	3200	5210	5022	-188	-3.61%
>38	9938	612	505	-107	-17.45%
>50	16215	145	115	-	-
>70	24388	25	37	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
36	50	2.39

630/0081

Actual versus target calibration level

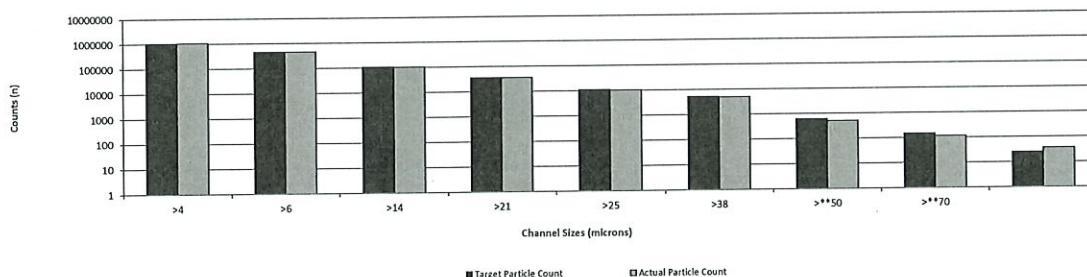

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000