

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
 (Suspension of ISO MTD in MIL-H-5606)
 No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	84	1056340	1045367	-10973	-1.04%
>6	210	459350	459894	544	0.12%
>14	1128	36410	36419	9	0.02%
>21	2250	10940	11124	184	1.68%
>25	3252	5210	5519	309	5.93%
>38	10058	612	689	77	12.63%
>**50	16391	145	136	-	-
>**70	24467	25	75	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
32	52	2.63

67010082

Actual versus target calibration level

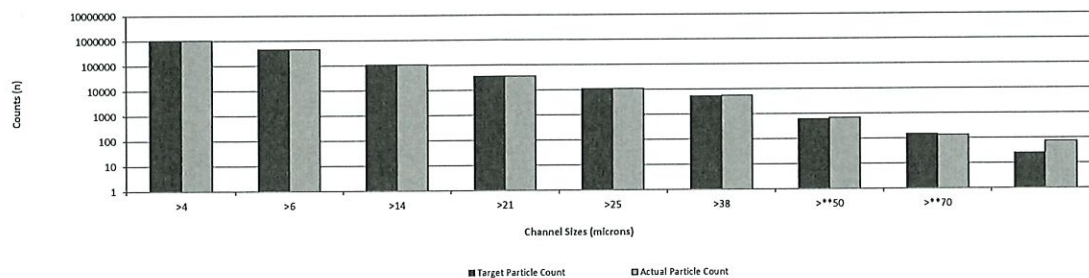

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
 Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
 Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	90	1056340	1058153	1813	0.17%
>6	220	459350	462471	3121	0.68%
>14	1148	36410	36666	256	0.70%
>21	2246	10940	11470	530	4.84%
>25	3270	5210	5437	227	4.36%
>38	10187	612	677	65	10.67%
>50	15905	145	166	-	-
>70	25124	25	28	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
30	60	3.00

63010083

Actual versus target calibration level

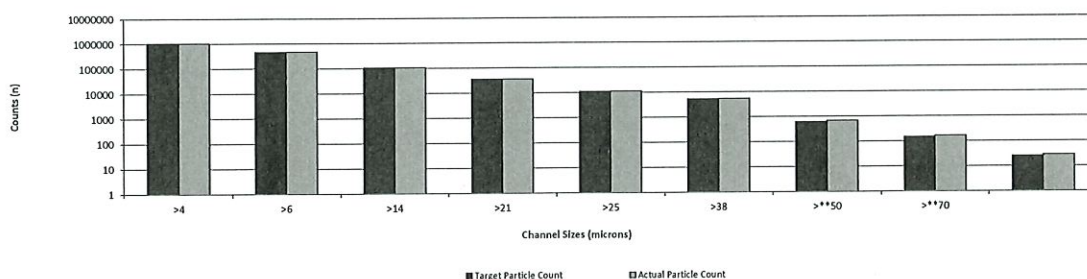

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000

CERTIFICATE OF CALIBRATION

WE HEREBY CERTIFY THAT THE CONTAMINATION MONITORING PRODUCT DETAILED BELOW HAS BEEN FULLY CALIBRATED WITH ISO MEDIUM TEST DUST (MTD) BASED ON ISO 11171:2020 ON TEST EQUIPMENT CERTIFIED TO ISO 11943 BY I.F.T.S (Institut de la Filtration et des Techniques Séparatives).

We hereby confirm that the above mentioned measuring system was calibrated according to DIN ISO 9001, under the observation of a certified quality assurance system. The measuring installation used for calibration are regularly calibrated to national standards by I.F.T.S. Should no national standards exist, the measuring procedure corresponds with the technical regulations and norms valid at the time of the measurement

PRODUCT TYPE	5.6mg/l RM8631b
SERIAL NUMBER	-1
CERTIFICATE NUMBER	-1 180626

REFERENCE MATERIAL BATCH NUMBER	RM8631b
DATE OF CALIBRATION	18/06/26
CALIBRATION RIG NUMBER	NOT SET

PARTICLE COUNT LIMITS AT 16mg/L CONCENTRATION
(Suspension of ISO MTD in MIL-H-5606)
No. particles reported per 100ml volume


Particle Size	Calibration Pulse Height	Target Particle Count	Actual Particle Count	Deviation	% Deviation (+/- 10%)
[microns (c)]	[mV]	[n]	[n]	[n]	[%]
>4	80	1056340	1063366	7026	0.67%
>6	198	459350	460235	885	0.19%
>14	1058	36410	35852	-558	-1.53%
>21	2152	10940	10467	-473	-4.32%
>25	3188	5210	4718	-492	-9.44%
>38	9840	612	536	-76	-12.39%
>**50	16332	145	97	-	-
>**70	24723	25	32	-	-

**These particle sizes are not yet certified by NIST

LS1 No Noise Threshold	LS1 Threshold Sensitivity	Sensitivity Threshold Ratio
[mV]	[mV]	[-]
35	45	2.29

63010084

Actual versus target calibration level

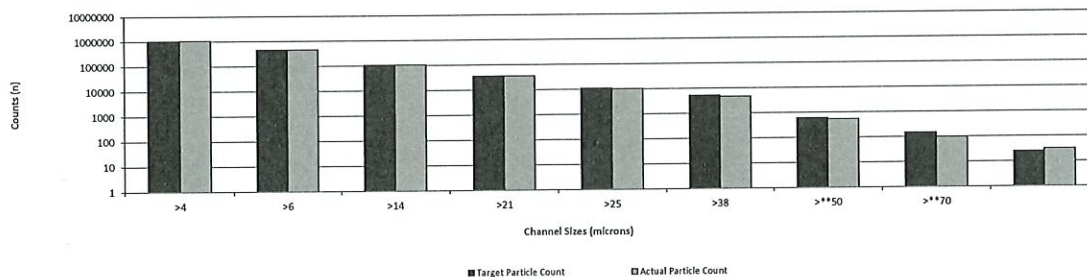

CALIBRATION RESULT **PASS**

RE-CALIBRATION DUE 1 YEAR FROM FIRST USE

CALIBRATED BY John Devereux

PASS - VERIFIED

Position Calibration Lab Technician

Newly purchased products are covered under warranty for 12 months from first use
Products being returned for re-calibration are verified for accuracy for a further 12 months. This does not extend the warranty.
Customers are responsible for managing the intervals between calibration's as defined within ISO 9001:2000