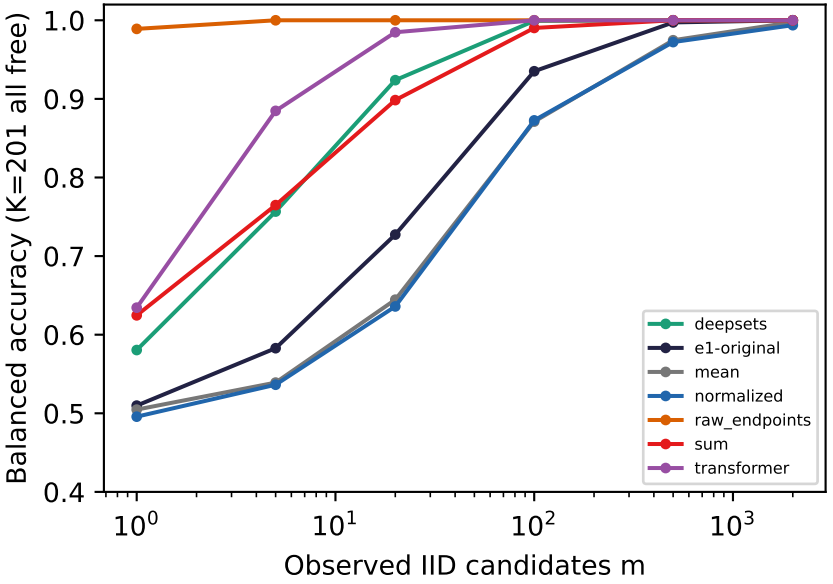
Balanced accuracy (K=201 all free)
1.0
0.9
0.8
0.7
0.6
0.5
0.4
10^0
10^1
10^2
10^3
Observed IID candidates m
deepsets
e1-original
mean
normalized
raw_endpoints
sum
transformer

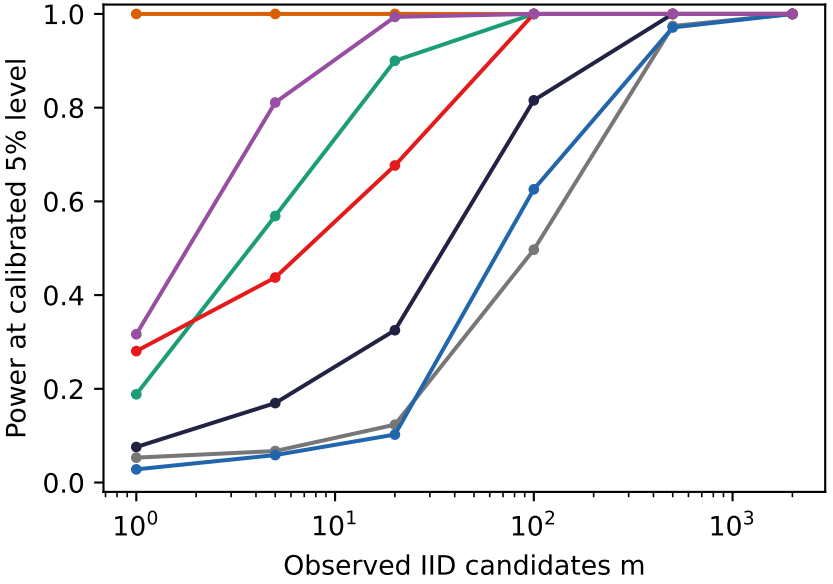
Power at calibrated 5% level
1.0
0.8
0.6
0.4
0.2
0.0
10^0
10^1
10^2
10^3
Observed IID candidates m