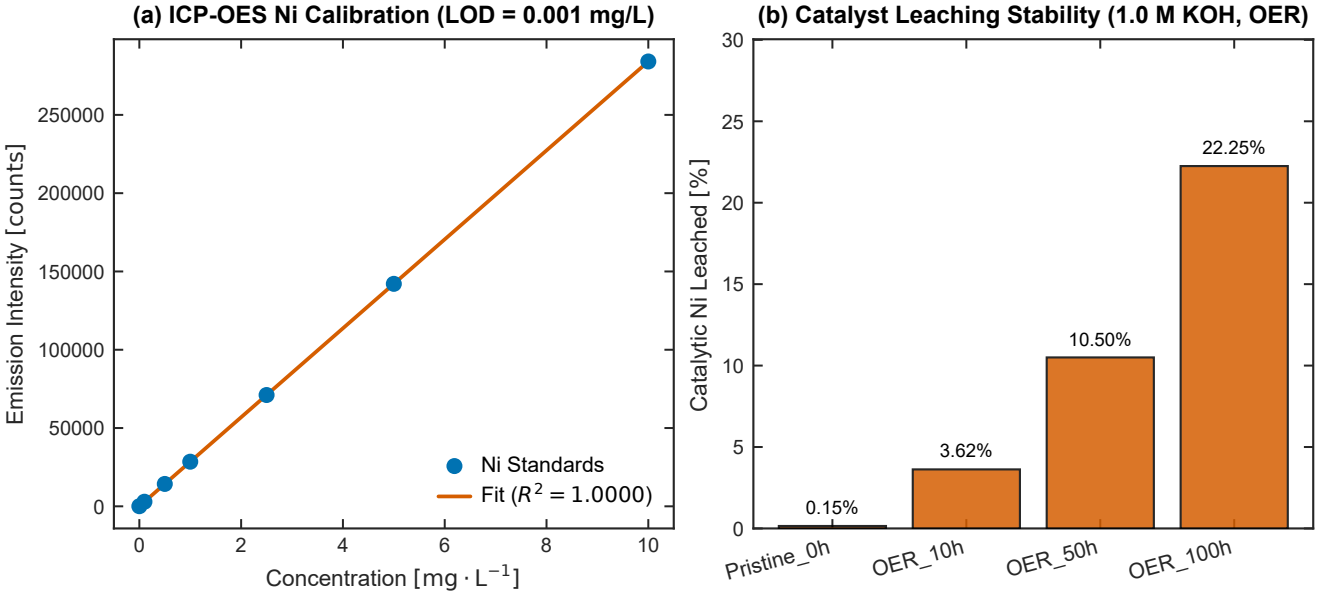

(a) ICP-OES Ni Calibration (LOD = 0.001 mg/L)
Emission Intensity [counts]
Concentration [mg · L^{-1}]
Ni Standards
Fit (R^2 = 1.0000)
(b) Catalyst Leaching Stability (1.0 M KOH, OER)
Catalytic Ni Leached [%]
0.15%
3.62%
10.50%
22.25%
Pristine_0h
OER_10h
OER_50h
OER_100h