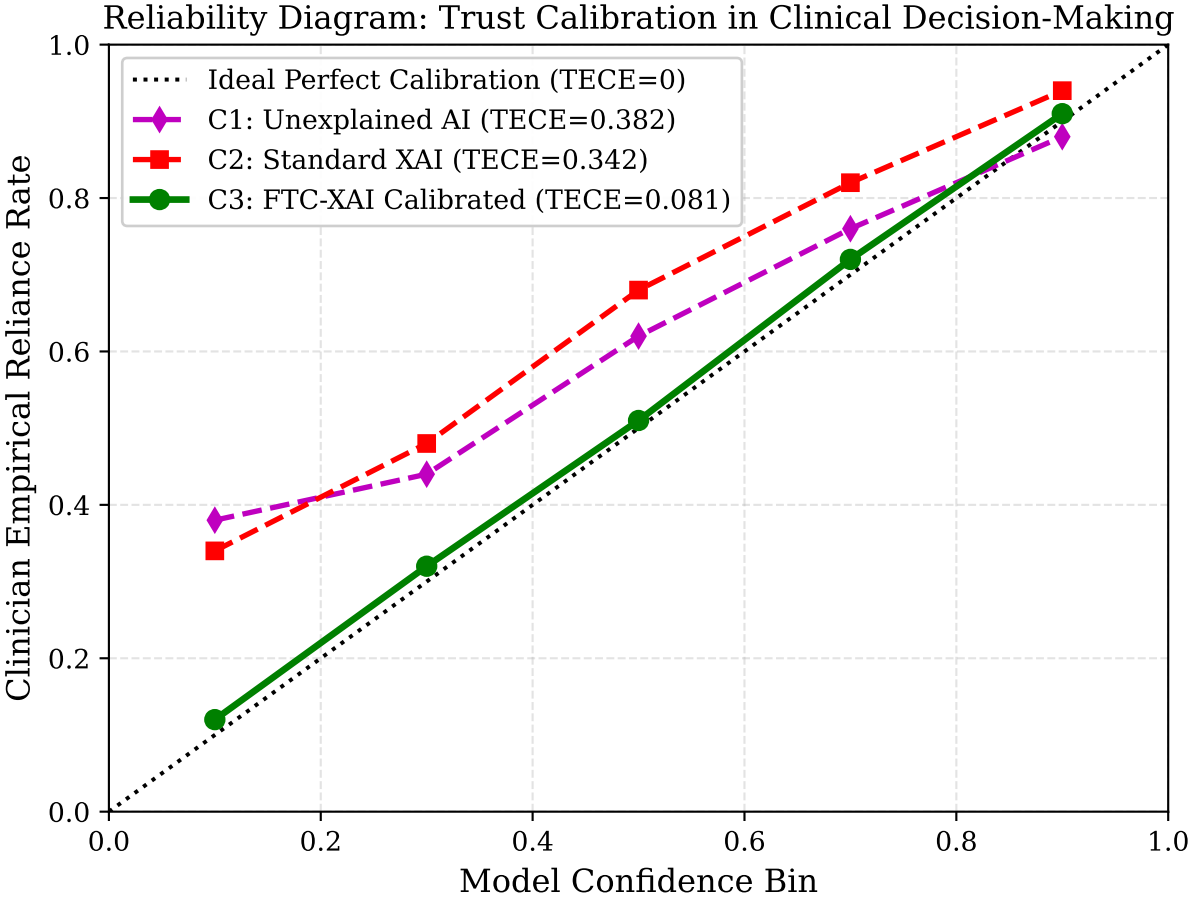
Reliability Diagram: Trust Calibration in Clinical Decision-Making
Ideal Perfect Calibration (TECE=0)
C1: Unexplained AI (TECE=0.382)
C2: Standard XAI (TECE=0.342)
C3: FTC-XAI Calibrated (TECE=0.081)
Clinician Empirical Reliance Rate
Model Confidence Bin
0.0
0.2
0.4
0.6
0.8
1.0